

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU081722\  
 Data File : VU050364.D  
 Acq On : 17 Aug 2022 19:52  
 Operator : SY/MD  
 Sample : N3734-09  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 WS-EDB-DBCP-TCP

Quant Time: Aug 18 06:10:14 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U081722DW.M  
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER  
 QLast Update : Thu Aug 18 06:06:02 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc      | Units   | Dev(Min) |
|-------------------------------|--------|------|----------|-----------|---------|----------|
| -----                         |        |      |          |           |         |          |
| Internal Standards            |        |      |          |           |         |          |
| 1) Fluorobenzene              | 6.115  | 96   | 36156    | 1.000     | ug/l    | # 0.00   |
| System Monitoring Compounds   |        |      |          |           |         |          |
| 57) 4-Bromofluorobenzene      | 10.639 | 95   | 8583     | 0.690     | ug/l    | 0.00     |
| Spiked Amount 1.000           |        |      | Recovery | =         | 69.000% |          |
| 68) 1,2-Dichlorobenzene-d4    | 12.195 | 152  | 10484    | 0.710     | ug/l    | 0.00     |
| Spiked Amount 1.000           |        |      | Recovery | =         | 71.000% |          |
| Target Compounds              |        |      |          |           |         |          |
|                               |        |      |          |           |         | Qvalue   |
| 3) Chloromethane              | 1.517  | 50   | 571      | 0.034     | ug/l    | # 73     |
| 4) Vinyl Chloride             | 1.604  | 62   | 49       | 0.003     | ug/l    | # 1      |
| 5) Bromomethane               | 1.854  | 94   | 248      | 0.037     | ug/l    | # 85     |
| 6) Chloroethane               | 1.938  | 64   | 120      | 0.013     | ug/l    | # 42     |
| 11) Allyl Chloride            | 2.915  | 41   | 272      | 0.016     | ug/l    | # 86     |
| 13) Acetone                   | 2.649  | 43   | 1847     | Below Cal |         | 92       |
| 14) Carbon Disulfide          | 2.790  | 76   | 1610     | 0.046     | ug/l    | # 71     |
| 15) Methylene Chloride        | 3.051  | 84   | 19569    | 0.953     | ug/l    | # 96     |
| 16) trans-1,2-Dichloroethene  | 3.356  | 96   | 67       | 0.006     | ug/l    | # 44     |
| 18) 2-Butanone                | 4.755  | 43   | 998      | 0.280     | ug/l    | # 75     |
| 19) Cyclohexane               | 5.366  | 56   | 107      | 0.008     | ug/l    | # 75     |
| 21) 2,2-Dichloropropane       | 4.668  | 77   | 41       | 0.003     | ug/l    | # 52     |
| 24) tert-Butyl Alcohol        | 3.202  | 59   | 3686     | 2.912     | ug/l    | # 73     |
| 25) Methyl tert-Butyl Ether   | 3.202  | 73   | 185      | 0.006     | ug/l    | # 1      |
| 27) Chloroform                | 5.086  | 83   | 661      | 0.031     | ug/l    | # 79     |
| 28) 1,1,1-Trichloroethane     | 5.301  | 97   | 22       | 0.001     | ug/l    | # 1      |
| 29) 1,1-Dichloropropene       | 5.536  | 75   | 102      | 0.008     | ug/l    | # 2      |
| 31) Isopropyl Ether           | 4.221  | 45   | 219      | 0.007     | ug/l    | # 85     |
| 32) Ethyl-t-butyl ether       | 4.726  | 59   | 306      | 0.012     | ug/l    | # 35     |
| 33) Tert-Amyl methyl ether    | 6.121  | 73   | 379      | 0.021     | ug/l    | # 42     |
| 34) Propionitrile             | 4.822  | 54   | 20       | 0.017     | ug/l    | # 1      |
| 35) Benzene                   | 5.758  | 78   | 266      | 0.006     | ug/l    | # 100    |
| 36) 1,2-Dichloroethane        | 5.809  | 62   | 19       | 0.001     | ug/l    | # 75     |
| 37) Trichloroethene           | 6.552  | 130  | 67       | 0.006     | ug/l    | # 1      |
| 39) Methacrylonitrile         | 4.986  | 41   | 123      | 0.032     | ug/l    | # 31     |
| 40) Methyl acrylate           | 5.012  | 55   | 43       | 0.006     | ug/l    | # 1      |
| 41) Tetrahydrofuran           | 5.089  | 42   | 202      | 0.094     | ug/l    | # 60     |
| 42) 1-Chlorobutane            | 5.443  | 56   | 92       | 0.005     | ug/l    | # 1      |
| 44) Bromodichloromethane      | 7.118  | 83   | 41       | 0.003     | ug/l    | # 26     |
| 45) 4-Methyl-2-Pentanone      | 7.828  | 43   | 629      | 0.087     | ug/l    | # 55     |
| 46) t-1,4-Dichloro-2-butene   | 10.828 | 75   | 17396    | 7.277     | ug/l    | # 20     |
| 49) Toluene                   | 7.983  | 92   | 147      | 0.006     | ug/l    | # 72     |
| 54) 2-Hexanone                | 8.719  | 43   | 556      | 0.113     | ug/l    | # 55     |
| 56) 1,2-Dibromoethane         | 8.935  | 107  | 15086    | 1.764     | ug/l    | # 98     |
| 58) Tetrachloroethene         | 8.558  | 164  | 59       | 0.006     | ug/l    | # 58     |
| 59) Chlorobenzene             | 9.455  | 112  | 297      | 0.011     | ug/l    | # 31     |
| 63) Ethyl Benzene             | 9.574  | 91   | 497      | 0.446     | ug/l    | # 44     |
| 64) m/p-Xylenes               | 9.700  | 106  | 317      | 0.821     | ug/l    | # 75     |
| 65) o-Xylene                  | 10.098 | 106  | 75       | 0.359     | ug/l    | # 1      |
| 66) Styrene                   | 10.124 | 104  | 298      | 0.474     | ug/l    | # 68     |
| 69) Isopropylbenzene          | 10.488 | 105  | 504      | 0.456     | ug/l    | # 85     |
| 70) 1,1,2,2-Tetrachloroethane | 10.790 | 83   | 42       | 0.003     | ug/l    | # 25     |
| 71) 1,2,3-Trichloropropane    | 10.828 | 75   | 17396    | 1.817     | ug/l    | # 81     |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU081722\  
 Data File : VU050364.D  
 Acq On : 17 Aug 2022 19:52  
 Operator : SY/MD  
 Sample : N3734-09  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 WS-EDB-DBCP-TCP

Quant Time: Aug 18 06:10:14 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U081722DW.M  
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER  
 QLast Update : Thu Aug 18 06:06:02 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-------|--------|----------|
| -----                         |        |      |          |       |        |          |
| 72) Bromobenzene              | 10.787 | 156  | 96       | 0.009 | ug/l   | 69       |
| 73) n-propylbenzene           | 10.912 | 120  | 113      | 0.515 | ug/l # | 1        |
| 74) 2-Chlorotoluene           | 10.989 | 126  | 161      | 0.313 | ug/l   | 87       |
| 75) 1,3,5-Trimethylbenzene    | 11.092 | 105  | 550      | 0.449 | ug/l   | 86       |
| 76) 4-Chlorotoluene           | 11.105 | 126  | 94       | 0.009 | ug/l   | 1        |
| 77) tert-Butylbenzene         | 11.420 | 119  | 437      | 0.388 | ug/l # | 85       |
| 78) 1,2,4-Trimethylbenzene    | 11.471 | 105  | 709      | 0.383 | ug/l   | 86       |
| 79) sec-Butylbenzene          | 11.645 | 105  | 1099     | 0.449 | ug/l # | 71       |
| 80) Nitrobenzene              | 13.211 | 77   | 68       | 0.082 | ug/l # | 42       |
| 81) p-Isopropyltoluene        | 11.793 | 119  | 1067     | 0.017 | ug/l # | 74       |
| 82) 1,3-Dichlorobenzene       | 11.748 | 146  | 813      | 0.035 | ug/l # | 69       |
| 83) 1,4-Dichlorobenzene       | 11.841 | 146  | 866      | 0.036 | ug/l # | 81       |
| 84) n-Butylbenzene            | 12.211 | 91   | 2242     | 0.519 | ug/l # | 86       |
| 85) 1,2-Dichlorobenzene       | 12.217 | 146  | 663      | 0.029 | ug/l   | 85       |
| 86) 1,2-Dibromo-3-Chloropr... | 13.002 | 75   | 1288     | 0.597 | ug/l   | 89       |
| 87) 1,2,4-Trichlorobenzene    | 13.844 | 180  | 1578     | 0.428 | ug/l # | 88       |
| 88) Hexachlorobutadiene       | 14.021 | 225  | 536      | 0.064 | ug/l   | 97       |
| 89) Naphthalene               | 14.092 | 128  | 4576     | 0.961 | ug/l # | 92       |
| 90) 1,2,3-Trichlorobenzene    | 14.333 | 180  | 1776     | 0.453 | ug/l   | 99       |
| -----                         |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU081722\  
Data File : VU050364.D  
Acq On : 17 Aug 2022 19:52  
Operator : SY/MD  
Sample : N3734-09  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP

Quant Time: Aug 18 06:10:14 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\524U081722DW.M  
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER  
QLast Update : Thu Aug 18 06:06:02 2022  
Response via : Initial Calibration




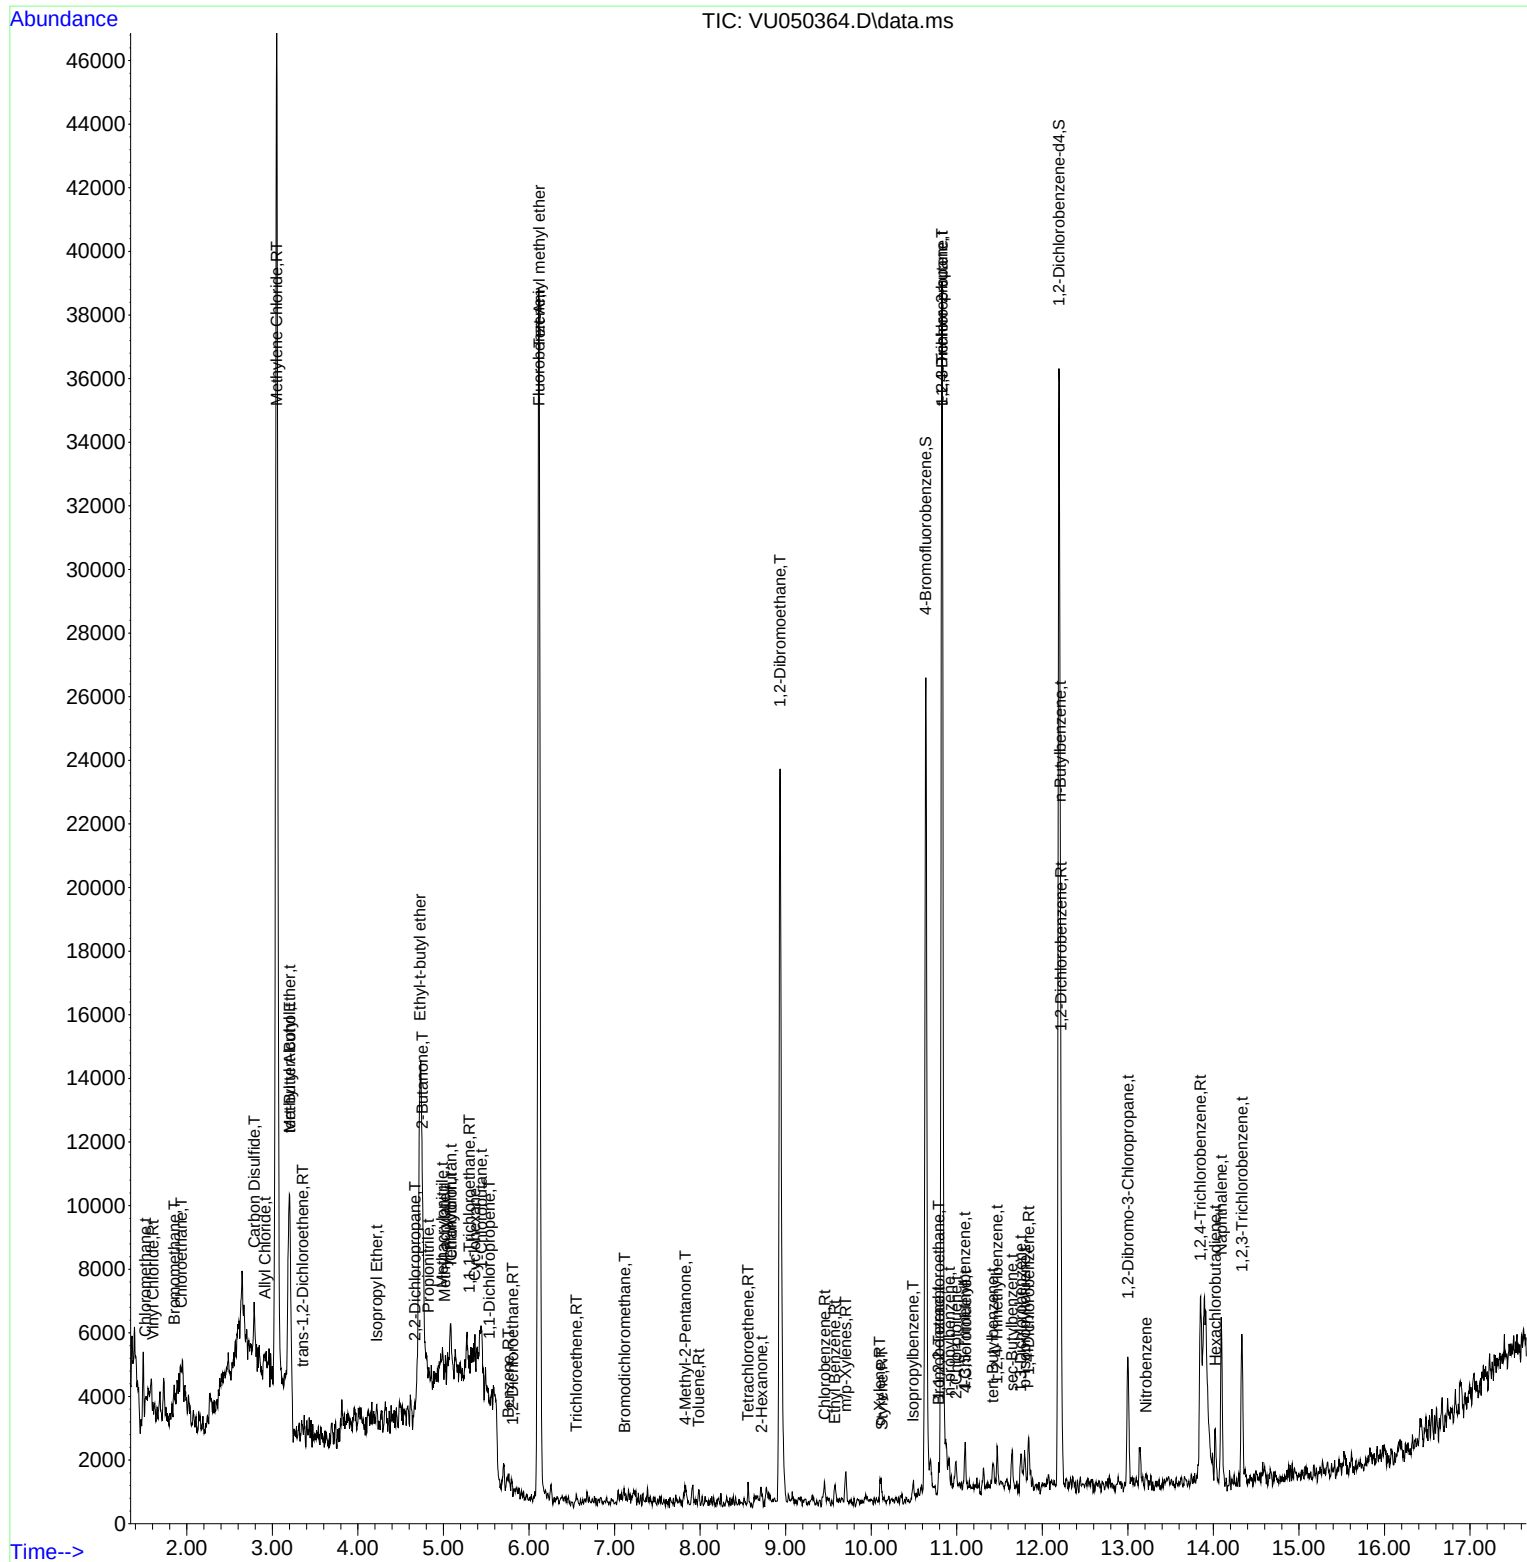




#1  
Fluorobenzene  
Concen: 1.000 ug/l  
RT: 6.115 min Scan# 14  
Delta R.T. -0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


|             |             |
|-------------|-------------|
| Tgt Ion: 96 | Resp: 36156 |
| Ion Ratio   | Lower Upper |
| 96 100      |             |
| 70 19.7     | 16.7 25.1   |
| 95 8.8      | 7.4 11.0    |
| 97 6.3      | 0.0 0.0#    |



#3  
Chloromethane  
Concen: 0.034 ug/l  
RT: 1.517 min Scan# 55  
Delta R.T. -0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

|             |           |       |  |
|-------------|-----------|-------|--|
| Tgt Ion: 50 | Resp: 571 |       |  |
| Ion Ratio   | Lower     | Upper |  |
| 50 100      |           |       |  |
| 52 47.6     | 26.1      | 39.1# |  |









#4  
 Vinyl Chloride  
 Concen: 0.003 ug/l  
 RT: 1.604 min Scan# 81  
 Delta R.T. -0.000 min  
 Lab File: VU050364.D  
 Acq: 17 Aug 2022 19:52




Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 WS-EDB-DBCP-TCP


Tgt Ion: 62 Resp: 49  
 Ion Ratio Lower Upper  
 62 100  
 64 103.1 25.5 38.3#

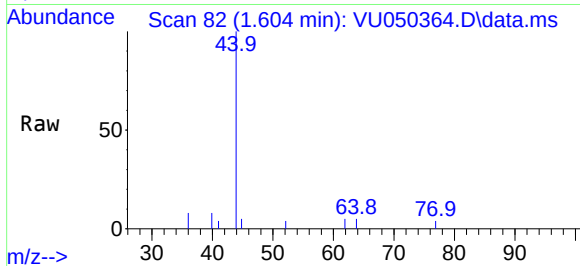

#5  
 Bromomethane  
 Concen: 0.037 ug/l  
 RT: 1.854 min Scan# 160  
 Delta R.T. -0.000 min  
 Lab File: VU050364.D  
 Acq: 17 Aug 2022 19:52

Tgt Ion: 94 Resp: 248  
 Ion Ratio Lower Upper  
 94 100  
 96 77.3 73.0 109.6




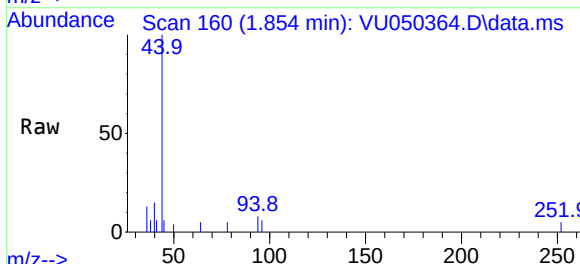




#6  
Chloroethane  
Concen: 0.013 ug/l  
RT: 1.938 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 64 Resp: 120  
Ion Ratio Lower Upper  
64 100  
66 0.0 25.8 38.6#

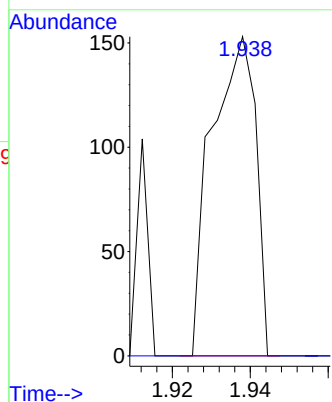

#11  
Allyl Chloride  
Concen: 0.016 ug/l  
RT: 2.915 min Scan# 490  
Delta R.T. -0.007 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 41 Resp: 272  
Ion Ratio Lower Upper  
41 100  
39 77.6 53.2 79.8









#13  
Acetone  
Concen: Below Cal  
RT: 2.649 min Scan# 407  
Delta R.T. 0.013 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 43 Resp: 1847  
Ion Ratio Lower Upper  
43 100  
58 28.3 26.2 39.2



#14  
Carbon Disulfide  
Concen: 0.046 ug/l  
RT: 2.790 min Scan# 451  
Delta R.T. -0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52


Tgt Ion: 76 Resp: 1610  
Ion Ratio Lower Upper  
76 100  
78 19.6 7.4 11.0#

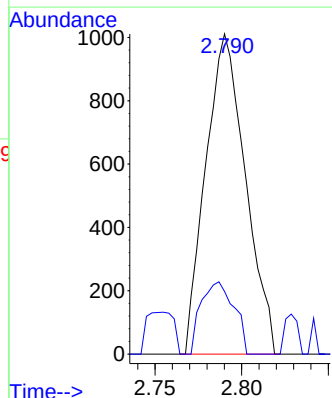






#15  
Methylene Chloride  
Concen: 0.953 ug/l  
RT: 3.051 min Scan# 51  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP



Tgt Ion: 84 Resp: 19569




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 49  | 122.8 | 104.6 | 157.0 |
| 51  | 39.7  | 0.0   | 81.4  |
| 86  | 65.6  | 52.6  | 78.8  |

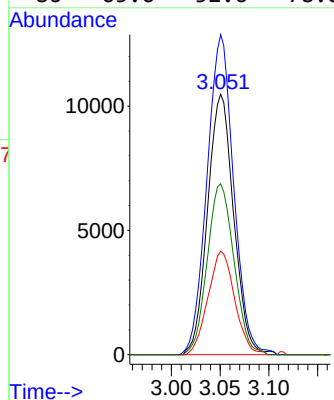


#16  
trans-1,2-Dichloroethene  
Concen: 0.006 ug/l  
RT: 3.356 min Scan# 627  
Delta R.T. -0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 96 Resp: 67

| Ion | Ratio | Lower | Upper  |
|-----|-------|-------|--------|
| 96  | 100   |       |        |
| 61  | 96.7  | 123.4 | 185.0# |
| 98  | 0.0   | 51.6  | 77.4#  |

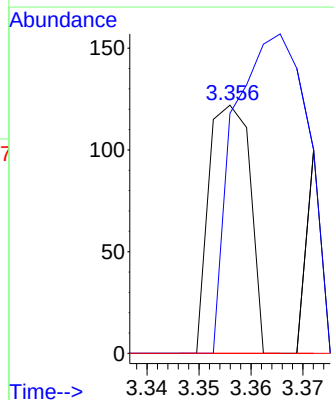









#18  
2-Butanone  
Concen: 0.280 ug/l  
RT: 4.755 min Scan# 1062  
Delta R.T. 0.016 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 43 Resp: 998  
Ion Ratio Lower Upper  
43 100  
57 0.0 0.0 18.0

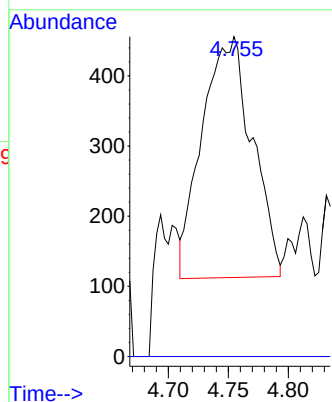

#19  
Cyclohexane  
Concen: 0.008 ug/l  
RT: 5.366 min Scan# 1252  
Delta R.T. -0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 56 Resp: 107  
Ion Ratio Lower Upper  
56 100  
69 0.0 24.2 36.4#  
84 67.3 63.4 95.2


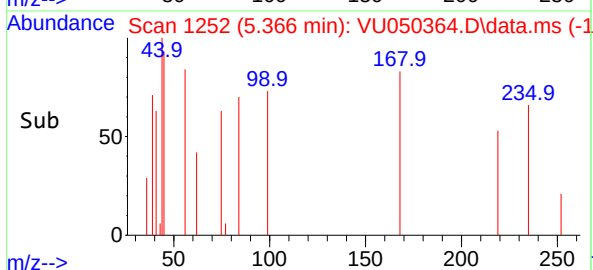






#21  
2,2-Dichloropropane  
Concen: 0.003 ug/l  
RT: 4.668 min Scan# 1035  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 77 Resp: 41  
Ion Ratio Lower Upper  
77 100  
97 0.0 18.5 27.7#



#24  
tert-Butyl Alcohol  
Concen: 2.912 ug/l  
RT: 3.202 min Scan# 579  
Delta R.T. -0.023 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 59 Resp: 3686  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.2 12.2#




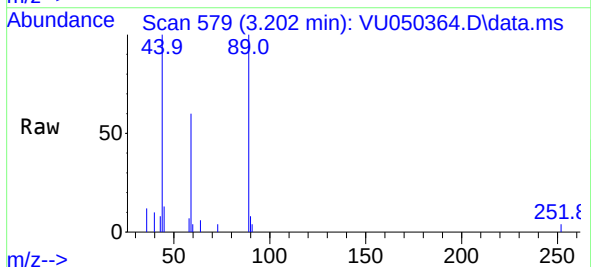




#25  
Methyl tert-Butyl Ether  
Concen: 0.006 ug/l  
RT: 3.202 min Scan# 51  
Delta R.T. -0.183 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 73 Resp: 185  
Ion Ratio Lower Upper  
73 100  
43 354.1 15.9 23.9#

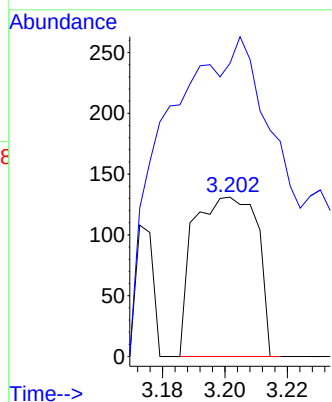

#27  
Chloroform  
Concen: 0.031 ug/l  
RT: 5.086 min Scan# 1165  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 83 Resp: 661  
Ion Ratio Lower Upper  
83 100  
85 49.8 0.0 133.6





#28

1,1,1-Trichloroethane

Concen: 0.001 ug/l

RT: 5.301 min Scan# 11

Delta R.T. -0.006 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :

WS-EDB-DBCP-TCP





Tgt Ion: 97 Resp: 22

Ion Ratio Lower Upper

97 100

99 745.5 32.1 96.5#

61 427.3 21.8 65.4#

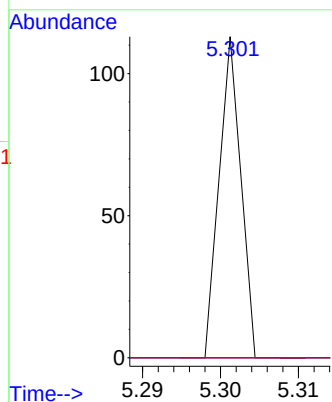

#29

1,1-Dichloropropene

Concen: 0.008 ug/l

RT: 5.536 min Scan# 1305

Delta R.T. 0.019 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52




Tgt Ion: 75 Resp: 102


Ion Ratio Lower Upper

75 100

110 0.0 17.3 52.0#

77 107.8 24.6 37.0#


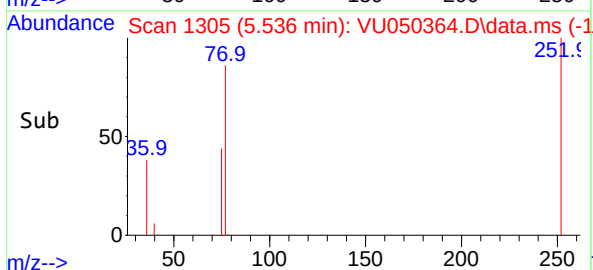






#31  
Isopropyl Ether  
Concen: 0.007 ug/l  
RT: 4.221 min Scan# 896  
Delta R.T. 0.196 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 45 Resp: 219  
Ion Ratio Lower Upper  
45 100  
43 57.5 23.8 71.2



#32  
Ethyl-t-butyl ether  
Concen: 0.012 ug/l  
RT: 4.726 min Scan# 1053  
Delta R.T. 0.196 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 59 Resp: 306  
Ion Ratio Lower Upper  
59 100  
87 0.0 32.5 48.7#









#33  
Tert-Amyl methyl ether  
Concen: 0.021 ug/l  
RT: 6.121 min Scan# 1437  
Delta R.T. 0.161 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 73 Resp: 379  
Ion Ratio Lower Upper  
73 100  
87 0.0 19.7 29.5#  
71 40.9 9.0 13.4#

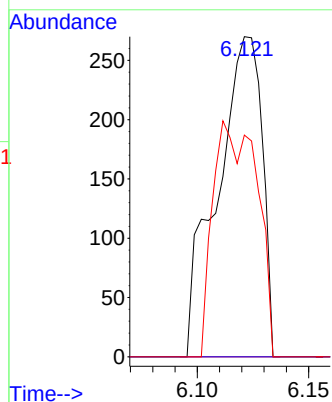

#34  
Propionitrile  
Concen: 0.017 ug/l  
RT: 4.822 min Scan# 1083  
Delta R.T. 0.019 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 54 Resp: 20  
Ion Ratio Lower Upper  
54 100  
52 0.0 15.0 22.6#  
55 0.0 12.6 19.0#  
40 265.0 4.2 6.4#


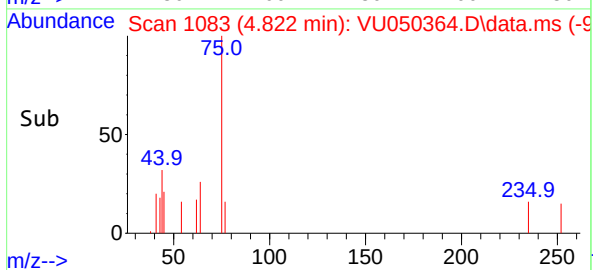

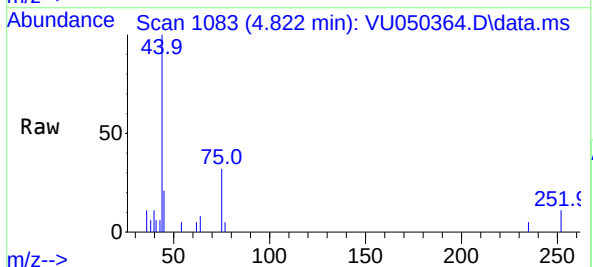




#35  
Benzene  
Concen: 0.006 ug/l  
RT: 5.758 min Scan# 11  
Delta R.T. -0.013 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 78 Resp: 266  
Ion Ratio Lower Upper  
78 100  
77 23.4 18.6 28.0



#36  
1,2-Dichloroethane  
Concen: 0.001 ug/l  
RT: 5.809 min Scan# 1390  
Delta R.T. 0.010 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 62 Resp: 19  
Ion Ratio Lower Upper  
62 100  
98 0.0 7.4 11.0#



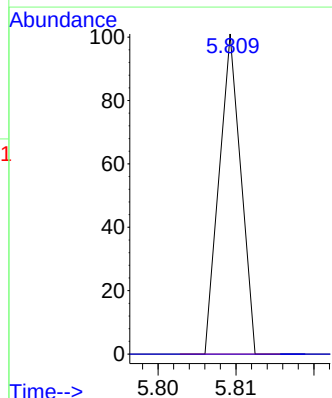
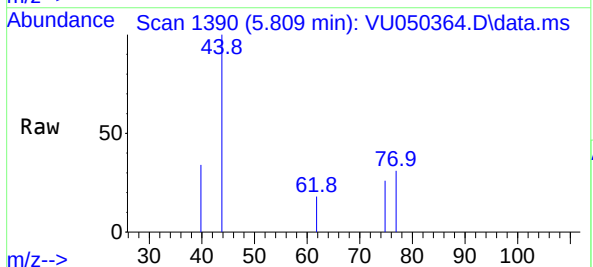




#37  
Trichloroethene  
Concen: 0.006 ug/l  
RT: 6.552 min Scan# 1  
Delta R.T. -0.016 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP

Tgt Ion:130 Resp: 67  
Ion Ratio Lower Upper  
130 100  
95 0.0 83.8 125.8#

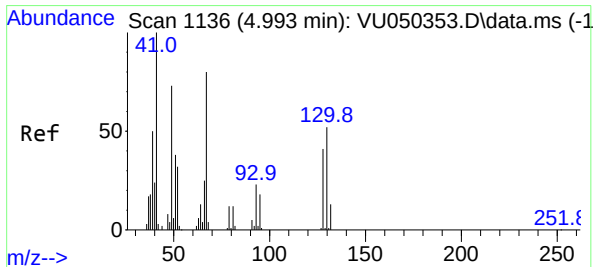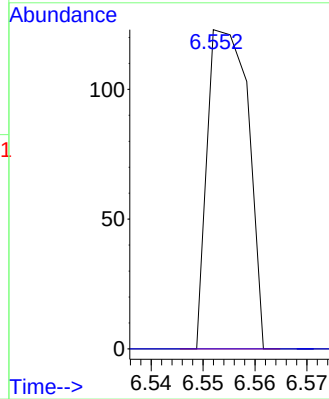


#39  
Methacrylonitrile  
Concen: 0.032 ug/l  
RT: 4.986 min Scan# 1134  
Delta R.T. -0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 41 Resp: 123  
Ion Ratio Lower Upper  
41 100  
67 0.0 59.4 89.0#  
39 16.3 42.2 63.2#  
52 0.0 23.7 35.5#

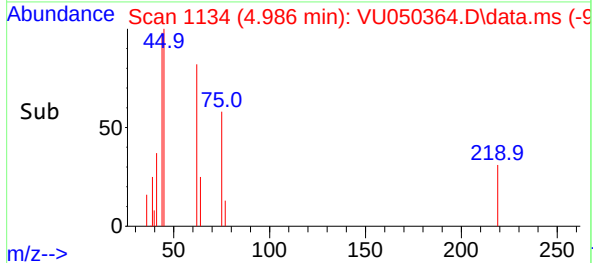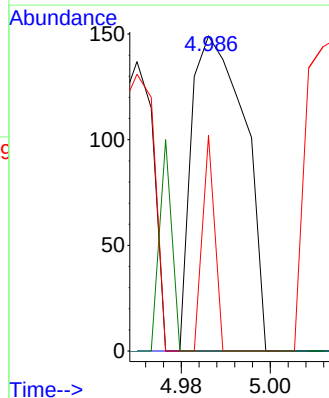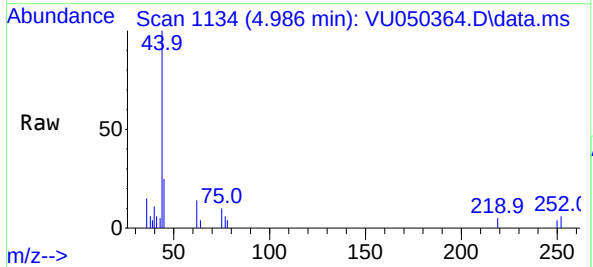









#40  
Methyl acrylate  
Concen: 0.006 ug/l  
RT: 5.012 min Scan# 1142  
Delta R.T. 0.148 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 55    | Resp: | 43    |
| Ion      | Ratio | Lower | Upper |
| 55       | 100   |       |       |
| 85       | 0.0   | 13.5  | 20.3# |
| 58       | 0.0   | 7.0   | 10.4# |
| 42       | 186.0 | 7.0   | 10.6# |

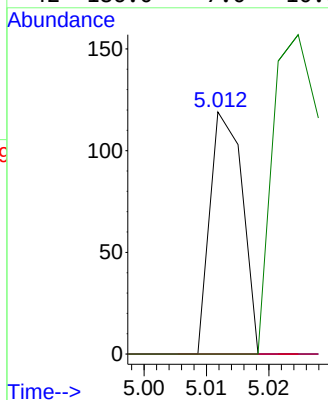

#41  
Tetrahydrofuran  
Concen: 0.094 ug/l  
RT: 5.089 min Scan# 1166  
Delta R.T. 0.010 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 202   |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 37.1  | 38.9  | 58.3# |
| 71       | 0.0   | 33.7  | 50.5# |



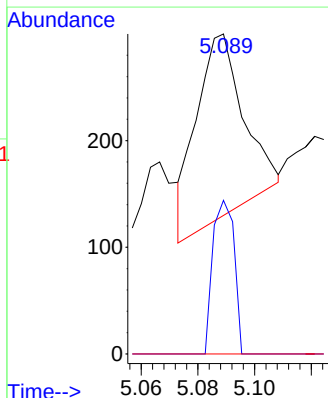





#42  
1-Chlorobutane  
Concen: 0.005 ug/l  
RT: 5.443 min Scan# 11  
Delta R.T. -0.010 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 56 Resp: 92  
Ion Ratio Lower Upper  
56 100  
41 137.0 26.4 79.2#

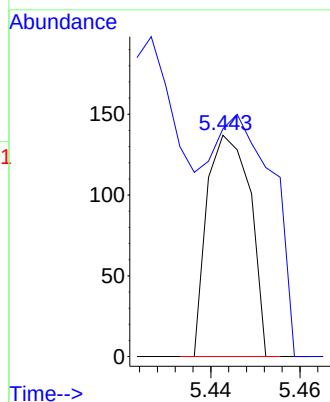

#44  
Bromodichloromethane  
Concen: 0.003 ug/l  
RT: 7.118 min Scan# 1797  
Delta R.T. -0.013 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 83 Resp: 41  
Ion Ratio Lower Upper  
83 100  
85 0.0 49.4 74.0#  
127 0.0 6.6 10.0#

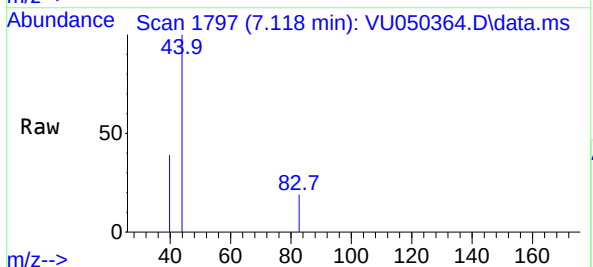



#45

4-Methyl-2-Pentanone

Concen: 0.087 ug/l

RT: 7.828 min Scan# 2015

Delta R.T. 0.010 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :

WS-EDB-DBCP-TCP





Tgt Ion: 43 Resp: 629

Ion Ratio Lower Upper

43 100

58 11.9 20.3 61.0#

85 0.0 14.6 21.8#

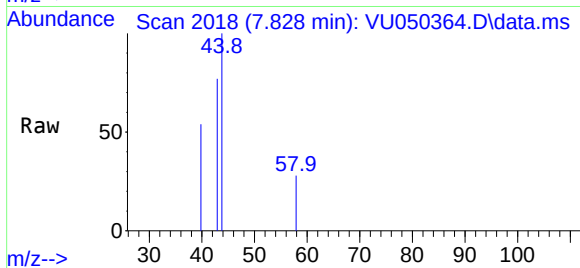

#46

t-1,4-Dichloro-2-butene

Concen: 7.277 ug/l

RT: 10.828 min Scan# 2951

Delta R.T. -0.006 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Tgt Ion: 75 Resp: 17396




Ion Ratio Lower Upper


75 100

53 0.0 64.4 96.6#

89 0.0 44.2 66.2#

88 0.0 32.8 49.2#

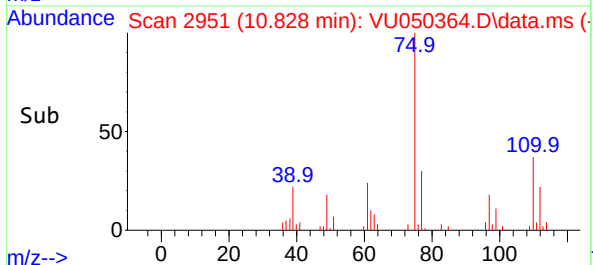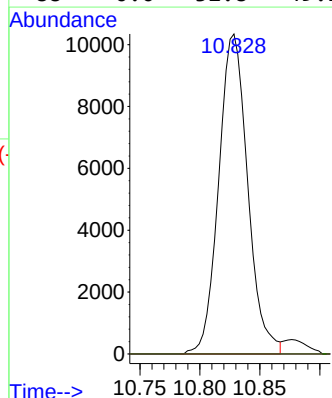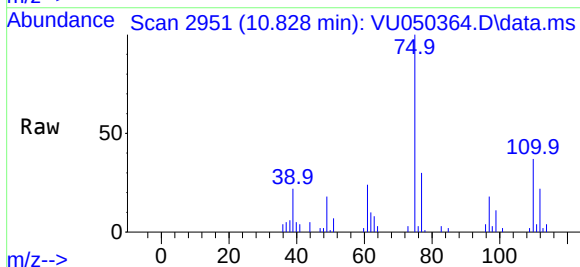



#49

Toluene

Concen: 0.006 ug/l

RT: 7.983 min Scan# 2067

Delta R.T. -0.003 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :





WS-EDB-DBCP-TCP

Tgt Ion: 92 Resp: 147

Ion Ratio Lower Upper

92 100

91 211.6 138.6 207.8#

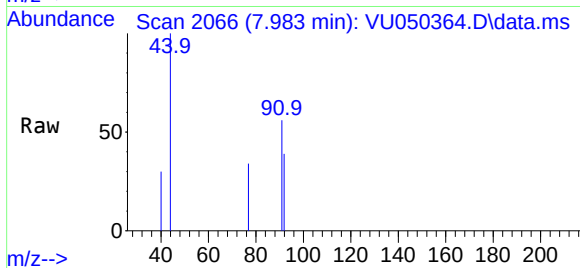

#54

2-Hexanone

Concen: 0.113 ug/l

RT: 8.719 min Scan# 2295

Delta R.T. 0.016 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52




Tgt Ion: 43 Resp: 556


Ion Ratio Lower Upper

43 100

58 23.6 37.1 77.1#

57 0.0 0.0 39.5


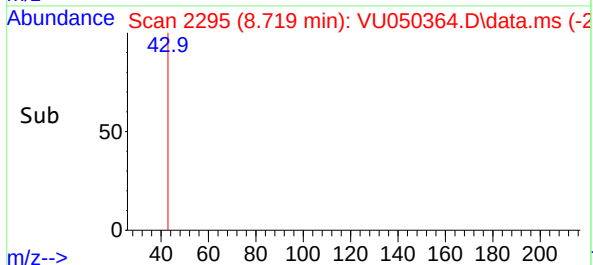
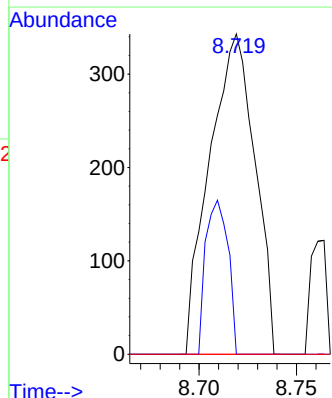
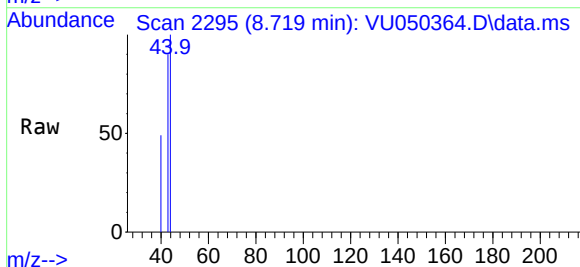




#56  
1,2-Dibromoethane  
Concen: 1.764 ug/l  
RT: 8.935 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion:107 Resp: 15086  
Ion Ratio Lower Upper  
107 100  
109 95.4 0.0 187.2

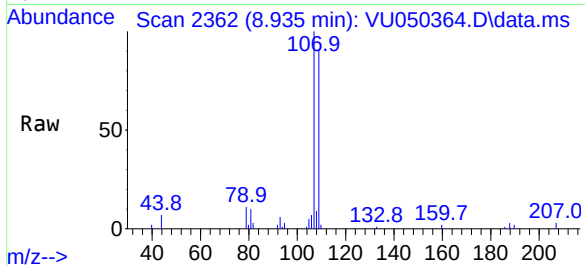

#57  
4-Bromofluorobenzene  
Concen: 0.690 ug/l  
RT: 10.639 min Scan# 2892  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52


Tgt Ion: 95 Resp: 8583  
Ion Ratio Lower Upper  
95 100  
174 84.5 62.4 93.6  
176 84.3 56.2 84.2#

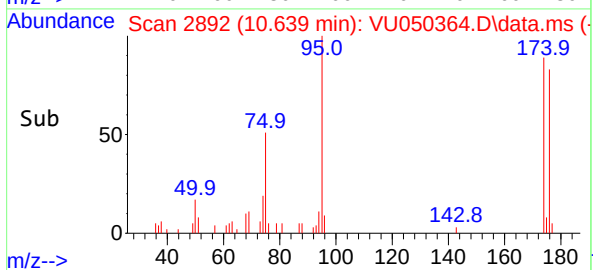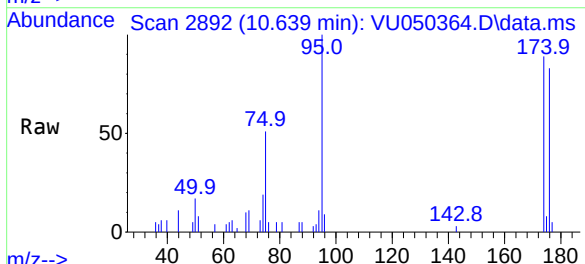

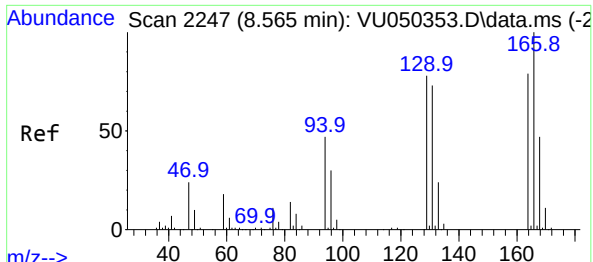




#58  
Tetrachloroethene  
Concen: 0.006 ug/l  
RT: 8.558 min Scan# 21  
Delta R.T. -0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP

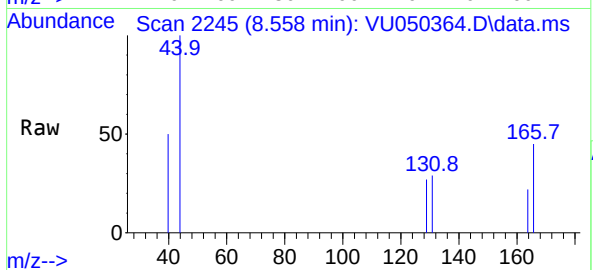

Tgt Ion:164 Resp: 59




| Ion | Ratio | Lower | Upper  |
|-----|-------|-------|--------|
| 164 | 100   |       |        |
| 166 | 201.9 | 102.4 | 153.6# |
| 129 | 120.4 | 79.5  | 119.3# |
| 131 | 130.1 | 77.4  | 116.2# |

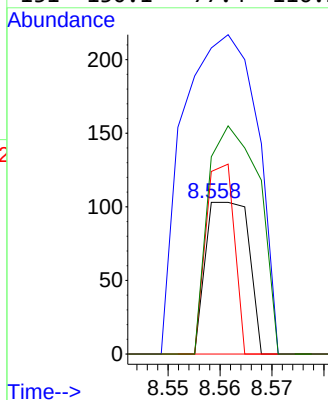


#59  
Chlorobenzene  
Concen: 0.011 ug/l  
RT: 9.455 min Scan# 2524  
Delta R.T. 0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion:112 Resp: 297

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 112 | 100   |       |       |
| 114 | 69.0  | 24.9  | 37.3# |

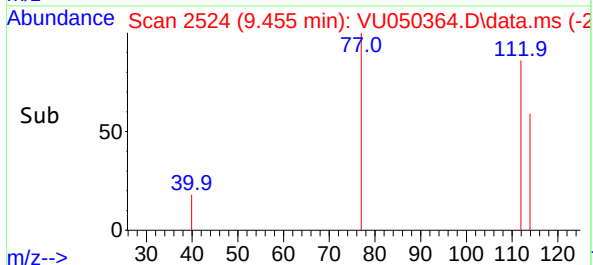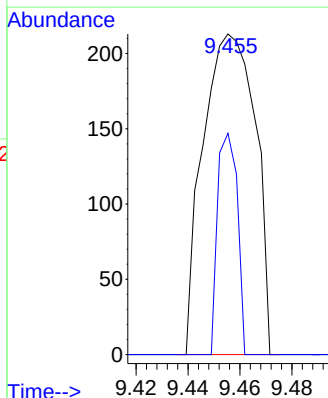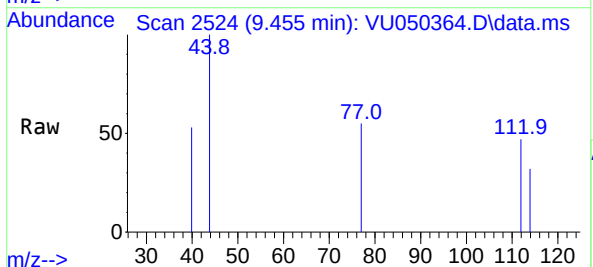



#63

Ethyl Benzene

Concen: 0.446 ug/l

RT: 9.574 min Scan# 21

Delta R.T. -0.004 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :





WS-EDB-DBCP-TCP

Tgt Ion: 91 Resp: 497

Ion Ratio Lower Upper

91 100

106 0.0 24.4 36.6#

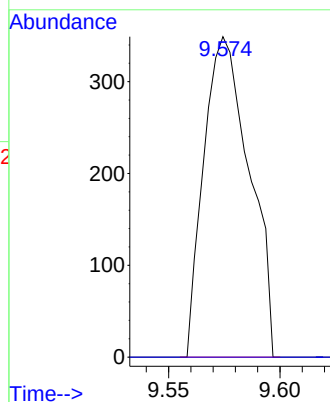

#64

m/p-Xylenes

Concen: 0.821 ug/l

RT: 9.700 min Scan# 2600

Delta R.T. -0.000 min

Lab File: VU050364.D




Acq: 17 Aug 2022 19:52


Tgt Ion: 106 Resp: 317

Ion Ratio Lower Upper

106 100

91 247.9 167.8 251.6









#65  
o-Xylene  
Concen: 0.359 ug/l  
RT: 10.098 min Scan# 21  
Delta R.T. -0.007 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP

Tgt Ion:106 Resp: 75  
Ion Ratio Lower Upper  
106 100  
91 477.3 111.1 333.2#




#66  
Styrene  
Concen: 0.474 ug/l  
RT: 10.124 min Scan# 2732  
Delta R.T. 0.006 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion:104 Resp: 298  
Ion Ratio Lower Upper  
104 100  
78 20.5 42.1 63.1#  
103 41.9 44.5 66.7#











#68  
1,2-Dichlorobenzene-d4  
Concen: 0.710 ug/l  
RT: 12.195 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion:152 Resp: 10484  
Ion Ratio Lower Upper  
152 100  
115 67.3 0.0 254.6  
150 160.9 0.0 623.6

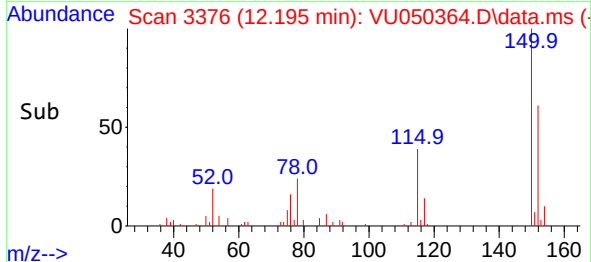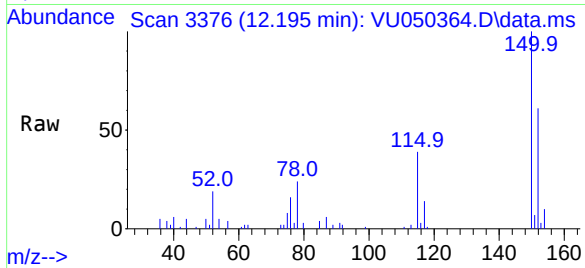

#69  
Isopropylbenzene  
Concen: 0.456 ug/l  
RT: 10.488 min Scan# 2845  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion:105 Resp: 504  
Ion Ratio Lower Upper  
105 100  
120 17.5 12.6 37.8


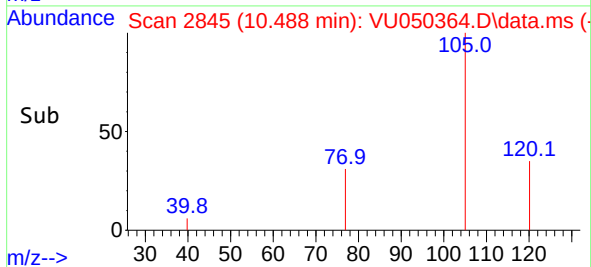

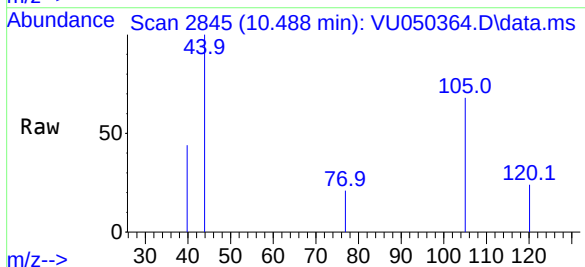




#70  
1,1,2,2-Tetrachloroethane  
Concen: 0.003 ug/l  
RT: 10.790 min Scan# 2939  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 83 Resp: 42  
Ion Ratio Lower Upper  
83 100  
131 0.0 7.7 11.5#  
85 0.0 51.2 76.8#

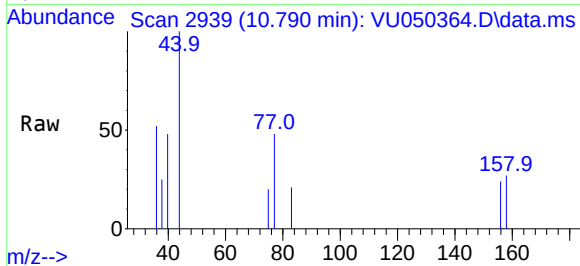

#71  
1,2,3-Trichloropropane  
Concen: 1.817 ug/l  
RT: 10.828 min Scan# 2951  
Delta R.T. 0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 75 Resp: 17396  
Ion Ratio Lower Upper  
75 100  
77 30.4 0.0 112.4  
110 36.4 0.0 70.6  
97 17.7 0.0 37.4




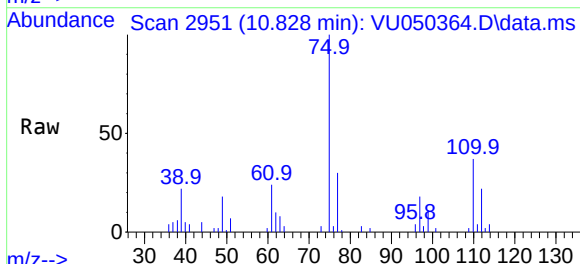




#72  
Bromobenzene  
Concen: 0.009 ug/l  
RT: 10.787 min Scan# 2938  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 156   | Resp: | 96    |
| Ion      | Ratio | Lower | Upper |
| 156      | 100   |       |       |
| 77       | 226.0 | 0.0   | 344.4 |
| 158      | 111.5 | 0.0   | 192.2 |

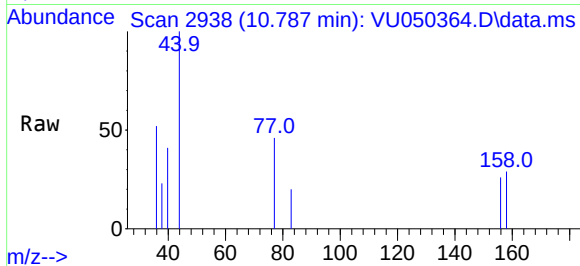

#73  
n-propylbenzene  
Concen: 0.515 ug/l  
RT: 10.912 min Scan# 2977  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 120   | Resp: | 113    |
| Ion      | Ratio | Lower | Upper  |
| 120      | 100   |       |        |
| 91       | 926.5 | 367.8 | 551.6# |




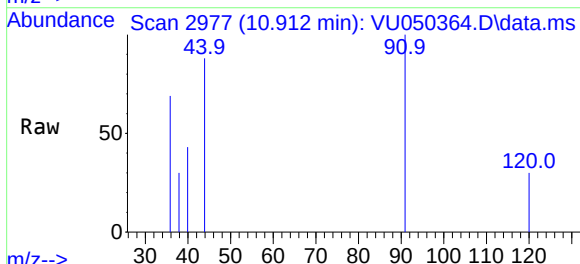




#74  
2-Chlorotoluene  
Concen: 0.313 ug/l  
RT: 10.989 min Scan# 3001  
Delta R.T. 0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion:126 Resp: 161  
Ion Ratio Lower Upper  
126 100  
91 337.3 0.0 620.6

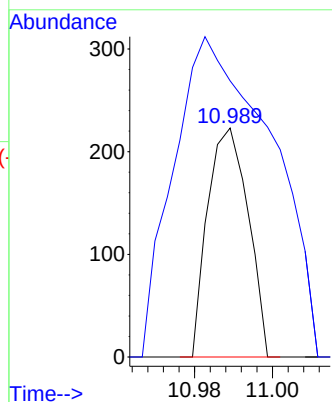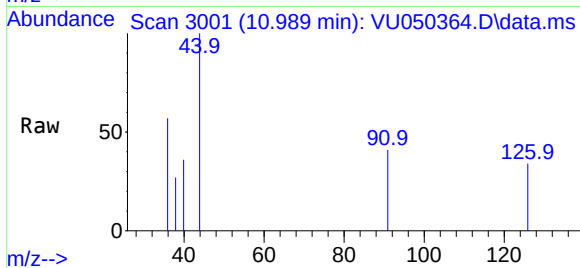

#75  
1,3,5-Trimethylbenzene  
Concen: 0.449 ug/l  
RT: 11.092 min Scan# 3033  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion:105 Resp: 550  
Ion Ratio Lower Upper  
105 100  
120 37.6 37.6 56.4


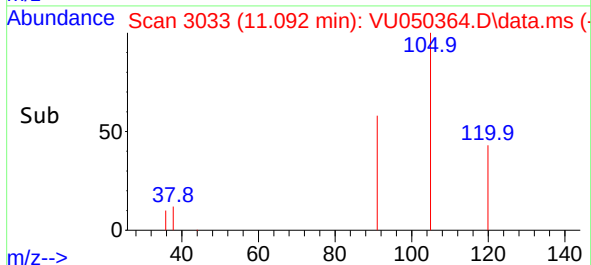

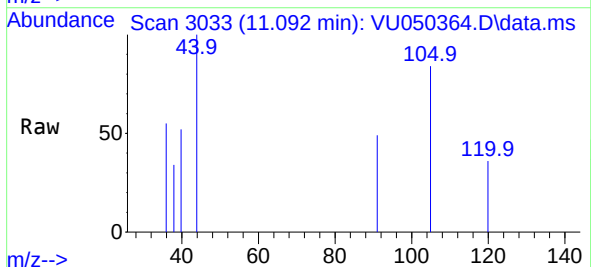




#76  
4-Chlorotoluene  
Concen: 0.009 ug/l  
RT: 11.105 min Scan# 3036  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion:126 Resp: 94  
Ion Ratio Lower Upper  
126 100  
91 628.7 0.0 738.8

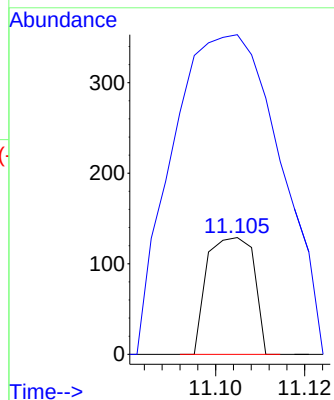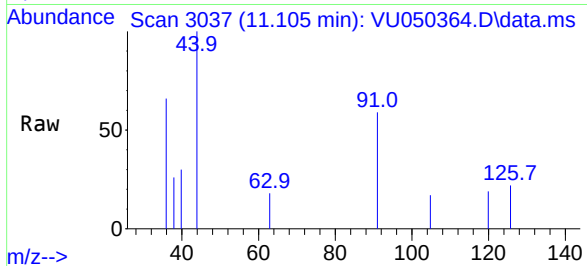

#77  
tert-Butylbenzene  
Concen: 0.388 ug/l  
RT: 11.420 min Scan# 3135  
Delta R.T. -0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion:119 Resp: 437  
Ion Ratio Lower Upper  
119 100  
91 58.1 30.4 91.3  
134 0.0 17.8 26.6#

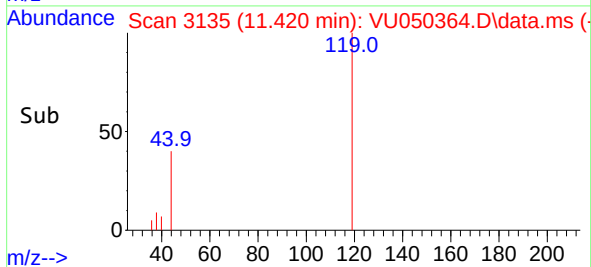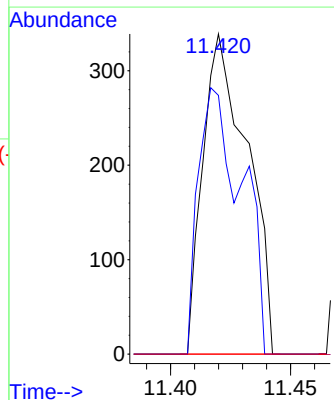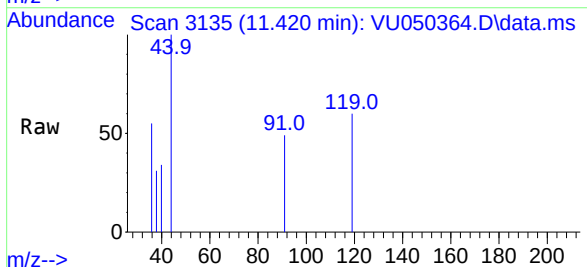



#78

1,2,4-Trimethylbenzene

Concen: 0.383 ug/l

RT: 11.471 min Scan# 3150

Delta R.T. 0.003 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :





WS-EDB-DBCP-TCP

Tgt Ion:105 Resp: 709

Ion Ratio Lower Upper

105 100

120 34.4 21.6 65.0

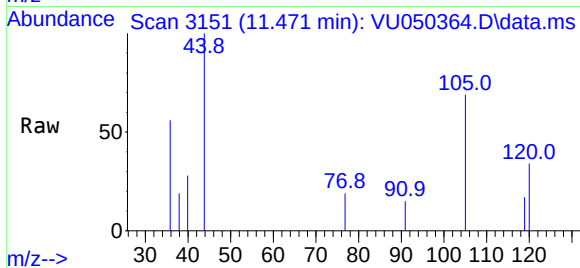

#79

sec-Butylbenzene

Concen: 0.449 ug/l

RT: 11.645 min Scan# 3205

Delta R.T. 0.000 min

Lab File: VU050364.D




Acq: 17 Aug 2022 19:52


Tgt Ion:105 Resp: 1099

Ion Ratio Lower Upper

105 100

134 6.3 15.4 23.0#


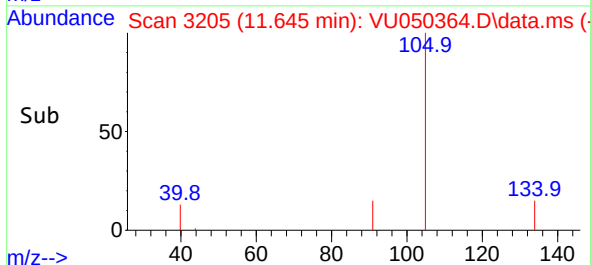
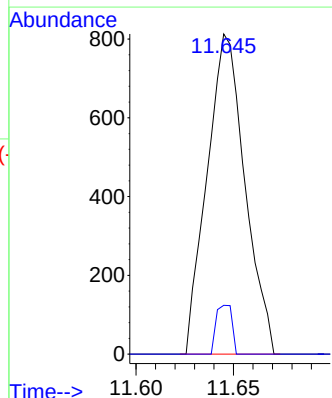
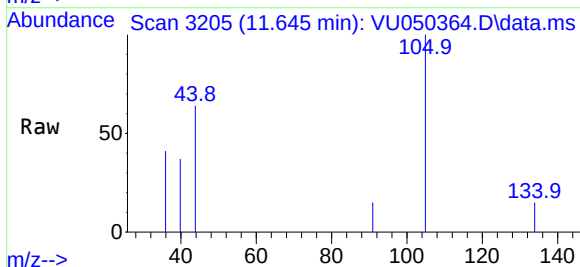




#80  
Nitrobenzene  
Concen: 0.082 ug/l  
RT: 13.211 min Scan# 30  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 77 Resp: 68  
Ion Ratio Lower Upper  
77 100  
123 0.0 18.1 64.3#  
65 0.0 10.8 13.8#



#81  
p-Isopropyltoluene  
Concen: 0.017 ug/l  
RT: 11.793 min Scan# 3251  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

Tgt Ion: 119 Resp: 1067  
Ion Ratio Lower Upper  
119 100  
134 14.1 20.5 30.7#  
91 10.1 19.8 29.6#





#82

1,3-Dichlorobenzene

Concen: 0.035 ug/l

RT: 11.748 min Scan# 3237

Delta R.T. -0.000 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :

WS-EDB-DBCP-TCP





Tgt Ion:146 Resp: 813

Ion Ratio Lower Upper

146 100

111 19.3 33.4 50.2#

148 42.6 51.2 76.8#

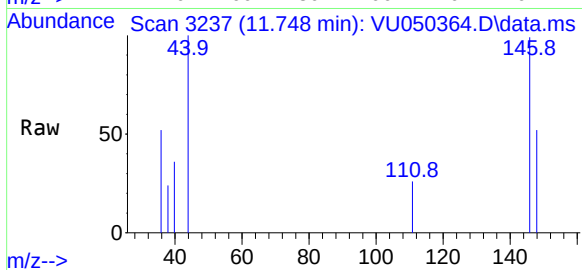

#83

1,4-Dichlorobenzene

Concen: 0.036 ug/l

RT: 11.841 min Scan# 3266

Delta R.T. 0.003 min

Lab File: VU050364.D

Acq: 17 Aug 2022 19:52




Tgt Ion:146 Resp: 866

Ion Ratio Lower Upper


146 100

111 37.8 32.6 49.0

148 43.0 51.6 77.4#

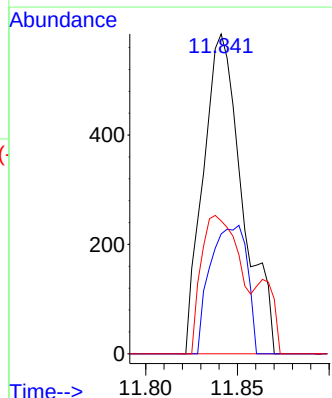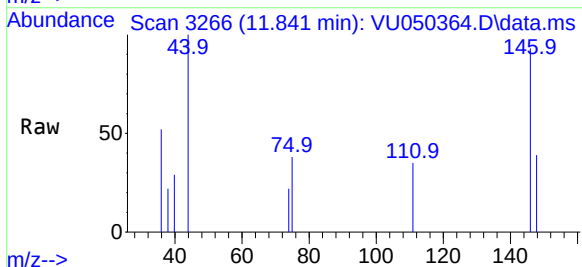









#84  
n-Butylbenzene  
Concen: 0.519 ug/l  
RT: 12.211 min Scan# 3381  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


|             |       |            |
|-------------|-------|------------|
| Tgt Ion: 91 | Resp: | 2242       |
| Ion Ratio   | Lower | Upper      |
| 91          | 100   |            |
| 92          | 40.5  | 42.3 63.5# |
| 134         | 20.8  | 19.6 29.4  |

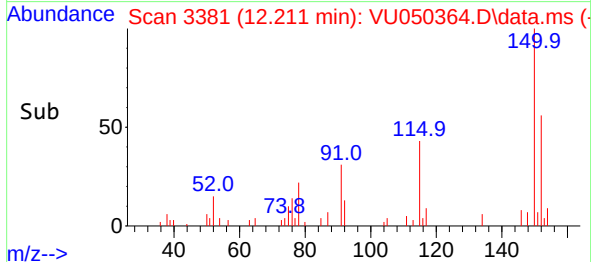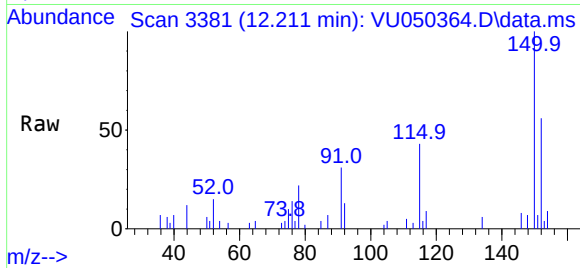

#85  
1,2-Dichlorobenzene  
Concen: 0.029 ug/l  
RT: 12.217 min Scan# 3383  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

|              |       |           |
|--------------|-------|-----------|
| Tgt Ion: 146 | Resp: | 663       |
| Ion Ratio    | Lower | Upper     |
| 146          | 100   |           |
| 111          | 51.9  | 22.1 66.1 |
| 148          | 77.8  | 32.1 96.3 |


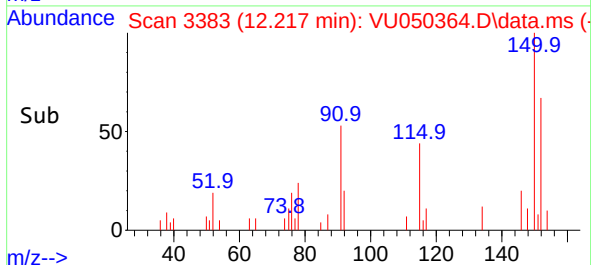
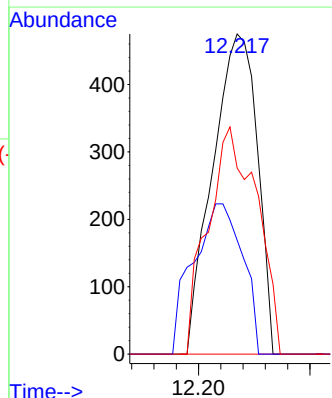
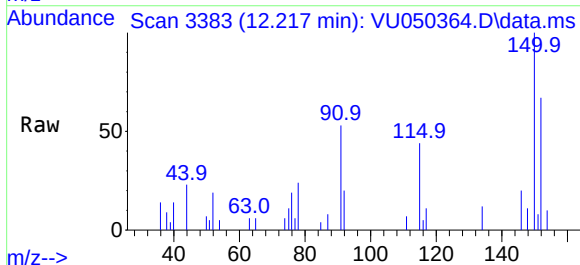




#86  
1,2-Dibromo-3-Chloropropane  
Concen: 0.597 ug/l  
RT: 13.002 min Scan# 30  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52




Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP


Tgt Ion: 75 Resp: 1288  
Ion Ratio Lower Upper  
75 100  
155 72.5 66.8 100.2  
157 94.3 83.8 125.8



#87  
1,2,4-Trichlorobenzene  
Concen: 0.428 ug/l  
RT: 13.844 min Scan# 3889  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52


Tgt Ion:180 Resp: 1578  
Ion Ratio Lower Upper  
180 100  
182 100.4 77.0 115.6  
145 11.3 25.7 38.5#

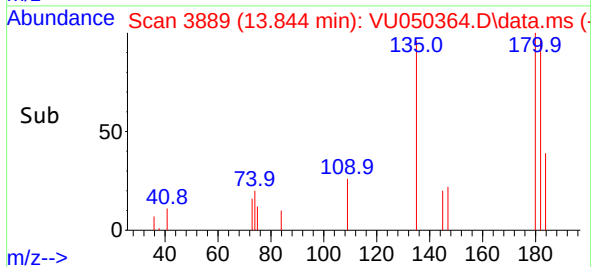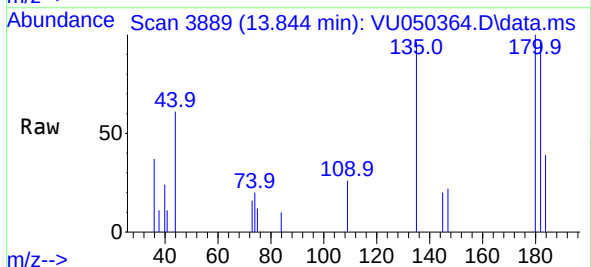






#88  
Hexachlorobutadiene  
Concen: 0.064 ug/l  
RT: 14.021 min Scan# 3944  
Delta R.T. -0.000 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52


Instrument :  
MSVOA\_U  
ClientSampleId :  
WS-EDB-DBCP-TCP

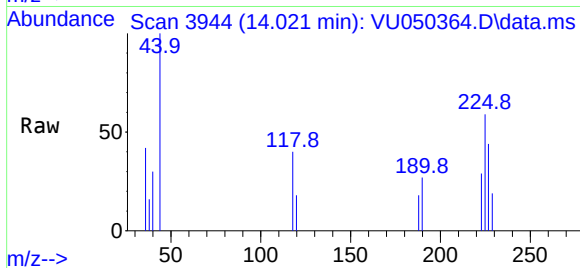



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 225   | Resp: | 536   |
| Ion      | Ratio | Lower | Upper |
| 225      | 100   |       |       |
| 223      | 59.7  | 50.6  | 76.0  |
| 227      | 61.9  | 50.7  | 76.1  |

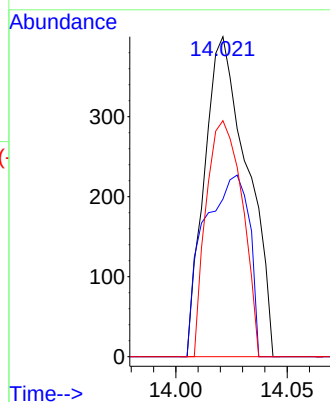


#89  
Naphthalene  
Concen: 0.961 ug/l  
RT: 14.092 min Scan# 3966  
Delta R.T. 0.003 min  
Lab File: VU050364.D  
Acq: 17 Aug 2022 19:52

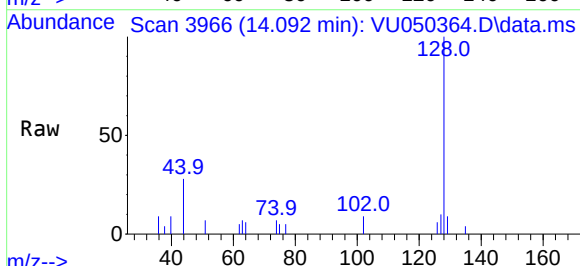

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 128   | Resp: | 4576  |
| Ion      | Ratio | Lower | Upper |
| 128      | 100   |       |       |
| 127      | 10.3  | 10.1  | 15.1  |
| 129      | 6.9   | 8.6   | 12.8  |





#90

1,2,3-Trichlorobenzene

Concen: 0.453 ug/l

RT: 14.333 min Scan# 40

Delta R.T. 0.003 min

Lab File: VU050364.D


Acq: 17 Aug 2022 19:52

Instrument :

MSVOA\_U

ClientSampleId :

WS-EDB-DBCP-TCP



Tgt Ion:180 Resp: 1776

Ion Ratio Lower Upper

180 100

182 95.9 76.6 114.8

145 32.6 27.3 40.9

