


Acetone

Response Ratio

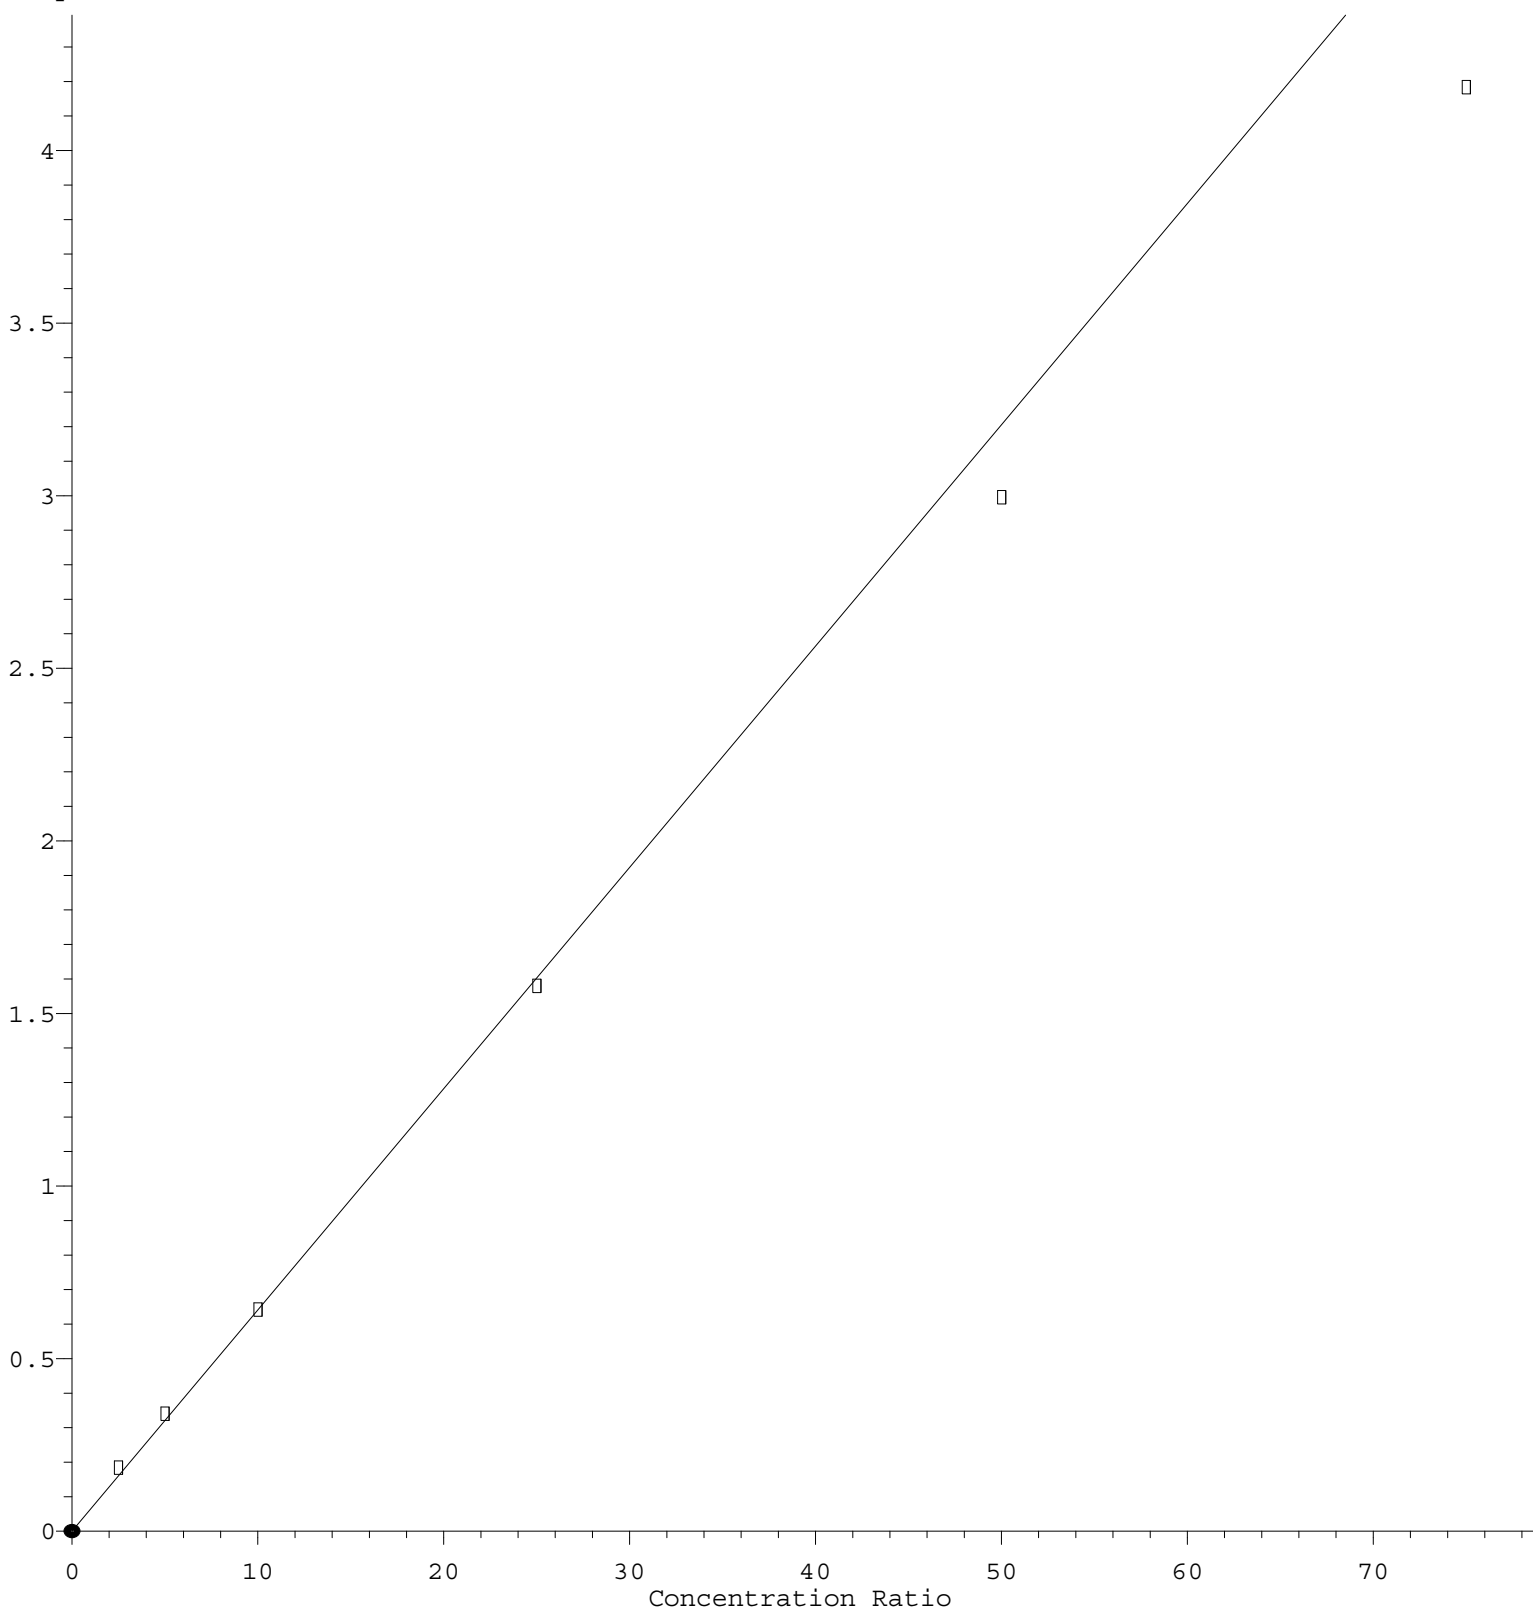

$$\text{Response} = 6.412\text{e-}002 * \text{Amt}$$


RF Rel Std Dev = 9.692% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

m/p-Xylenes

Response Ratio

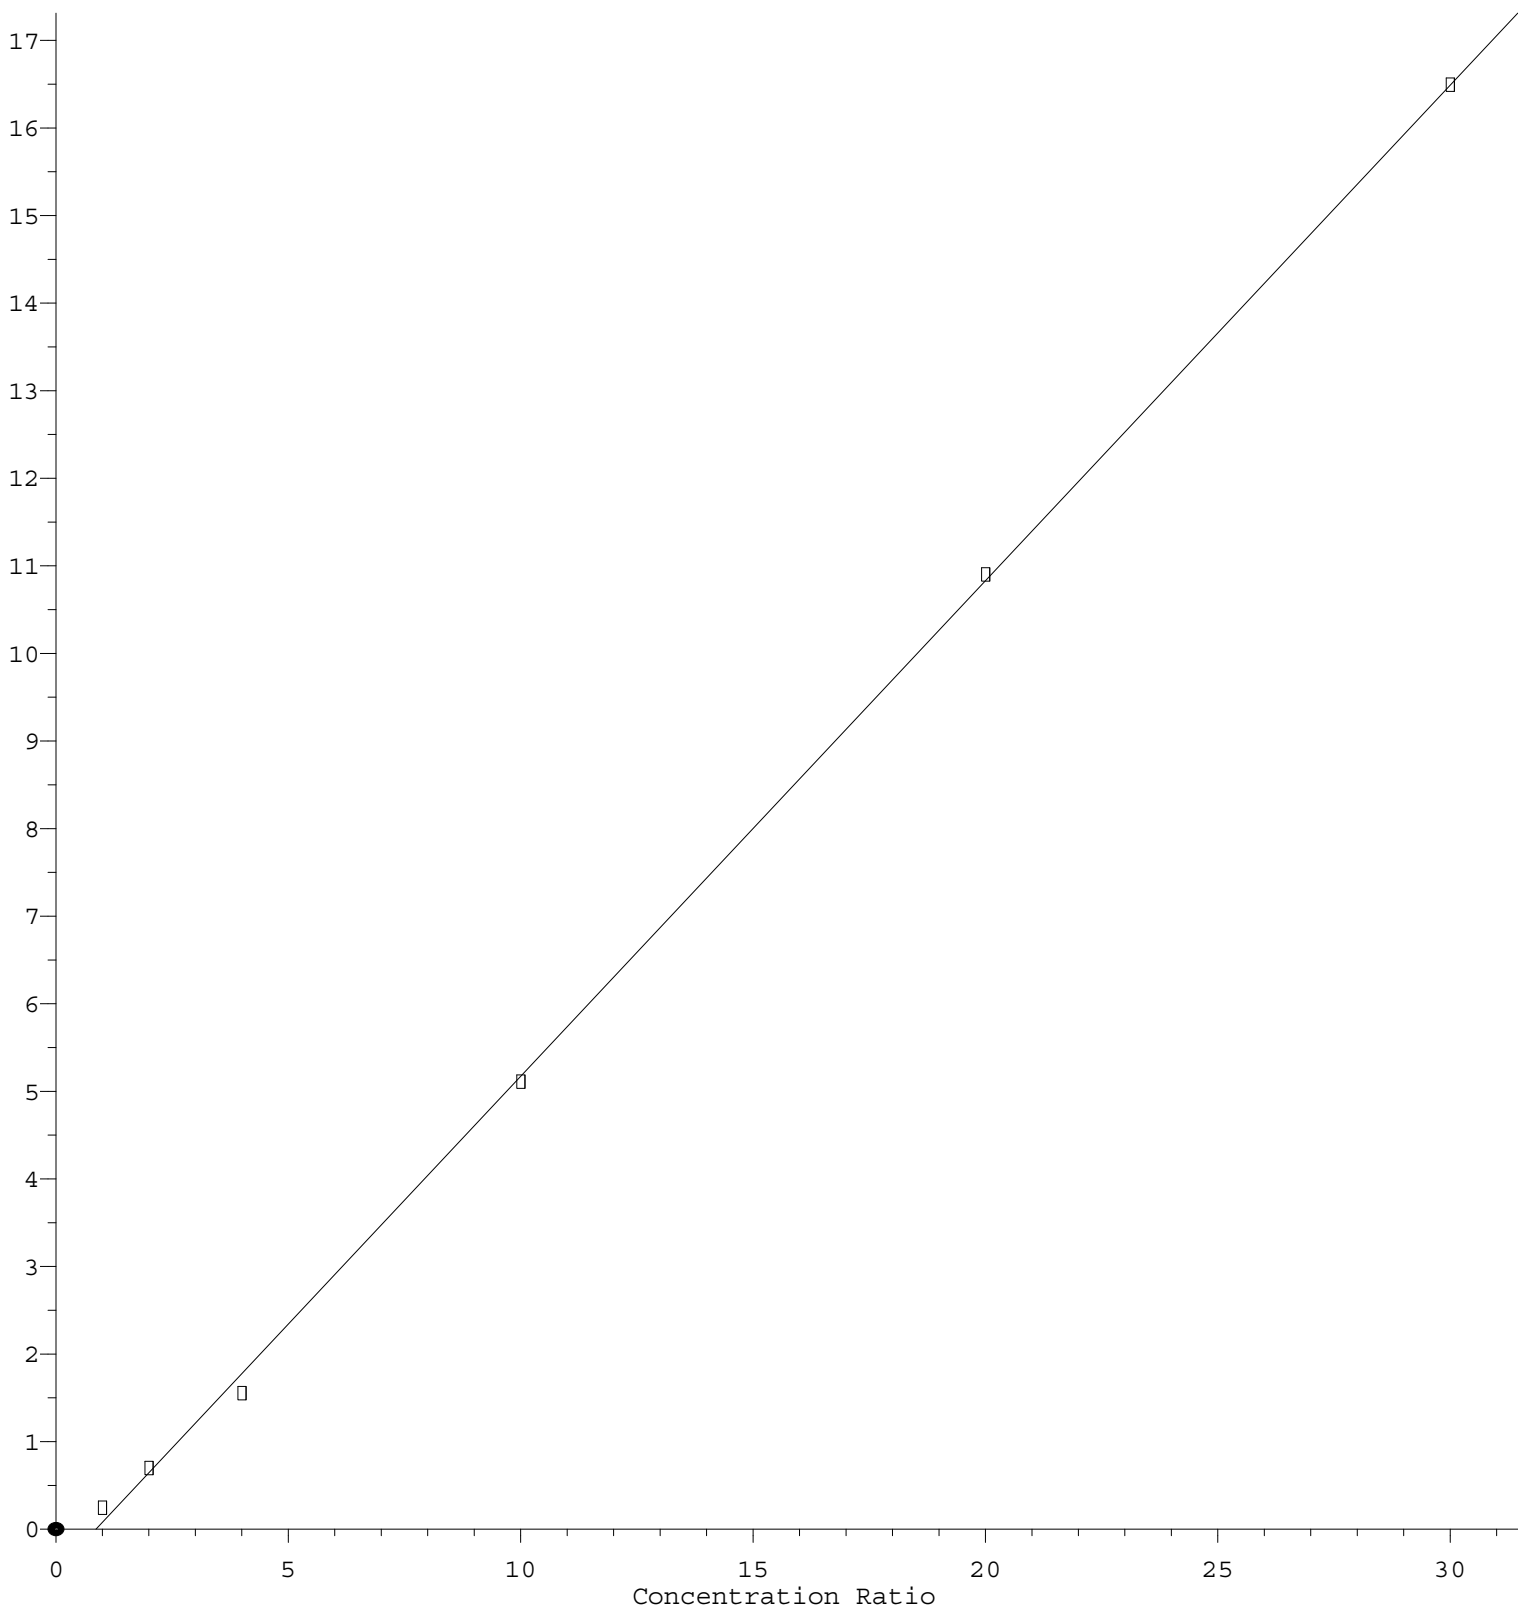

$$\text{Response} = 5.662\text{e-}001 * \text{Amt} - 4.887\text{e-}001$$


Coef of Det (r^2) = 0.999588 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

Styrene

Response Ratio

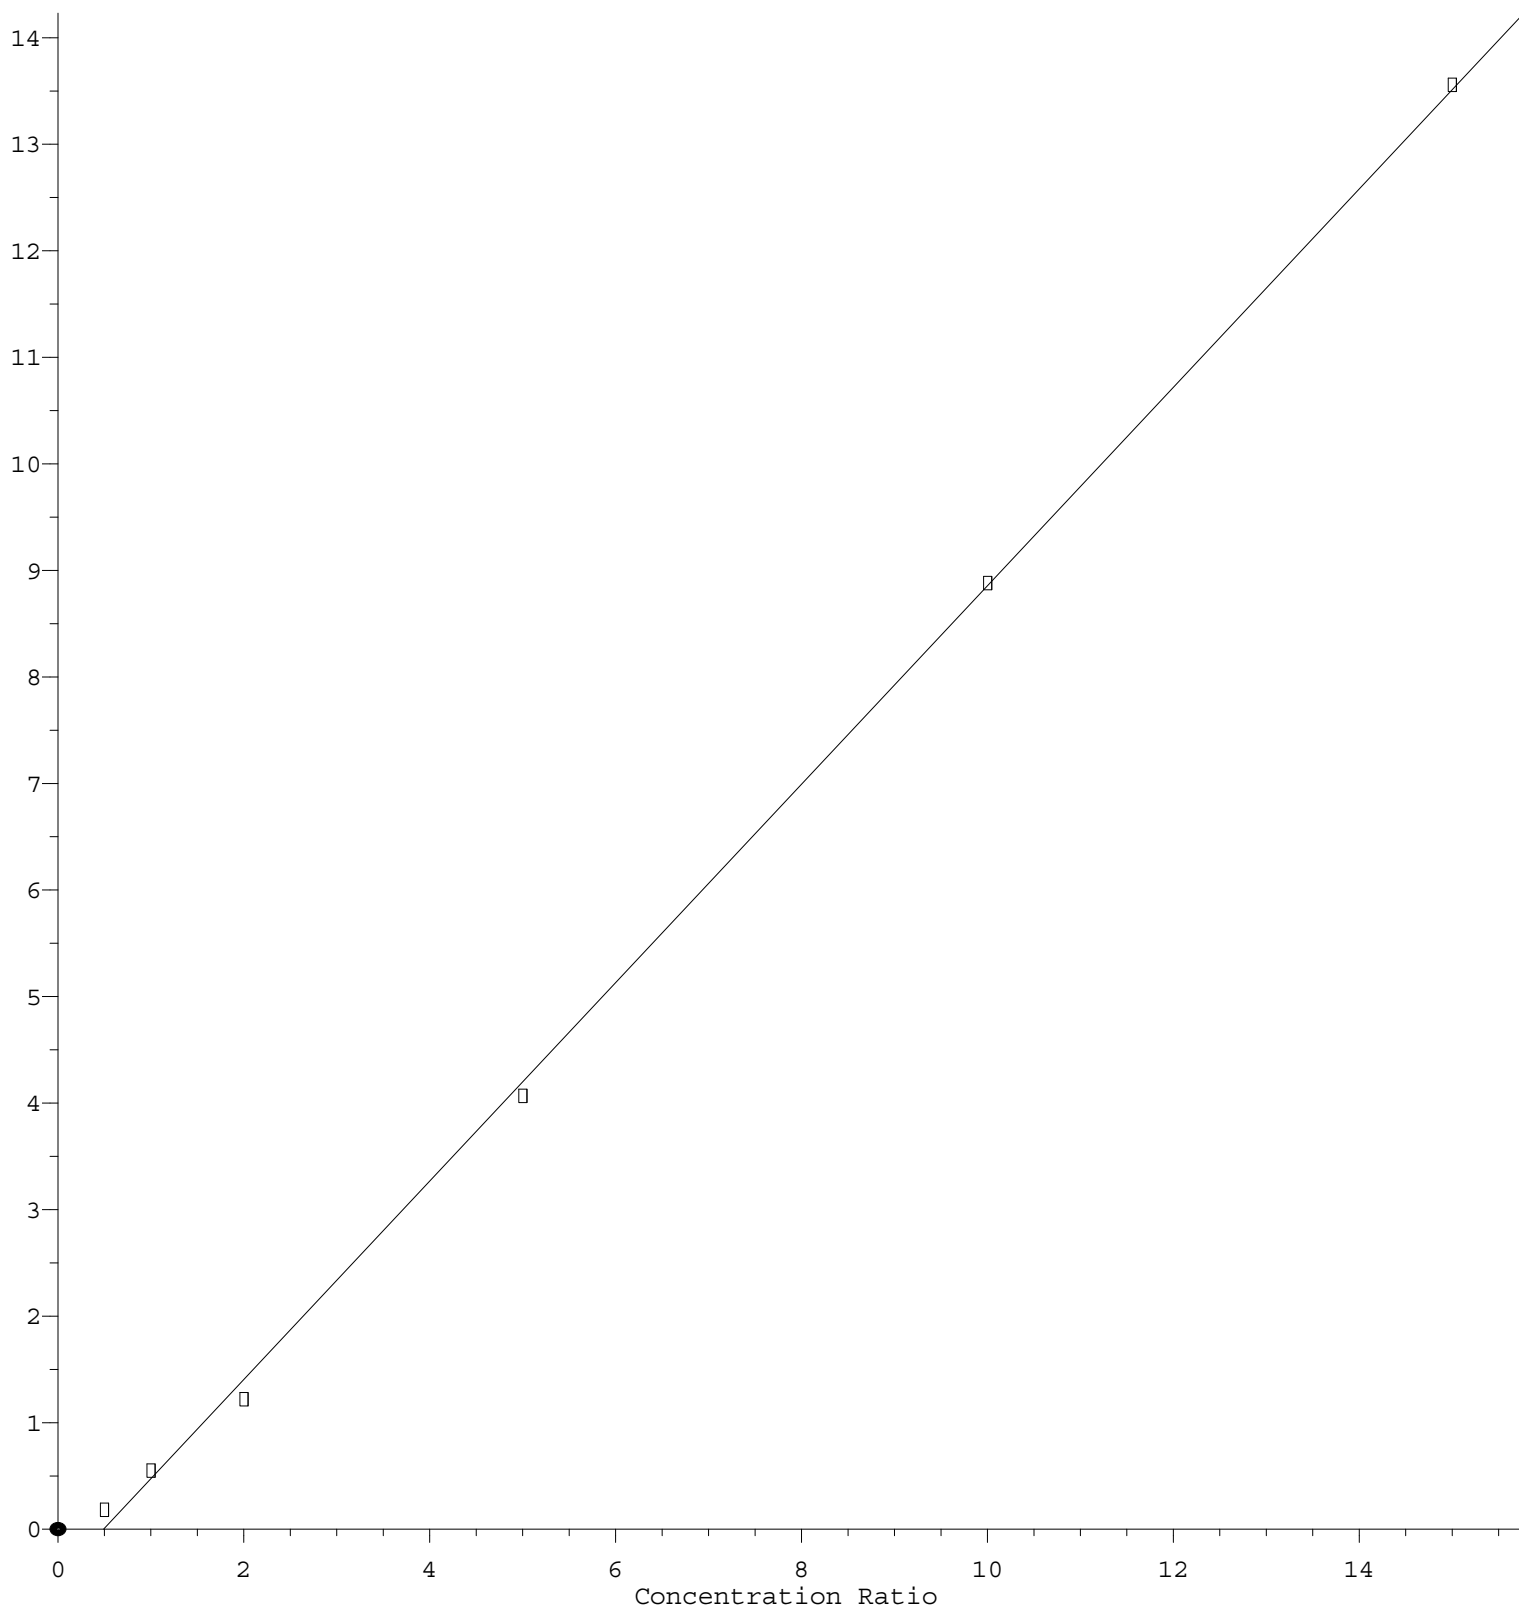

$$\text{Response} = 9.315\text{e-}001 * \text{Amt} - 4.587\text{e-}001$$


Coef of Det (r^2) = 0.999383 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

n-propylbenzene

Response Ratio

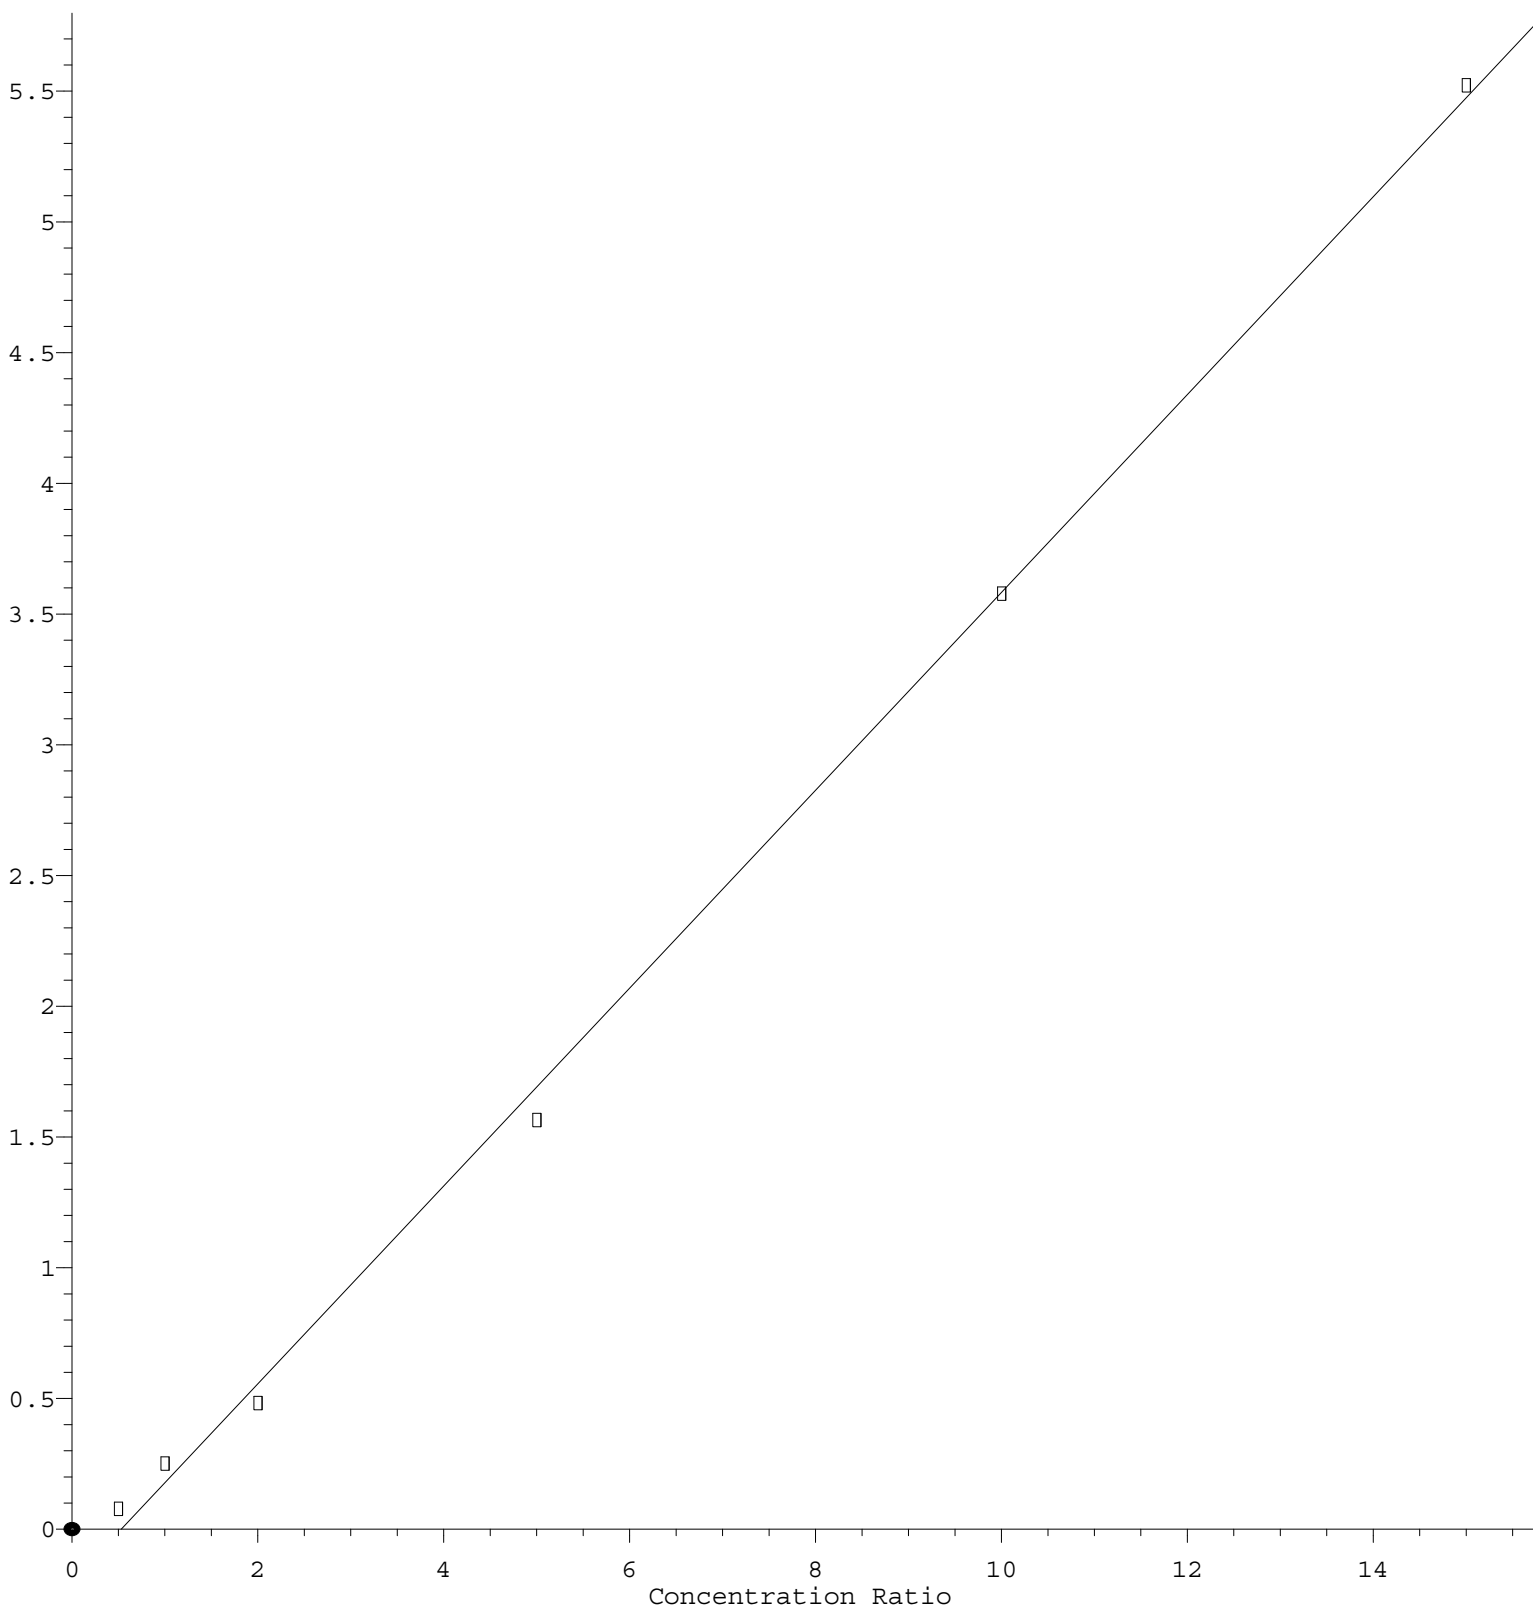

$$\text{Response} = 3.782\text{e-}001 * \text{Amt} - 1.990\text{e-}001$$


Coef of Det (r^2) = 0.998470 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

1,3,5-Trimethylbenzene


Response Ratio

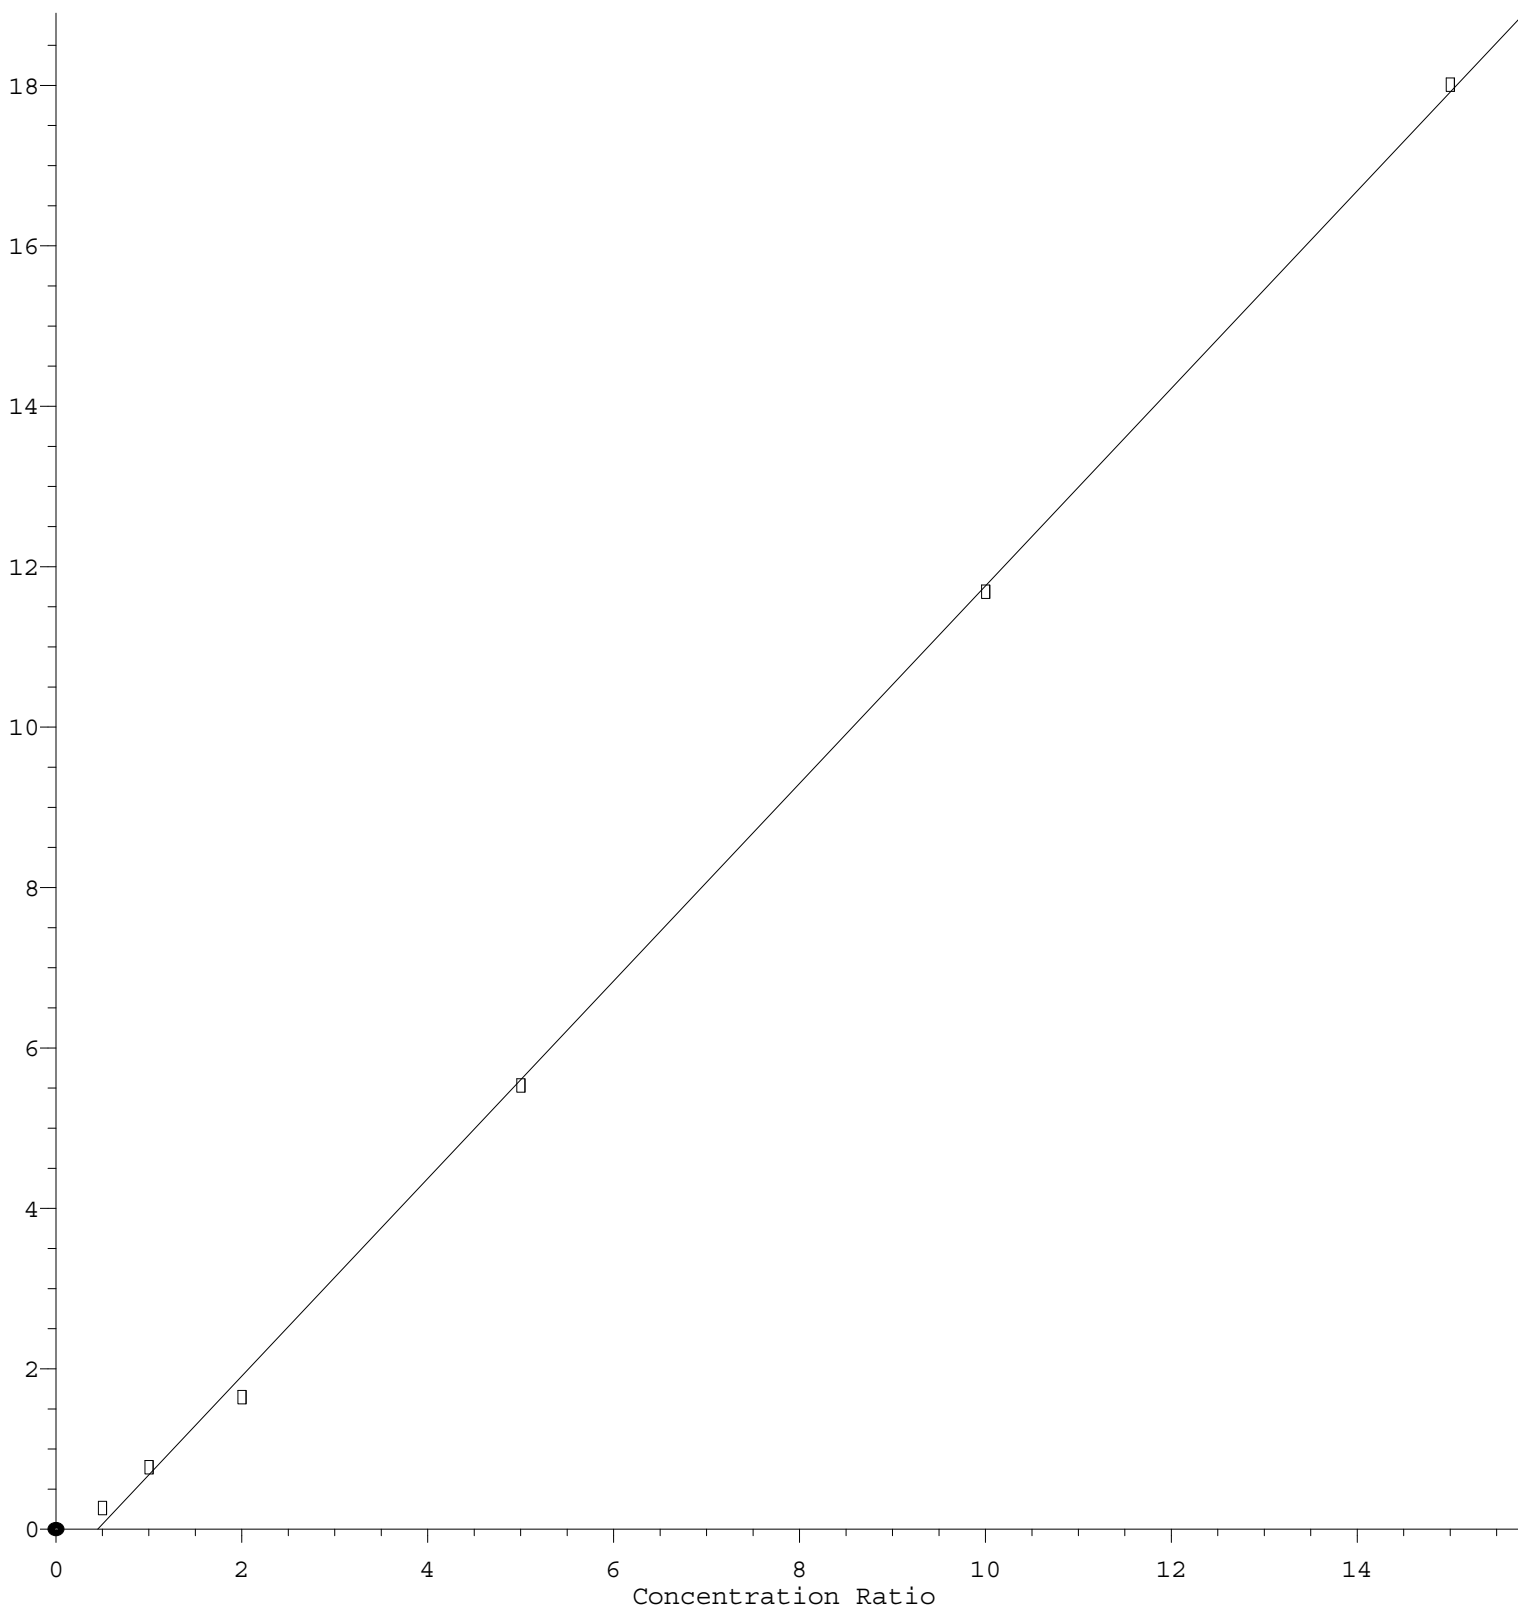

Response = 1.232e+000 * Amt - 5.596e-001
 Coef of Det (r^2) = 0.999465 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M
 Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

1,2,4-Trimethylbenzene

Response Ratio

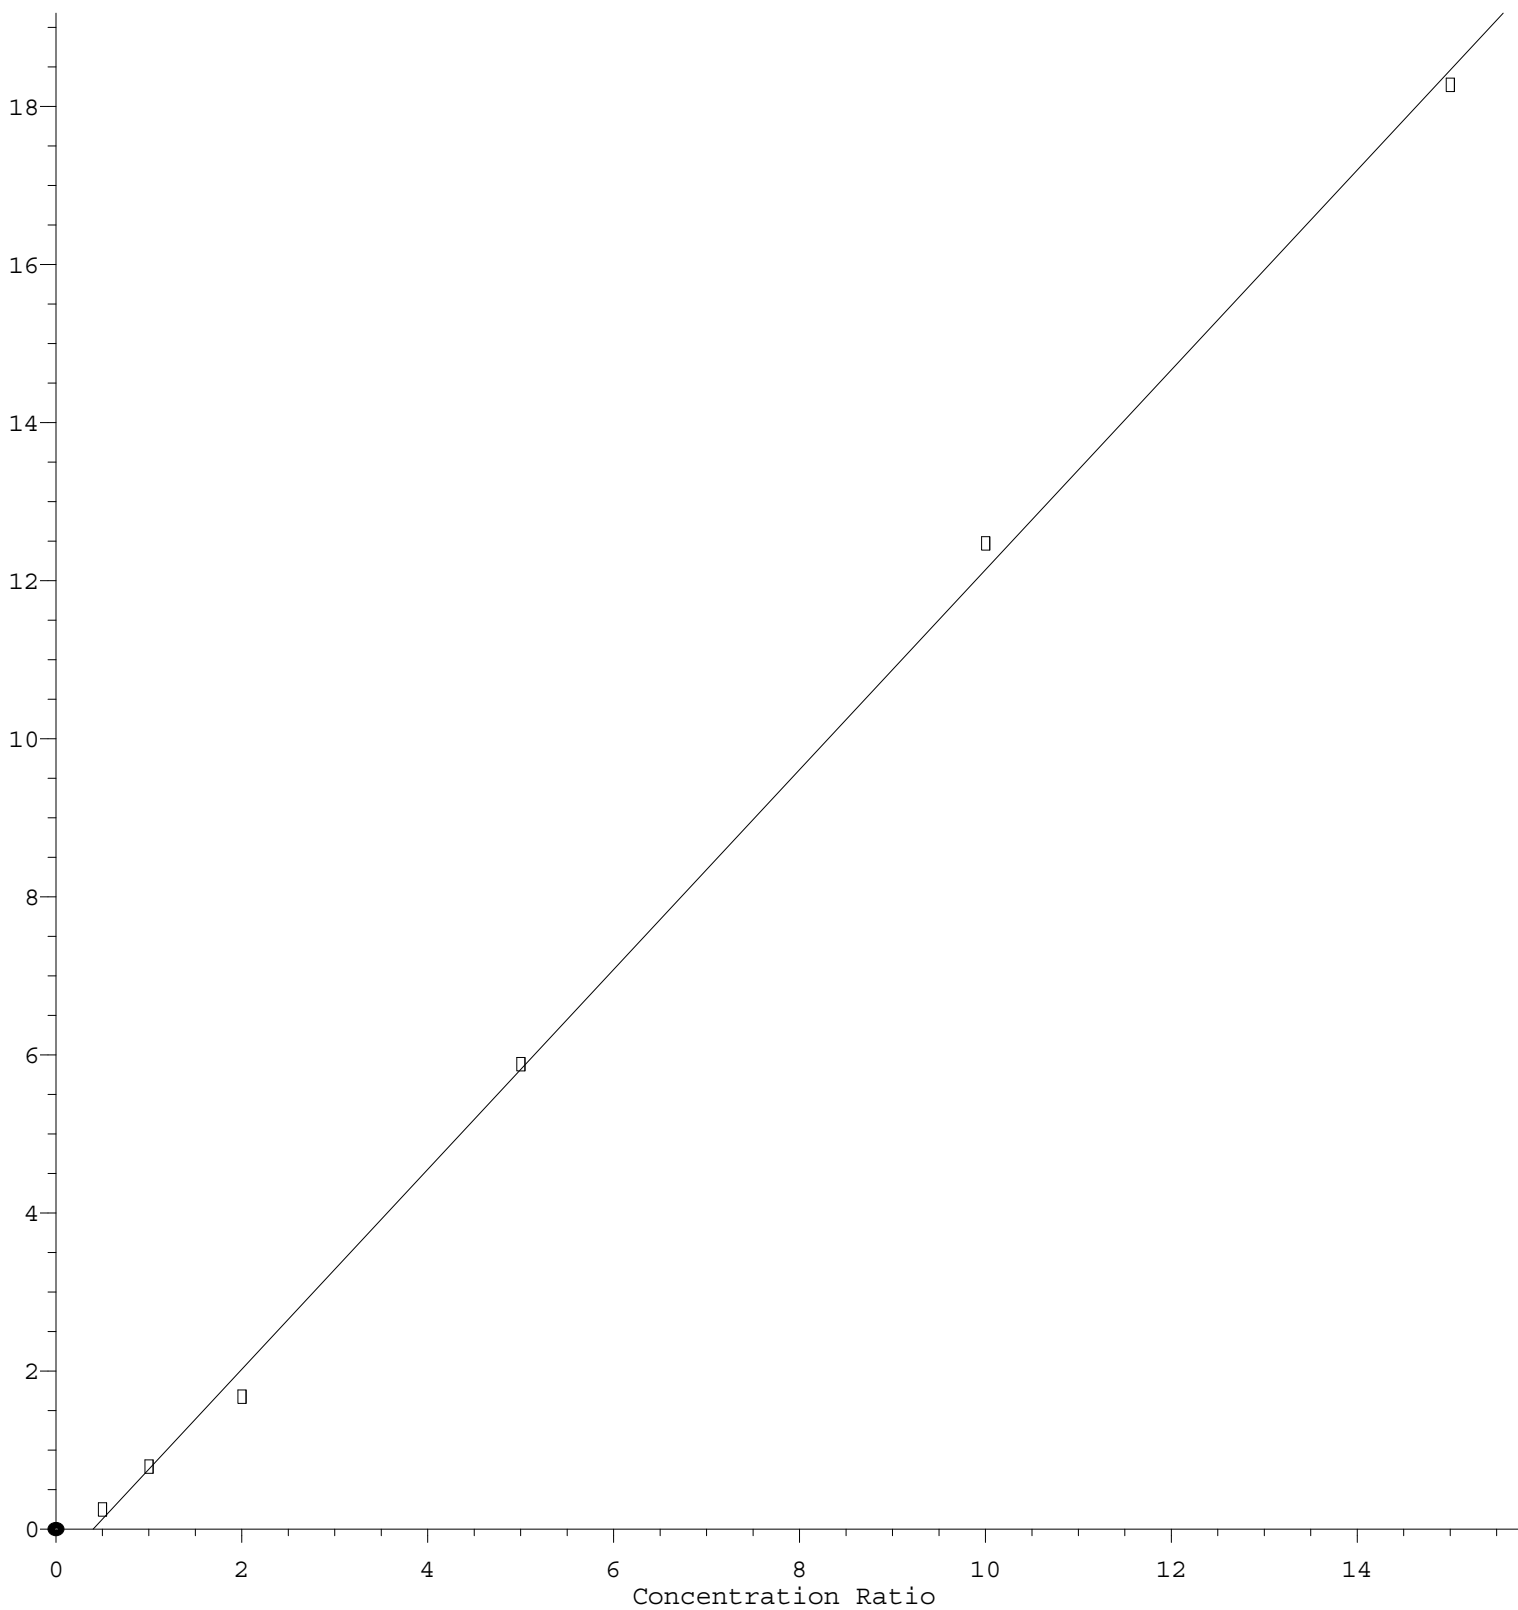

$$\text{Response} = 1.265\text{e}+000 * \text{Amt} - 5.060\text{e}-001$$


Coef of Det (r^2) = 0.998935 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

1,2,4-Trichlorobenzene

Response Ratio

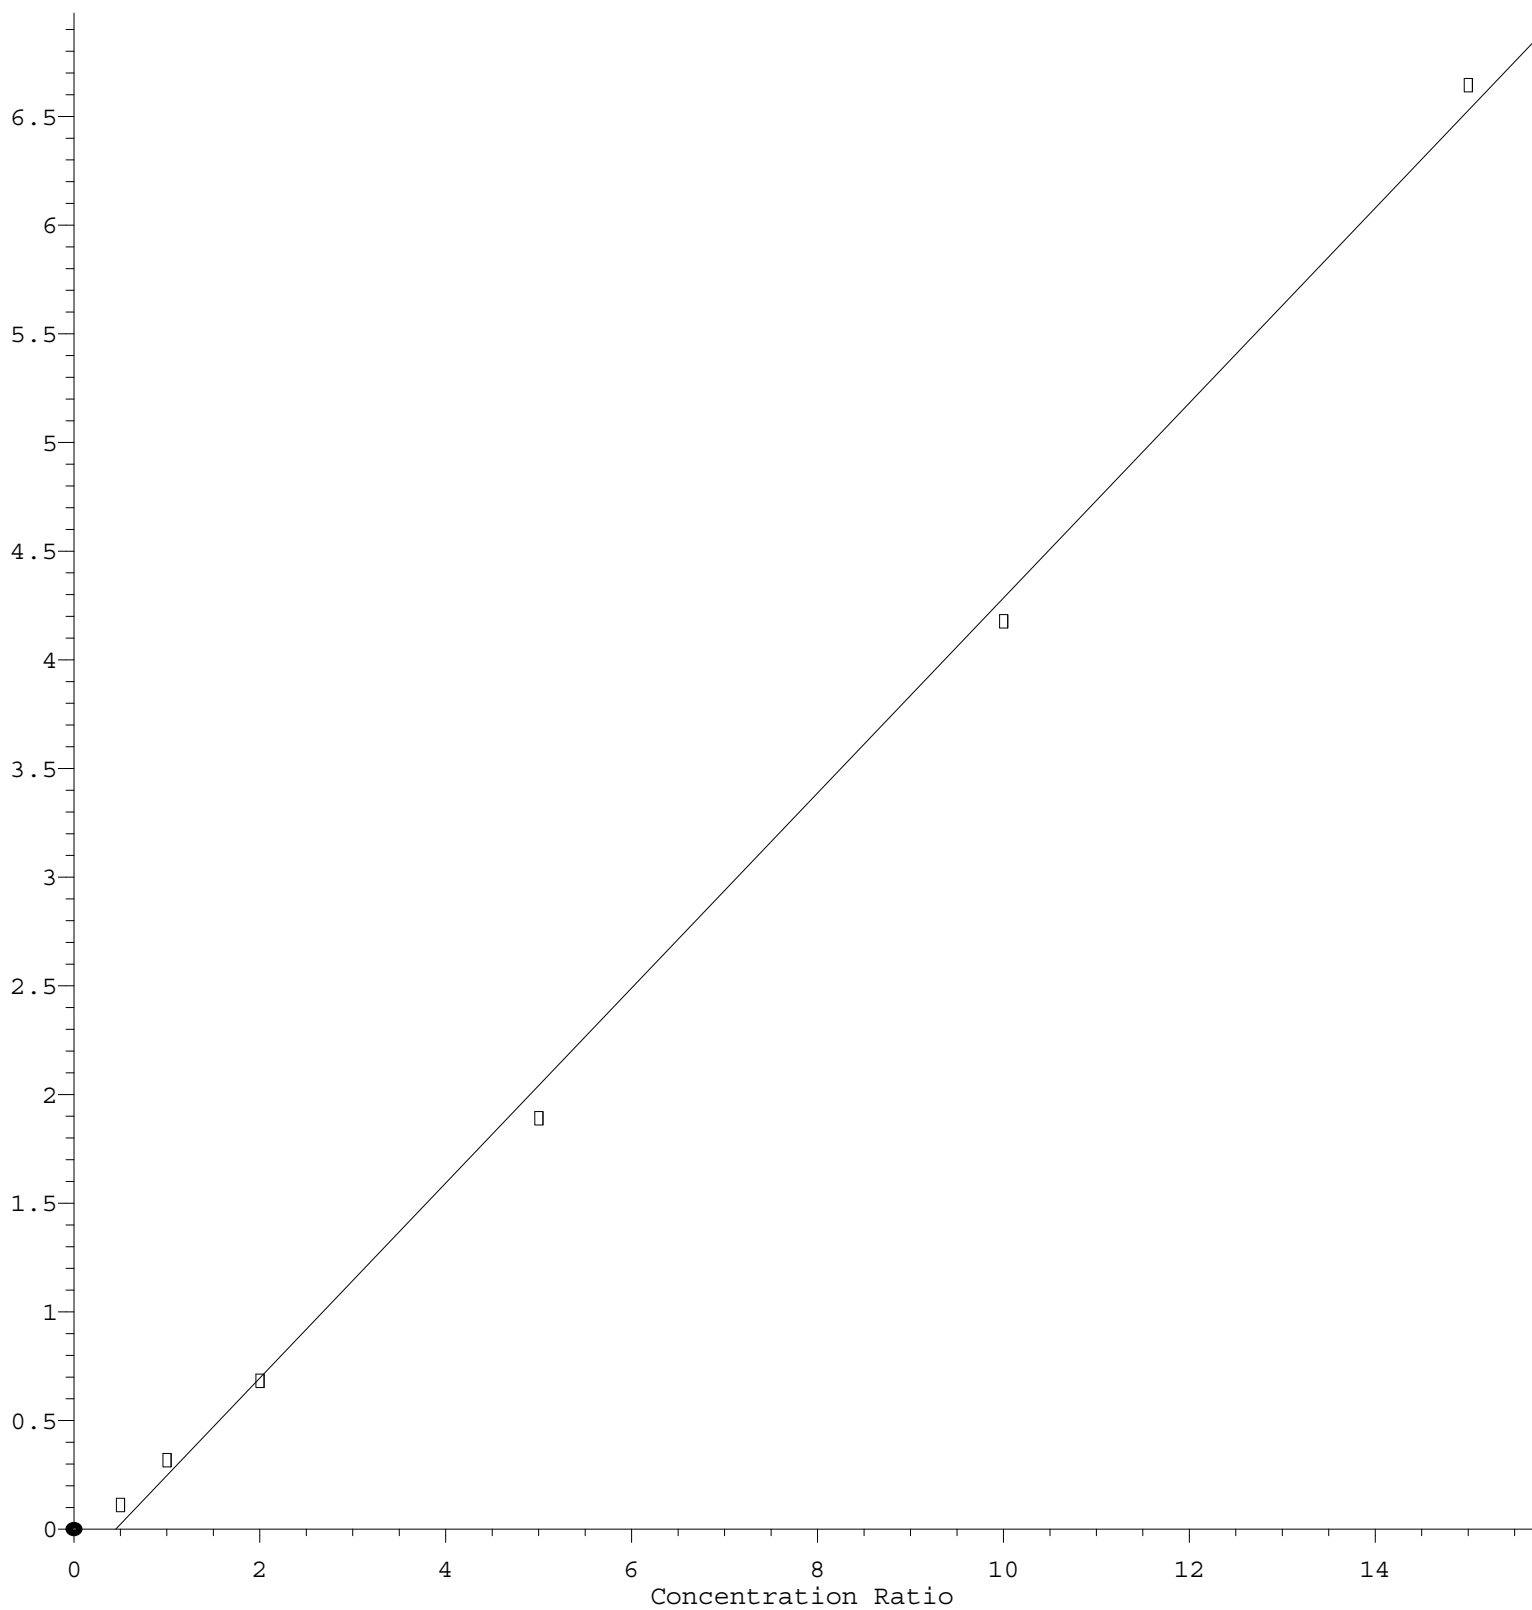

$$\text{Response} = 4.485\text{e-}001 * \text{Amt} - 2.008\text{e-}001$$


Coef of Det (r^2) = 0.998211 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M

Calibration Table Last Updated: Thu Aug 18 08:54:48 2022

Naphthalene

Response Ratio

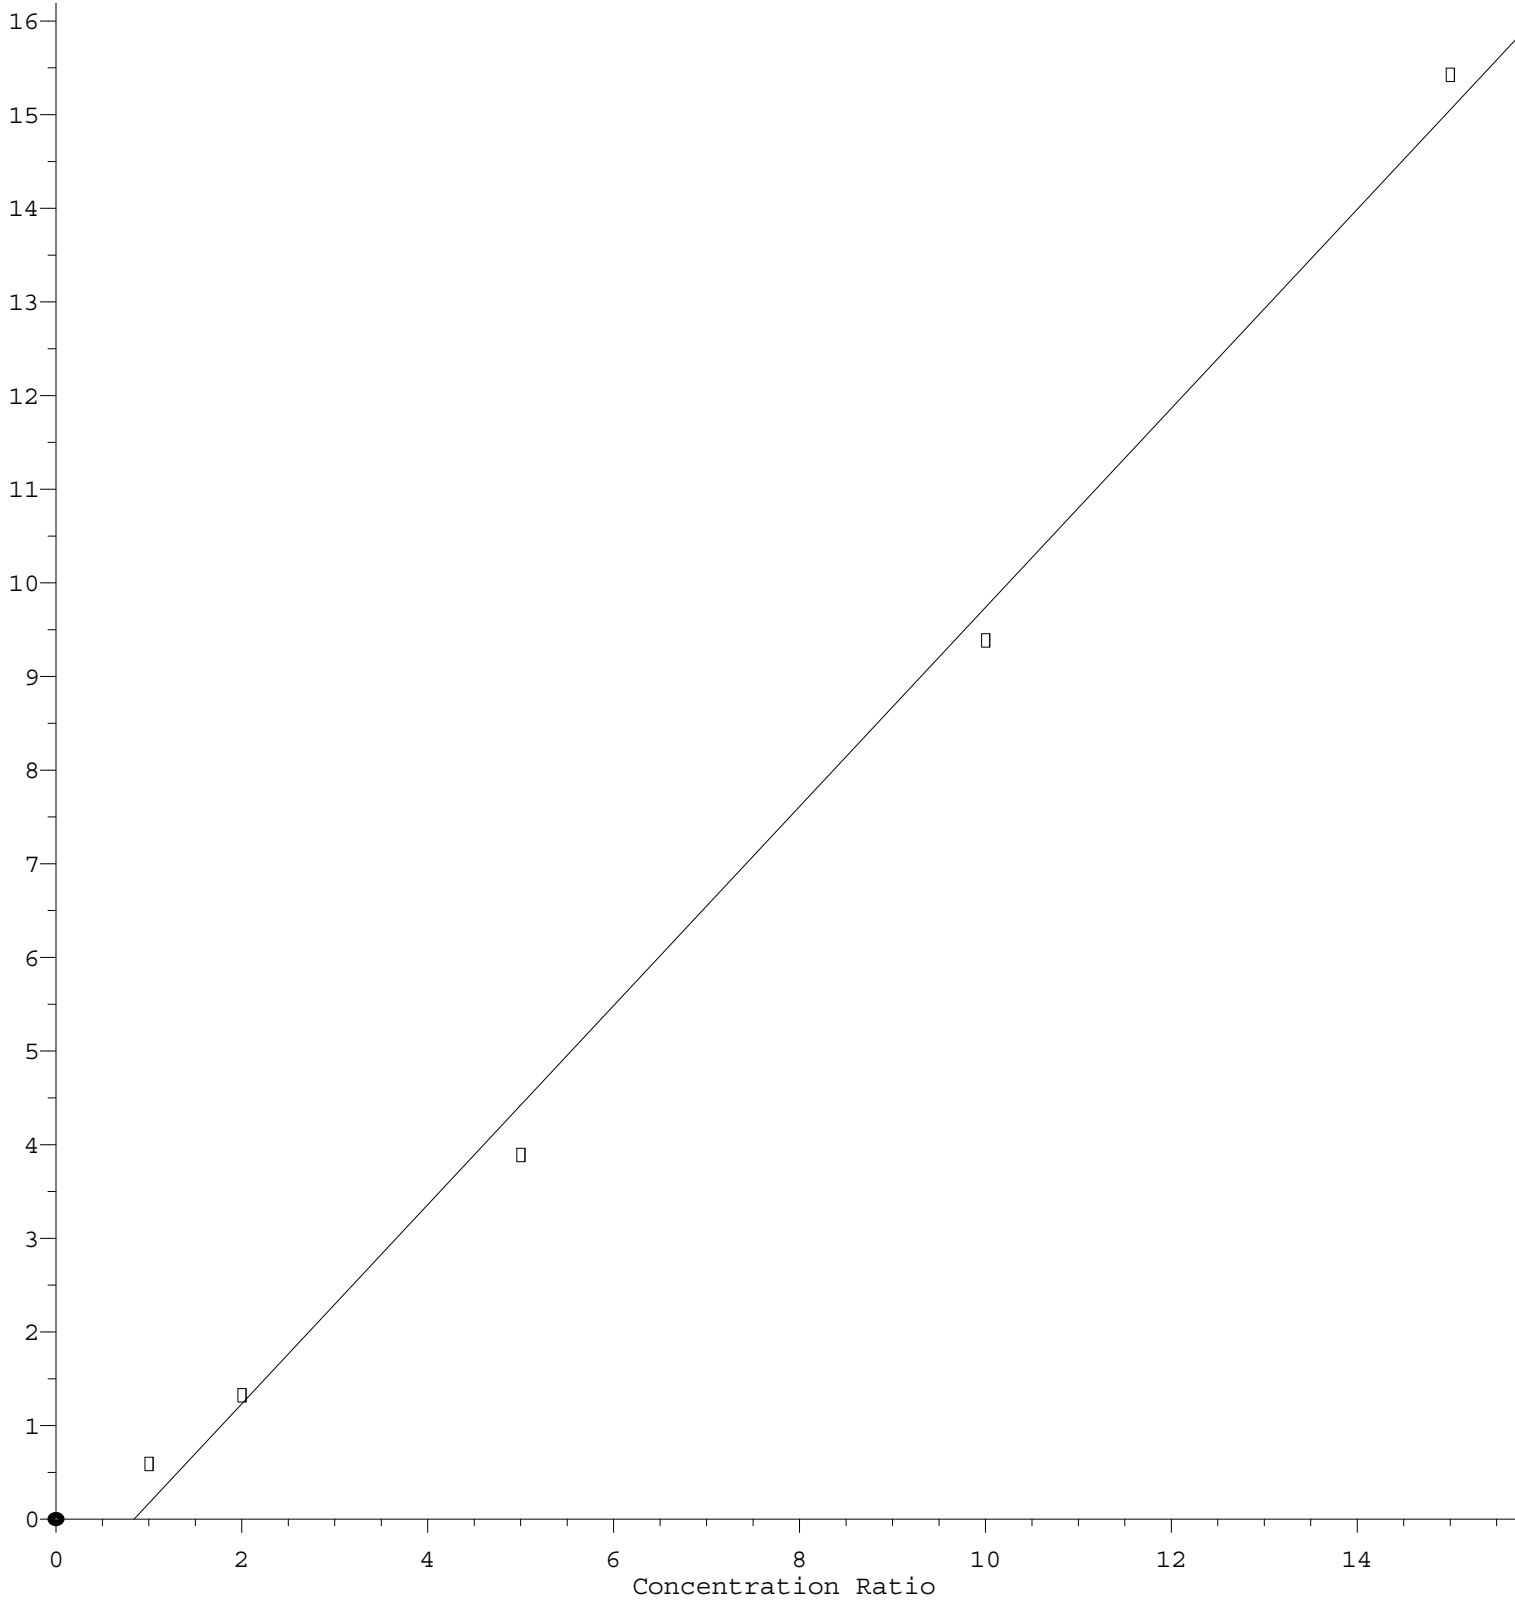

$\text{Response} = 1.063\text{e}+000 * \text{Amt} - 8.953\text{e}-001$
 Coef of Det (r^2) = 0.995297 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081722DW.M
 Calibration Table Last Updated: Thu Aug 18 08:54:48 2022