

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081722\
 Data File : VU050358.D
 Acq On : 17 Aug 2022 17:07
 Operator : SY/MD
 Sample : VU0817WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0817WBL01

Quant Time: Aug 18 06:08:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081722DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Aug 18 06:06:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.112	96	30428	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	8383	0.801	ug/l	0.00
Spiked Amount 1.000			Recovery	=	80.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	9931	0.799	ug/l	0.00
Spiked Amount 1.000			Recovery	=	80.000%	
Target Compounds						
15) Methylene Chloride	3.038	84	13906	0.805	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081722\
Data File : VU050358.D
Acq On : 17 Aug 2022 17:07
Operator : SY/MD
Sample : VU0817WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0817WBL01

Quant Time: Aug 18 06:08:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Aug 18 06:06:02 2022
Response via : Initial Calibration




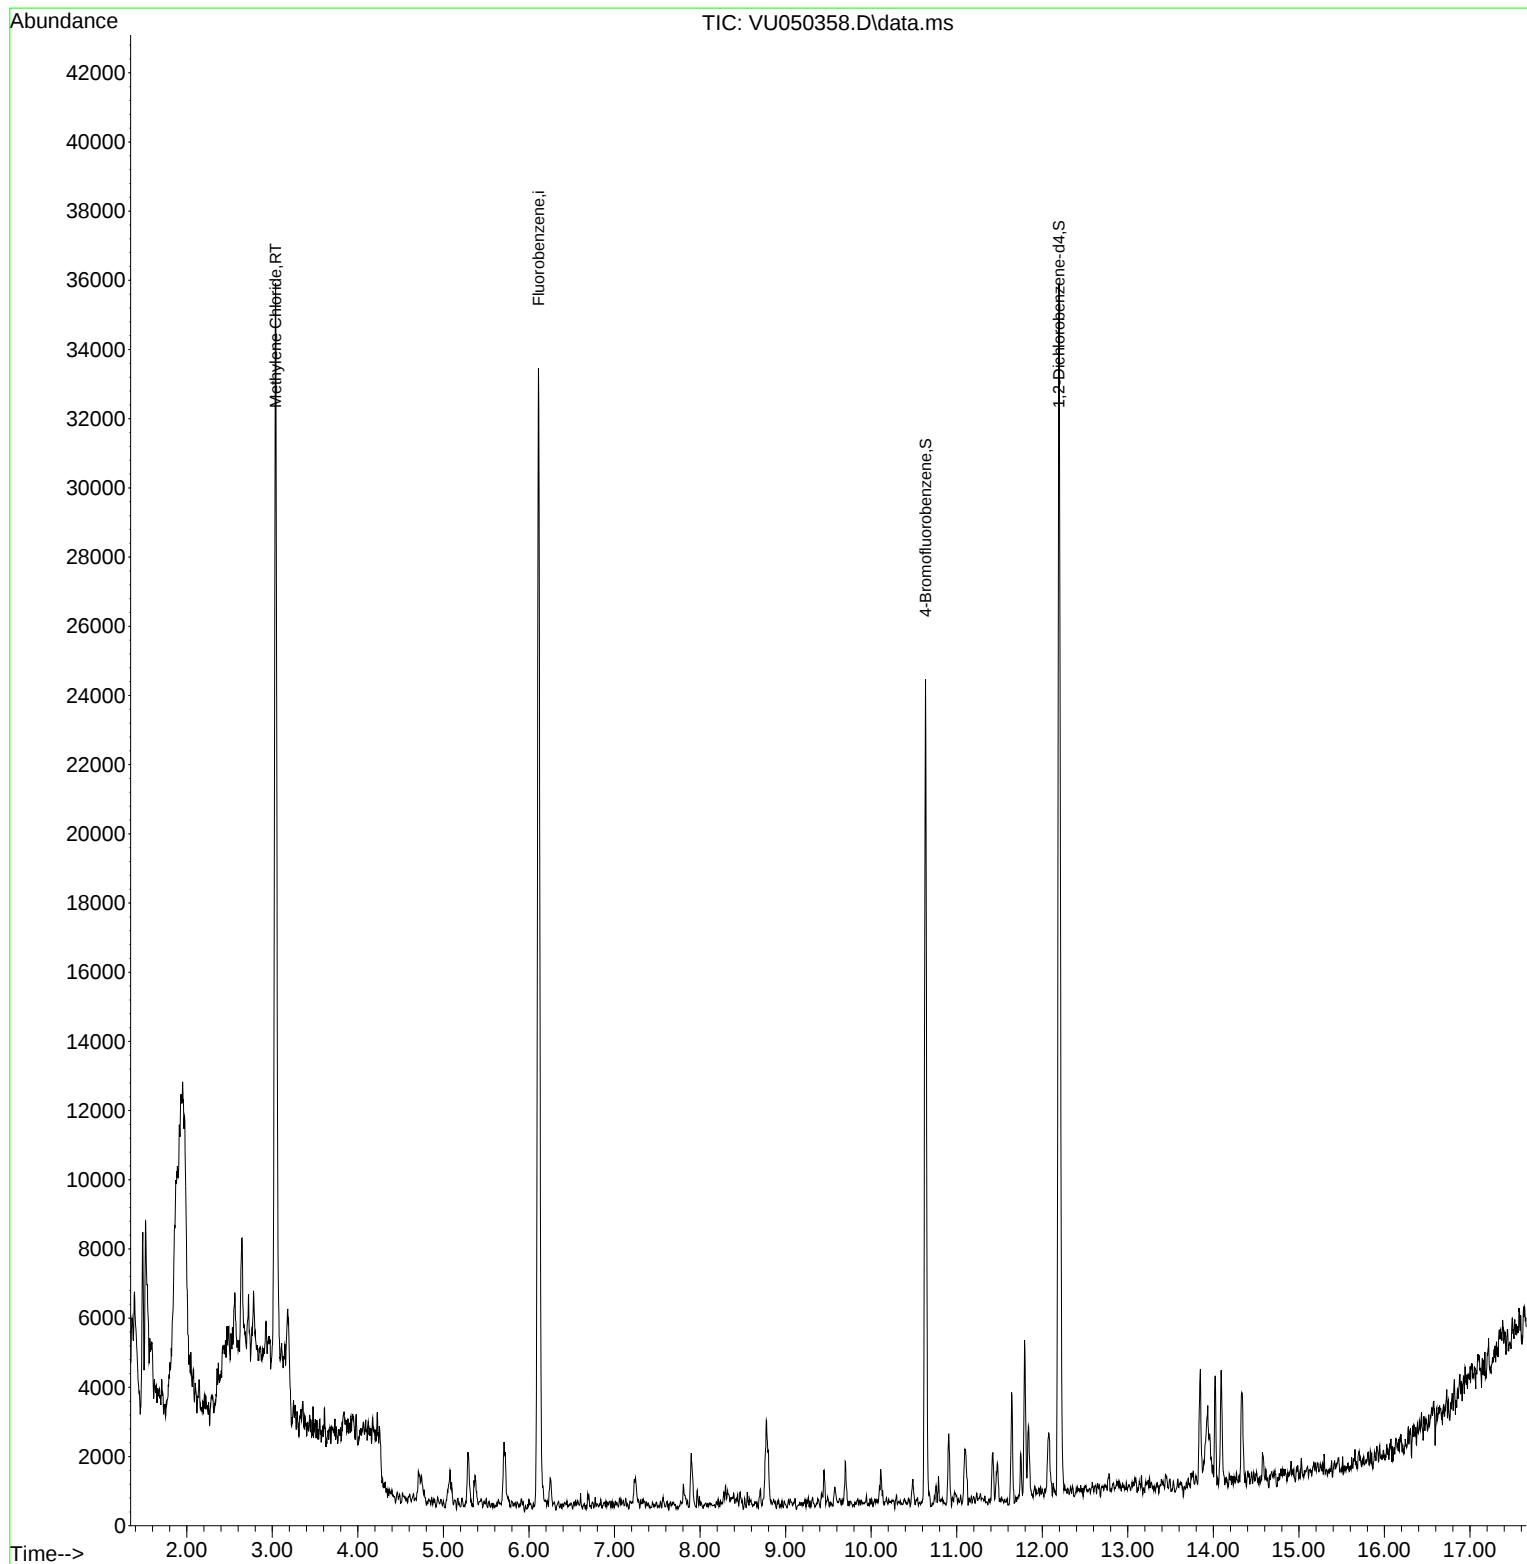


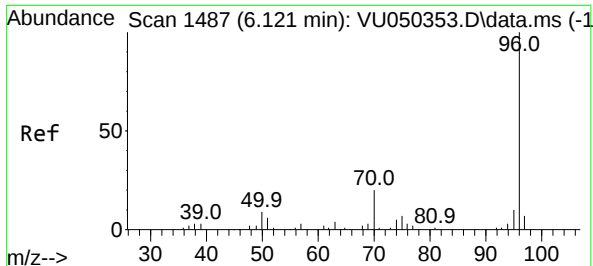

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1487
Delta R.T. -0.009 min
Lab File: VU050358.D
Acq: 17 Aug 2022 17:07




Instrument :
MSVOA_U
ClientSampleId :
VU0817WBL01


Tgt Ion: 96	Resp: 30428
Ion Ratio	Lower Upper
96 100	
70 21.0	16.7 25.1
95 10.2	7.4 11.0
97 6.4	0.0 0.0

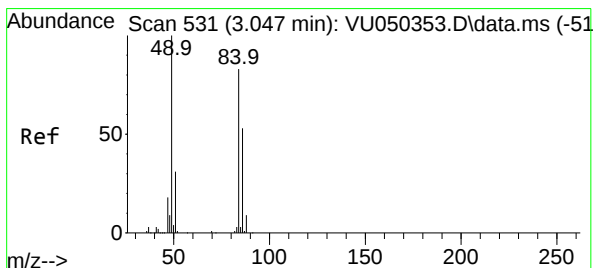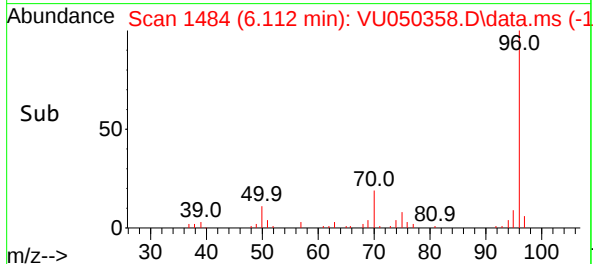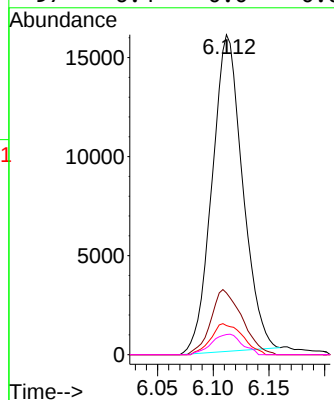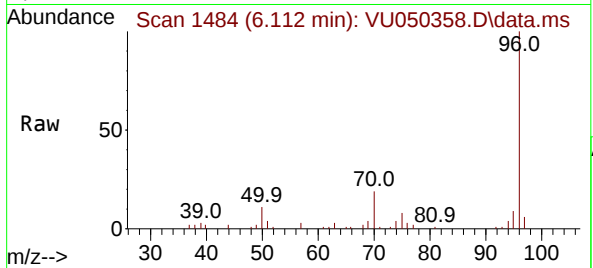

#15
Methylene Chloride
Concen: 0.805 ug/l
RT: 3.038 min Scan# 528
Delta R.T. -0.009 min
Lab File: VU050358.D
Acq: 17 Aug 2022 17:07

Tgt Ion: 84	Resp: 13906
Ion Ratio	Lower Upper
84 100	
49 123.8	104.6 157.0
51 38.0	0.0 81.4
86 66.1	52.6 78.8


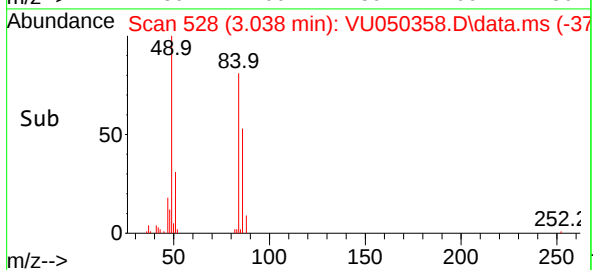
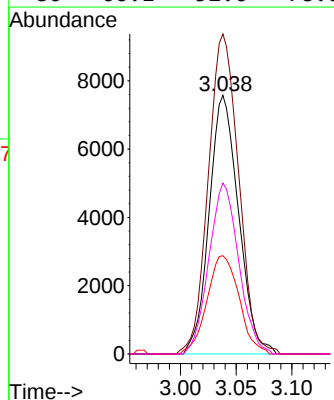
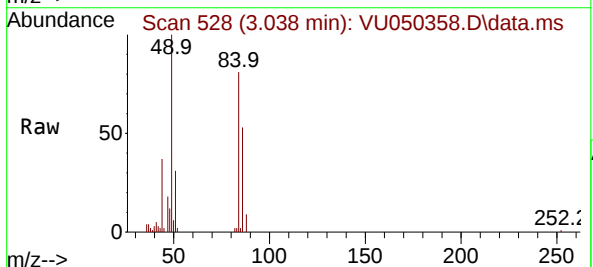


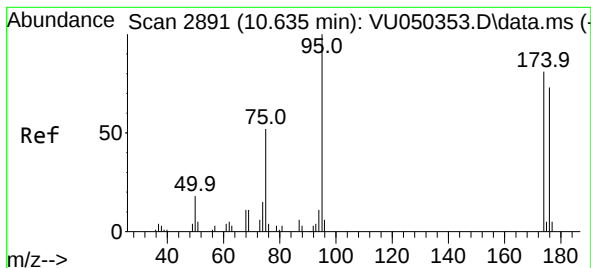

#57
 4-Bromofluorobenzene
 Concen: 0.801 ug/l
 RT: 10.636 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VU050358.D
 Acq: 17 Aug 2022 17:07

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0817WBL01

Tgt Ion: 95 Resp: 8383
 Ion Ratio Lower Upper
 95 100
 174 77.6 62.4 93.6
 176 80.4 56.2 84.2

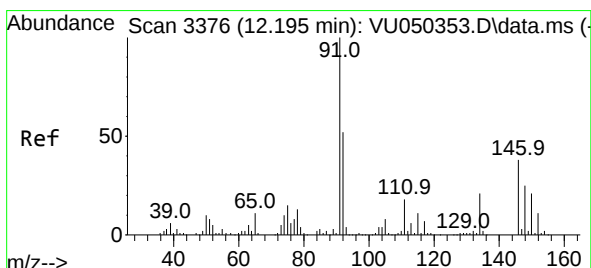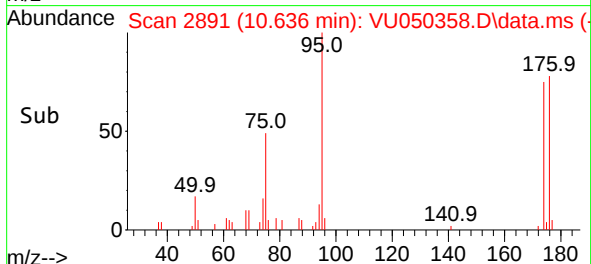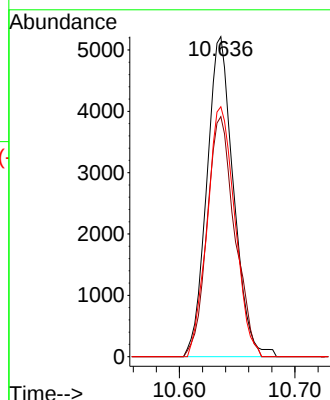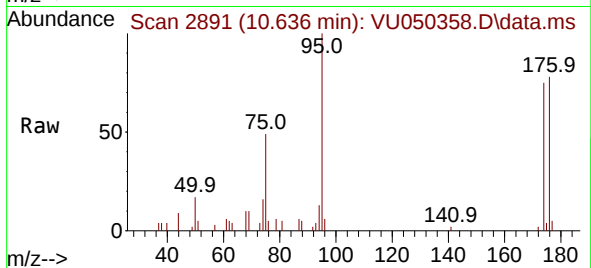

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.799 ug/l
 RT: 12.195 min Scan# 3376
 Delta R.T. 0.000 min
 Lab File: VU050358.D
 Acq: 17 Aug 2022 17:07

Tgt Ion: 152 Resp: 9931
 Ion Ratio Lower Upper
 152 100
 115 65.0 0.0 254.6
 150 152.2 0.0 623.6

