


t-1,4-Dichloro-2-butene

Response Ratio

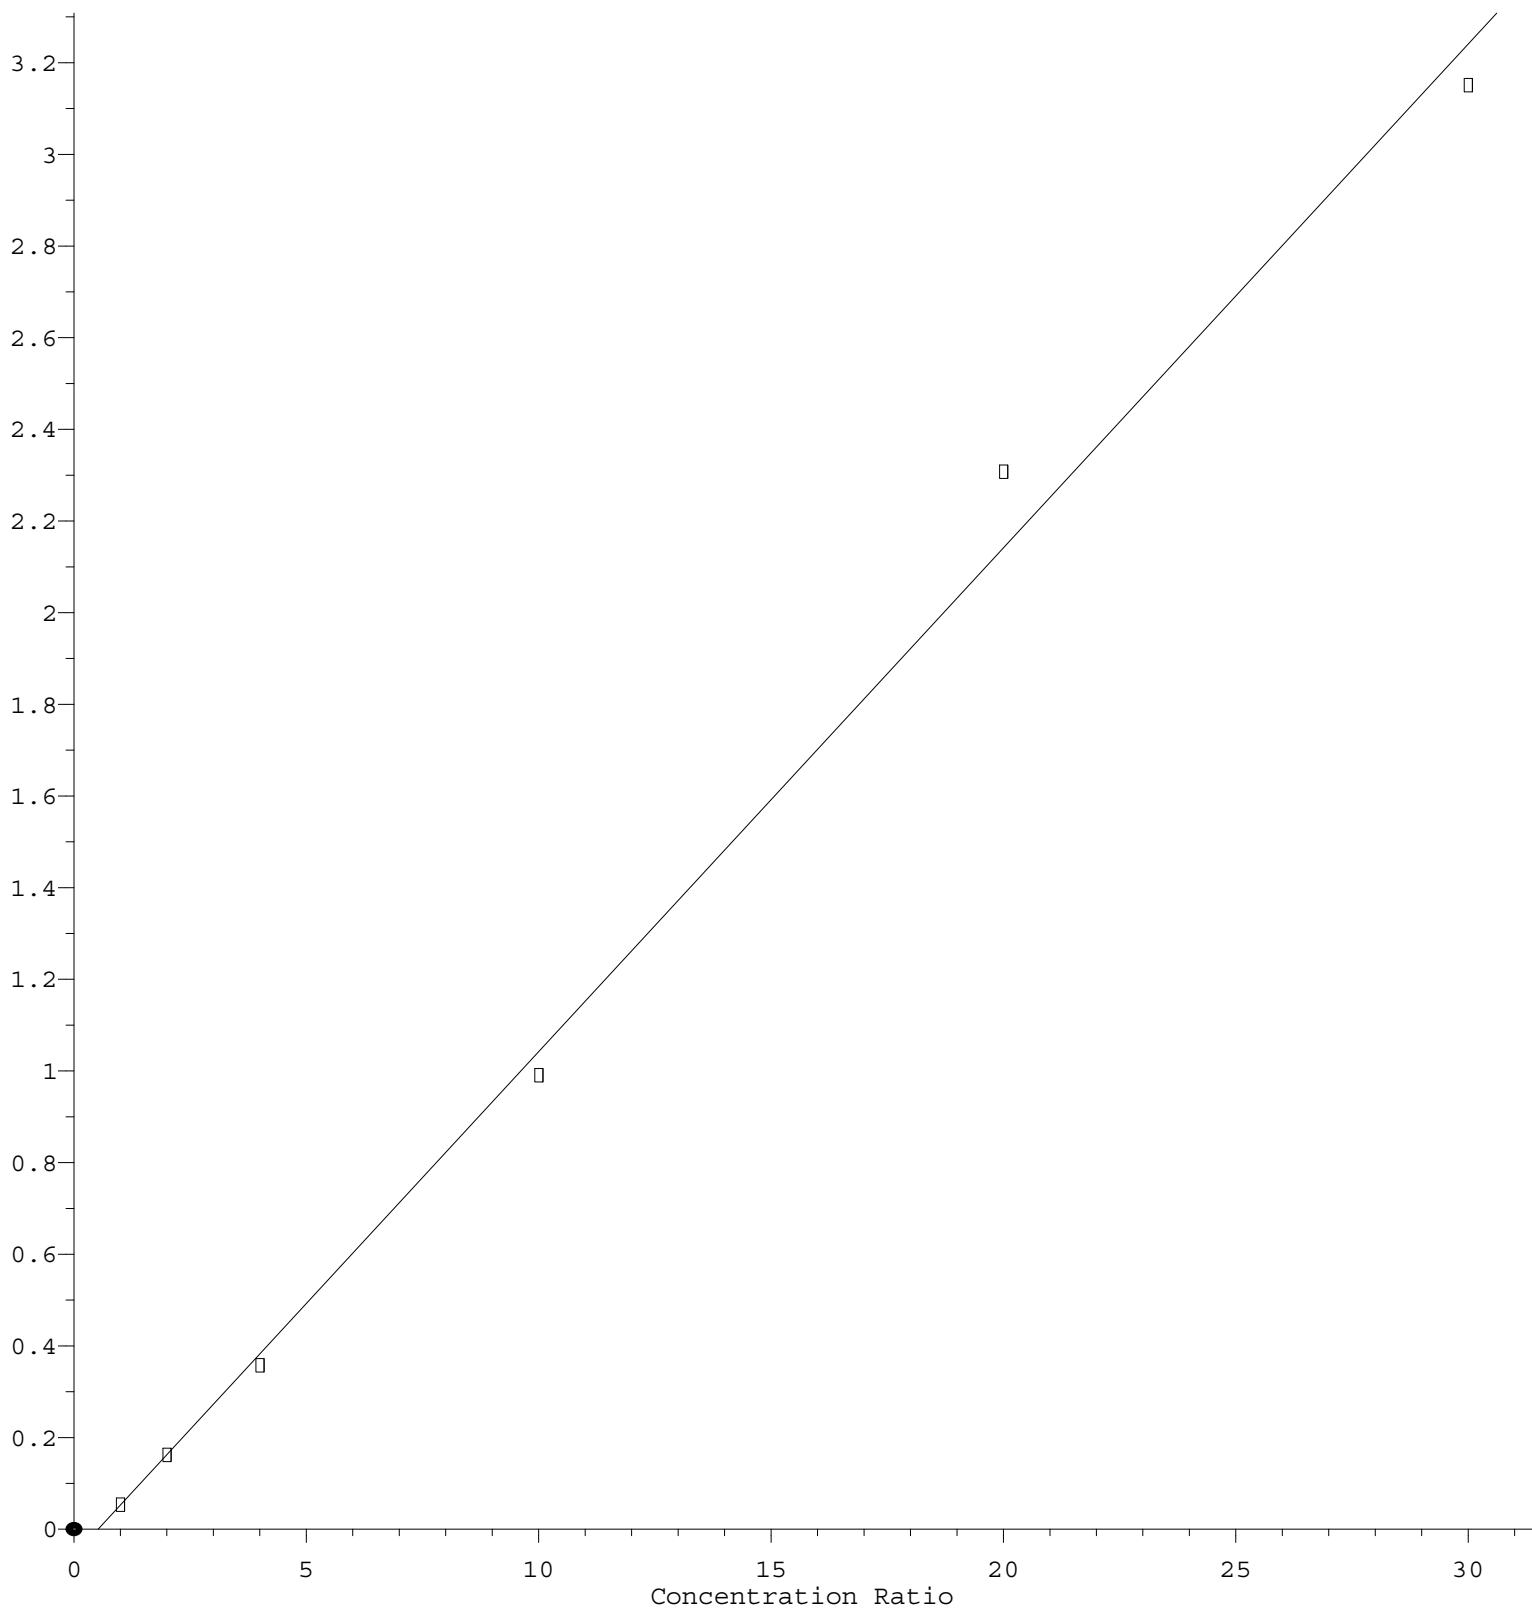

$$\text{Response} = 1.099\text{e-}001 * \text{Amt} - 5.759\text{e-}002$$


Coef of Det (r^2) = 0.995240 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Methyl methacrylate

Response Ratio

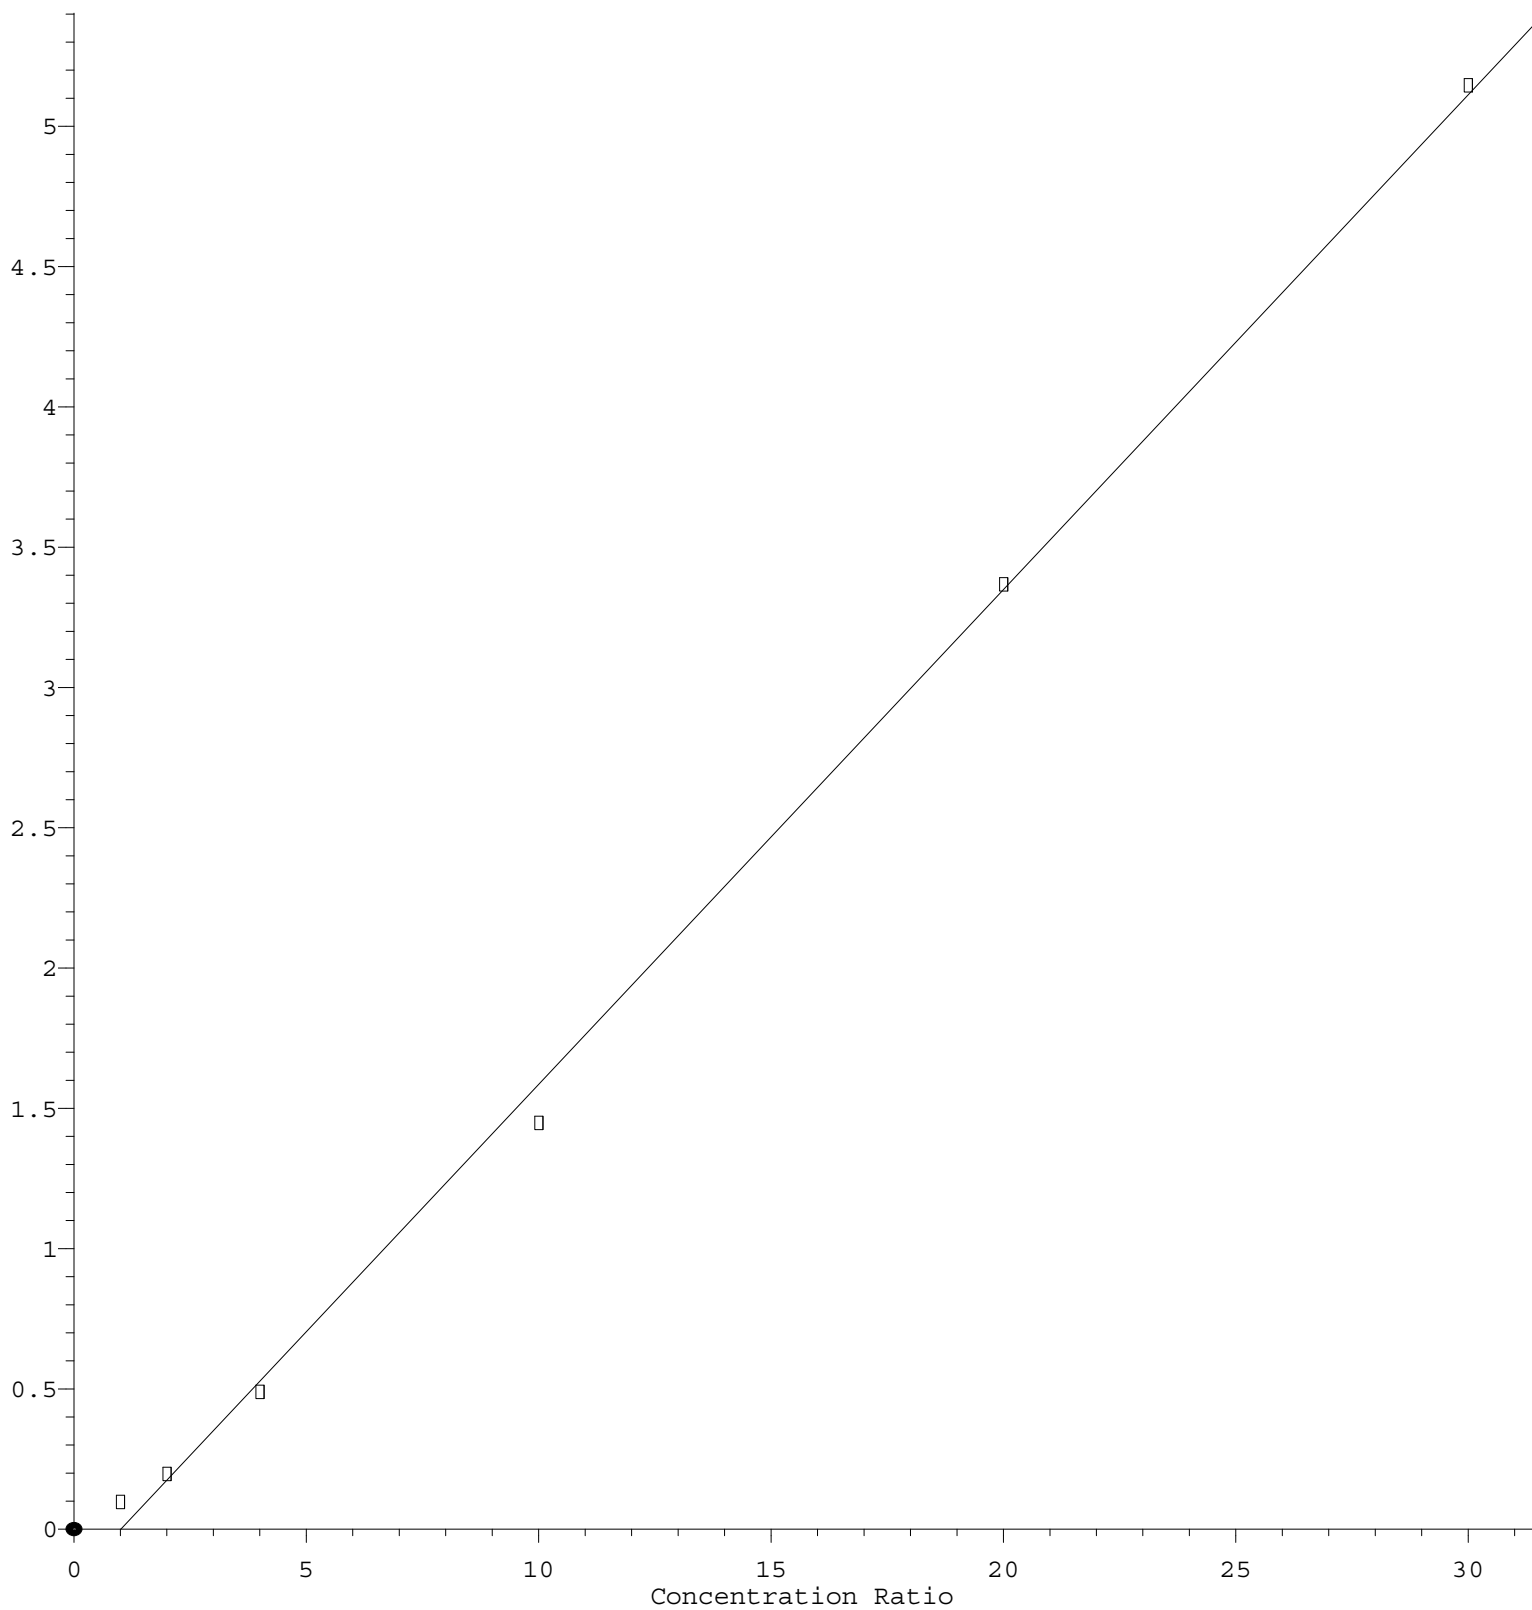

$$\text{Response} = 1.764\text{e-}001 * \text{Amt} - 1.790\text{e-}001$$


Coef of Det (r^2) = 0.998472 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Ethyl methacrylate

Response Ratio

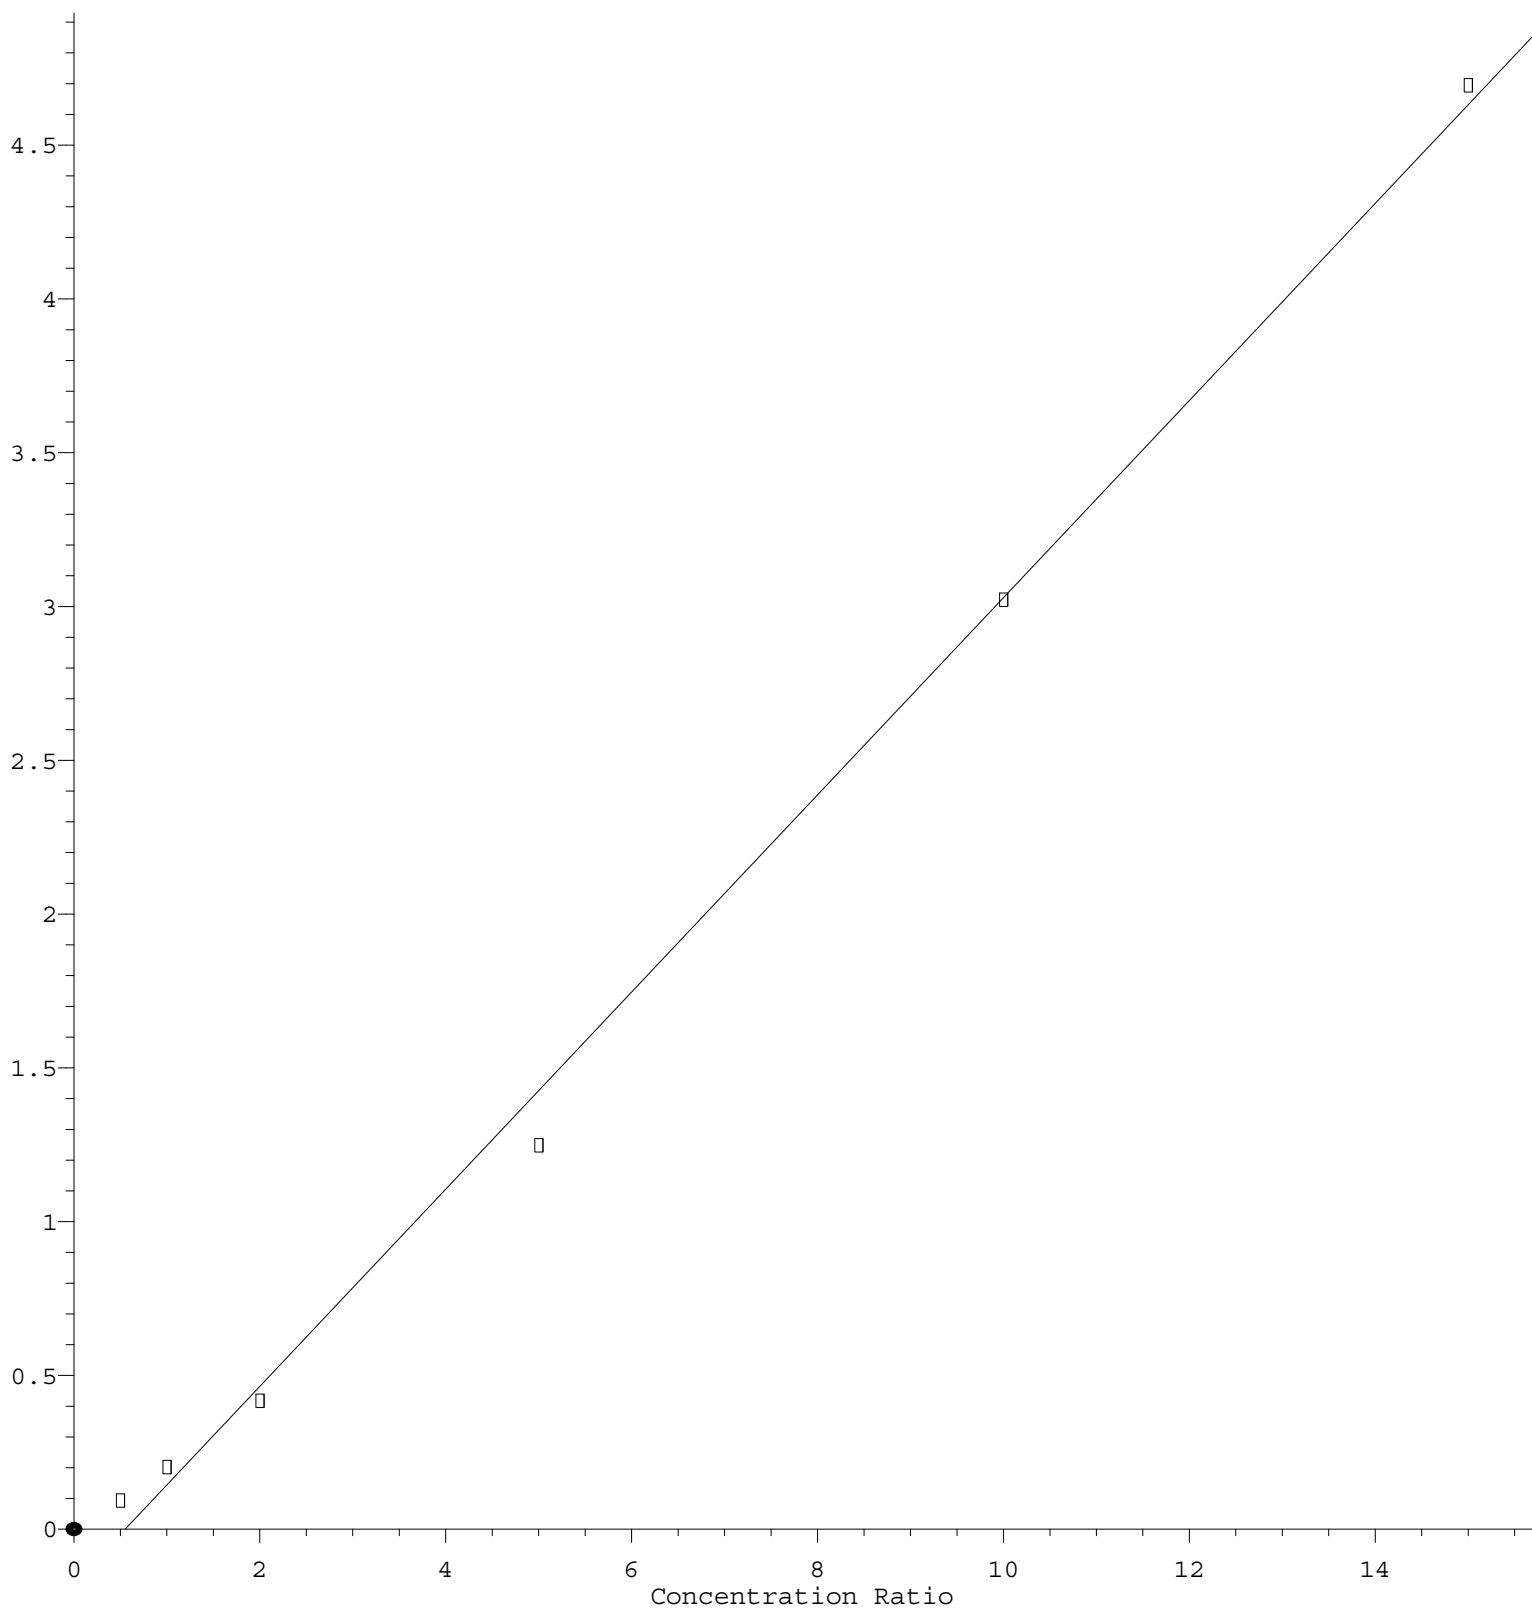

$$\text{Response} = 3.206\text{e-}001 * \text{Amt} - 1.772\text{e-}001$$


Coef of Det (r^2) = 0.996929 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Ethyl Benzene

Response Ratio

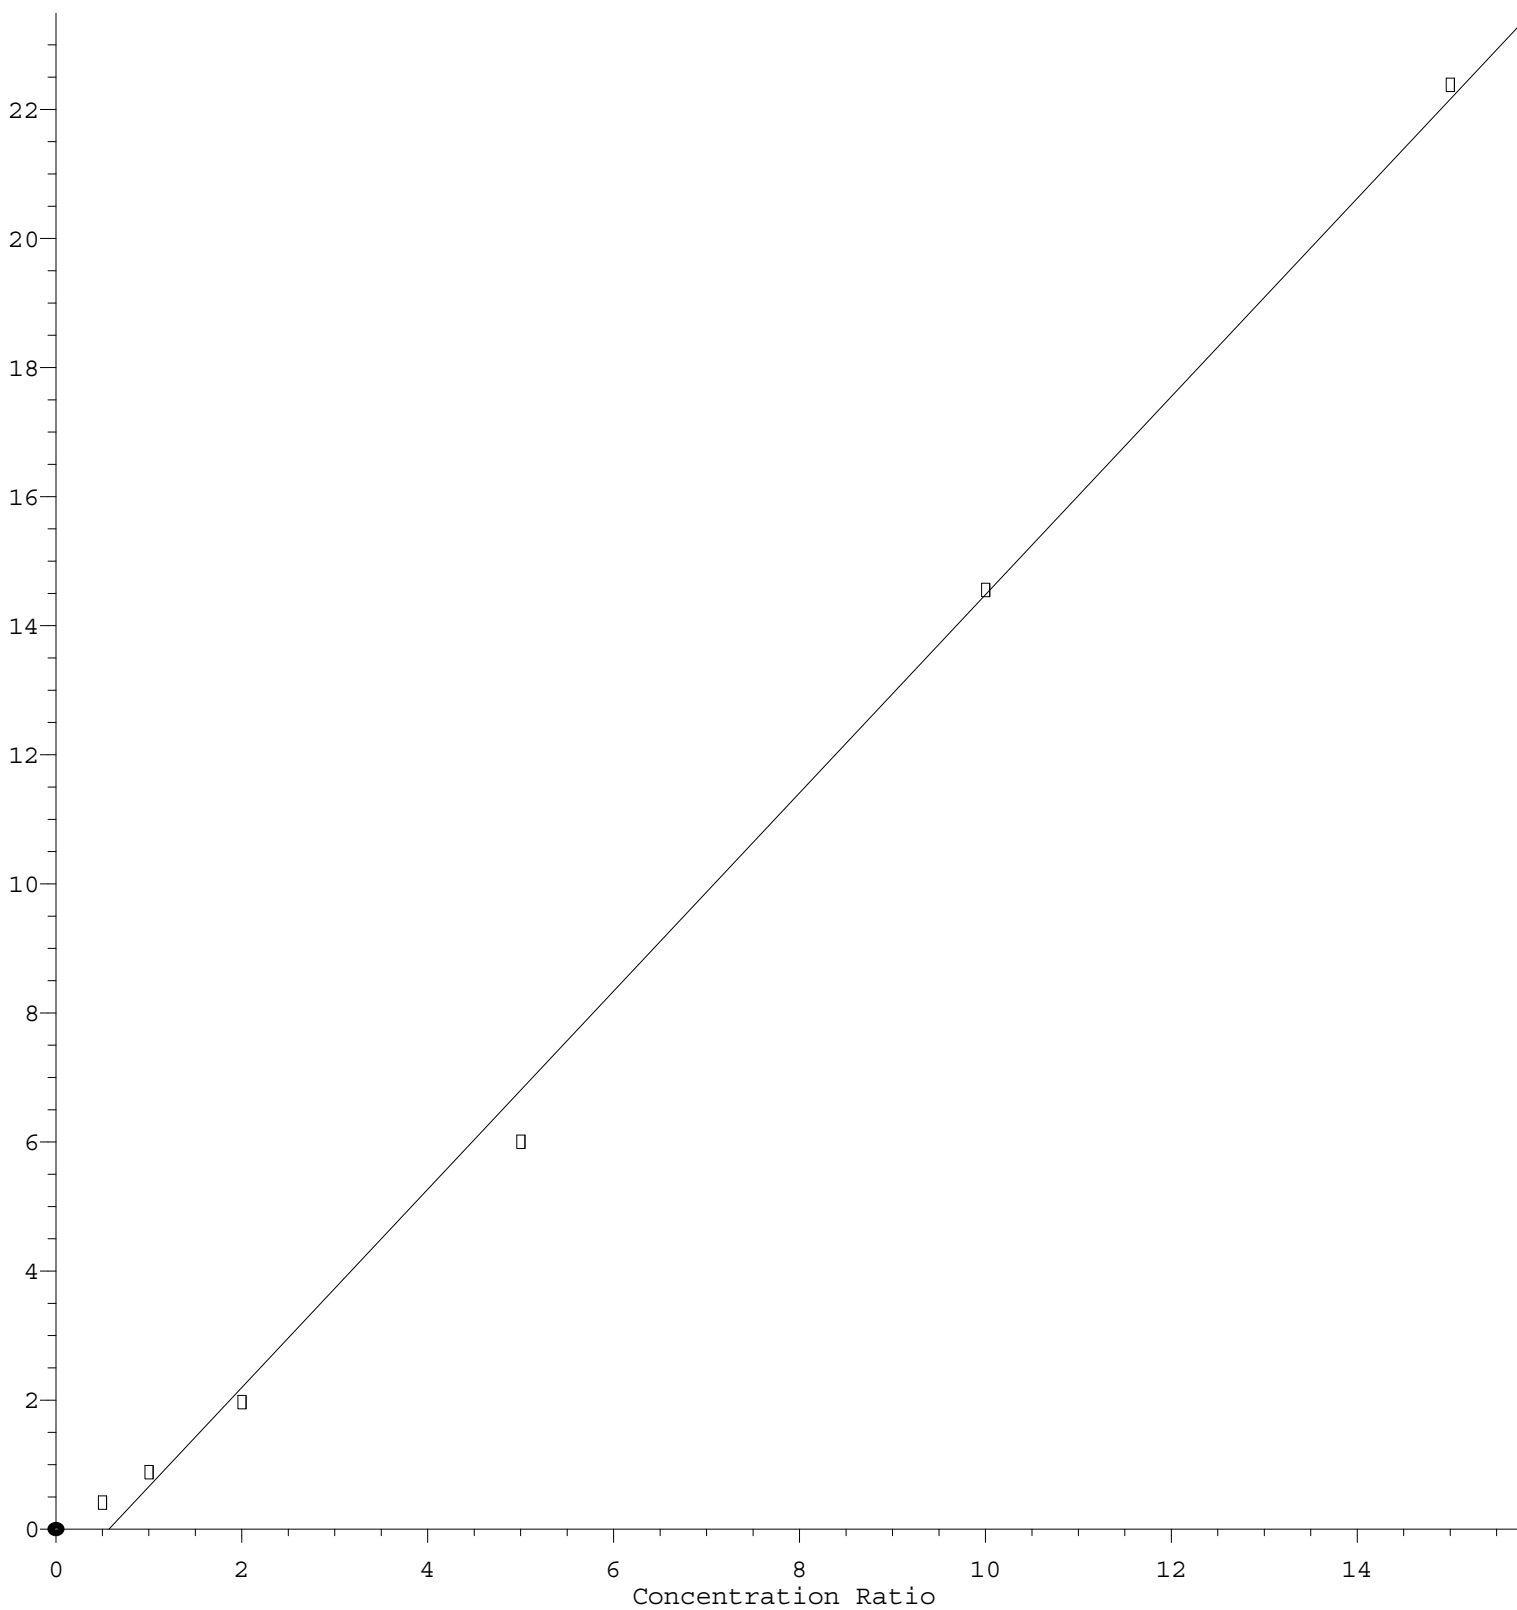

$$\text{Response} = 1.536\text{e}+000 * \text{Amt} - 8.754\text{e}-001$$


Coef of Det (r^2) = 0.997315 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

m/p-Xylenes

Response Ratio

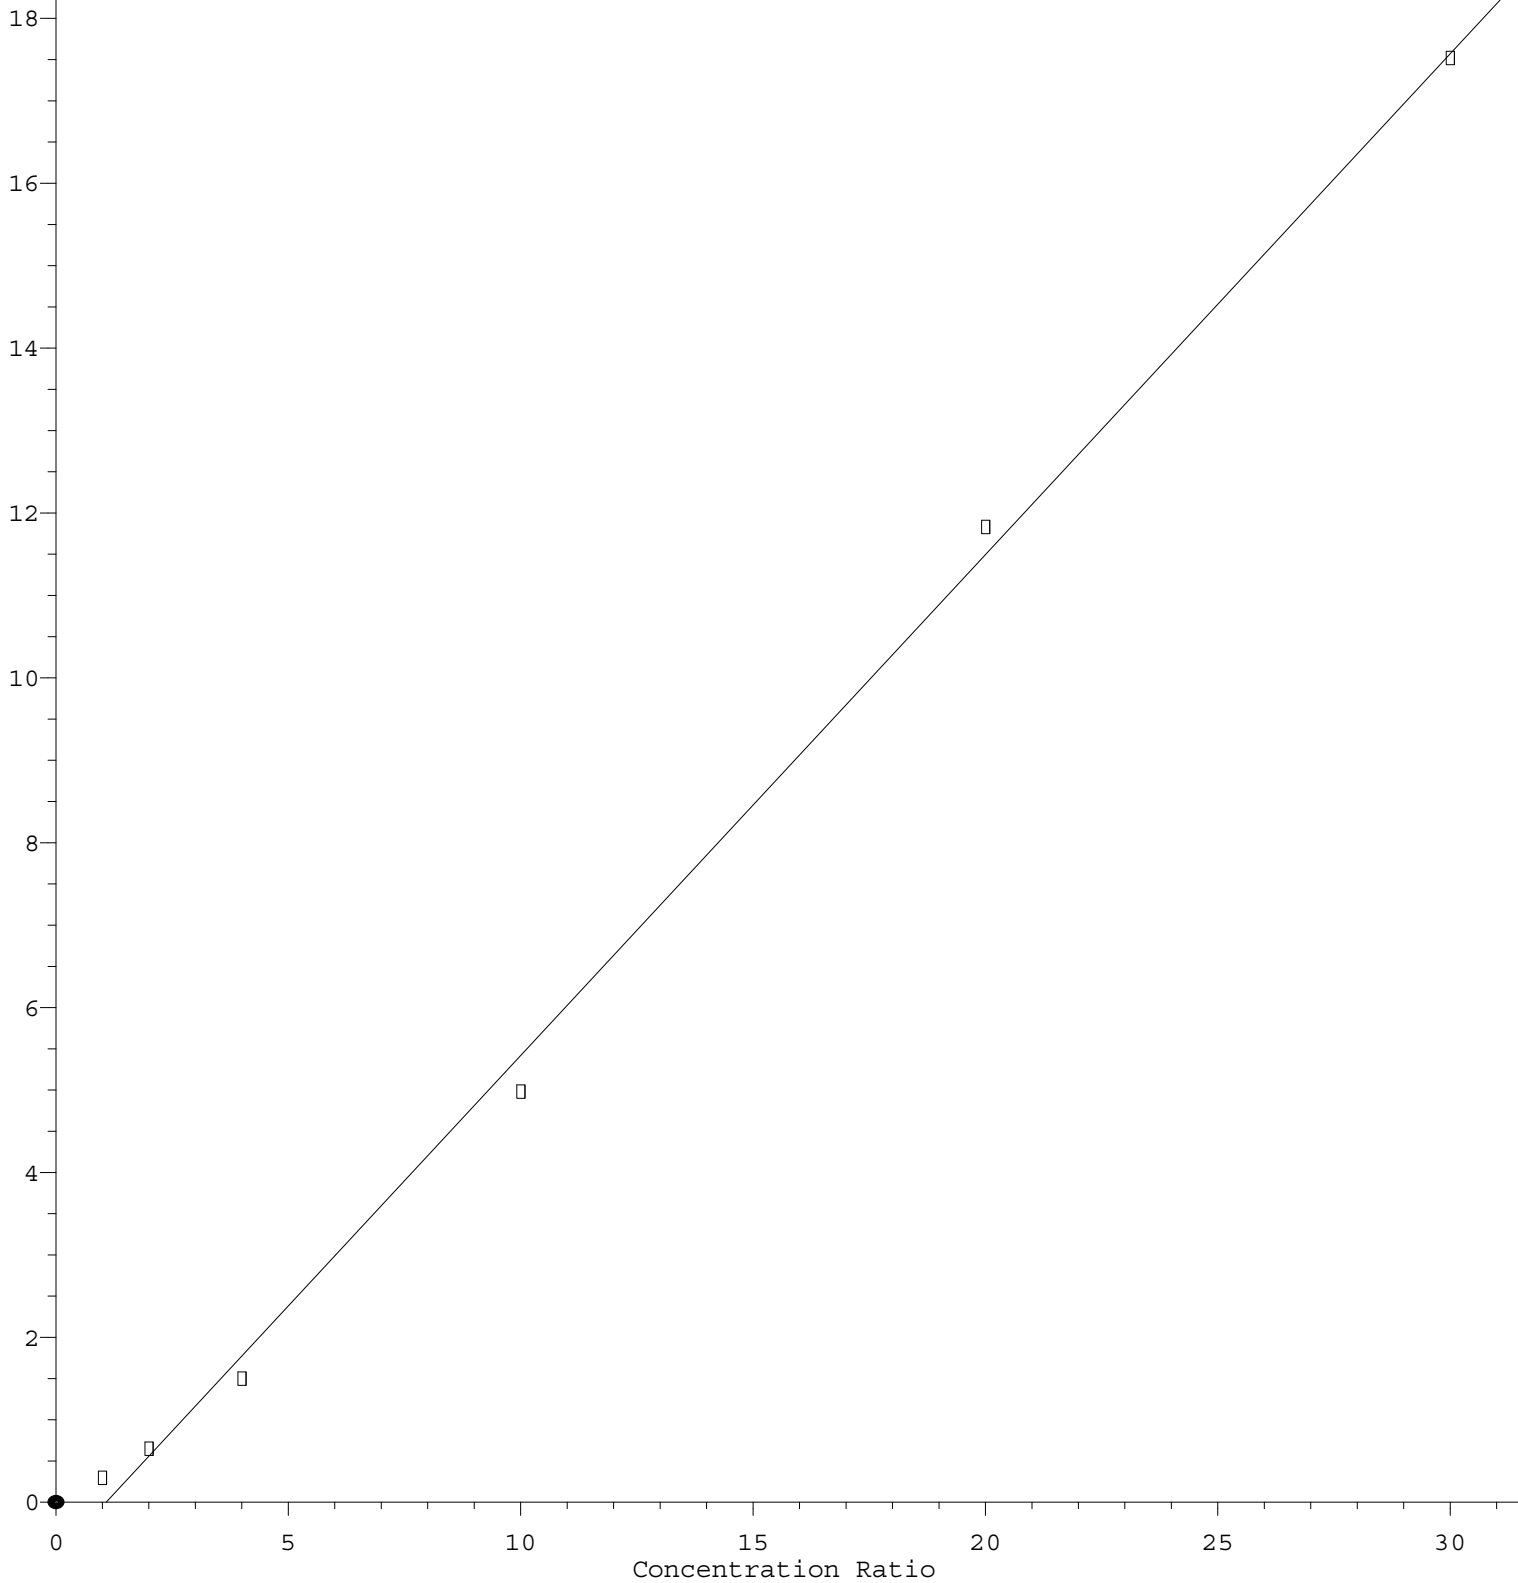

$$\text{Response} = 6.078\text{e-}001 * \text{Amt} - 6.591\text{e-}001$$


Coef of Det (r^2) = 0.997961 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

o-Xylene

Response Ratio

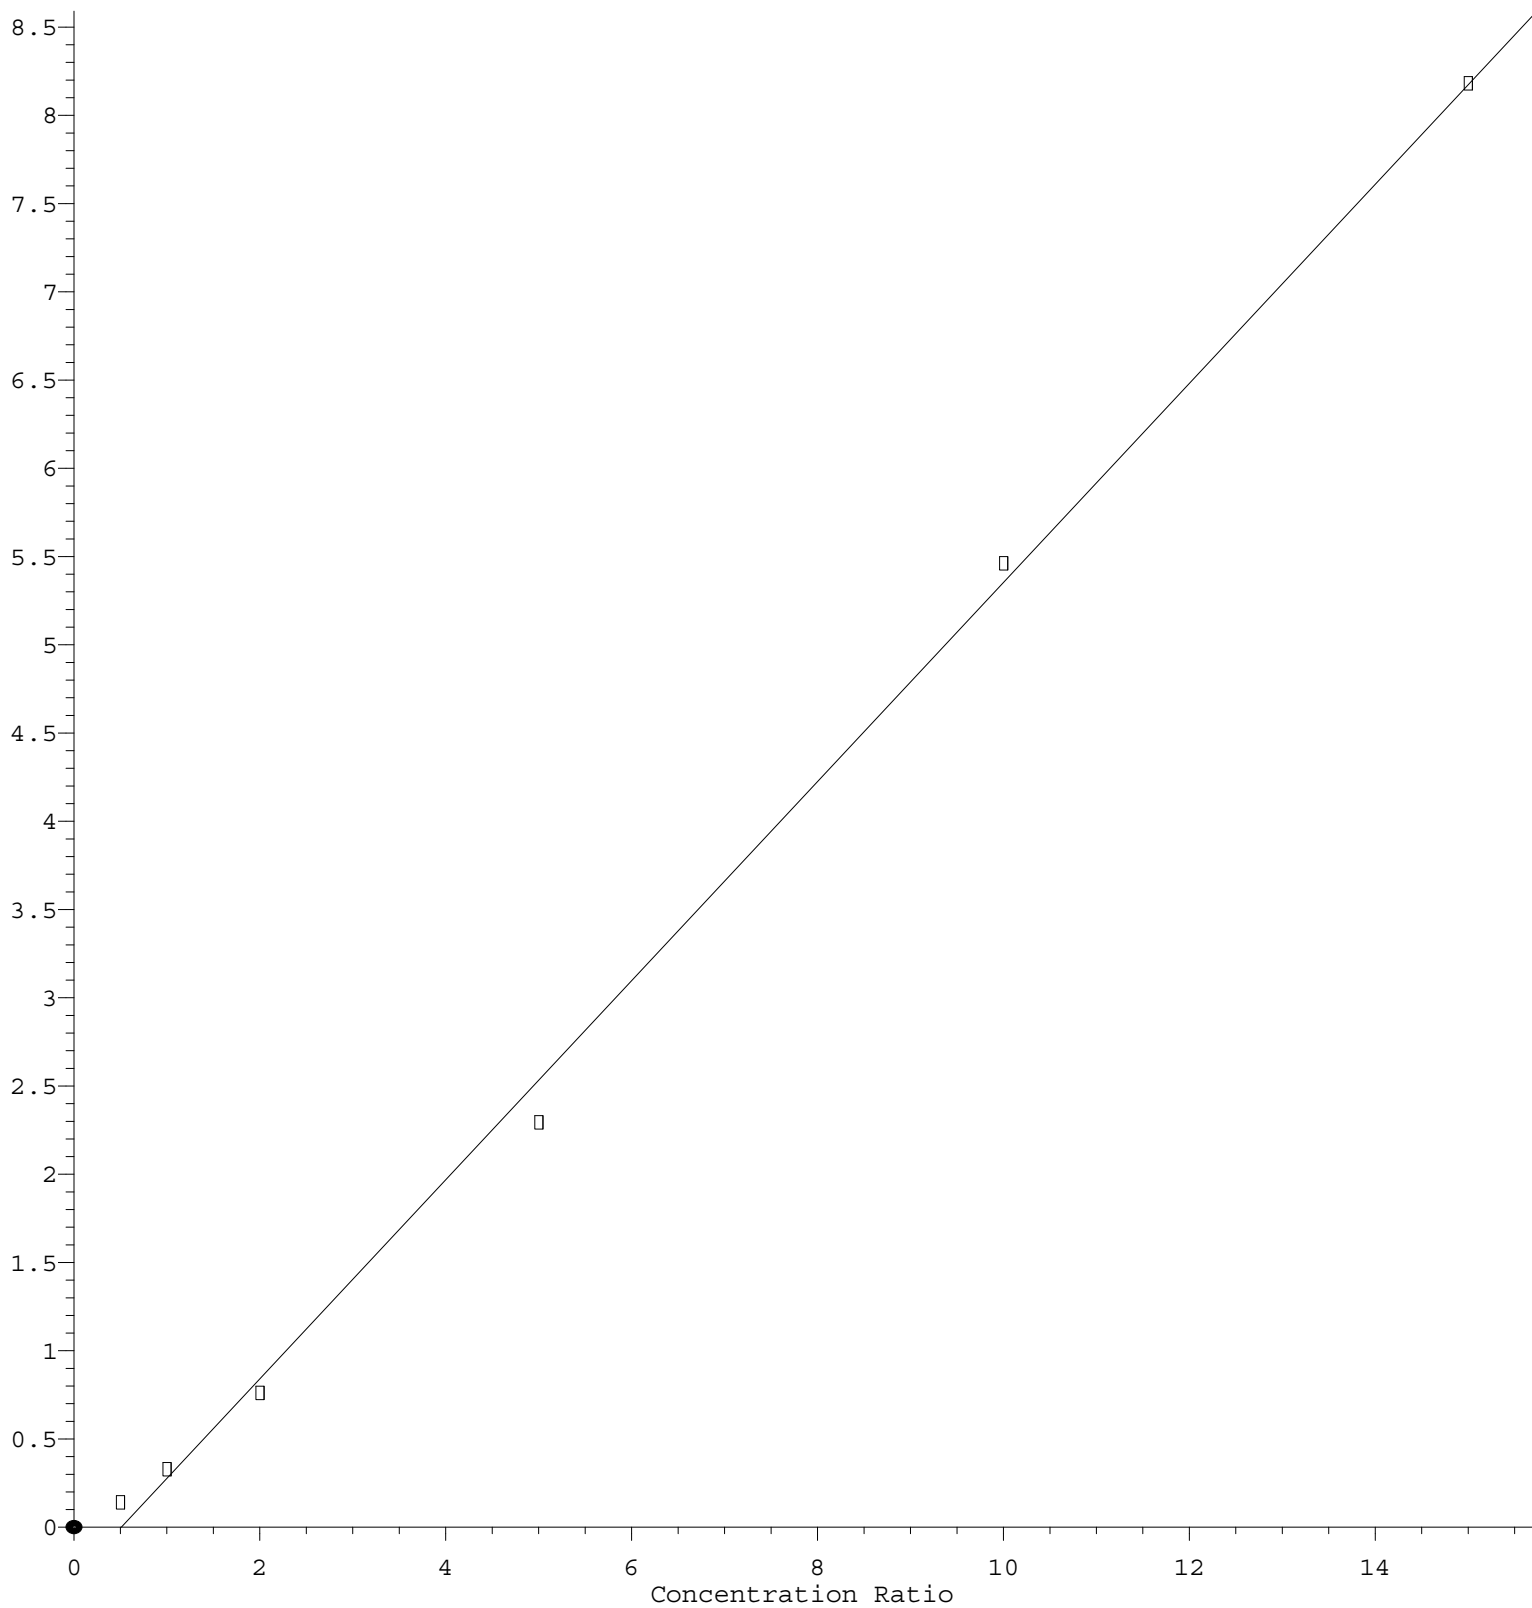

$$\text{Response} = 5.641\text{e-}001 * \text{Amt} - 2.885\text{e-}001$$


Coef of Det (r^2) = 0.998150 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Styrene


Response Ratio

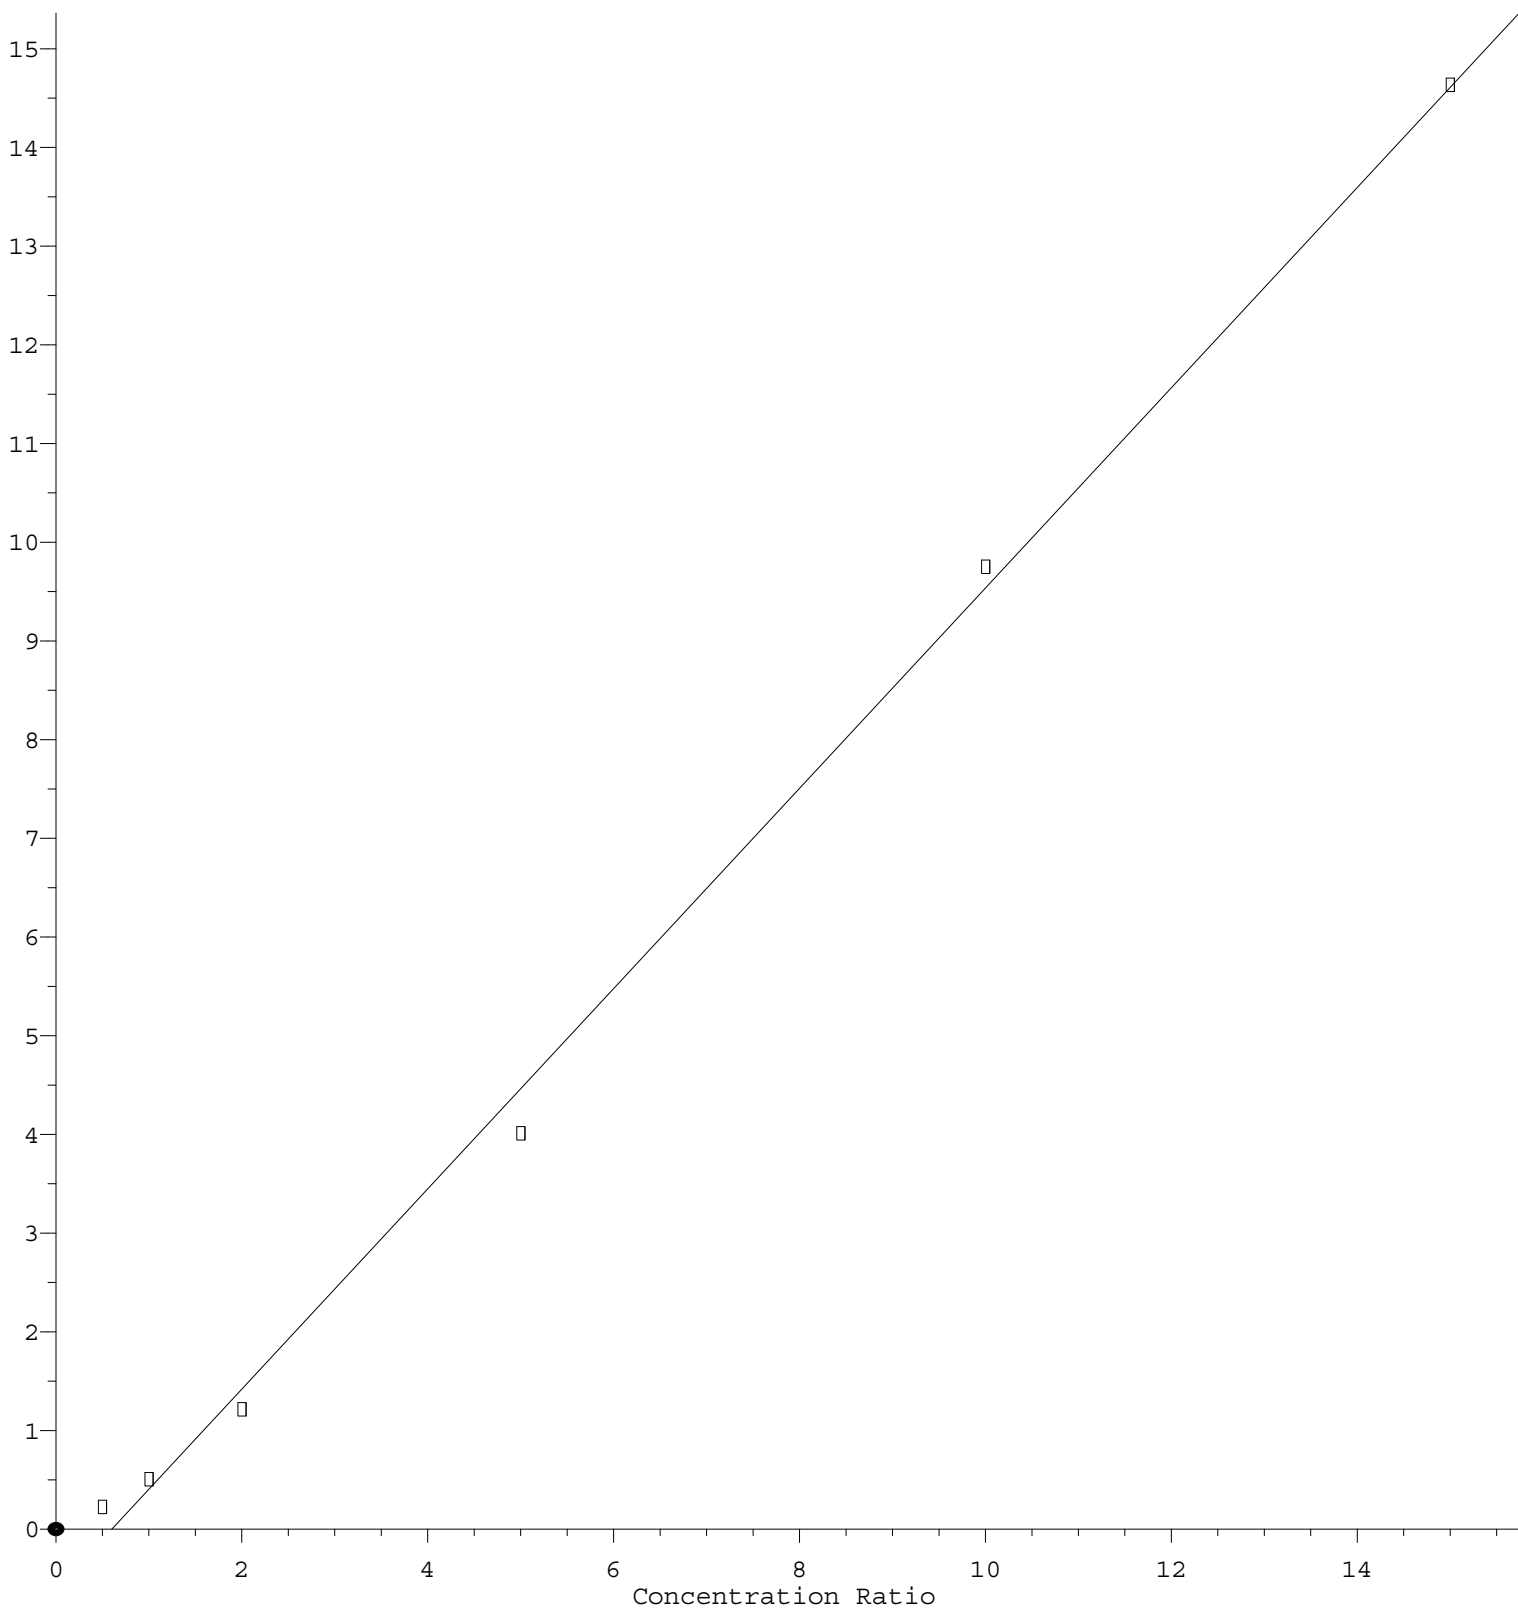

$\text{Response} = 1.015\text{e}+000 * \text{Amt} - 6.094\text{e}-001$
 Coef of Det (r^2) = 0.997627 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M
 Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Isopropylbenzene

Response Ratio

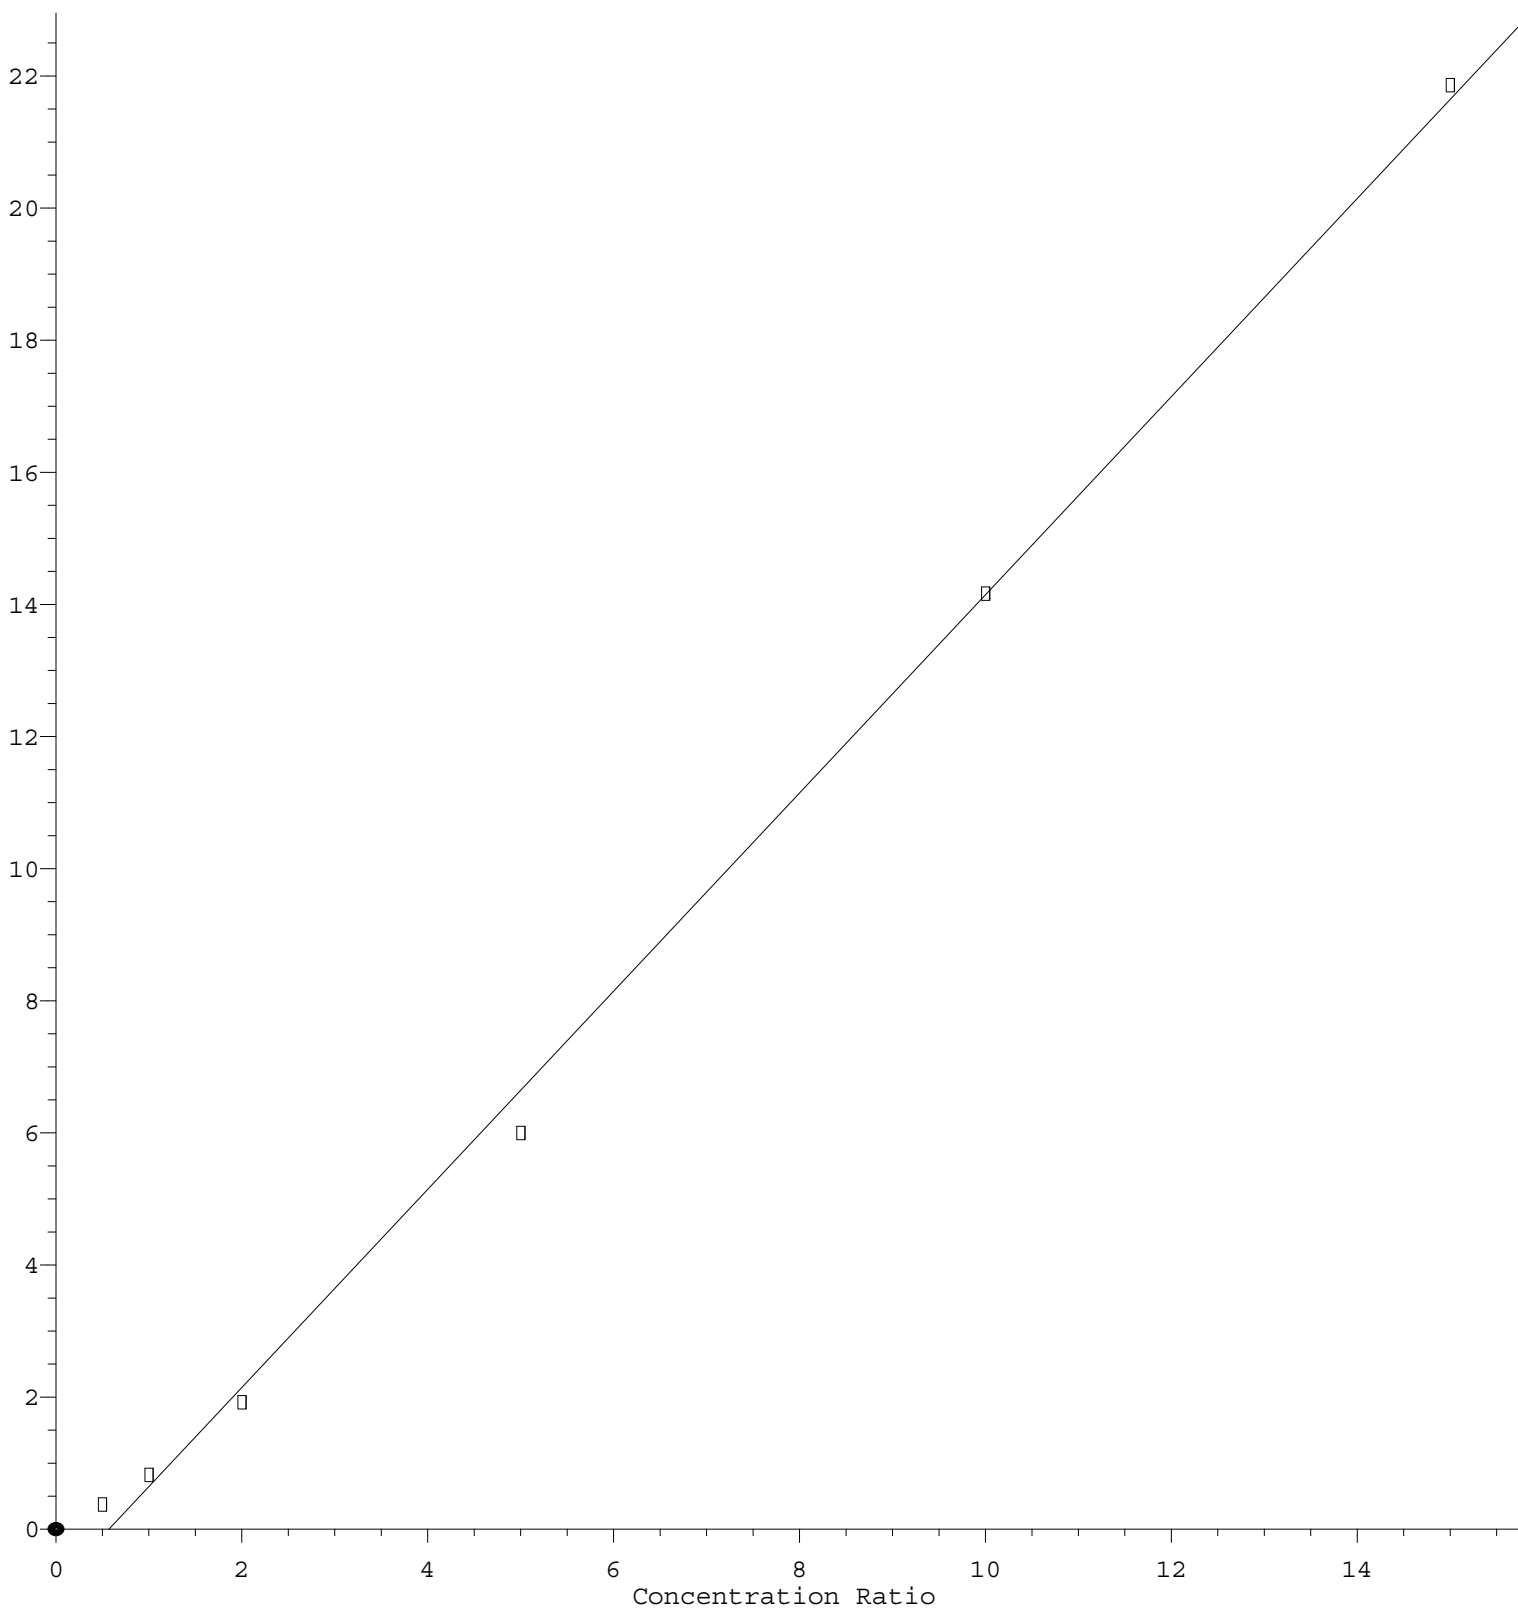

$$\text{Response} = 1.500\text{e}+000 * \text{Amt} - 8.544\text{e}-001$$


Coef of Det (r^2) = 0.997951 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

n-propylbenzene

Response Ratio

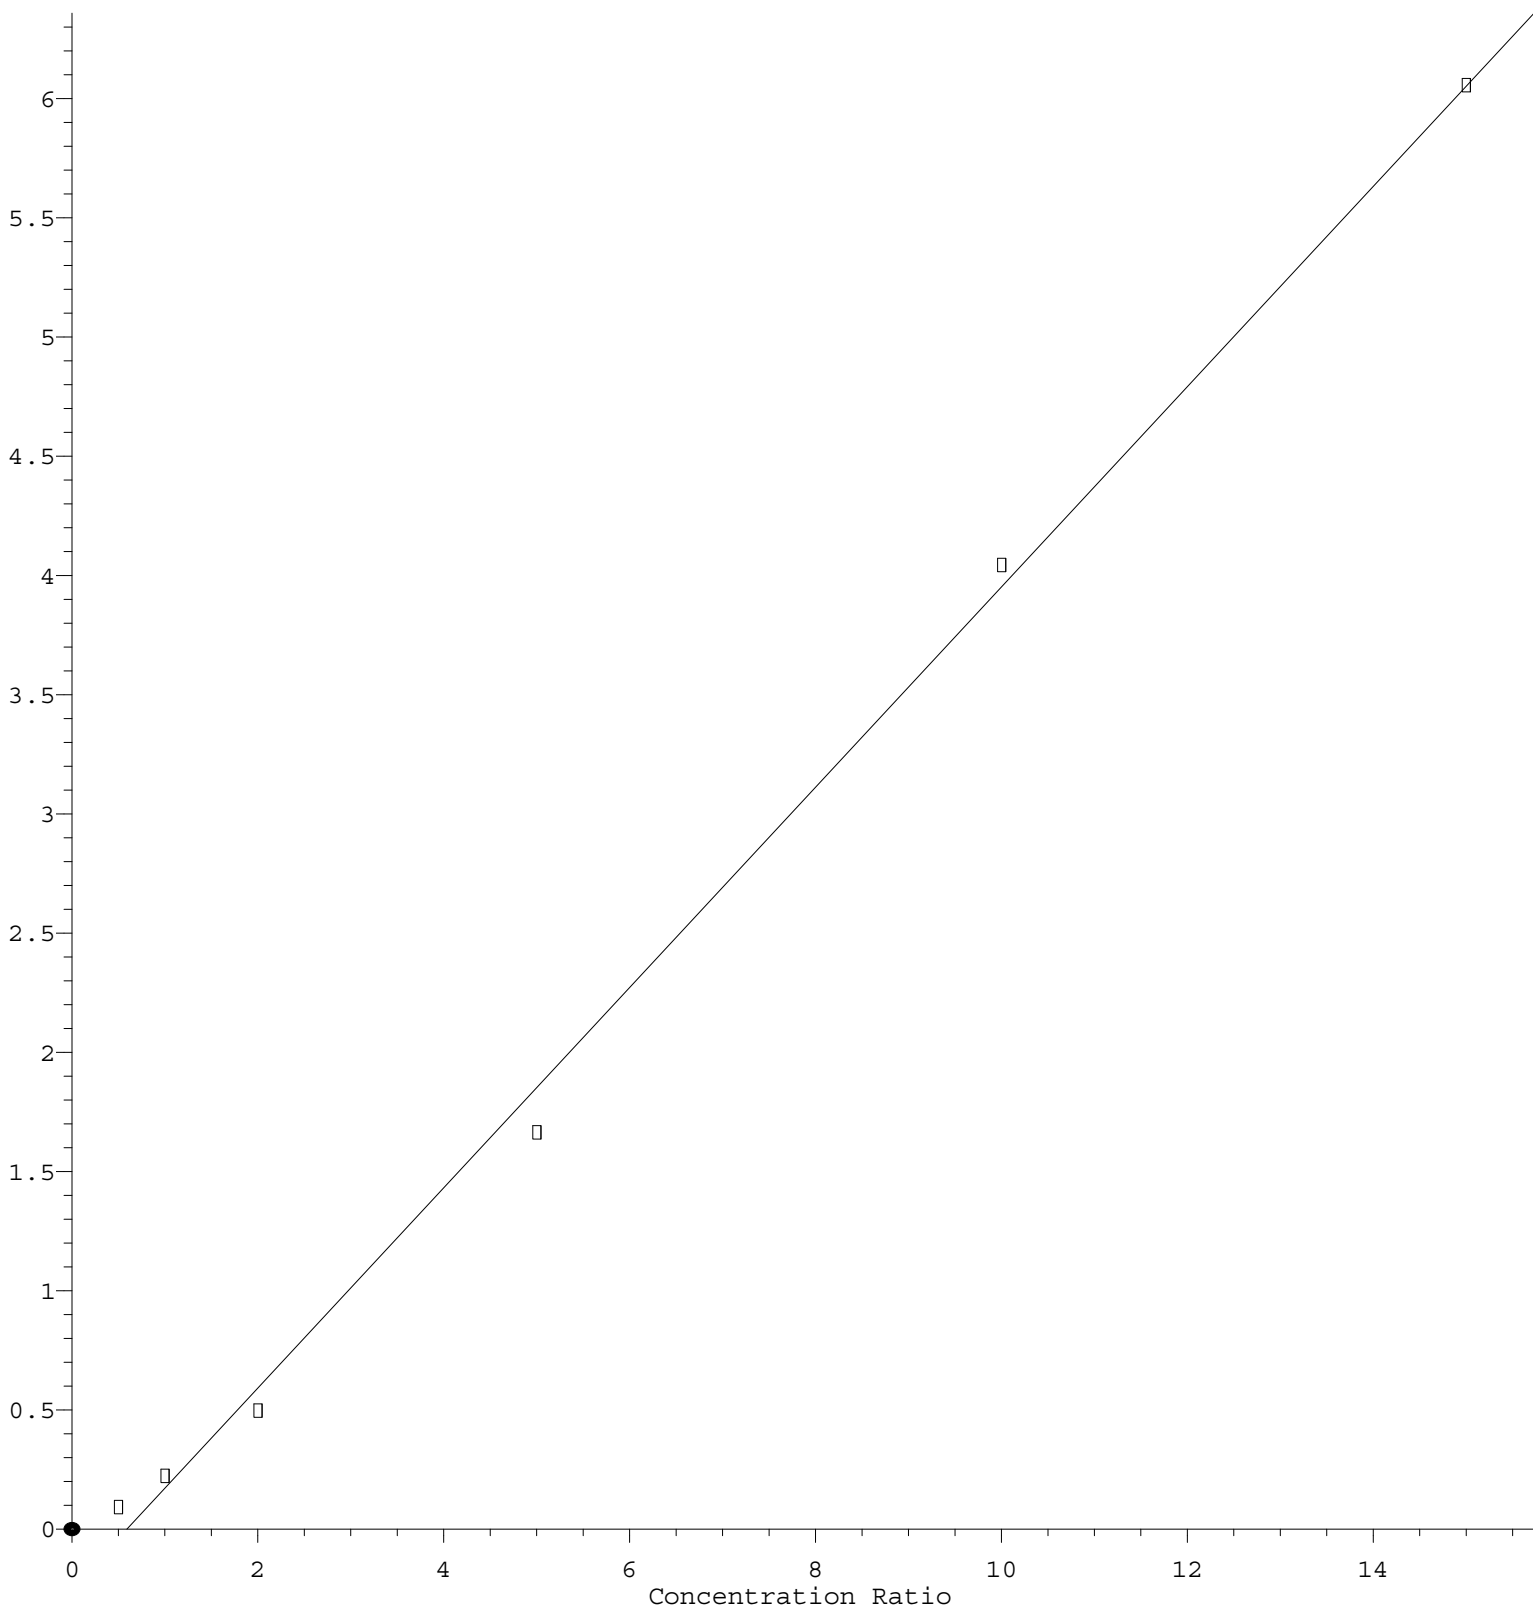

$$\text{Response} = 4.199\text{e-}001 * \text{Amt} - 2.487\text{e-}001$$


Coef of Det (r^2) = 0.997568 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

2-Chlorotoluene

Response Ratio

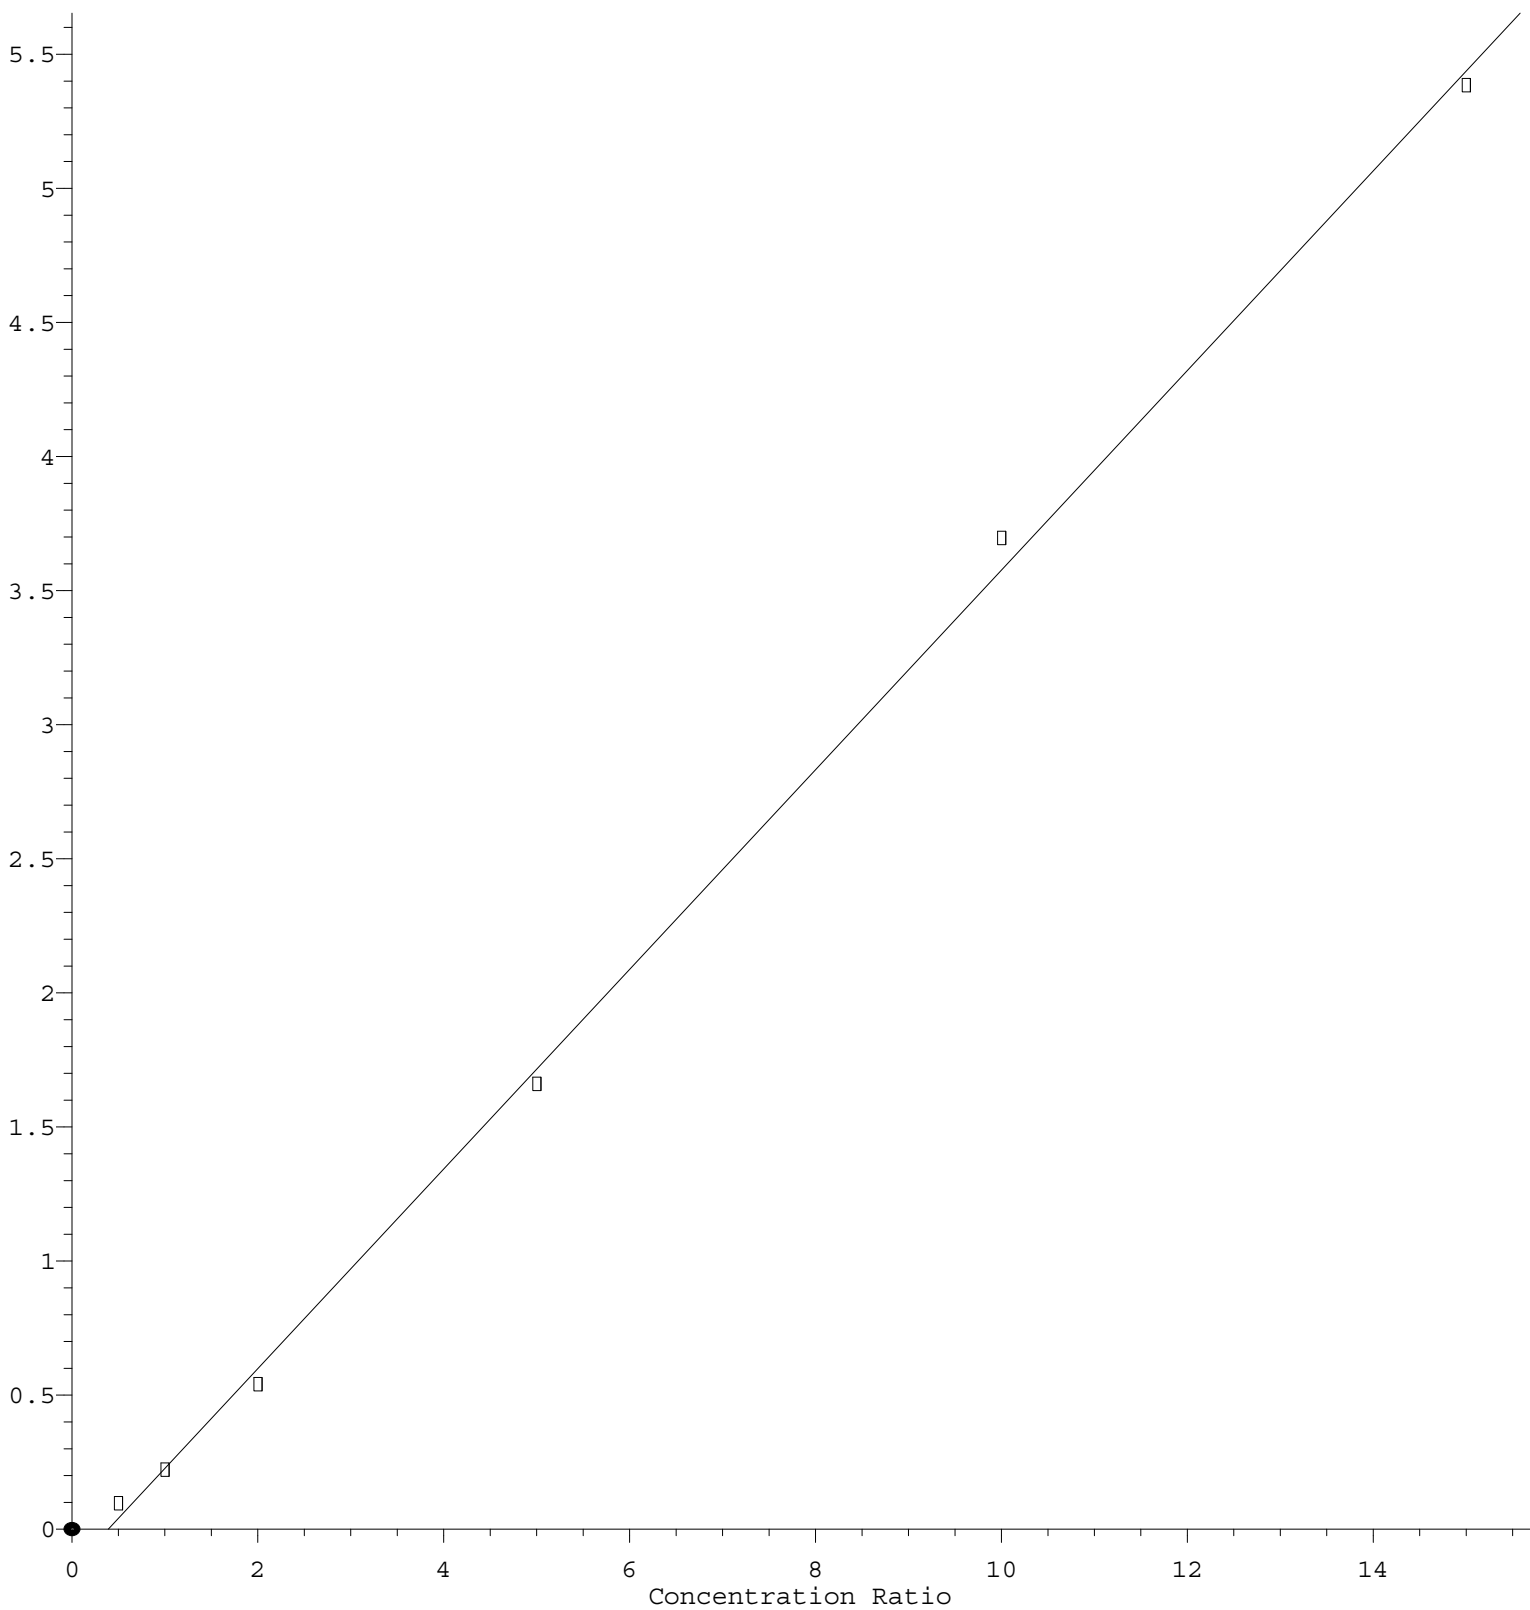

$$\text{Response} = 3.722\text{e-}001 * \text{Amt} - 1.451\text{e-}001$$


Coef of Det (r^2) = 0.998851 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

1,3,5-Trimethylbenzene

Response Ratio

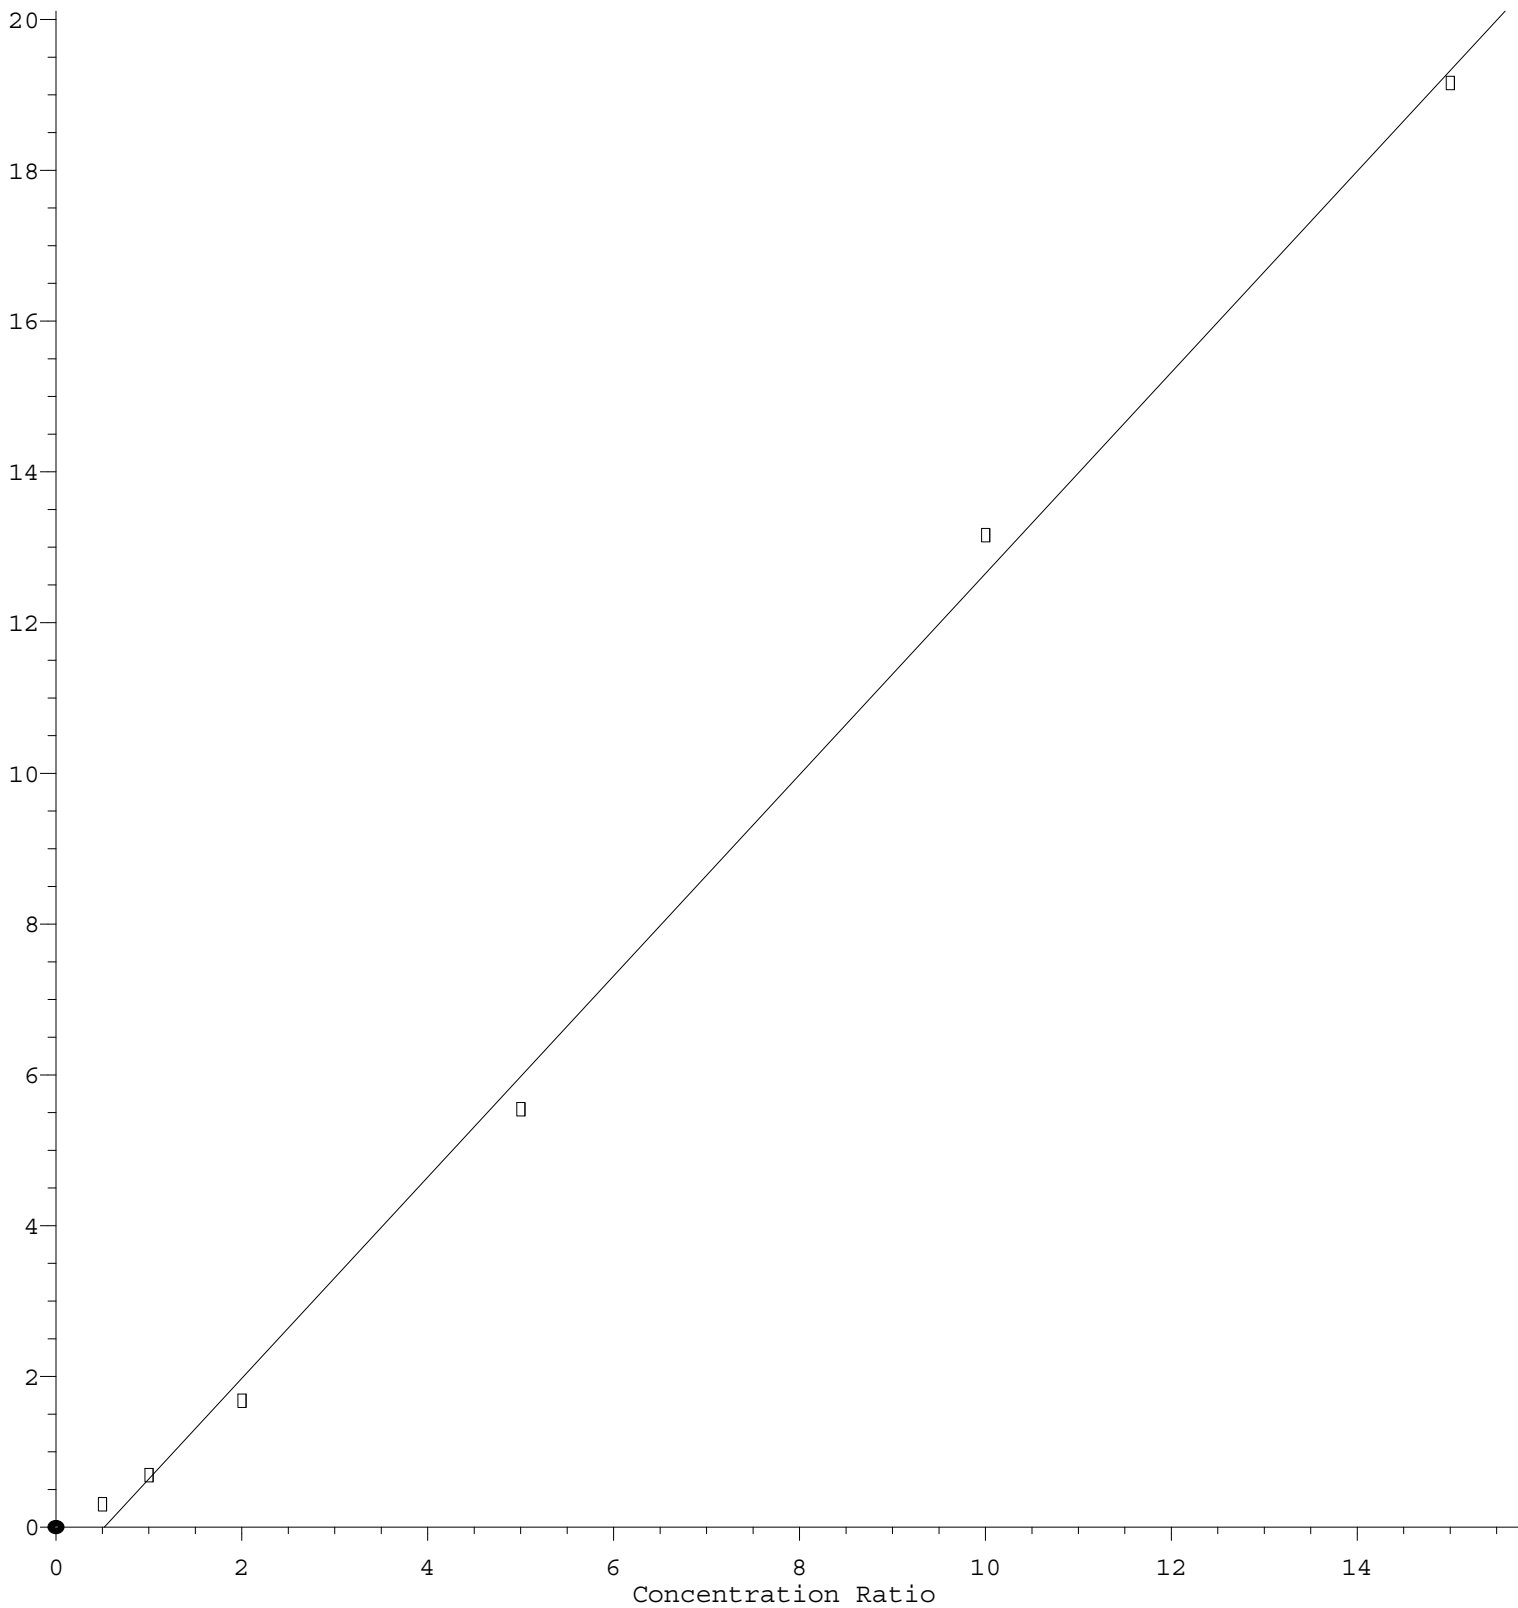

$$\text{Response} = 1.335\text{e}+000 * \text{Amt} - 6.993\text{e}-001$$


Coef of Det (r^2) = 0.997747 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

4-Chlorotoluene

Response Ratio

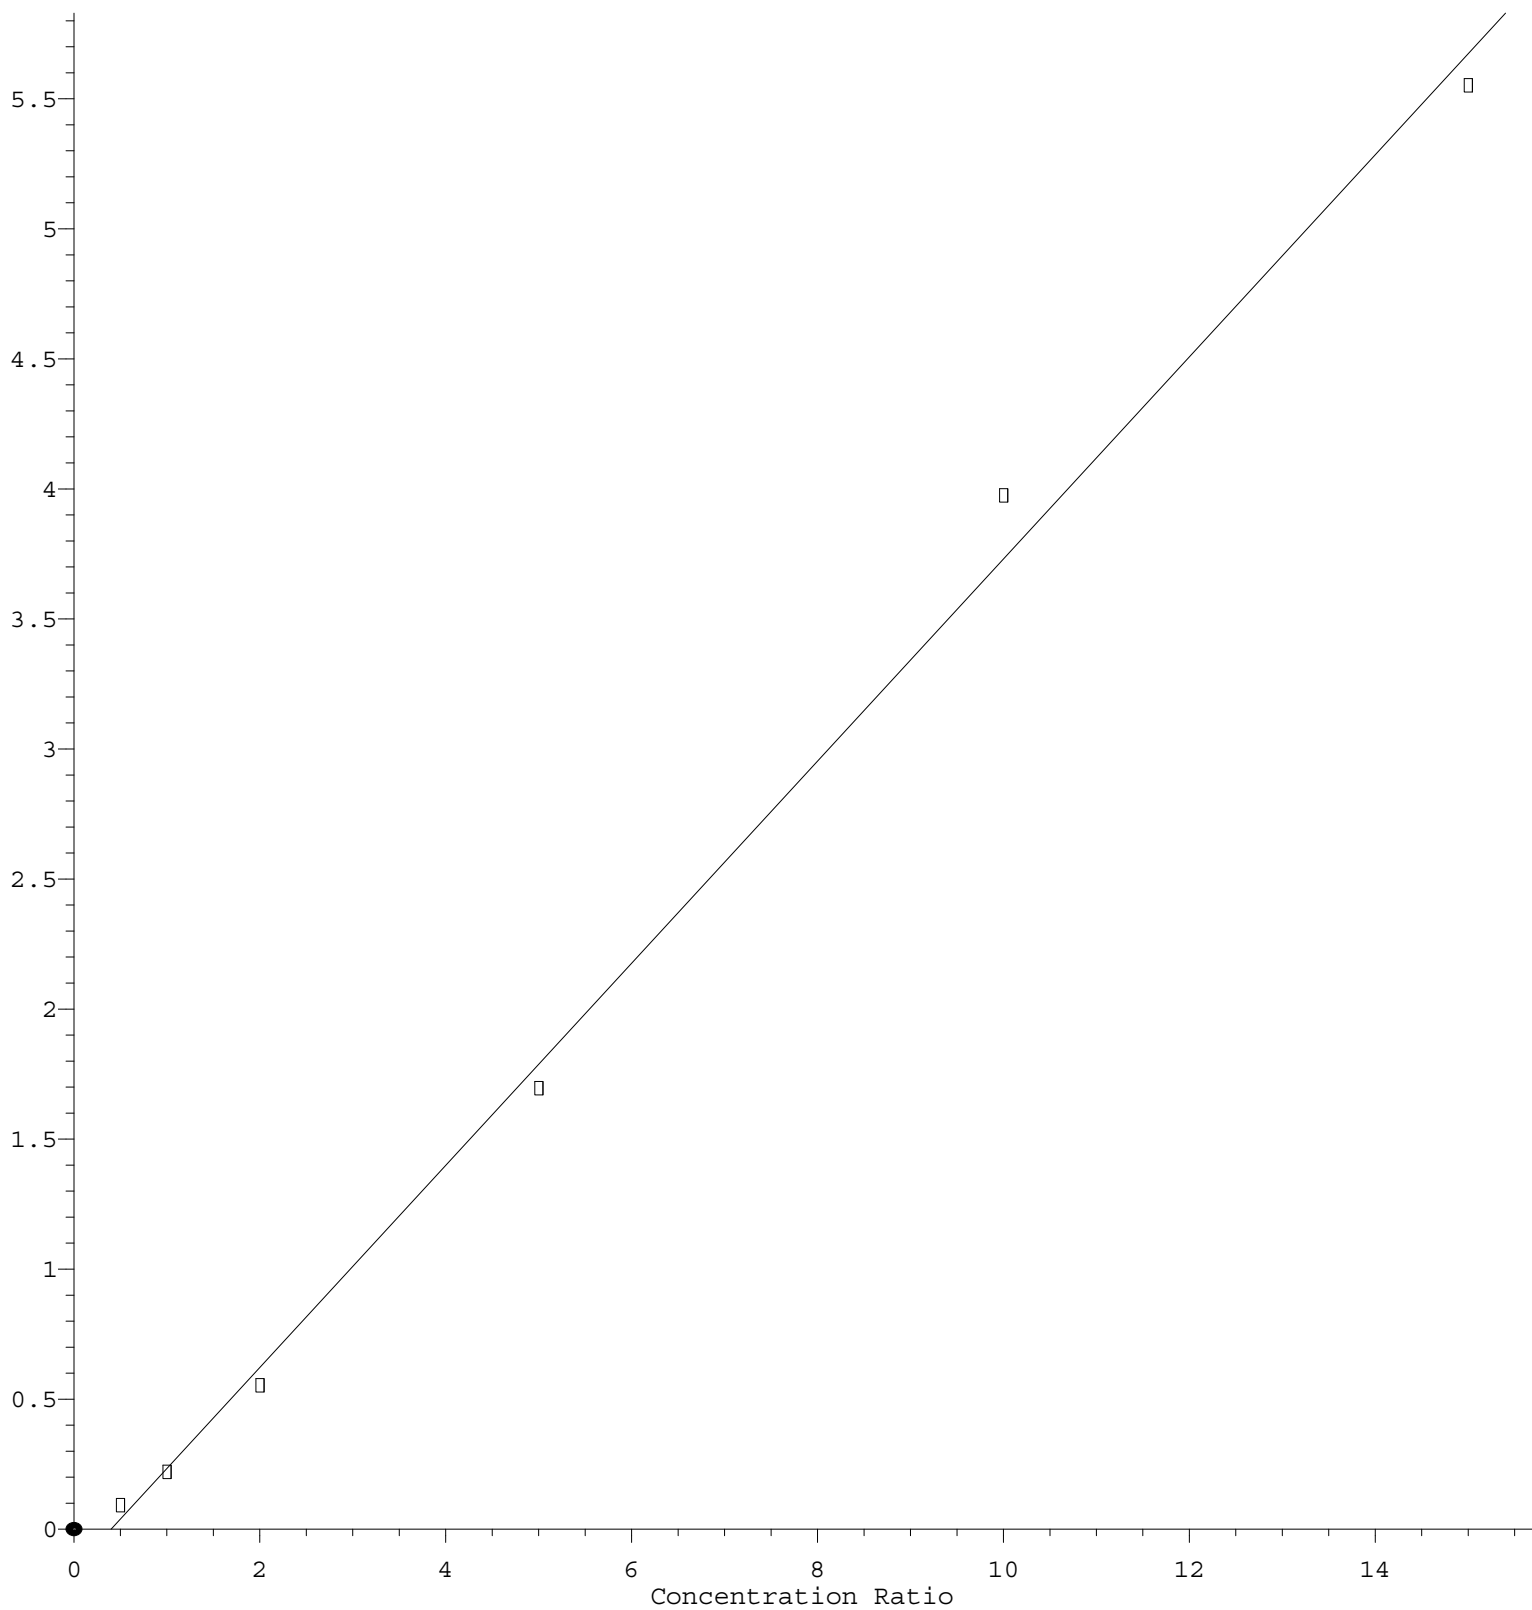

$$\text{Response} = 3.887\text{e-}001 * \text{Amt} - 1.559\text{e-}001$$


Coef of Det (r^2) = 0.996444 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

tert-Butylbenzene

Response Ratio

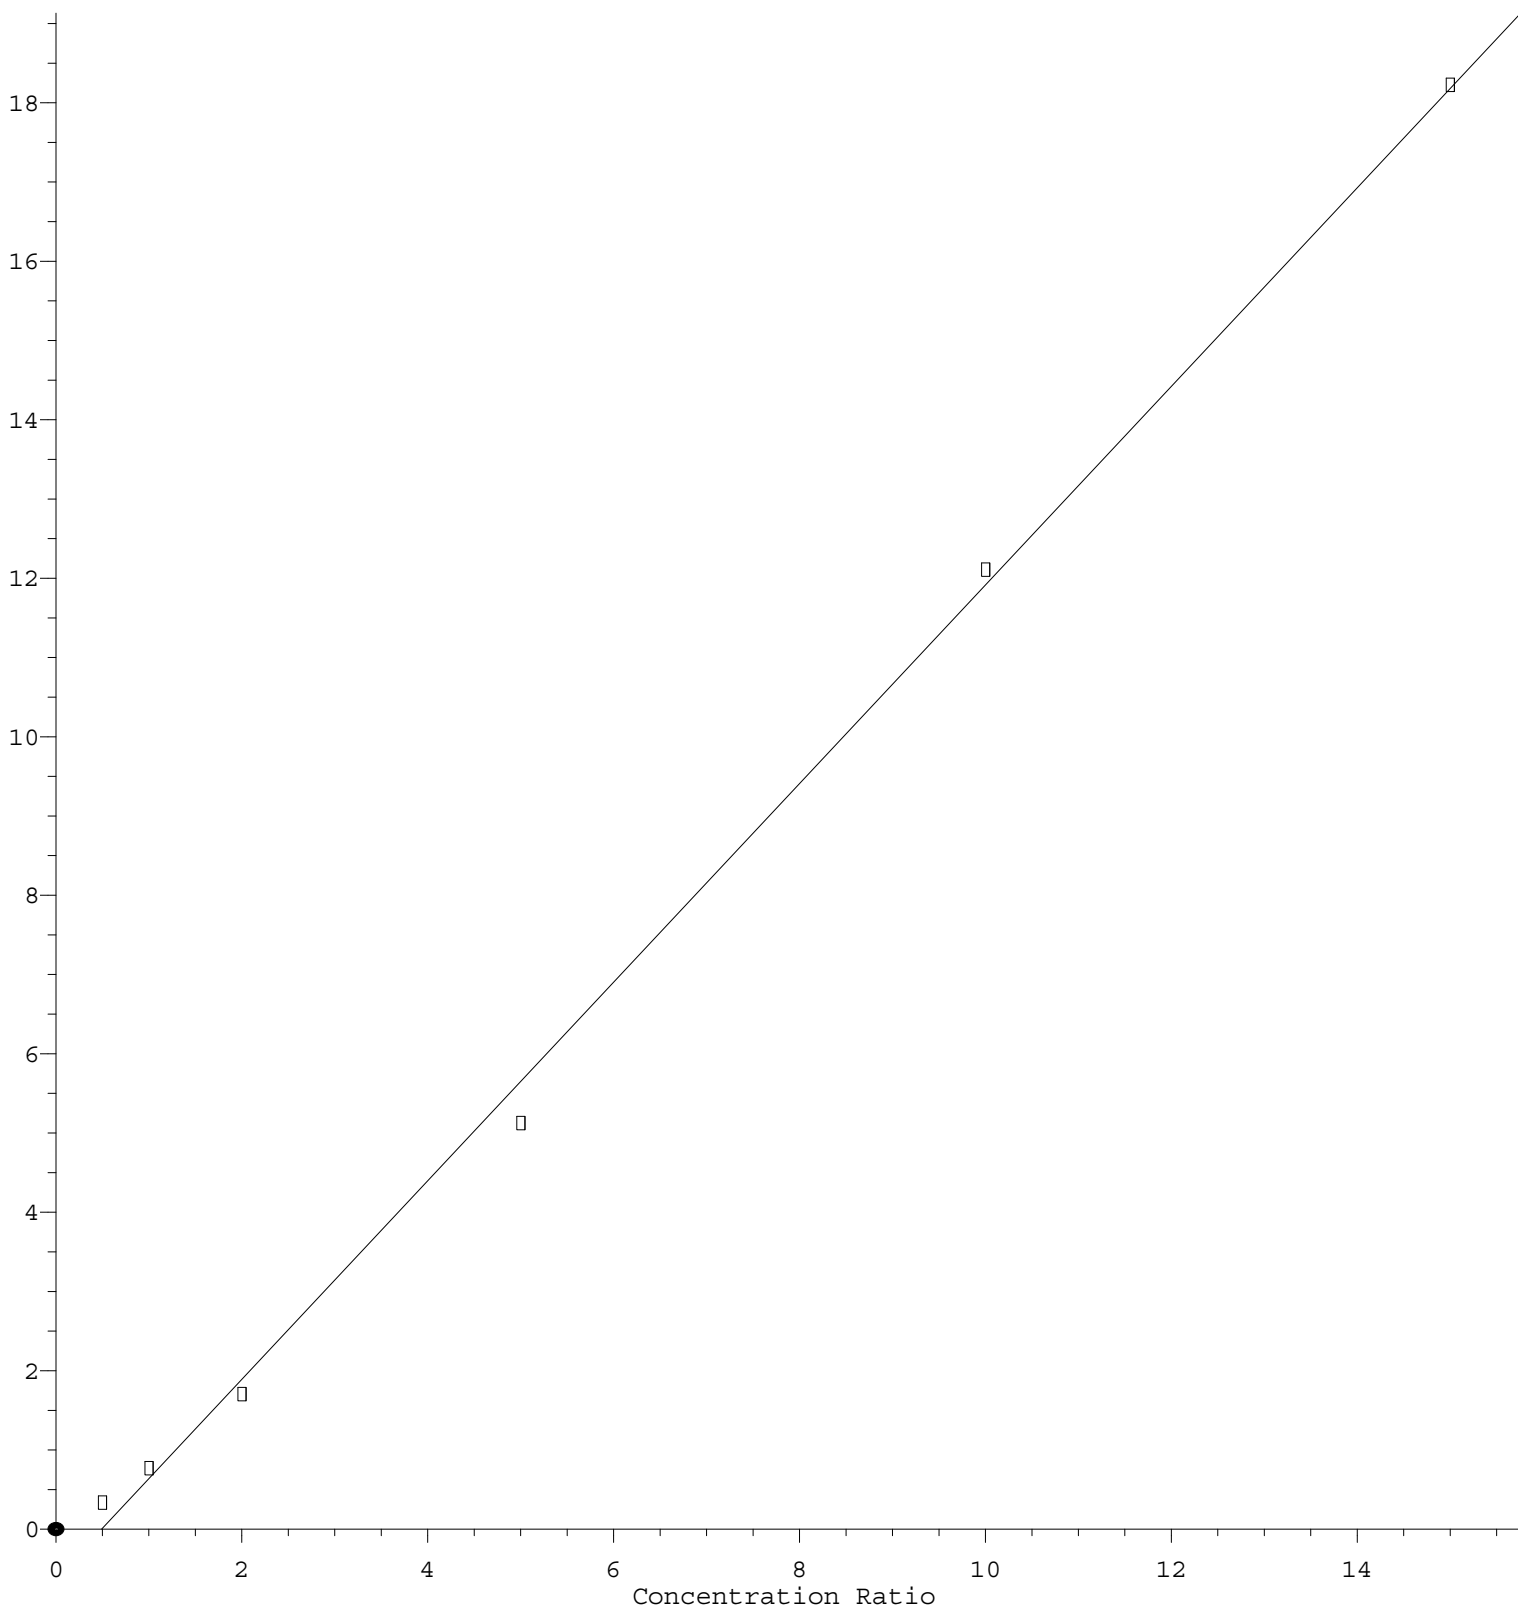

$$\text{Response} = 1.253\text{e}+000 * \text{Amt} - 6.190\text{e}-001$$


Coef of Det (r^2) = 0.998213 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

1,2,4-Trimethylbenzene

Response Ratio

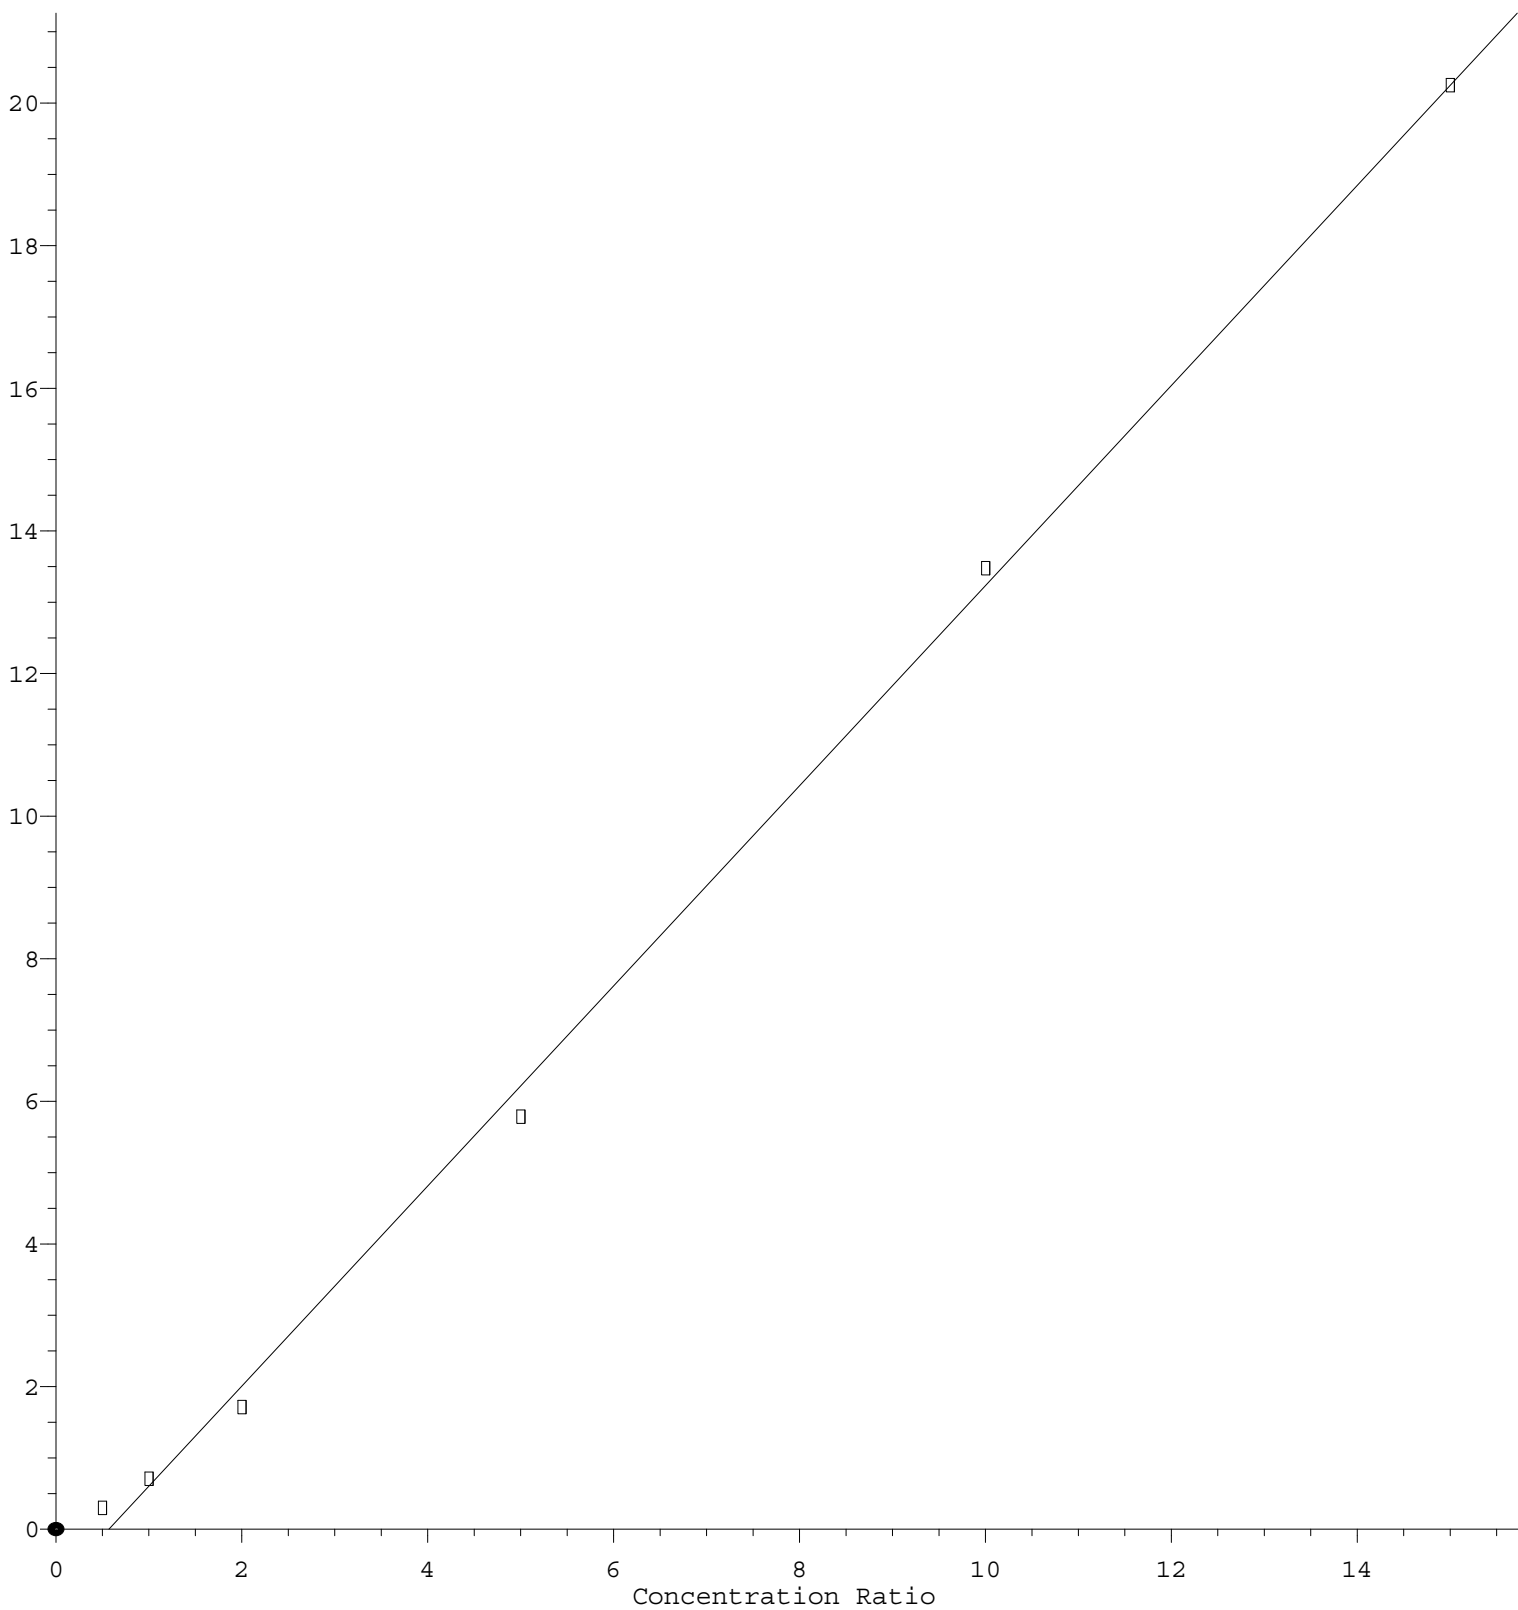

$$\text{Response} = 1.403\text{e}+000 * \text{Amt} - 7.933\text{e}-001$$


Coef of Det (r^2) = 0.998489 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

sec-Butylbenzene


Response Ratio

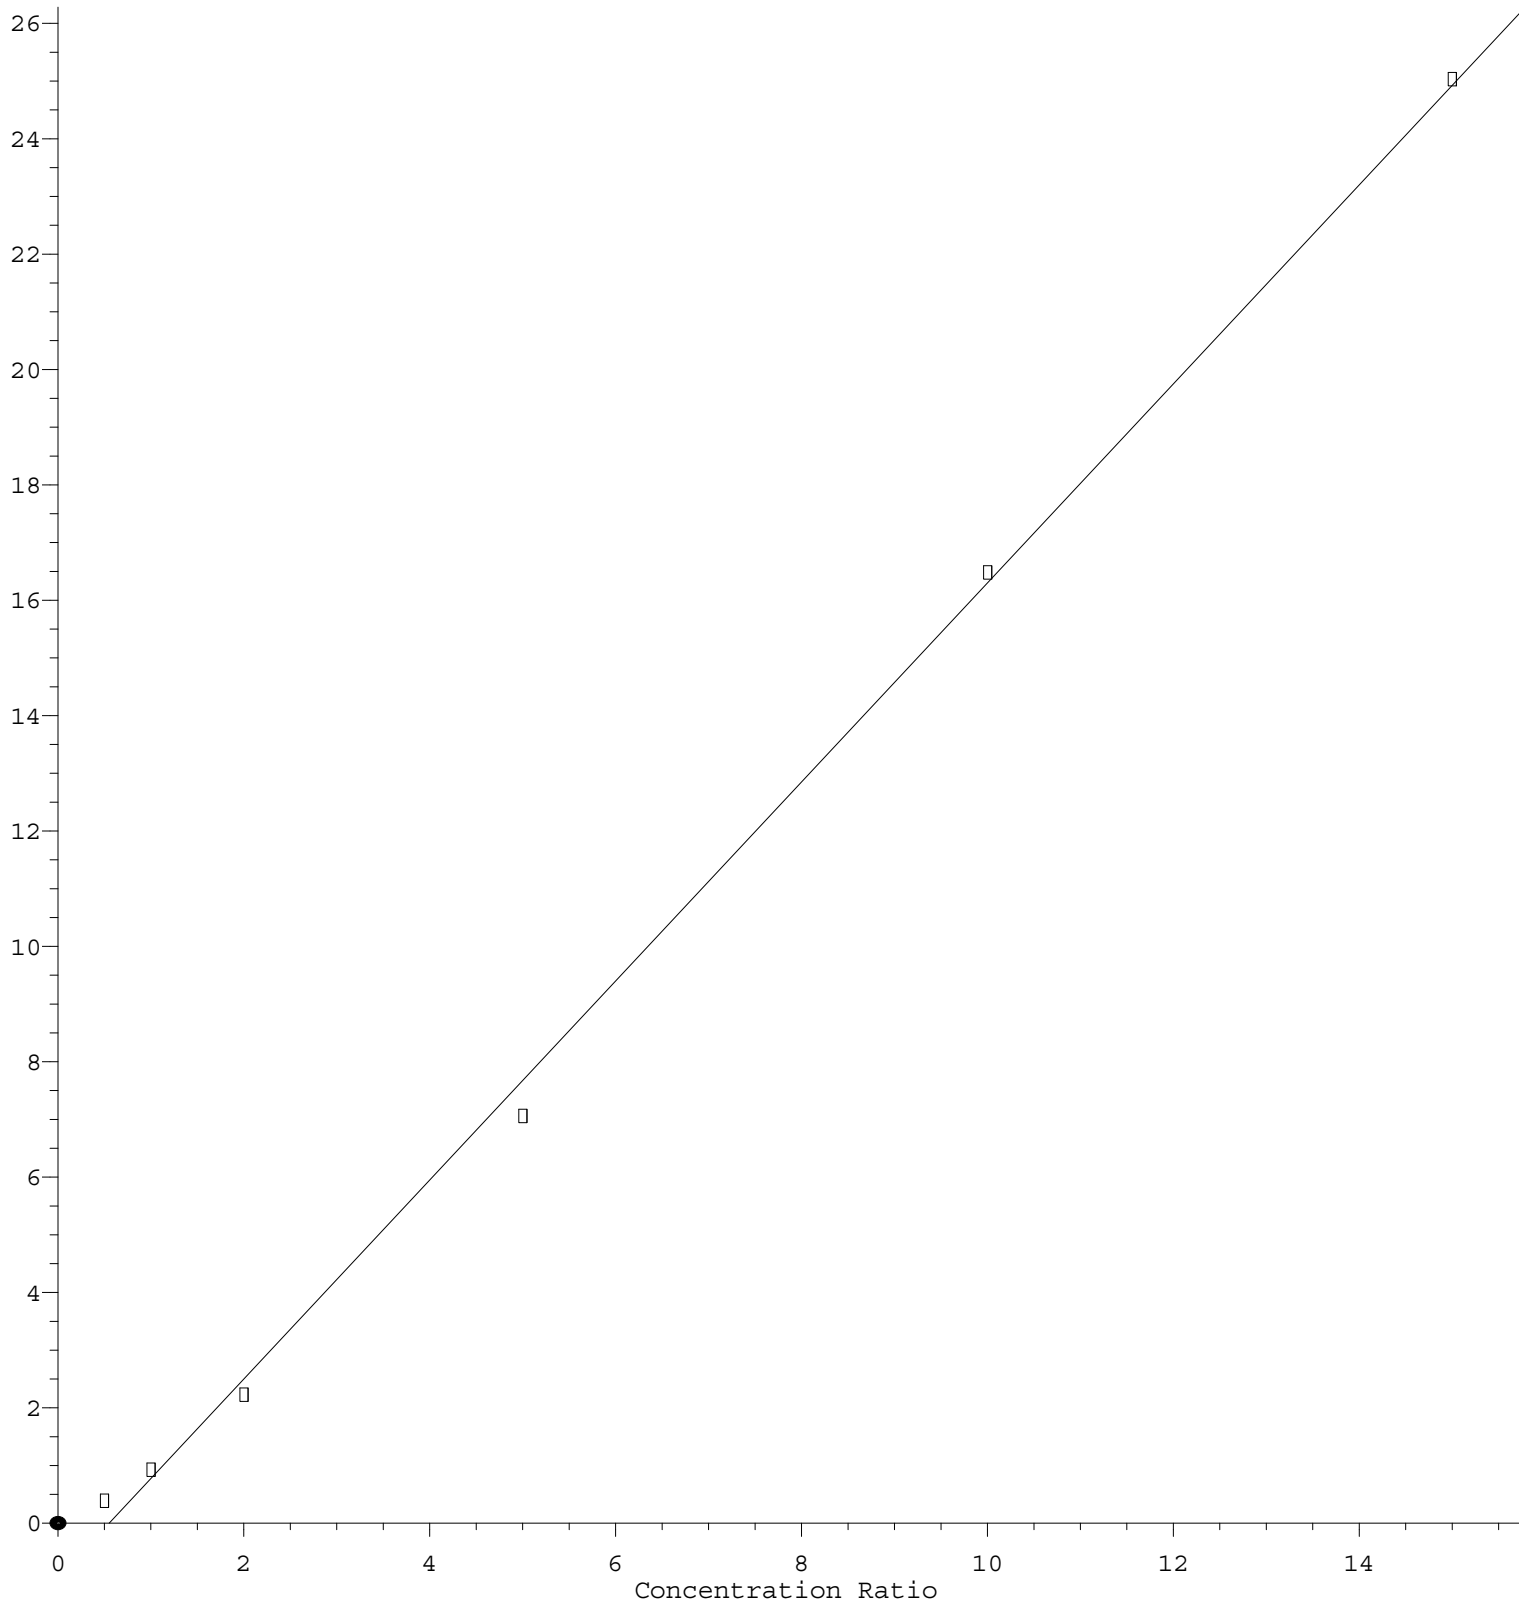

Response = 1.725e+000 * Amt - 9.469e-001
 Coef of Det (r^2) = 0.998507 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M
 Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

p-Isopropyltoluene

Response Ratio

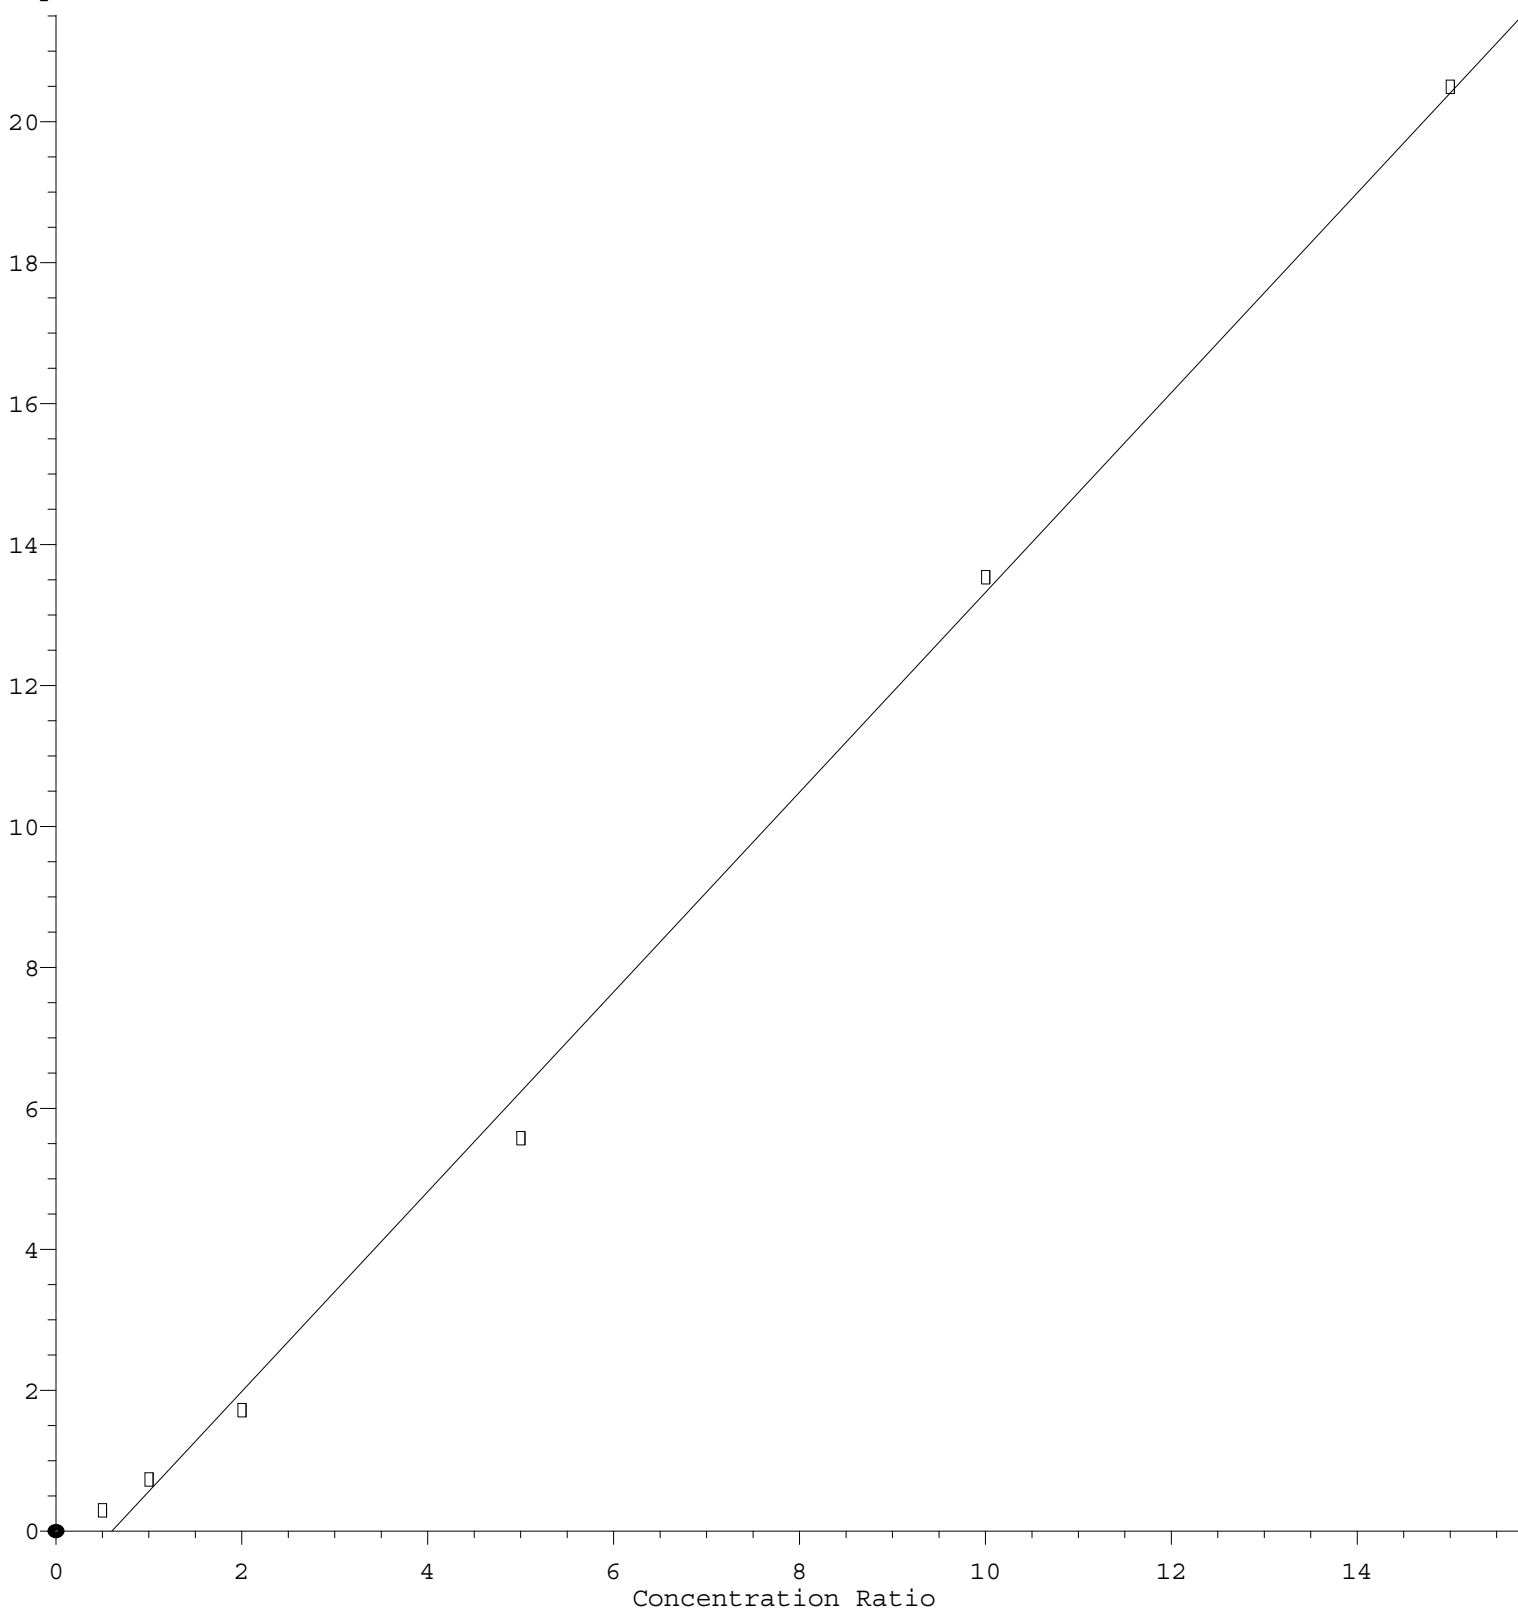

$$\text{Response} = 1.418\text{e}+000 * \text{Amt} - 8.577\text{e}-001$$


Coef of Det (r^2) = 0.997705 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

p-Isopropyltoluene

Response Ratio

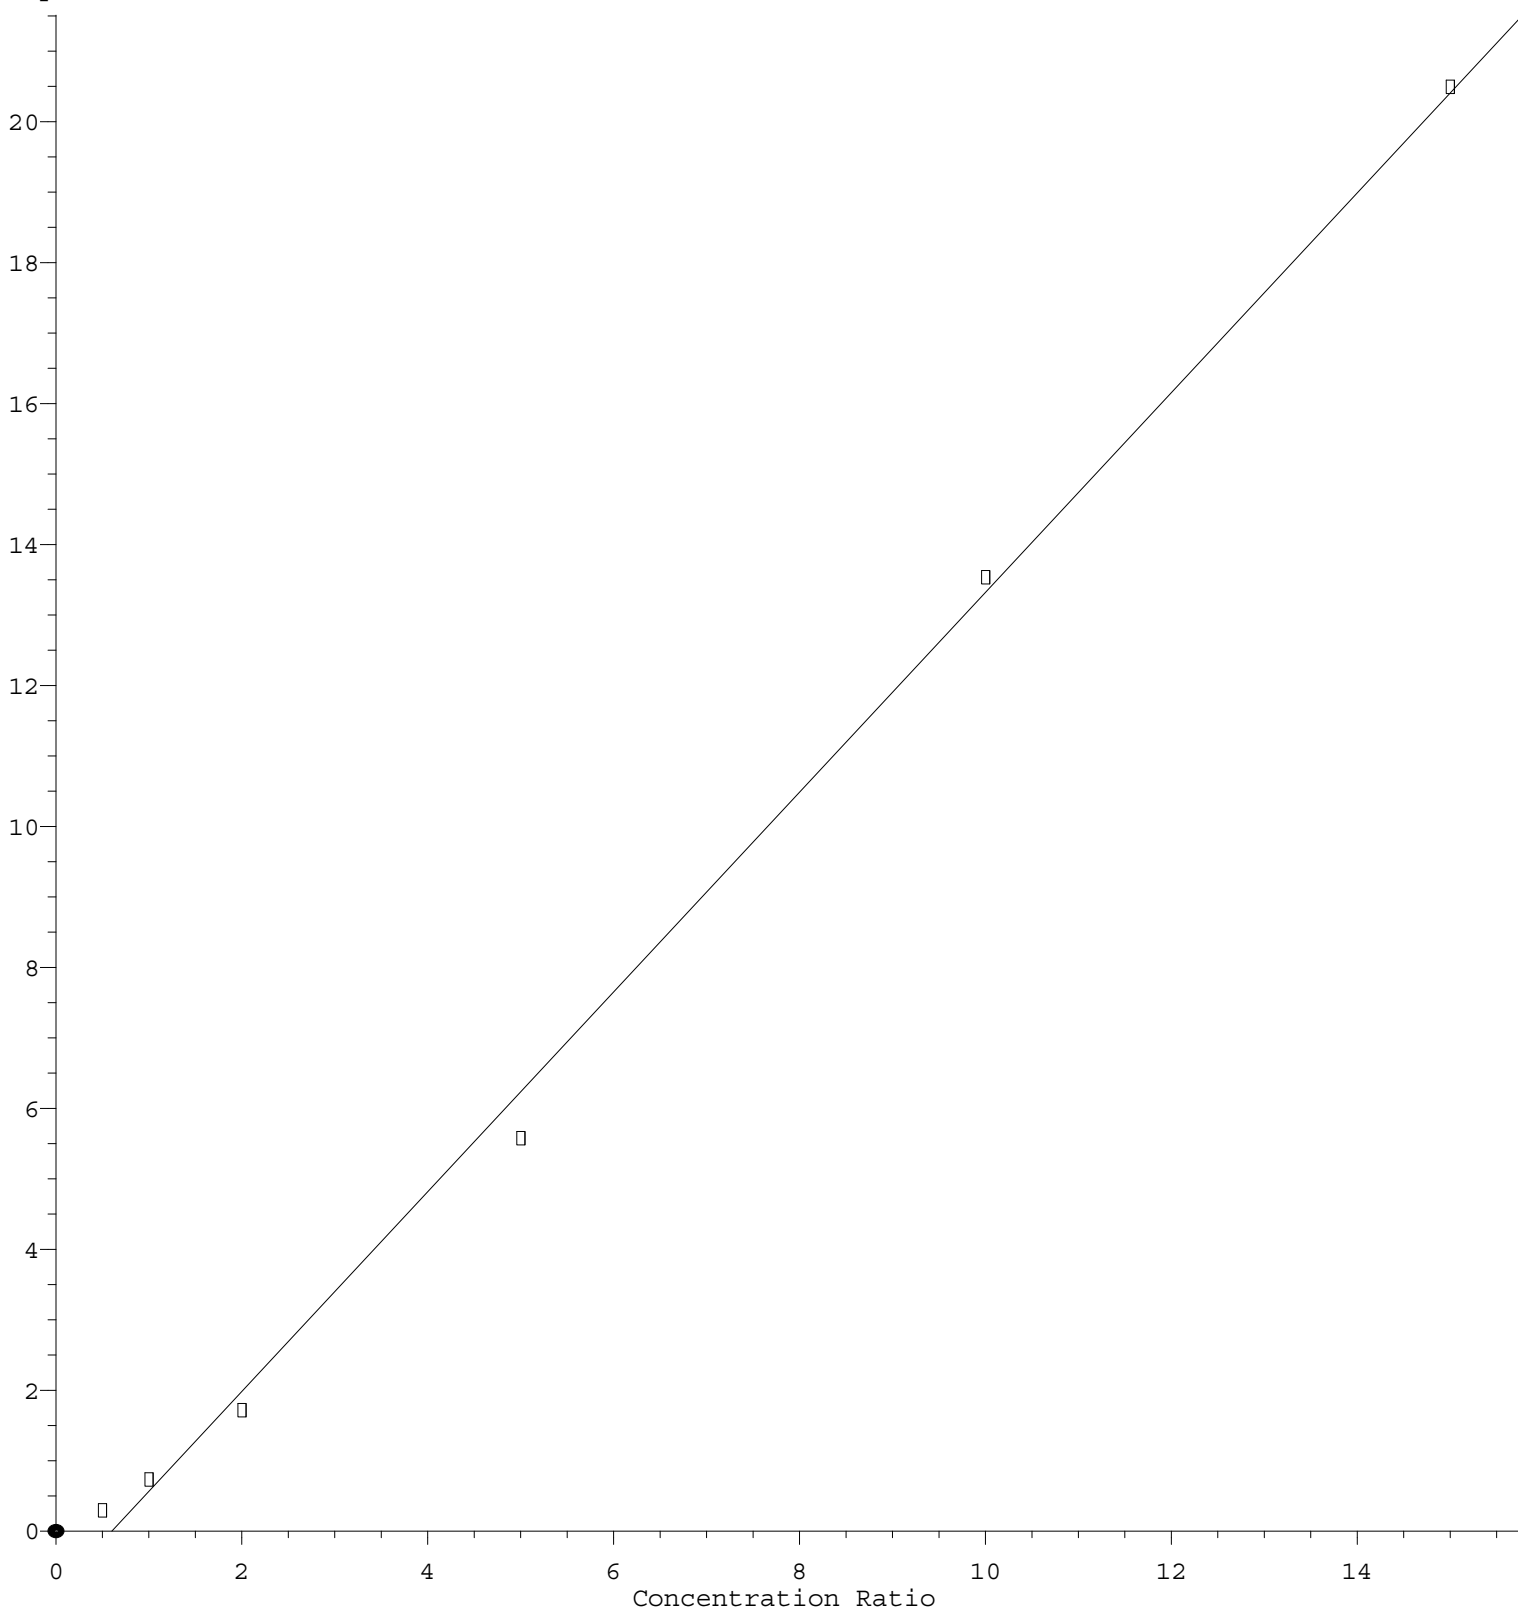

$$\text{Response} = 1.418\text{e}+000 * \text{Amt} - 8.577\text{e}-001$$


Coef of Det (r^2) = 0.997705 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

n-Butylbenzene

Response Ratio

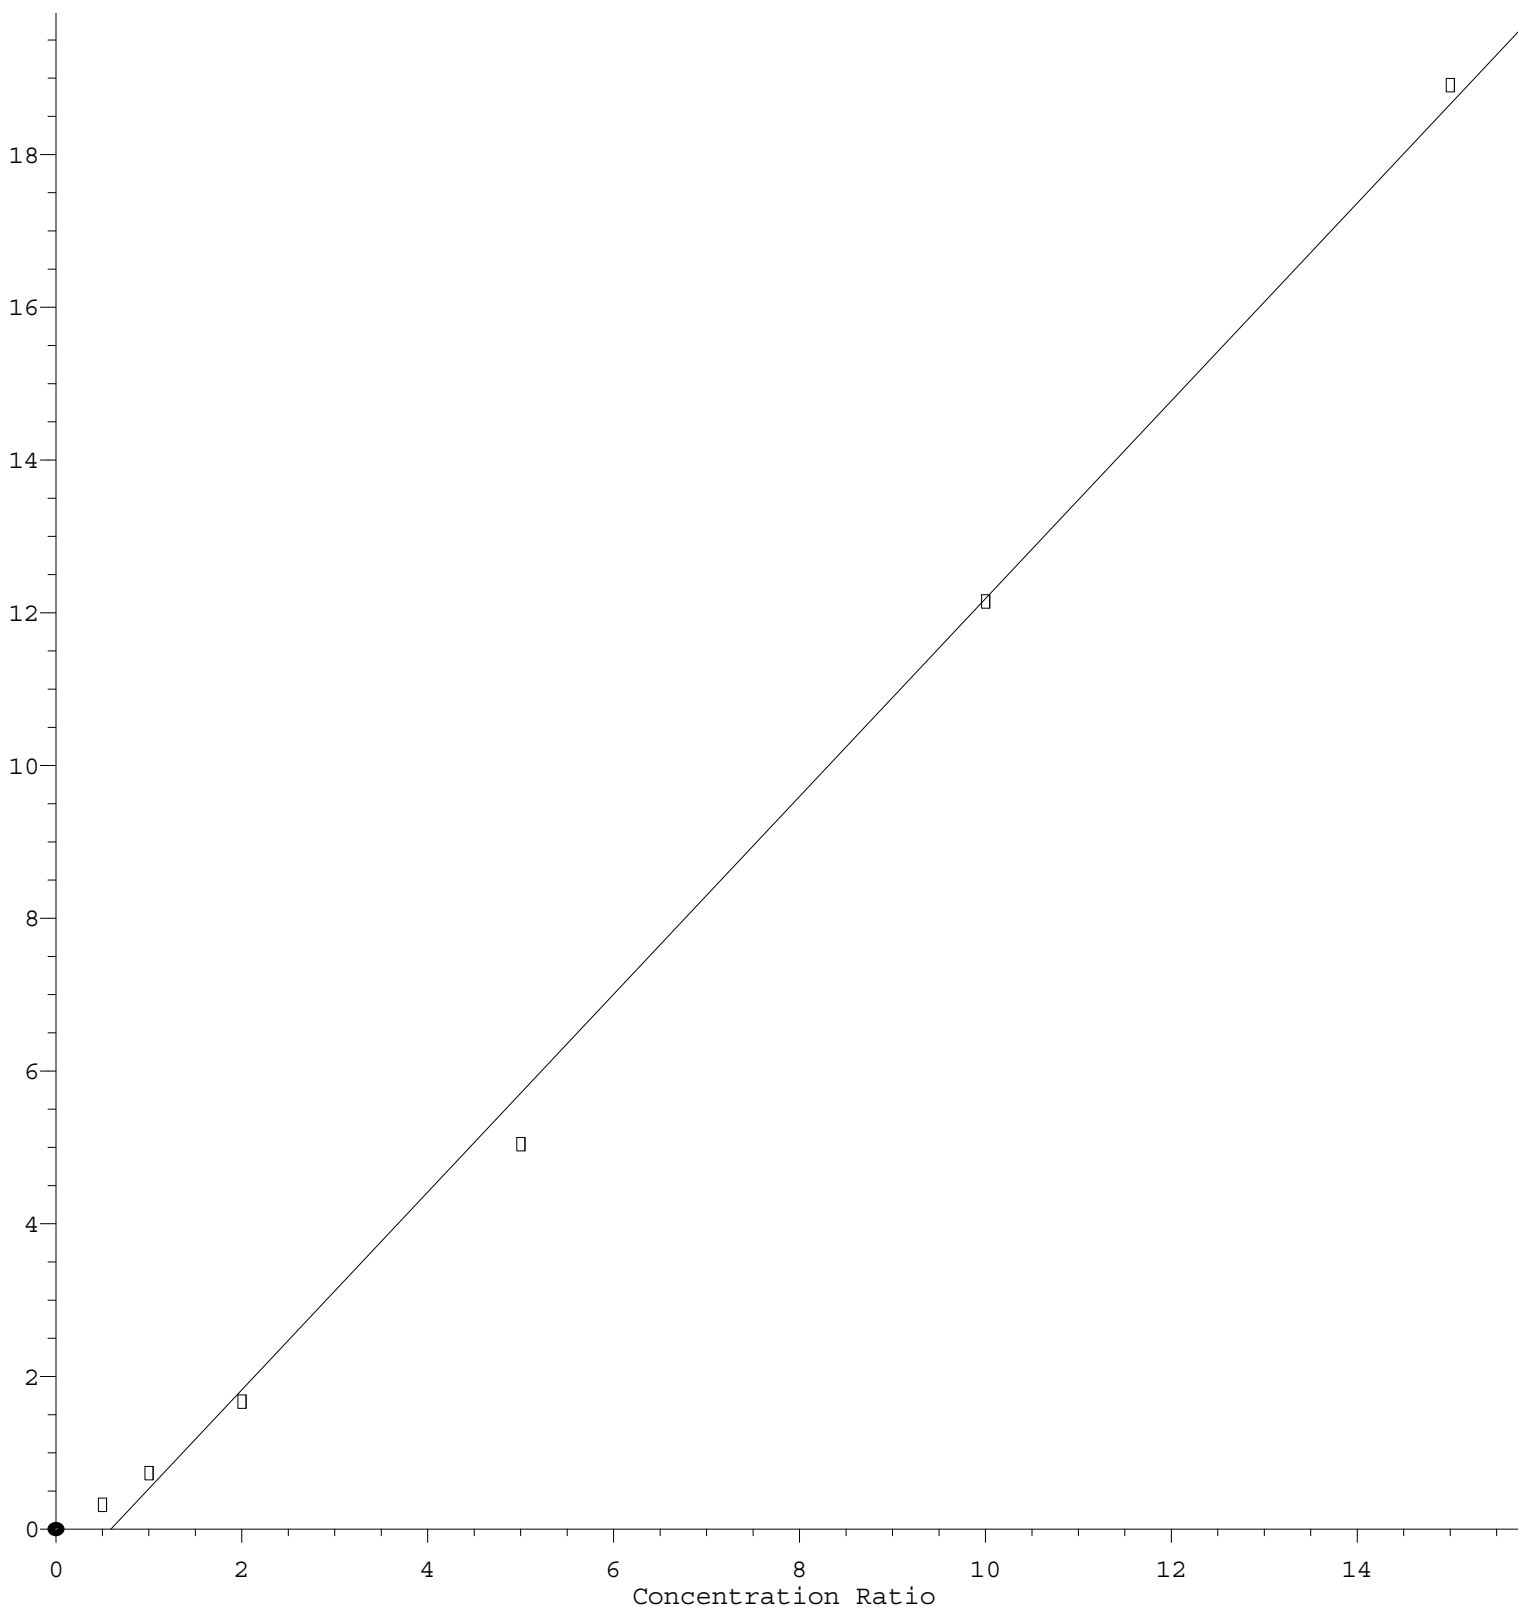

$$\text{Response} = 1.295\text{e}+000 * \text{Amt} - 7.598\text{e}-001$$


Coef of Det (r^2) = 0.997297 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

n-Butylbenzene

Response Ratio

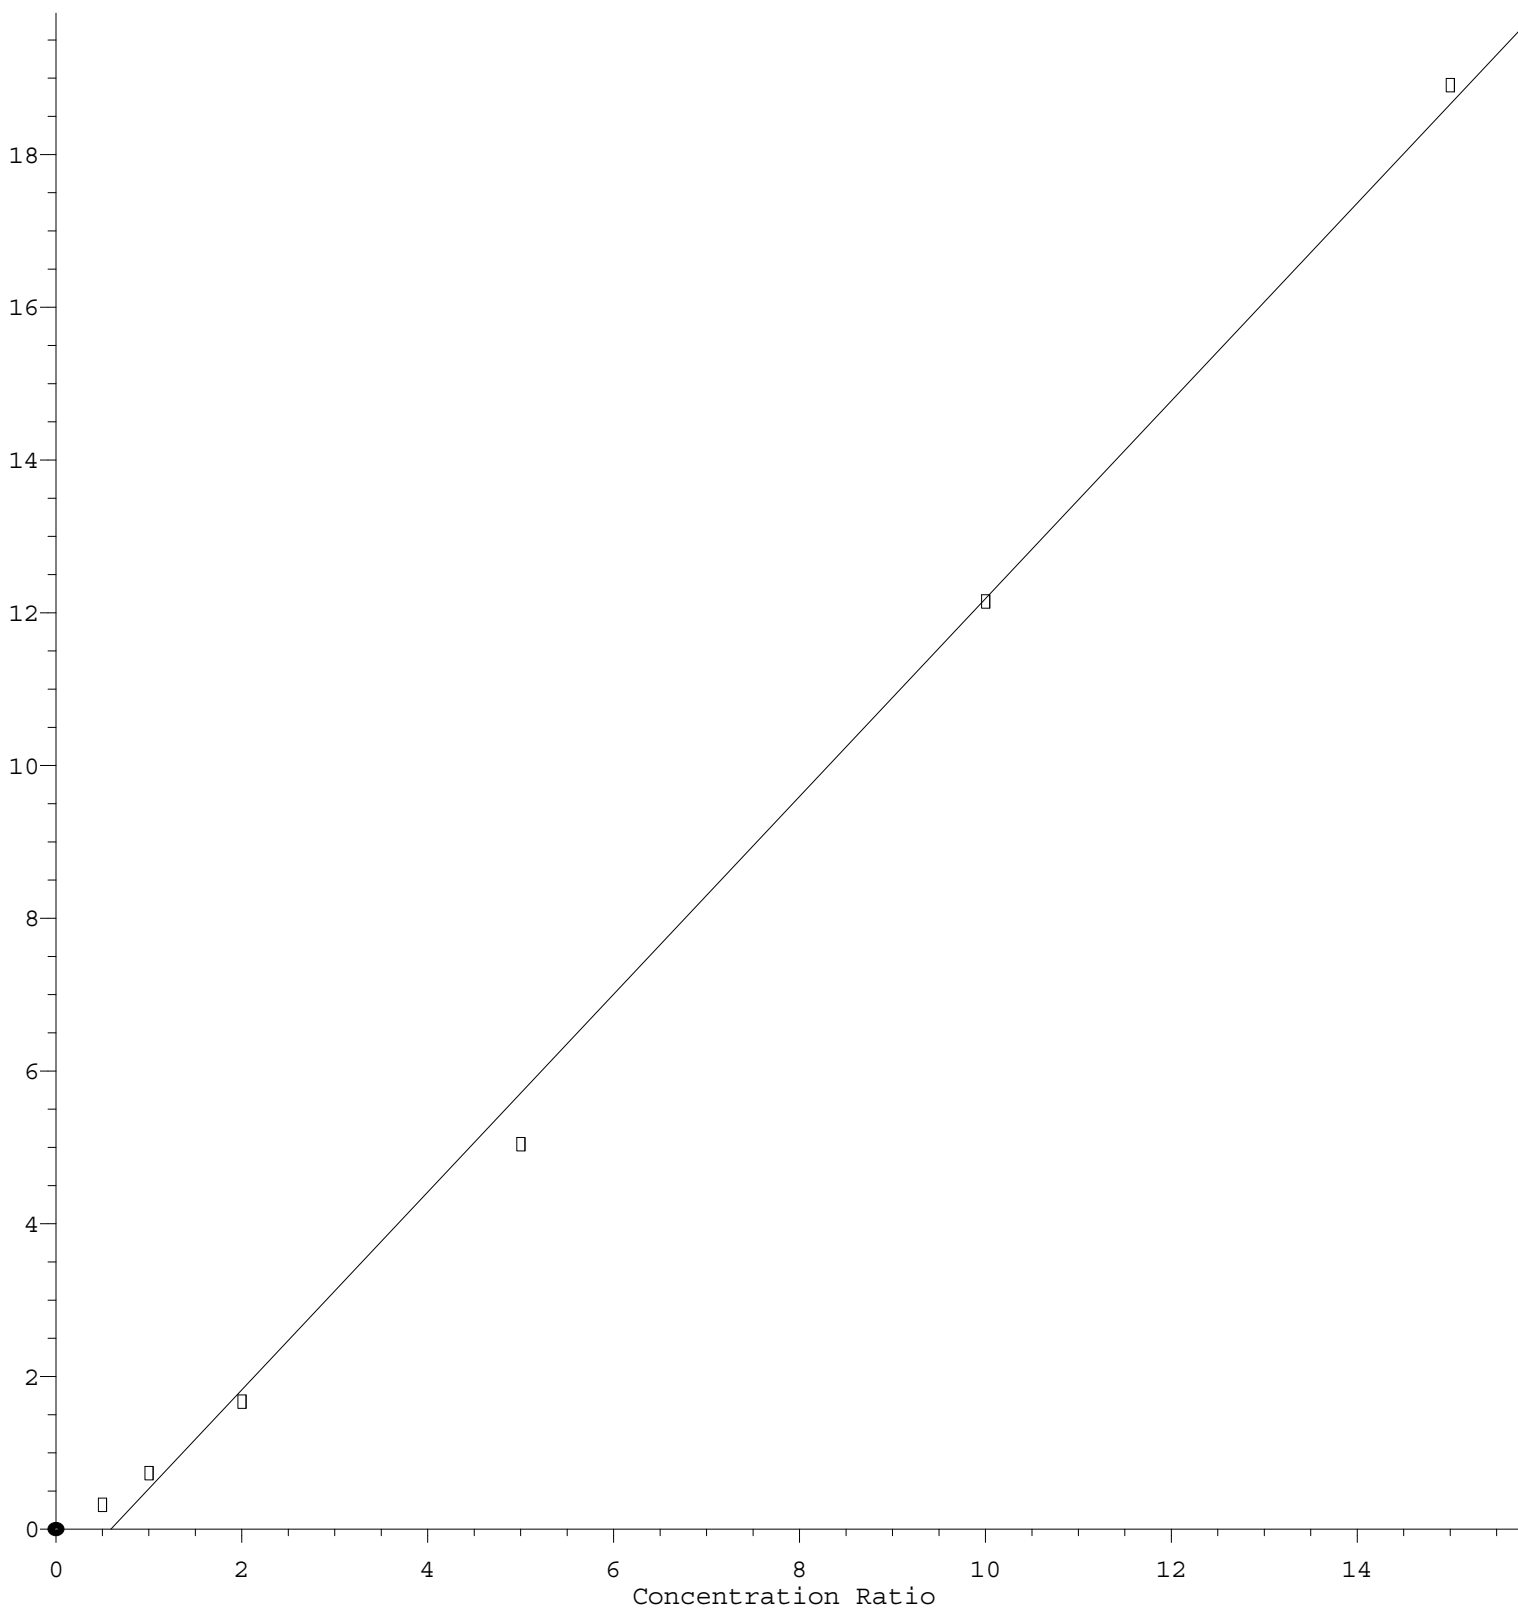

$$\text{Response} = 1.295\text{e}+000 * \text{Amt} - 7.598\text{e}-001$$


Coef of Det (r^2) = 0.997297 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

n-Butylbenzene

Response Ratio

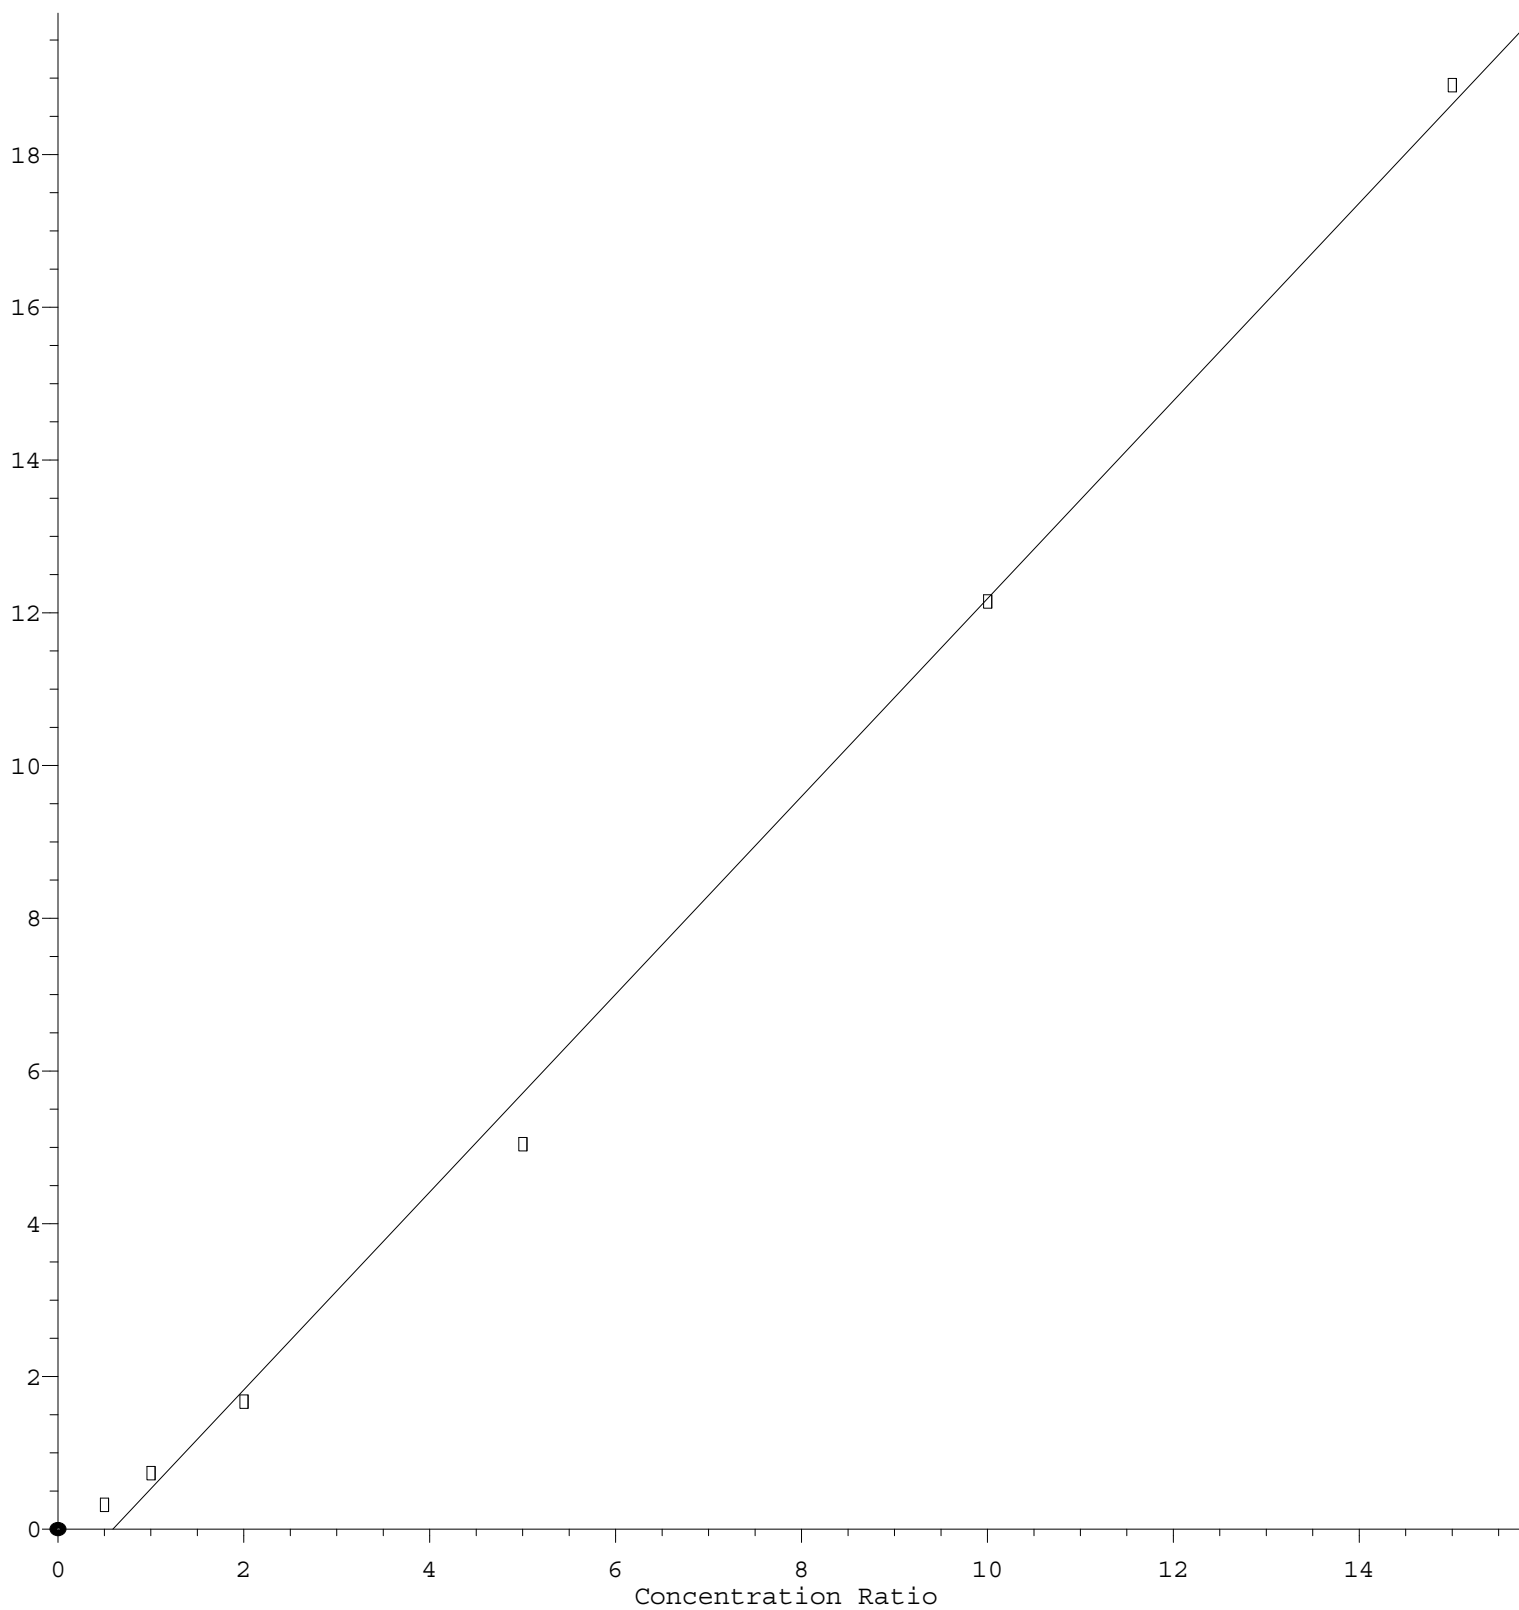

$$\text{Response} = 1.295\text{e}+000 * \text{Amt} - 7.598\text{e}-001$$


Coef of Det (r^2) = 0.997297 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

Naphthalene


Response Ratio

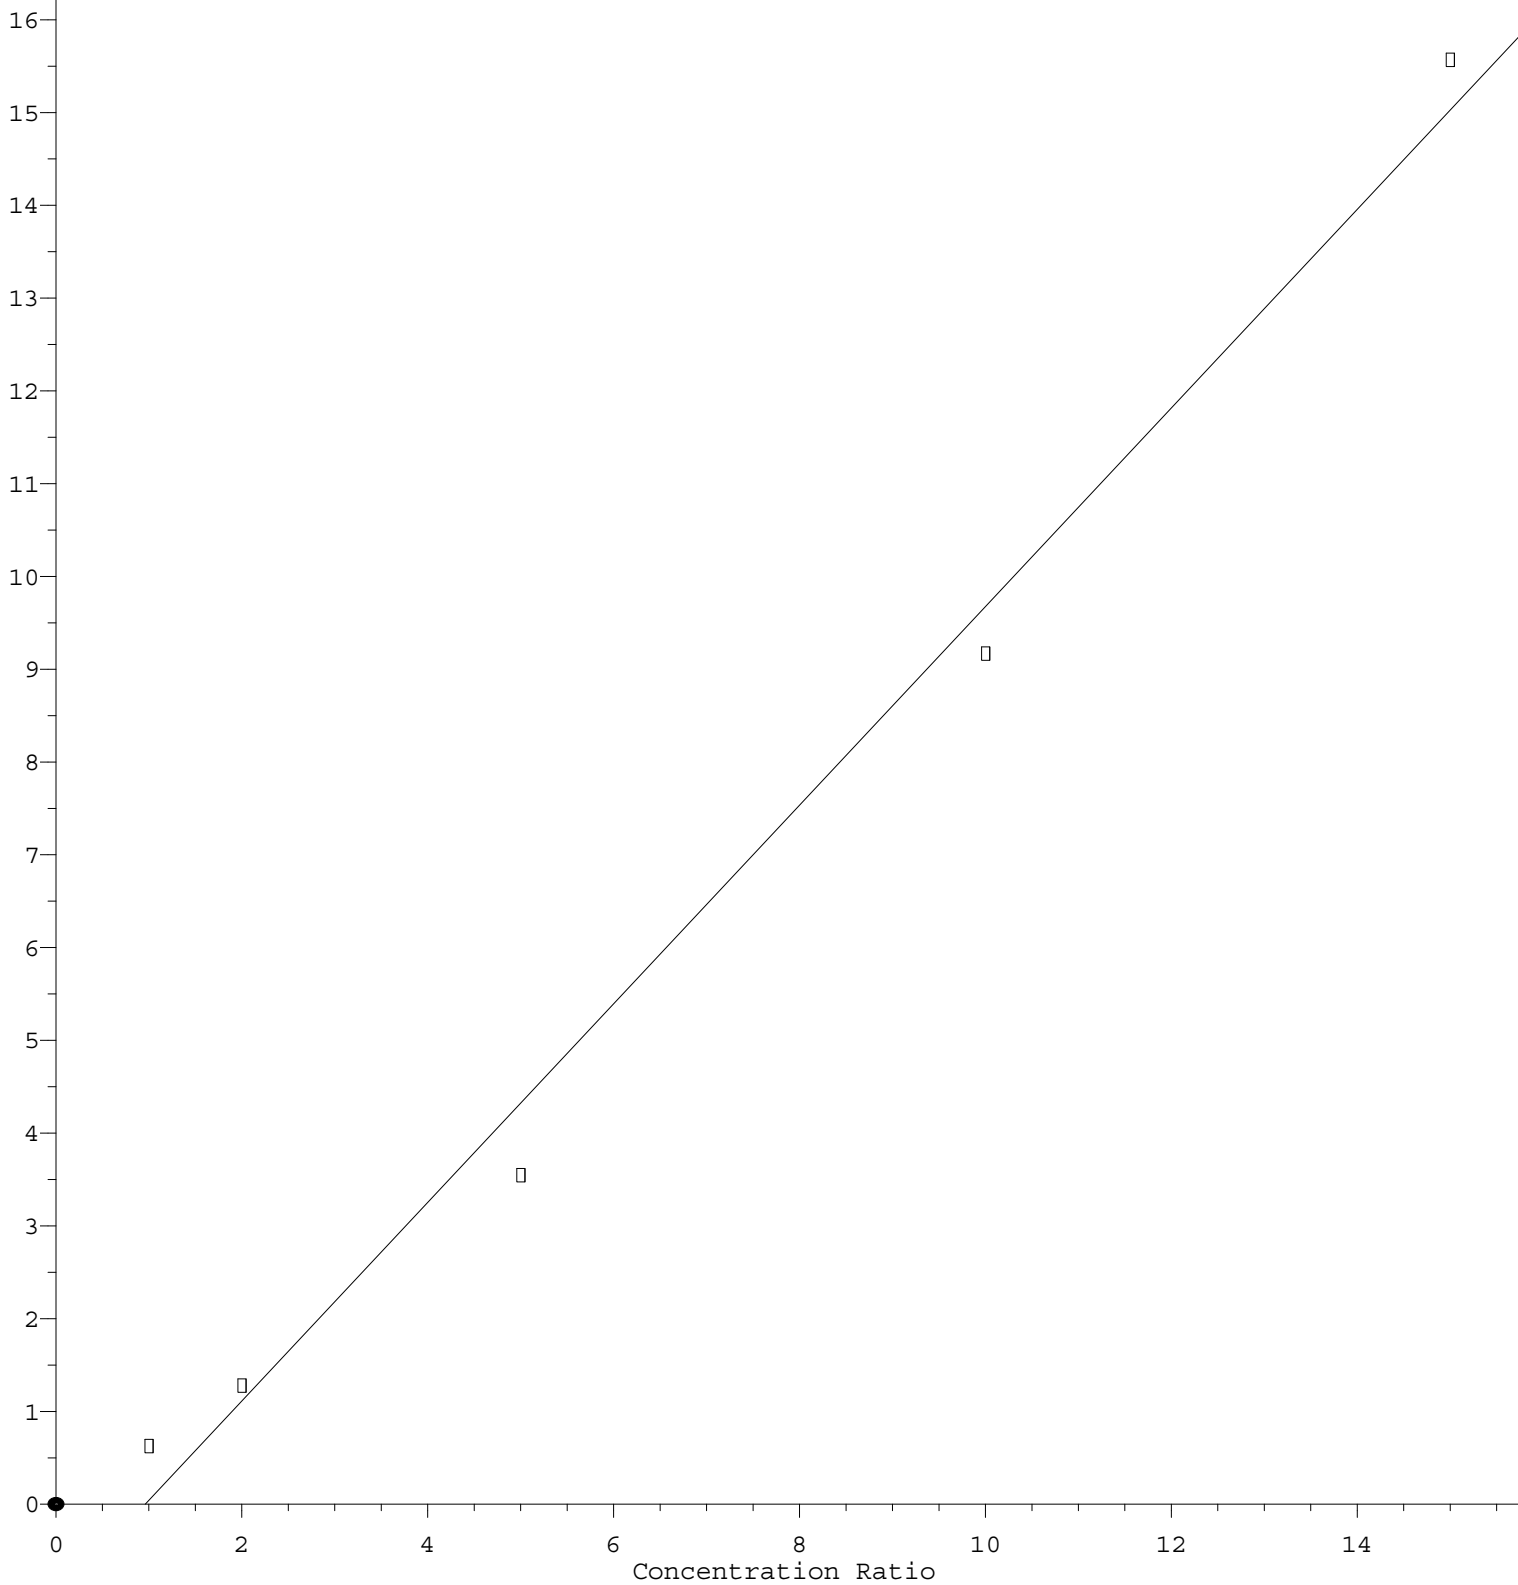

Response = 1.070e+000 * Amt - 1.028e+000
 Coef of Det (r^2) = 0.990409 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M
 Calibration Table Last Updated: Thu Aug 25 14:01:59 2022

1,2,3-Trichlorobenzene

Response Ratio

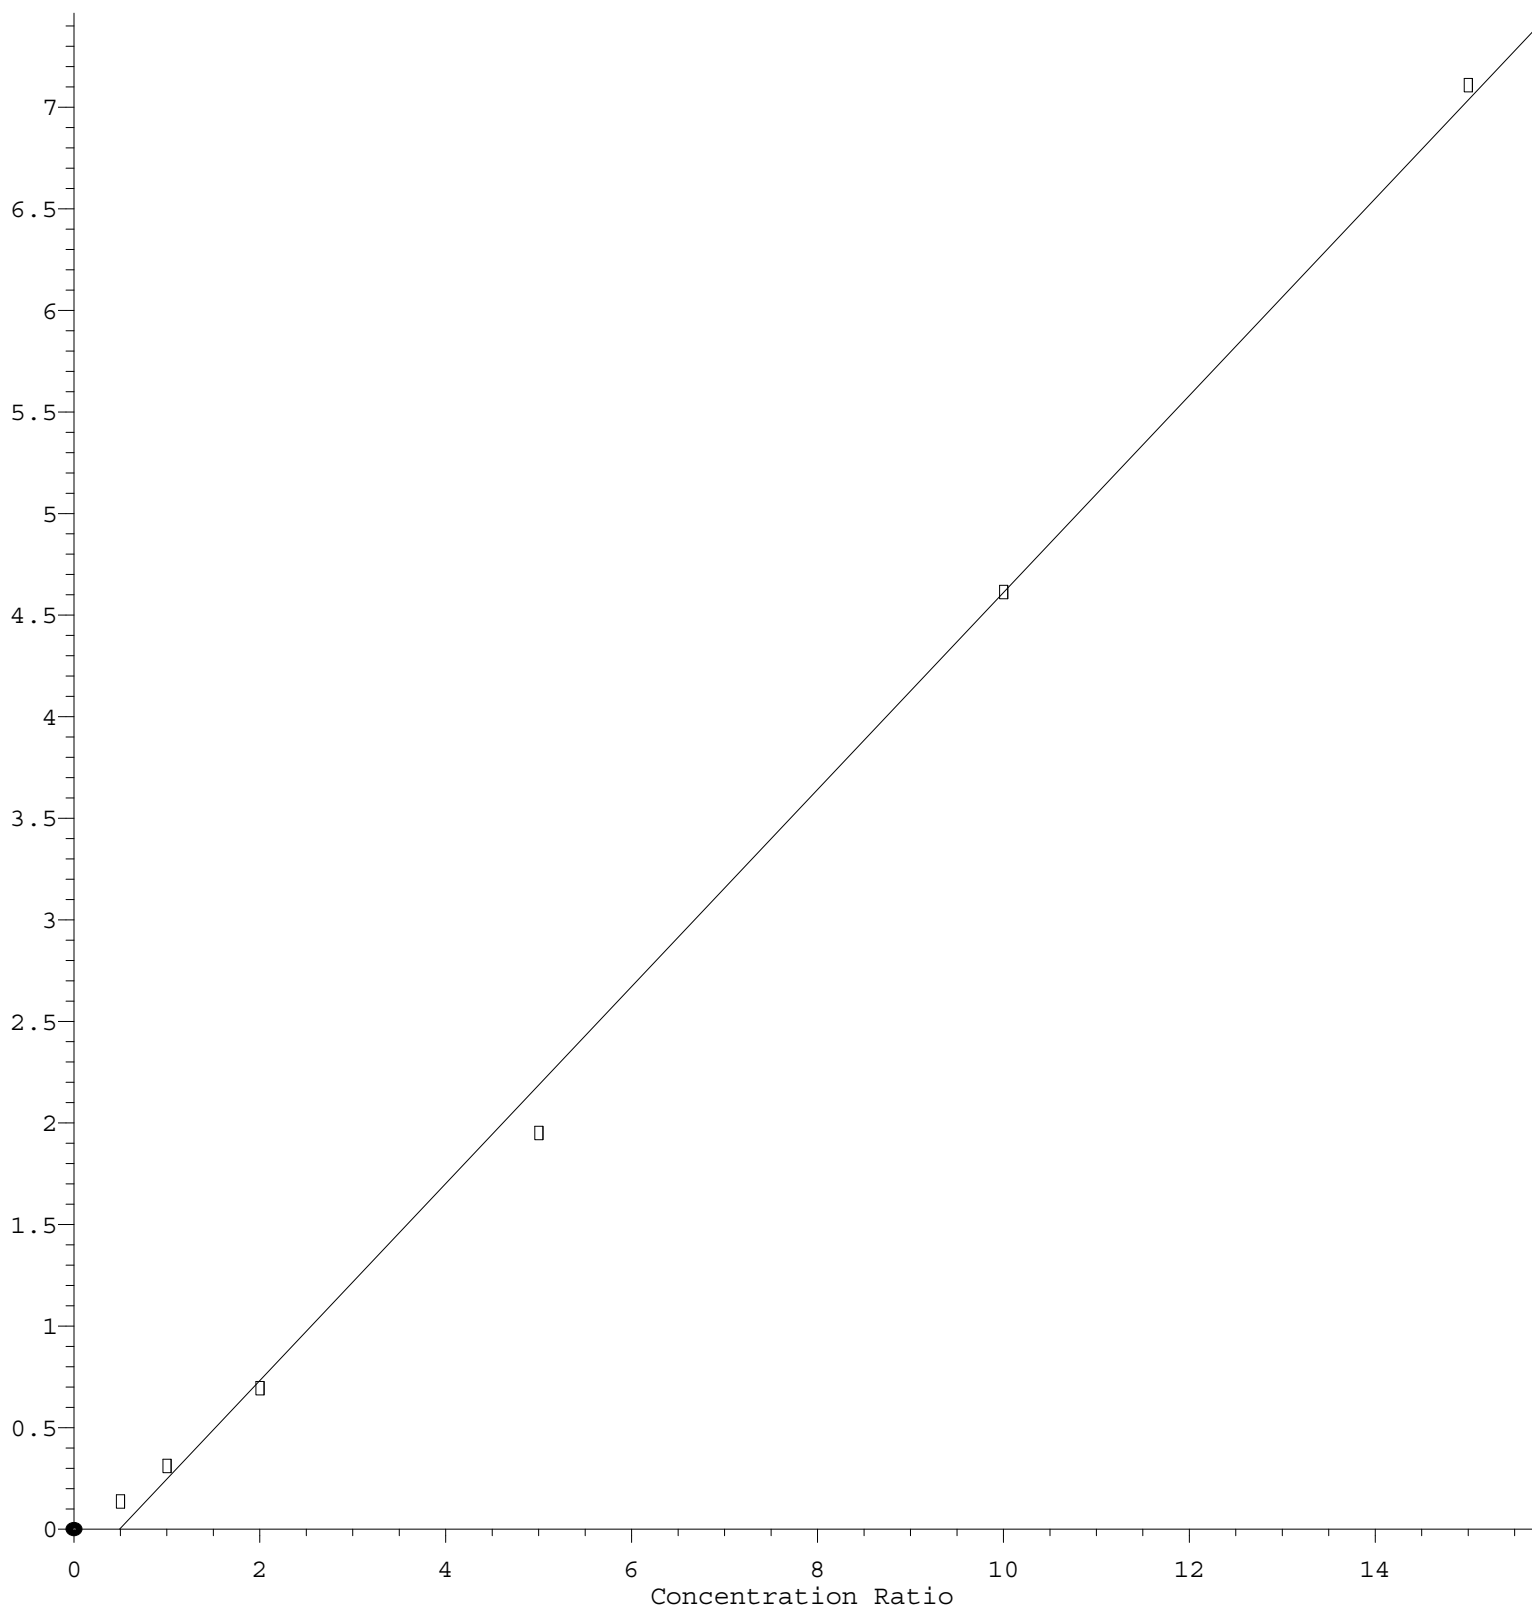

$$\text{Response} = 4.849\text{e-}001 * \text{Amt} - 2.389\text{e-}001$$

Coef of Det (r^2) = 0.997877 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U081922DW.M

Calibration Table Last Updated: Thu Aug 25 14:01:59 2022