

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081922\
 Data File : VU050379.D
 Acq On : 19 Aug 2022 20:01
 Operator : SY/MD
 Sample : VU0819WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0819WBL02

Quant Time: Aug 20 06:23:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Aug 19 15:06:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.150	96	30342	1.000	ug/l	# 0.04
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.645	95	7800	0.755	ug/l	0.00
Spiked Amount 1.000			Recovery	=	76.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	9661	0.791	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081922\
Data File : VU050379.D
Acq On : 19 Aug 2022 20:01
Operator : SY/MD
Sample : VU0819WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0819WBL02

Quant Time: Aug 20 06:23:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Aug 19 15:06:59 2022
Response via : Initial Calibration




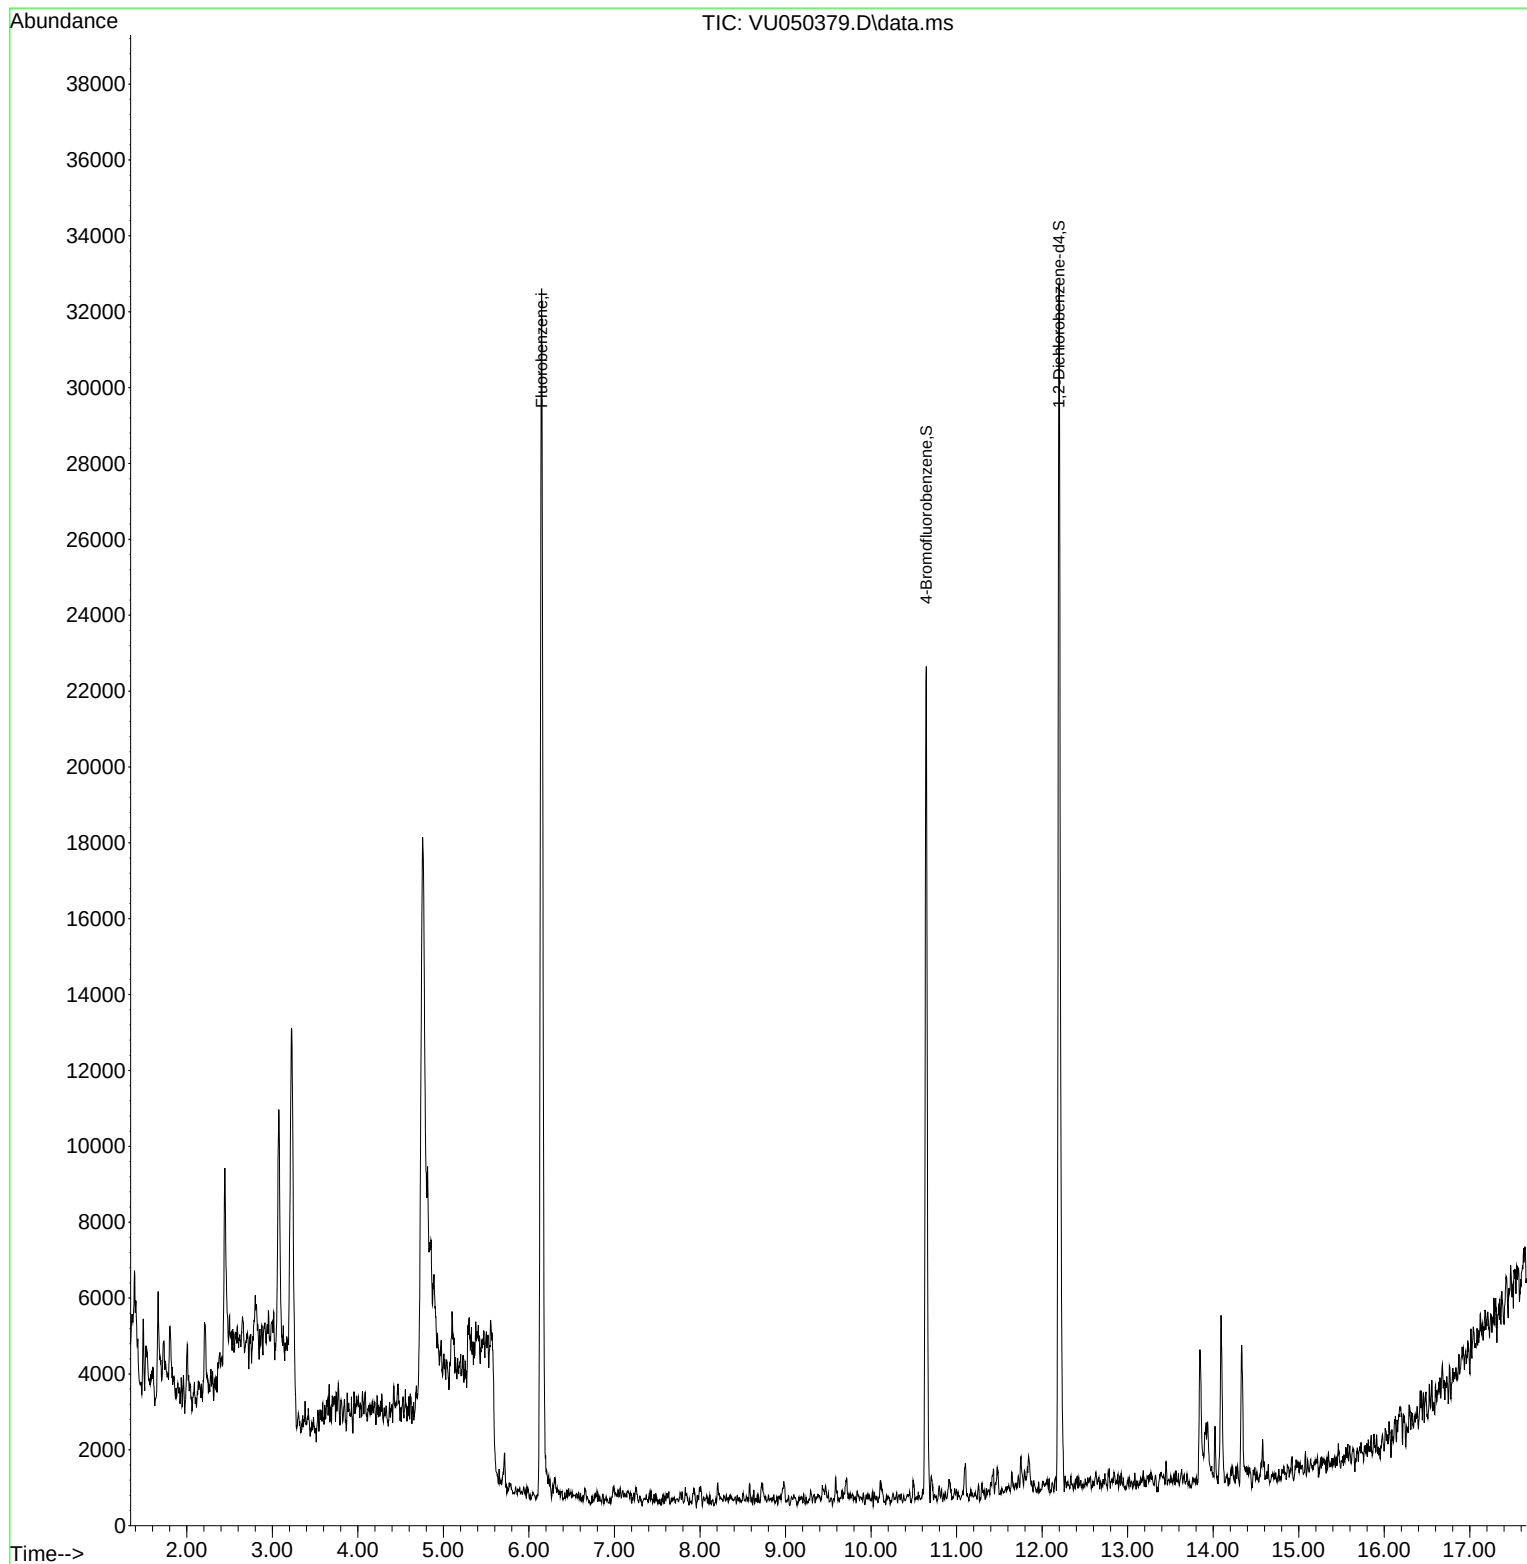


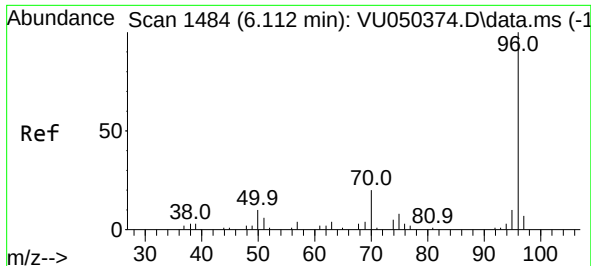

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.150 min Scan# 1484
Delta R.T. 0.038 min
Lab File: VU050379.D
Acq: 19 Aug 2022 20:01




Instrument :
MSVOA_U
ClientSampleId :
VU0819WBL02


Tgt Ion: 96	Resp: 30342
Ion Ratio	Lower Upper
96 100	
70 20.7	16.7 25.1
95 9.6	7.4 11.0
97 6.5	0.0 0.0

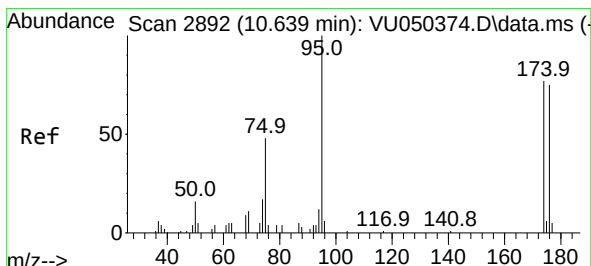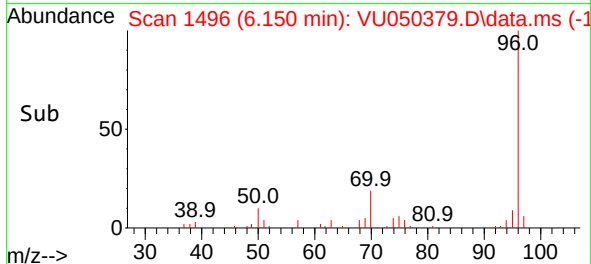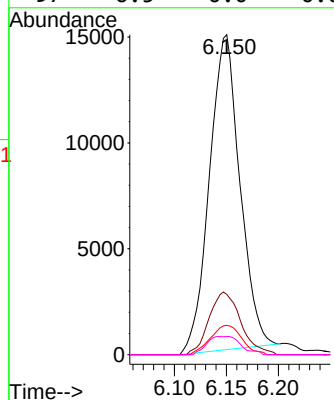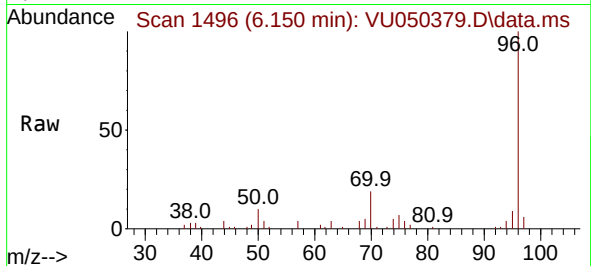

#57
4-Bromofluorobenzene
Concen: 0.755 ug/l
RT: 10.645 min Scan# 2894
Delta R.T. 0.006 min
Lab File: VU050379.D
Acq: 19 Aug 2022 20:01


Tgt Ion: 95	Resp: 7800
Ion Ratio	Lower Upper
95 100	
174 83.6	62.4 93.6
176 79.2	56.2 84.2

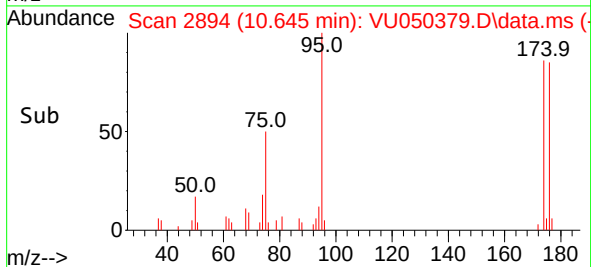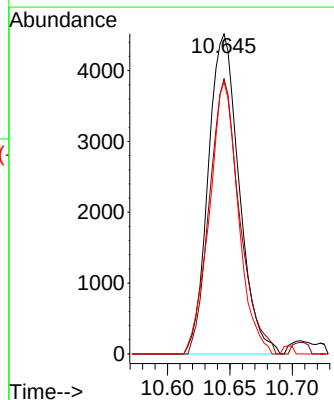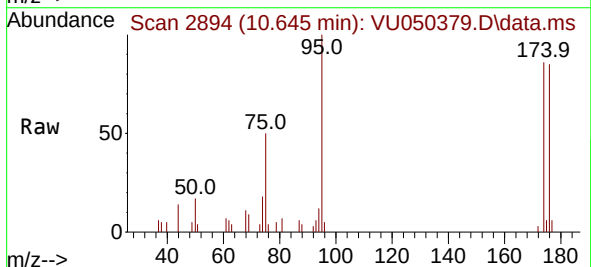

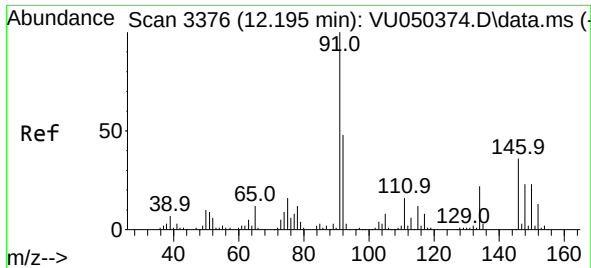

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.791 ug/l
 RT: 12.198 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU050379.D
 Acq: 19 Aug 2022 20:01

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0819WBL02

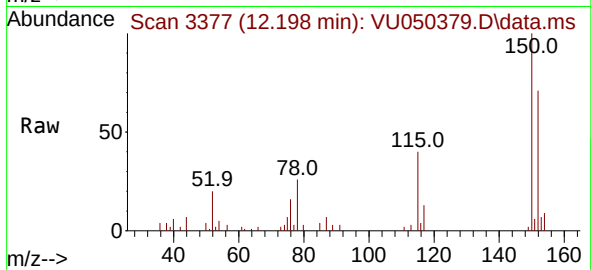

Tgt Ion:	152	Resp:	9661
Ion	Ratio	Lower	Upper
152	100		
115	60.7	0.0	254.6
150	153.2	0.0	623.6

