

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081922\
 Data File : VU050387.D
 Acq On : 20 Aug 2022 00:09
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Aug 20 06:31:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Aug 19 15:06:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.102	96	33868	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	8183	0.710	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	
68) 1,2-Dichlorobenzene-d4	12.198	152	9986	0.733	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081922\
Data File : VU050387.D
Acq On : 20 Aug 2022 00:09
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Aug 20 06:31:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Aug 19 15:06:59 2022
Response via : Initial Calibration

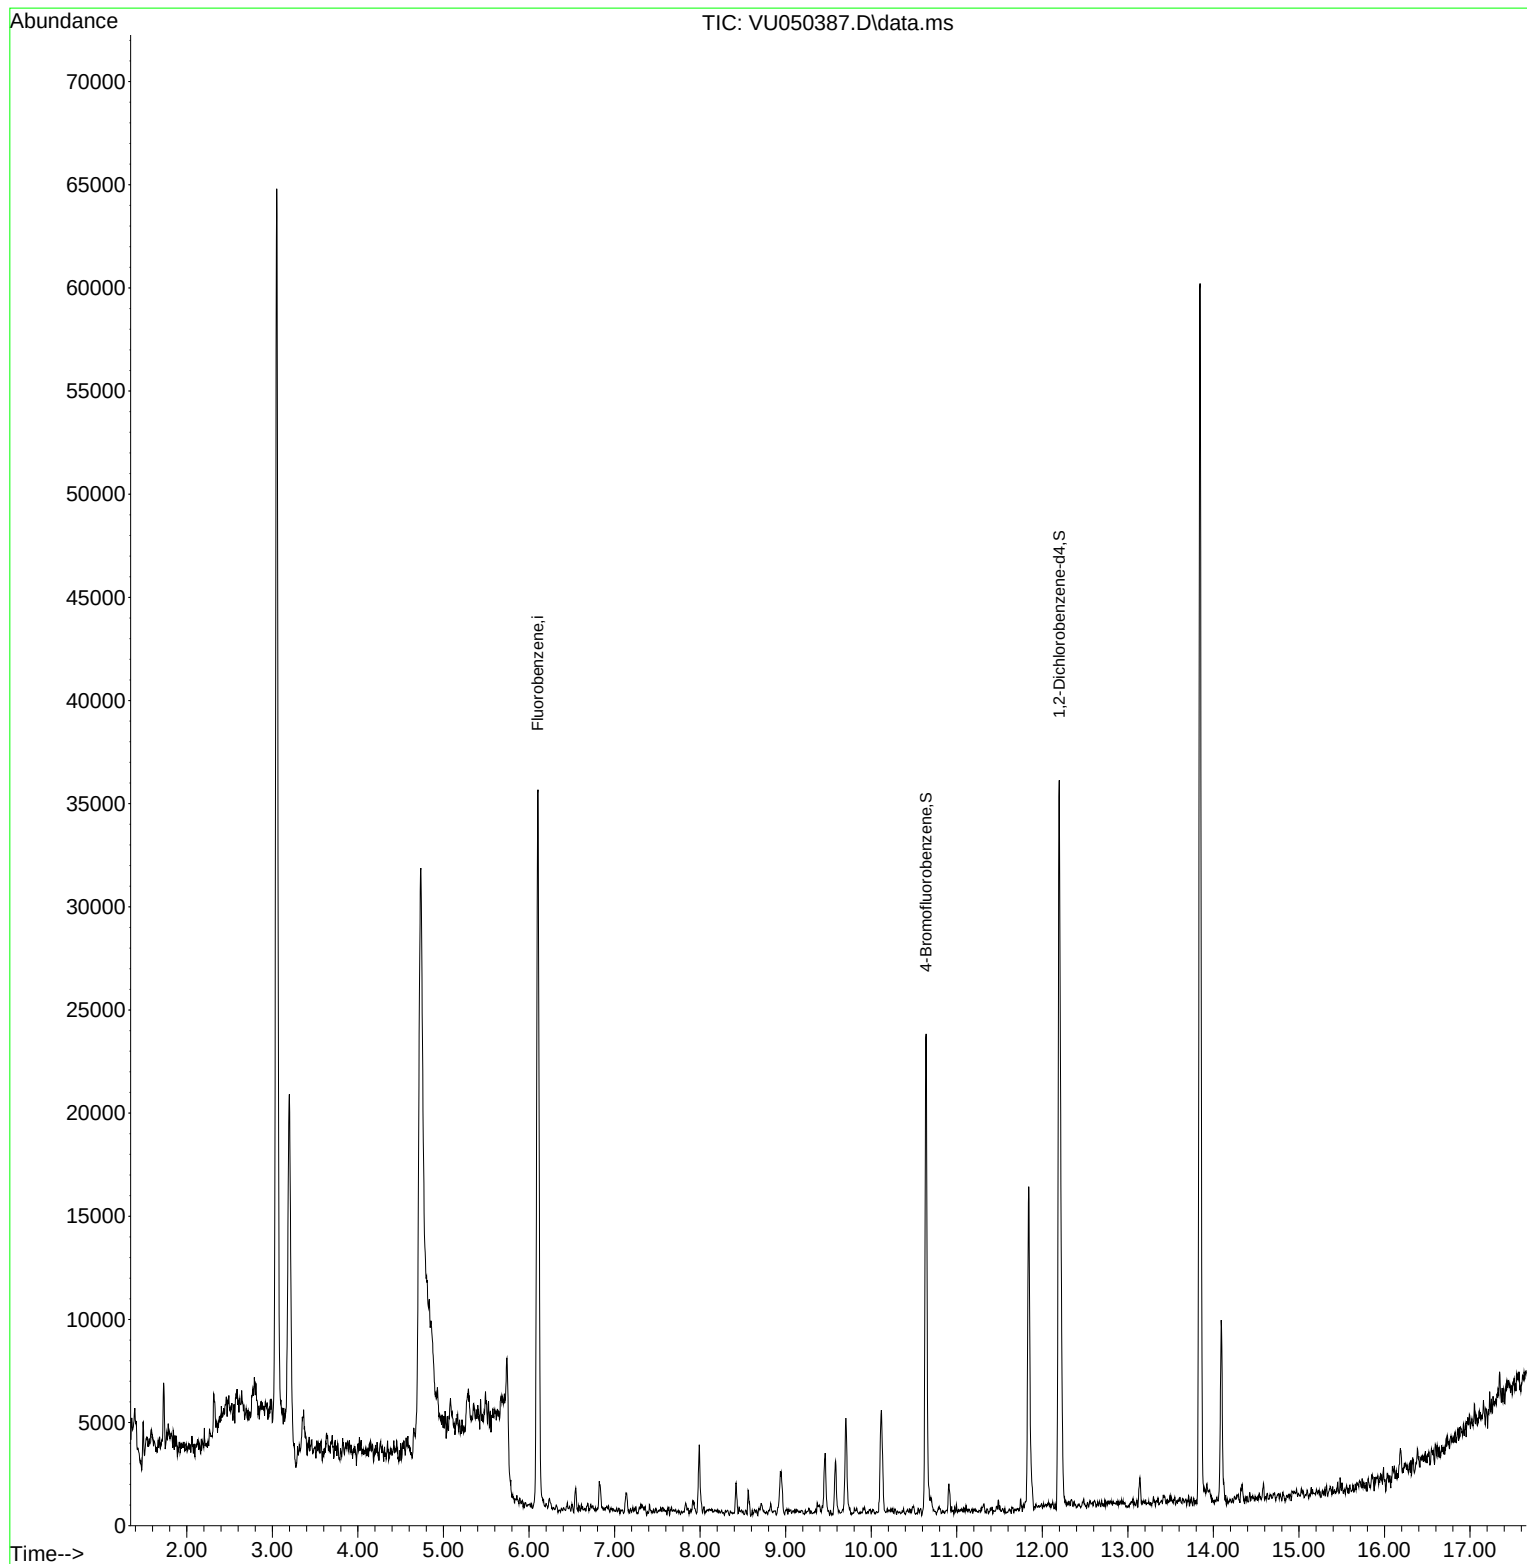




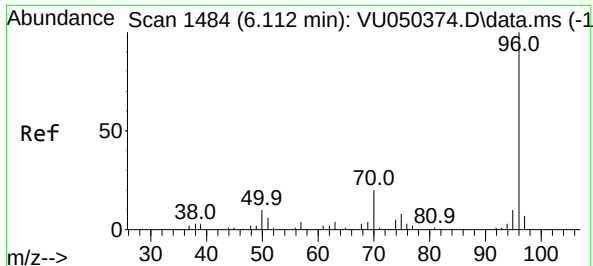


#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.102 min Scan# 1484
Delta R.T. -0.010 min
Lab File: VU050387.D
Acq: 20 Aug 2022 00:09

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Tgt Ion: 96 Resp: 33868




Ion	Ratio	Lower	Upper
96	100		
70	19.5	16.7	25.1
95	9.5	7.4	11.0
97	6.3	0.0	0.0

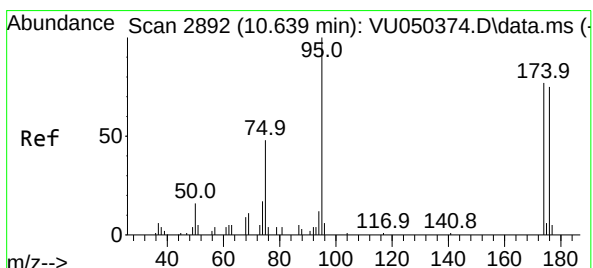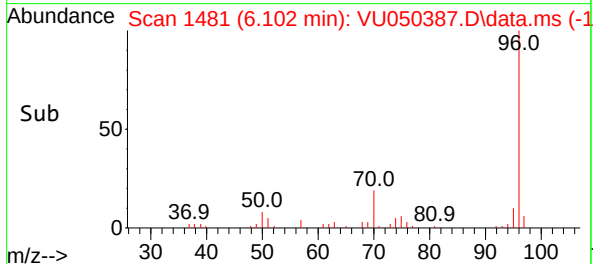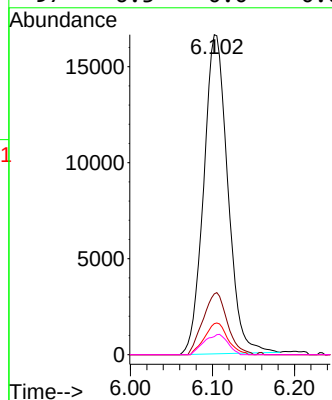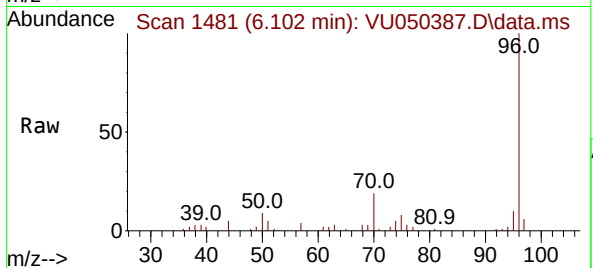


#57
4-Bromofluorobenzene
Concen: 0.710 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU050387.D
Acq: 20 Aug 2022 00:09

Tgt Ion: 95 Resp: 8183

Ion	Ratio	Lower	Upper
95	100		
174	87.1	62.4	93.6
176	83.0	56.2	84.2

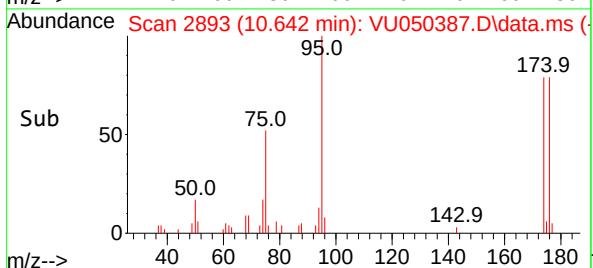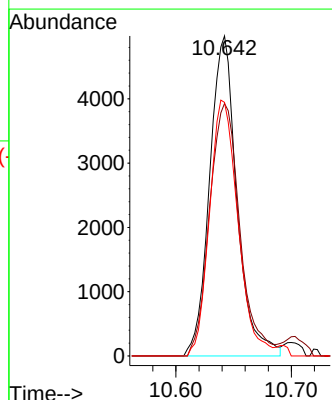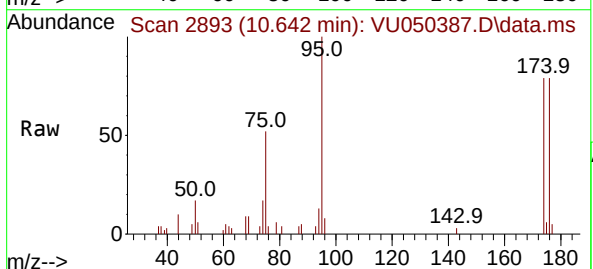

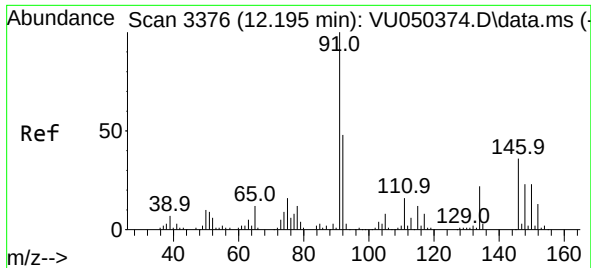

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.733 ug/l
 RT: 12.198 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU050387.D
 Acq: 20 Aug 2022 00:09

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Tgt Ion:	152	Resp:	9986
Ion	Ratio	Lower	Upper
152	100		
115	61.9	0.0	254.6
150	159.8	0.0	623.6

