


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU081922\
Data File : VU050377.D
Acq On : 19 Aug 2022 17:05
Operator : SY/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Aug 25 14:01:59 2022

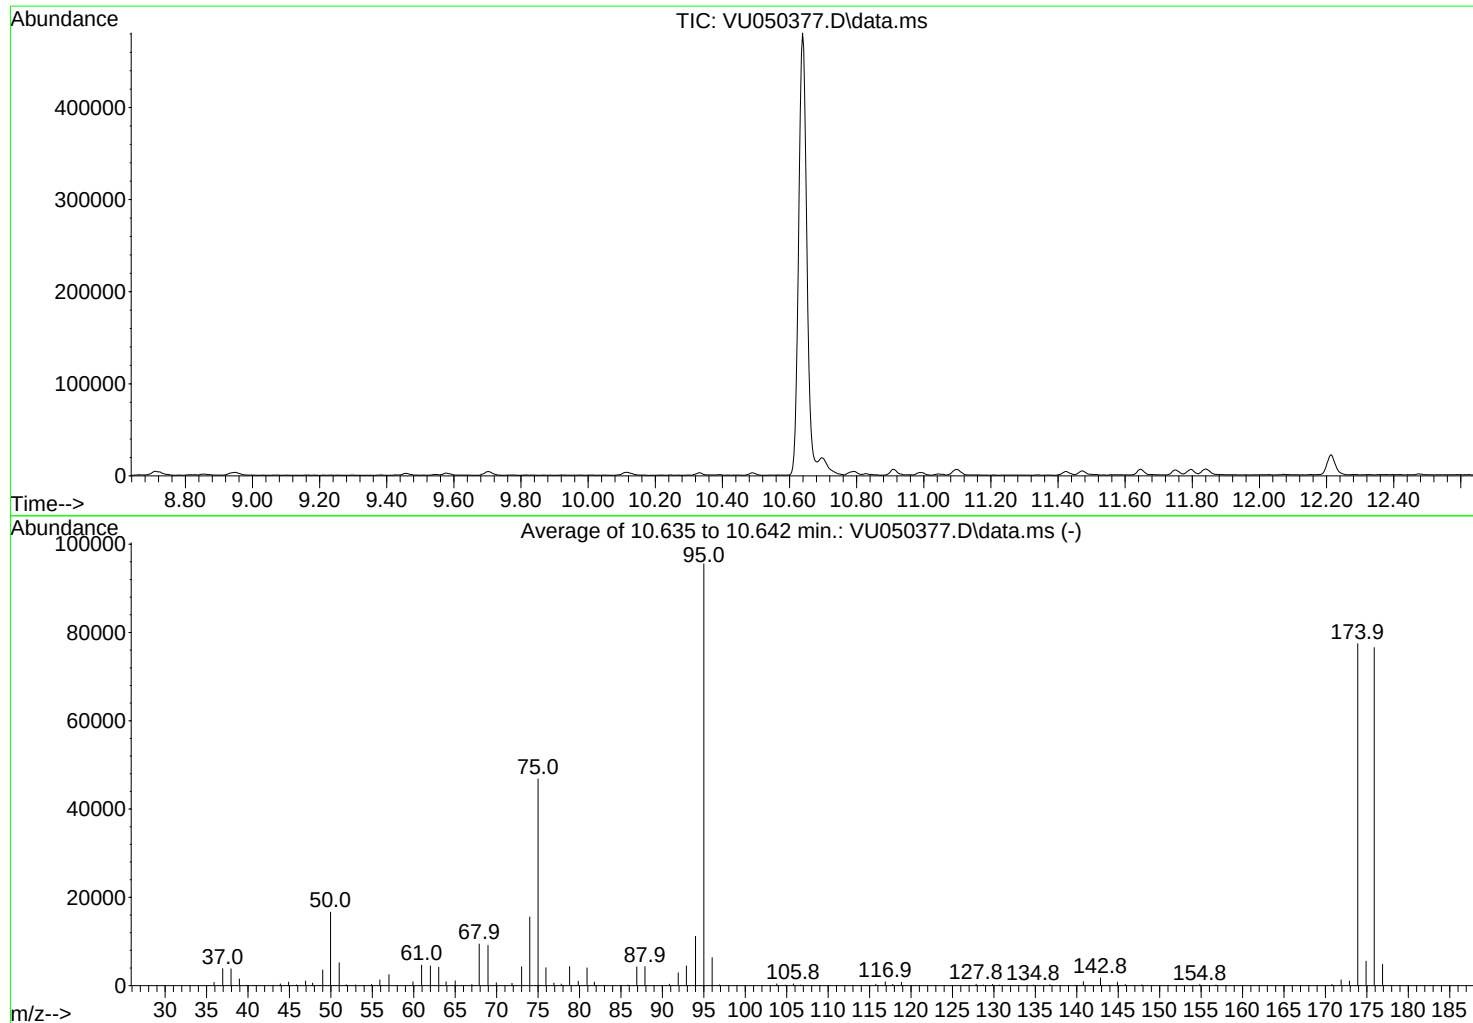

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	16643	PASS
75	95	30	60	49.0	46821	PASS
95	95	100	100	100.0	95549	PASS
96	95	5	9	6.6	6334	PASS
173	174	0.00	2	1.4	1050	PASS
174	95	50	100	81.1	77461	PASS
175	174	5	9	7.1	5537	PASS
176	174	95	101	98.9	76576	PASS
177	176	5	9	6.3	4819	PASS