
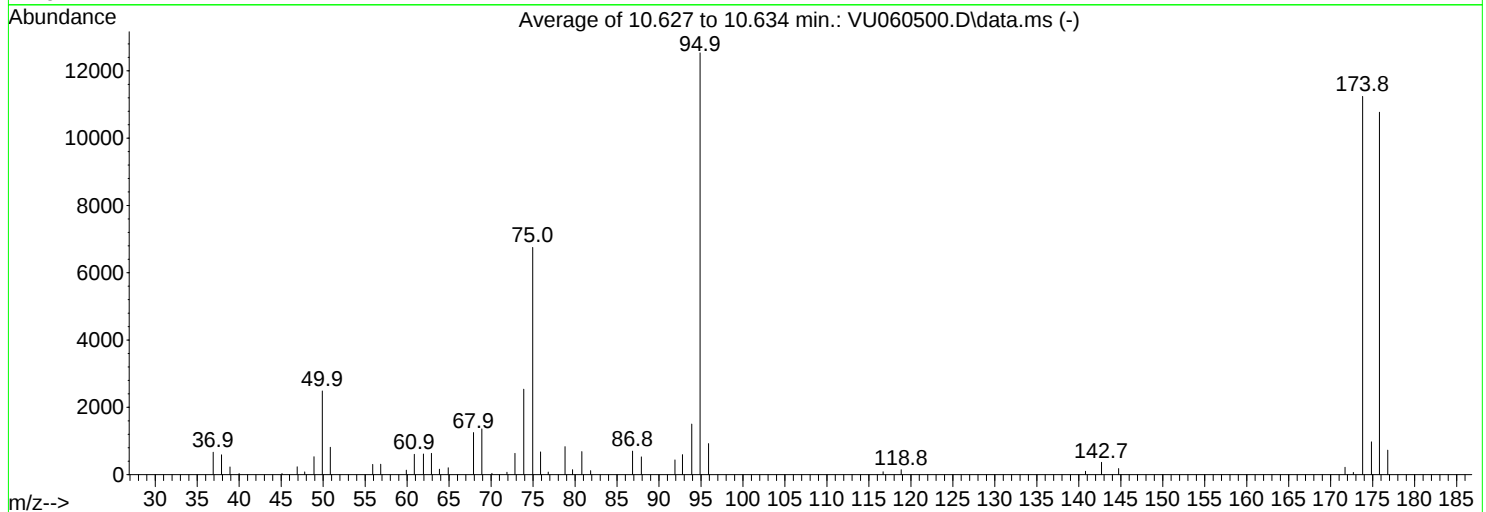


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082224\
Data File : VU060500.D
Acq On : 22 Aug 2024 13:10
Operator : MD/SY
Sample : BFB188
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB188

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Aug 24 01:12:47 2024

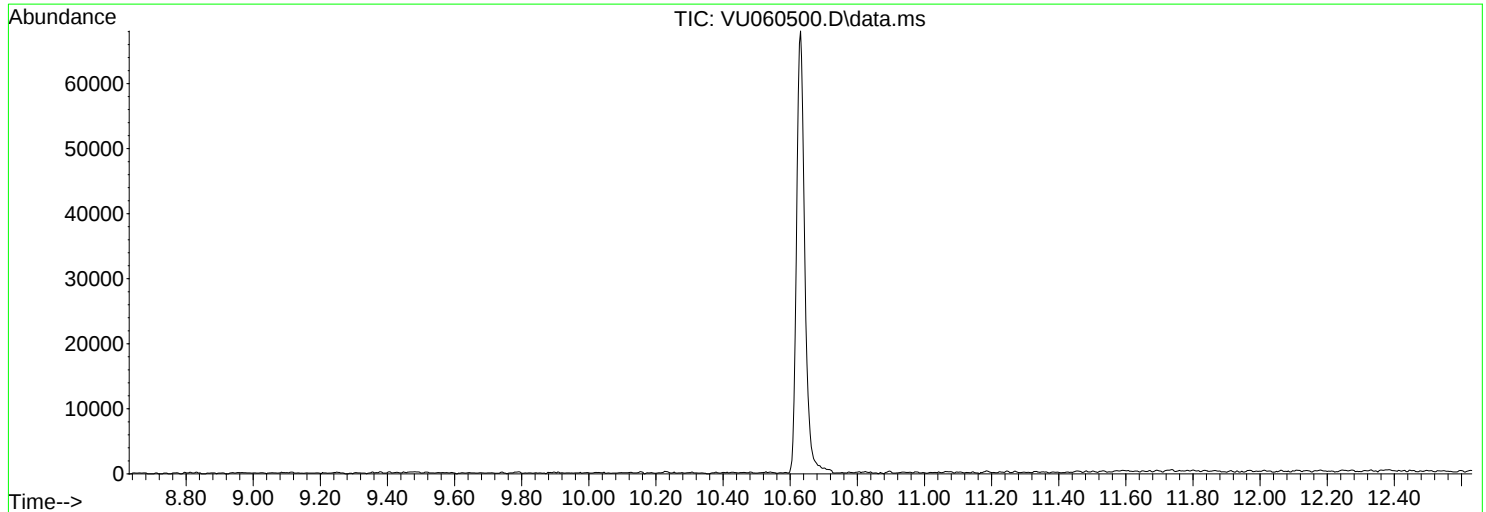

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	2487	PASS
75	95	30	80	53.9	6753	PASS
95	95	100	100	100.0	12535	PASS
96	95	5	9	7.4	922	PASS
173	174	0.00	2	0.6	67	PASS
174	95	50	120	89.7	11241	PASS
175	174	5	9	8.7	976	PASS
176	174	95	101	95.8	10771	PASS
177	176	5	9	6.8	728	PASS

m/z	Abundance
43.90	207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
36.90	637.0
37.90	600.0
38.90	221.0
40.00	100.0
43.80	178.0
45.10	103.0
46.90	231.0
48.90	567.0
49.90	2687.0
50.90	790.0
55.90	293.0
56.80	353.0
59.90	112.0
60.80	561.0
62.00	590.0
62.90	610.0
63.80	144.0
64.90	196.0
67.90	1331.0
68.90	1315.0
71.90	115.0
72.80	624.0
73.90	2626.0
74.90	6760.0
75.90	705.0
76.80	121.0
78.80	814.0
79.70	164.0
80.80	712.0
81.90	119.0
86.80	701.0
87.90	543.0
91.90	453.0
92.80	626.0
93.90	1420.0
94.90	12697.0
95.90	1009.0
118.80	150.0
142.70	345.0
144.70	172.0
171.70	206.0
172.70	202.0
173.80	11092.0
174.90	923.0
175.80	10446.0
176.80	774.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
36.90	664.0
37.90	583.0
38.90	245.0
43.90	154.0
46.90	243.0
47.80	117.0
48.90	569.0
49.90	2543.0
50.80	841.0
55.90	316.0
56.80	303.0
59.90	142.0
60.90	611.0
61.90	598.0
62.90	666.0
63.80	168.0
64.90	207.0
67.90	1261.0
68.90	1385.0
71.90	104.0
72.80	636.0
73.90	2611.0
75.00	6954.0
75.90	706.0
76.80	109.0
78.80	878.0
79.70	152.0
80.80	677.0
81.90	114.0
86.90	724.0
87.90	562.0
91.90	454.0
92.80	580.0
93.90	1538.0
94.90	12925.0
95.90	954.0
116.70	119.0
118.90	146.0
140.80	116.0
142.70	386.0
144.80	188.0
171.70	229.0
173.80	11665.0
174.80	1015.0
175.80	11146.0
176.80	761.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188

m/z	Abundance
36.90	691.0
37.90	588.0
38.90	215.0
43.90	158.0
46.90	231.0
47.80	133.0
48.90	460.0
49.90	2230.0
50.80	809.0
55.90	302.0
56.90	269.0
59.90	141.0
60.90	643.0
61.90	652.0
62.90	617.0
63.90	176.0
64.90	211.0
67.90	1155.0
68.90	1383.0
70.10	108.0
72.90	640.0
73.90	2373.0
75.00	6544.0
75.90	614.0
78.80	811.0
79.70	129.0
80.80	673.0
81.70	121.0
86.90	665.0
87.90	483.0
91.90	402.0
92.80	578.0
93.90	1553.0
94.90	11983.0
95.90	802.0
116.70	132.0
118.90	142.0
140.80	184.0
142.70	365.0
144.80	185.0
171.70	225.0
173.80	10965.0
174.80	991.0
175.80	10722.0
176.80	650.0

Instrument :
MSVOA_U
ClientSampleId :
BFB188