

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
 Data File : VU060517.D
 Acq On : 23 Aug 2024 18:20
 Operator : MD/SY
 Sample : P3711-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E24A4

Quant Time: Aug 24 01:48:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 24 01:46:38 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	140319	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	141121	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152	59196	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.595	65	31939	5.153	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.000%	
7) Chloroethane-d5		1.907	69	33315	3.548	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.000%	
11) 1,1-Dichloroethene-d2		2.560	65	15793	4.324	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.400%	
20) 2-Butanone-d5		4.634	46	123037	57.731	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.460%	
24) Chloroform-d		5.055	84	82506	4.669	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4		5.695	65	46618	5.056	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%	
32) Benzene-d6		5.721	84	156320	5.066	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%	
36) 1,2-Dichloropropane-d6		6.682	67	56538	5.679	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.600%	
41) Toluene-d8		7.891	98	125897	4.349	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%	
43) trans-1,3-Dichloroprop...		8.177	79	17647	4.953	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.000%	
46) 2-Hexanone-d5		8.631	63	82917	48.608	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.220%	
56) 1,1,2,2-Tetrachloroeth...		10.749	84	45939	5.185	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4		12.187	152	50155	5.746	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.000%	
Target Compounds							
13) Acetone		2.647	43	26240	14.714	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
Data File : VU060517.D
Acq On : 23 Aug 2024 18:20
Operator : MD/SY
Sample : P3711-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E24A4

Quant Time: Aug 24 01:48:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 24 01:46:38 2024
Response via : Initial Calibration

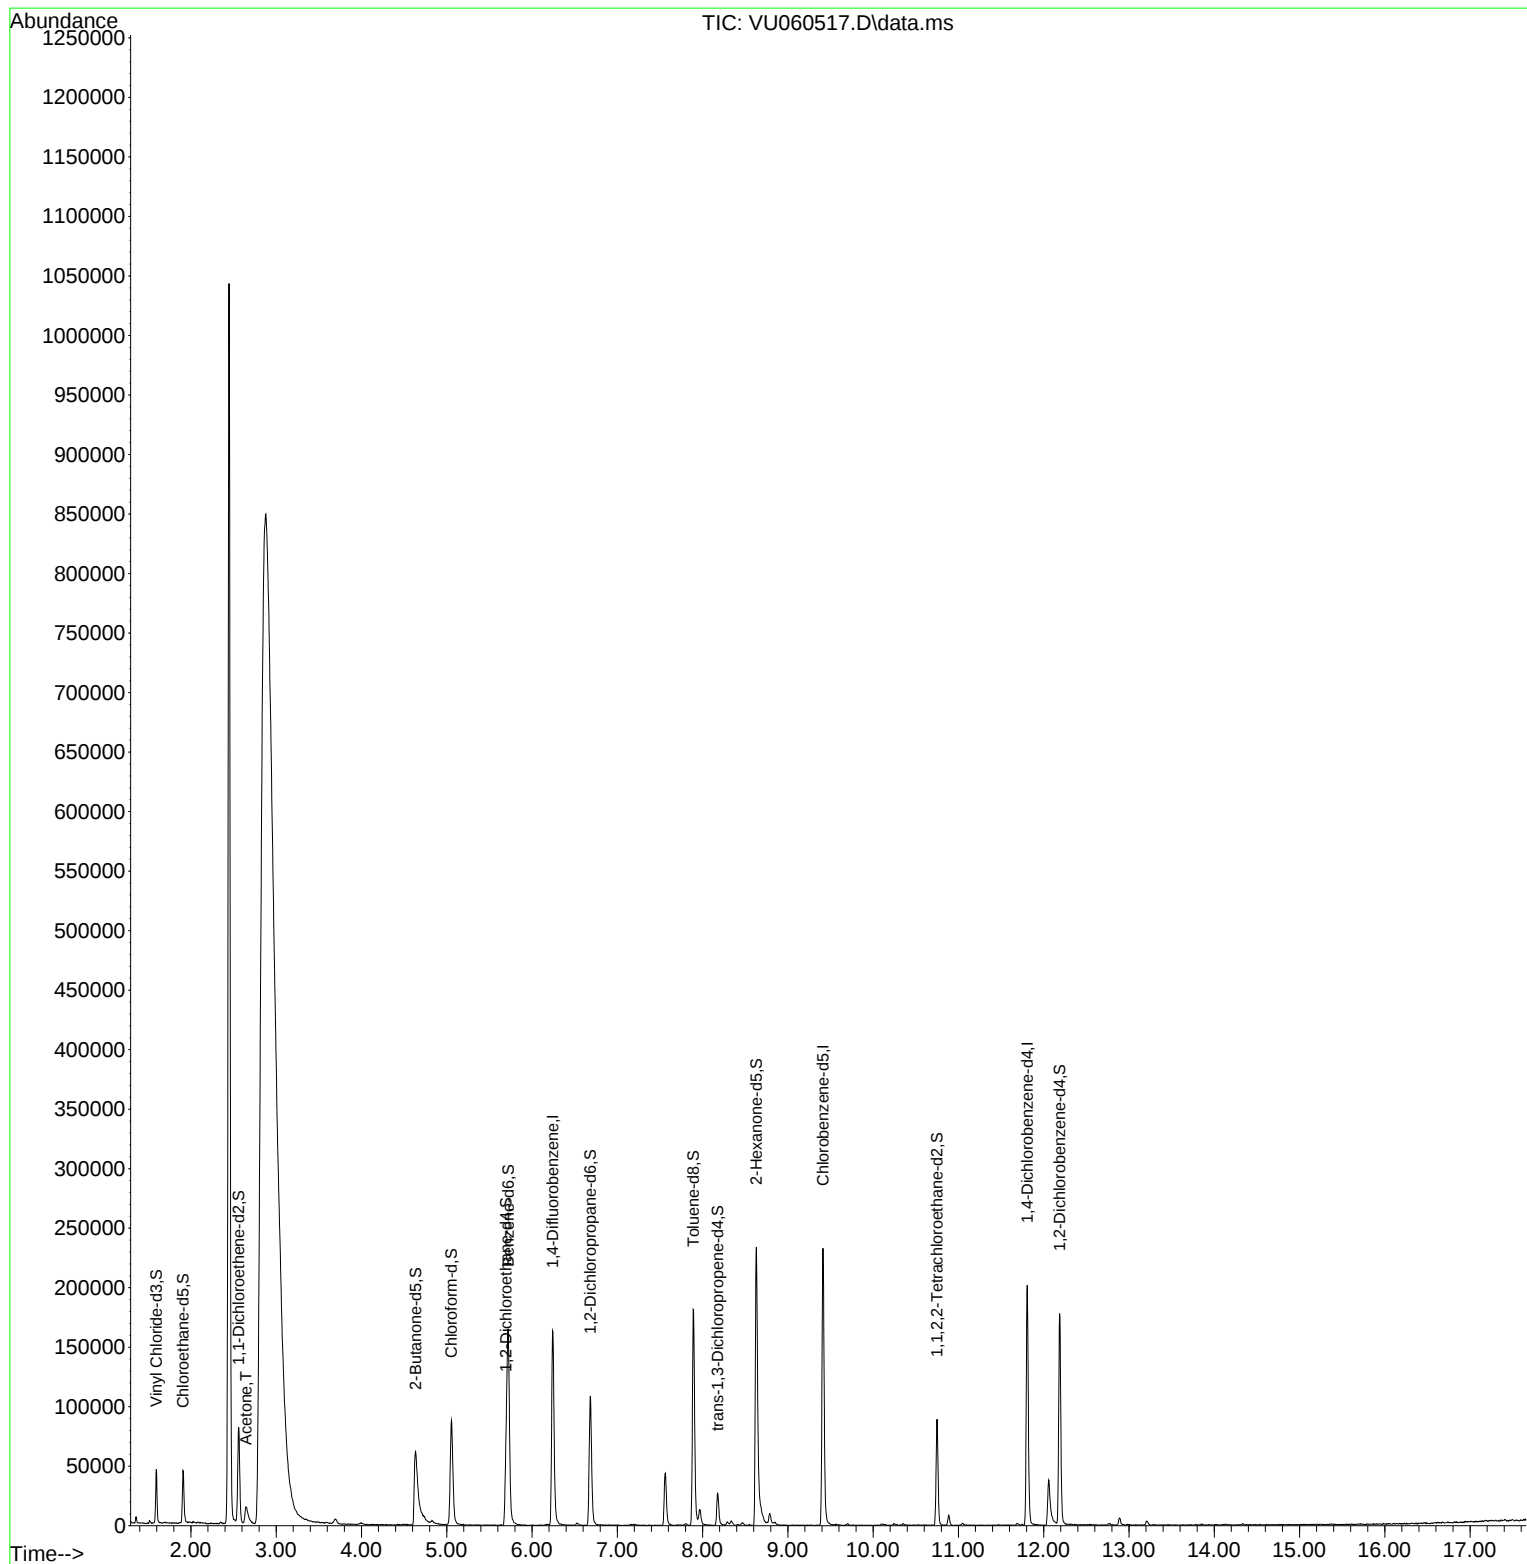

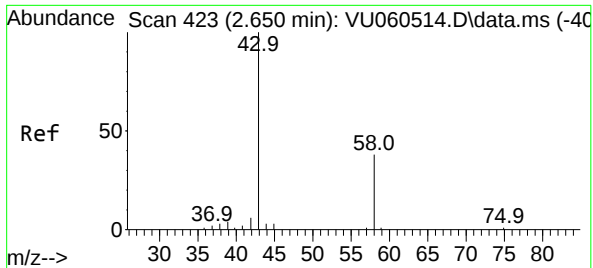

#13
 Acetone
 Concen: 14.714 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: VU060517.D
 Acq: 23 Aug 2024 18:20

Instrument :
 MSVOA_U
 ClientSampleId :
 E24A4

Tgt Ion: 43 Resp: 26240
 Ion Ratio Lower Upper
 43 100
 58 35.0 0.0 66.8

