

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
 Data File : VU060527.D
 Acq On : 23 Aug 2024 22:22
 Operator : MD/SY
 Sample : P3711-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2495

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	108	rVB	24239	26653	9.55%	1.106%
2	1.689	113	124	128	rBV2	1783	2907	1.04%	0.121%
3	1.727	128	136	146	rVB	22265	27801	9.97%	1.154%
4	1.911	183	193	209	rBV	40173	54953	19.70%	2.281%
5	2.560	383	395	410	rBV2	49146	80502	28.86%	3.341%
6	3.174	575	586	606	rVB	6526	15829	5.67%	0.657%
7	3.692	738	747	760	rVB7	2811	6005	2.15%	0.249%
8	4.634	1026	1040	1082	rBV2	36515	128406	46.03%	5.330%
9	5.055	1155	1171	1193	rBV	56267	125366	44.94%	5.203%
10	5.718	1359	1377	1398	rBV3	104113	278974	100.00%	11.579%
11	6.242	1529	1540	1566	rBV	103214	201975	72.40%	8.383%
12	6.682	1663	1677	1699	rBV2	69192	135494	48.57%	5.624%
13	7.560	1939	1950	1967	rBV2	27173	49304	17.67%	2.046%
14	7.894	2038	2054	2075	rBV	115333	207656	74.44%	8.619%
15	8.177	2131	2142	2157	rBV3	15741	28551	10.23%	1.185%
16	8.631	2273	2283	2317	rBV2	129902	269854	96.73%	11.201%
17	9.412	2513	2526	2553	rBV	154932	266305	95.46%	11.053%
18	10.750	2929	2942	2961	rBV	65116	107596	38.57%	4.466%
19	11.807	3259	3271	3292	rBV	128101	212276	76.09%	8.811%
20	12.187	3376	3389	3408	rBV2	108753	182879	65.55%	7.591%




Sum of corrected areas: 2409286

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
Data File : VU060527.D
Acq On : 23 Aug 2024 22:22
Operator : MD/SY
Sample : P3711-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2495

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

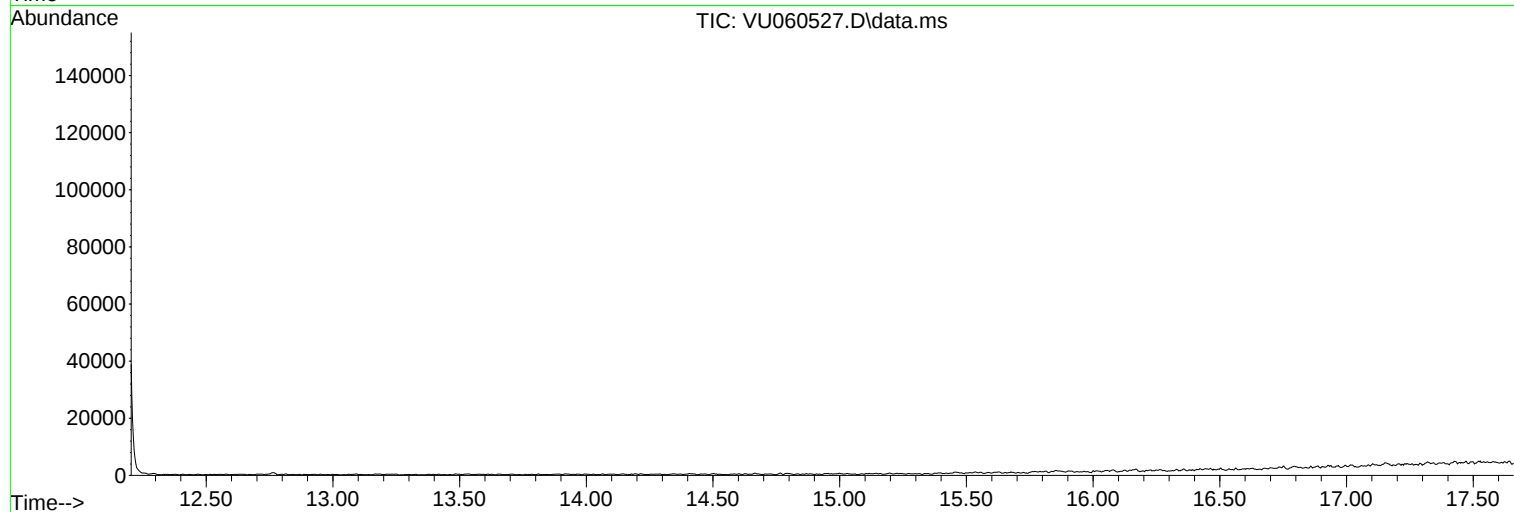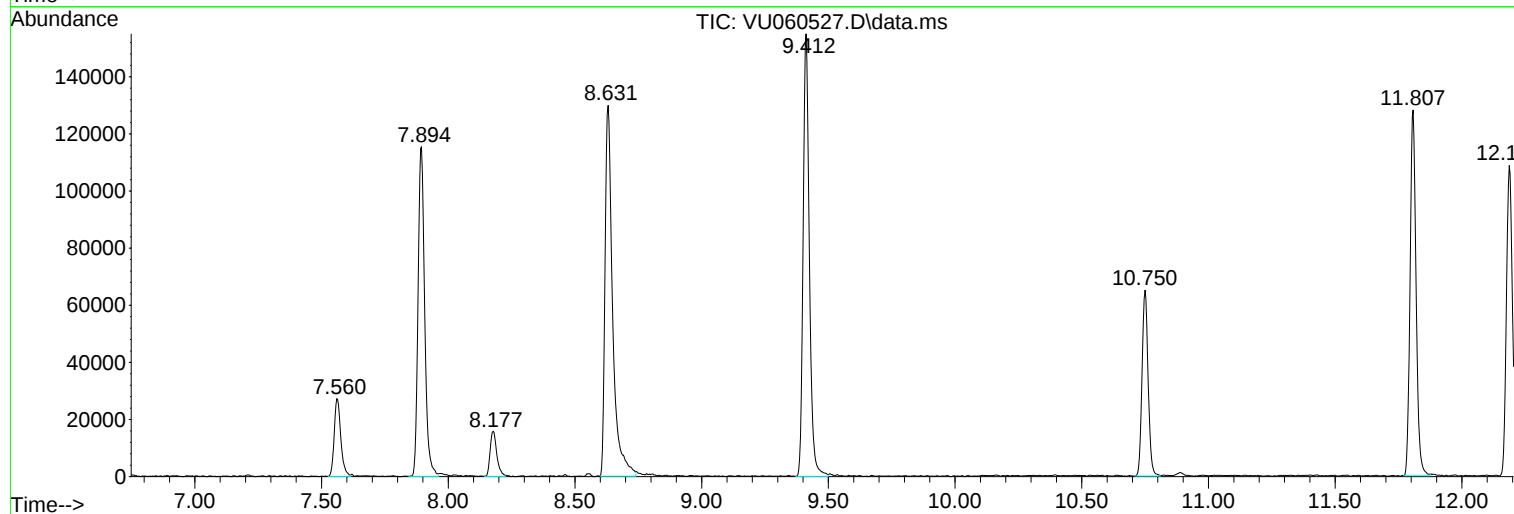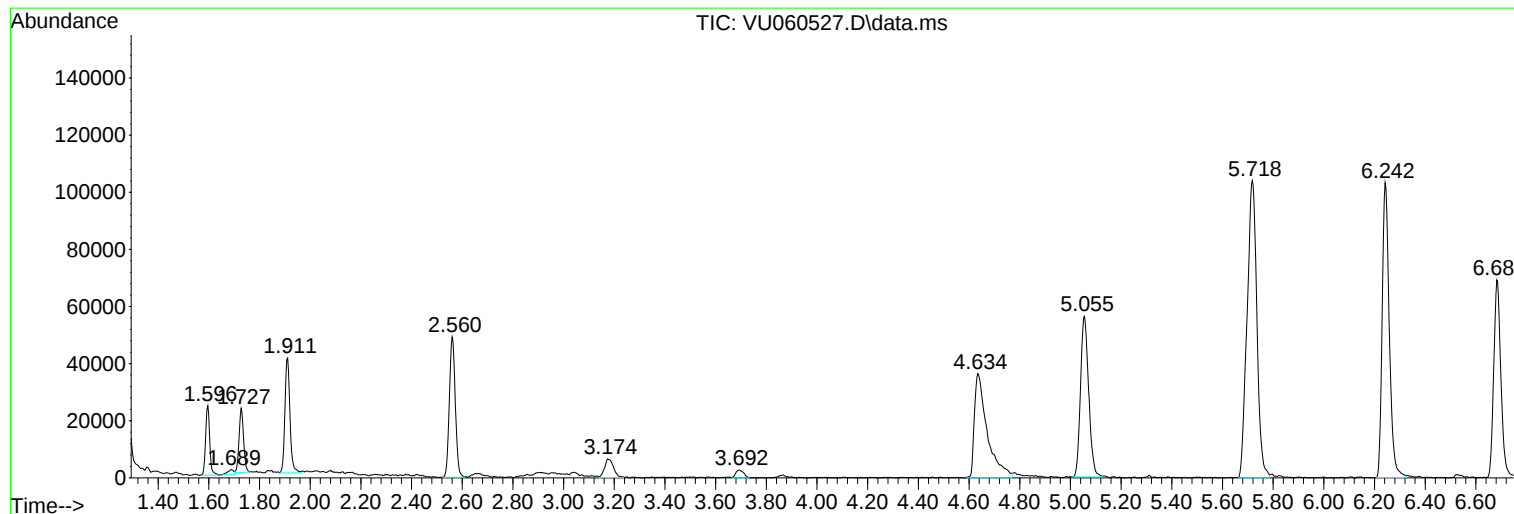

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
Data File : VU060527.D
Acq On : 23 Aug 2024 22:22
Operator : MD/SY
Sample : P3711-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2495

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
Data File : VU060527.D
Acq On : 23 Aug 2024 22:22
Operator : MD/SY
Sample : P3711-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2495

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc