


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU082324\
Data File : VU060507.D
Acq On : 23 Aug 2024 11:14
Operator : MD/SY
Sample : BFB189
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB189

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Aug 27 05:49:06 2024

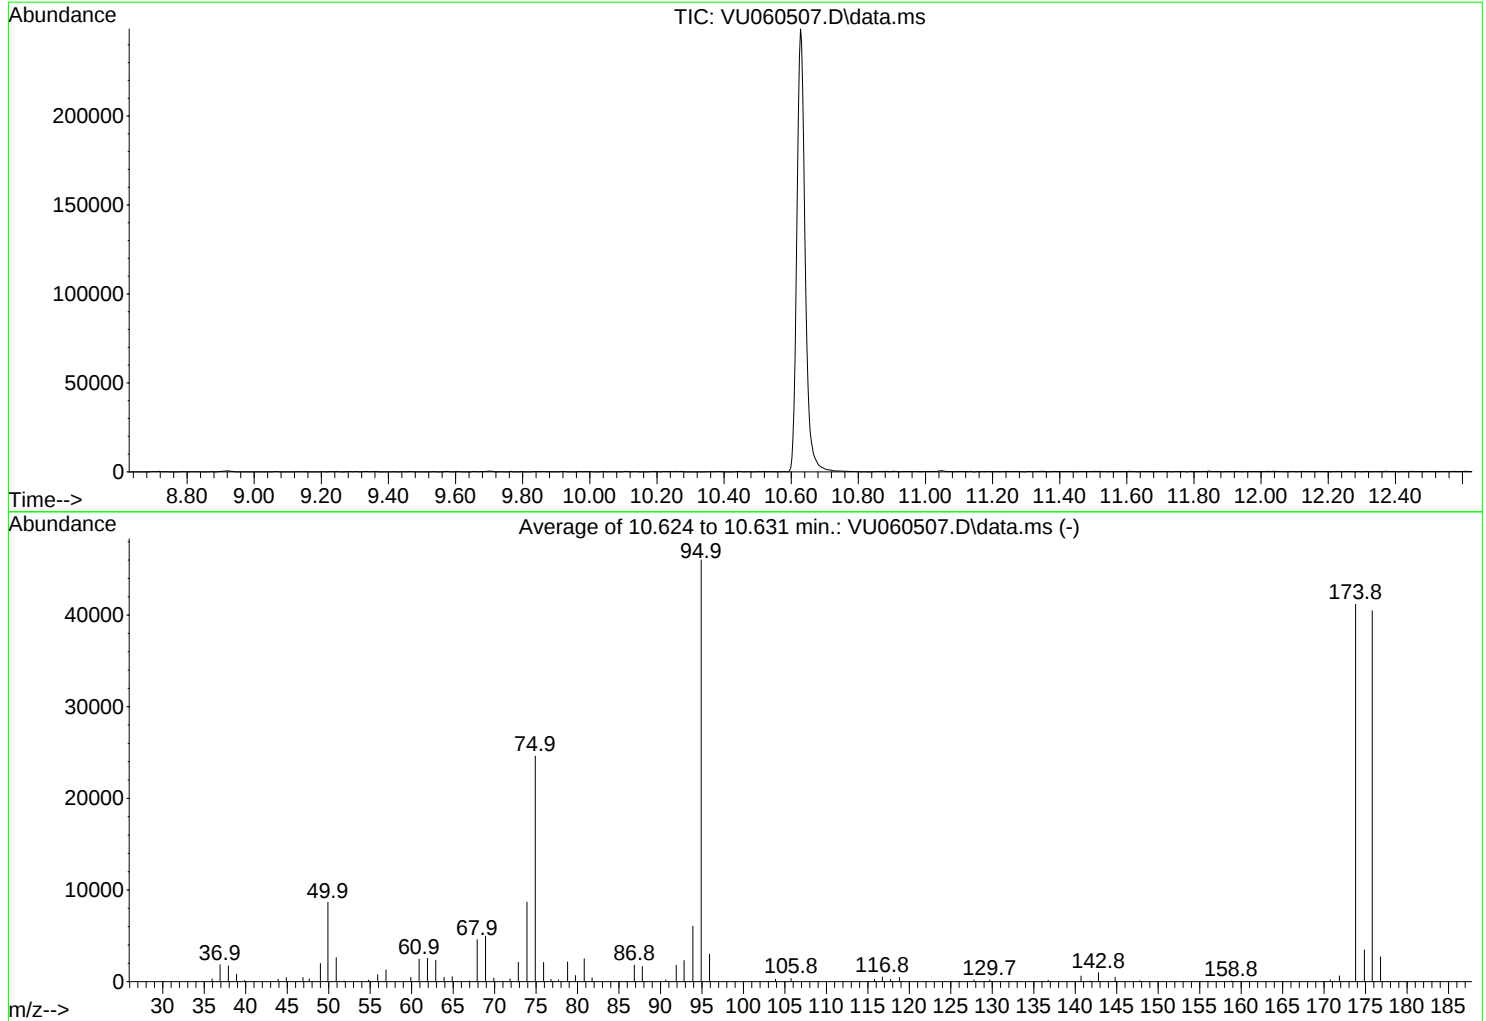

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	8642	PASS
75	95	30	80	53.5	24613	PASS
95	95	100	100	100.0	46029	PASS
96	95	5	9	6.5	3001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.5	41179	PASS
175	174	5	9	8.4	3463	PASS
176	174	95	101	98.3	40469	PASS
177	176	5	9	6.7	2715	PASS

m/z	Abundance
43.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
36.00	297.0
36.90	1784.0
37.90	1668.0
38.90	764.0
39.90	120.0
43.90	361.0
44.90	444.0
46.90	529.0
47.60	302.0
49.00	1842.0
49.90	8506.0
50.90	2637.0
54.80	190.0
55.90	776.0
56.90	1301.0
59.90	443.0
60.90	2442.0
61.90	2584.0
62.90	2254.0
63.90	458.0
64.90	544.0
67.90	4658.0
68.90	4862.0
69.90	413.0
71.90	284.0
72.80	1885.0
73.90	8306.0
74.90	23952.0
75.90	2028.0
76.80	253.0
77.80	183.0
78.80	2130.0
79.80	598.0
80.80	2527.0
81.70	426.0
86.90	1611.0
87.80	1612.0
90.70	214.0
91.90	1813.0
92.80	2144.0
93.90	5843.0
94.90	44752.0
95.90	2868.0
103.90	216.0
105.70	334.0
115.80	211.0
116.80	457.0
117.70	264.0
118.80	430.0
127.80	147.0
128.60	105.0
129.70	201.0
136.70	178.0
140.70	592.0
141.80	104.0
142.80	995.0
144.80	467.0
147.80	131.0
158.80	117.0
170.80	211.0
171.80	553.0
173.80	39184.0
174.90	3386.0
175.80	38520.0
176.80	2701.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
35.90	338.0
36.90	1923.0
37.90	1705.0
38.90	825.0
39.80	128.0
43.90	369.0
44.90	454.0
46.90	446.0
47.60	303.0
49.00	2007.0
49.90	8846.0
50.90	2676.0
51.90	106.0
53.00	104.0
54.80	168.0
55.90	803.0
56.90	1278.0
59.90	476.0
60.90	2524.0
61.90	2643.0
62.90	2457.0
63.90	488.0
64.90	558.0
67.00	142.0
67.90	4681.0
68.90	5077.0
69.90	395.0
71.90	333.0
72.80	2189.0
73.90	8949.0
74.90	25352.0
75.90	2152.0
76.80	268.0
77.70	175.0
78.80	2223.0
79.70	693.0
80.80	2586.0
81.80	438.0
86.90	1889.0
87.80	1676.0
90.60	212.0
91.90	1859.0
92.90	2348.0
93.90	6305.0
94.90	47416.0
95.90	3099.0
103.90	270.0
105.70	363.0
115.80	257.0
116.80	538.0
117.80	286.0
118.80	470.0
127.80	198.0
129.70	199.0
136.70	175.0
140.70	599.0
141.80	124.0
142.80	994.0
144.80	505.0
147.80	111.0
158.80	110.0
170.70	209.0
171.90	656.0
173.80	42440.0
174.80	3600.0
175.80	41864.0
176.80	2798.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
35.90	321.0
36.90	1856.0
37.90	1738.0
38.90	821.0
39.80	111.0
43.90	366.0
44.90	419.0
46.90	370.0
47.70	294.0
49.00	2058.0
49.90	8575.0
50.90	2523.0
51.80	119.0
54.80	172.0
55.90	747.0
56.90	1250.0
59.90	515.0
60.90	2433.0
61.90	2404.0
62.90	2307.0
63.90	457.0
64.90	502.0
67.00	118.0
67.90	4422.0
68.90	4963.0
69.90	358.0
71.80	338.0
72.90	2261.0
73.90	8785.0
74.90	24536.0
75.90	2085.0
76.80	283.0
77.60	221.0
78.80	2097.0
79.70	706.0
80.80	2386.0
81.80	432.0
85.90	102.0
86.80	1907.0
87.80	1688.0
90.60	176.0
91.90	1666.0
92.90	2411.0
93.90	6008.0
94.90	45920.0
95.90	3035.0
103.80	287.0
105.80	371.0
115.80	267.0
116.70	535.0
117.80	262.0
118.80	507.0
127.80	224.0
129.70	175.0
136.80	123.0
140.70	637.0
142.80	949.0
144.80	509.0
147.80	101.0
170.80	183.0
171.90	657.0
173.80	41912.0
174.80	3403.0
175.80	41024.0
176.80	2646.0
177.80	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189