

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU083119\
 Data File : VU034108.D
 Acq On : 30 Aug 2019 19:00
 Operator : JC/SP
 Sample : K4529-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-T2-(1.9)

Quant Time: Aug 31 03:41:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	525116	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.86	114	831688	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	795625	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.47	152	406224	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.29	65	309306	45.97	ug/l	0.00
Spiked Amount			Recovery	=	91.94%	
35) Dibromofluoromethane	4.86	113	262758	45.55	ug/l	0.00
Spiked Amount			Recovery	=	91.10%	
50) Toluene-d8	7.55	98	1049766	48.60	ug/l	0.00
Spiked Amount			Recovery	=	97.20%	
62) 4-Bromofluorobenzene	10.29	95	381772	45.44	ug/l	0.00
Spiked Amount			Recovery	=	90.88%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	734	Below Cal		94
5) Bromomethane	1.63	94	814	Below Cal		84
8) Diethyl Ether	2.09	74	1321	0.379	ug/l	85
11) Tert butyl alcohol	2.82	59	4079	2.629	ug/l #	73
13) Acrolein	2.19	56	400	0.613	ug/l #	1
16) Acetone	2.31	43	33999	9.903	ug/l	99
18) Methyl Acetate	2.61	43	4880	0.550	ug/l	94
20) Methylene Chloride	2.69	84	10698	1.646	ug/l	94
25) 2-Butanone	4.27	43	3849	0.806	ug/l	97
29) Tetrahydrofuran	4.64	42	791	0.269	ug/l #	43
31) Cyclohexane	4.96	56	9682	0.964	ug/l #	1
36) 1,1-Dichloropropene	4.96	75	37321	4.744	ug/l #	49
37) Ethyl Acetate	4.27	43	3849	0.437	ug/l #	68
38) Carbon Tetrachloride	4.96	117	46168	6.080	ug/l #	15
43) Isopropyl Acetate	5.53	43	124694	9.304	ug/l	99
48) Methyl methacrylate	6.52	41	7044	1.089	ug/l #	14
49) 1,4-Dioxane	6.61	88	42	0.259	ug/l #	1
51) 4-Methyl-2-Pentanone	7.40	43	105969	11.449	ug/l #	46
54) cis-1,3-Dichloropropene	7.40	75	56889	5.683	ug/l #	59
56) Ethyl methacrylate	8.00	69	189	0.990	ug/l #	27
57) 1,3-Dichloropropane	8.40	76	9462	0.899	ug/l #	42
59) 2-Hexanone	8.30	43	126633	18.124	ug/l #	23
76) 1,2,3-Trichloropropane	10.29	75	182406	19.923	ug/l #	37
81) trans-1,4-Dichloro-2-buten	10.29	75	182406	67.085	ug/l #	100
93) 1,2,4-Trichlorobenzene	13.50	180	132	1.129	ug/l #	61
95) Naphthalene	13.75	128	1796	1.858	ug/l #	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU083119\
Data File : VU034108.D
Acq On : 30 Aug 2019 19:00
Operator : JC/SP
Sample : K4529-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)

Quant Time: Aug 31 03:41:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

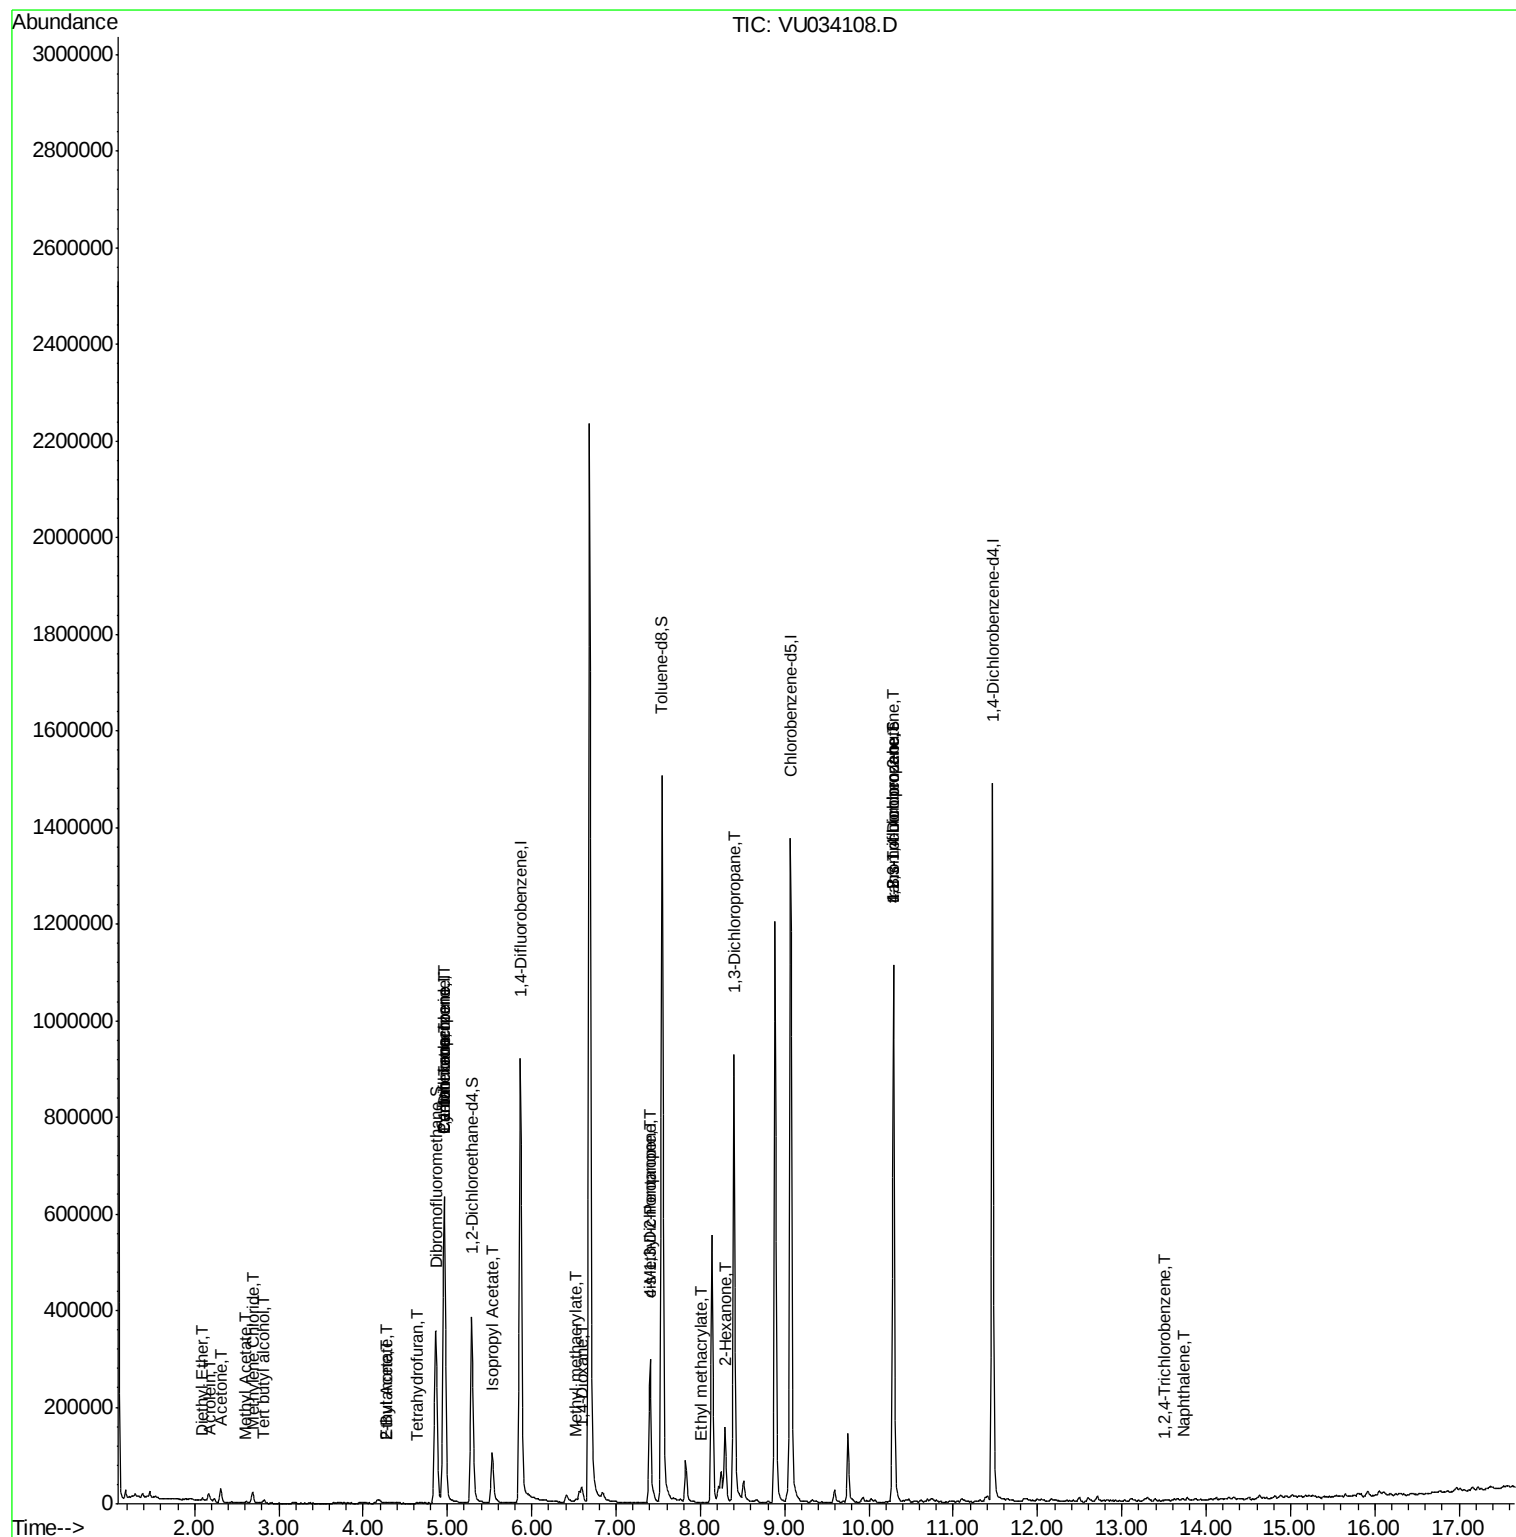



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :


T9-12-13-T2-(1.9)

Tgt Ion:168 Resp: 525116

Ion Ratio Lower Upper

168 100

99 54.0 42.3 63.5



Abundance Ion 167.90 (167.60 to 168.60): VU034108.D (-1185) (-)

Ion 98.90 (98.60 to 99.60): VU034108.D (-1185) (-)

4.96

250000

200000

150000



100000

50000

0

4.90 5.00 5.10

Time-->



#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 74

Delta R.T. 0.01 min

Lab File: VU034108.D


Acq: 30 Aug 2019 19:00

Tgt Ion: 50 Resp: 734

Ion Ratio Lower Upper

50 100

52 36.1 26.2 39.4



Abundance Ion 49.90 (49.60 to 50.60): VU034108.D (-63) (-)

Ion 51.90 (51.60 to 52.60): VU034108.D (-63) (-)

1.33

600


400

200

0

1.30 1.32 1.34 1.36

Time-->





#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 169

Delta R.T. 0.04 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :


T9-12-13-T2-(1.9)

Tgt Ion: 94 Resp: 814




Ion Ratio Lower Upper

94 100

96 80.2 76.3 114.5

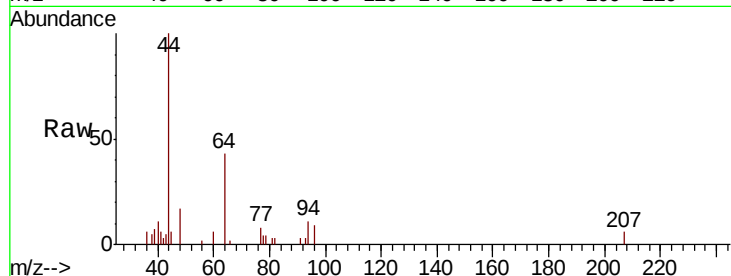

Abundance Ion 93.90 (93.60 to 94.60): VU034108.D (-143) (-)

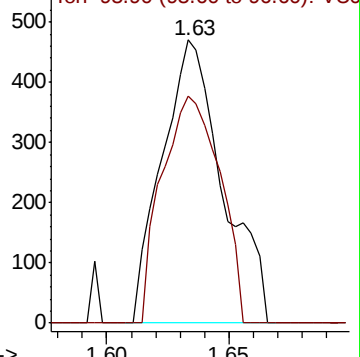

#8

Diethyl Ether

Concen: 0.379 ug/l

RT: 2.09 min Scan# 312

Delta R.T. 0.00 min

Lab File: VU034108.D


Acq: 30 Aug 2019 19:00

Tgt Ion: 74 Resp: 1321



Ion Ratio Lower Upper


74 100

45 119.2 51.8 155.5



Abundance Ion 74.00 (73.70 to 74.70): VU034108.D (-300) (-)




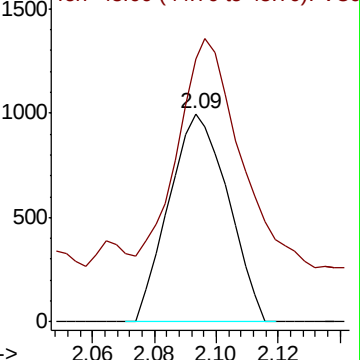


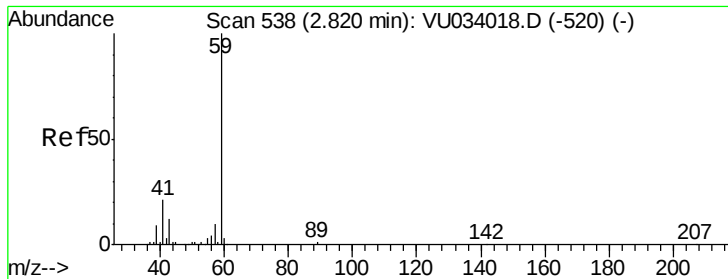

#11
Tert butyl alcohol
Concen: 2.629 ug/l
RT: 2.82 min Scan# 539
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion: 59 Resp: 4079
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

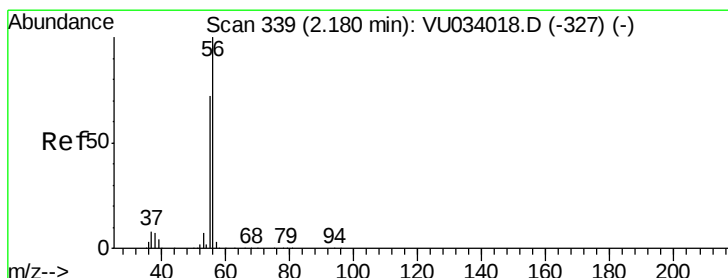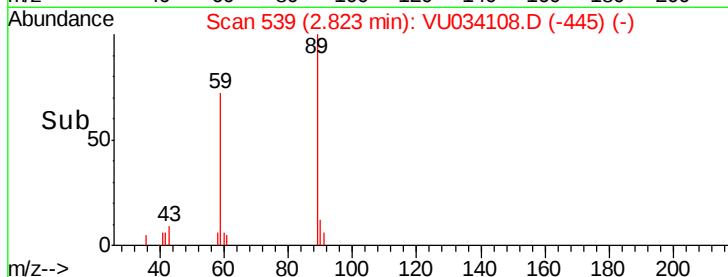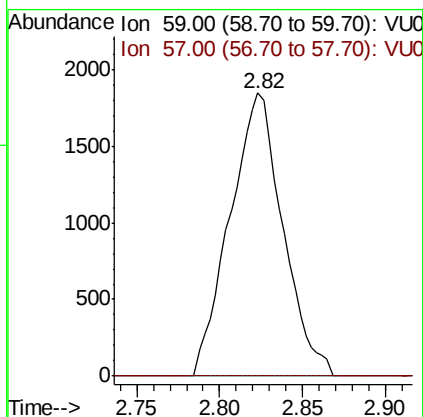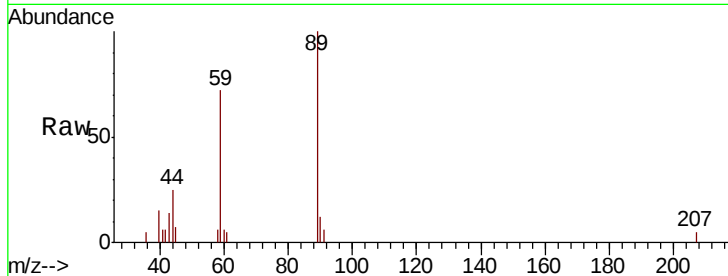

#13
Acrolein
Concen: 0.613 ug/l
RT: 2.19 min Scan# 341
Delta R.T. 0.01 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion: 56 Resp: 400
Ion Ratio Lower Upper
56 100
55 166.3 57.1 85.7#

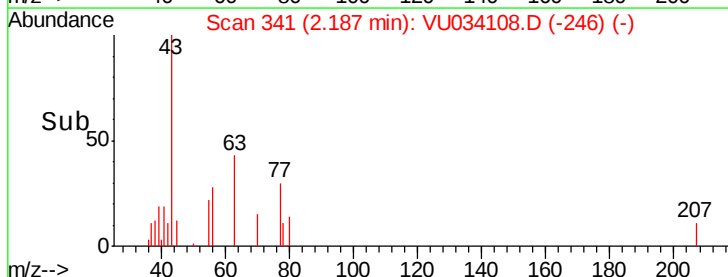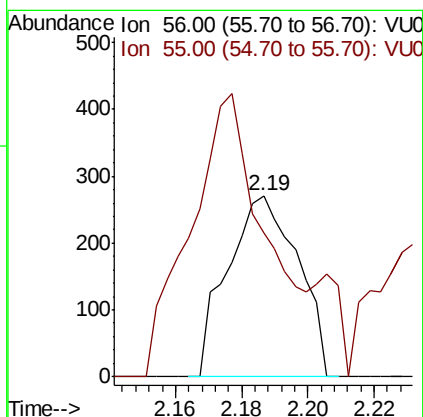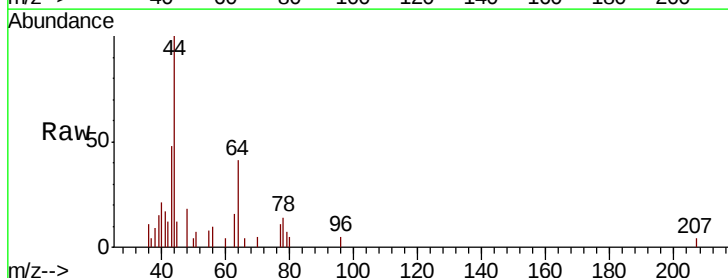

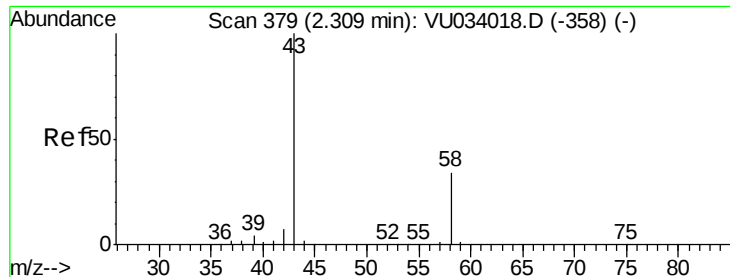

#16

Acetone

Concen: 9.903 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :


T9-12-13-T2-(1.9)

Tgt Ion: 43 Resp: 33999




Ion Ratio Lower Upper

43 100

58 33.9 26.8 40.2

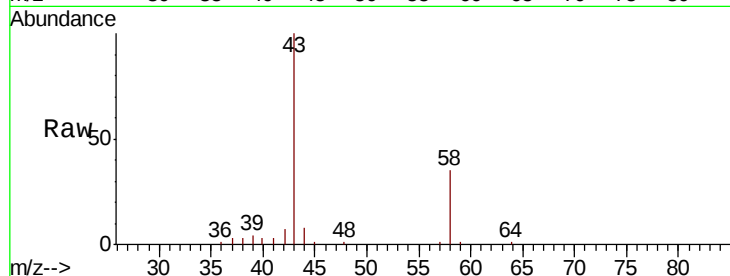

Abundance Ion 43.00 (42.70 to 43.70): VU034108.D (-380) (-)

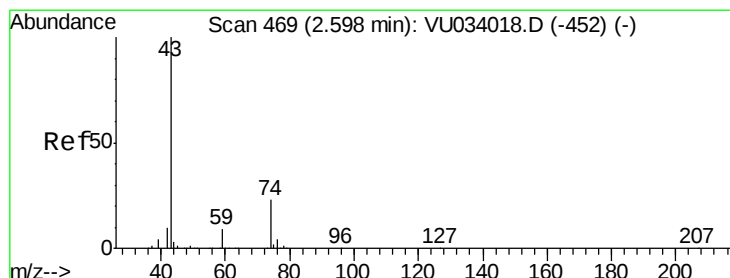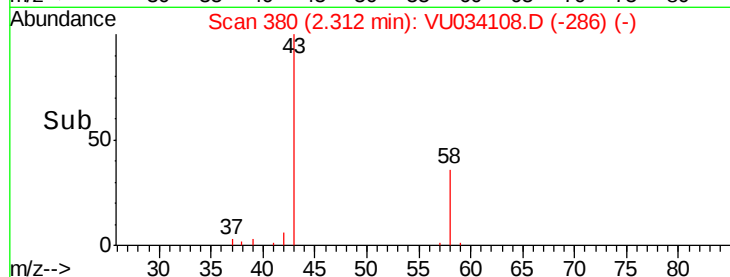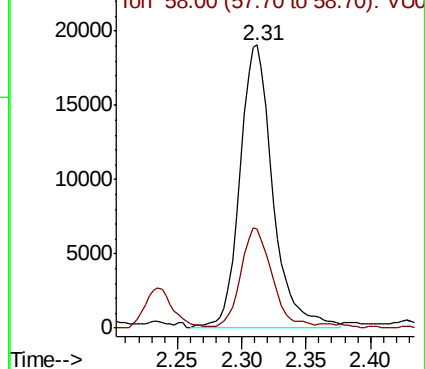

#18

Methyl Acetate

Concen: 0.550 ug/l

RT: 2.61 min Scan# 472

Delta R.T. 0.01 min

Lab File: VU034108.D


Acq: 30 Aug 2019 19:00

Tgt Ion: 43 Resp: 4880



Ion Ratio Lower Upper


43 100

74 21.1 19.2 28.8

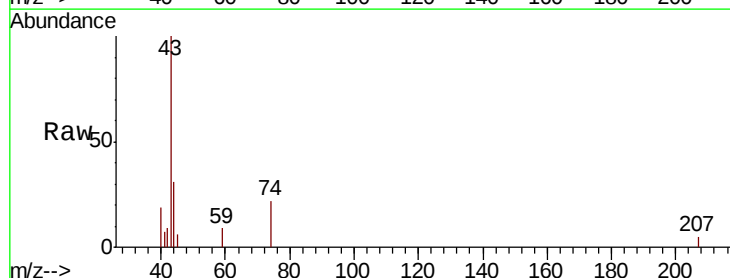

Abundance Ion 43.00 (42.70 to 43.70): VU034108.D (-472) (-)



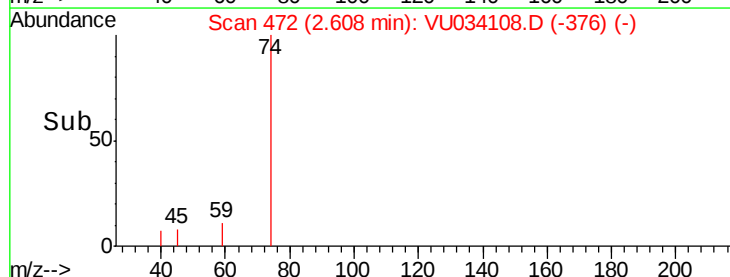
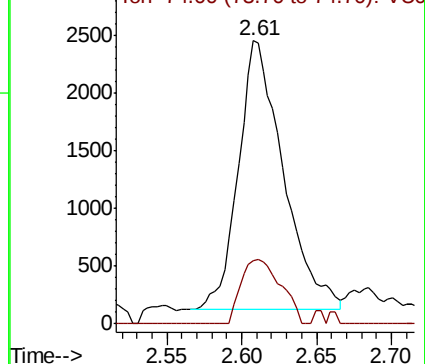




#20
Methylene Chloride
Concen: 1.646 ug/l
RT: 2.69 min Scan# 497
Delta R.T. 0.01 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion:	84	Resp:	10698
Ion	Ratio	Lower	Upper
84	100		
49	115.2	100.2	150.4
51	36.4	30.8	46.2
86	64.7	52.5	78.7

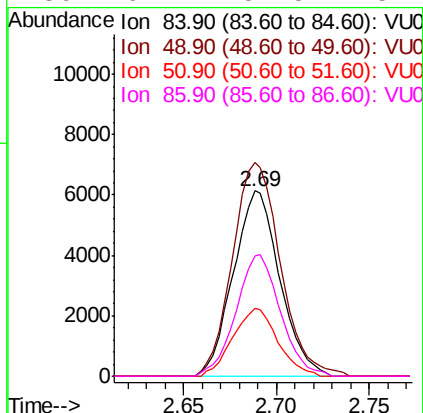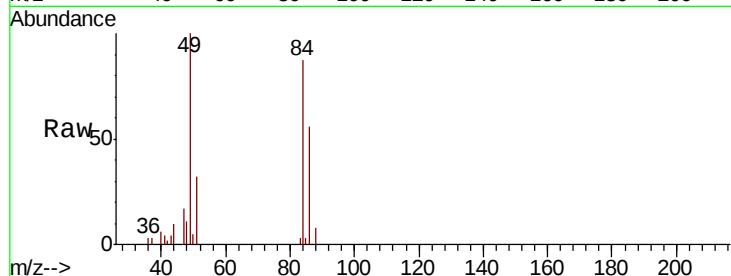

#25
2-Butanone
Concen: 0.806 ug/l
RT: 4.27 min Scan# 989
Delta R.T. 0.04 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion:	43	Resp:	3849
Ion	Ratio	Lower	Upper
43	100		
72	28.2	21.2	31.8

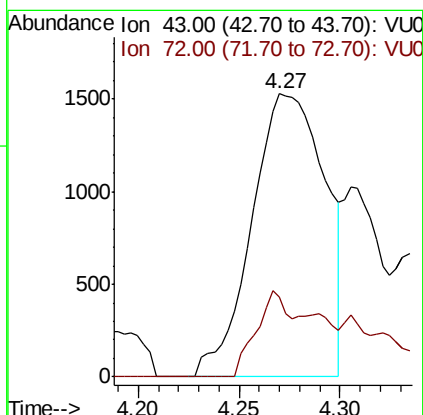



#29

Tetrahydrofuran

Concen: 0.269 ug/l

RT: 4.64 min Scan# 1105

Delta R.T. 0.03 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-T2-(1.9)


Tgt Ion: 42 Resp: 791

Ion Ratio Lower Upper

42 100

72 10.7 35.8 53.6#




71 2.5 34.0 51.0#

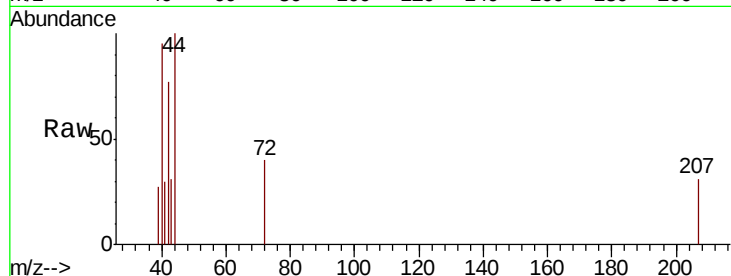

Abundance Ion 42.00 (41.70 to 42.70): VU034108.D (-1105) (-)

Ion 72.00 (71.70 to 72.70): VU034108.D (-1105) (-)

Ion 71.00 (70.70 to 71.70): VU034108.D (-1105) (-)

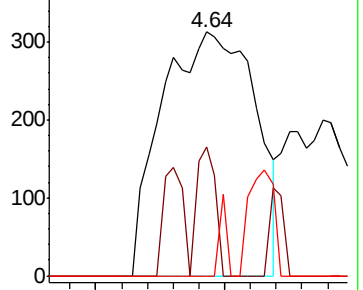

#31

Cyclohexane

Concen: 0.964 ug/l

RT: 4.96 min Scan# 1203

Delta R.T. -0.01 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00


Tgt Ion: 56 Resp: 9682

Ion Ratio Lower Upper

56 100

69 199.5 25.4 38.0#



84 166.6 65.8 98.8#




Abundance Ion 56.00 (55.70 to 56.70): VU034108.D (-1186) (-)

Ion 69.00 (68.70 to 69.70): VU034108.D (-1186) (-)

Ion 84.00 (83.70 to 84.70): VU034108.D (-1186) (-)




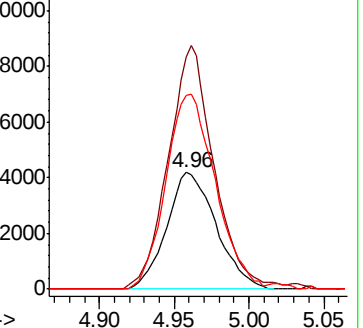




#33
 1,2-Dichloroethane-d4
 Concen: 45.969 ug/l
 RT: 5.29 min Scan# 1305
 Delta R.T. 0.00 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-T2-(1.9)


Tgt Ion: 65 Resp: 309306
 Ion Ratio Lower Upper
 65 100
 67 54.4 0.0 110.6

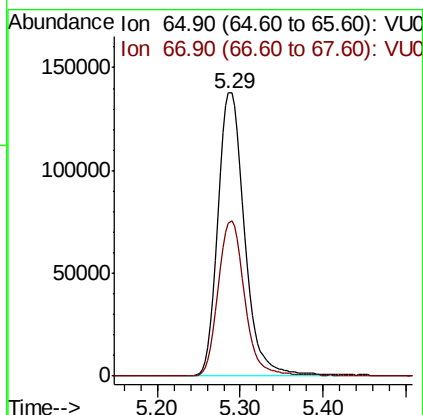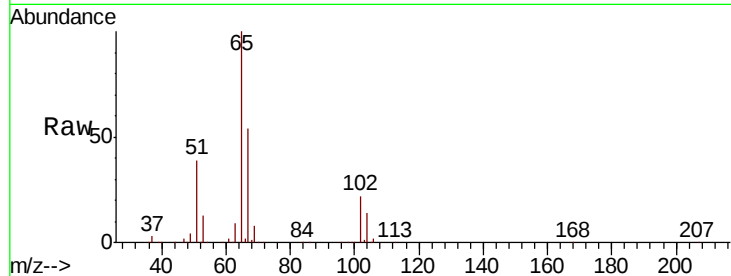

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.86 min Scan# 1485
 Delta R.T. 0.00 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00

Tgt Ion: 114 Resp: 831688
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 42.0
 88 16.3 0.0 32.0


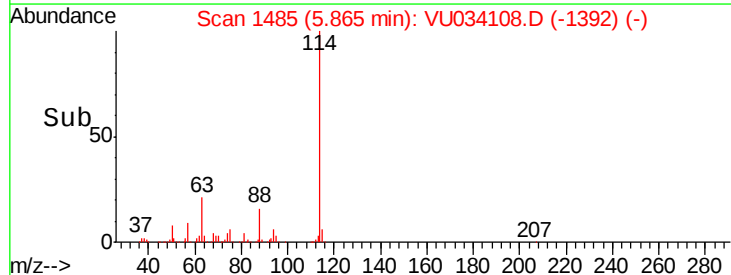
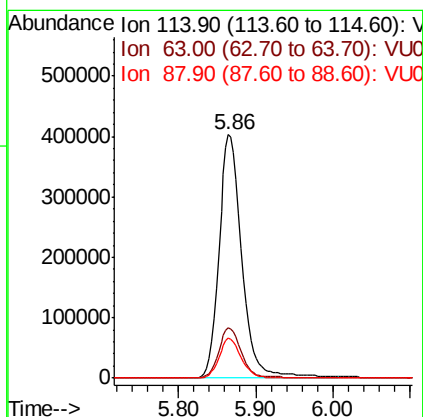



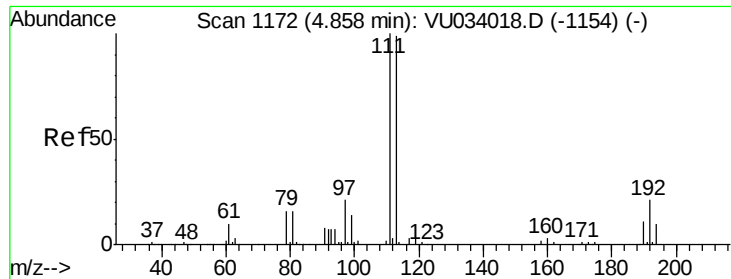

#35
 Dibromofluoromethane
 Concen: 45.550 ug/l
 RT: 4.86 min Scan# 1172
 Delta R.T. 0.00 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-T2-(1.9)


Tgt Ion	Ratio	Lower	Upper
113	100		
111	100.6	81.7	122.5
192	20.8	17.1	25.7

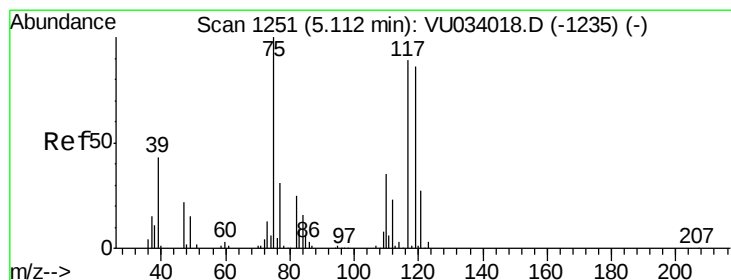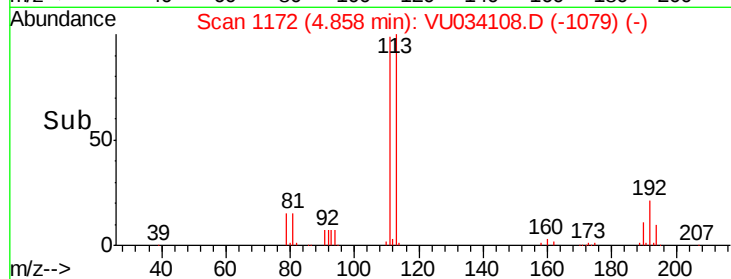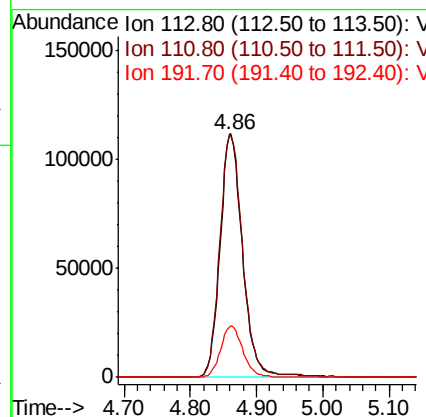

#36
 1,1-Dichloropropene
 Concen: 4.744 ug/l
 RT: 4.96 min Scan# 1203
 Delta R.T. -0.15 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.4	17.8	53.5#
77	0.0	25.0	37.4#


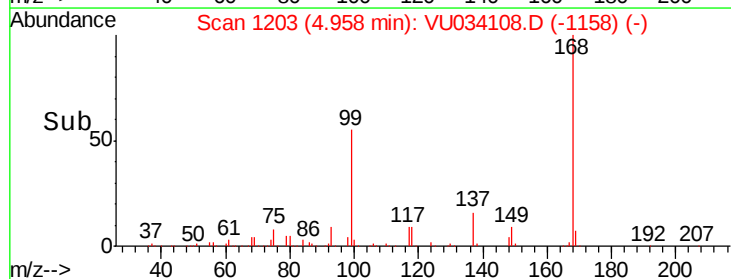
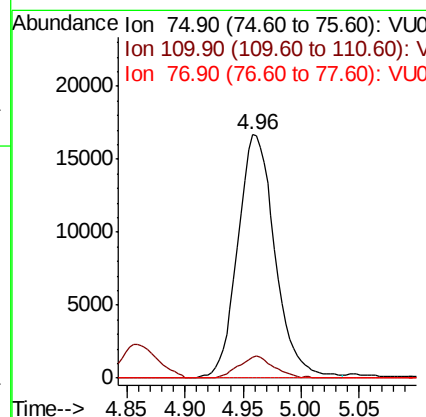
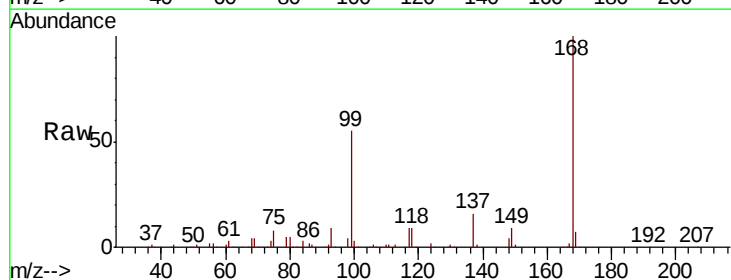




#37
Ethyl Acetate
Concen: 0.437 ug/l
RT: 4.27 min Scan# 989
Delta R.T. -0.08 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion: 43 Resp: 3849
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 8.6 12.8#

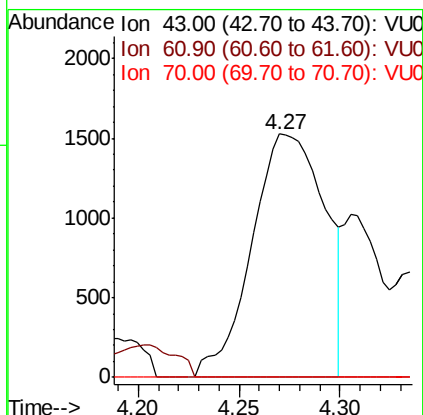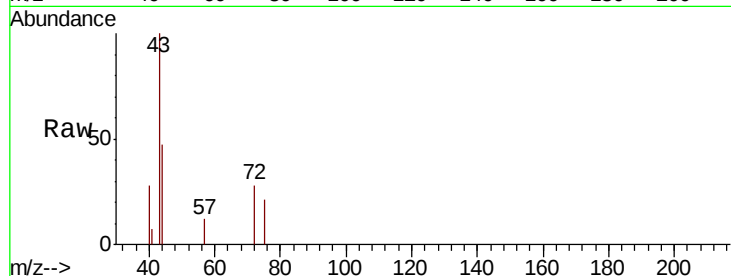

#38
Carbon Tetrachloride
Concen: 6.080 ug/l
RT: 4.96 min Scan# 1204
Delta R.T. -0.15 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion: 117 Resp: 46168
Ion Ratio Lower Upper
117 100
119 4.5 77.0 115.4#
121 0.0 23.9 35.9#

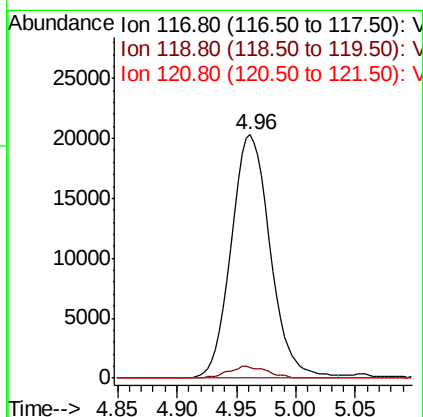

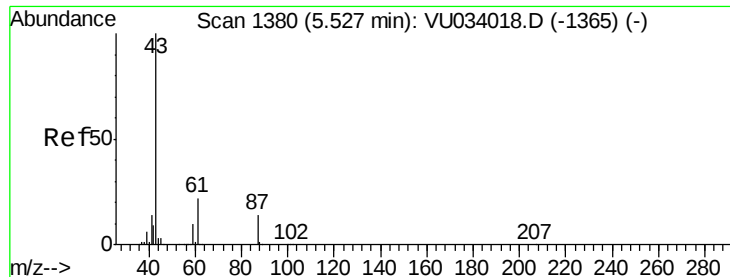

#43

Isopropyl Acetate

Concen: 9.304 ug/l

RT: 5.53 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampleId :

T9-12-13-T2-(1.9)


Tgt Ion: 43 Resp: 124694

Ion Ratio Lower Upper

43 100

61 20.9 17.2 25.8




87 13.2 10.8 16.2

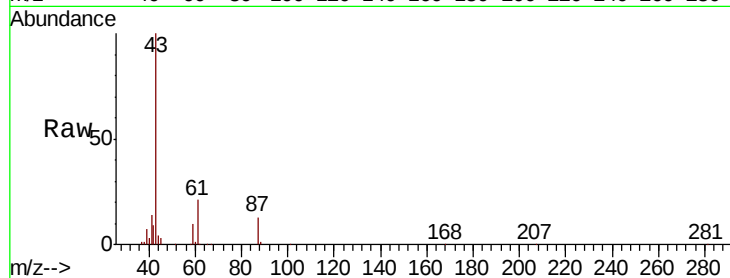

Abundance Ion 43.00 (42.70 to 43.70): VU034108.D (-1365) (-)

Ion 61.00 (60.70 to 61.70): VU034108.D (-1365) (-)

Ion 87.00 (86.70 to 87.70): VU034108.D (-1365) (-)

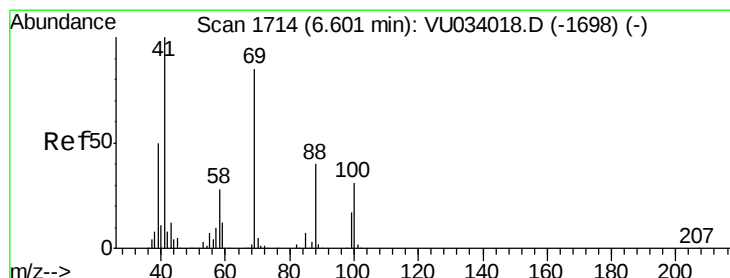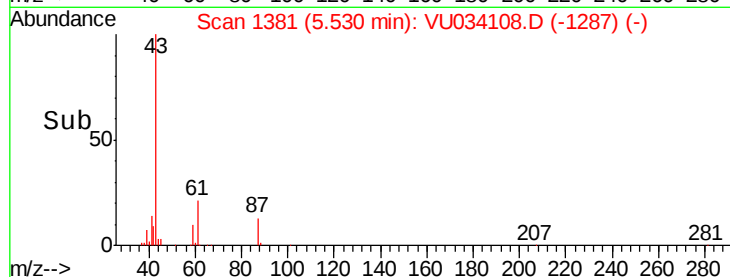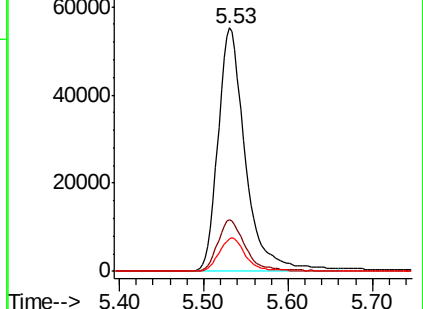

#48

Methyl methacrylate

Concen: 1.089 ug/l

RT: 6.52 min Scan# 1690

Delta R.T. -0.08 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00


Tgt Ion: 41 Resp: 7044

Ion Ratio Lower Upper

41 100

69 0.0 69.5 104.3#



39 0.0 40.3 60.5#

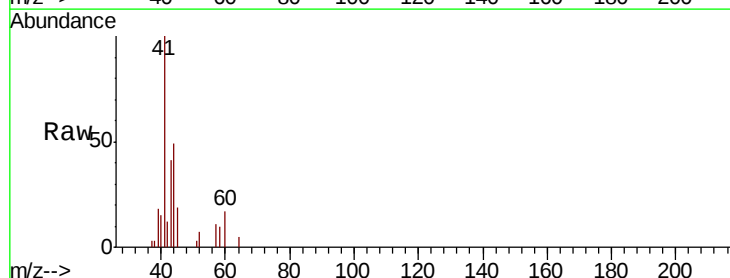


Abundance Ion 41.00 (40.70 to 41.70): VU034108.D (-1698) (-)

Ion 69.00 (68.70 to 69.70): VU034108.D (-1698) (-)

Ion 39.00 (38.70 to 39.70): VU034108.D (-1698) (-)



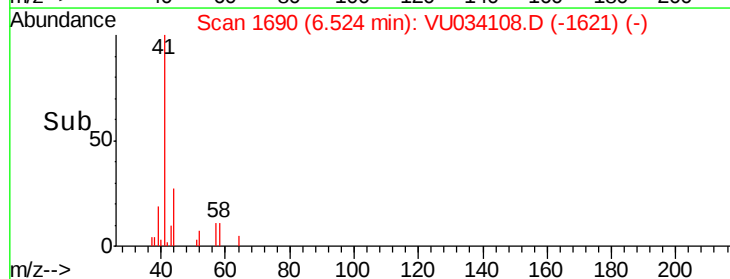
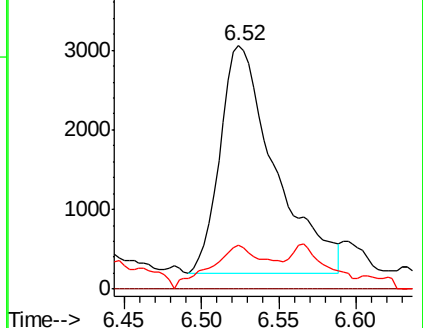




#49
1,4-Dioxane
Concen: 0.259 ug/l
RT: 6.61 min Scan# 1717
Delta R.T. 0.02 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion: 88 Resp: 42
Ion Ratio Lower Upper
88 100
43 0.0 24.8 37.2#
58 2040.5 59.3 88.9#

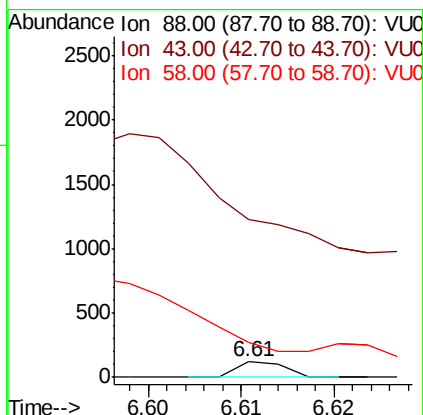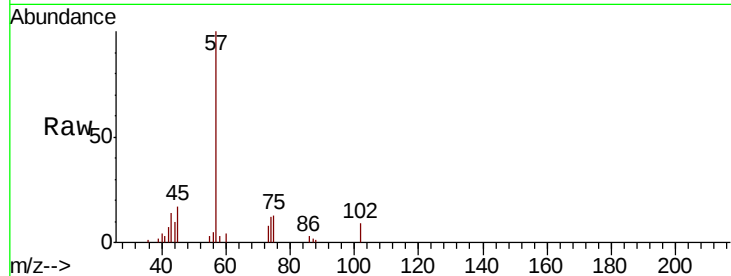

#50
Toluene-d8
Concen: 48.601 ug/l
RT: 7.55 min Scan# 2008
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion: 98 Resp: 1049766
Ion Ratio Lower Upper
98 100
100 64.9 50.3 75.5


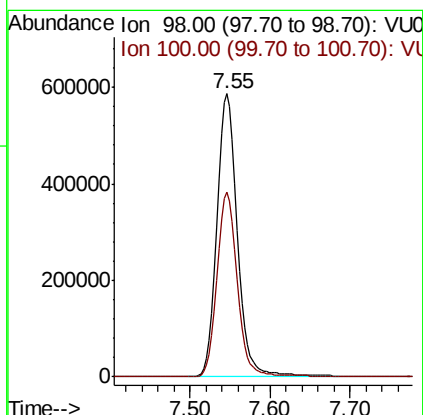




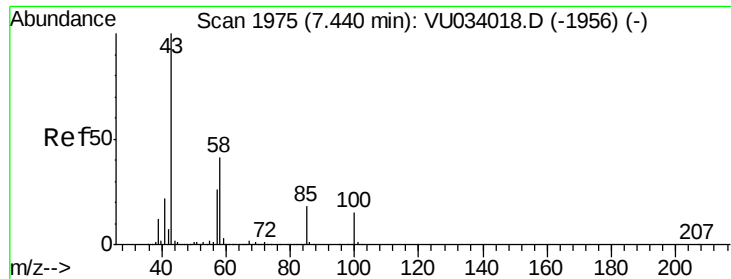

#51
 4-Methyl-2-Pentanone
 Concen: 11.449 ug/l
 RT: 7.40 min Scan# 1963
 Delta R.T. -0.04 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00




Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-T2-(1.9)


Tgt Ion: 43 Resp: 105969
 Ion Ratio Lower Upper
 43 100
 58 7.0 32.2 48.4#

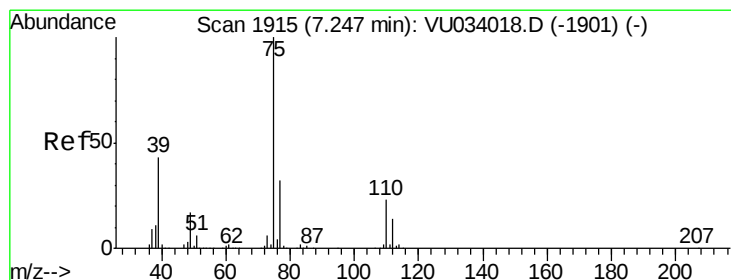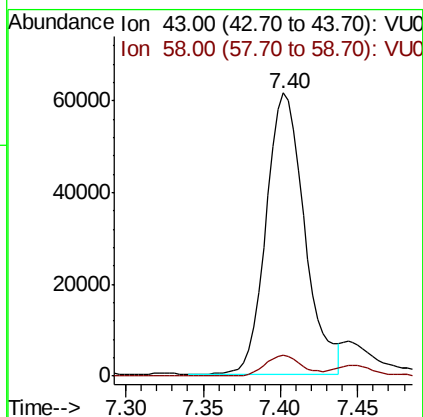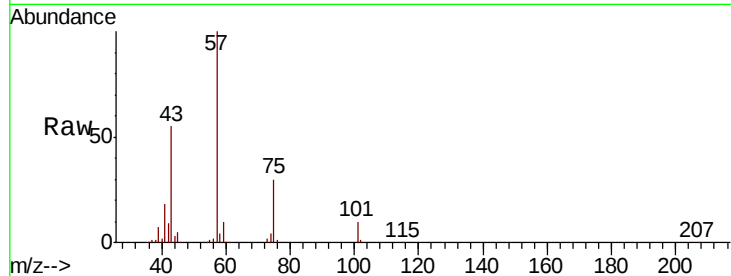

#54
 cis-1,3-Dichloropropene
 Concen: 5.683 ug/l
 RT: 7.40 min Scan# 1963
 Delta R.T. 0.15 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00

Tgt Ion: 75 Resp: 56889
 Ion Ratio Lower Upper
 75 100
 77 0.3 25.2 37.8#
 39 24.5 34.6 51.8#



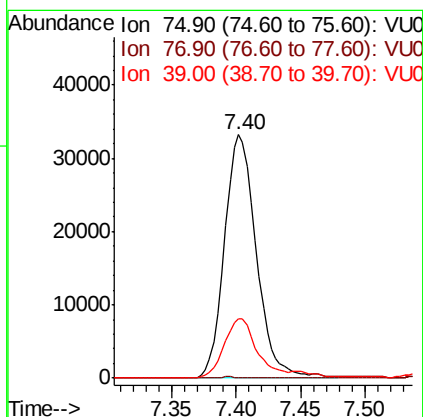



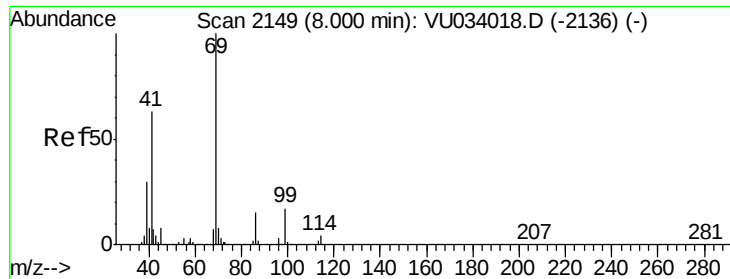

#56
Ethyl methacrylate
Concen: 0.990 ug/l
RT: 8.00 min Scan# 2150
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion: 69 Resp: 189
Ion Ratio Lower Upper
69 100
41 0.0 50.7 76.1#
39 0.0 24.2 36.2#

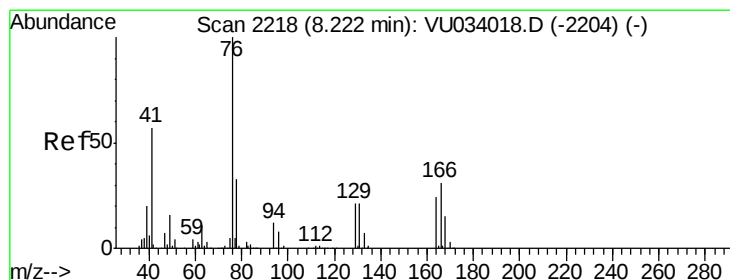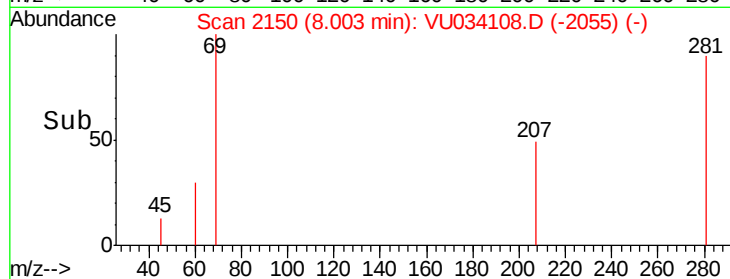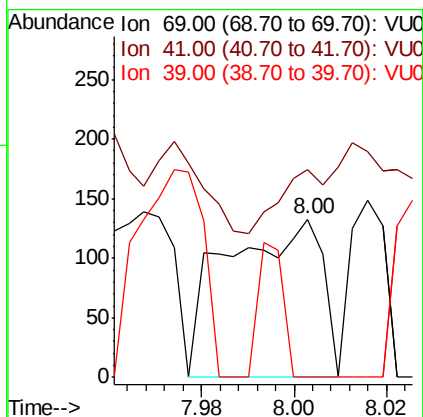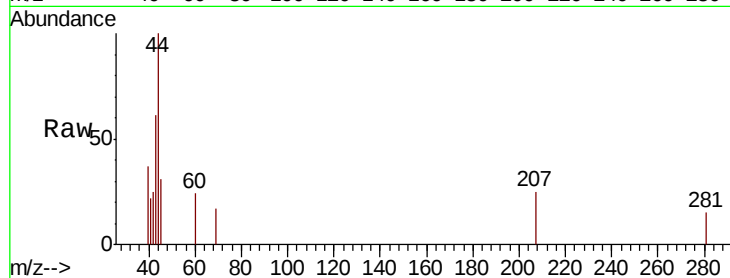

#57
1,3-Dichloropropane
Concen: 0.899 ug/l
RT: 8.40 min Scan# 2273
Delta R.T. 0.18 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion: 76 Resp: 9462
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.4#


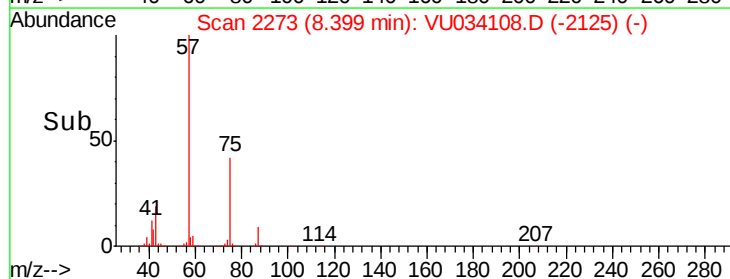
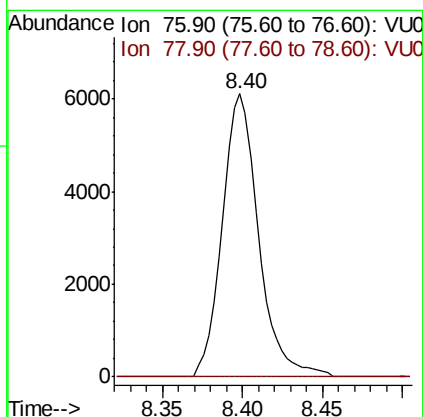
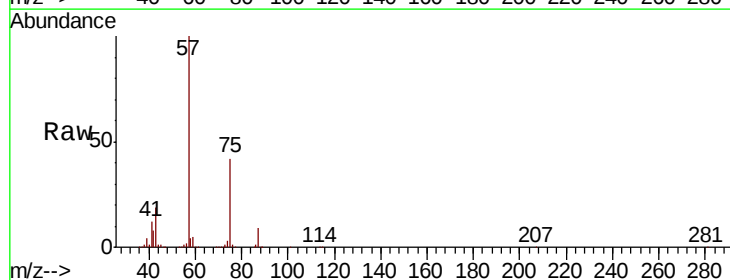


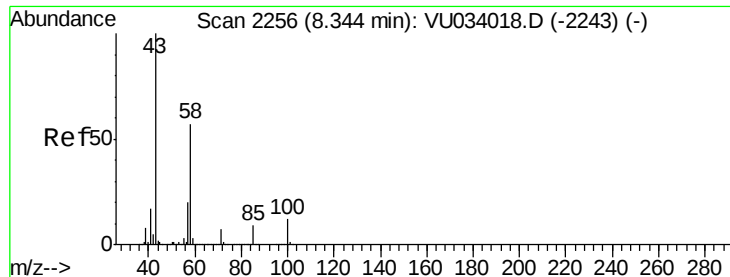

#59
2-Hexanone
Concen: 18.124 ug/l
RT: 8.30 min Scan# 2241
Delta R.T. -0.05 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion: 43 Resp: 126633
Ion Ratio Lower Upper
43 100
58 0.0 28.4 85.3#

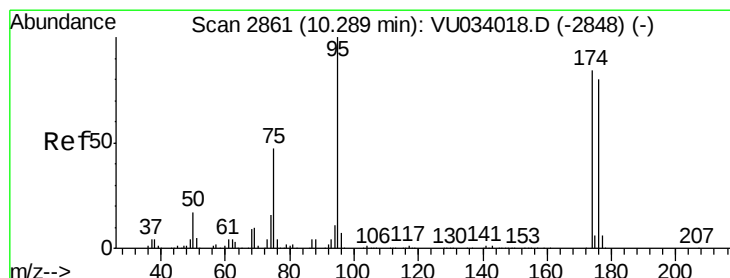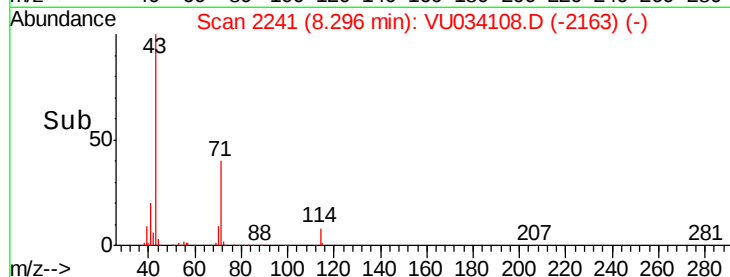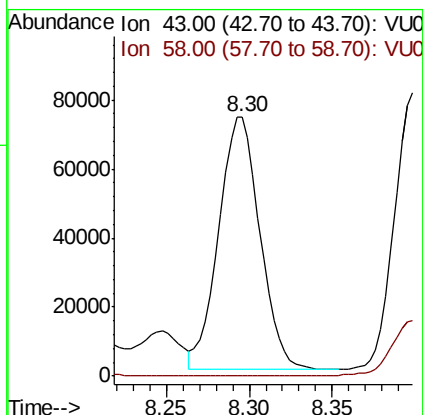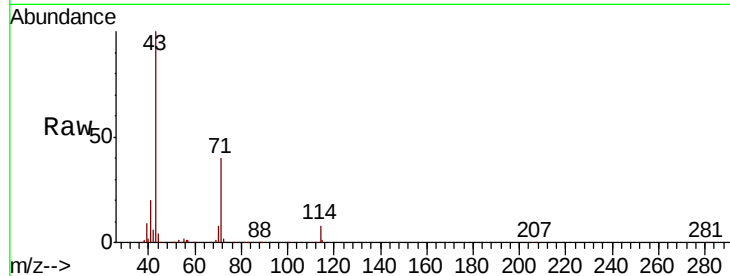

#62
4-Bromofluorobenzene
Concen: 45.438 ug/l
RT: 10.29 min Scan# 2861
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion: 95 Resp: 381772
Ion Ratio Lower Upper
95 100
174 83.4 0.0 168.8
176 81.0 0.0 161.8


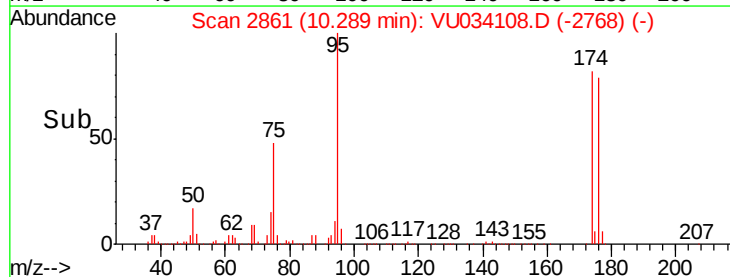
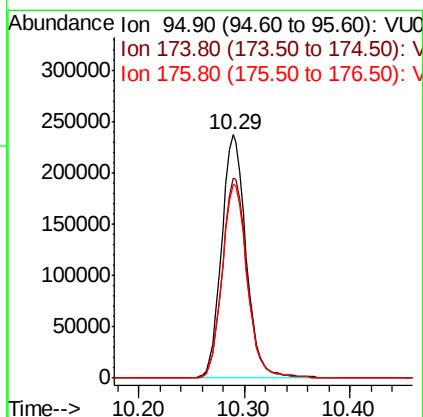
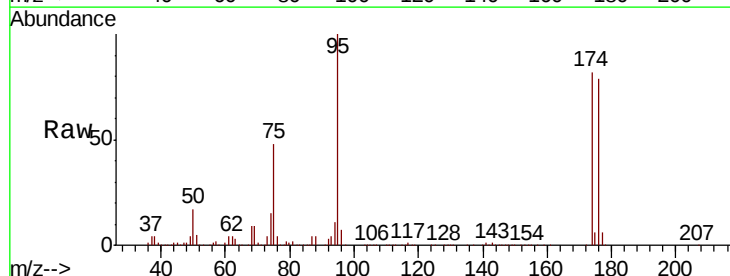


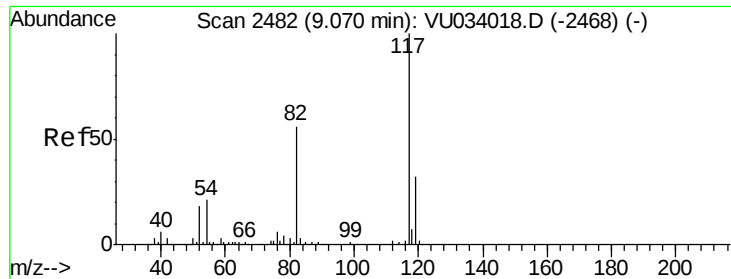

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.07 min Scan# 2482
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00




Instrument :
MSVOA_U
ClientSampleId :
T9-12-13-T2-(1.9)


Tgt Ion	Ratio	Lower	Upper
117	100		
82	55.7	45.1	67.7
119	31.6	25.4	38.0

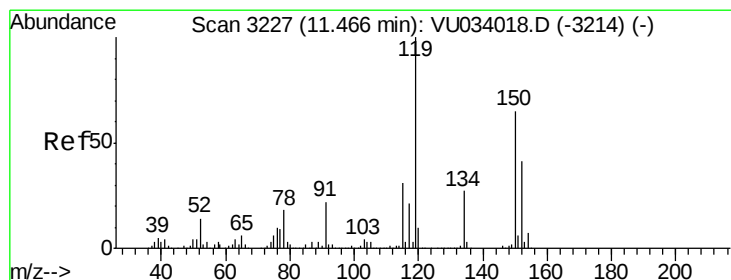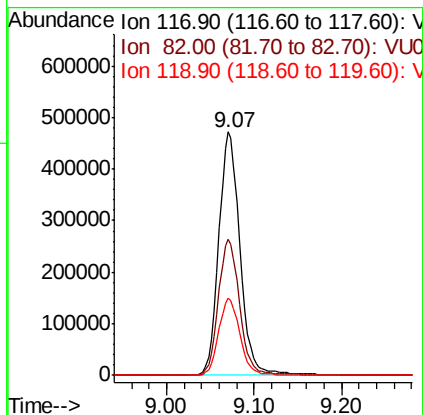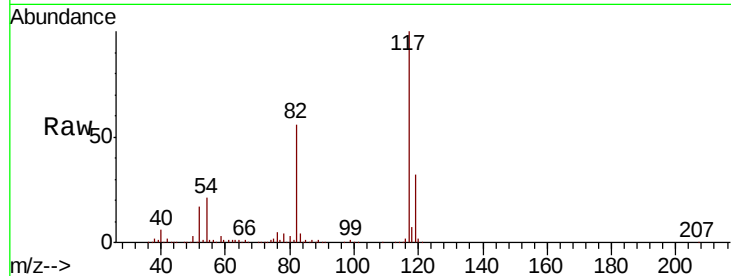

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.47 min Scan# 3227
Delta R.T. 0.00 min
Lab File: VU034108.D
Acq: 30 Aug 2019 19:00

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.3	41.1	123.3
150	158.0	0.0	348.8

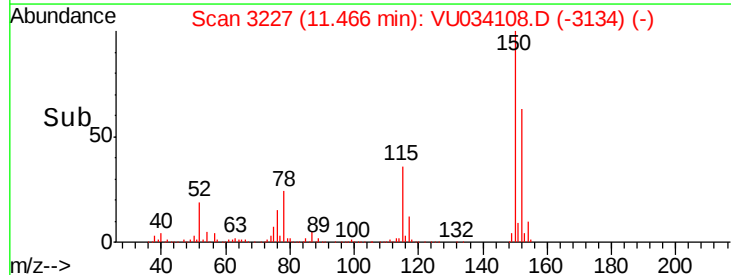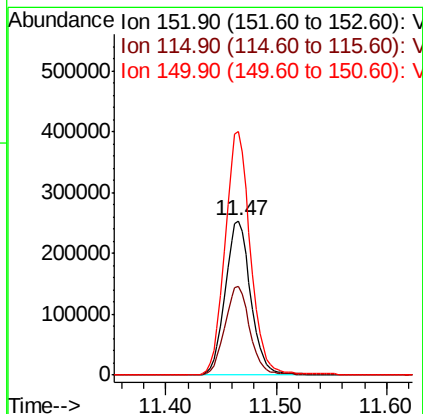

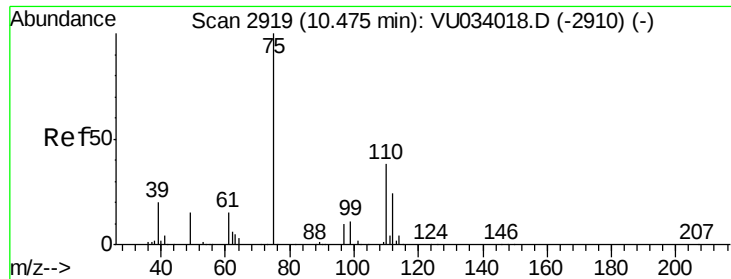

#76

1,2,3-Trichloropropane

Concen: 19.923 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.19 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00

Instrument :

MSVOA_U

ClientSampled :


T9-12-13-T2-(1.9)

Tgt Ion: 75 Resp: 182406

Ion Ratio Lower Upper




75 100

77 1.0 20.1 60.2#

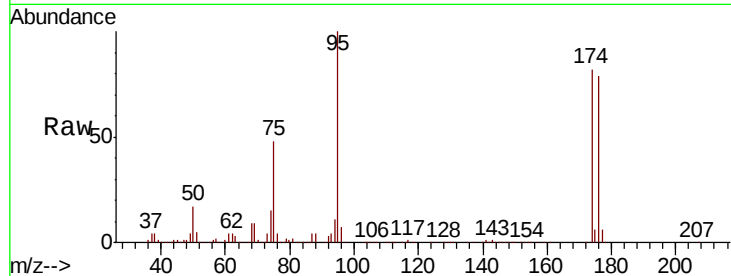

Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

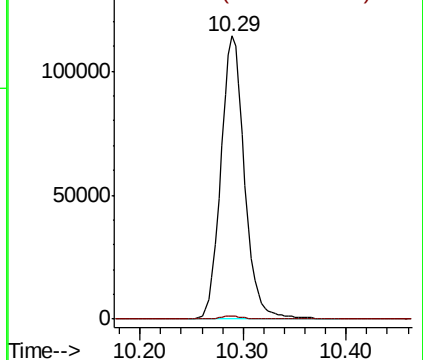

#81

trans-1,4-Dichloro-2-butene

Concen: 67.085 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.21 min

Lab File: VU034108.D

Acq: 30 Aug 2019 19:00


Tgt Ion: 75 Resp: 182406

Ion Ratio Lower Upper

75 100

53 0.1 0.0 0.0#



89 0.0 0.0 0.0




Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 53.00 (52.70 to 53.70): VU0

Ion 88.90 (88.60 to 89.60): VU0



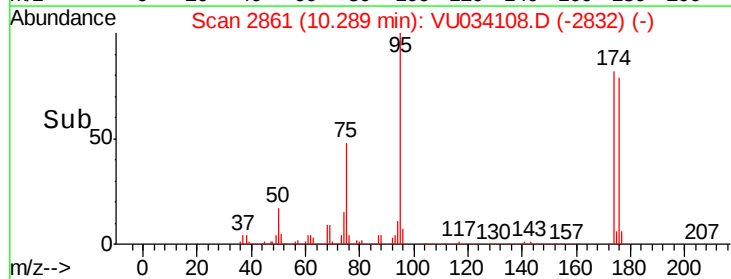
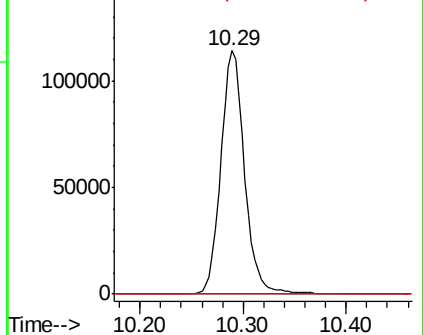


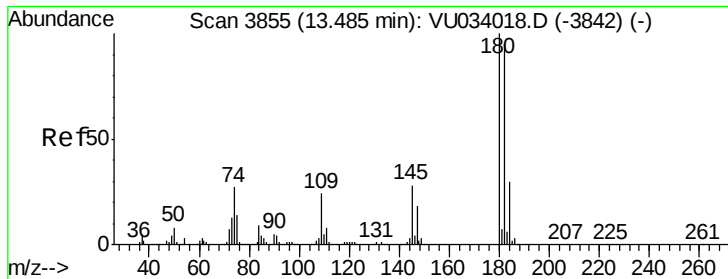

#93
 1,2,4-Trichlorobenzene
 Concen: 1.129 ug/l
 RT: 13.50 min Scan# 3859
 Delta R.T. 0.01 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00

Instrument :
 MSVOA_U
 ClientSampleId :
 T9-12-13-T2-(1.9)

Tgt Ion:180 Resp: 132
 Ion Ratio Lower Upper
 180 100
 182 61.4 47.4 142.2
 145 0.0 14.1 42.3#

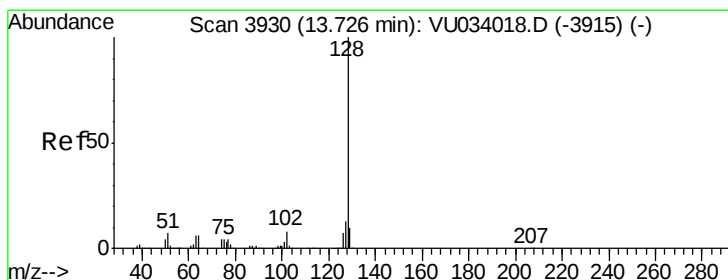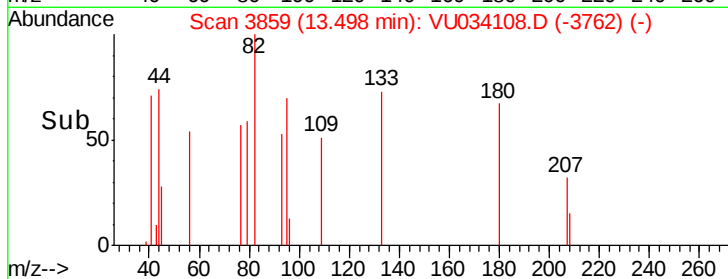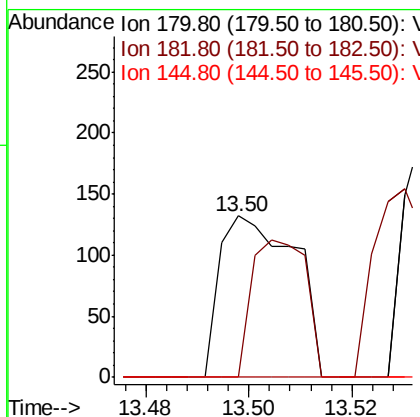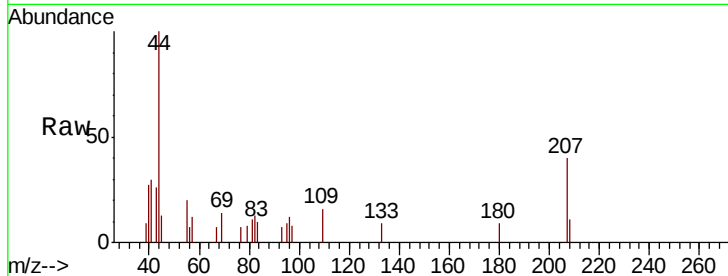

#95
 Naphthalene
 Concen: 1.858 ug/l
 RT: 13.75 min Scan# 3936
 Delta R.T. 0.02 min
 Lab File: VU034108.D
 Acq: 30 Aug 2019 19:00

Tgt Ion:128 Resp: 1796
 Ion Ratio Lower Upper
 128 100
 127 1.1 10.2 15.4#
 129 0.0 8.4 12.6#

