


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU083119\
 Data File : VU034082.D
 Acq On : 30 Aug 2019 08:45
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Title : SW846 8260
 Last Update : Thu Aug 29 04:11:12 2019

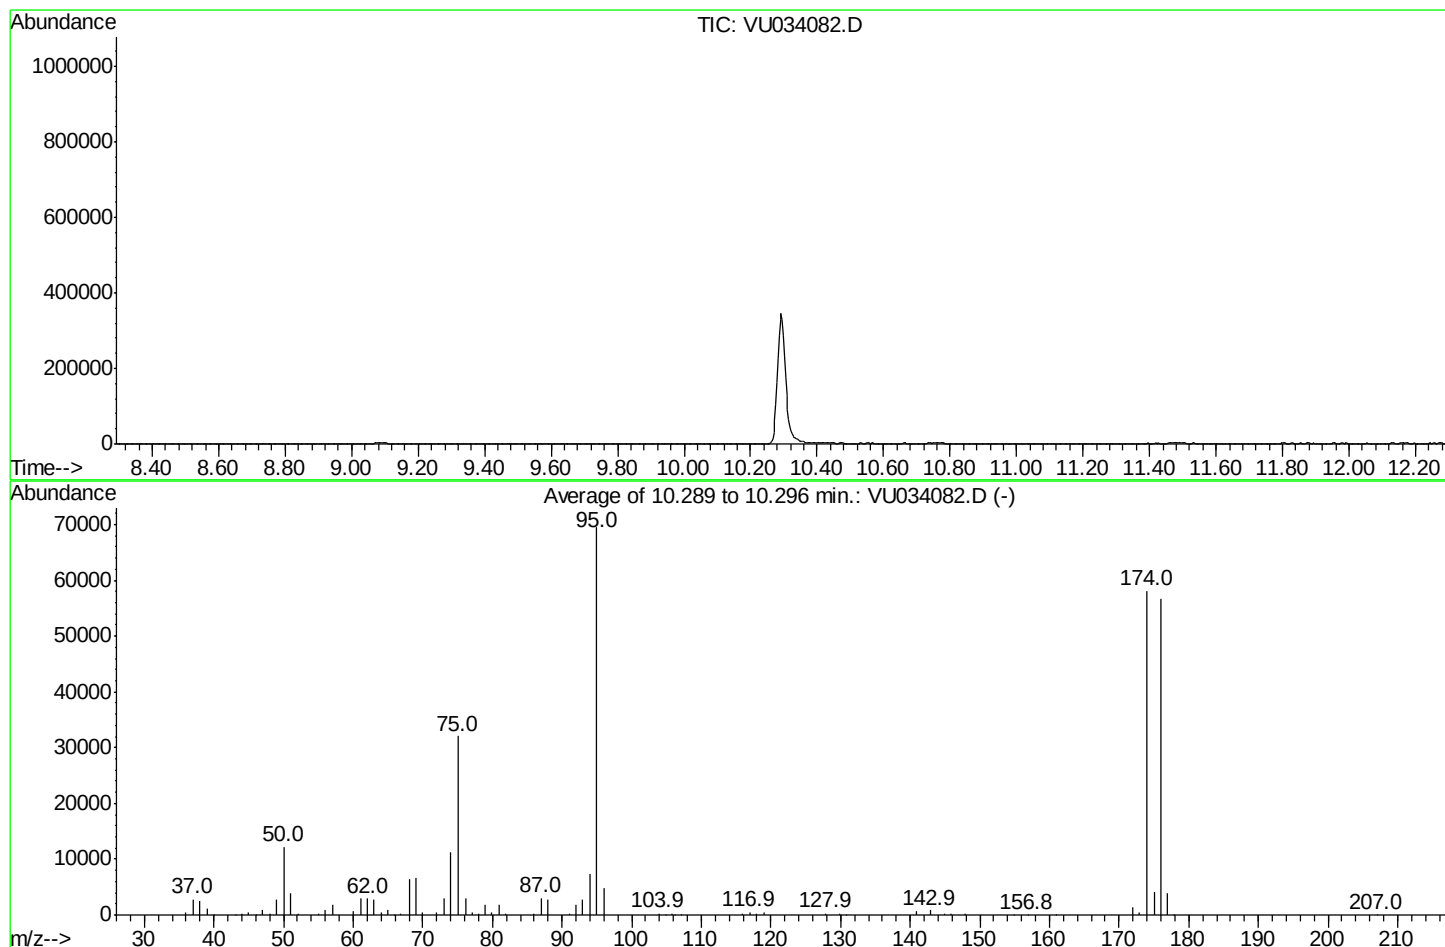

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	12201	PASS
75	95	30	60	46.1	32064	PASS
95	95	100	100	100.0	69506	PASS
96	95	5	9	7.0	4873	PASS
173	174	0.00	2	0.9	499	PASS
174	95	50	100	83.7	58184	PASS
175	174	5	9	7.2	4200	PASS
176	174	95	101	97.5	56709	PASS
177	176	5	9	7.0	3959	PASS