

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
 Data File : VU050700.D
 Acq On : 09 Sep 2022 13:46
 Operator : SY/MD
 Sample : VU0909WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	102	rBV	113467	143238	10.87%	1.473%
2	1.906	167	176	193	rBV	92478	129807	9.85%	1.335%
3	2.562	368	380	397	rBV	245956	403097	30.59%	4.146%
4	2.697	419	422	425	rBV2	542	370	0.03%	0.004%
5	2.732	431	433	435	rBV	316	135	0.01%	0.001%
6	3.044	521	530	539	rBV6	2624	4909	0.37%	0.050%
7	3.186	567	574	579	rBV2	1258	2004	0.15%	0.021%
8	3.456	656	658	660	rBV	221	100	0.01%	0.001%
9	3.530	675	681	685	rBV2	408	384	0.03%	0.004%
10	3.642	713	716	718	rBV2	173	94	0.01%	0.001%
11	3.771	750	756	760	rVB2	399	459	0.03%	0.005%
12	3.793	760	763	770	rBV2	323	421	0.03%	0.004%
13	3.842	775	778	781	rBV2	168	129	0.01%	0.001%
14	3.909	796	799	803	rBV2	239	190	0.01%	0.002%
15	4.064	841	847	850	rBV2	229	228	0.02%	0.002%
16	4.128	864	867	870	rBV	244	162	0.01%	0.002%
17	4.157	873	876	878	rBV2	377	292	0.02%	0.003%
18	4.398	949	951	952	rBV	133	63	0.00%	0.001%
19	4.620	1008	1020	1070	rBV	132140	356294	27.04%	3.664%
20	5.060	1142	1157	1185	rBV	241241	544233	41.30%	5.597%
21	5.324	1236	1239	1242	rVB2	375	207	0.02%	0.002%
22	5.459	1279	1281	1285	rVB	194	111	0.01%	0.001%
23	5.514	1295	1298	1301	rBV	155	137	0.01%	0.001%
24	5.639	1334	1337	1341	rVB2	212	162	0.01%	0.002%
25	5.726	1341	1364	1389	rBV2	478218	1317605	100.00%	13.551%
26	6.182	1503	1506	1510	rVB2	305	213	0.02%	0.002%
27	6.250	1513	1527	1550	rBV	380679	735281	55.80%	7.562%
28	6.623	1640	1643	1646	rBV2	284	183	0.01%	0.002%
29	6.690	1649	1664	1691	rBV	307476	614178	46.61%	6.317%
30	7.186	1812	1818	1832	rBV3	1333	2572	0.20%	0.026%
31	7.292	1846	1851	1852	rBV	418	223	0.02%	0.002%
32	7.565	1924	1936	1958	rBV	147398	270553	20.53%	2.783%
33	7.790	2002	2006	2008	rBV2	428	410	0.03%	0.004%
34	7.832	2013	2019	2021	rBV2	303	290	0.02%	0.003%
35	7.899	2026	2040	2066	rBV	549989	975291	74.02%	10.030%
36	8.179	2115	2127	2146	rBV	108360	186474	14.15%	1.918%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
 Data File : VU050700.D
 Acq On : 09 Sep 2022 13:46
 Operator : SY/MD
 Sample : VU0909WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	8.481	2218	2221	2227	rBV3	309	247	0.02%	0.003%
38	8.507	2227	2229	2231	rBV2	259	136	0.01%	0.001%
39	8.542	2239	2240	2241	rBV	178	50	0.00%	0.001%
40	8.555	2241	2244	2249	rVB2	300	258	0.02%	0.003%
41	8.636	2257	2269	2313	rBV5	262048	743742	56.45%	7.649%
42	8.925	2355	2359	2362	rVB	312	252	0.02%	0.003%
43	8.944	2362	2365	2367	rBV2	146	90	0.01%	0.001%
44	8.960	2367	2370	2373	rBV2	368	320	0.02%	0.003%
45	9.060	2399	2401	2403	rBV2	312	182	0.01%	0.002%
46	9.160	2428	2432	2434	rBV2	369	286	0.02%	0.003%
47	9.205	2442	2446	2450	rBV2	297	311	0.02%	0.003%
48	9.417	2499	2512	2549	rBV	533324	920205	69.84%	9.464%
49	10.221	2758	2762	2768	rBV2	373	434	0.03%	0.004%
50	10.340	2795	2799	2800	rBV	269	202	0.02%	0.002%
51	10.478	2839	2842	2844	rBV	288	177	0.01%	0.002%
52	10.758	2916	2929	2949	rBV	481013	796843	60.48%	8.195%
53	10.909	2975	2976	2978	rVB	352	122	0.01%	0.001%
54	11.256	3081	3084	3087	rVB2	354	170	0.01%	0.002%
55	11.562	3176	3179	3181	rBV	272	159	0.01%	0.002%
56	11.812	3245	3257	3278	rBV	439232	723006	54.87%	7.436%
57	12.047	3327	3330	3335	rBV2	302	271	0.02%	0.003%
58	12.131	3354	3356	3362	rBV2	309	204	0.02%	0.002%
59	12.195	3362	3376	3398	rBV	499951	843659	64.03%	8.677%
60	12.484	3462	3466	3469	rBV2	659	534	0.04%	0.005%
61	12.619	3505	3508	3512	rBV2	656	511	0.04%	0.005%
62	12.774	3553	3556	3558	rBV2	533	292	0.02%	0.003%
63	12.954	3610	3612	3614	rBV	319	144	0.01%	0.001%




Sum of corrected areas: 9723306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050700.D
Acq On : 09 Sep 2022 13:46
Operator : SY/MD
Sample : VU0909WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

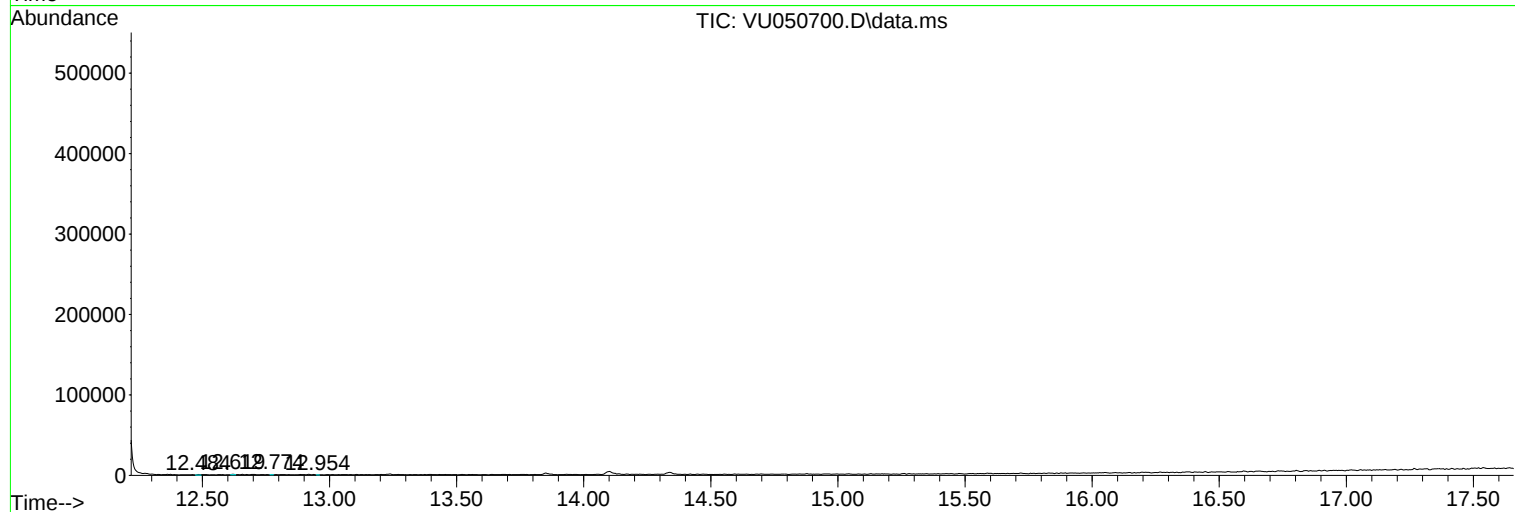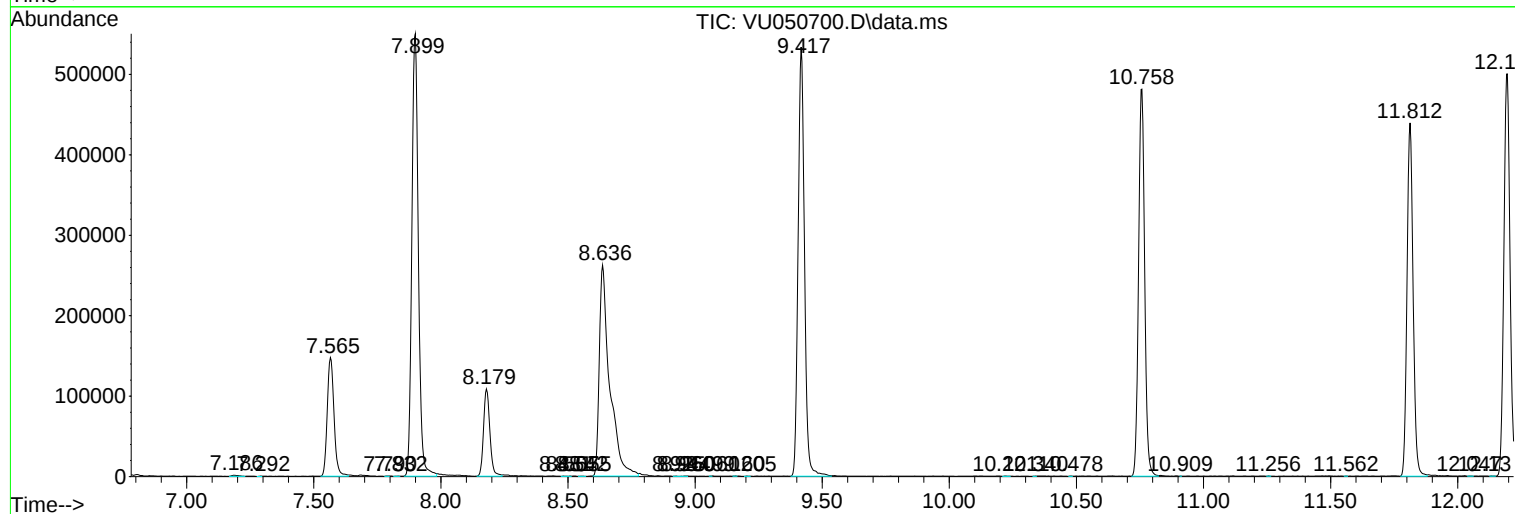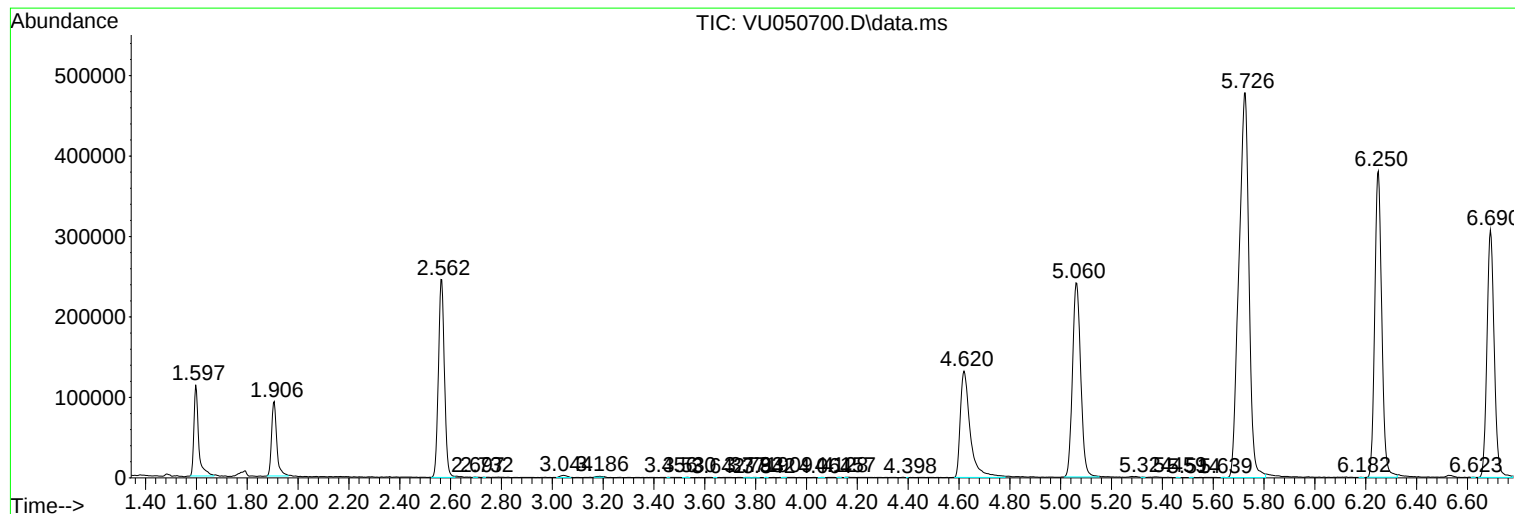

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050700.D
Acq On : 09 Sep 2022 13:46
Operator : SY/MD
Sample : VU0909WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050700.D
Acq On : 09 Sep 2022 13:46
Operator : SY/MD
Sample : VU0909WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK189

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc