

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
 Data File : VU050703.D
 Acq On : 09 Sep 2022 16:41
 Operator : SY/MD
 Sample : N4482-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	105	rBV	150397	199947	13.72%	1.951%
2	1.906	168	176	201	rVB	114114	160318	11.00%	1.564%
3	2.565	368	381	398	rBV	311375	509442	34.96%	4.971%
4	2.848	466	469	474	rVB2	271	193	0.01%	0.002%
5	2.909	482	488	492	rBV2	364	503	0.03%	0.005%
6	2.941	496	498	501	rBV	267	83	0.01%	0.001%
7	3.044	521	530	540	rBV3	2194	3414	0.23%	0.033%
8	3.244	589	592	602	rVB2	274	415	0.03%	0.004%
9	3.289	602	606	608	rBV	212	133	0.01%	0.001%
10	3.494	668	670	675	rVB2	260	158	0.01%	0.002%
11	3.546	683	686	695	rVB2	178	161	0.01%	0.002%
12	3.642	713	716	718	rBV	257	200	0.01%	0.002%
13	3.710	735	737	739	rBV	154	90	0.01%	0.001%
14	3.771	753	756	758	rBV	161	115	0.01%	0.001%
15	3.867	783	786	787	rBV	148	83	0.01%	0.001%
16	3.977	815	820	823	rBV2	172	140	0.01%	0.001%
17	4.089	852	855	857	rBV2	101	57	0.00%	0.001%
18	4.121	862	865	867	rBV2	164	124	0.01%	0.001%
19	4.234	897	900	905	rBV2	248	232	0.02%	0.002%
20	4.276	908	913	917	rBV2	306	274	0.02%	0.003%
21	4.324	923	928	930	rBV2	193	156	0.01%	0.002%
22	4.340	930	933	936	rVB2	215	141	0.01%	0.001%
23	4.440	961	964	965	rBV2	174	109	0.01%	0.001%
24	4.623	1009	1021	1060	rBV2	116989	322260	22.12%	3.145%
25	4.999	1135	1138	1141	rBV2	334	238	0.02%	0.002%
26	5.063	1142	1158	1184	rBV	263253	590702	40.54%	5.764%
27	5.604	1324	1326	1330	rVB	285	176	0.01%	0.002%
28	5.649	1338	1340	1342	rBV	118	63	0.00%	0.001%
29	5.726	1342	1364	1393	rBV2	536013	1457115	100.00%	14.218%
30	6.250	1513	1527	1554	rBV	390250	755808	51.87%	7.375%
31	6.526	1606	1613	1624	rBV8	2630	5107	0.35%	0.050%
32	6.616	1637	1641	1643	rBV2	411	301	0.02%	0.003%
33	6.690	1649	1664	1695	rBV	330618	658290	45.18%	6.424%
34	6.893	1723	1727	1729	rBV2	407	253	0.02%	0.002%
35	6.925	1734	1737	1739	rBV2	315	188	0.01%	0.002%
36	6.967	1747	1750	1753	rBV	207	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
 Data File : VU050703.D
 Acq On : 09 Sep 2022 16:41
 Operator : SY/MD
 Sample : N4482-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	7.025	1764	1768	1770	rVB2	224	140	0.01%	0.001%
38	7.044	1772	1774	1776	rBV	176	75	0.01%	0.001%
39	7.185	1812	1818	1824	rBV3	953	1282	0.09%	0.013%
40	7.330	1860	1863	1864	rBV	228	116	0.01%	0.001%
41	7.449	1897	1900	1902	rBV	186	119	0.01%	0.001%
42	7.565	1922	1936	1960	rBV	164265	299267	20.54%	2.920%
43	7.793	2005	2007	2008	rBV	166	59	0.00%	0.001%
44	7.816	2013	2014	2016	rBV	304	92	0.01%	0.001%
45	7.899	2026	2040	2071	rBV	629905	1120447	76.89%	10.933%
46	8.179	2116	2127	2149	rBV	113526	199098	13.66%	1.943%
47	8.584	2249	2253	2256	rBV2	323	281	0.02%	0.003%
48	8.639	2256	2270	2323	rVV8	228126	697753	47.89%	6.809%
49	8.935	2360	2362	2364	rBV2	261	130	0.01%	0.001%
50	9.359	2491	2494	2498	rBV2	283	234	0.02%	0.002%
51	9.417	2499	2512	2531	rBV	533649	920350	63.16%	8.981%
52	10.758	2916	2929	2954	rBV	468210	772543	53.02%	7.538%
53	10.896	2969	2972	2974	rBV	250	153	0.01%	0.001%
54	10.935	2982	2984	2987	rBV	373	232	0.02%	0.002%
55	11.250	3079	3082	3084	rBV	346	247	0.02%	0.002%
56	11.571	3179	3182	3183	rBV	271	148	0.01%	0.001%
57	11.812	3245	3257	3274	rBV	430348	710536	48.76%	6.933%
58	11.996	3311	3314	3316	rBV2	498	314	0.02%	0.003%
59	12.195	3363	3376	3400	rBV	523536	856682	58.79%	8.359%
60	12.713	3535	3537	3540	rBV2	432	214	0.01%	0.002%
61	13.060	3642	3645	3649	rBV3	409	393	0.03%	0.004%




Sum of corrected areas: 10248047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050703.D
Acq On : 09 Sep 2022 16:41
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

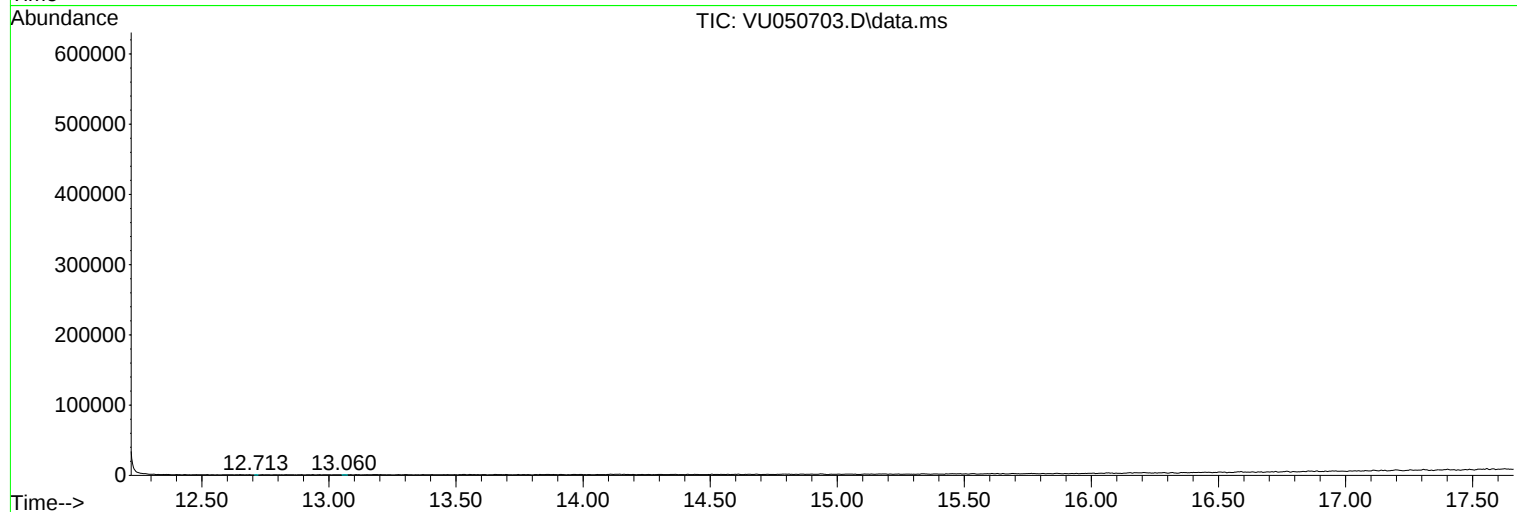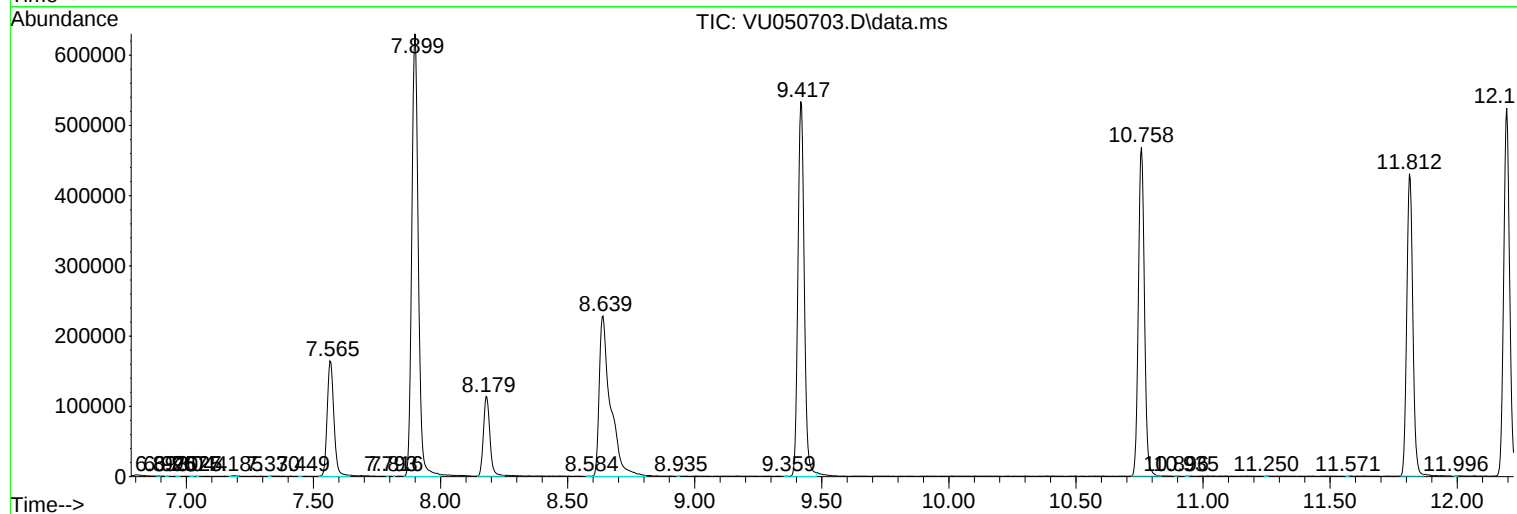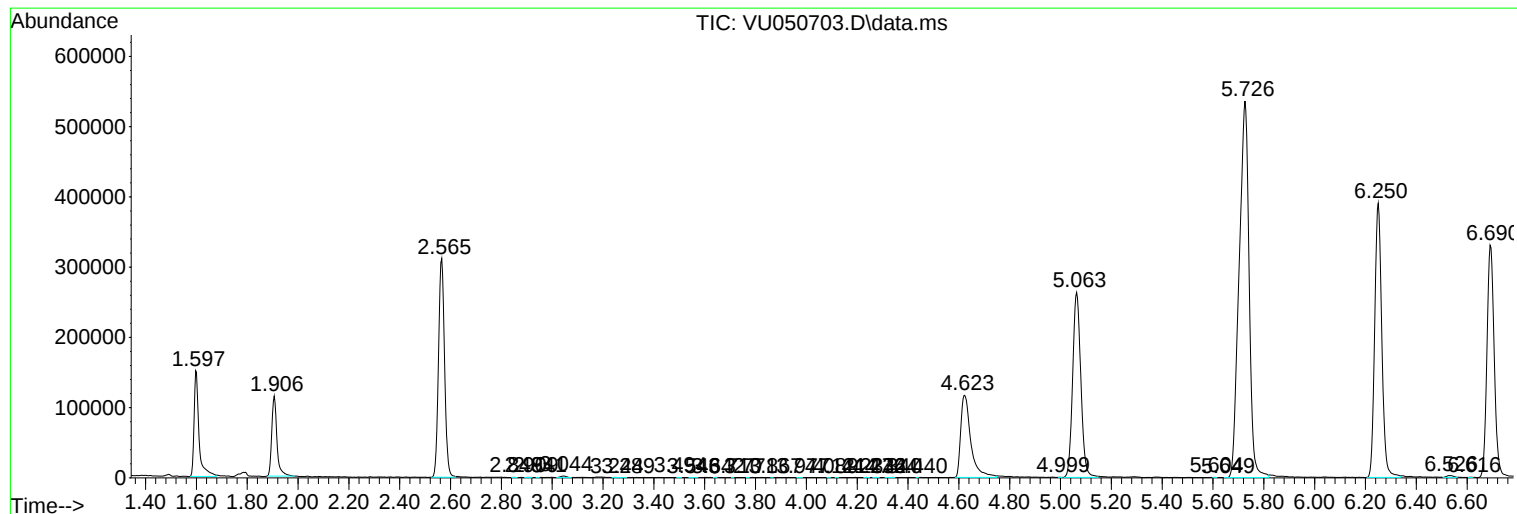

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050703.D
Acq On : 09 Sep 2022 16:41
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
Data File : VU050703.D
Acq On : 09 Sep 2022 16:41
Operator : SY/MD
Sample : N4482-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------