
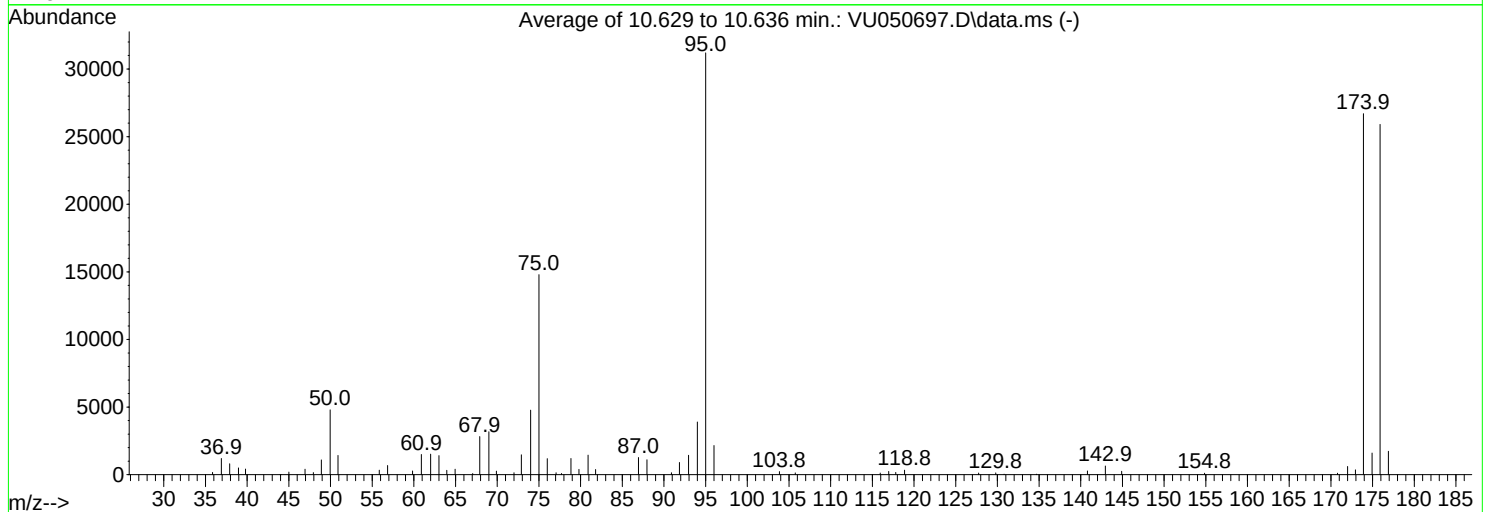


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090922\
 Data File : VU050697.D
 Acq On : 09 Sep 2022 11:08
 Operator : SY/MD
 Sample : BFB123
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB123

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 10 01:20:12 2022

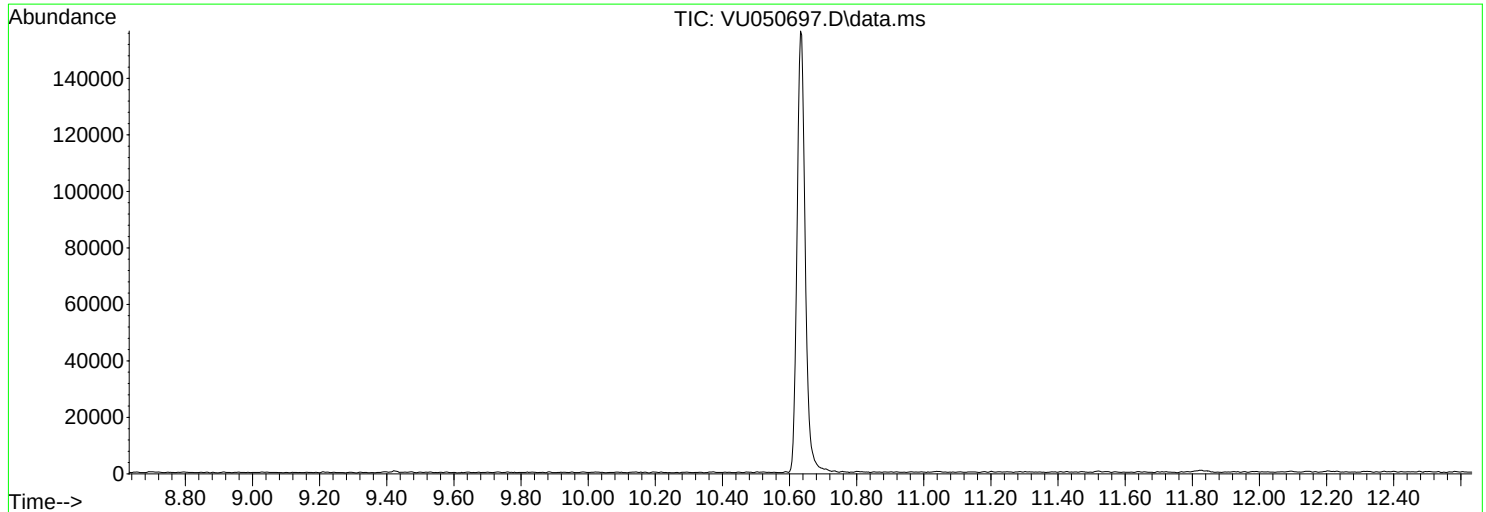

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	4794	PASS
75	95	30	80	47.4	14792	PASS
95	95	100	100	100.0	31197	PASS
96	95	5	9	6.9	2152	PASS
173	174	0.00	2	1.3	354	PASS
174	95	50	120	85.6	26704	PASS
175	174	5	9	6.0	1602	PASS
176	174	95	101	97.0	25907	PASS
177	176	5	9	6.7	1724	PASS

Scan 2878 (10.594 min): VU050697.D\data.ms
BFB123

m/z	Abundance
40.00	162.0
43.90	439.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.80	158.0
36.90	1251.0
37.90	805.0
39.00	472.0
39.80	582.0
44.00	448.0
45.00	198.0
46.90	312.0
48.00	132.0
48.90	1085.0
50.00	4966.0
50.90	1396.0
55.90	273.0
56.90	727.0
59.80	246.0
60.90	1327.0
62.00	1331.0
63.00	1369.0
63.90	252.0
64.90	320.0
67.00	132.0
67.90	2679.0
69.00	2841.0
69.90	238.0
72.00	135.0
72.90	1457.0
74.00	4555.0
75.00	14279.0
76.00	1254.0
77.00	124.0
77.70	145.0
78.80	1129.0
79.80	382.0
80.90	1382.0
81.80	288.0
87.00	1197.0
87.90	1137.0
90.90	134.0
91.80	841.0
92.90	1282.0
94.00	3575.0
95.00	29704.0
96.00	2018.0
103.80	186.0
105.80	113.0
115.90	110.0
116.90	235.0
117.80	173.0
118.90	300.0
127.80	105.0
129.80	123.0
130.80	118.0
140.80	243.0
142.90	653.0
144.90	241.0
154.90	105.0
172.00	578.0
173.00	323.0
173.90	25352.0
174.90	1550.0
175.90	24512.0
176.90	1457.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.90	170.0
36.90	1245.0
37.90	824.0
38.90	510.0
39.80	635.0
44.00	456.0
45.00	191.0
47.00	441.0
48.00	174.0
48.90	1117.0
49.90	4906.0
50.90	1458.0
55.90	334.0
56.90	710.0
59.90	275.0
60.90	1546.0
62.00	1601.0
63.00	1486.0
64.00	334.0
65.00	409.0
67.10	131.0
67.90	2867.0
69.00	3252.0
69.90	267.0
72.00	140.0
72.90	1483.0
74.00	4862.0
75.00	15187.0
76.00	1182.0
77.10	160.0
77.70	111.0
78.90	1220.0
79.80	404.0
80.90	1520.0
81.80	394.0
86.90	1257.0
87.90	1147.0
90.90	160.0
91.90	942.0
92.90	1484.0
94.00	3985.0
95.00	31952.0
96.00	2239.0
103.90	246.0
105.70	146.0
116.00	116.0
116.90	241.0
117.80	170.0
118.80	333.0
127.70	121.0
129.80	118.0
140.80	277.0
143.00	653.0
144.90	260.0
154.80	107.0
170.80	151.0
172.00	610.0
172.90	361.0
173.90	27616.0
174.90	1603.0
175.90	26656.0
176.90	1787.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.90	175.0
36.90	1100.0
37.90	803.0
38.90	520.0
39.80	525.0
44.00	428.0
45.00	178.0
47.00	450.0
47.90	163.0
48.90	1056.0
49.90	4511.0
50.90	1393.0
55.80	379.0
56.80	599.0
59.90	314.0
60.90	1585.0
62.00	1604.0
63.00	1383.0
64.00	388.0
65.00	489.0
67.90	2912.0
69.00	3408.0
69.90	290.0
72.00	144.0
72.90	1447.0
74.00	4905.0
75.00	14909.0
76.00	1129.0
77.10	139.0
78.90	1251.0
79.80	396.0
80.90	1436.0
81.80	444.0
86.90	1354.0
88.00	1032.0
90.90	142.0
91.90	900.0
93.00	1526.0
94.00	4108.0
95.00	31936.0
96.00	2199.0
103.90	234.0
105.70	144.0
116.00	115.0
117.00	233.0
117.80	156.0
118.80	349.0
127.70	128.0
129.80	142.0
134.70	106.0
140.80	293.0
143.00	596.0
144.90	254.0
154.80	104.0
170.80	165.0
172.00	612.0
172.90	377.0
173.90	27144.0
175.00	1653.0
175.90	26552.0
176.90	1927.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123