

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
 Data File : VU063580.D
 Acq On : 15 Sep 2025 15:44
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Quant Time: Sep 16 05:51:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Sep 16 05:42:14 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.097	96	33411	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.628	95	11435	0.919	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	12678	0.999	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.000%	
Target Compounds						
						Qvalue
3) Chloromethane	1.519	50	805	0.075	ug/l	99
4) Vinyl Chloride	1.596	62	119904	10.250	ug/l	99
5) Bromomethane	1.847	94	681	0.094	ug/l	97
7) Trichlorofluoromethane	2.130	101	1313	0.076	ug/l	94
9) 1,1-Dichloroethene	2.570	96	41246	4.737	ug/l	99
10) Iodomethane	2.712	142	908	0.072	ug/l #	72
11) Allyl Chloride	2.901	41	224	0.015	ug/l #	1
12) Acrylonitrile	3.551	53	20	0.008	ug/l #	18
14) Carbon Disulfide	2.779	76	405	0.022	ug/l #	1
15) Methylene Chloride	3.030	84	107748	9.366	ug/l	97
16) trans-1,2-Dichloroethene	3.339	96	96272	10.377	ug/l	93
17) 1,1-Dichloroethane	3.853	63	1027	0.048	ug/l #	85
18) 2-Butanone	4.705	43	319	0.075	ug/l	78
19) Cyclohexane	5.345	56	75	0.004	ug/l #	1
20) Methylcyclohexane	6.779	83	824	0.053	ug/l #	31
21) 2,2-Dichloropropane	4.644	77	675	0.043	ug/l #	1
22) cis-1,2-Dichloroethene	4.647	96	43008	3.776	ug/l	89
23) Diethyl Ether	2.374	59	190	0.025	ug/l #	26
25) Methyl tert-Butyl Ether	3.358	73	1418	0.055	ug/l	99
26) Bromochloromethane	4.966	128	376	0.082	ug/l #	25
27) Chloroform	5.078	83	670	0.032	ug/l	86
28) 1,1,1-Trichloroethane	5.297	97	227793	13.935	ug/l	99
29) 1,1-Dichloropropene	5.509	75	2895	0.191	ug/l #	69
30) Carbon Tetrachloride	5.503	117	21029	1.747	ug/l	97
31) Isopropyl Ether	3.982	45	142	0.004	ug/l	65
32) Ethyl-t-butyl ether	4.496	59	44	0.001	ug/l #	36
33) Tert-Amyl methyl ether	5.834	73	162	0.006	ug/l #	58
35) Benzene	5.757	78	411096	9.402	ug/l	97
36) 1,2-Dichloroethane	5.782	62	135709	9.198	ug/l	99
37) Trichloroethene	6.528	130	106354	9.772	ug/l	98
38) 1,2-Dichloropropane	6.779	63	165721	14.306	ug/l	100
39) Methacrylonitrile	4.982	41	134	0.029	ug/l #	1
40) Methyl acrylate	4.847	55	42	0.007	ug/l #	1
41) Tetrahydrofuran	5.049	42	489	0.200	ug/l #	39
42) 1-Chlorobutane	5.438	56	110	0.005	ug/l #	1
43) Dibromomethane	6.904	93	1003	0.181	ug/l #	52
45) 4-Methyl-2-Pentanone	7.801	43	994	0.143	ug/l #	76
46) t-1,4-Dichloro-2-butene	10.814	75	409	0.157	ug/l #	21
47) Methyl methacrylate	6.978	69	66	0.013	ug/l #	7
48) Ethyl methacrylate	8.342	69	108	0.012	ug/l #	1
49) Toluene	7.956	92	48001	2.023	ug/l	97
50) t-1,3-Dichloropropene	8.207	75	1359	0.153	ug/l	89
51) cis-1,3-Dichloropropene	7.599	75	2632	0.223	ug/l	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
 Data File : VU063580.D
 Acq On : 15 Sep 2025 15:44
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Quant Time: Sep 16 05:51:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Sep 16 05:42:14 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
52) 1,1,2-Trichloroethane	8.390	97	114914	14.618	ug/l	97
53) 1,3-Dichloropropane	8.570	76	703	0.051	ug/l	90
54) 2-Hexanone	8.699	43	912	0.179	ug/l #	49
58) Tetrachloroethene	8.538	164	101804	9.498	ug/l	96
59) Chlorobenzene	9.438	112	446307	16.323	ug/l	99
60) 1,1,1,2-Tetrachloroethane	9.528	131	811	0.091	ug/l	97
61) Pentachloroethane	11.412	117	80	0.012	ug/l #	10
63) Ethyl Benzene	9.560	91	691760	14.817	ug/l	98
64) m/p-Xylenes	9.686	106	209151	11.658	ug/l	100
65) o-Xylene	10.091	106	209563	11.670	ug/l	98
66) Styrene	10.107	104	73010	2.547	ug/l #	58
69) Isopropylbenzene	10.477	105	7707	0.177	ug/l	98
70) 1,1,2,2-Tetrachloroethane	10.776	83	198	0.020	ug/l #	51
71) 1,2,3-Trichloropropane	10.814	75	409	0.055	ug/l #	43
72) Bromobenzene	10.779	156	911	0.081	ug/l	90
73) n-propylbenzene	10.898	120	4511	0.358	ug/l	89
74) 2-Chlorotoluene	10.978	126	625	0.055	ug/l	44
75) 1,3,5-Trimethylbenzene	11.081	105	3839	0.094	ug/l	95
76) 4-Chlorotoluene	11.094	126	1203	0.101	ug/l	96
77) tert-Butylbenzene	11.412	119	2037	0.052	ug/l	89
78) 1,2,4-Trimethylbenzene	11.467	105	3558	0.090	ug/l	98
79) sec-Butylbenzene	11.634	105	6821	0.128	ug/l	99
81) p-Isopropyltoluene	11.785	119	7641	0.178	ug/l	97
83) 1,4-Dichlorobenzene	11.830	146	140967	6.030	ug/l	99
84) n-Butylbenzene	12.203	91	6322	0.157	ug/l	97
85) 1,2-Dichlorobenzene	12.203	146	125252	5.706	ug/l	98
87) 1,2,4-Trichlorobenzene	13.833	180	250047	18.812	ug/l	98
88) Hexachlorobutadiene	14.013	225	442	0.053	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063580.D
Acq On : 15 Sep 2025 15:44
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Time: Sep 16 05:51:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Sep 16 05:42:14 2025
Response via : Initial Calibration




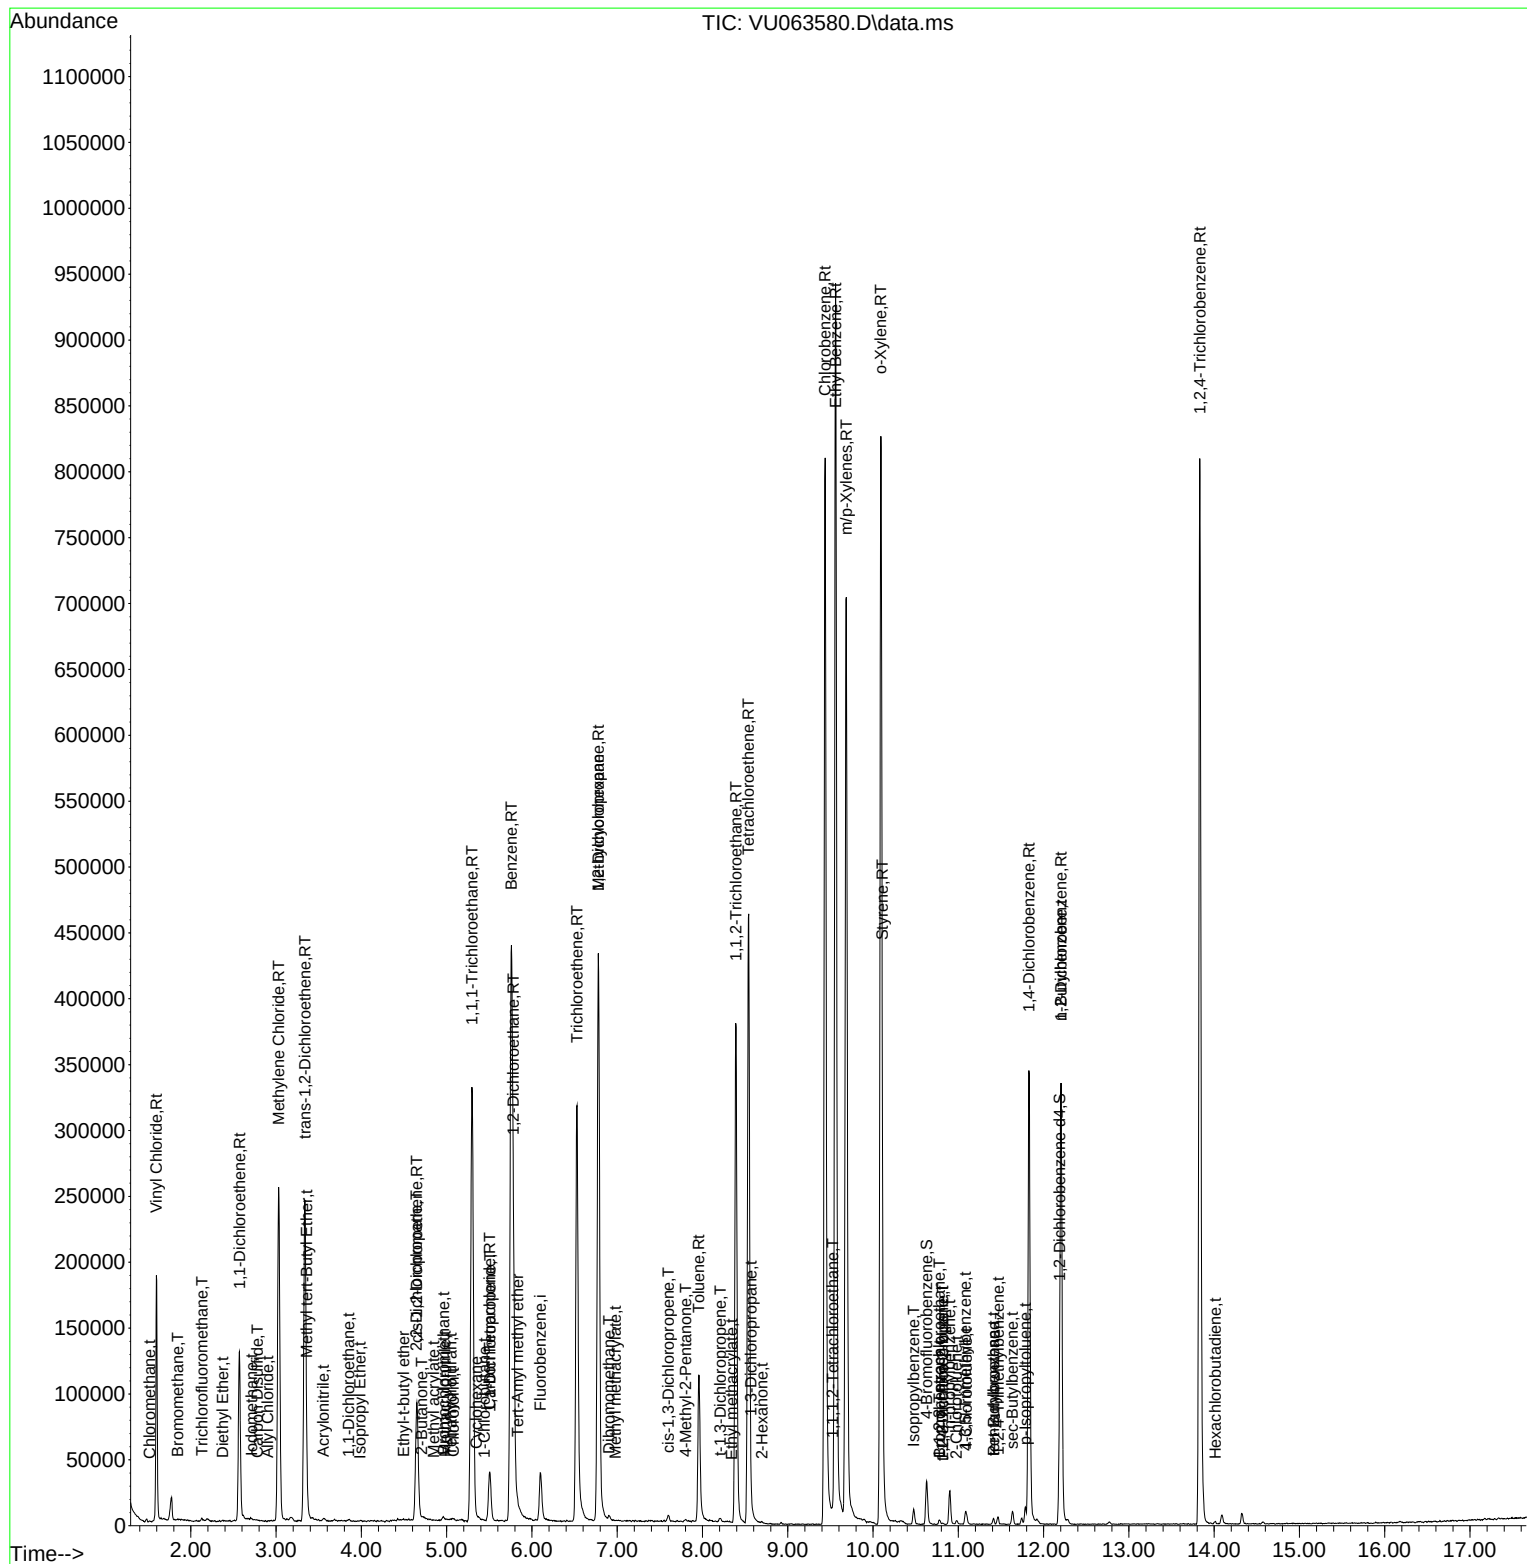




#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.097 min Scan# 1496
Delta R.T. -0.003 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 96	Resp: 33411
Ion Ratio	Lower Upper
96 100	
70 20.4	15.5 23.3
95 8.3	7.7 11.5
97 0.0	0.0 0.0

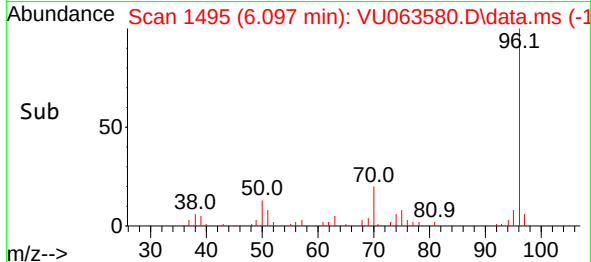

#3
Chloromethane
Concen: 0.075 ug/l
RT: 1.519 min Scan# 71
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 50	Resp: 805
Ion Ratio	Lower Upper
50 100	
52 32.4	25.6 38.4




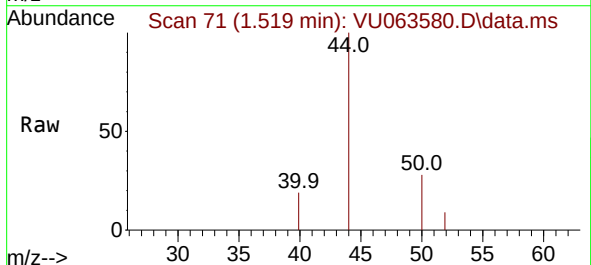


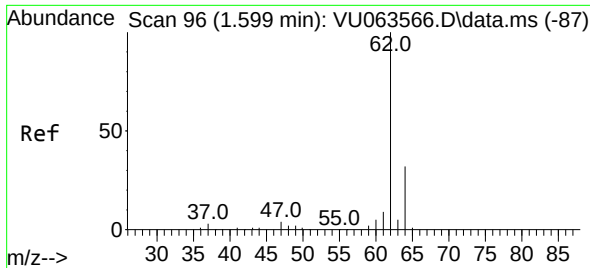

#4
 Vinyl Chloride
 Concen: 10.250 ug/l
 RT: 1.596 min Scan# 91
 Delta R.T. -0.003 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44




Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS


Tgt Ion: 62 Resp: 119904
 Ion Ratio Lower Upper
 62 100
 64 31.5 25.5 38.3

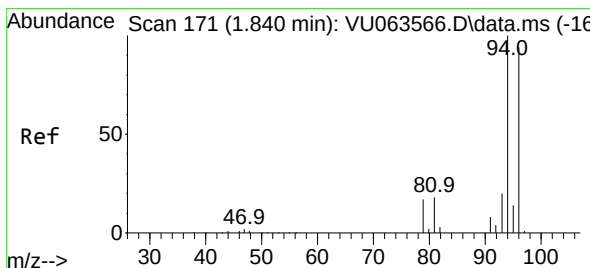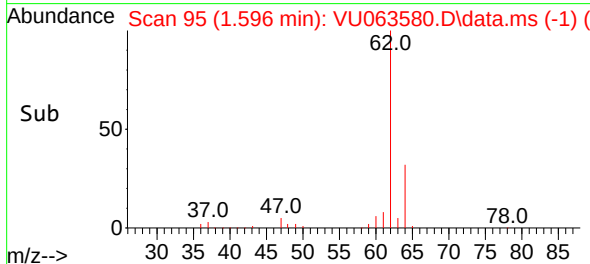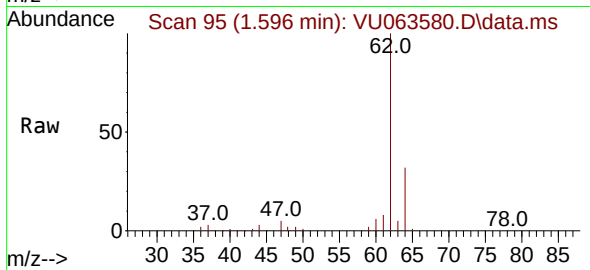

#5
 Bromomethane
 Concen: 0.094 ug/l
 RT: 1.847 min Scan# 173
 Delta R.T. 0.007 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44

Tgt Ion: 94 Resp: 681
 Ion Ratio Lower Upper
 94 100
 96 90.8 75.1 112.7


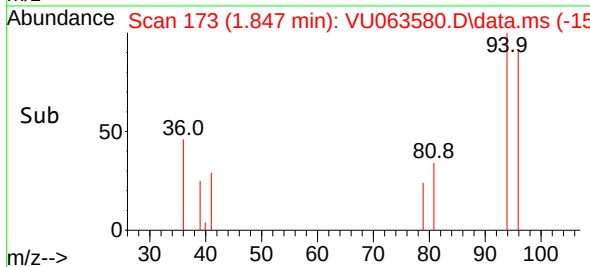

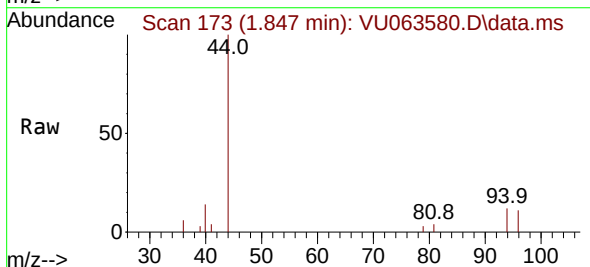




#7
 Trichlorofluoromethane
 Concen: 0.076 ug/l
 RT: 2.130 min Scan# 2
 Delta R.T. 0.004 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44




Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS


Tgt Ion:101 Resp: 1313
 Ion Ratio Lower Upper
 101 100
 103 58.7 50.8 76.2



#9
 1,1-Dichloroethene
 Concen: 4.737 ug/l
 RT: 2.570 min Scan# 398
 Delta R.T. 0.004 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44

Tgt Ion: 96 Resp: 41246
 Ion Ratio Lower Upper
 96 100
 61 182.9 0.0 543.9
 98 64.4 0.0 125.8









#10
Iodomethane
Concen: 0.072 ug/l
RT: 2.712 min Scan# 441
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:142 Resp: 908
Ion Ratio Lower Upper
142 100
127 29.2 38.6 58.0#

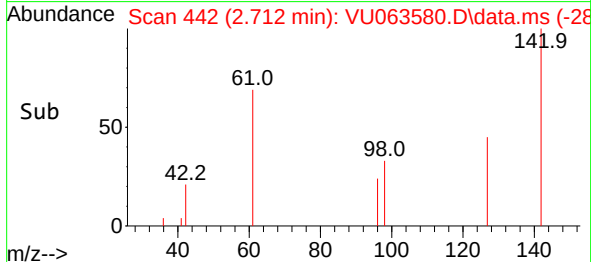

#11
Allyl Chloride
Concen: 0.015 ug/l
RT: 2.901 min Scan# 501
Delta R.T. -0.009 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 41 Resp: 224
Ion Ratio Lower Upper
41 100
39 183.0 61.2 91.8#

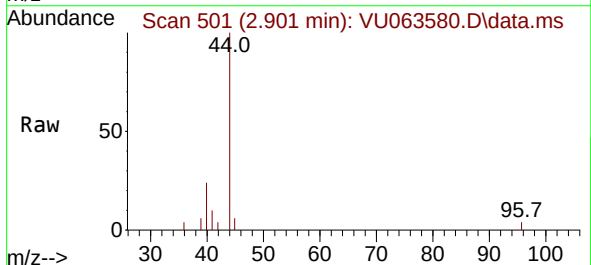



#12

Acrylonitrile

Concen: 0.008 ug/l

RT: 3.551 min Scan# 70

Delta R.T. 0.248 min

Lab File: VU063580.D


Acq: 15 Sep 2025 15:44

Instrument :




MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS



Tgt Ion:	53	Resp:	20
Ion	Ratio	Lower	Upper
53	100		
52	0.0	65.0	97.4#
51	0.0	31.2	46.8#

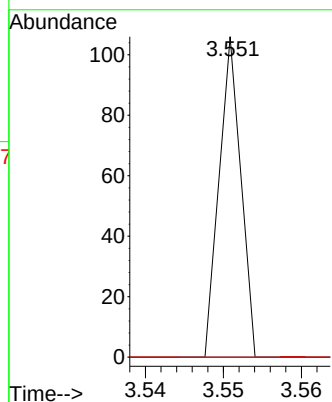

#14

Carbon Disulfide

Concen: 0.022 ug/l




RT: 2.779 min Scan# 463


Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Tgt Ion:	76	Resp:	405
Ion	Ratio	Lower	Upper
76	100		
78	49.2	7.3	10.9#


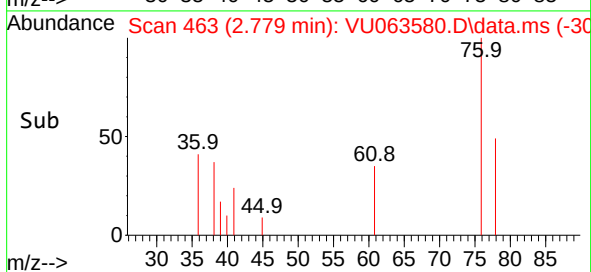
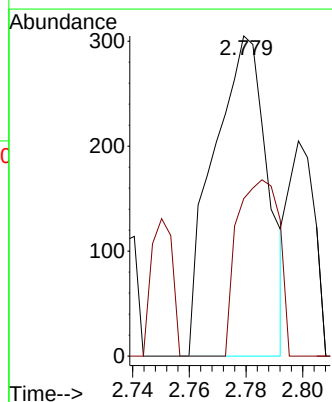





#15
Methylene Chloride
Concen: 9.366 ug/l
RT: 3.030 min Scan# 541
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:	84	Resp:	107748
Ion	Ratio	Lower	Upper
84	100		
49	144.1	111.8	167.6
51	44.3	0.0	86.0
86	64.5	50.8	76.2



#16
trans-1,2-Dichloroethene
Concen: 10.377 ug/l
RT: 3.339 min Scan# 637
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:	96	Resp:	96272
Ion	Ratio	Lower	Upper
96	100		
61	150.5	127.8	191.6
98	62.7	53.8	80.8





#17

1,1-Dichloroethane

Concen: 0.048 ug/l

RT: 3.853 min Scan# 796

Delta R.T. 0.004 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion: 63 Resp: 1027

Ion Ratio Lower Upper

63 100

98 0.0 2.9 8.8#

100 0.0 2.0 5.8#

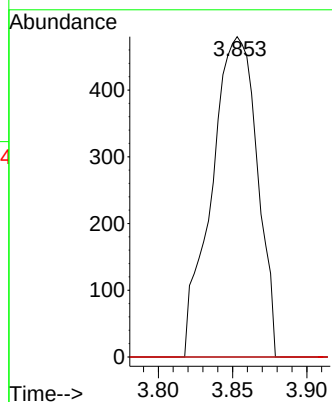

#18

2-Butanone

Concen: 0.075 ug/l

RT: 4.705 min Scan# 1062

Delta R.T. -0.003 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 43 Resp: 319

Ion Ratio Lower Upper

43 100

57 0.0 0.0 15.8

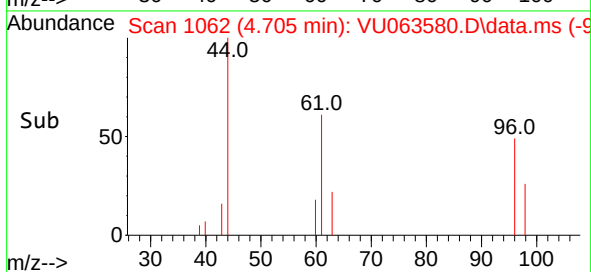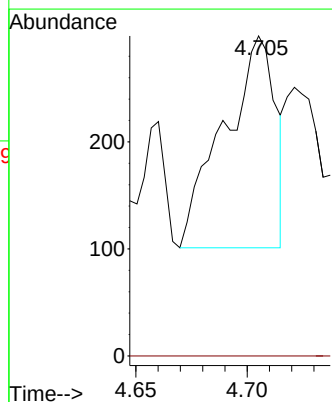



#19

Cyclohexane

Concen: 0.004 ug/l

RT: 5.345 min Scan# 1

Delta R.T. -0.016 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44





Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS

Tgt Ion:	56	Resp:	75
Ion	Ratio	Lower	Upper
56	100		
69	0.0	22.7	34.1#
84	5728.0	59.4	89.0#

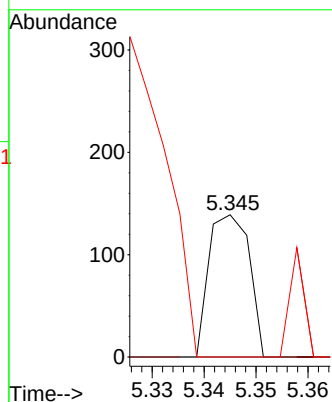

#20

Methylcyclohexane

Concen: 0.053 ug/l




RT: 6.779 min Scan# 1707


Delta R.T. 0.039 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Tgt Ion:	83	Resp:	824
Ion	Ratio	Lower	Upper
83	100		
55	14.1	66.7	100.1#
98	80.5	35.9	53.9#


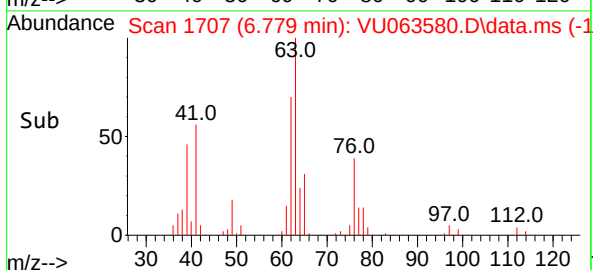






#21
2,2-Dichloropropane
Concen: 0.043 ug/l
RT: 4.644 min Scan# 1043
Delta R.T. -0.003 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 77 Resp: 675
Ion Ratio Lower Upper
77 100
97 220.0 17.5 26.3#

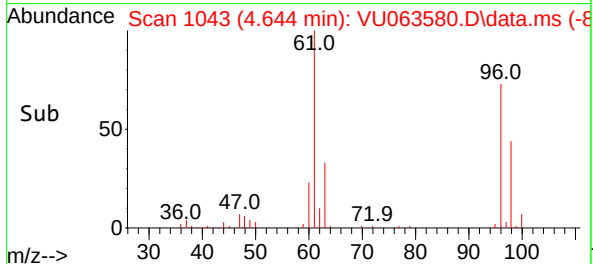

#22
cis-1,2-Dichloroethene
Concen: 3.776 ug/l
RT: 4.647 min Scan# 1044
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 96 Resp: 43008
Ion Ratio Lower Upper
96 100
61 144.2 0.0 411.0
98 62.0 31.9 95.9

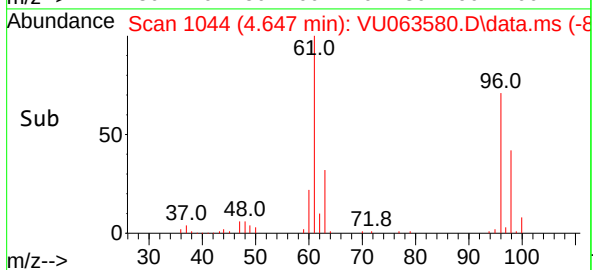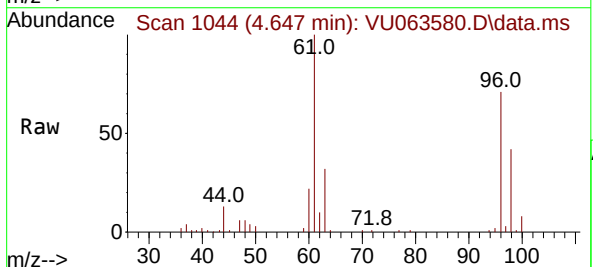



#23

Diethyl Ether

Concen: 0.025 ug/l

RT: 2.374 min Scan# 31

Delta R.T. 0.007 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion: 59 Resp: 190

Ion Ratio Lower Upper

59 100

45 194.7 59.0 88.6#

74 74.2 57.8 86.6

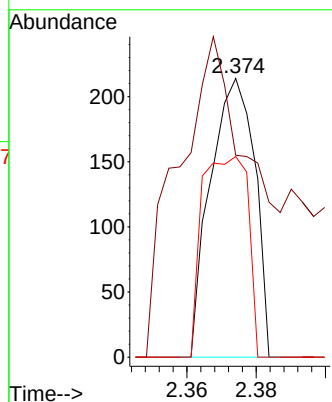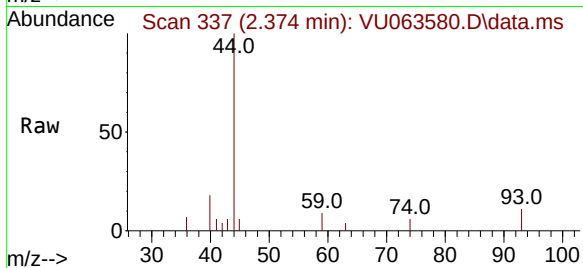

#25

Methyl tert-Butyl Ether

Concen: 0.055 ug/l

RT: 3.358 min Scan# 643

Delta R.T. 0.000 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 73 Resp: 1418

Ion Ratio Lower Upper

73 100

43 23.3 18.1 27.1

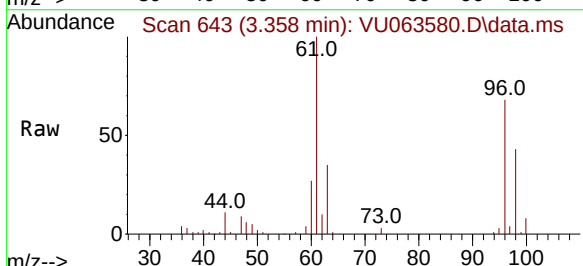



#26

Bromochloromethane

Concen: 0.082 ug/l

RT: 4.966 min Scan# 1140

Delta R.T. 0.010 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion:128 Resp: 376

Ion Ratio Lower Upper

128 100

49 327.9 0.0 410.2

130 206.9 103.4 155.0#

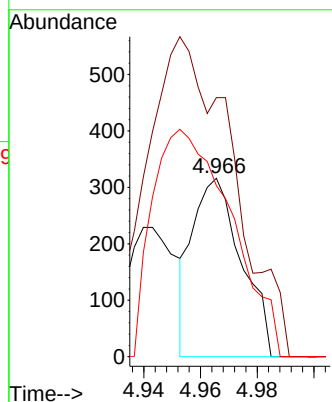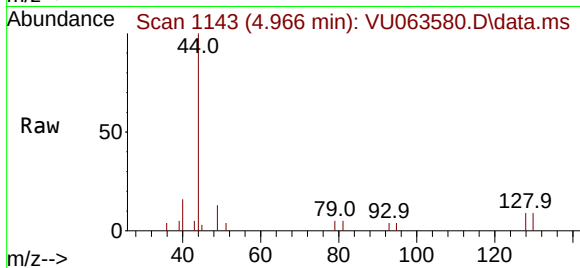

#27

Chloroform

Concen: 0.032 ug/l

RT: 5.078 min Scan# 1178

Delta R.T. 0.007 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 83 Resp: 670

Ion Ratio Lower Upper

83 100

85 53.7 0.0 128.6

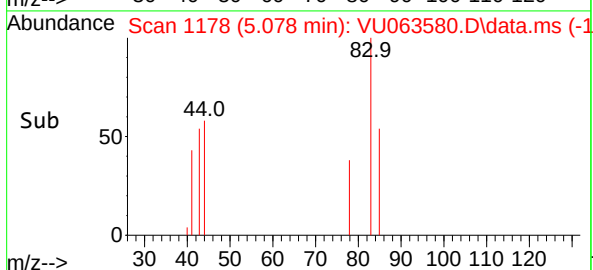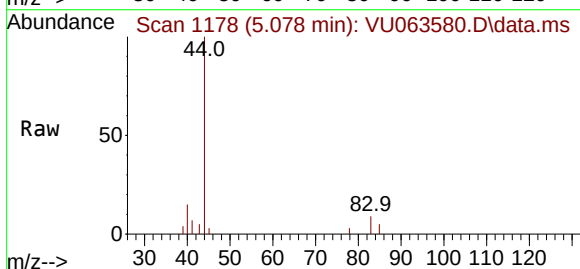



#28

1,1,1-Trichloroethane

Concen: 13.935 ug/l

RT: 5.297 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion: 97 Resp: 227793

Ion Ratio Lower Upper

97 100

99 63.9 32.4 97.0

61 50.4 25.1 75.4

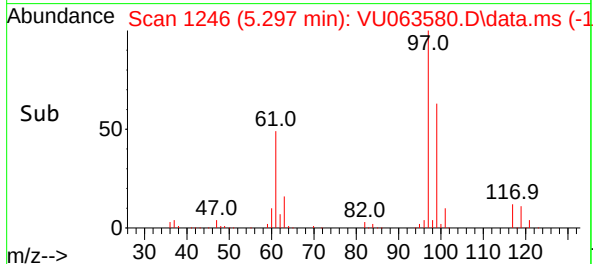

#29

1,1-Dichloropropene

Concen: 0.191 ug/l

RT: 5.509 min Scan# 1312

Delta R.T. 0.004 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44




Tgt Ion: 75 Resp: 2895


Ion Ratio Lower Upper

75 100

110 28.4 16.4 49.4

77 0.0 24.6 37.0#


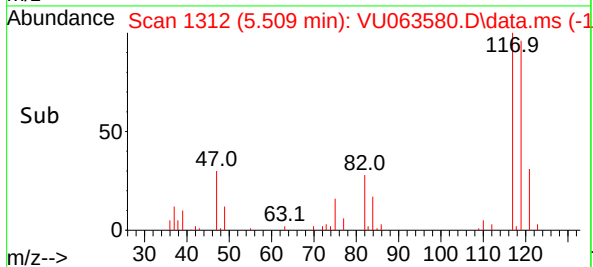

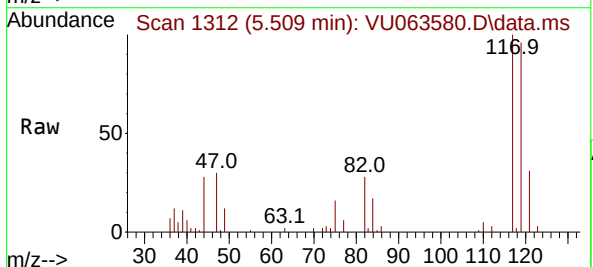




#30
Carbon Tetrachloride
Concen: 1.747 ug/l
RT: 5.503 min Scan# 117
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:117 Resp: 21029
Ion Ratio Lower Upper
117 100
119 98.2 75.7 113.5
121 30.8 25.4 38.0

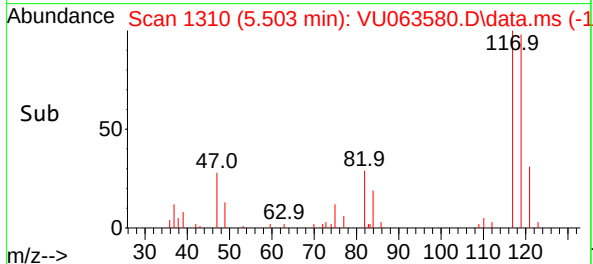

#31
Isopropyl Ether
Concen: 0.004 ug/l
RT: 3.982 min Scan# 837
Delta R.T. -0.009 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 45 Resp: 142
Ion Ratio Lower Upper
45 100
43 76.8 26.2 78.6




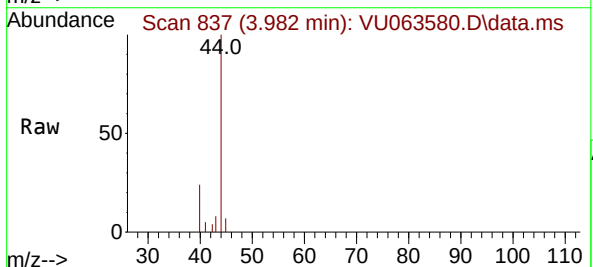




#32
Ethyl-t-butyl ether
Concen: 0.001 ug/l
RT: 4.496 min Scan# 91
Delta R.T. -0.006 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 59 Resp: 44
Ion Ratio Lower Upper
59 100
87 0.0 31.2 46.8#



#33
Tert-Amyl methyl ether
Concen: 0.006 ug/l
RT: 5.834 min Scan# 1413
Delta R.T. -0.106 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 73 Resp: 162
Ion Ratio Lower Upper
73 100
87 0.0 19.0 28.6#
71 0.0 9.4 14.2#









#35
Benzene
Concen: 9.402 ug/l
RT: 5.757 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 78 Resp: 411096
Ion Ratio Lower Upper
78 100
77 23.1 19.8 29.8

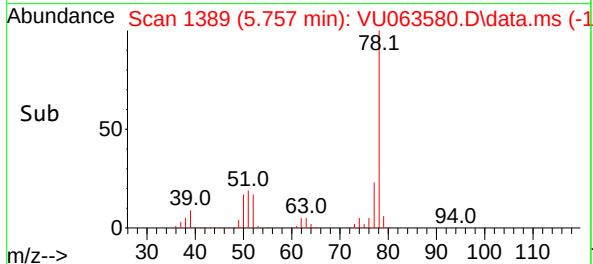

#36
1,2-Dichloroethane
Concen: 9.198 ug/l
RT: 5.782 min Scan# 1397
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 62 Resp: 135709
Ion Ratio Lower Upper
62 100
98 7.6 6.3 9.5


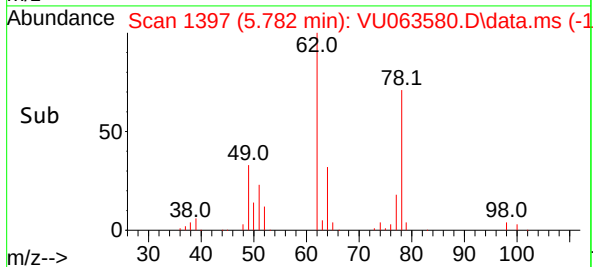

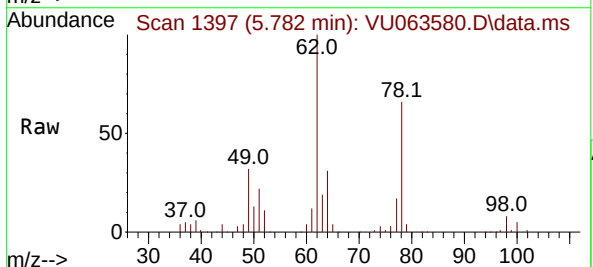




#37
 Trichloroethene
 Concen: 9.772 ug/l
 RT: 6.528 min Scan# 1
 Delta R.T. 0.004 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44




Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS


Tgt Ion:130 Resp: 106354
 Ion Ratio Lower Upper
 130 100
 95 105.2 85.4 128.2

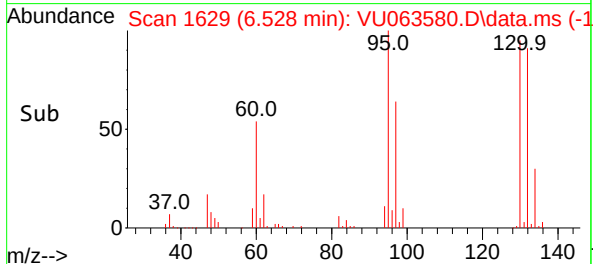

#38
 1,2-Dichloropropane
 Concen: 14.306 ug/l
 RT: 6.779 min Scan# 1707
 Delta R.T. 0.000 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44

Tgt Ion: 63 Resp: 165721
 Ion Ratio Lower Upper
 63 100
 65 31.1 24.9 37.3


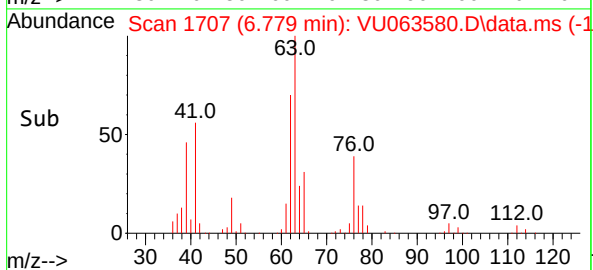

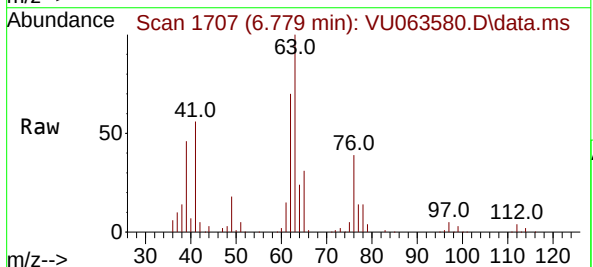




#39
Methacrylonitrile
Concen: 0.029 ug/l
RT: 4.982 min Scan# 1144
Delta R.T. 0.013 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:	41	Resp:	134
Ion	Ratio	Lower	Upper
41	100		
67	0.0	57.7	86.5#
39	254.5	44.6	67.0#
52	0.0	25.5	38.3#

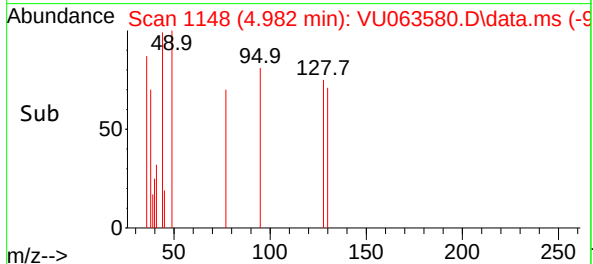

#40
Methyl acrylate
Concen: 0.007 ug/l
RT: 4.847 min Scan# 1106
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:	55	Resp:	42
Ion	Ratio	Lower	Upper
55	100		
85	0.0	12.8	19.2#
58	0.0	6.6	10.0#
42	245.2	8.4	12.6#

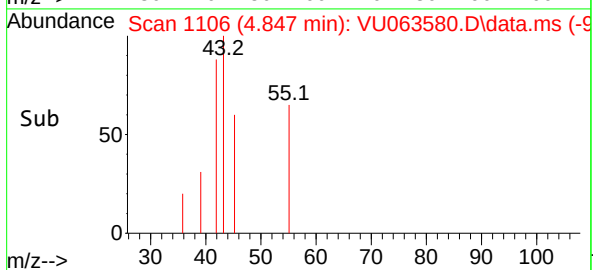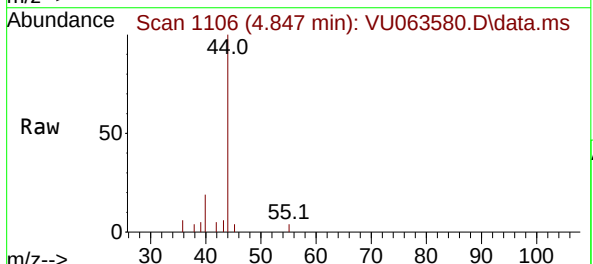



#41

Tetrahydrofuran

Concen: 0.200 ug/l

RT: 5.049 min Scan# 1169

Delta R.T. -0.009 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion: 42 Resp: 489

Ion Ratio Lower Upper

42 100

72 0.0 34.1 51.1#

71 4.3 29.9 44.9#

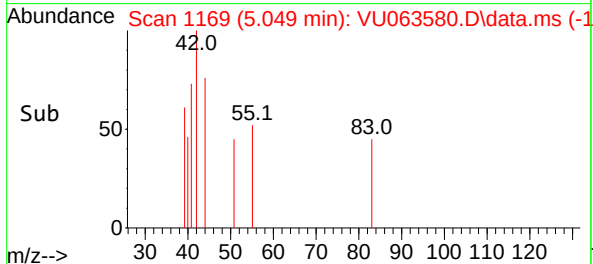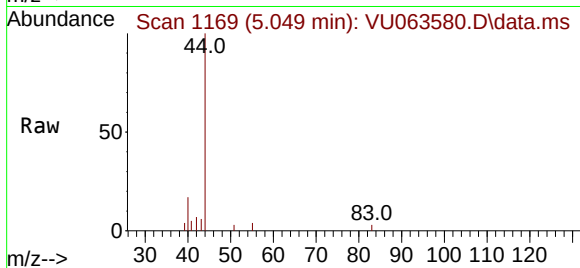

#42

1-Chlorobutane

Concen: 0.005 ug/l

RT: 5.438 min Scan# 1290

Delta R.T. 0.000 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 56 Resp: 110

Ion Ratio Lower Upper

56 100

41 141.8 28.3 84.9#

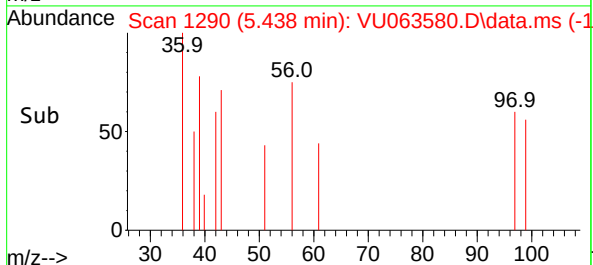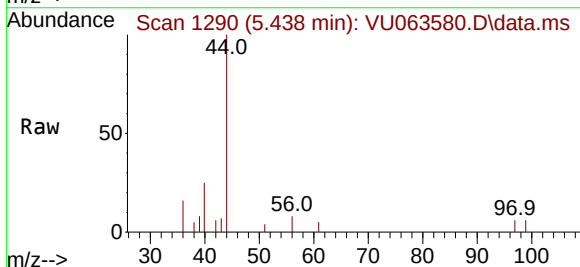



#43

Dibromomethane

Concen: 0.181 ug/l

RT: 6.904 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS





Tgt Ion: 93 Resp: 1003

Ion Ratio Lower Upper

93 100

95 0.0 66.6 100.0#

174 83.7 72.7 109.1

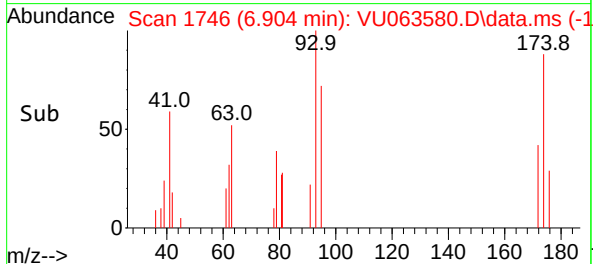

#45

4-Methyl-2-Pentanone

Concen: 0.143 ug/l

RT: 7.801 min Scan# 2025

Delta R.T. 0.007 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44




Tgt Ion: 43 Resp: 994


Ion Ratio Lower Upper

43 100

58 27.2 18.9 56.9


85 0.0 13.3 19.9#

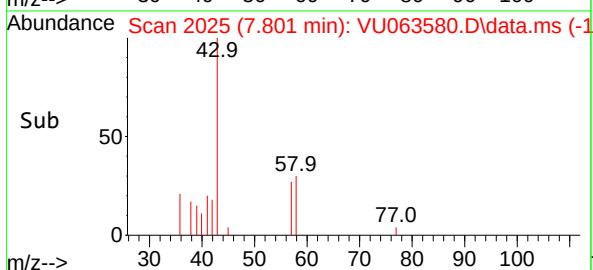






#46
t-1,4-Dichloro-2-butene
Concen: 0.157 ug/l
RT: 10.814 min Scan# 2962
Delta R.T. -0.003 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Instrument : MSVOA_U
ClientSampleId : WS0725-PT-RVOA-WS







Tgt Ion:	75	Resp:	409
Ion	Ratio	Lower	Upper
75	100		
53	17.1	43.2	64.8#
89	109.8	21.9	32.9#
88	0.0	17.9	26.9#

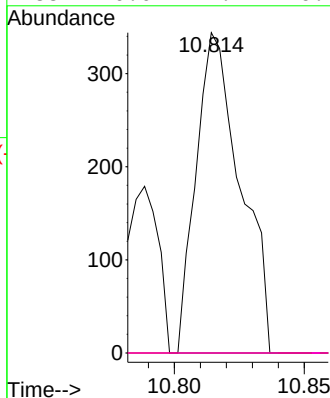

#47
Methyl methacrylate
Concen: 0.013 ug/l
RT: 6.978 min Scan# 1769
Delta R.T. 0.020 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:	69	Resp:	66
Ion	Ratio	Lower	Upper
69	100		
41	0.0	0.0	236.8
39	0.0	57.8	86.6#
100	0.0	27.5	41.3#

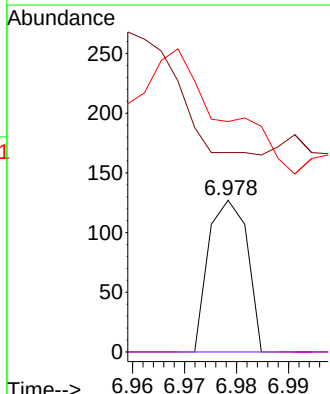



#48

Ethyl methacrylate

Concen: 0.012 ug/l

RT: 8.342 min Scan# 2190

Delta R.T. 0.010 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :





WS0725-PT-RVOA-WS

Tgt Ion: 69 Resp: 108

Ion Ratio Lower Upper

69 100

41 188.0 33.7 101.1#



#49

Toluene

Concen: 2.023 ug/l

RT: 7.956 min Scan# 2073

Delta R.T. -0.003 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 92 Resp: 48001

Ion Ratio Lower Upper

92 100

91 178.3 139.4 209.2









#50
 t-1,3-Dichloropropene
 Concen: 0.153 ug/l
 RT: 8.207 min Scan# 2150
 Delta R.T. 0.004 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44




Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS


Tgt Ion: 75 Resp: 1359
 Ion Ratio Lower Upper
 75 100
 77 24.8 24.8 37.2

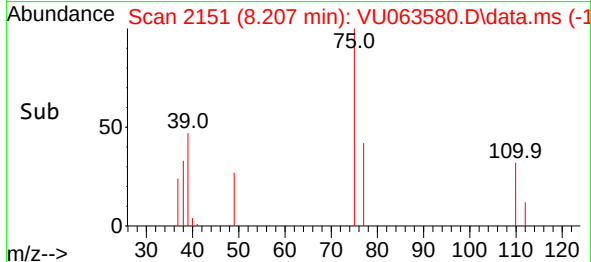

#51
 cis-1,3-Dichloropropene
 Concen: 0.223 ug/l
 RT: 7.599 min Scan# 1962
 Delta R.T. 0.000 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44

Tgt Ion: 75 Resp: 2632
 Ion Ratio Lower Upper
 75 100
 77 33.2 25.2 37.8
 39 54.9 38.8 58.2

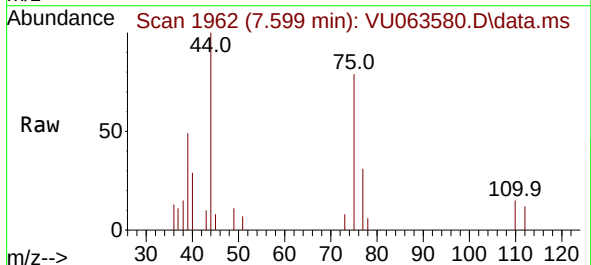



#52

1,1,2-Trichloroethane

Concen: 14.618 ug/l

RT: 8.390 min Scan# 21

Delta R.T. -0.003 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS

Tgt Ion: 97 Resp: 114914





Ion Ratio Lower Upper

97 100

83 89.8 68.5 102.7

85 57.7 45.0 67.6

99 62.4 48.6 72.8



#53

1,3-Dichloropropane

Concen: 0.051 ug/l

RT: 8.570 min Scan# 2264

Delta R.T. 0.004 min

Lab File: VU063580.D




Acq: 15 Sep 2025 15:44


Tgt Ion: 76 Resp: 703

Ion Ratio Lower Upper

76 100

78 27.3 26.2 39.2









#54
2-Hexanone
Concen: 0.179 ug/l
RT: 8.699 min Scan# 2104
Delta R.T. 0.013 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:	43	Resp:	912
Ion	Ratio	Lower	Upper
43	100		
58	13.7	32.7	72.7#
57	0.0	0.0	38.2



#57
4-Bromofluorobenzene
Concen: 0.919 ug/l
RT: 10.628 min Scan# 2904
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:	95	Resp:	11435
Ion	Ratio	Lower	Upper
95	100		
174	81.3	64.7	97.1
176	81.8	66.2	99.4









#58
Tetrachloroethene
Concen: 9.498 ug/l
RT: 8.538 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:164 Resp: 101804
Ion Ratio Lower Upper
164 100
166 125.4 106.4 159.6
129 99.1 81.4 122.2
131 96.5 77.7 116.5

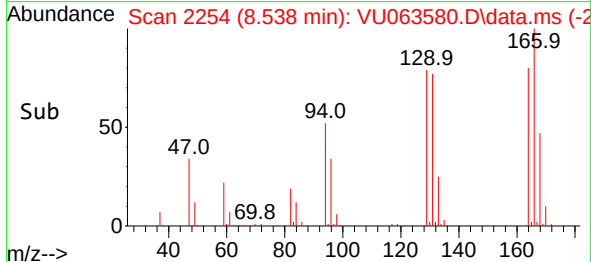

#59
Chlorobenzene
Concen: 16.323 ug/l
RT: 9.438 min Scan# 2534
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:112 Resp: 446307
Ion Ratio Lower Upper
112 100
114 32.0 25.0 37.4


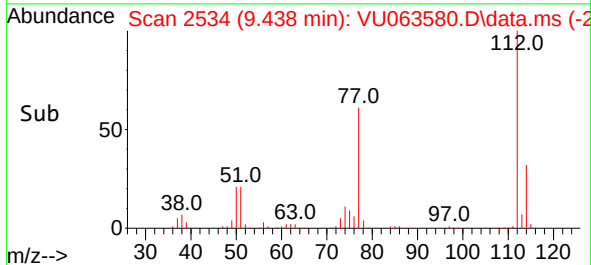






#60
1,1,1,2-Tetrachloroethane
Concen: 0.091 ug/l
RT: 9.528 min Scan# 21
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:131 Resp: 811
Ion Ratio Lower Upper
131 100
133 94.7 75.8 113.8
119 71.0 51.8 77.6



#61
Pentachloroethane
Concen: 0.012 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. -0.006 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:117 Resp: 80
Ion Ratio Lower Upper
117 100
167 0.0 62.6 93.8#




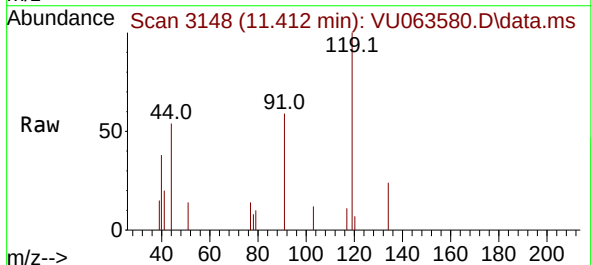




#63
Ethyl Benzene
Concen: 14.817 ug/l
RT: 9.560 min Scan# 2572
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 91 Resp: 691760
Ion Ratio Lower Upper
91 100
106 30.8 23.8 35.8



#64
m/p-Xylenes
Concen: 11.658 ug/l
RT: 9.686 min Scan# 2611
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 106 Resp: 209151
Ion Ratio Lower Upper
106 100
91 208.1 167.0 250.4





#65

o-Xylene

Concen: 11.670 ug/l

RT: 10.091 min Scan# 2737

Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :





WS0725-PT-RVOA-WS

Tgt Ion:106 Resp: 209563

Ion Ratio Lower Upper

106 100

91 220.9 108.7 326.1

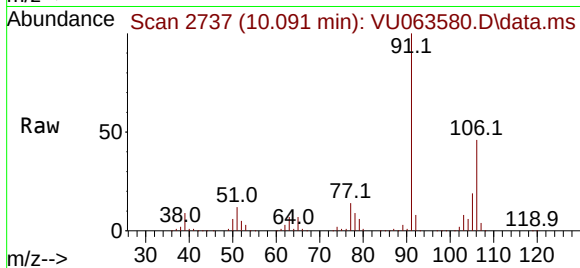

#66

Styrene

Concen: 2.547 ug/l

RT: 10.107 min Scan# 2742

Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44




Tgt Ion:104 Resp: 73010


Ion Ratio Lower Upper

104 100

78 82.7 41.2 61.8#

103 83.6 44.2 66.2#




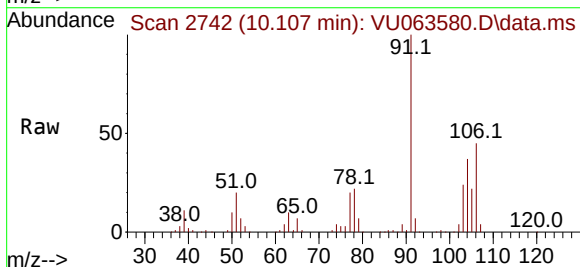




#68
 1,2-Dichlorobenzene-d4
 Concen: 0.999 ug/l
 RT: 12.187 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44




Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS


Tgt Ion:152 Resp: 12678
 Ion Ratio Lower Upper
 152 100
 115 65.5 0.0 260.6
 150 250.2 0.0 661.8



#69
 Isopropylbenzene
 Concen: 0.177 ug/l
 RT: 10.477 min Scan# 2857
 Delta R.T. 0.000 min
 Lab File: VU063580.D
 Acq: 15 Sep 2025 15:44

Tgt Ion:105 Resp: 7707
 Ion Ratio Lower Upper
 105 100
 120 26.1 12.7 38.0









#70
1,1,2,2-Tetrachloroethane
Concen: 0.020 ug/l
RT: 10.776 min Scan# 2950
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 83 Resp: 198
Ion Ratio Lower Upper
83 100
131 0.0 7.7 11.5#
85 24.2 52.2 78.4#

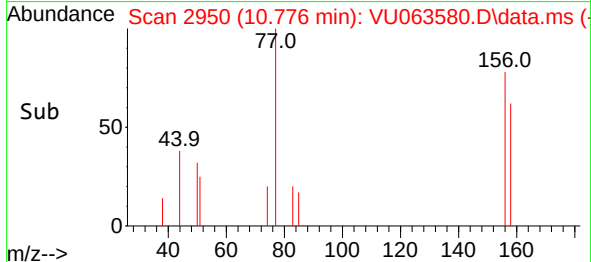

#71
1,2,3-Trichloropropane
Concen: 0.055 ug/l
RT: 10.814 min Scan# 2962
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 75 Resp: 409
Ion Ratio Lower Upper
75 100
77 405.9 0.0 0.0#
110 0.0 0.0 77.6
97 0.0 0.0 39.6




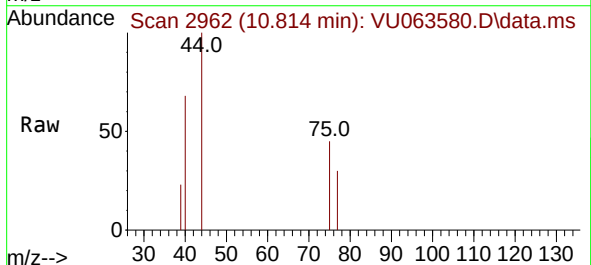




#72
Bromobenzene
Concen: 0.081 ug/l
RT: 10.779 min Scan# 2950
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:156 Resp: 911
Ion Ratio Lower Upper
156 100
77 182.2 0.0 323.0
158 99.7 0.0 195.4



#73
n-propylbenzene
Concen: 0.358 ug/l
RT: 10.898 min Scan# 2988
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:120 Resp: 4511
Ion Ratio Lower Upper
120 100
91 462.9 349.1 523.7









#74
2-Chlorotoluene
Concen: 0.055 ug/l
RT: 10.978 min Scan# 3013
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:126 Resp: 625
Ion Ratio Lower Upper
126 100
91 416.6 0.0 609.4

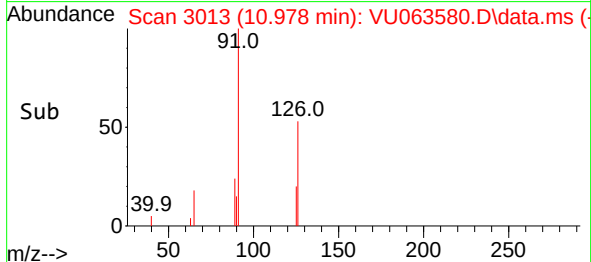

#75
1,3,5-Trimethylbenzene
Concen: 0.094 ug/l
RT: 11.081 min Scan# 3045
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:105 Resp: 3839
Ion Ratio Lower Upper
105 100
120 44.1 38.0 57.0




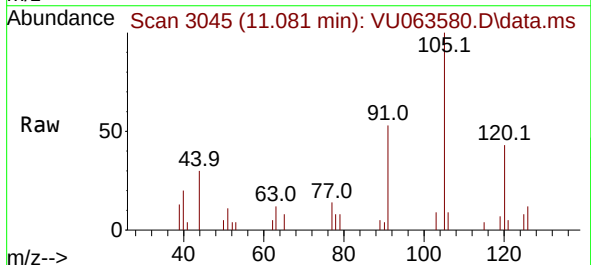




#76
4-Chlorotoluene
Concen: 0.101 ug/l
RT: 11.094 min Scan# 3048
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:126 Resp: 1203
Ion Ratio Lower Upper
126 100
91 348.5 0.0 679.4

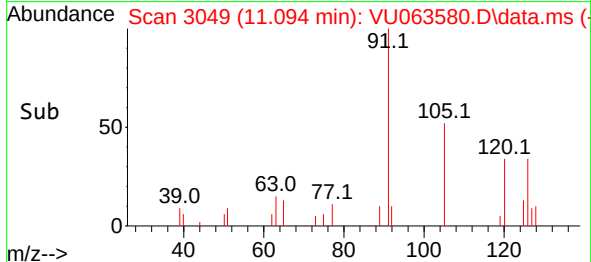

#77
tert-Butylbenzene
Concen: 0.052 ug/l
RT: 11.412 min Scan# 3148
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:119 Resp: 2037
Ion Ratio Lower Upper
119 100
91 71.5 31.0 93.0
134 20.4 19.0 28.6




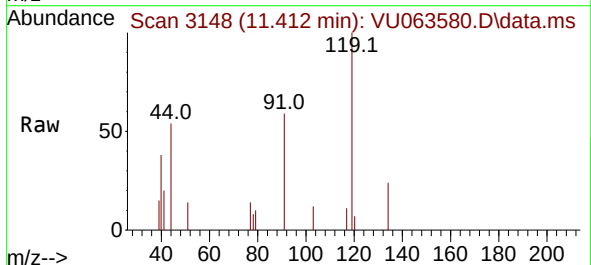




#78
1,2,4-Trimethylbenzene
Concen: 0.090 ug/l
RT: 11.467 min Scan# 3165
Delta R.T. 0.007 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:105 Resp: 3558
Ion Ratio Lower Upper
105 100
120 43.8 22.4 67.3



#79
sec-Butylbenzene
Concen: 0.128 ug/l
RT: 11.634 min Scan# 3217
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:105 Resp: 6821
Ion Ratio Lower Upper
105 100
134 19.0 15.6 23.4









#81
p-Isopropyltoluene
Concen: 0.178 ug/l
RT: 11.785 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion:	119	Resp:	7641
Ion Ratio	Lower	Upper	
119	100		
134	25.2	20.6	30.8
91	27.3	19.8	29.6



#83
1,4-Dichlorobenzene
Concen: 6.030 ug/l
RT: 11.830 min Scan# 3278
Delta R.T. 0.004 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion:	146	Resp:	140967
Ion Ratio	Lower	Upper	
146	100		
111	39.8	31.6	47.4
148	64.3	51.8	77.8









#84
n-Butylbenzene
Concen: 0.157 ug/l
RT: 12.203 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44




Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS


Tgt Ion: 91	Resp: 6322
Ion Ratio	Lower Upper
91	100
92	48.7 41.3 61.9
134	25.0 19.9 29.9



#85
1,2-Dichlorobenzene
Concen: 5.706 ug/l
RT: 12.203 min Scan# 3394
Delta R.T. 0.000 min
Lab File: VU063580.D
Acq: 15 Sep 2025 15:44

Tgt Ion: 146	Resp: 125252
Ion Ratio	Lower Upper
146	100
111	44.0 21.0 63.0
148	64.4 31.8 95.3

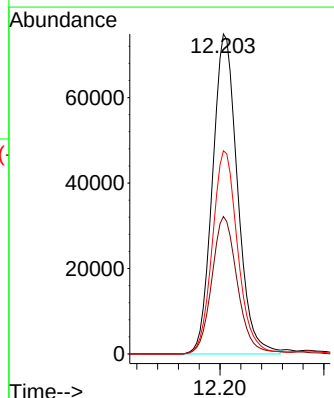



#87

1,2,4-Trichlorobenzene

Concen: 18.812 ug/l

RT: 13.833 min Scan# 3901

Delta R.T. 0.000 min

Lab File: VU063580.D


Acq: 15 Sep 2025 15:44

Instrument :

MSVOA_U

ClientSampleId :

WS0725-PT-RVOA-WS






Tgt Ion:180 Resp: 250047

Ion Ratio Lower Upper

180 100

182 94.5 77.1 115.7

145 31.6 25.0 37.4

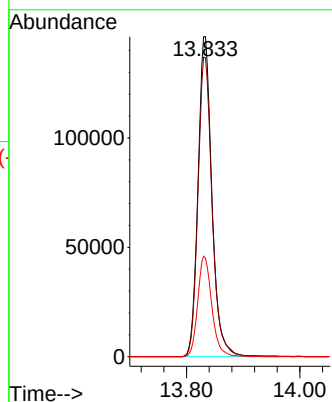

#88

Hexachlorobutadiene

Concen: 0.053 ug/l

RT: 14.013 min Scan# 3957

Delta R.T. 0.000 min

Lab File: VU063580.D

Acq: 15 Sep 2025 15:44

Tgt Ion:225 Resp: 442

Ion Ratio Lower Upper

225 100

223 66.3 50.2 75.2

227 49.5 51.6 77.4#

