

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
 Data File : VU063572.D
 Acq On : 15 Sep 2025 10:34
 Operator : MD/SY
 Sample : VU0915WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0915WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.776	146	151	160	rVB4	18359	24876	27.47%	8.302%
2	2.123	254	259	262	rBV5	1503	1423	1.57%	0.475%
3	2.676	429	431	437	rVB4	1332	1129	1.25%	0.377%
4	3.030	532	541	554	rVB3	7367	12609	13.92%	4.208%
5	3.155	575	580	581	rBV2	1610	1292	1.43%	0.431%
6	3.223	597	601	605	rBV3	1015	1039	1.15%	0.347%
7	3.547	699	702	707	rBV6	1294	1375	1.52%	0.459%
8	4.586	1020	1025	1029	rBV5	1050	1192	1.32%	0.398%
9	5.245	1227	1230	1232	rBV4	1522	1113	1.23%	0.371%
10	6.097	1482	1495	1520	rBV	41043	90567	100.00%	30.225%
11	6.441	1600	1602	1621	rVB3	2803	4409	4.87%	1.471%
12	6.521	1621	1627	1635	rVB6	1096	1445	1.60%	0.482%
13	10.631	2895	2905	2919	rBV2	30601	52877	58.38%	17.646%
14	11.415	3144	3149	3154	rVB4	855	935	1.03%	0.312%
15	11.634	3211	3217	3227	rBV4	1201	1727	1.91%	0.576%
16	11.791	3261	3266	3276	rVB5	1090	1692	1.87%	0.565%
17	11.840	3276	3281	3291	rBV6	1115	1920	2.12%	0.641%
18	12.078	3347	3355	3362	rBV7	1083	1606	1.77%	0.536%
19	12.190	3379	3390	3410	rBV2	40495	76073	84.00%	25.388%
20	12.762	3560	3568	3569	rBV2	1187	1202	1.33%	0.401%
21	13.849	3896	3906	3913	rBV6	2577	4597	5.08%	1.534%
22	14.094	3976	3982	3983	rBV3	4078	3054	3.37%	1.019%
23	14.328	4046	4055	4064	rBV6	3063	4746	5.24%	1.584%
24	14.566	4123	4129	4139	rVB3	1171	2094	2.31%	0.699%
25	16.161	4618	4625	4627	rBV5	939	1111	1.23%	0.371%
26	16.679	4781	4786	4789	rBV5	990	920	1.02%	0.307%
27	17.109	4918	4920	4926	rVB4	1065	908	1.00%	0.303%
28	17.248	4959	4963	4970	rBV7	1086	1716	1.89%	0.573%




Sum of corrected areas: 299647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063572.D
Acq On : 15 Sep 2025 10:34
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0915WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

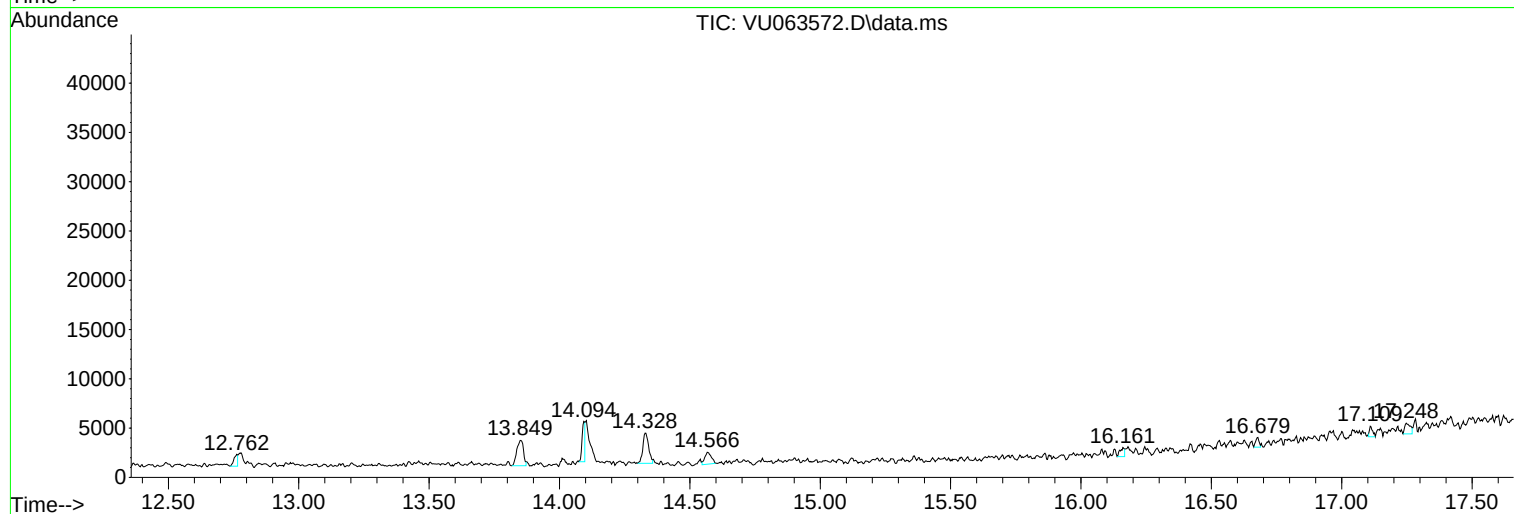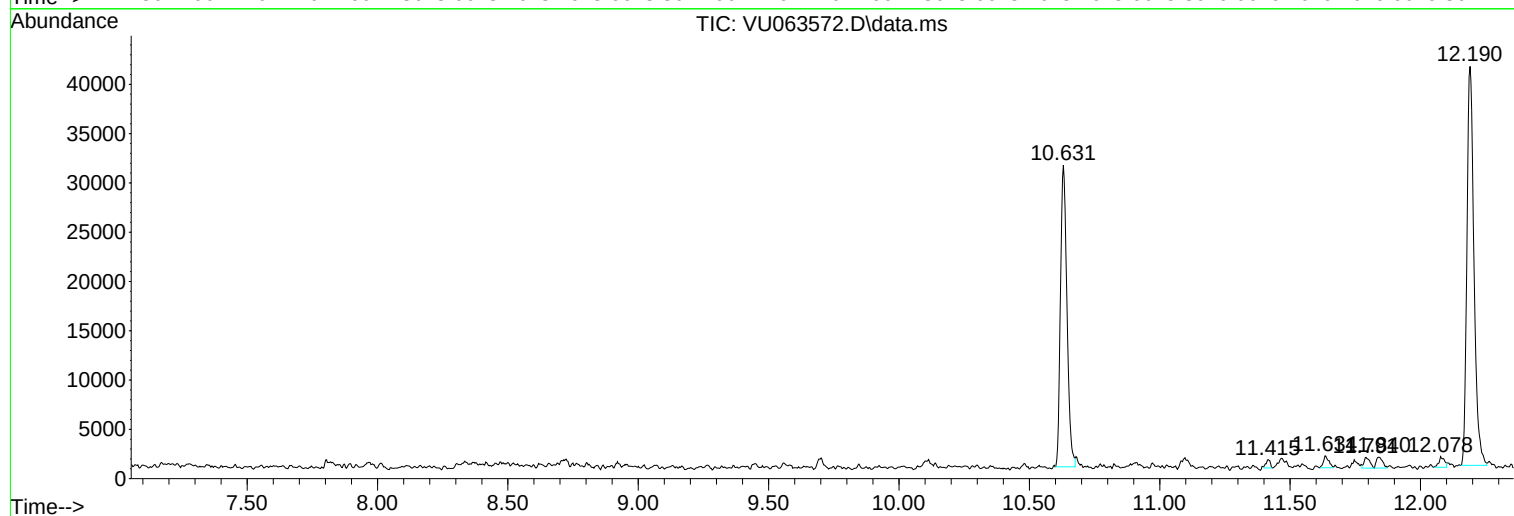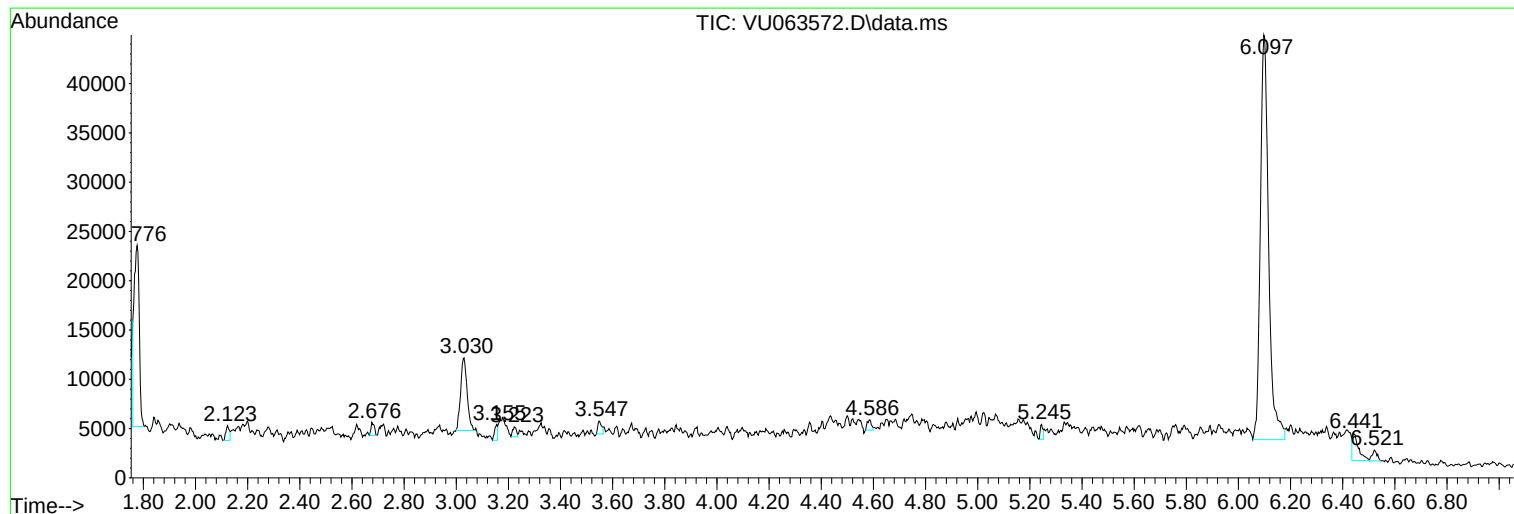

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063572.D
Acq On : 15 Sep 2025 10:34
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0915WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063572.D
Acq On : 15 Sep 2025 10:34
Operator : MD/SY
Sample : VU0915WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0915WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------