

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
 Data File : VU063580.D
 Acq On : 15 Sep 2025 15:44
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.770	145	149	160	rVB	16592	22194	1.37%	0.146%
2	2.570	384	398	410	rBV	128445	214355	13.22%	1.406%
3	3.030	528	541	560	rBV	252826	469334	28.95%	3.079%
4	3.335	623	636	659	rBV	243578	492988	30.41%	3.234%
5	4.650	1031	1045	1062	rBV	88815	200196	12.35%	1.313%
6	5.297	1228	1246	1268	rBV	329950	748768	46.18%	4.912%
7	5.506	1297	1311	1330	rBV3	36952	82117	5.06%	0.539%
8	5.760	1374	1390	1431	rBV2	436668	1240990	76.54%	8.140%
9	6.097	1484	1495	1510	rBV2	36077	75032	4.63%	0.492%
10	6.528	1613	1629	1659	rBV	315486	644108	39.73%	4.225%
11	6.779	1692	1707	1741	rBV	430034	844613	52.10%	5.540%
12	7.956	2062	2073	2093	rBV	110694	207730	12.81%	1.363%
13	8.390	2195	2208	2234	rBV	378780	660848	40.76%	4.335%
14	8.541	2242	2255	2290	rBV	462047	840104	51.82%	5.511%
15	9.438	2519	2534	2556	rBV	809460	1418812	87.51%	9.307%
16	9.560	2560	2572	2598	rVV	939397	1621270	100.00%	10.635%
17	9.686	2599	2611	2645	rVB	698775	1252800	77.27%	8.218%
18	10.091	2723	2737	2772	rBV2	825868	1516599	93.54%	9.948%
19	10.477	2847	2857	2867	rBV	11307	17166	1.06%	0.113%
20	10.628	2894	2904	2918	rBV	32682	56054	3.46%	0.368%
21	10.901	2974	2989	3002	rBV	25618	41860	2.58%	0.275%
22	11.088	3037	3047	3064	rBV4	9811	19388	1.20%	0.127%
23	11.827	3268	3277	3301	rVB	341984	563714	34.77%	3.698%
24	12.203	3375	3394	3412	rBV2	334999	620764	38.29%	4.072%
25	13.830	3888	3900	3927	rBV	808904	1372964	84.68%	9.006%


Sum of corrected areas: 15244768

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063580.D
Acq On : 15 Sep 2025 15:44
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

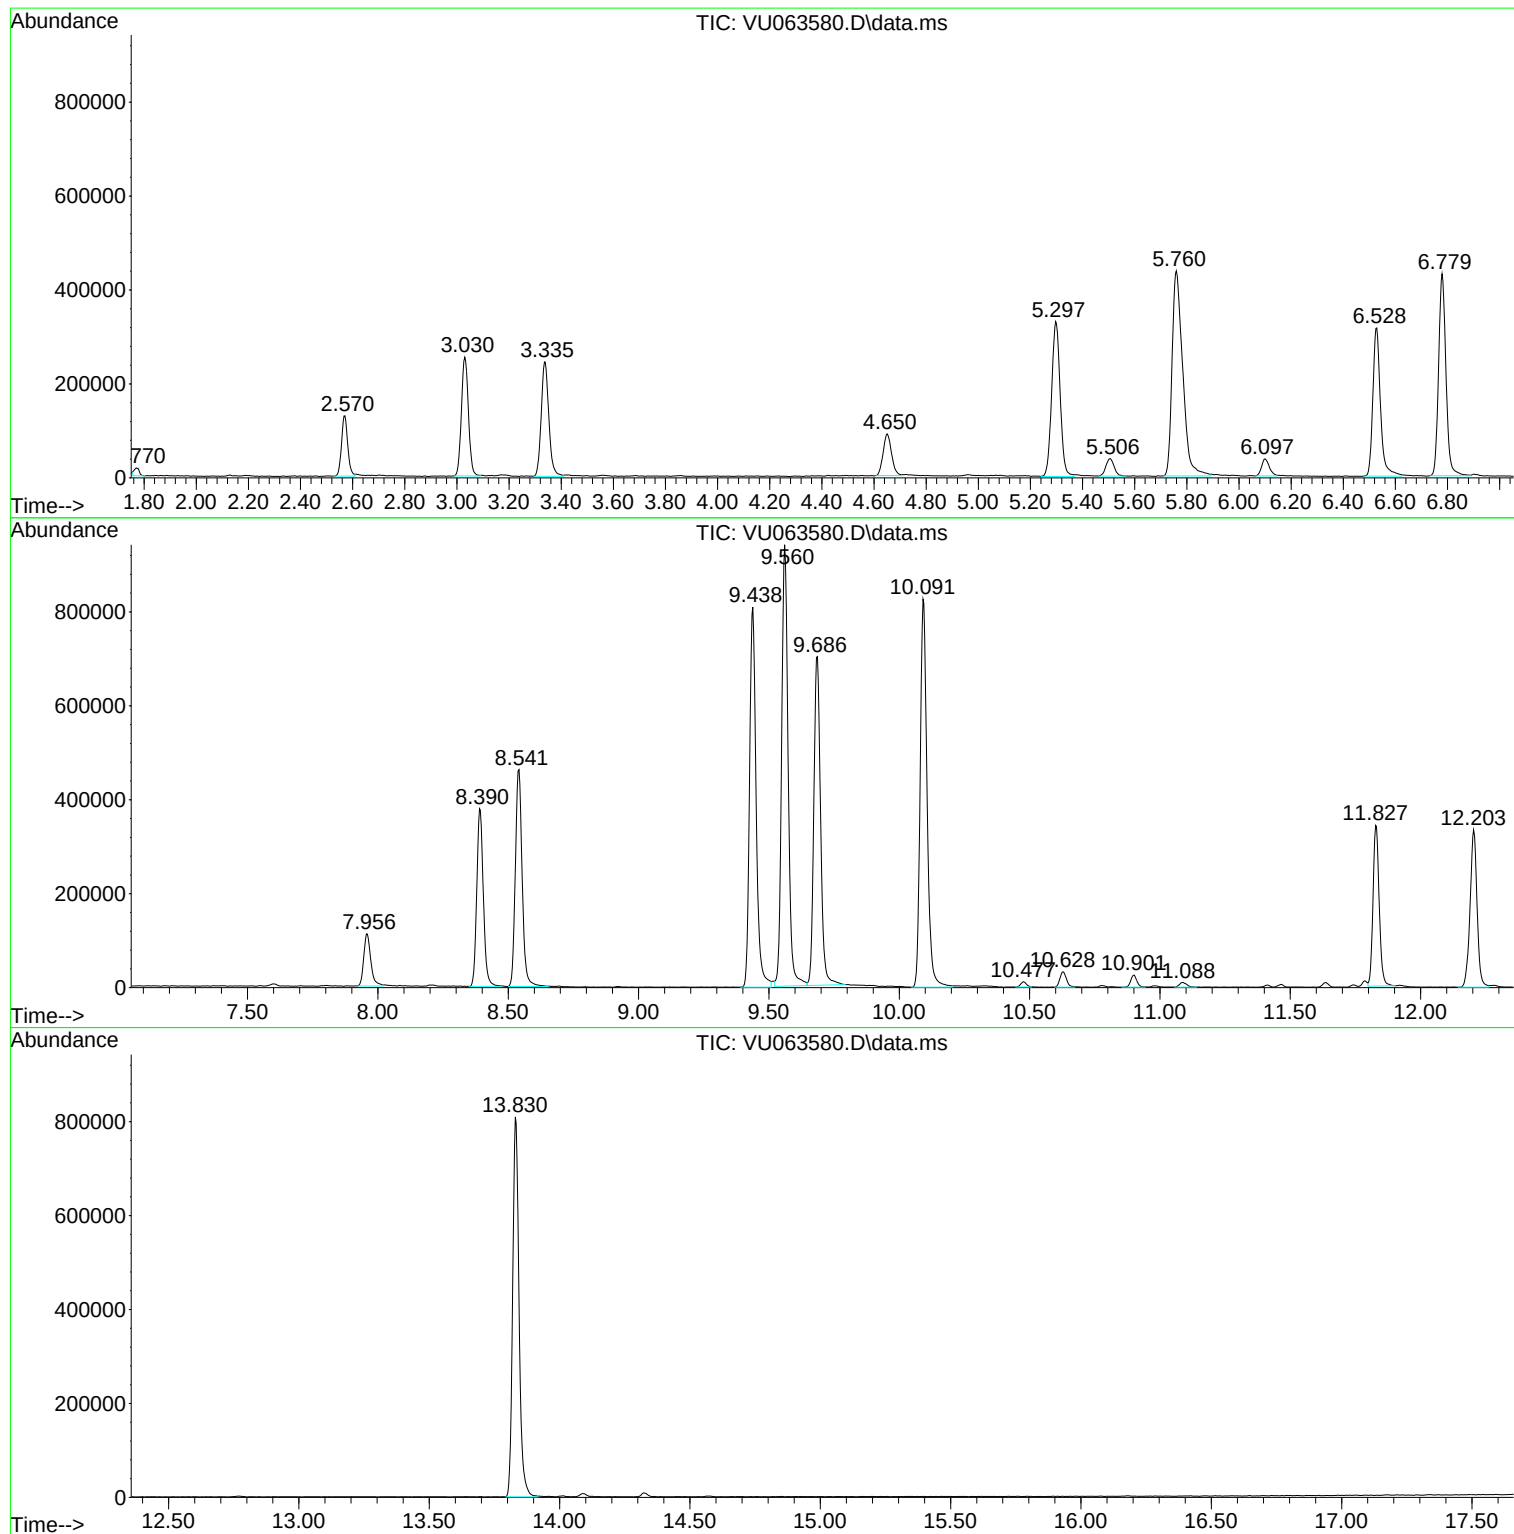

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063580.D
Acq On : 15 Sep 2025 15:44
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063580.D
Acq On : 15 Sep 2025 15:44
Operator : MD/SY
Sample : Q2552-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------