

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
 Data File : VU063582.D
 Acq On : 15 Sep 2025 16:44
 Operator : MD/SY
 Sample : Q2552-08
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.840	163	171	186	rVB	45177	64187	2.22%	0.256%
2	2.129	249	261	278	rBV	734967	1109046	38.27%	4.417%
3	3.030	531	541	559	rVB2	20222	39515	1.36%	0.157%
4	3.357	623	643	670	rBV	936790	2183966	75.37%	8.697%
5	3.853	782	797	816	rBV	100253	238949	8.25%	0.952%
6	4.647	1025	1044	1068	rBV2	246560	613618	21.18%	2.444%
7	4.959	1125	1141	1169	rBV2	213583	477556	16.48%	1.902%
8	5.509	1296	1312	1348	rBV	318978	715672	24.70%	2.850%
9	6.094	1483	1494	1514	rBV2	45350	96938	3.35%	0.386%
10	6.525	1618	1628	1640	rBV3	18032	35452	1.22%	0.141%
11	6.904	1732	1746	1769	rBV	186038	358120	12.36%	1.426%
12	7.595	1947	1961	1982	rBV	376508	664334	22.93%	2.646%
13	8.200	2136	2149	2175	rBV	216571	372438	12.85%	1.483%
14	8.566	2242	2263	2282	rBV2	81452	184470	6.37%	0.735%
15	9.441	2524	2535	2548	rBV2	17507	30748	1.06%	0.122%
16	9.524	2548	2561	2588	rBV2	608784	1067344	36.84%	4.251%
17	9.688	2600	2612	2633	rVB3	22279	40466	1.40%	0.161%
18	10.094	2727	2738	2753	rBV2	19181	36065	1.24%	0.144%
19	10.473	2842	2856	2886	rBV	479365	780840	26.95%	3.110%
20	10.627	2891	2904	2925	rVB3	34099	62922	2.17%	0.251%
21	10.772	2937	2949	2957	rBV2	476106	803035	27.71%	3.198%
22	10.814	2957	2962	2976	rVB2	190180	295795	10.21%	1.178%
23	10.897	2976	2988	3004	rBV	1218030	1939950	66.95%	7.726%
24	10.978	3004	3013	3027	rVB	167839	273569	9.44%	1.089%
25	11.084	3034	3046	3073	rVB4	599082	1087773	37.54%	4.332%
26	11.409	3134	3147	3155	rBV	362878	568077	19.61%	2.262%
27	11.460	3155	3163	3189	rVB	274932	443421	15.30%	1.766%
28	11.634	3202	3217	3236	rBV	948782	1479383	51.06%	5.892%
29	11.737	3238	3249	3255	rVV	353702	558499	19.27%	2.224%
30	11.785	3255	3264	3301	rVB	1315434	2071902	71.50%	8.251%
31	12.200	3378	3393	3410	rBV	785537	1255814	43.34%	5.001%
32	13.833	3886	3901	3917	rBV5	25426	54430	1.88%	0.217%
33	14.010	3940	3956	3968	rBV	1843654	2897611	100.00%	11.539%
34	14.081	3968	3978	4001	rVB	279797	493999	17.05%	1.967%
35	14.322	4039	4053	4080	rBV	1027443	1714495	59.17%	6.828%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063582.D
Acq On : 15 Sep 2025 16:44
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER




Sum of corrected areas: 25110399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063582.D
Acq On : 15 Sep 2025 16:44
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

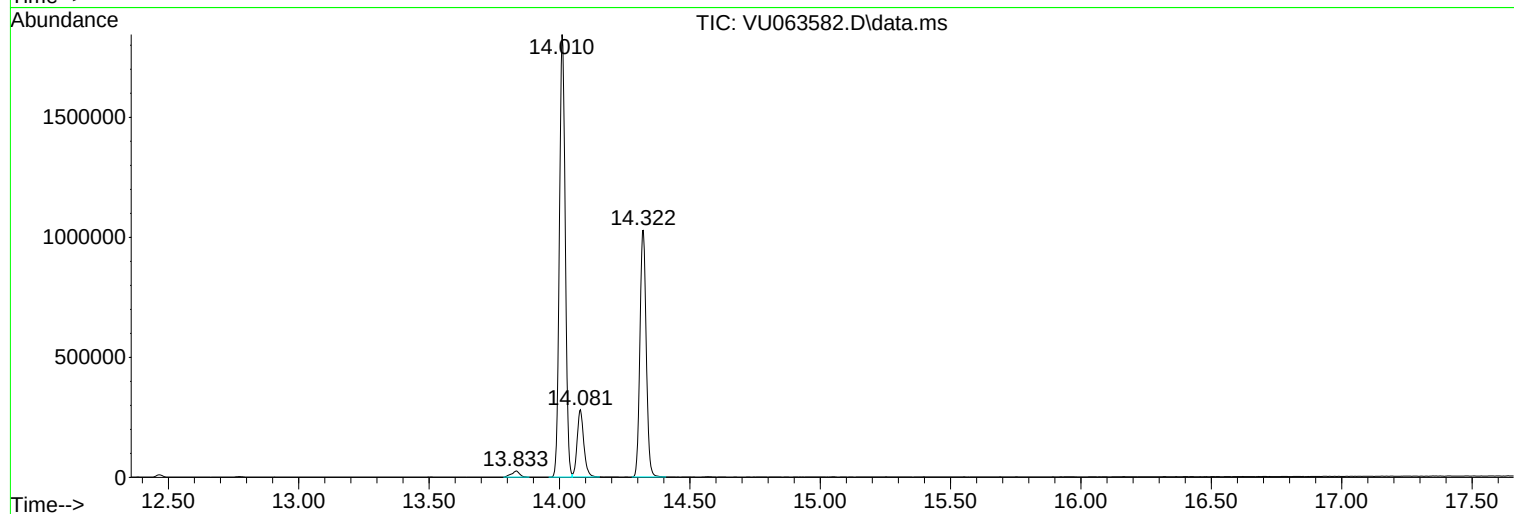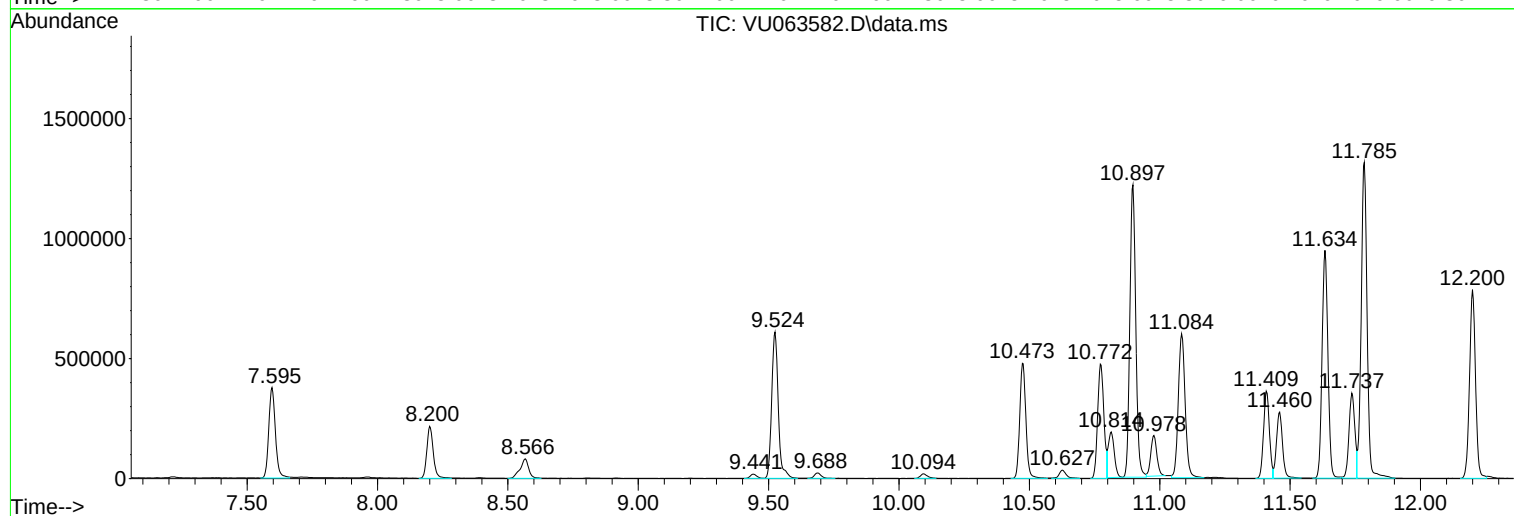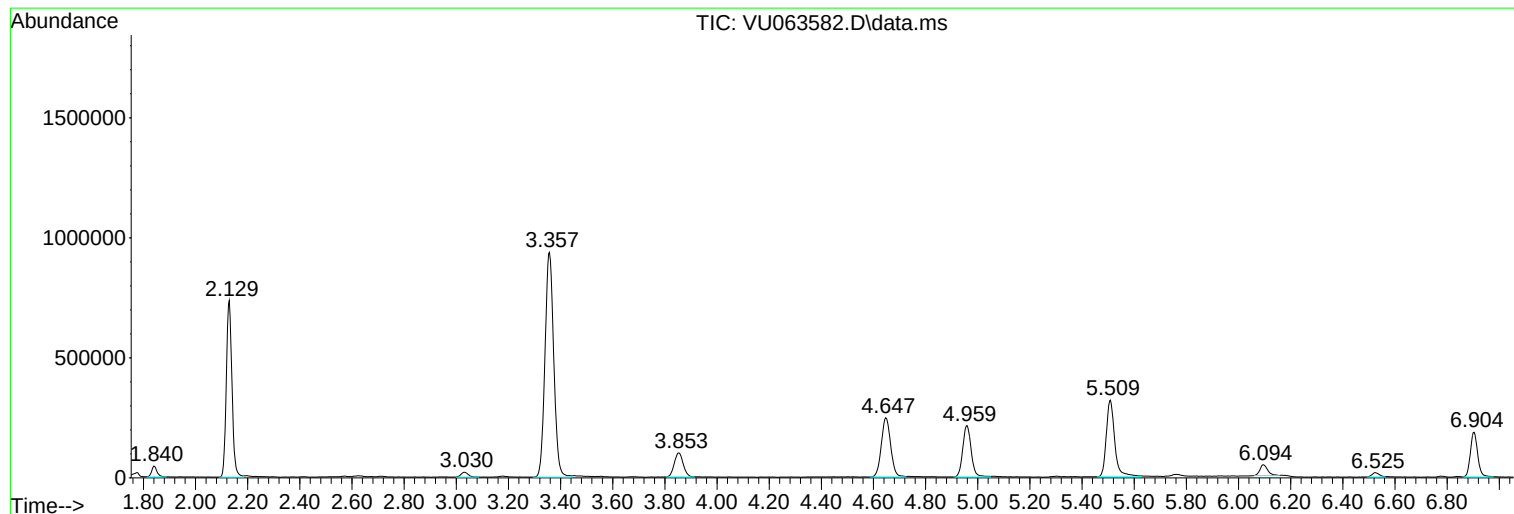

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063582.D
Acq On : 15 Sep 2025 16:44
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063582.D
Acq On : 15 Sep 2025 16:44
Operator : MD/SY
Sample : Q2552-08
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------