


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091525\
Data File : VU063570.D
Acq On : 15 Sep 2025 08:18
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U091225DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Sat Sep 13 03:31:19 2025

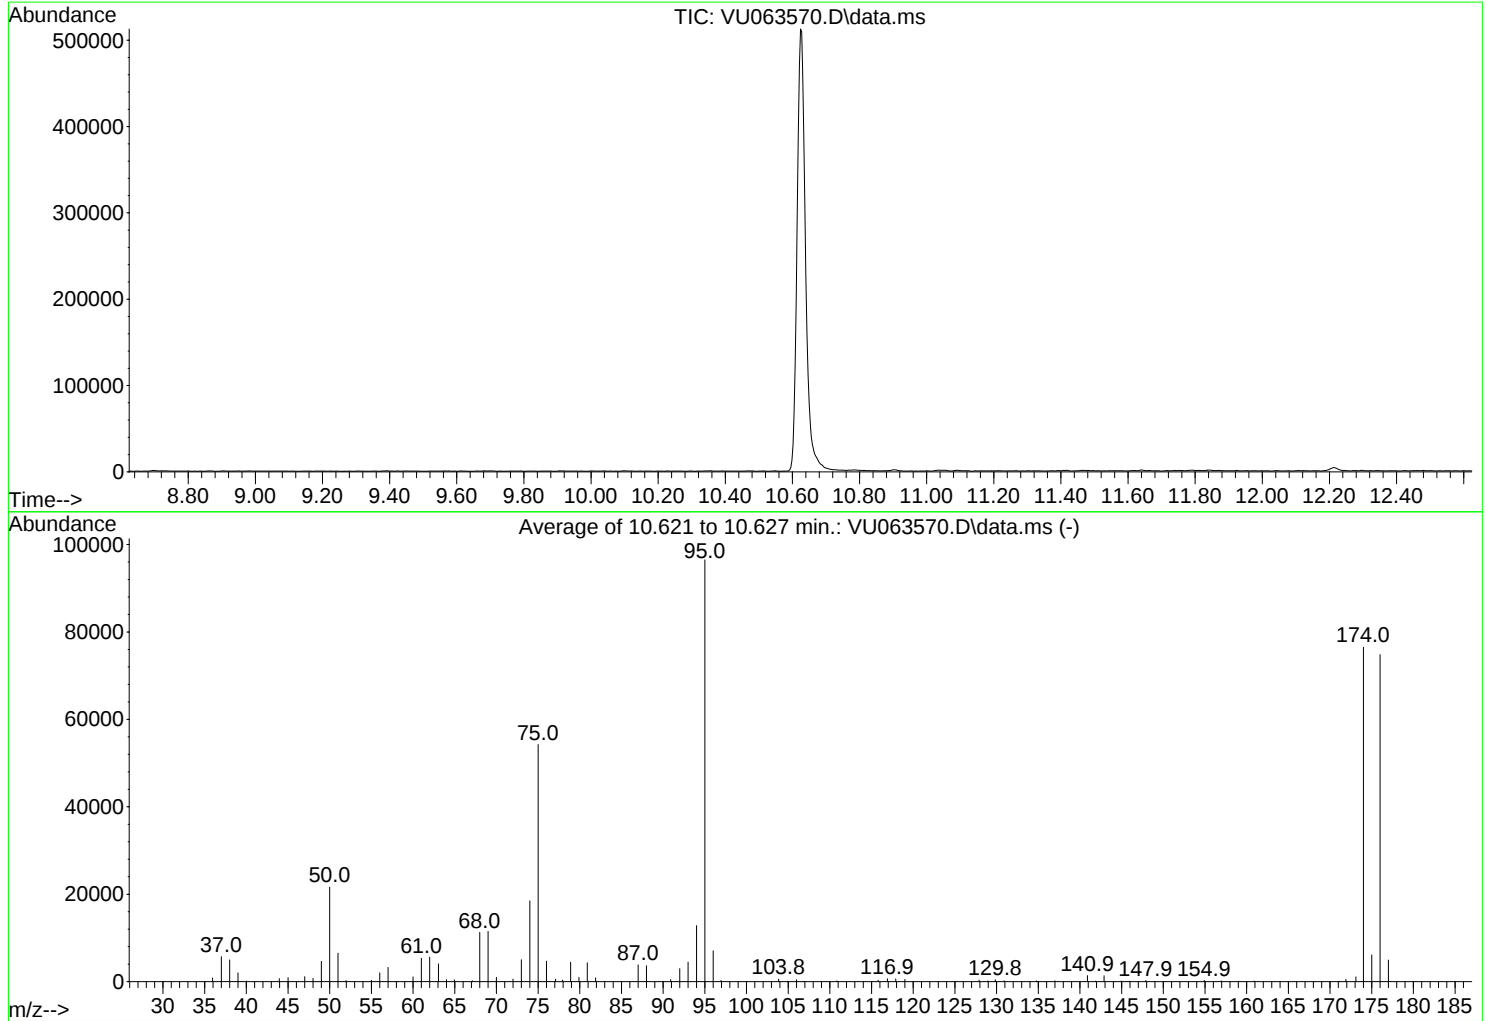

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	21627	PASS
75	95	30	60	56.2	54261	PASS
95	95	100	100	100.0	96501	PASS
96	95	5	9	7.3	7049	PASS
173	174	0.00	2	1.4	1084	PASS
174	95	50	100	79.3	76499	PASS
175	174	5	9	8.0	6111	PASS
176	174	95	101	97.8	74837	PASS
177	176	5	9	6.6	4947	PASS