

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091624\
 Data File : VU060788.D
 Acq On : 16 Sep 2024 18:37
 Operator : MD/SY
 Sample : P3967-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Quant Time: Sep 17 01:56:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 17 01:47:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	143150	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	150773	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	58609	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	59971	4.658	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.200%
7) Chloroethane-d5	1.911	69	47169	5.145	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.000%
11) 1,1-Dichloroethene-d2	2.560	65	23374	5.122	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.400%
20) 2-Butanone-d5	4.637	46	106135	51.348	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.700%
24) Chloroform-d	5.055	84	97740	4.966	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.695	65	48627	5.169	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.400%
32) Benzene-d6	5.721	84	195379	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
36) 1,2-Dichloropropane-d6	6.682	67	63859	5.107	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.894	98	165440	4.490	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	8.177	79	21507	4.779	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.600%
46) 2-Hexanone-d5	8.631	63	80721	45.467	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.940%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49203	5.023	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	58347	5.925	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.400%
Target Compounds						Qvalue
13) Acetone	2.657	43	17319	12.559	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091624\
Data File : VU060788.D
Acq On : 16 Sep 2024 18:37
Operator : MD/SY
Sample : P3967-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Time: Sep 17 01:56:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 17 01:47:23 2024
Response via : Initial Calibration

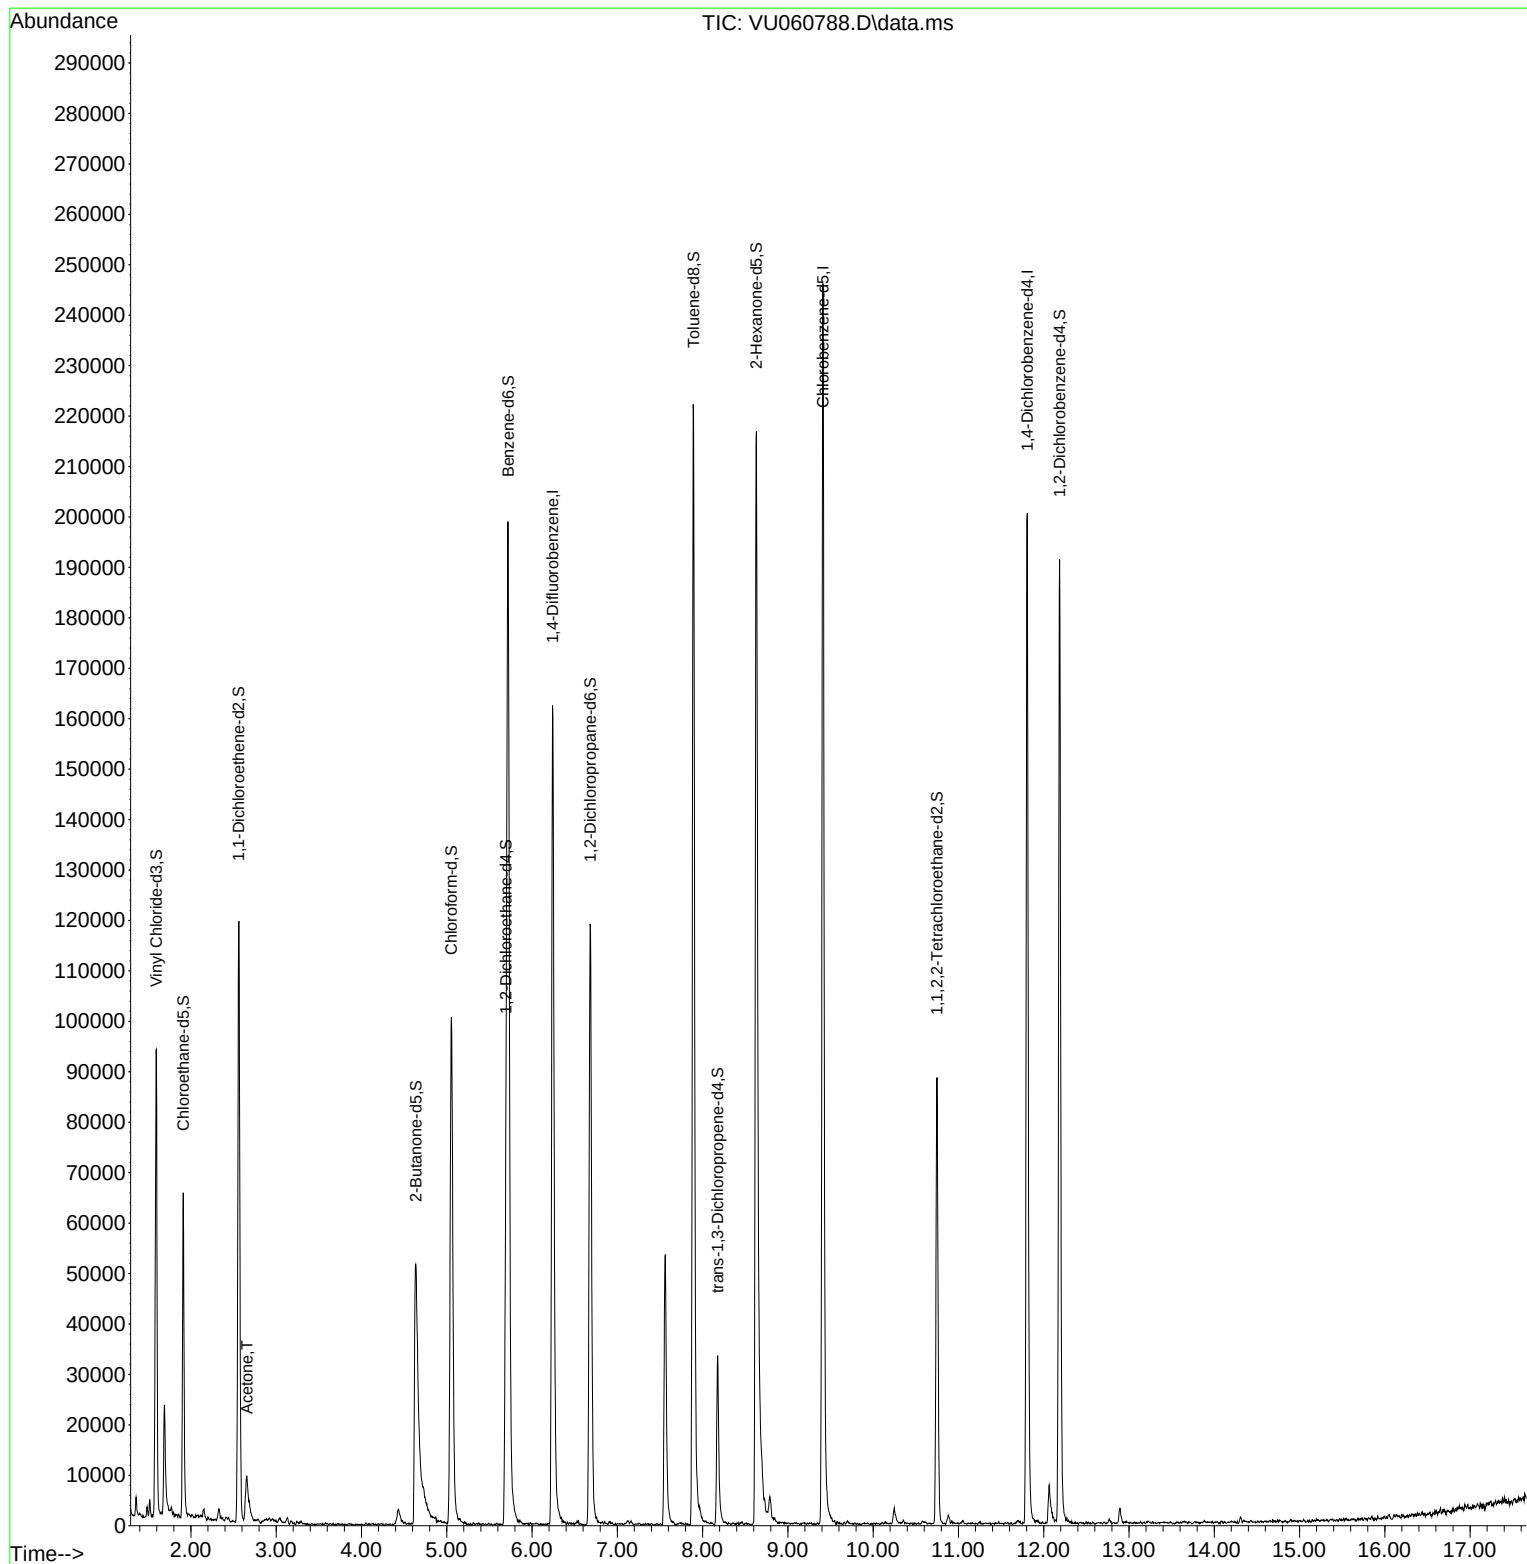

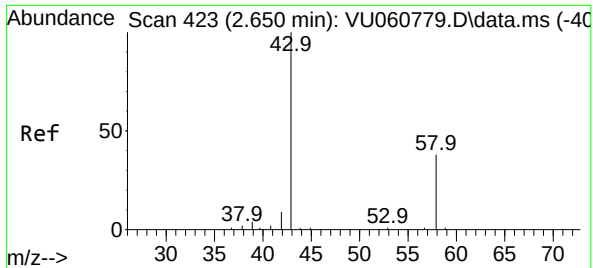

#13
 Acetone
 Concen: 12.559 ug/L
 RT: 2.657 min Scan# 41
 Delta R.T. 0.007 min
 Lab File: VU060788.D
 Acq: 16 Sep 2024 18:37

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Tgt Ion: 43 Resp: 17319
 Ion Ratio Lower Upper
 43 100
 58 38.3 0.0 69.6

