


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091624\
Data File : VU060772.D
Acq On : 16 Sep 2024 09:44
Operator : MD/SY
Sample : BFB197
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB197

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 18 02:40:24 2024

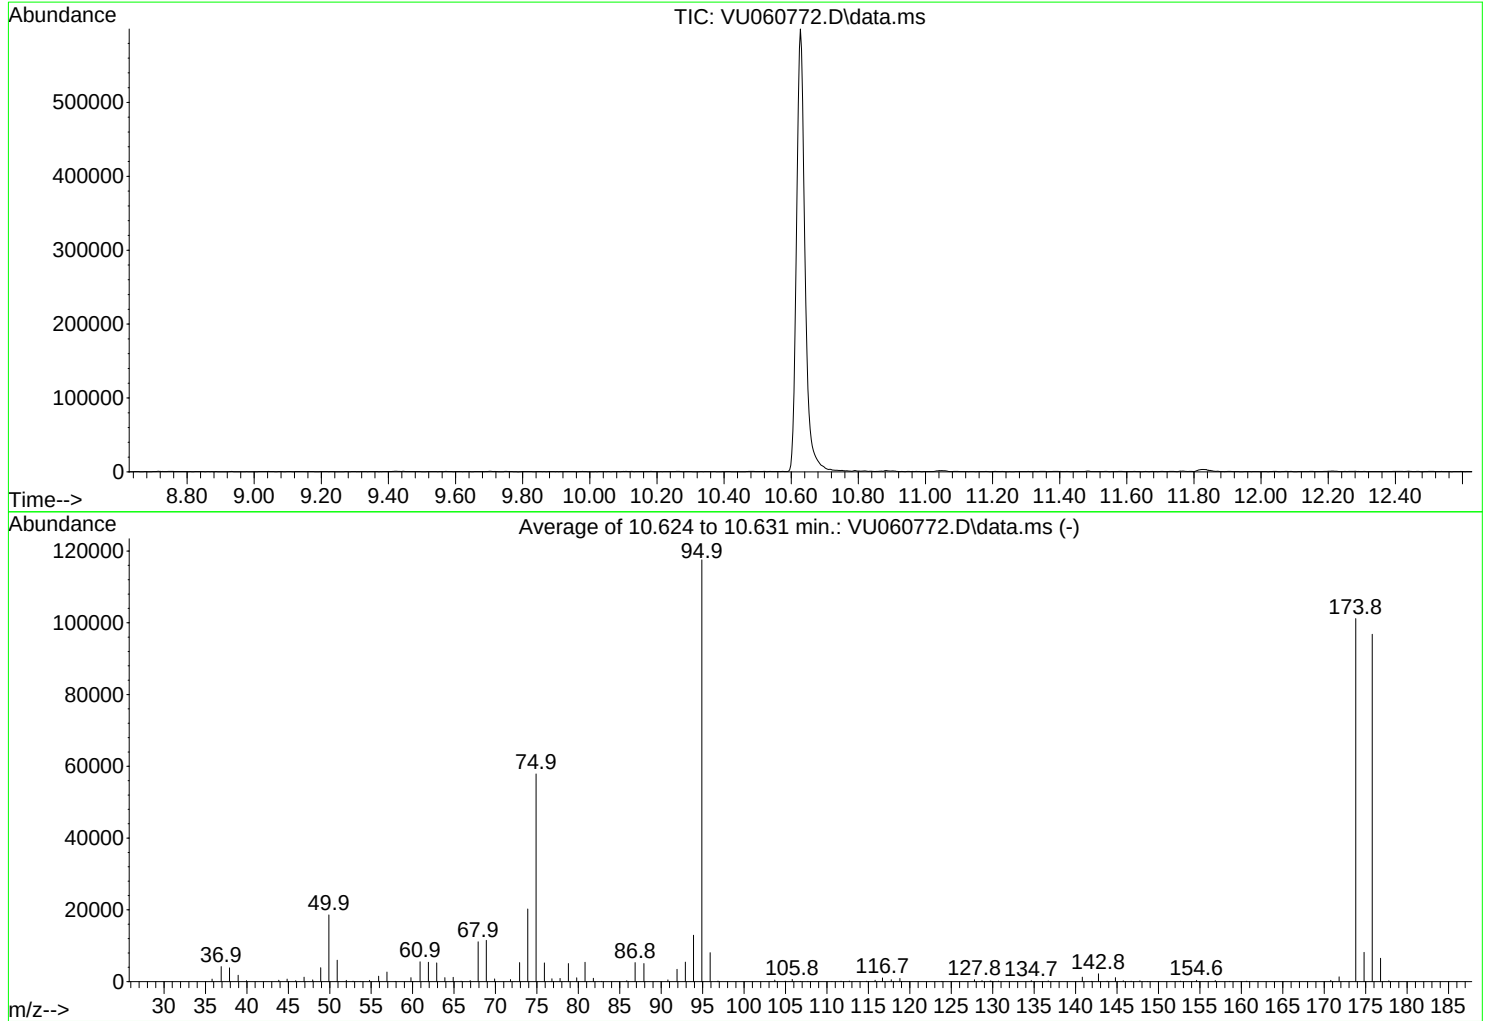

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	18595	PASS
75	95	30	80	49.2	57864	PASS
95	95	100	100	100.0	117539	PASS
96	95	5	9	6.9	8058	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.1	101165	PASS
175	174	5	9	8.1	8167	PASS
176	174	95	101	95.7	96805	PASS
177	176	5	9	6.7	6519	PASS

m/z	Abundance
39.70	149.0
43.90	394.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
35.80	747.0
36.90	4189.0
37.90	3840.0
38.90	1807.0
40.00	276.0
43.80	758.0
44.80	661.0
45.90	244.0
46.90	1297.0
47.90	522.0
48.90	3846.0
49.90	18840.0
50.90	6043.0
52.10	381.0
52.80	149.0
53.80	148.0
54.80	492.0
55.90	1530.0
56.90	2816.0
57.90	108.0
59.80	1195.0
60.90	5600.0
61.90	5236.0
62.90	5220.0
63.90	1034.0
64.90	1099.0
65.90	118.0
67.00	256.0
67.90	10977.0
68.90	11274.0
69.90	735.0
71.80	494.0
72.90	5033.0
73.90	20112.0
74.90	58080.0
75.90	5587.0
76.80	661.0
77.80	771.0
78.80	5232.0
79.80	1037.0
80.80	5411.0
81.80	948.0
82.80	122.0
85.90	355.0
86.80	5281.0
87.90	4954.0
90.80	532.0
91.90	3409.0
92.90	5282.0
93.90	13236.0
94.90	115848.0
95.90	7810.0
96.80	198.0
103.70	542.0
105.00	151.0
105.80	580.0
107.70	113.0
110.60	102.0
111.70	147.0
112.70	230.0
114.80	168.0
115.80	387.0
116.70	1134.0
117.80	557.0
118.80	892.0
123.80	116.0
127.80	596.0
128.70	319.0
129.70	369.0
130.70	196.0
134.70	280.0
136.70	167.0
140.80	1257.0
142.80	2164.0
143.80	139.0
144.80	1232.0
145.70	246.0
146.70	120.0
147.80	234.0
152.80	110.0
154.60	340.0
156.90	300.0
160.70	159.0
170.80	415.0
171.80	1331.0
173.80	98384.0
174.80	7979.0
175.80	93136.0
176.80	6317.0
177.80	262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
35.80	765.0
36.90	4318.0
37.90	3974.0
38.90	1826.0
40.00	281.0
43.90	807.0
44.90	693.0
45.90	307.0
46.90	1220.0
48.00	500.0
48.90	4052.0
49.90	19112.0
50.90	6165.0
52.00	367.0
52.80	158.0
53.70	139.0
54.80	389.0
55.90	1565.0
56.90	2673.0
59.80	1144.0
60.90	5593.0
61.90	5623.0
62.90	5444.0
63.90	1105.0
64.90	1285.0
65.80	107.0
66.90	309.0
67.90	11330.0
68.90	11955.0
69.90	753.0
71.80	607.0
72.90	5514.0
73.90	20920.0
74.90	59568.0
75.90	5316.0
76.80	851.0
77.80	944.0
78.80	5231.0
79.80	1119.0
80.80	5591.0
81.80	957.0
82.80	100.0
85.90	234.0
86.90	5502.0
87.90	5258.0
90.80	508.0
91.90	3537.0
92.90	5635.0
93.90	13022.0
94.90	121336.0
95.90	8372.0
96.80	187.0
103.70	463.0
104.90	151.0
105.80	657.0
106.80	138.0
107.70	109.0
111.70	167.0
112.70	196.0
114.80	163.0
115.80	403.0
116.70	1072.0
117.70	523.0
118.80	928.0
123.90	127.0
127.80	601.0
128.70	328.0
129.70	327.0
130.70	202.0
134.60	336.0
136.70	233.0
140.80	1298.0
141.90	178.0
142.80	2191.0
143.80	167.0
144.80	1119.0
145.80	275.0
146.70	127.0
147.80	281.0
148.70	116.0
152.60	122.0
154.60	416.0
156.90	326.0
158.60	140.0
160.70	153.0
170.70	339.0
171.80	1350.0
173.80	103968.0
174.80	8515.0
175.80	99824.0
176.80	6761.0
177.80	286.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197

m/z	Abundance
35.80	643.0
36.90	4032.0
37.90	3723.0
39.00	1682.0
39.90	288.0
43.90	846.0
44.90	825.0
45.90	273.0
46.90	1195.0
48.00	521.0
48.90	3790.0
49.90	17832.0
50.90	5756.0
51.90	303.0
52.80	128.0
54.80	259.0
55.90	1392.0
56.90	2583.0
57.90	124.0
59.80	991.0
60.90	5349.0
61.90	5346.0
62.90	5014.0
63.90	1159.0
64.90	1232.0
65.80	130.0
66.90	329.0
67.90	10957.0
68.90	11257.0
69.90	742.0
71.80	603.0
72.90	5338.0
73.90	19664.0
74.90	55944.0
75.90	4737.0
76.80	960.0
77.80	907.0
78.80	4688.0
79.80	1084.0
80.80	5205.0
81.80	884.0
82.80	117.0
85.70	157.0
86.90	5173.0
87.90	4902.0
90.80	397.0
91.90	3395.0
92.90	5425.0
93.90	12481.0
94.90	115432.0
95.90	7993.0
96.90	167.0
103.70	376.0
104.90	143.0
105.80	630.0
106.80	166.0
111.70	155.0
112.60	128.0
114.80	143.0
115.80	414.0
116.70	832.0
117.70	520.0
118.80	897.0
127.80	478.0
128.70	230.0
129.90	355.0
130.70	157.0
134.60	261.0
136.70	241.0
140.80	1199.0
141.90	164.0
142.70	2202.0
143.80	147.0
144.80	947.0
145.80	320.0
146.70	102.0
147.70	254.0
152.50	125.0
154.60	382.0
156.80	296.0
158.60	130.0
160.60	116.0
170.90	284.0
171.80	1314.0
173.80	101144.0
174.80	8006.0
175.80	97456.0
176.80	6480.0
177.80	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB197