

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050838.D
 Acq On : 20 Sep 2022 18:00
 Operator : JC/MD
 Sample : N4651-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB2	351687	438782	19.44%	2.329%
2	1.909	170	177	200	rVB	238458	322942	14.31%	1.714%
3	2.565	368	381	397	rBV	447051	740511	32.82%	3.931%
4	2.745	434	437	441	rBV3	688	624	0.03%	0.003%
5	2.790	443	451	459	rBV4	2698	4866	0.22%	0.026%
6	2.964	499	505	510	rVB4	1274	1327	0.06%	0.007%
7	3.044	522	530	540	rVB7	1932	3510	0.16%	0.019%
8	3.086	540	543	548	rVB2	578	351	0.02%	0.002%
9	3.134	555	558	563	rVB3	739	512	0.02%	0.003%
10	3.170	564	569	570	rBV2	1161	914	0.04%	0.005%
11	3.353	611	626	641	rBV2	28866	57102	2.53%	0.303%
12	3.465	657	661	664	rBV2	587	477	0.02%	0.003%
13	3.655	713	720	726	rBV3	494	859	0.04%	0.005%
14	3.710	733	737	743	rBV2	459	508	0.02%	0.003%
15	3.867	768	786	810	rBV	384780	911024	40.37%	4.836%
16	4.018	830	833	837	rVB3	622	368	0.02%	0.002%
17	4.404	950	953	956	rVV3	527	343	0.02%	0.002%
18	4.575	1001	1006	1008	rBV3	416	348	0.02%	0.002%
19	4.665	1009	1034	1064	rBV2	788247	2256555	100.00%	11.978%
20	5.063	1141	1158	1179	rBV	368504	807983	35.81%	4.289%
21	5.314	1221	1236	1253	rBV	213629	479949	21.27%	2.548%
22	5.456	1273	1280	1281	rBV4	427	466	0.02%	0.002%
23	5.526	1297	1302	1305	rVB4	599	613	0.03%	0.003%
24	5.613	1324	1329	1335	rBV3	256	361	0.02%	0.002%
25	5.722	1342	1363	1396	rBV2	774259	2115417	93.75%	11.228%
26	6.047	1460	1464	1469	rVV3	849	814	0.04%	0.004%
27	6.076	1469	1473	1479	rVV3	540	565	0.03%	0.003%
28	6.124	1486	1488	1493	rVB3	838	612	0.03%	0.003%
29	6.247	1511	1526	1554	rBV	609748	1160579	51.43%	6.160%
30	6.542	1603	1618	1637	rBV3	101972	196779	8.72%	1.044%
31	6.690	1649	1664	1683	rBV	488233	949979	42.10%	5.042%
32	6.899	1727	1729	1732	rVB2	641	360	0.02%	0.002%
33	6.941	1738	1742	1748	rVB3	606	523	0.02%	0.003%
34	6.973	1748	1752	1753	rBV3	1047	656	0.03%	0.003%
35	7.002	1754	1761	1763	rBV5	1990	2745	0.12%	0.015%
36	7.086	1783	1787	1791	rBV2	694	788	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050838.D
 Acq On : 20 Sep 2022 18:00
 Operator : JC/MD
 Sample : N4651-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.192	1808	1820	1824	rBV5	2129	3429	0.15%	0.018%
38	7.247	1834	1837	1849	rVB2	582	765	0.03%	0.004%
39	7.417	1885	1890	1895	rBV	445	388	0.02%	0.002%
40	7.449	1895	1900	1904	rVB2	518	524	0.02%	0.003%
41	7.565	1923	1936	1956	rBV	247264	438577	19.44%	2.328%
42	7.793	2003	2007	2011	rBV4	841	865	0.04%	0.005%
43	7.896	2025	2039	2055	rBV	881404	1517297	67.24%	8.054%
44	8.179	2115	2127	2144	rBV	175367	295505	13.10%	1.569%
45	8.401	2187	2196	2206	rBV8	3954	6747	0.30%	0.036%
46	8.472	2209	2218	2219	rBV6	1480	1492	0.07%	0.008%
47	8.552	2232	2243	2256	rVB3	69318	116699	5.17%	0.619%
48	8.632	2256	2268	2307	rBV2	622275	1193344	52.88%	6.334%
49	8.992	2376	2380	2383	rBV3	469	441	0.02%	0.002%
50	9.131	2418	2423	2428	rBV3	500	430	0.02%	0.002%
51	9.163	2429	2433	2436	rBV4	539	509	0.02%	0.003%
52	9.263	2461	2464	2467	rBV3	568	391	0.02%	0.002%
53	9.417	2498	2512	2544	rBV	828274	1383493	61.31%	7.343%
54	9.571	2555	2560	2563	rBV5	998	800	0.04%	0.004%
55	9.687	2590	2596	2597	rBV3	990	933	0.04%	0.005%
56	9.700	2597	2600	2608	rVB5	1649	1569	0.07%	0.008%
57	9.764	2616	2620	2622	rBV3	751	513	0.02%	0.003%
58	9.957	2675	2680	2684	rBV2	345	387	0.02%	0.002%
59	9.976	2684	2686	2690	rBV4	421	337	0.01%	0.002%
60	10.041	2704	2706	2714	rVV2	485	605	0.03%	0.003%
61	10.115	2720	2729	2737	rVB6	1561	2763	0.12%	0.015%
62	10.176	2744	2748	2754	rBV3	343	483	0.02%	0.003%
63	10.365	2801	2807	2811	rBV2	255	334	0.01%	0.002%
64	10.404	2812	2819	2823	rVB3	463	562	0.02%	0.003%
65	10.478	2838	2842	2845	rBV2	539	421	0.02%	0.002%
66	10.494	2845	2847	2854	rVB2	624	499	0.02%	0.003%
67	10.668	2890	2901	2910	rVB6	2733	4777	0.21%	0.025%
68	10.754	2914	2928	2952	rBV	667226	1073153	47.56%	5.696%
69	10.844	2952	2956	2960	rVB3	686	552	0.02%	0.003%
70	10.867	2960	2963	2966	rBV3	1109	854	0.04%	0.005%
71	10.889	2966	2970	2975	rBV3	832	802	0.04%	0.004%
72	11.037	3013	3016	3021	rVB2	392	337	0.01%	0.002%
73	11.089	3026	3032	3034	rBV	1158	935	0.04%	0.005%
74	11.410	3129	3132	3135	rVB	596	384	0.02%	0.002%
75	11.462	3138	3148	3156	rBV10	2905	6368	0.28%	0.034%
76	11.700	3215	3222	3229	rVB4	1509	2168	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050838.D
 Acq On : 20 Sep 2022 18:00
 Operator : JC/MD
 Sample : N4651-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.745	3231	3236	3244	rVB5	2023	2746	0.12%	0.015%
78	11.812	3244	3257	3281	rBV	670511	1083911	48.03%	5.753%
79	12.063	3329	3335	3347	rVB9	2482	4746	0.21%	0.025%
80	12.192	3361	3375	3401	rBV	736254	1193868	52.91%	6.337%
81	12.397	3437	3439	3441	rBV3	679	373	0.02%	0.002%
82	12.426	3446	3448	3453	rVB2	690	453	0.02%	0.002%
83	12.639	3509	3514	3516	rBV2	469	433	0.02%	0.002%
84	12.709	3533	3536	3538	rBV3	515	333	0.01%	0.002%
85	12.764	3552	3553	3560	rVB4	503	420	0.02%	0.002%
86	12.909	3595	3598	3601	rVB4	554	435	0.02%	0.002%
87	12.925	3601	3603	3608	rVB	610	472	0.02%	0.003%
88	13.012	3627	3630	3634	rBV3	686	461	0.02%	0.002%
89	13.111	3659	3661	3665	rVB2	798	445	0.02%	0.002%
90	13.147	3670	3672	3677	rBV3	675	543	0.02%	0.003%
91	13.224	3691	3696	3702	rVB5	2401	2486	0.11%	0.013%
92	13.471	3769	3773	3775	rBV3	543	478	0.02%	0.003%
93	13.645	3825	3827	3832	rVB3	954	615	0.03%	0.003%
94	13.677	3832	3837	3839	rBV2	464	431	0.02%	0.002%
95	13.712	3845	3848	3850	rBV2	572	358	0.02%	0.002%
96	13.844	3882	3889	3899	rVB8	4171	5712	0.25%	0.030%
97	13.989	3929	3934	3936	rBV3	1720	1512	0.07%	0.008%
98	14.092	3956	3966	3978	rBV	6120	9711	0.43%	0.052%
99	14.330	4033	4040	4051	rVB5	3632	6003	0.27%	0.032%
100	14.523	4097	4100	4103	rBV2	578	452	0.02%	0.002%




Sum of corrected areas: 18839941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050838.D
Acq On : 20 Sep 2022 18:00
Operator : JC/MD
Sample : N4651-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

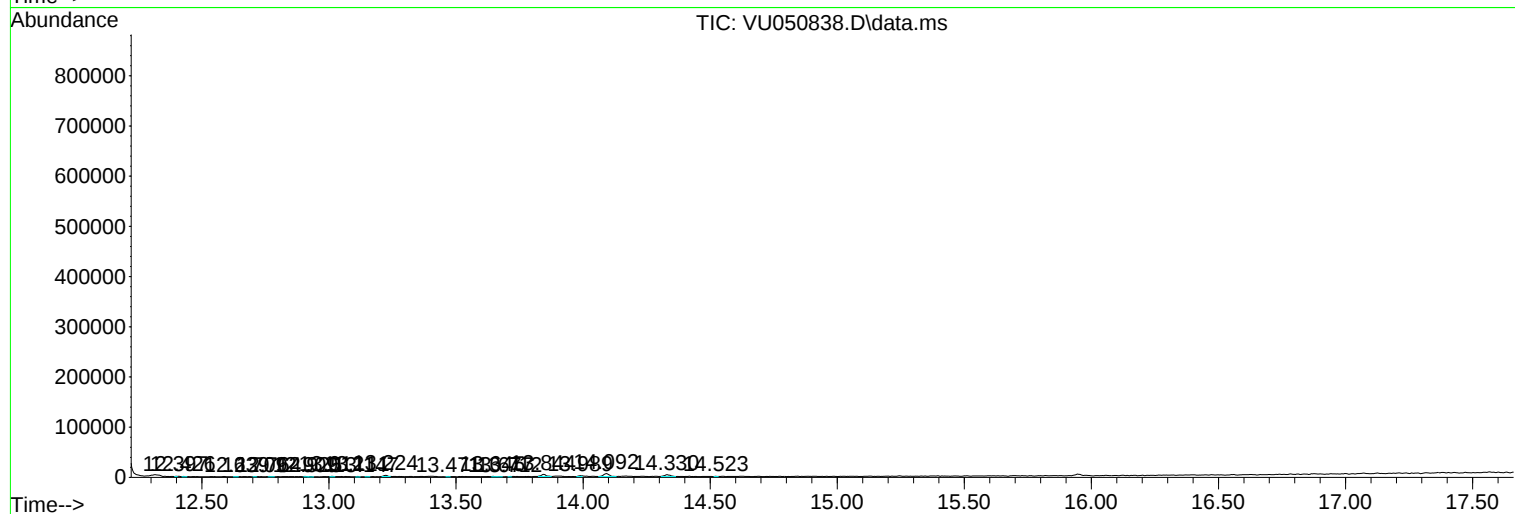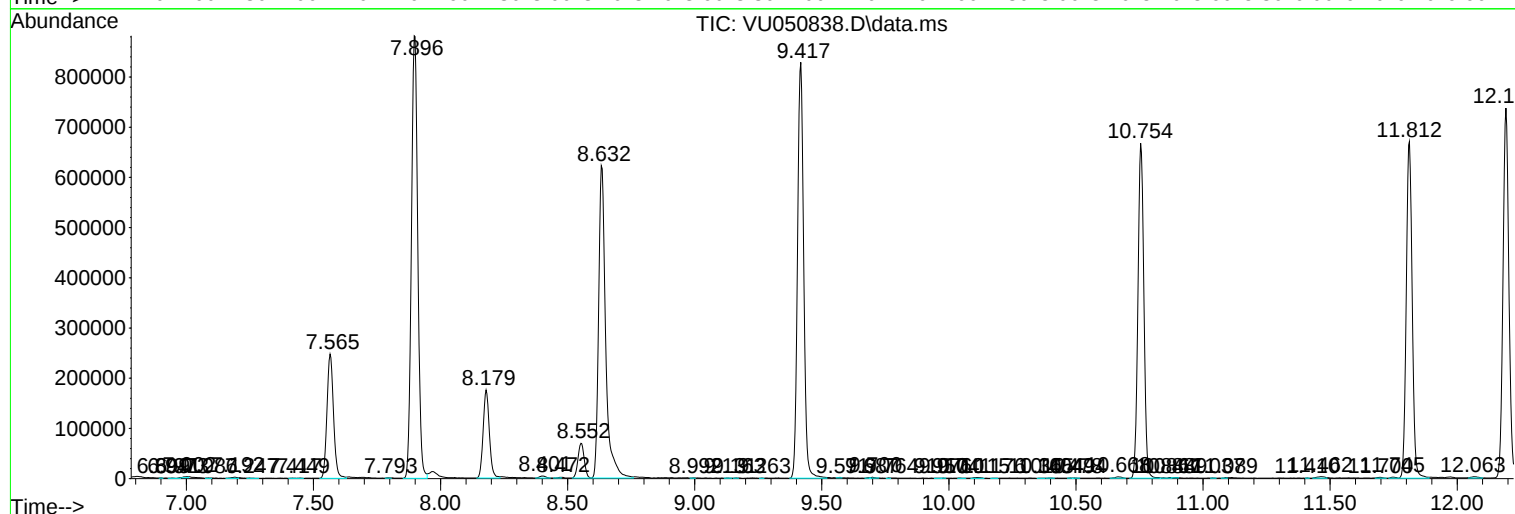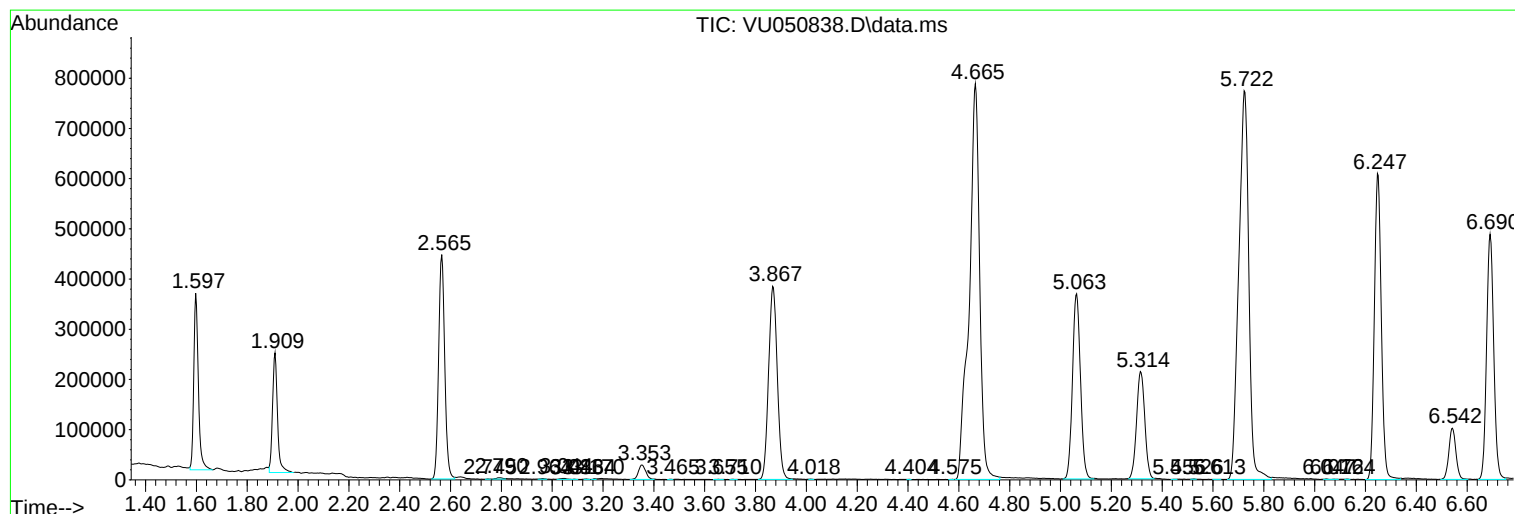

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050838.D
Acq On : 20 Sep 2022 18:00
Operator : JC/MD
Sample : N4651-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050838.D
Acq On : 20 Sep 2022 18:00
Operator : JC/MD
Sample : N4651-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------