

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050840.D
 Acq On : 20 Sep 2022 18:47
 Operator : JC/MD
 Sample : N4651-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	271374	316775	16.37%	2.211%
2	1.906	168	176	199	rVB	203328	282917	14.62%	1.975%
3	2.482	352	355	358	rBV3	982	802	0.04%	0.006%
4	2.565	367	381	395	rBV	404938	670415	34.65%	4.679%
5	2.768	432	444	459	rBV3	11478	26933	1.39%	0.188%
6	2.842	464	467	469	rBV2	519	334	0.02%	0.002%
7	2.900	483	485	488	rVB3	641	345	0.02%	0.002%
8	3.041	523	529	533	rBV4	1573	1662	0.09%	0.012%
9	3.183	562	573	585	rVB6	2711	6225	0.32%	0.043%
10	3.356	625	627	632	rVB2	815	579	0.03%	0.004%
11	3.707	732	736	739	rVB2	459	324	0.02%	0.002%
12	3.845	775	779	781	rBV2	414	314	0.02%	0.002%
13	3.867	781	786	789	rBV2	1016	902	0.05%	0.006%
14	3.973	816	819	825	rVB2	484	325	0.02%	0.002%
15	4.018	825	833	837	rBV2	270	435	0.02%	0.003%
16	4.179	879	883	887	rVV3	361	376	0.02%	0.003%
17	4.385	942	947	958	rBV2	319	462	0.02%	0.003%
18	4.572	1001	1005	1007	rBV2	581	456	0.02%	0.003%
19	4.620	1007	1020	1045	rBV	208477	511482	26.44%	3.570%
20	4.906	1107	1109	1112	rBV2	517	318	0.02%	0.002%
21	4.967	1125	1128	1135	rVB3	637	565	0.03%	0.004%
22	5.060	1141	1157	1180	rBV	342108	754997	39.03%	5.269%
23	5.314	1221	1236	1251	rVB2	53906	121924	6.30%	0.851%
24	5.404	1262	1264	1268	rBV3	539	413	0.02%	0.003%
25	5.430	1268	1272	1278	rVB3	557	556	0.03%	0.004%
26	5.469	1278	1284	1286	rBV	322	315	0.02%	0.002%
27	5.485	1287	1289	1293	rVV	412	349	0.02%	0.002%
28	5.559	1305	1312	1314	rVV2	331	364	0.02%	0.003%
29	5.723	1341	1363	1398	rBV2	718506	1934565	100.00%	13.502%
30	6.115	1482	1485	1489	rVV3	735	574	0.03%	0.004%
31	6.137	1489	1492	1495	rVB3	483	355	0.02%	0.002%
32	6.247	1512	1526	1547	rBV	564700	1064895	55.05%	7.432%
33	6.530	1601	1614	1628	rVB10	6342	13131	0.68%	0.092%
34	6.604	1634	1637	1638	rBV2	576	359	0.02%	0.003%
35	6.690	1648	1664	1683	rBV	456239	890298	46.02%	6.214%
36	6.880	1721	1723	1726	rVB3	706	317	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050840.D
 Acq On : 20 Sep 2022 18:47
 Operator : JC/MD
 Sample : N4651-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.925	1735	1737	1743	rVB3	571	526	0.03%	0.004%
38	6.973	1745	1752	1755	rBV4	893	894	0.05%	0.006%
39	7.022	1765	1767	1772	rBV	492	508	0.03%	0.004%
40	7.073	1781	1783	1788	rVB3	499	383	0.02%	0.003%
41	7.189	1811	1819	1821	rBV4	1299	1412	0.07%	0.010%
42	7.202	1821	1823	1828	rVB	1150	683	0.04%	0.005%
43	7.404	1881	1886	1890	rBV2	419	463	0.02%	0.003%
44	7.565	1921	1936	1957	rBV	228104	403661	20.87%	2.817%
45	7.694	1970	1976	1978	rBV4	1051	1037	0.05%	0.007%
46	7.896	2025	2039	2055	rBV	818650	1407070	72.73%	9.820%
47	8.121	2106	2109	2112	rBV2	507	379	0.02%	0.003%
48	8.179	2115	2127	2145	rBV	161173	272636	14.09%	1.903%
49	8.333	2172	2175	2178	rVB4	604	418	0.02%	0.003%
50	8.395	2190	2194	2195	rBV	561	411	0.02%	0.003%
51	8.468	2213	2217	2218	rVV2	913	737	0.04%	0.005%
52	8.478	2218	2220	2224	rVB2	1379	784	0.04%	0.005%
53	8.552	2234	2243	2252	rVB4	9682	15216	0.79%	0.106%
54	8.632	2252	2268	2299	rBV2	587789	1099548	56.84%	7.674%
55	8.787	2314	2316	2326	rVB8	2386	3038	0.16%	0.021%
56	9.205	2443	2446	2450	rBV2	494	365	0.02%	0.003%
57	9.279	2464	2469	2472	rBV3	609	526	0.03%	0.004%
58	9.417	2499	2512	2541	rBV	776275	1294800	66.93%	9.037%
59	9.565	2553	2558	2562	rBV5	869	767	0.04%	0.005%
60	9.629	2576	2578	2584	rVV3	720	614	0.03%	0.004%
61	9.697	2592	2599	2608	rVB4	1480	2218	0.11%	0.015%
62	9.822	2633	2638	2643	rBV4	560	680	0.04%	0.005%
63	9.874	2648	2654	2656	rBV2	461	528	0.03%	0.004%
64	10.018	2694	2699	2702	rBV2	390	361	0.02%	0.003%
65	10.112	2723	2728	2730	rBV3	629	482	0.02%	0.003%
66	10.256	2770	2773	2777	rVB	496	327	0.02%	0.002%
67	10.671	2893	2902	2909	rBV4	2548	3719	0.19%	0.026%
68	10.755	2916	2928	2945	rBV	633372	1014303	52.43%	7.079%
69	10.973	2993	2996	3001	rBV	392	369	0.02%	0.003%
70	11.038	3012	3016	3018	rBV2	479	312	0.02%	0.002%
71	11.086	3026	3031	3032	rBV2	824	633	0.03%	0.004%
72	11.407	3127	3131	3137	rVB3	573	626	0.03%	0.004%
73	11.452	3137	3145	3146	rBV4	1427	1348	0.07%	0.009%
74	11.578	3180	3184	3189	rVV2	663	606	0.03%	0.004%
75	11.697	3215	3221	3227	rVB5	1162	1483	0.08%	0.010%
76	11.738	3227	3234	3241	rBV5	1470	2324	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050840.D
 Acq On : 20 Sep 2022 18:47
 Operator : JC/MD
 Sample : N4651-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3282	rBV	635348	1017373	52.59%	7.100%
78	12.066	3328	3336	3346	rBV7	3384	6104	0.32%	0.043%
79	12.192	3358	3375	3400	rBV	688628	1134259	58.63%	7.916%
80	12.317	3406	3414	3418	rBV4	3862	5835	0.30%	0.041%
81	12.890	3585	3592	3594	rBV4	407	501	0.03%	0.003%
82	12.912	3597	3599	3604	rVB4	476	310	0.02%	0.002%
83	13.102	3655	3658	3660	rBV3	592	495	0.03%	0.003%
84	13.131	3665	3667	3671	rVV2	684	354	0.02%	0.002%
85	13.150	3671	3673	3676	rVB2	695	385	0.02%	0.003%
86	13.221	3690	3695	3702	rVB3	1146	1398	0.07%	0.010%
87	13.288	3714	3716	3719	rBV2	675	373	0.02%	0.003%
88	13.597	3806	3812	3815	rBV3	476	491	0.03%	0.003%
89	13.703	3842	3845	3849	rBV2	475	374	0.02%	0.003%
90	13.754	3858	3861	3865	rVB2	769	603	0.03%	0.004%
91	13.812	3877	3879	3883	rVV2	599	375	0.02%	0.003%
92	13.848	3885	3890	3896	rVV6	1947	2395	0.12%	0.017%
93	13.909	3905	3909	3911	rBV3	524	484	0.03%	0.003%
94	13.989	3929	3934	3941	rBV6	1528	2235	0.12%	0.016%
95	14.095	3958	3967	3975	rBV3	3694	5364	0.28%	0.037%
96	14.246	4011	4014	4019	rVB3	637	557	0.03%	0.004%
97	14.475	4082	4085	4088	rBV2	641	400	0.02%	0.003%
98	14.684	4147	4150	4155	rBV3	524	557	0.03%	0.004%
99	15.346	4352	4356	4358	rBV2	771	743	0.04%	0.005%
100	15.941	4538	4541	4546	rBV5	2944	2702	0.14%	0.019%




Sum of corrected areas: 14328220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050840.D
Acq On : 20 Sep 2022 18:47
Operator : JC/MD
Sample : N4651-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

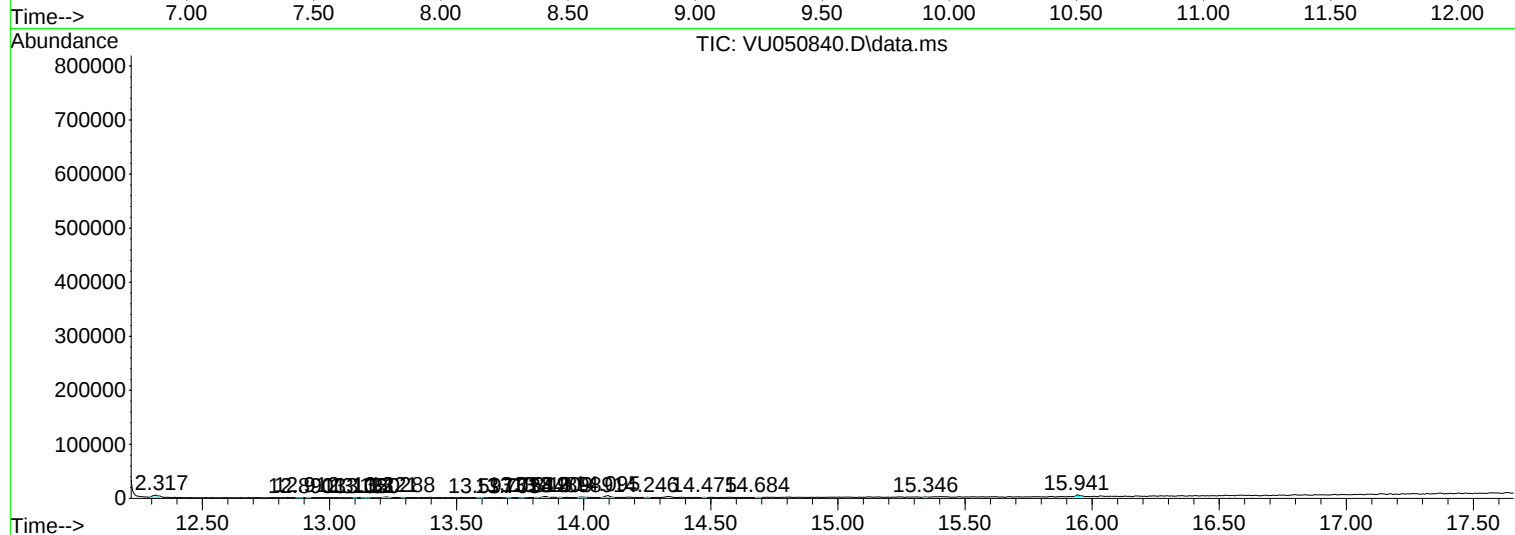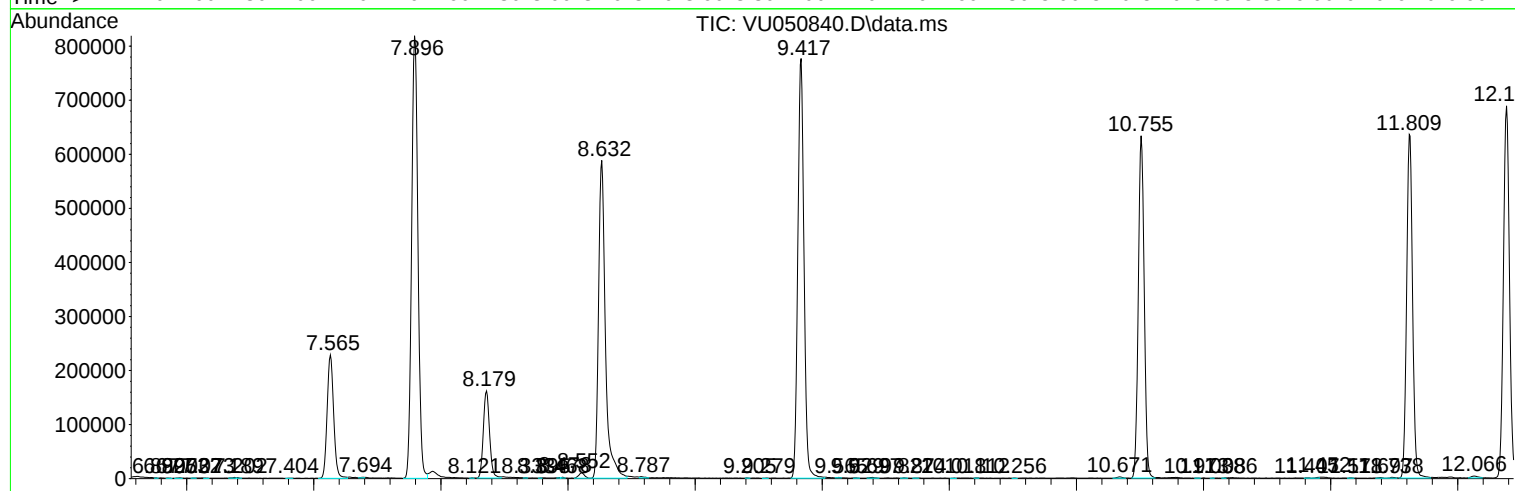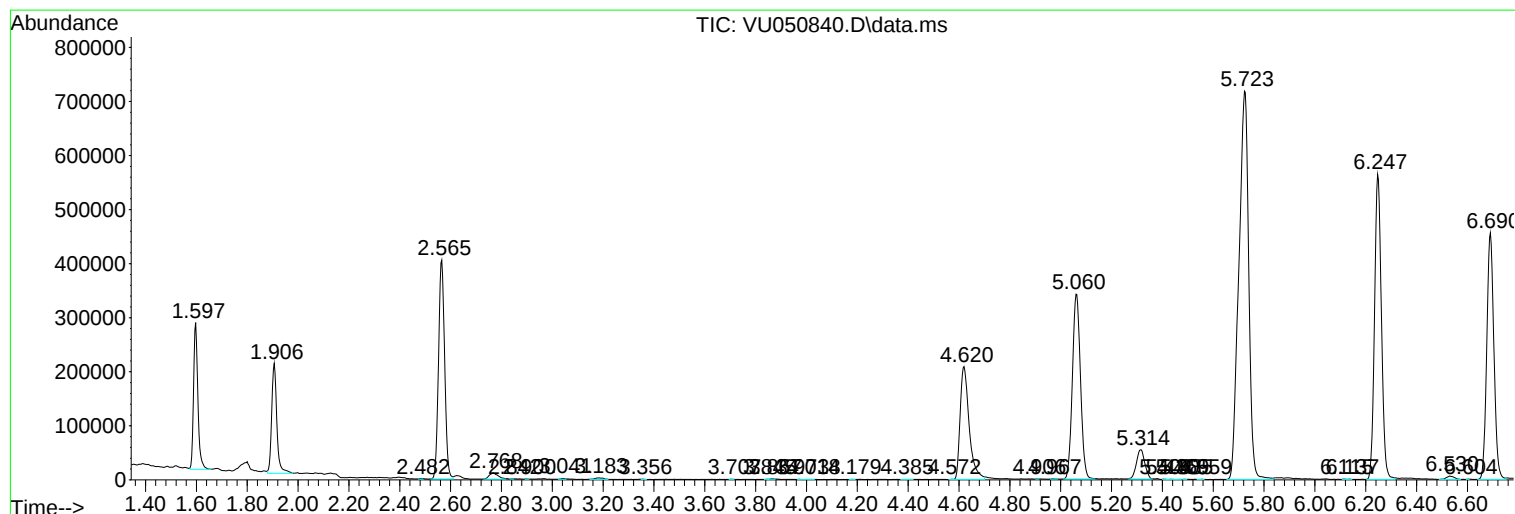

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050840.D
Acq On : 20 Sep 2022 18:47
Operator : JC/MD
Sample : N4651-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050840.D
Acq On : 20 Sep 2022 18:47
Operator : JC/MD
Sample : N4651-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------