

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050841.D
 Acq On : 20 Sep 2022 19:10
 Operator : JC/MD
 Sample : N4651-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	278210	336104	16.53%	2.236%
2	1.906	168	176	201	rVB	211343	289920	14.26%	1.929%
3	2.565	368	381	395	rBV	430532	715630	35.19%	4.760%
4	2.777	433	447	461	rBV3	5754	17245	0.85%	0.115%
5	2.954	495	502	513	rVB6	1490	2758	0.14%	0.018%
6	3.038	521	528	529	rBV6	1653	1473	0.07%	0.010%
7	3.118	548	553	556	rBV	441	422	0.02%	0.003%
8	3.186	564	574	578	rBV5	1549	2847	0.14%	0.019%
9	3.343	620	623	624	rBV	733	401	0.02%	0.003%
10	3.703	726	735	736	rBV2	546	505	0.02%	0.003%
11	3.813	765	769	772	rBV2	373	334	0.02%	0.002%
12	3.871	774	787	800	rVV	5651	12033	0.59%	0.080%
13	4.237	894	901	903	rBV2	334	384	0.02%	0.003%
14	4.301	918	921	926	rBV	391	362	0.02%	0.002%
15	4.392	946	949	954	rBV	374	377	0.02%	0.003%
16	4.620	1008	1020	1051	rBV	214433	539338	26.52%	3.588%
17	4.967	1125	1128	1132	rVB4	344	324	0.02%	0.002%
18	5.060	1139	1157	1181	rBV	360714	798466	39.26%	5.312%
19	5.163	1187	1189	1193	rBV	533	384	0.02%	0.003%
20	5.202	1199	1201	1203	rBV2	552	334	0.02%	0.002%
21	5.314	1220	1236	1255	rBV2	168801	378904	18.63%	2.521%
22	5.530	1299	1303	1306	rBV2	691	616	0.03%	0.004%
23	5.723	1341	1363	1389	rBV2	755431	2033540	100.00%	13.527%
24	6.031	1456	1459	1464	rVB3	595	566	0.03%	0.004%
25	6.105	1479	1482	1484	rBV3	617	428	0.02%	0.003%
26	6.141	1490	1493	1495	rVB3	731	397	0.02%	0.003%
27	6.247	1510	1526	1546	rBV	560710	1065388	52.39%	7.087%
28	6.353	1556	1559	1561	rBV3	794	479	0.02%	0.003%
29	6.469	1592	1595	1599	rVB3	458	378	0.02%	0.003%
30	6.491	1599	1602	1605	rBV3	706	326	0.02%	0.002%
31	6.536	1605	1616	1627	rVB9	7387	15063	0.74%	0.100%
32	6.581	1627	1630	1631	rBV2	893	418	0.02%	0.003%
33	6.591	1631	1633	1639	rVB3	774	486	0.02%	0.003%
34	6.690	1649	1664	1686	rBV	472181	926291	45.55%	6.162%
35	6.948	1742	1744	1748	rVB3	455	323	0.02%	0.002%
36	7.044	1769	1774	1778	rBV3	845	867	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050841.D
 Acq On : 20 Sep 2022 19:10
 Operator : JC/MD
 Sample : N4651-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.063	1778	1780	1786	rVB2	621	441	0.02%	0.003%
38	7.186	1810	1818	1820	rBV3	1530	1758	0.09%	0.012%
39	7.395	1878	1883	1887	rBV2	362	390	0.02%	0.003%
40	7.565	1923	1936	1953	rBV	240783	421045	20.71%	2.801%
41	7.690	1972	1975	1979	rVB5	840	587	0.03%	0.004%
42	7.771	1996	2000	2006	rBV3	527	489	0.02%	0.003%
43	7.800	2006	2009	2011	rBV	452	399	0.02%	0.003%
44	7.896	2025	2039	2055	rBV	867614	1475130	72.54%	9.813%
45	8.179	2115	2127	2146	rBV	165963	282014	13.87%	1.876%
46	8.401	2193	2196	2200	rBV4	576	477	0.02%	0.003%
47	8.469	2212	2217	2230	rVB5	1957	3231	0.16%	0.021%
48	8.552	2233	2243	2254	rVB3	19863	32015	1.57%	0.213%
49	8.633	2255	2268	2299	rBV2	613099	1147068	56.41%	7.630%
50	8.986	2374	2378	2380	rBV3	665	538	0.03%	0.004%
51	9.005	2380	2384	2387	rVV5	767	633	0.03%	0.004%
52	9.173	2434	2436	2440	rVB2	775	518	0.03%	0.003%
53	9.337	2484	2487	2491	rBV3	367	320	0.02%	0.002%
54	9.417	2498	2512	2542	rBV	786208	1297444	63.80%	8.631%
55	9.568	2557	2559	2566	rVB3	899	848	0.04%	0.006%
56	9.607	2567	2571	2576	rVB3	777	639	0.03%	0.004%
57	9.690	2593	2597	2598	rBV3	813	573	0.03%	0.004%
58	9.816	2630	2636	2638	rBV	352	328	0.02%	0.002%
59	9.980	2684	2687	2692	rVB2	455	349	0.02%	0.002%
60	10.099	2721	2724	2726	rBV2	1025	626	0.03%	0.004%
61	10.304	2785	2788	2795	rBV3	653	794	0.04%	0.005%
62	10.475	2838	2841	2844	rBV	481	318	0.02%	0.002%
63	10.674	2895	2903	2912	rVB5	2171	3247	0.16%	0.022%
64	10.755	2914	2928	2948	rBV	650168	1045611	51.42%	6.956%
65	10.877	2959	2966	2968	rBV5	894	1024	0.05%	0.007%
66	11.218	3068	3072	3077	rBV3	489	469	0.02%	0.003%
67	11.285	3091	3093	3100	rBV3	336	393	0.02%	0.003%
68	11.411	3128	3132	3135	rBV3	467	316	0.02%	0.002%
69	11.459	3139	3147	3149	rBV3	1838	2727	0.13%	0.018%
70	11.555	3174	3177	3180	rBV2	495	314	0.02%	0.002%
71	11.575	3180	3183	3185	rBV	713	487	0.02%	0.003%
72	11.697	3214	3221	3228	rBV5	1031	1526	0.08%	0.010%
73	11.742	3231	3235	3236	rBV4	741	447	0.02%	0.003%
74	11.751	3236	3238	3243	rVB	995	546	0.03%	0.004%
75	11.809	3243	3256	3275	rBV	618773	991020	48.73%	6.592%
76	12.066	3328	3336	3343	rVV9	2843	4806	0.24%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050841.D
 Acq On : 20 Sep 2022 19:10
 Operator : JC/MD
 Sample : N4651-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3392	rBV	717452	1150858	56.59%	7.656%
78	12.356	3424	3426	3434	rVB3	930	718	0.04%	0.005%
79	12.523	3475	3478	3481	rBV	445	317	0.02%	0.002%
80	12.584	3494	3497	3501	rVB	588	397	0.02%	0.003%
81	12.716	3535	3538	3541	rVB3	609	370	0.02%	0.002%
82	12.767	3548	3554	3556	rBV3	693	733	0.04%	0.005%
83	12.854	3577	3581	3584	rBV3	690	527	0.03%	0.004%
84	12.896	3591	3594	3595	rBV2	773	406	0.02%	0.003%
85	13.124	3659	3665	3668	rBV3	776	909	0.04%	0.006%
86	13.224	3690	3696	3700	rBV4	1194	1234	0.06%	0.008%
87	13.259	3704	3707	3708	rBV2	666	377	0.02%	0.003%
88	13.507	3781	3784	3789	rBV2	484	390	0.02%	0.003%
89	13.697	3840	3843	3847	rBV2	422	369	0.02%	0.002%
90	13.848	3886	3890	3897	rVB6	1612	1874	0.09%	0.012%
91	13.893	3898	3904	3907	rBV5	667	894	0.04%	0.006%
92	13.909	3907	3909	3914	rBV3	478	383	0.02%	0.003%
93	14.089	3959	3965	3966	rBV4	1916	1583	0.08%	0.011%
94	14.179	3991	3993	3997	rVB3	750	473	0.02%	0.003%
95	14.272	4018	4022	4028	rVB3	689	698	0.03%	0.005%
96	14.330	4036	4040	4044	rBV3	1567	1307	0.06%	0.009%
97	14.378	4051	4055	4057	rBV2	456	362	0.02%	0.002%
98	14.571	4111	4115	4119	rBV4	563	627	0.03%	0.004%
99	14.999	4244	4248	4250	rBV2	798	541	0.03%	0.004%
100	15.012	4250	4252	4257	rVV3	512	395	0.02%	0.003%




Sum of corrected areas: 15032758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050841.D
Acq On : 20 Sep 2022 19:10
Operator : JC/MD
Sample : N4651-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

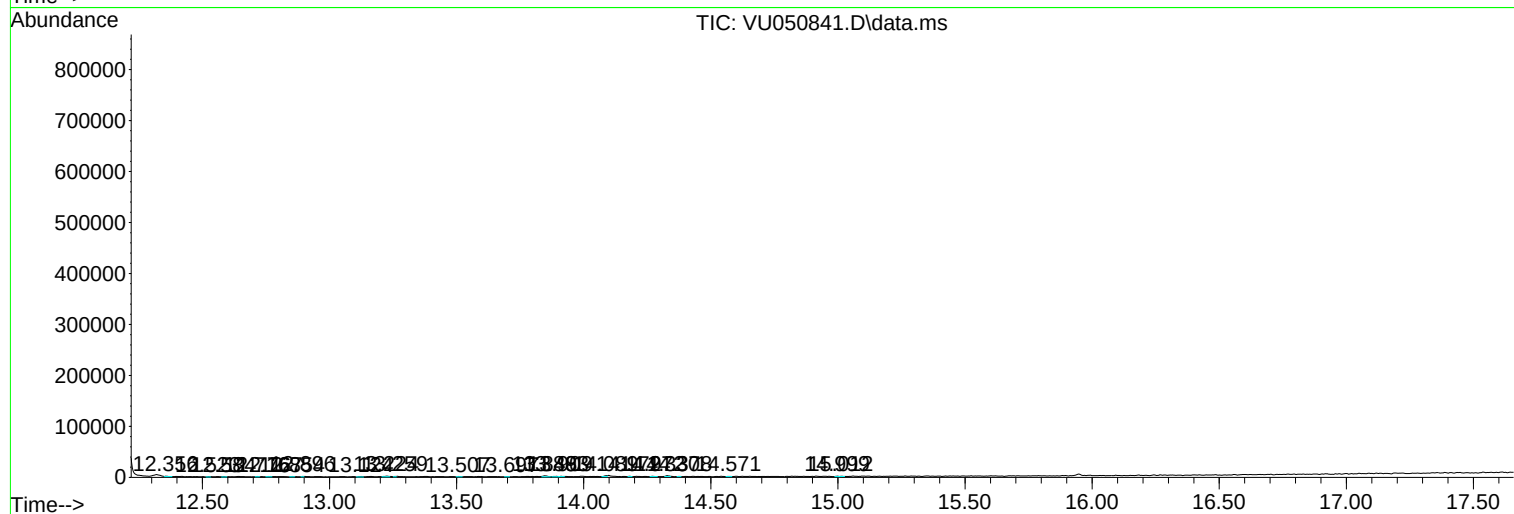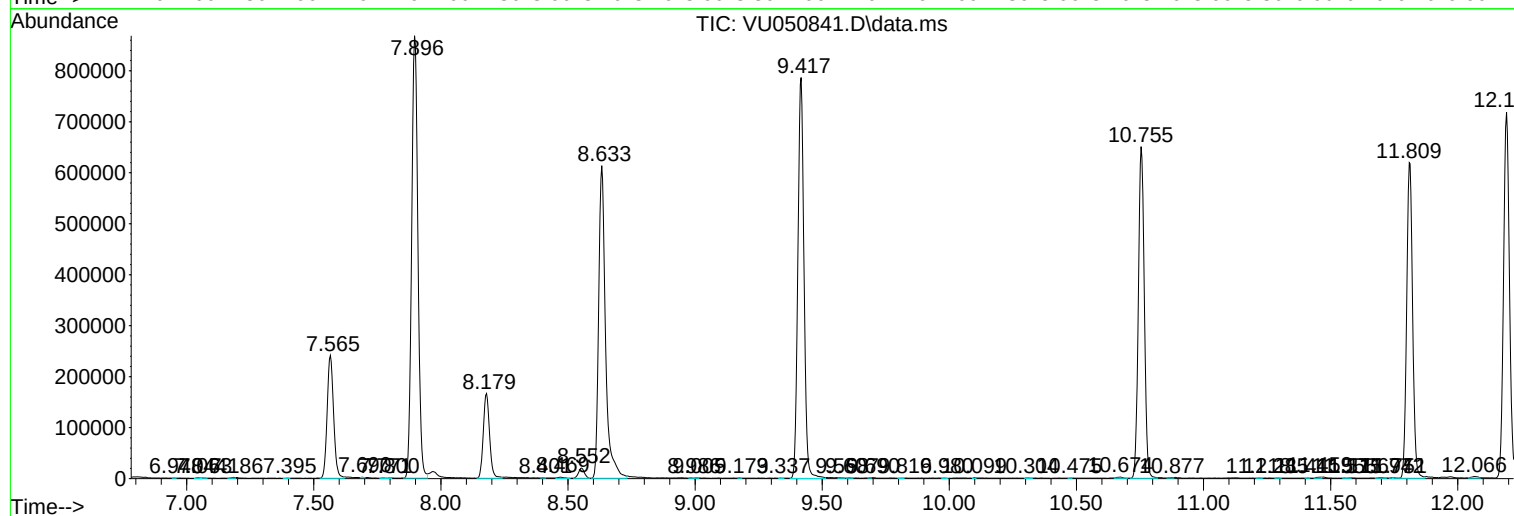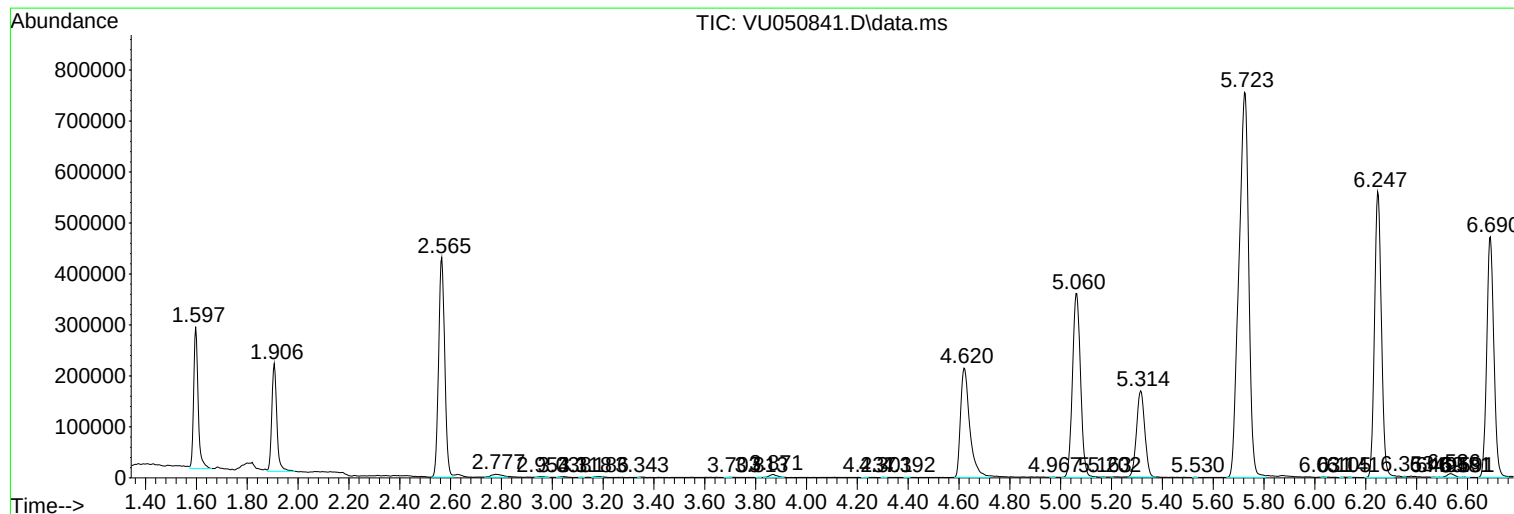

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050841.D
Acq On : 20 Sep 2022 19:10
Operator : JC/MD
Sample : N4651-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050841.D
Acq On : 20 Sep 2022 19:10
Operator : JC/MD
Sample : N4651-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc