

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050842.D
 Acq On : 20 Sep 2022 19:34
 Operator : JC/MD
 Sample : N4651-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	270886	324543	16.75%	2.097%
2	1.906	168	176	194	rVB	205654	278058	14.35%	1.797%
3	2.565	368	381	397	rBV2	439214	775823	40.03%	5.013%
4	2.797	438	453	469	rBV	4852	15389	0.79%	0.099%
5	2.919	487	491	494	rBV	858	666	0.03%	0.004%
6	2.954	498	502	507	rVV5	580	698	0.04%	0.005%
7	3.102	545	548	553	rBV4	728	628	0.03%	0.004%
8	3.173	564	570	571	rBV3	886	808	0.04%	0.005%
9	3.286	602	605	611	rVB3	443	446	0.02%	0.003%
10	3.353	617	626	636	rBV4	5482	10581	0.55%	0.068%
11	3.392	636	638	645	rVB3	889	757	0.04%	0.005%
12	3.745	743	748	752	rBV2	394	354	0.02%	0.002%
13	3.803	763	766	768	rBV2	546	375	0.02%	0.002%
14	3.867	768	786	809	rVV	168518	399060	20.59%	2.579%
15	3.993	821	825	829	rVB3	505	410	0.02%	0.003%
16	4.080	849	852	855	rBV2	514	406	0.02%	0.003%
17	4.096	855	857	861	rVB2	454	319	0.02%	0.002%
18	4.125	861	866	871	rBV2	417	536	0.03%	0.003%
19	4.298	917	920	924	rBV	368	326	0.02%	0.002%
20	4.472	964	974	977	rBV2	457	598	0.03%	0.004%
21	4.514	981	987	990	rBV2	484	381	0.02%	0.002%
22	4.559	999	1001	1005	rBV2	303	312	0.02%	0.002%
23	4.623	1008	1021	1050	rBV2	209820	640713	33.06%	4.140%
24	4.864	1091	1096	1099	rBV4	552	481	0.02%	0.003%
25	5.060	1141	1157	1180	rBV2	349493	762727	39.36%	4.928%
26	5.314	1218	1236	1254	rBV2	194903	441416	22.78%	2.852%
27	5.507	1292	1296	1300	rBV4	556	426	0.02%	0.003%
28	5.642	1334	1338	1342	rBV2	550	556	0.03%	0.004%
29	5.723	1342	1363	1380	rBV2	726077	1937988	100.00%	12.523%
30	5.970	1438	1440	1443	rVV3	875	484	0.02%	0.003%
31	5.986	1443	1445	1449	rVB3	850	464	0.02%	0.003%
32	6.035	1456	1460	1461	rBV	503	339	0.02%	0.002%
33	6.073	1469	1472	1475	rBV3	539	359	0.02%	0.002%
34	6.247	1512	1526	1553	rBV	557404	1062122	54.81%	6.863%
35	6.411	1574	1577	1581	rVB3	807	615	0.03%	0.004%
36	6.543	1603	1618	1634	rBV2	67608	132055	6.81%	0.853%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050842.D
 Acq On : 20 Sep 2022 19:34
 Operator : JC/MD
 Sample : N4651-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.691	1649	1664	1685	rBV	456510	888868	45.87%	5.744%
38	6.983	1744	1755	1765	rBV3	6988	14073	0.73%	0.091%
39	7.189	1810	1819	1827	rBV7	1876	3154	0.16%	0.020%
40	7.318	1852	1859	1862	rBV2	377	409	0.02%	0.003%
41	7.565	1923	1936	1952	rBV	226716	400079	20.64%	2.585%
42	7.681	1970	1972	1975	rBV3	630	438	0.02%	0.003%
43	7.700	1975	1978	1979	rBV4	807	532	0.03%	0.003%
44	7.896	2025	2039	2054	rBV	817977	1403866	72.44%	9.071%
45	8.179	2115	2127	2144	rVV	158195	269756	13.92%	1.743%
46	8.401	2191	2196	2202	rVB5	1478	1901	0.10%	0.012%
47	8.465	2212	2216	2218	rBV4	1057	796	0.04%	0.005%
48	8.552	2231	2243	2256	rBV2	93135	156231	8.06%	1.010%
49	8.633	2256	2268	2300	rBV2	597187	1116194	57.60%	7.212%
50	8.893	2347	2349	2352	rVB4	617	338	0.02%	0.002%
51	8.916	2352	2356	2359	rBV3	1124	1194	0.06%	0.008%
52	9.034	2390	2393	2396	rBV3	425	354	0.02%	0.002%
53	9.112	2412	2417	2419	rBV3	519	446	0.02%	0.003%
54	9.279	2465	2469	2474	rBV2	297	346	0.02%	0.002%
55	9.417	2498	2512	2541	rBV	777550	1287833	66.45%	8.322%
56	9.600	2567	2569	2573	rVB3	547	335	0.02%	0.002%
57	9.690	2590	2597	2604	rVB4	933	1394	0.07%	0.009%
58	9.787	2624	2627	2632	rVB2	568	526	0.03%	0.003%
59	9.867	2649	2652	2655	rBV	439	330	0.02%	0.002%
60	10.031	2698	2703	2708	rVV2	300	427	0.02%	0.003%
61	10.243	2766	2769	2774	rBV2	486	389	0.02%	0.003%
62	10.333	2791	2797	2800	rVB	439	394	0.02%	0.003%
63	10.356	2800	2804	2806	rBV	585	415	0.02%	0.003%
64	10.491	2839	2846	2850	rVB3	749	979	0.05%	0.006%
65	10.671	2893	2902	2911	rVB4	1846	3145	0.16%	0.020%
66	10.755	2915	2928	2946	rBV	641081	1013745	52.31%	6.550%
67	10.870	2958	2964	2966	rBV5	464	502	0.03%	0.003%
68	11.044	3010	3018	3020	rBV2	371	470	0.02%	0.003%
69	11.089	3027	3032	3037	rBV5	608	741	0.04%	0.005%
70	11.115	3037	3040	3044	rVB4	415	339	0.02%	0.002%
71	11.231	3070	3076	3078	rBV2	442	469	0.02%	0.003%
72	11.327	3100	3106	3108	rBV2	443	415	0.02%	0.003%
73	11.456	3142	3146	3149	rBV2	1302	1165	0.06%	0.008%
74	11.575	3179	3183	3185	rBV2	552	381	0.02%	0.002%
75	11.639	3200	3203	3206	rBV2	534	340	0.02%	0.002%
76	11.690	3213	3219	3220	rBV3	1040	833	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050842.D
 Acq On : 20 Sep 2022 19:34
 Operator : JC/MD
 Sample : N4651-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.745	3233	3236	3240	rBV3	980	704	0.04%	0.005%
78	11.809	3244	3256	3281	rBV	606072	989330	51.05%	6.393%
79	11.938	3292	3296	3301	rVV5	1105	1069	0.06%	0.007%
80	11.973	3301	3307	3310	rVB3	1246	1271	0.07%	0.008%
81	12.067	3329	3336	3348	rVB6	3855	6835	0.35%	0.044%
82	12.192	3362	3375	3394	rVV	688198	1094329	56.47%	7.071%
83	12.603	3499	3503	3507	rVB2	566	576	0.03%	0.004%
84	12.771	3551	3555	3557	rBV	777	470	0.02%	0.003%
85	12.896	3591	3594	3597	rBV6	714	556	0.03%	0.004%
86	12.976	3615	3619	3621	rBV2	395	325	0.02%	0.002%
87	13.054	3641	3643	3646	rBV2	532	363	0.02%	0.002%
88	13.211	3686	3692	3693	rBV4	563	621	0.03%	0.004%
89	13.266	3707	3709	3713	rVB3	675	392	0.02%	0.003%
90	13.394	3742	3749	3754	rVB4	955	1422	0.07%	0.009%
91	13.472	3769	3773	3776	rVB2	775	538	0.03%	0.003%
92	13.497	3776	3781	3782	rBV	511	385	0.02%	0.002%
93	13.755	3857	3861	3863	rVV2	487	394	0.02%	0.003%
94	13.838	3884	3887	3888	rBV2	862	476	0.02%	0.003%
95	14.092	3958	3966	3974	rBV3	1913	3345	0.17%	0.022%
96	14.337	4038	4042	4048	rVB5	1525	1483	0.08%	0.010%
97	14.671	4143	4146	4150	rBV3	503	571	0.03%	0.004%
98	15.005	4247	4250	4253	rBV2	572	451	0.02%	0.003%
99	15.433	4380	4383	4386	rBV3	833	590	0.03%	0.004%
100	15.944	4537	4542	4544	rBV4	2776	2661	0.14%	0.017%




Sum of corrected areas: 15475918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050842.D
Acq On : 20 Sep 2022 19:34
Operator : JC/MD
Sample : N4651-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

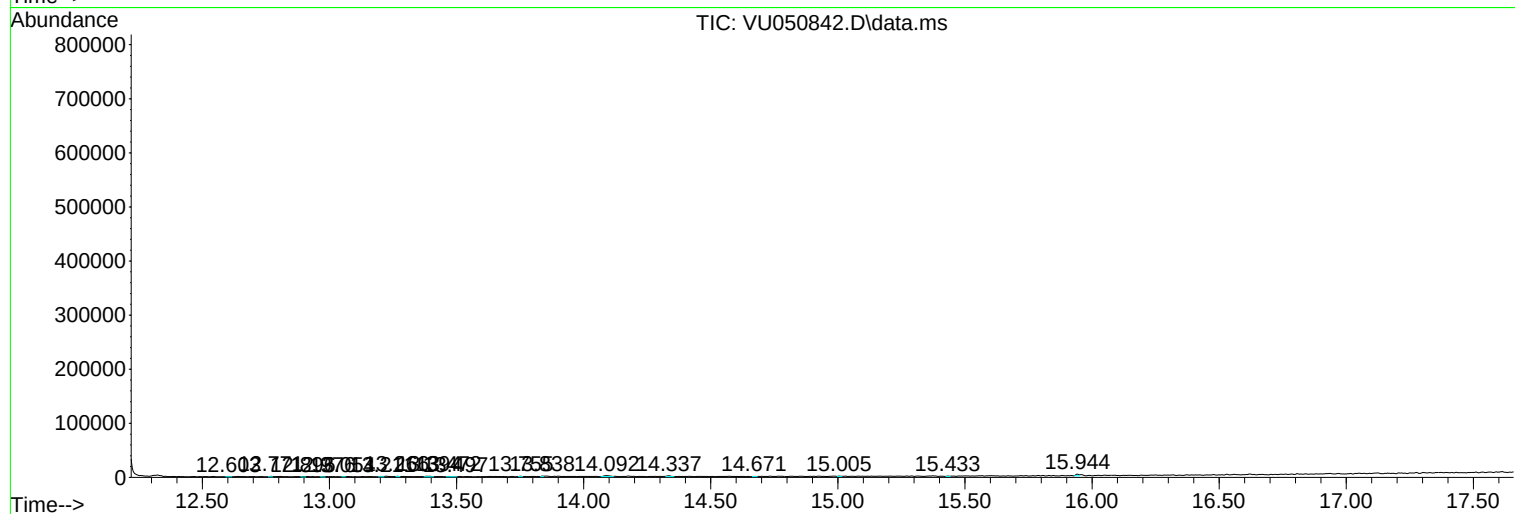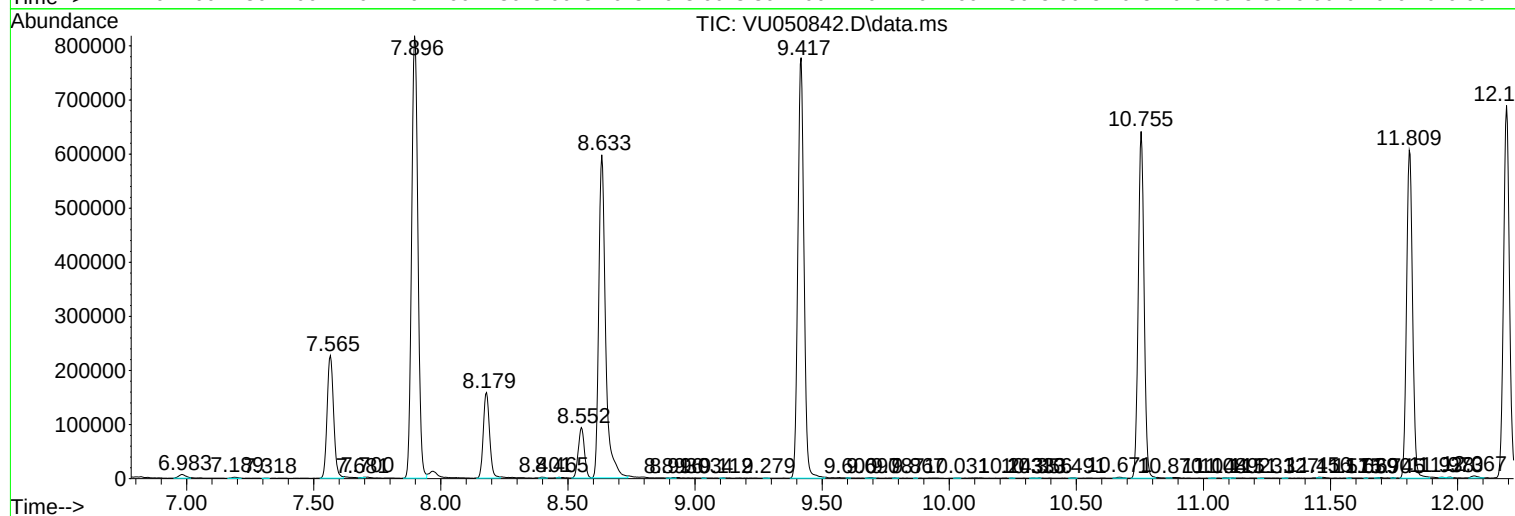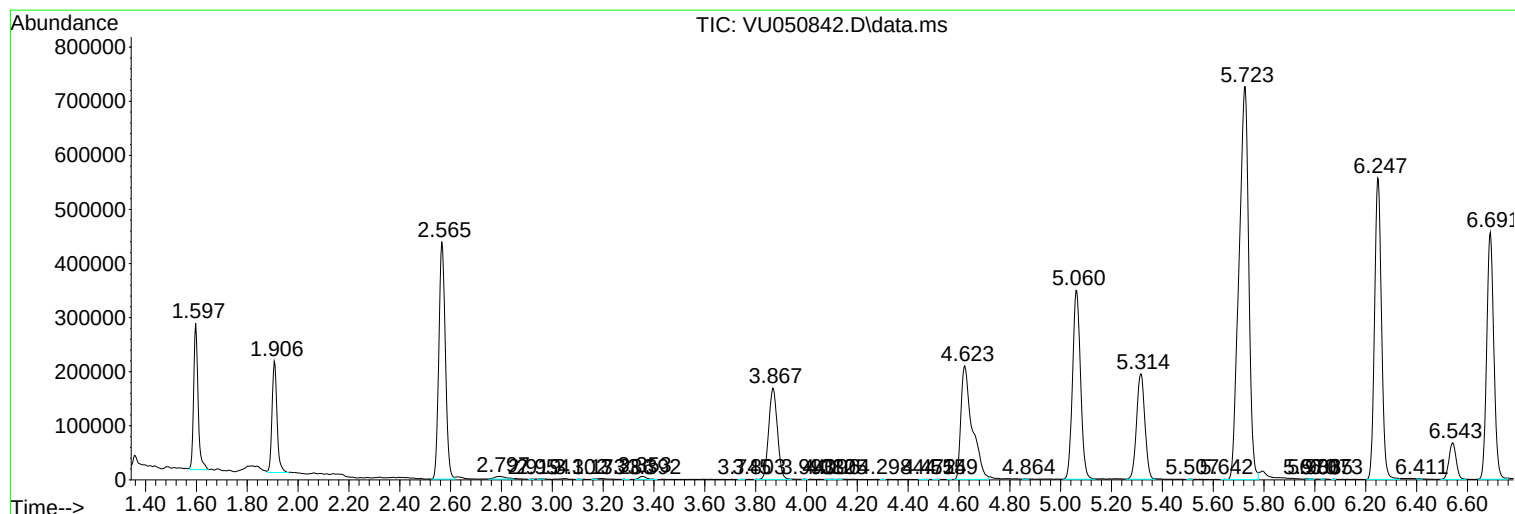

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050842.D
Acq On : 20 Sep 2022 19:34
Operator : JC/MD
Sample : N4651-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050842.D
Acq On : 20 Sep 2022 19:34
Operator : JC/MD
Sample : N4651-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------