

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050843.D
 Acq On : 20 Sep 2022 19:58
 Operator : JC/MD
 Sample : N4651-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	219300	258937	15.84%	1.877%
2	1.906	169	176	195	rVB	187678	252229	15.43%	1.828%
3	2.481	351	355	357	rBV2	875	659	0.04%	0.005%
4	2.565	368	381	398	rBV	349032	579794	35.47%	4.202%
5	2.793	441	452	454	rBV5	3927	5749	0.35%	0.042%
6	3.044	522	530	539	rVB4	1745	2907	0.18%	0.021%
7	3.173	565	570	573	rBV3	929	991	0.06%	0.007%
8	3.356	616	627	641	rBV3	10400	20658	1.26%	0.150%
9	3.494	666	670	672	rBV2	451	333	0.02%	0.002%
10	3.581	694	697	700	rBV2	401	300	0.02%	0.002%
11	3.690	728	731	735	rVB2	611	435	0.03%	0.003%
12	3.867	762	786	810	rBV	203323	482817	29.54%	3.499%
13	3.999	822	827	830	rVB3	425	325	0.02%	0.002%
14	4.034	830	838	840	rBV2	441	580	0.04%	0.004%
15	4.626	1006	1022	1028	rBV	200113	446079	27.29%	3.233%
16	4.857	1091	1094	1096	rVB3	549	311	0.02%	0.002%
17	4.919	1110	1113	1116	rVB3	855	587	0.04%	0.004%
18	4.938	1118	1119	1123	rVB2	532	354	0.02%	0.003%
19	4.960	1123	1126	1130	rVB2	603	364	0.02%	0.003%
20	5.063	1141	1158	1182	rBV	291252	642133	39.28%	4.654%
21	5.243	1209	1214	1218	rBV4	848	898	0.05%	0.007%
22	5.314	1218	1236	1255	rVV	372380	836644	51.18%	6.064%
23	5.623	1326	1332	1335	rBV2	406	389	0.02%	0.003%
24	5.726	1342	1364	1382	rBV2	604701	1634639	100.00%	11.848%
25	5.983	1442	1444	1448	rVB4	781	381	0.02%	0.003%
26	6.047	1461	1464	1472	rVB4	847	898	0.05%	0.007%
27	6.089	1472	1477	1480	rBV3	368	330	0.02%	0.002%
28	6.115	1480	1485	1488	rBV2	486	486	0.03%	0.004%
29	6.250	1510	1527	1548	rBV	530563	1014031	62.03%	7.350%
30	6.475	1591	1597	1605	rBV4	1293	2060	0.13%	0.015%
31	6.539	1605	1617	1631	rBV6	16623	35171	2.15%	0.255%
32	6.591	1631	1633	1636	rVB3	691	345	0.02%	0.003%
33	6.690	1649	1664	1685	rBV	385427	756089	46.25%	5.480%
34	6.986	1748	1756	1757	rBV4	1729	1694	0.10%	0.012%
35	7.173	1808	1814	1815	rBV3	486	420	0.03%	0.003%
36	7.192	1815	1820	1822	rBV4	869	879	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050843.D
 Acq On : 20 Sep 2022 19:58
 Operator : JC/MD
 Sample : N4651-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.565	1922	1936	1953	rBV	187438	333699	20.41%	2.419%
38	7.896	2026	2039	2054	rBV	681342	1165195	71.28%	8.445%
39	8.134	2109	2113	2115	rBV3	331	305	0.02%	0.002%
40	8.179	2115	2127	2145	rBV	130968	225575	13.80%	1.635%
41	8.340	2175	2177	2181	rVB3	720	415	0.03%	0.003%
42	8.365	2181	2185	2191	rBV4	414	427	0.03%	0.003%
43	8.504	2226	2228	2232	rVB2	517	370	0.02%	0.003%
44	8.552	2232	2243	2255	rBV3	48395	82840	5.07%	0.600%
45	8.632	2257	2268	2302	rBV2	540995	1041606	63.72%	7.550%
46	8.841	2331	2333	2335	rBV2	672	315	0.02%	0.002%
47	8.877	2342	2344	2347	rBV2	463	330	0.02%	0.002%
48	8.928	2358	2360	2365	rVB3	744	452	0.03%	0.003%
49	8.960	2365	2370	2372	rBV3	404	317	0.02%	0.002%
50	8.979	2373	2376	2381	rBV4	552	506	0.03%	0.004%
51	9.028	2387	2391	2394	rBV2	346	330	0.02%	0.002%
52	9.140	2422	2426	2428	rVV2	538	397	0.02%	0.003%
53	9.417	2496	2512	2537	rBV	729089	1216696	74.43%	8.819%
54	9.677	2586	2593	2595	rBV4	627	686	0.04%	0.005%
55	9.697	2595	2599	2604	rVB4	950	1053	0.06%	0.008%
56	9.754	2613	2617	2619	rVV	319	301	0.02%	0.002%
57	9.770	2619	2622	2624	rVV2	730	430	0.03%	0.003%
58	9.799	2628	2631	2634	rVB2	594	342	0.02%	0.002%
59	10.098	2719	2724	2727	rBV3	472	378	0.02%	0.003%
60	10.478	2838	2842	2850	rVB3	445	525	0.03%	0.004%
61	10.664	2895	2900	2909	rVB4	1821	2602	0.16%	0.019%
62	10.754	2915	2928	2947	rBV	547773	883700	54.06%	6.405%
63	10.867	2960	2963	2965	rBV2	568	388	0.02%	0.003%
64	10.893	2967	2971	2981	rVB6	1466	2391	0.15%	0.017%
65	11.118	3035	3041	3043	rBV2	724	616	0.04%	0.004%
66	11.137	3043	3047	3051	rVB2	771	625	0.04%	0.005%
67	11.214	3067	3071	3074	rBV3	282	301	0.02%	0.002%
68	11.262	3080	3086	3090	rBV3	495	563	0.03%	0.004%
69	11.468	3139	3150	3160	rVV9	1371	3213	0.20%	0.023%
70	11.523	3165	3167	3172	rVB2	510	357	0.02%	0.003%
71	11.680	3212	3216	3218	rBV	541	421	0.03%	0.003%
72	11.693	3218	3220	3227	rVB3	1022	837	0.05%	0.006%
73	11.748	3233	3237	3240	rBV3	448	472	0.03%	0.003%
74	11.812	3244	3257	3279	rBV	572386	918901	56.21%	6.660%
75	11.967	3302	3305	3306	rBV2	729	393	0.02%	0.003%
76	12.066	3327	3336	3340	rBV6	1990	2725	0.17%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050843.D
 Acq On : 20 Sep 2022 19:58
 Operator : JC/MD
 Sample : N4651-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.192	3362	3375	3399	rBV	560865	911049	55.73%	6.603%
78	12.397	3434	3439	3441	rBV3	715	609	0.04%	0.004%
79	12.410	3441	3443	3447	rBV2	656	413	0.03%	0.003%
80	12.513	3470	3475	3482	rVB	553	688	0.04%	0.005%
81	12.555	3484	3488	3490	rBV2	582	506	0.03%	0.004%
82	12.661	3517	3521	3525	rVV2	536	513	0.03%	0.004%
83	12.725	3538	3541	3545	rBV3	514	437	0.03%	0.003%
84	12.786	3558	3560	3563	rVB	451	299	0.02%	0.002%
85	12.915	3598	3600	3606	rVV4	417	418	0.03%	0.003%
86	12.963	3611	3615	3618	rBV2	470	366	0.02%	0.003%
87	12.983	3618	3621	3627	rVB2	537	397	0.02%	0.003%
88	13.015	3627	3631	3633	rBV2	414	403	0.02%	0.003%
89	13.381	3741	3745	3748	rBV4	858	631	0.04%	0.005%
90	13.513	3783	3786	3792	rVB3	529	536	0.03%	0.004%
91	13.844	3885	3889	3894	rVB5	1183	1216	0.07%	0.009%
92	14.028	3942	3946	3950	rBV2	556	615	0.04%	0.004%
93	14.047	3950	3952	3956	rVV3	591	377	0.02%	0.003%
94	14.272	4020	4022	4028	rVB3	913	781	0.05%	0.006%
95	14.552	4106	4109	4112	rVB2	646	374	0.02%	0.003%
96	14.571	4112	4115	4118	rBV3	740	577	0.04%	0.004%
97	15.143	4291	4293	4296	rVB3	962	468	0.03%	0.003%
98	15.336	4349	4353	4354	rBV2	646	395	0.02%	0.003%
99	15.683	4459	4461	4463	rBV2	791	346	0.02%	0.003%
100	16.092	4585	4588	4589	rBV3	1067	692	0.04%	0.005%




Sum of corrected areas: 13796997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050843.D
Acq On : 20 Sep 2022 19:58
Operator : JC/MD
Sample : N4651-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

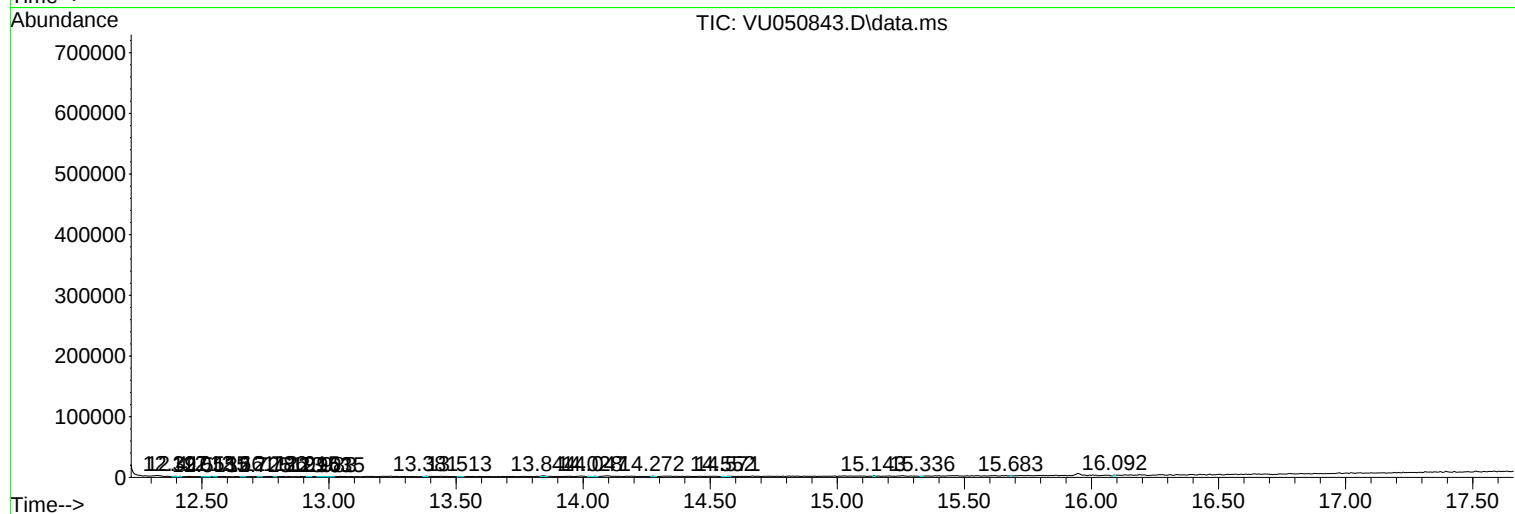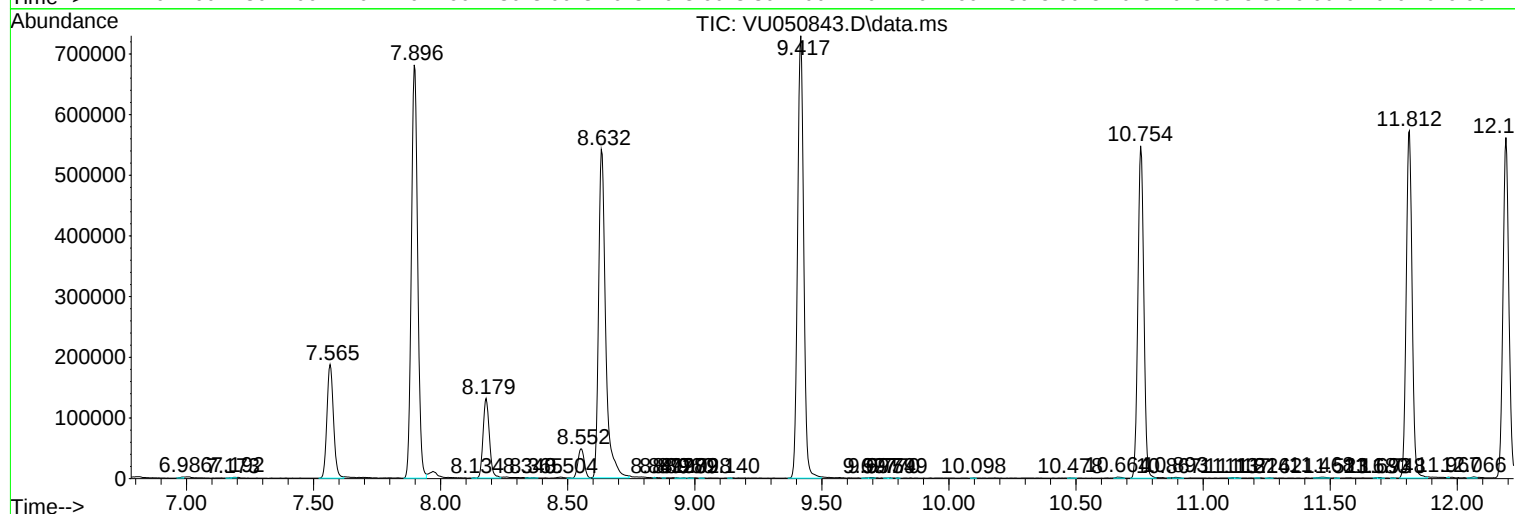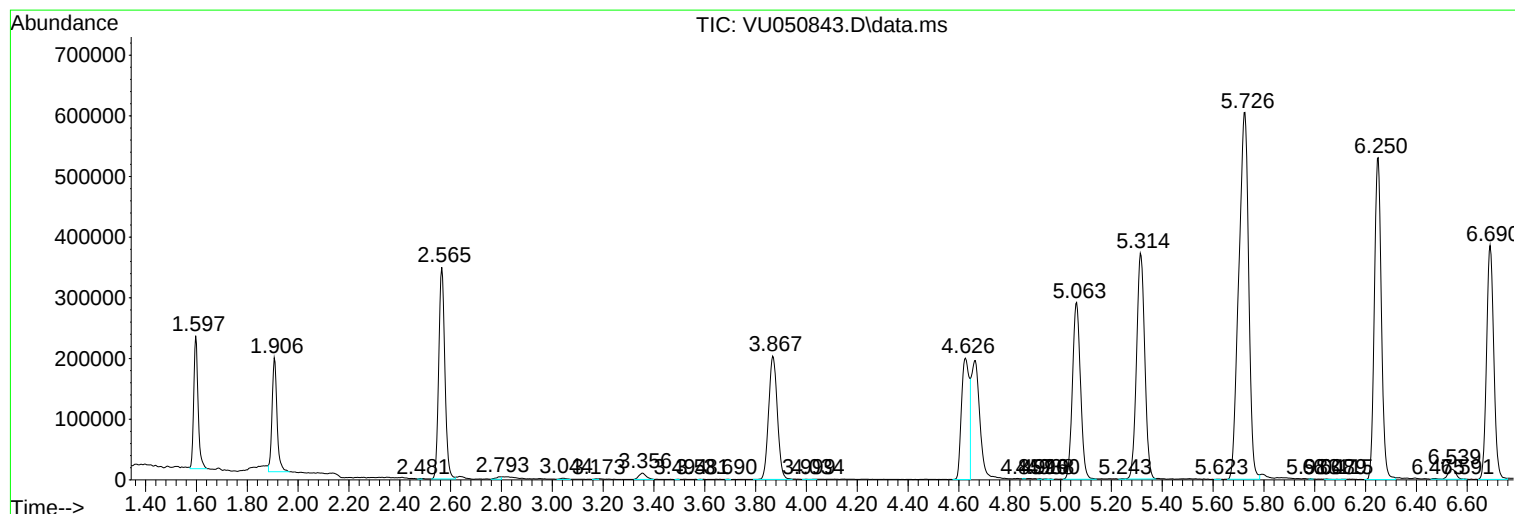

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050843.D
Acq On : 20 Sep 2022 19:58
Operator : JC/MD
Sample : N4651-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050843.D
Acq On : 20 Sep 2022 19:58
Operator : JC/MD
Sample : N4651-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------