

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050844.D
 Acq On : 20 Sep 2022 20:21
 Operator : JC/MD
 Sample : N4651-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	97	rVB	274992	331481	17.26%	2.302%
2	1.906	170	176	192	rVB	201849	261373	13.61%	1.815%
3	2.565	368	381	397	rBV	397359	654236	34.07%	4.544%
4	2.954	498	502	508	rBV4	1102	1350	0.07%	0.009%
5	3.089	541	544	546	rBV3	246	172	0.01%	0.001%
6	3.131	555	557	559	rBV	287	122	0.01%	0.001%
7	3.186	562	574	582	rBV3	3248	6681	0.35%	0.046%
8	3.285	604	605	608	rBV	204	114	0.01%	0.001%
9	3.356	616	627	643	rVB3	9616	19192	1.00%	0.133%
10	3.423	643	648	651	rBV2	355	308	0.02%	0.002%
11	3.552	682	688	692	rVB2	371	379	0.02%	0.003%
12	3.674	720	726	729	rBV2	468	440	0.02%	0.003%
13	3.742	745	747	751	rBV2	302	180	0.01%	0.001%
14	3.867	769	786	807	rBV2	171778	404698	21.08%	2.811%
15	4.102	853	859	865	rBV4	357	421	0.02%	0.003%
16	4.179	879	883	887	rBV3	446	318	0.02%	0.002%
17	4.234	895	900	904	rVB3	416	382	0.02%	0.003%
18	4.253	904	906	910	rVB2	162	144	0.01%	0.001%
19	4.279	910	914	915	rBV	190	114	0.01%	0.001%
20	4.301	918	921	923	rBV	168	114	0.01%	0.001%
21	4.343	930	934	940	rBV2	685	813	0.04%	0.006%
22	4.430	957	961	962	rBV	271	195	0.01%	0.001%
23	4.552	996	999	1002	rBV	346	321	0.02%	0.002%
24	4.575	1004	1006	1008	rBV2	298	115	0.01%	0.001%
25	4.626	1008	1022	1026	rBV	214979	428938	22.34%	2.979%
26	5.063	1140	1158	1180	rBV	344423	753423	39.24%	5.233%
27	5.314	1220	1236	1256	rBV2	87398	196399	10.23%	1.364%
28	5.504	1293	1295	1298	rVB	273	117	0.01%	0.001%
29	5.520	1298	1300	1301	rBV2	279	116	0.01%	0.001%
30	5.571	1314	1316	1319	rBV2	315	194	0.01%	0.001%
31	5.597	1321	1324	1326	rBV	274	208	0.01%	0.001%
32	5.645	1336	1339	1341	rBV	311	148	0.01%	0.001%
33	5.722	1341	1363	1395	rBV2	713586	1920141	100.00%	13.336%
34	6.166	1499	1501	1505	rBV2	300	234	0.01%	0.002%
35	6.250	1512	1527	1549	rBV	533153	1007189	52.45%	6.995%
36	6.542	1604	1618	1631	rBV4	26896	53010	2.76%	0.368%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050844.D
 Acq On : 20 Sep 2022 20:21
 Operator : JC/MD
 Sample : N4651-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1689	rBV	450287	880189	45.84%	6.113%
38	6.906	1728	1731	1732	rBV3	369	169	0.01%	0.001%
39	6.935	1737	1740	1744	rVB2	507	268	0.01%	0.002%
40	6.989	1744	1757	1761	rBV3	3769	6590	0.34%	0.046%
41	7.095	1786	1790	1795	rBV3	345	355	0.02%	0.002%
42	7.137	1801	1803	1808	rVB2	275	202	0.01%	0.001%
43	7.185	1808	1818	1828	rBV5	2038	3401	0.18%	0.024%
44	7.253	1836	1839	1842	rBV2	244	165	0.01%	0.001%
45	7.365	1871	1874	1877	rBV2	419	258	0.01%	0.002%
46	7.404	1884	1886	1890	rVB2	388	213	0.01%	0.001%
47	7.430	1891	1894	1896	rBV2	224	121	0.01%	0.001%
48	7.472	1904	1907	1910	rVB2	311	190	0.01%	0.001%
49	7.491	1910	1913	1917	rVB	206	140	0.01%	0.001%
50	7.565	1923	1936	1952	rBV	222385	390989	20.36%	2.715%
51	7.774	1999	2001	2005	rBV2	362	182	0.01%	0.001%
52	7.803	2006	2010	2013	rVB4	481	360	0.02%	0.003%
53	7.896	2026	2039	2055	rBV	805122	1381451	71.95%	9.594%
54	8.179	2115	2127	2150	rBV	153458	262904	13.69%	1.826%
55	8.398	2190	2195	2202	rBV4	1503	2051	0.11%	0.014%
56	8.468	2211	2217	2233	rVB5	2231	3965	0.21%	0.028%
57	8.552	2233	2243	2254	rVB2	17671	29132	1.52%	0.202%
58	8.632	2256	2268	2304	rBV2	612045	1144897	59.63%	7.951%
59	8.941	2362	2364	2368	rBV3	397	213	0.01%	0.001%
60	9.050	2396	2398	2402	rBV2	436	284	0.01%	0.002%
61	9.089	2407	2410	2412	rBV3	598	391	0.02%	0.003%
62	9.127	2420	2422	2430	rVB3	477	389	0.02%	0.003%
63	9.169	2431	2435	2438	rBV3	528	420	0.02%	0.003%
64	9.188	2438	2441	2444	rBV3	483	391	0.02%	0.003%
65	9.320	2478	2482	2483	rBV2	252	171	0.01%	0.001%
66	9.417	2498	2512	2544	rBV	728760	1215538	63.30%	8.442%
67	9.600	2566	2569	2571	rBV2	643	362	0.02%	0.003%
68	9.626	2574	2577	2580	rVB2	742	451	0.02%	0.003%
69	9.677	2589	2593	2596	rBV4	687	679	0.04%	0.005%
70	9.700	2596	2600	2605	rVB5	1014	1056	0.05%	0.007%
71	9.751	2613	2616	2619	rBV	465	254	0.01%	0.002%
72	9.828	2635	2640	2642	rBV2	390	323	0.02%	0.002%
73	9.886	2655	2658	2662	rBV	277	207	0.01%	0.001%
74	10.024	2698	2701	2702	rBV	243	150	0.01%	0.001%
75	10.150	2737	2740	2747	rVB4	441	416	0.02%	0.003%
76	10.259	2771	2774	2777	rBV2	195	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050844.D
 Acq On : 20 Sep 2022 20:21
 Operator : JC/MD
 Sample : N4651-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.282	2778	2781	2783	rBV	370	220	0.01%	0.002%
78	10.301	2783	2787	2790	rBV2	428	354	0.02%	0.002%
79	10.356	2801	2804	2806	rBV	300	173	0.01%	0.001%
80	10.401	2816	2818	2822	rVB2	340	247	0.01%	0.002%
81	10.426	2822	2826	2831	rVB2	371	338	0.02%	0.002%
82	10.452	2831	2834	2836	rBV	250	128	0.01%	0.001%
83	10.468	2836	2839	2841	rBV	318	189	0.01%	0.001%
84	10.487	2841	2845	2848	rVB2	626	469	0.02%	0.003%
85	10.561	2866	2868	2869	rBV	336	179	0.01%	0.001%
86	10.671	2895	2902	2910	rVB5	2737	3506	0.18%	0.024%
87	10.754	2915	2928	2953	rBV	632156	1009538	52.58%	7.011%
88	11.282	3088	3092	3096	rBV2	281	289	0.02%	0.002%
89	11.346	3109	3112	3114	rVB	210	113	0.01%	0.001%
90	11.362	3114	3117	3120	rBV2	353	304	0.02%	0.002%
91	11.565	3178	3180	3181	rBV	283	144	0.01%	0.001%
92	11.581	3181	3185	3193	rVB4	709	863	0.04%	0.006%
93	11.745	3233	3236	3244	rBV4	866	1031	0.05%	0.007%
94	11.809	3244	3256	3287	rBV	575536	927961	48.33%	6.445%
95	12.192	3363	3375	3408	rVB	665460	1076224	56.05%	7.474%
96	12.433	3448	3450	3454	rBV2	485	243	0.01%	0.002%
97	12.761	3549	3552	3554	rBV	630	417	0.02%	0.003%
98	13.092	3653	3655	3659	rVB2	710	481	0.03%	0.003%
99	13.391	3745	3748	3753	rBV3	976	946	0.05%	0.007%
100	13.847	3887	3890	3891	rBV	892	549	0.03%	0.004%




Sum of corrected areas: 14398684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050844.D
Acq On : 20 Sep 2022 20:21
Operator : JC/MD
Sample : N4651-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

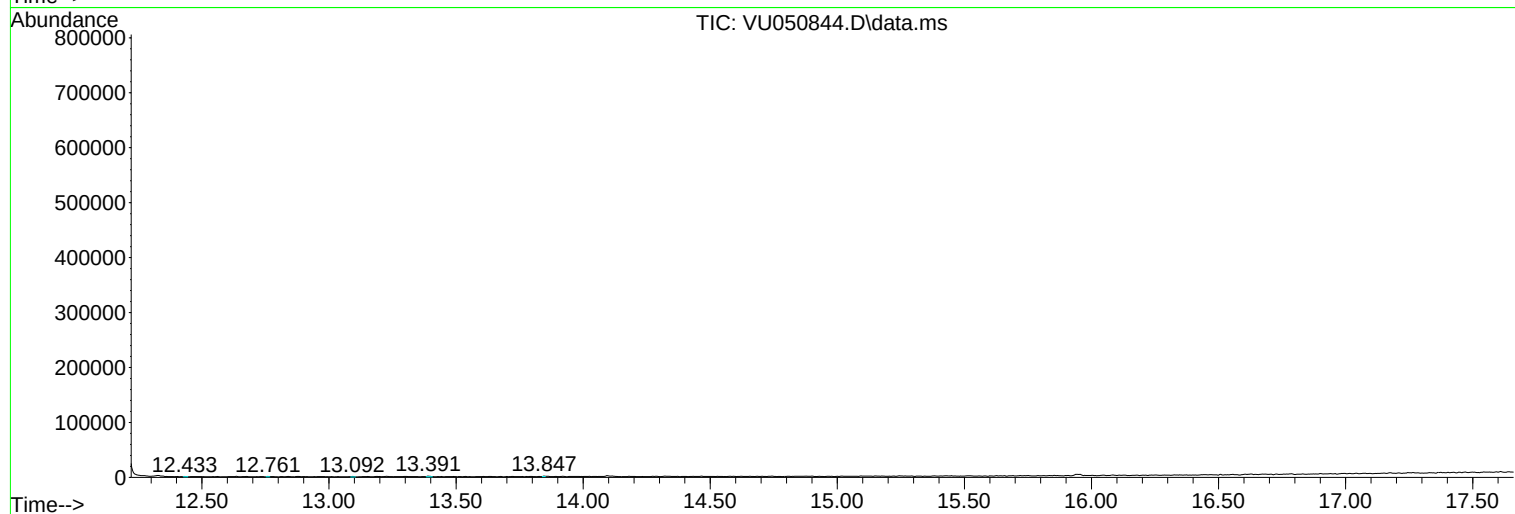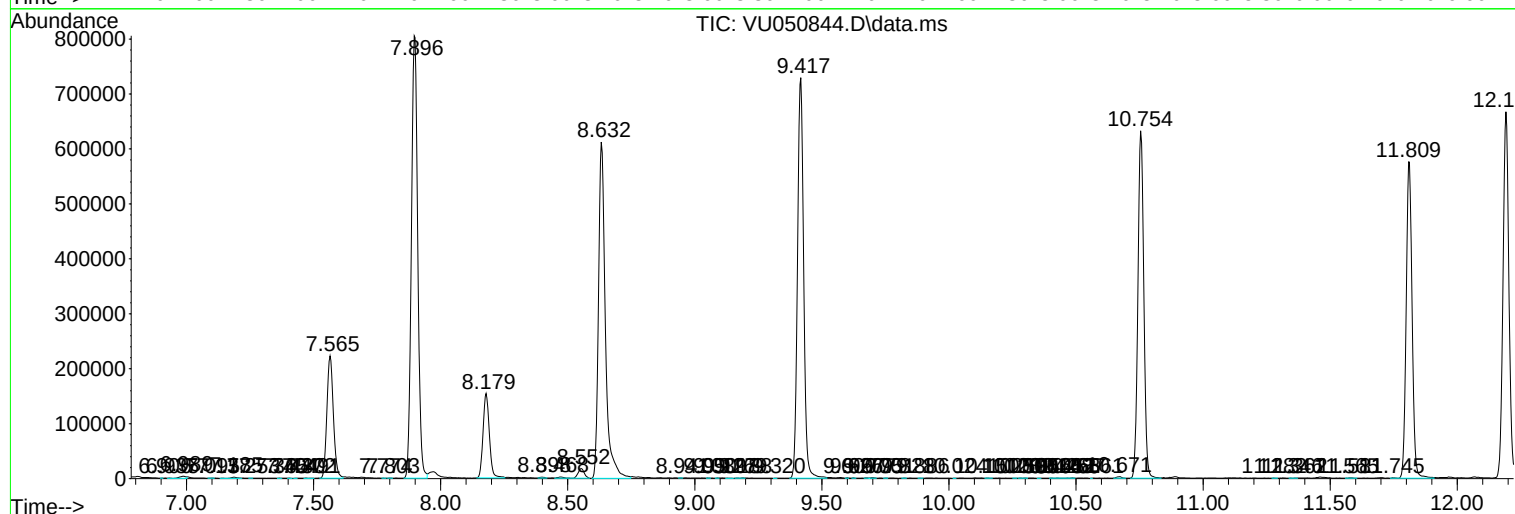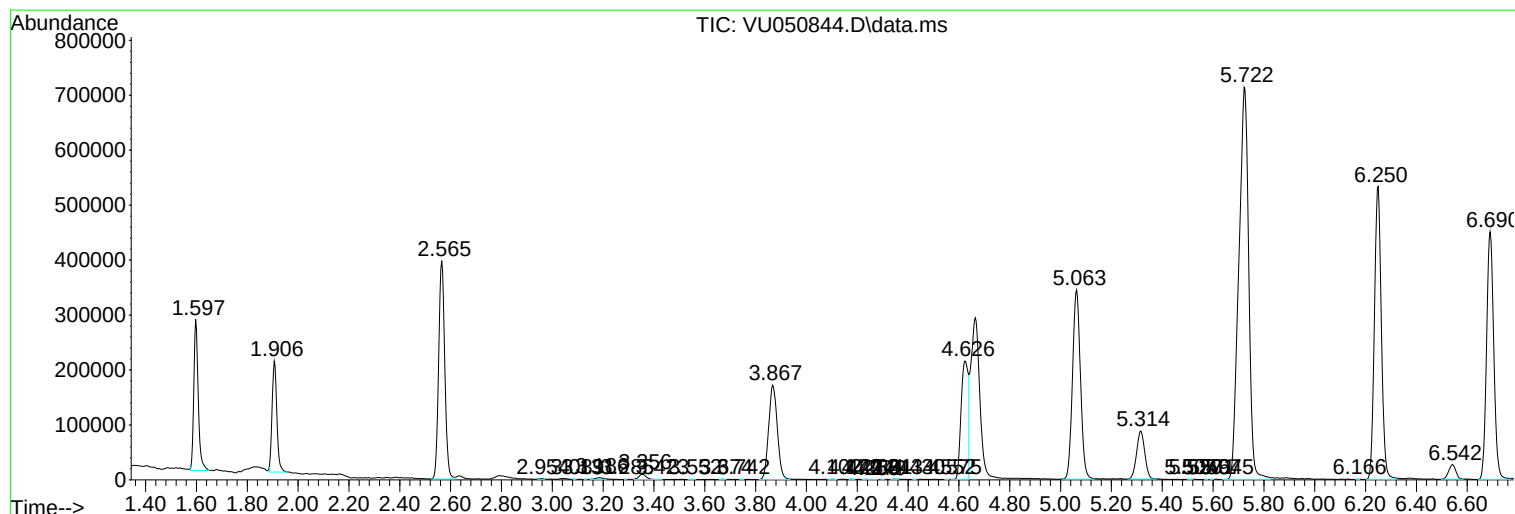

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050844.D
Acq On : 20 Sep 2022 20:21
Operator : JC/MD
Sample : N4651-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050844.D
Acq On : 20 Sep 2022 20:21
Operator : JC/MD
Sample : N4651-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc