

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050845.D
 Acq On : 20 Sep 2022 20:45
 Operator : JC/MD
 Sample : N4651-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	94	rVB	227225	258561	15.47%	2.138%
2	1.906	169	176	195	rVB	172380	239907	14.35%	1.983%
3	2.565	369	381	395	rBV	349581	568948	34.03%	4.704%
4	3.141	557	560	561	rBV	308	151	0.01%	0.001%
5	3.240	588	591	595	rBV	232	178	0.01%	0.001%
6	3.465	659	661	664	rVB	283	142	0.01%	0.001%
7	3.520	675	678	682	rVB2	403	245	0.01%	0.002%
8	3.629	709	712	714	rVB	226	112	0.01%	0.001%
9	3.713	735	738	741	rBV	316	199	0.01%	0.002%
10	3.780	753	759	762	rBV2	380	382	0.02%	0.003%
11	3.867	775	786	805	rVB2	12125	26825	1.60%	0.222%
12	3.938	805	808	811	rBV2	286	238	0.01%	0.002%
13	3.993	822	825	828	rBV	387	300	0.02%	0.002%
14	4.025	833	835	839	rVB2	385	217	0.01%	0.002%
15	4.073	847	850	853	rVB	346	185	0.01%	0.002%
16	4.099	853	858	861	rBV2	602	536	0.03%	0.004%
17	4.176	877	882	884	rBV	366	292	0.02%	0.002%
18	4.224	894	897	901	rBV	197	165	0.01%	0.001%
19	4.311	920	924	929	rVB2	493	430	0.03%	0.004%
20	4.353	929	937	938	rBV	380	413	0.02%	0.003%
21	4.494	977	981	984	rBV	437	326	0.02%	0.003%
22	4.620	1008	1020	1055	rBV	206762	542174	32.43%	4.482%
23	5.060	1142	1157	1182	rBV	297579	653978	39.12%	5.407%
24	5.430	1268	1272	1275	rBV3	185	141	0.01%	0.001%
25	5.517	1294	1299	1302	rBV2	380	358	0.02%	0.003%
26	5.530	1302	1303	1305	rVV2	205	60	0.00%	0.000%
27	5.542	1305	1307	1310	rBV2	212	126	0.01%	0.001%
28	5.613	1326	1329	1335	rBV	255	294	0.02%	0.002%
29	5.636	1335	1336	1339	rBV2	183	72	0.00%	0.001%
30	5.723	1342	1363	1391	rBV2	623265	1671807	100.00%	13.821%
31	6.034	1458	1460	1461	rBV	458	197	0.01%	0.002%
32	6.108	1480	1483	1484	rBV2	449	308	0.02%	0.003%
33	6.186	1504	1507	1508	rBV	183	88	0.01%	0.001%
34	6.247	1512	1526	1546	rBV	453922	859792	51.43%	7.108%
35	6.536	1605	1616	1625	rVB7	5024	10077	0.60%	0.083%
36	6.690	1649	1664	1687	rBV	391395	767541	45.91%	6.345%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050845.D
 Acq On : 20 Sep 2022 20:45
 Operator : JC/MD
 Sample : N4651-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.960	1743	1748	1749	rBV2	710	513	0.03%	0.004%
38	7.189	1811	1819	1827	rBV7	1515	2588	0.15%	0.021%
39	7.272	1843	1845	1848	rVB2	170	80	0.00%	0.001%
40	7.288	1848	1850	1855	rVB	192	126	0.01%	0.001%

41	7.314	1855	1858	1862	rBV2	385	271	0.02%	0.002%
42	7.330	1862	1863	1866	rVB	187	63	0.00%	0.001%
43	7.349	1866	1869	1871	rBV	183	122	0.01%	0.001%
44	7.378	1875	1878	1879	rBV	104	56	0.00%	0.000%
45	7.388	1879	1881	1883	rBV	319	151	0.01%	0.001%

46	7.427	1890	1893	1900	rVB2	408	443	0.03%	0.004%
47	7.456	1900	1902	1905	rBV	241	181	0.01%	0.001%
48	7.565	1924	1936	1957	rBV	189941	334503	20.01%	2.765%
49	7.796	2002	2008	2010	rBV2	542	630	0.04%	0.005%
50	7.896	2026	2039	2054	rBV	693929	1190555	71.21%	9.842%

51	8.179	2114	2127	2144	rBV	135662	227771	13.62%	1.883%
52	8.401	2194	2196	2199	rBV3	381	276	0.02%	0.002%
53	8.468	2209	2217	2228	rVB2	1652	2692	0.16%	0.022%
54	8.555	2242	2244	2250	rVB3	666	520	0.03%	0.004%
55	8.632	2255	2268	2296	rBV2	563128	1051204	62.88%	8.690%

56	9.054	2397	2399	2403	rBV3	246	202	0.01%	0.002%
57	9.137	2424	2425	2426	rBV3	243	67	0.00%	0.001%
58	9.279	2463	2469	2471	rBV	325	286	0.02%	0.002%
59	9.353	2490	2492	2495	rBV2	133	58	0.00%	0.000%
60	9.417	2498	2512	2537	rBV	629505	1041369	62.29%	8.609%

61	9.639	2578	2581	2583	rBV	405	235	0.01%	0.002%
62	9.693	2592	2598	2606	rBV3	1151	1668	0.10%	0.014%
63	9.857	2647	2649	2652	rBV2	184	105	0.01%	0.001%
64	9.893	2657	2660	2661	rBV2	395	223	0.01%	0.002%
65	9.963	2678	2682	2686	rBV2	423	331	0.02%	0.003%

66	10.111	2725	2728	2730	rVB	334	166	0.01%	0.001%
67	10.179	2747	2749	2755	rVB	243	171	0.01%	0.001%
68	10.230	2761	2765	2772	rVB2	666	584	0.03%	0.005%
69	10.430	2824	2827	2828	rBV	276	143	0.01%	0.001%
70	10.671	2894	2902	2910	rBV6	2266	2820	0.17%	0.023%

71	10.754	2916	2928	2943	rBV	560920	903864	54.07%	7.472%
72	11.015	3007	3009	3013	rBV3	412	225	0.01%	0.002%
73	11.053	3018	3021	3023	rBV	487	246	0.01%	0.002%
74	11.092	3028	3033	3034	rBV2	292	239	0.01%	0.002%
75	11.102	3034	3036	3038	rBV3	414	222	0.01%	0.002%

76	11.240	3076	3079	3082	rBV2	333	300	0.02%	0.002%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050845.D
Acq On : 20 Sep 2022 20:45
Operator : JC/MD
Sample : N4651-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ47

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Title : VOC Analysis

77	11.812	3245	3257	3282	rBV	488450	788169	47.14%	6.516%
78	12.192	3362	3375	3394	rBV	574127	933369	55.83%	7.716%
79	12.430	3444	3449	3452	rBV4	1201	1282	0.08%	0.011%
80	12.822	3569	3571	3575	rBV3	809	573	0.03%	0.005%
81	13.423	3756	3758	3763	rBV2	702	669	0.04%	0.006%




Sum of corrected areas: 12096096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050845.D
Acq On : 20 Sep 2022 20:45
Operator : JC/MD
Sample : N4651-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

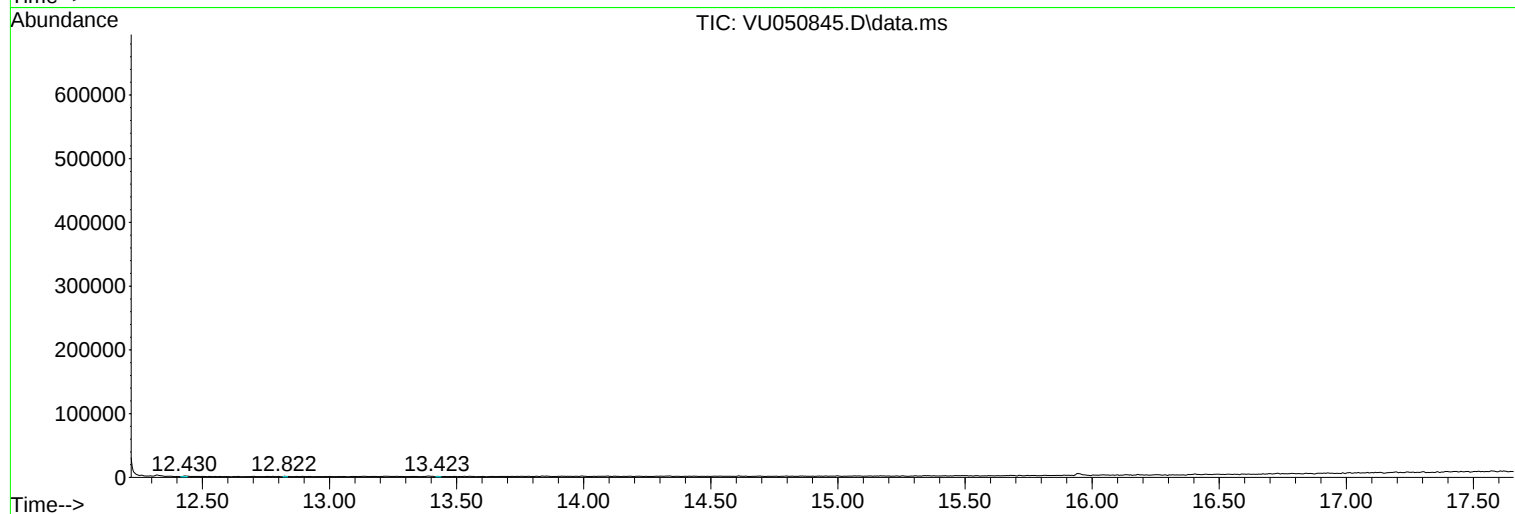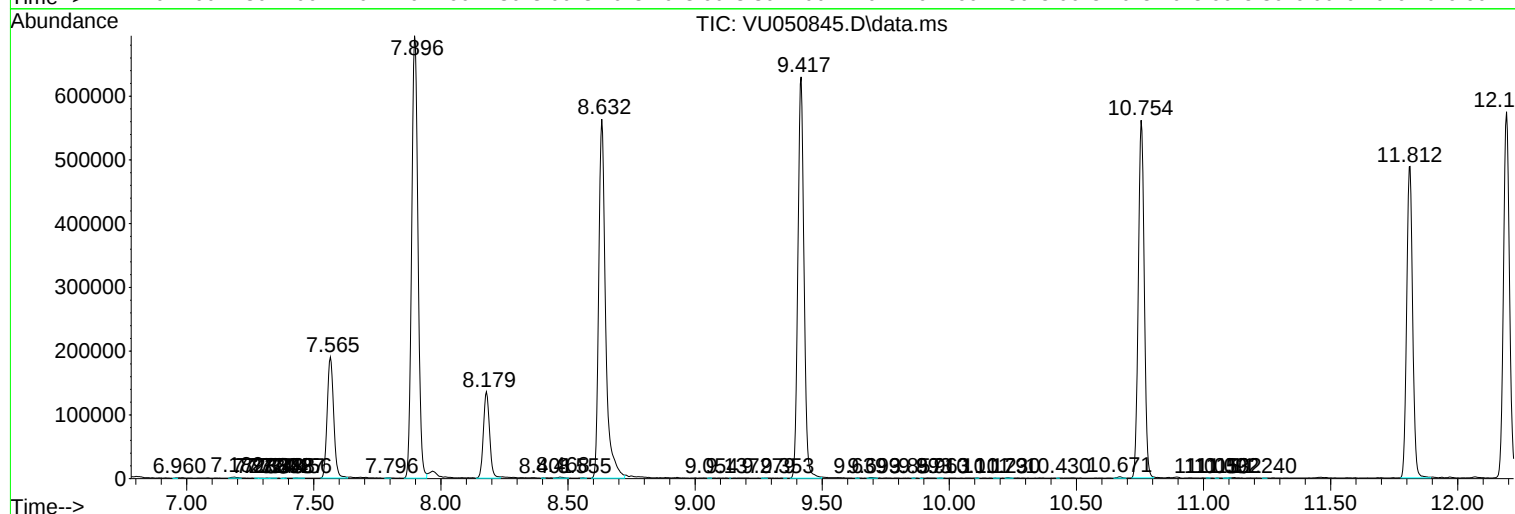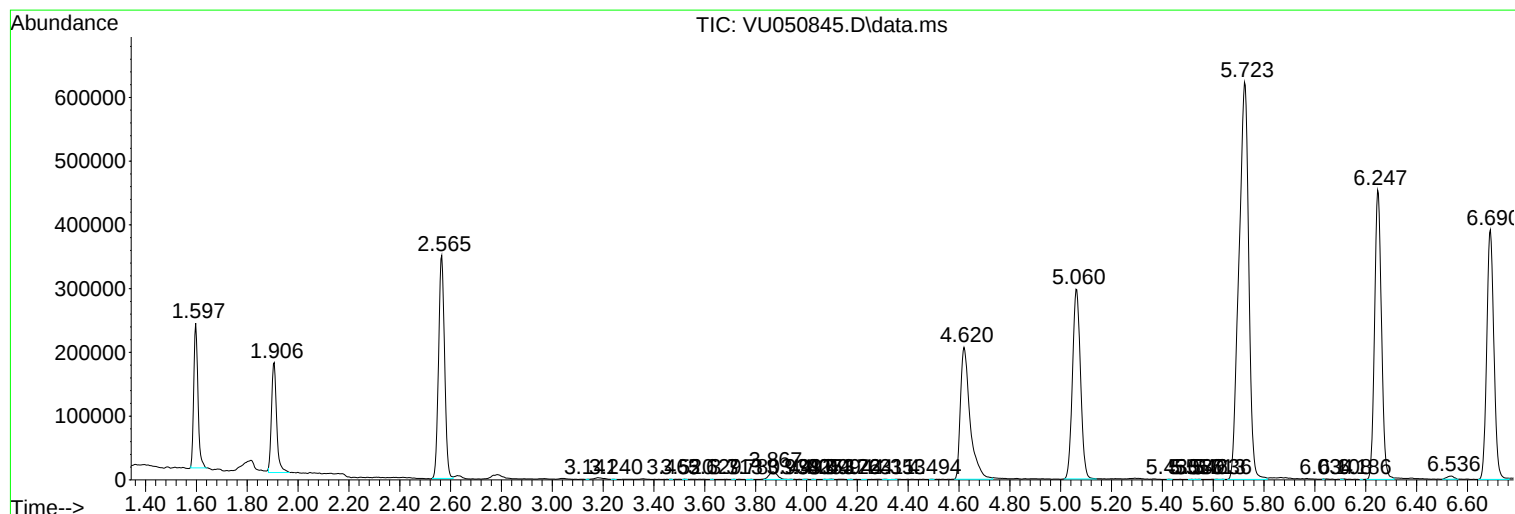

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050845.D
Acq On : 20 Sep 2022 20:45
Operator : JC/MD
Sample : N4651-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050845.D
Acq On : 20 Sep 2022 20:45
Operator : JC/MD
Sample : N4651-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------