

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050846.D
 Acq On : 20 Sep 2022 21:08
 Operator : JC/MD
 Sample : N4651-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	224215	270359	16.45%	2.021%
2	1.906	169	176	193	rVB	190712	252375	15.36%	1.887%
3	2.565	368	381	399	rBV3	386476	703059	42.79%	5.257%
4	2.729	429	432	433	rBV	577	278	0.02%	0.002%
5	2.832	461	464	466	rBV	665	463	0.03%	0.003%
6	2.912	487	489	491	rBV3	500	295	0.02%	0.002%
7	3.047	520	531	541	rVB3	5654	10406	0.63%	0.078%
8	3.128	551	556	559	rBV	276	290	0.02%	0.002%
9	3.182	559	573	590	rBV	22444	52045	3.17%	0.389%
10	3.285	603	605	611	rVB2	389	322	0.02%	0.002%
11	3.317	611	615	617	rBV	479	343	0.02%	0.003%
12	3.356	617	627	637	rVB4	2917	5992	0.36%	0.045%
13	3.530	678	681	686	rVV	345	306	0.02%	0.002%
14	3.636	711	714	720	rVB2	510	460	0.03%	0.003%
15	3.867	769	786	809	rBV	74232	179403	10.92%	1.341%
16	4.073	846	850	856	rVB2	269	296	0.02%	0.002%
17	4.144	869	872	876	rVV	374	287	0.02%	0.002%
18	4.182	881	884	887	rVB3	509	338	0.02%	0.003%
19	4.243	898	903	908	rVV3	306	286	0.02%	0.002%
20	4.295	916	919	924	rVB2	434	287	0.02%	0.002%
21	4.366	938	941	950	rVB	466	558	0.03%	0.004%
22	4.536	987	994	996	rBV2	407	414	0.03%	0.003%
23	4.626	1008	1022	1062	rBV	210331	658474	40.08%	4.923%
24	4.813	1077	1080	1083	rVB2	675	345	0.02%	0.003%
25	4.983	1131	1133	1137	rVB	538	327	0.02%	0.002%
26	5.060	1141	1157	1177	rBV	294914	655485	39.89%	4.901%
27	5.314	1218	1236	1257	rBV2	238107	540974	32.93%	4.045%
28	5.452	1275	1279	1281	rVV3	558	327	0.02%	0.002%
29	5.472	1281	1285	1287	rVV3	399	335	0.02%	0.003%
30	5.507	1291	1296	1302	rVV6	537	646	0.04%	0.005%
31	5.722	1341	1363	1384	rBV2	615236	1643042	100.00%	12.285%
32	6.124	1486	1488	1493	rVB3	485	320	0.02%	0.002%
33	6.192	1507	1509	1512	rVB2	469	296	0.02%	0.002%
34	6.247	1512	1526	1548	rBV	476474	907874	55.26%	6.788%
35	6.398	1570	1573	1582	rVB6	1266	1403	0.09%	0.010%
36	6.542	1604	1618	1638	rVB5	48119	94875	5.77%	0.709%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050846.D
 Acq On : 20 Sep 2022 21:08
 Operator : JC/MD
 Sample : N4651-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1648	1664	1683	rBV	386853	760538	46.29%	5.686%
38	6.796	1689	1697	1698	rBV5	1324	1464	0.09%	0.011%
39	7.144	1802	1805	1809	rVB2	419	338	0.02%	0.003%
40	7.192	1809	1820	1825	rBV5	2227	3146	0.19%	0.024%
41	7.449	1893	1900	1903	rBV3	259	324	0.02%	0.002%
42	7.565	1921	1936	1953	rBV	185791	329786	20.07%	2.466%
43	7.687	1970	1974	1977	rBV4	702	599	0.04%	0.004%
44	7.896	2024	2039	2056	rBV	677372	1167506	71.06%	8.729%
45	8.179	2114	2127	2153	rBV	128958	226085	13.76%	1.690%
46	8.365	2182	2185	2188	rBV2	442	311	0.02%	0.002%
47	8.398	2189	2195	2204	rVB7	1833	3101	0.19%	0.023%
48	8.456	2210	2213	2215	rBV2	746	558	0.03%	0.004%
49	8.472	2215	2218	2223	rVB4	1137	985	0.06%	0.007%
50	8.552	2232	2243	2256	rBV	69107	115201	7.01%	0.861%
51	8.632	2256	2268	2300	rBV2	544918	1043696	63.52%	7.803%
52	8.976	2370	2375	2379	rBV3	483	487	0.03%	0.004%
53	8.996	2379	2381	2386	rBV3	587	565	0.03%	0.004%
54	9.102	2410	2414	2419	rVB3	655	579	0.04%	0.004%
55	9.131	2419	2423	2431	rVB3	552	548	0.03%	0.004%
56	9.218	2447	2450	2455	rVB2	369	298	0.02%	0.002%
57	9.417	2497	2512	2539	rBV	659402	1094757	66.63%	8.185%
58	9.574	2557	2561	2565	rVB4	680	651	0.04%	0.005%
59	9.684	2592	2595	2597	rBV	546	389	0.02%	0.003%
60	9.697	2597	2599	2606	rVB4	1056	939	0.06%	0.007%
61	9.764	2616	2620	2625	rBV2	412	407	0.02%	0.003%
62	10.002	2690	2694	2697	rBV2	522	376	0.02%	0.003%
63	10.246	2764	2770	2773	rBV	578	737	0.04%	0.006%
64	10.269	2773	2777	2783	rVB2	681	684	0.04%	0.005%
65	10.356	2801	2804	2809	rVB3	373	336	0.02%	0.003%
66	10.497	2844	2848	2850	rBV2	417	349	0.02%	0.003%
67	10.671	2895	2902	2911	rBV6	1595	2373	0.14%	0.018%
68	10.754	2915	2928	2955	rVV	548917	882425	53.71%	6.598%
69	10.896	2967	2972	2977	rVB3	924	980	0.06%	0.007%
70	11.092	3028	3033	3035	rBV2	472	483	0.03%	0.004%
71	11.121	3037	3042	3047	rVV4	679	692	0.04%	0.005%
72	11.452	3138	3145	3147	rBV2	1343	1192	0.07%	0.009%
73	11.574	3180	3183	3187	rVB3	445	371	0.02%	0.003%
74	11.693	3218	3220	3226	rVB4	505	490	0.03%	0.004%
75	11.745	3232	3236	3239	rBV3	383	293	0.02%	0.002%
76	11.812	3243	3257	3282	rBV	502973	820408	49.93%	6.134%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050846.D
 Acq On : 20 Sep 2022 21:08
 Operator : JC/MD
 Sample : N4651-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.947	3295	3299	3301	rBV2	754	577	0.04%	0.004%
78	11.973	3304	3307	3315	rVB6	1592	1834	0.11%	0.014%
79	12.060	3332	3334	3335	rBV2	1104	504	0.03%	0.004%
80	12.192	3360	3375	3395	rBV	562405	906453	55.17%	6.777%
81	12.536	3479	3482	3487	rVB2	650	542	0.03%	0.004%
82	12.578	3491	3495	3500	rVB2	533	480	0.03%	0.004%
83	12.735	3541	3544	3549	rBV	539	405	0.02%	0.003%
84	12.761	3549	3552	3556	rBV3	655	573	0.03%	0.004%
85	13.176	3678	3681	3684	rVB2	610	414	0.03%	0.003%
86	13.201	3687	3689	3693	rVV2	454	304	0.02%	0.002%
87	13.224	3693	3696	3702	rVB4	814	699	0.04%	0.005%
88	13.372	3740	3742	3744	rVV	593	358	0.02%	0.003%
89	13.388	3744	3747	3751	rVV4	1181	925	0.06%	0.007%
90	13.423	3754	3758	3762	rBV3	432	447	0.03%	0.003%
91	13.848	3885	3890	3898	rBV4	993	1158	0.07%	0.009%
92	13.973	3924	3929	3932	rBV3	404	447	0.03%	0.003%
93	14.323	4035	4038	4041	rBV4	858	697	0.04%	0.005%
94	14.455	4076	4079	4081	rBV2	634	407	0.02%	0.003%
95	14.603	4123	4125	4130	rVB3	510	303	0.02%	0.002%
96	14.954	4230	4234	4236	rBV2	699	533	0.03%	0.004%
97	15.301	4339	4342	4348	rBV4	780	741	0.05%	0.006%
98	15.577	4425	4428	4431	rBV6	765	597	0.04%	0.004%
99	15.767	4485	4487	4489	rBV4	852	407	0.02%	0.003%
100	15.947	4536	4543	4551	rBV7	4320	6073	0.37%	0.045%




Sum of corrected areas: 13374910

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050846.D
Acq On : 20 Sep 2022 21:08
Operator : JC/MD
Sample : N4651-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

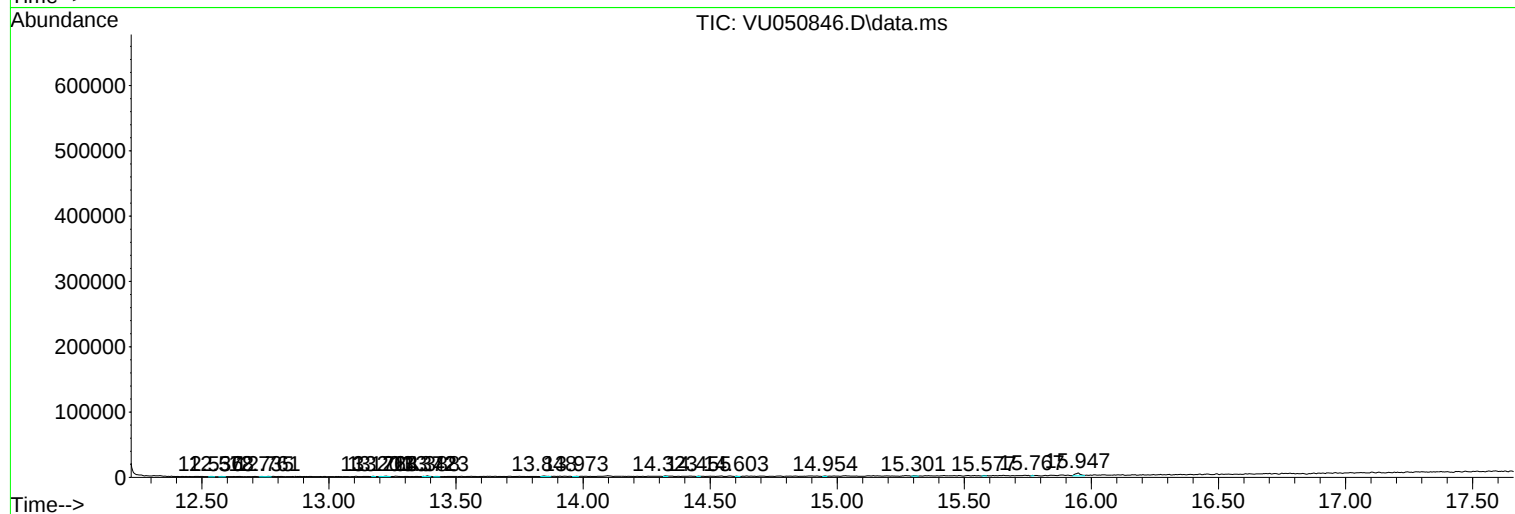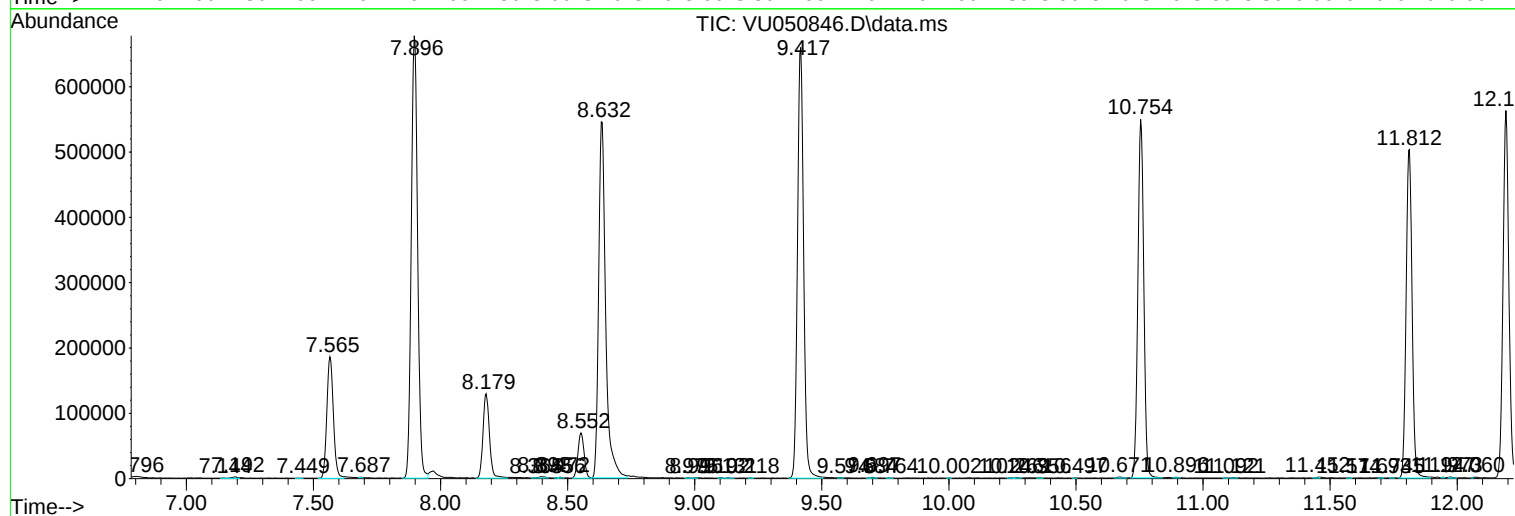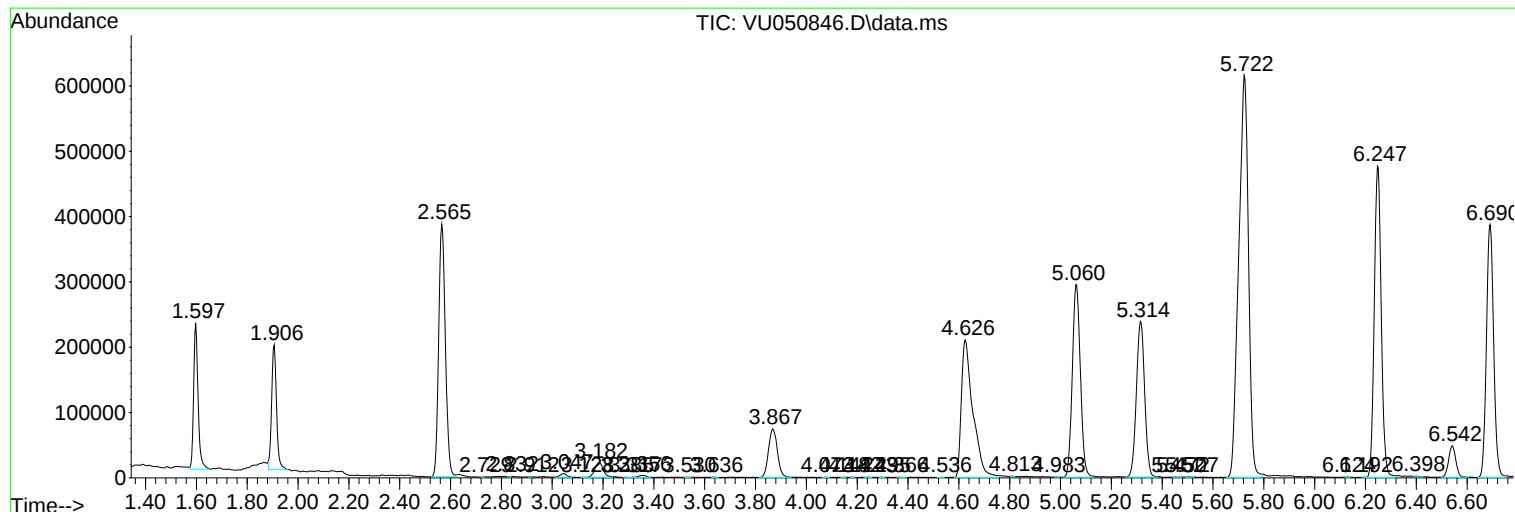

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050846.D
Acq On : 20 Sep 2022 21:08
Operator : JC/MD
Sample : N4651-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050846.D
Acq On : 20 Sep 2022 21:08
Operator : JC/MD
Sample : N4651-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------