

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050847.D
 Acq On : 20 Sep 2022 21:32
 Operator : JC/MD
 Sample : N4651-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB2	271413	341408	21.68%	2.771%
2	1.906	168	176	197	rVB	170578	238129	15.13%	1.933%
3	2.221	272	274	279	rBV4	1163	664	0.04%	0.005%
4	2.565	369	381	397	rVV	340035	555123	35.26%	4.505%
5	2.694	419	421	426	rBV3	567	500	0.03%	0.004%
6	2.848	467	469	474	rVB3	708	526	0.03%	0.004%
7	3.044	518	530	540	rBV3	6116	11221	0.71%	0.091%
8	3.124	548	555	558	rBV	336	391	0.02%	0.003%
9	3.186	558	574	596	rVB2	27335	65447	4.16%	0.531%
10	3.353	615	626	638	rBV2	9136	17937	1.14%	0.146%
11	3.449	651	656	659	rBV3	311	323	0.02%	0.003%
12	3.755	748	751	760	rVB2	406	527	0.03%	0.004%
13	3.867	767	786	812	rVV	250006	591486	37.57%	4.800%
14	4.047	839	842	847	rVB4	462	406	0.03%	0.003%
15	4.115	857	863	866	rBV3	349	381	0.02%	0.003%
16	4.446	962	966	971	rVB3	396	370	0.02%	0.003%
17	4.623	1005	1021	1024	rBV	216029	370983	23.56%	3.011%
18	4.864	1094	1096	1101	rBV4	916	824	0.05%	0.007%
19	5.060	1141	1157	1177	rBV	283230	618215	39.27%	5.017%
20	5.182	1192	1195	1200	rBV4	473	430	0.03%	0.003%
21	5.234	1209	1211	1217	rVB2	586	482	0.03%	0.004%
22	5.317	1223	1237	1249	rVB3	8408	18791	1.19%	0.153%
23	5.472	1278	1285	1290	rBV2	493	580	0.04%	0.005%
24	5.722	1340	1363	1384	rBV2	583037	1574400	100.00%	12.778%
25	5.957	1434	1436	1438	rBV2	840	459	0.03%	0.004%
26	6.105	1479	1482	1488	rVB4	545	540	0.03%	0.004%
27	6.134	1488	1491	1495	rBV3	495	377	0.02%	0.003%
28	6.250	1509	1527	1552	rBV	432716	834772	53.02%	6.775%
29	6.542	1602	1618	1630	rBV5	22837	46512	2.95%	0.377%
30	6.690	1647	1664	1684	rBV	371556	728062	46.24%	5.909%
31	6.893	1724	1727	1730	rVB2	519	335	0.02%	0.003%
32	6.919	1730	1735	1740	rVB	430	375	0.02%	0.003%
33	7.012	1761	1764	1770	rVB3	427	495	0.03%	0.004%
34	7.050	1770	1776	1778	rBV2	592	602	0.04%	0.005%
35	7.185	1810	1818	1830	rBV5	1935	3350	0.21%	0.027%
36	7.565	1923	1936	1952	rBV	176821	309571	19.66%	2.512%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050847.D
 Acq On : 20 Sep 2022 21:32
 Operator : JC/MD
 Sample : N4651-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.690	1971	1975	1982	rVB6	678	770	0.05%	0.006%
38	7.896	2019	2039	2054	rBV	644250	1105850	70.24%	8.975%
39	8.031	2078	2081	2083	rBV2	765	404	0.03%	0.003%
40	8.127	2109	2111	2114	rVB2	593	327	0.02%	0.003%
41	8.179	2114	2127	2146	rBV	125259	215517	13.69%	1.749%
42	8.404	2187	2197	2205	rBV6	1828	3421	0.22%	0.028%
43	8.465	2214	2216	2227	rVB3	914	1104	0.07%	0.009%
44	8.555	2238	2244	2252	rBV6	1681	2422	0.15%	0.020%
45	8.632	2256	2268	2308	rBV2	514689	976945	62.05%	7.929%
46	8.909	2350	2354	2359	rBV4	667	666	0.04%	0.005%
47	9.082	2404	2408	2412	rBV3	626	517	0.03%	0.004%
48	9.144	2423	2427	2430	rBV2	405	331	0.02%	0.003%
49	9.417	2499	2512	2543	rBV	610348	1008197	64.04%	8.182%
50	9.571	2554	2560	2570	rVB3	5441	7919	0.50%	0.064%
51	9.690	2586	2597	2608	rBV2	7415	12903	0.82%	0.105%
52	9.934	2668	2673	2679	rBV2	473	544	0.03%	0.004%
53	10.041	2702	2706	2711	rVB3	410	451	0.03%	0.004%
54	10.098	2714	2724	2738	rVB3	13246	21127	1.34%	0.171%
55	10.243	2765	2769	2774	rVB	488	376	0.02%	0.003%
56	10.279	2774	2780	2786	rBV3	487	644	0.04%	0.005%
57	10.414	2817	2822	2827	rBV2	252	333	0.02%	0.003%
58	10.488	2835	2845	2850	rBV4	1980	2693	0.17%	0.022%
59	10.668	2893	2901	2910	rVB5	1795	2322	0.15%	0.019%
60	10.754	2914	2928	2947	rBV	529061	850453	54.02%	6.902%
61	10.835	2951	2953	2957	rVV2	388	330	0.02%	0.003%
62	10.861	2957	2961	2966	rVB3	803	832	0.05%	0.007%
63	10.902	2966	2974	2984	rVB3	3325	4868	0.31%	0.040%
64	10.957	2987	2991	2994	rBV2	336	327	0.02%	0.003%
65	10.999	2994	3004	3015	rBV2	9132	14237	0.90%	0.116%
66	11.092	3022	3033	3040	rBV3	4203	6220	0.40%	0.050%
67	11.291	3088	3095	3107	rVB4	7171	10373	0.66%	0.084%
68	11.468	3139	3150	3161	rVB2	21044	33276	2.11%	0.270%
69	11.584	3183	3186	3189	rVB2	688	369	0.02%	0.003%
70	11.693	3211	3220	3230	rBV5	1061	1868	0.12%	0.015%
71	11.745	3230	3236	3240	rVB3	864	780	0.05%	0.006%
72	11.809	3242	3256	3275	rBV	473815	764008	48.53%	6.201%
73	11.896	3275	3283	3296	rVB3	11634	18470	1.17%	0.150%
74	11.973	3301	3307	3312	rVV6	1411	1945	0.12%	0.016%
75	12.095	3335	3345	3353	rBV5	4103	6432	0.41%	0.052%
76	12.192	3362	3375	3394	rBV	541129	876801	55.69%	7.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050847.D
 Acq On : 20 Sep 2022 21:32
 Operator : JC/MD
 Sample : N4651-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.362	3424	3428	3432	rBV3	525	427	0.03%	0.003%
78	12.481	3455	3465	3478	rVB5	5582	10496	0.67%	0.085%
79	12.568	3490	3492	3497	rBV3	524	401	0.03%	0.003%
80	12.709	3530	3536	3539	rBV3	568	741	0.05%	0.006%
81	12.729	3539	3542	3547	rVB2	502	460	0.03%	0.004%
82	12.873	3584	3587	3590	rBV2	703	421	0.03%	0.003%
83	12.902	3593	3596	3599	rVB3	687	472	0.03%	0.004%
84	12.931	3602	3605	3610	rBV2	396	424	0.03%	0.003%
85	12.979	3615	3620	3623	rVB4	528	481	0.03%	0.004%
86	13.018	3629	3632	3636	rBV3	688	610	0.04%	0.005%
87	13.092	3651	3655	3659	rBV3	518	460	0.03%	0.004%
88	13.131	3665	3667	3671	rBV3	487	431	0.03%	0.003%
89	13.224	3693	3696	3703	rVB3	845	885	0.06%	0.007%
90	13.262	3703	3708	3712	rBV3	1299	1121	0.07%	0.009%
91	13.577	3803	3806	3811	rBV	451	394	0.03%	0.003%
92	14.095	3959	3967	3975	rBV4	2022	3090	0.20%	0.025%
93	14.169	3987	3990	3993	rBV3	428	332	0.02%	0.003%
94	14.452	4073	4078	4082	rBV2	579	628	0.04%	0.005%
95	14.475	4082	4085	4090	rVB4	592	490	0.03%	0.004%
96	14.568	4111	4114	4120	rVB3	717	650	0.04%	0.005%
97	14.645	4135	4138	4142	rVB2	780	631	0.04%	0.005%
98	15.121	4283	4286	4288	rBV2	665	406	0.03%	0.003%
99	15.860	4514	4516	4519	rVB2	1134	580	0.04%	0.005%
100	15.944	4538	4542	4552	rVB8	3771	4228	0.27%	0.034%




Sum of corrected areas: 12321625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050847.D
Acq On : 20 Sep 2022 21:32
Operator : JC/MD
Sample : N4651-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

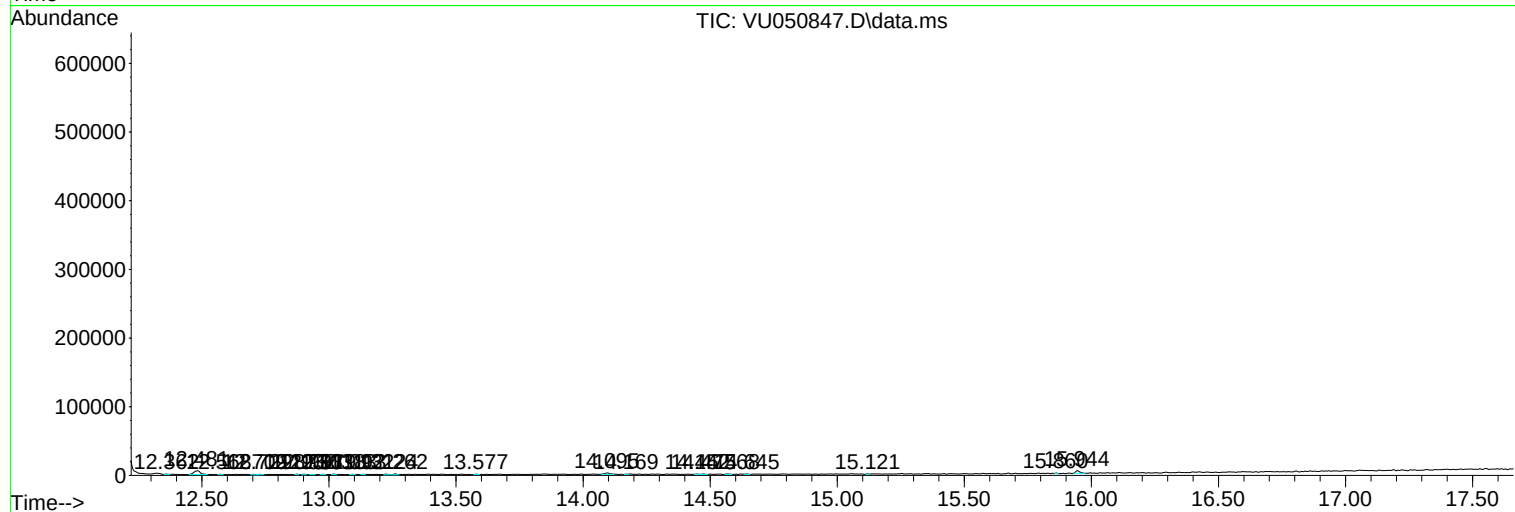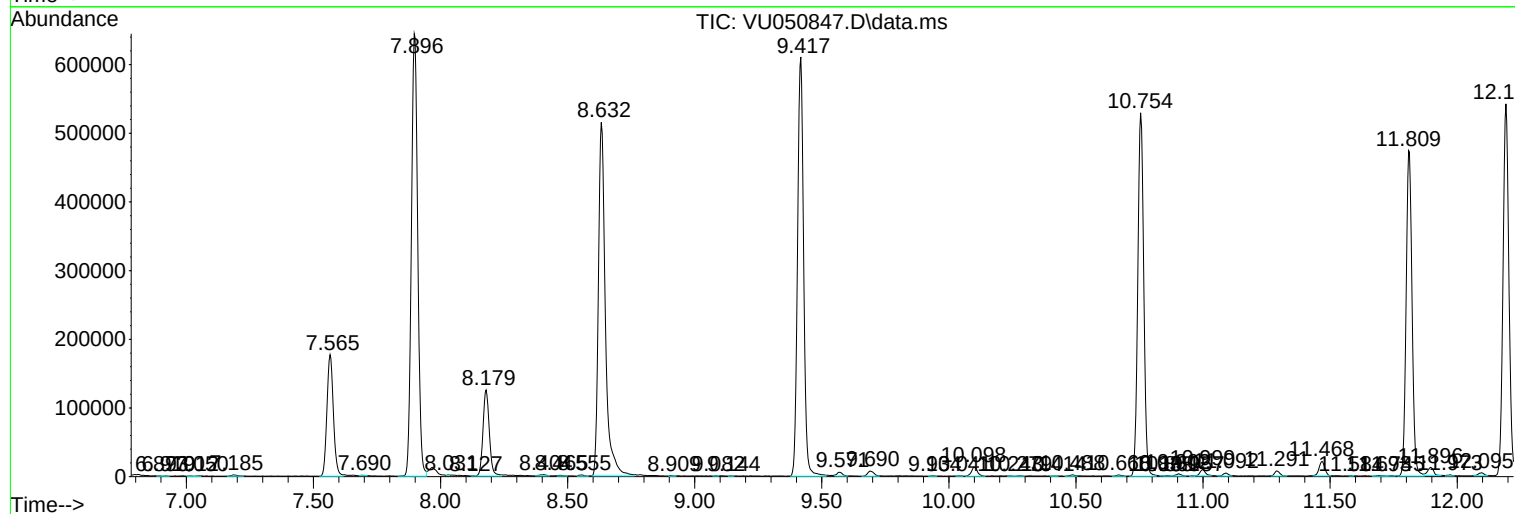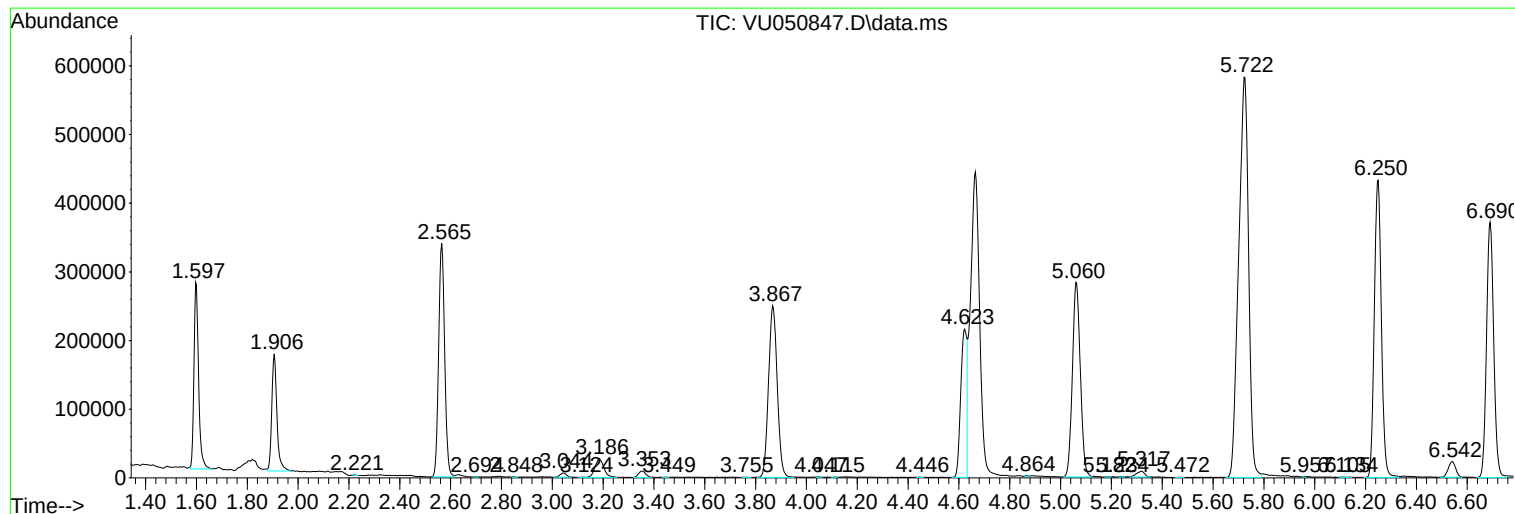

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050847.D
Acq On : 20 Sep 2022 21:32
Operator : JC/MD
Sample : N4651-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050847.D
Acq On : 20 Sep 2022 21:32
Operator : JC/MD
Sample : N4651-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------