

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050848.D
 Acq On : 20 Sep 2022 21:56
 Operator : JC/MD
 Sample : N4651-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB2	277109	344431	21.13%	2.706%
2	1.906	169	176	195	rVB	180992	250493	15.37%	1.968%
3	2.565	367	381	399	rBV	339708	567203	34.80%	4.457%
4	2.739	432	435	441	rVB5	685	643	0.04%	0.005%
5	2.777	441	447	448	rBV2	948	845	0.05%	0.007%
6	2.813	455	458	462	rBV2	971	516	0.03%	0.004%
7	2.874	475	477	481	rVB2	529	318	0.02%	0.002%
8	2.928	492	494	497	rBV2	443	339	0.02%	0.003%
9	3.044	520	530	545	rVB3	6680	12535	0.77%	0.098%
10	3.125	551	555	558	rVV3	485	389	0.02%	0.003%
11	3.182	559	573	596	rVV2	20590	49973	3.07%	0.393%
12	3.356	615	627	638	rBV3	9753	19365	1.19%	0.152%
13	3.414	643	645	652	rBV	469	373	0.02%	0.003%
14	3.478	661	665	668	rVB3	365	304	0.02%	0.002%
15	3.867	766	786	811	rBV	255692	606235	37.20%	4.763%
16	4.327	926	929	933	rBV2	369	345	0.02%	0.003%
17	4.626	1007	1022	1024	rBV	223578	367335	22.54%	2.886%
18	5.063	1141	1158	1178	rBV	291530	643406	39.48%	5.056%
19	5.314	1225	1236	1248	rVB5	8222	18967	1.16%	0.149%
20	5.385	1256	1258	1265	rVB5	862	768	0.05%	0.006%
21	5.722	1341	1363	1383	rBV2	606493	1629755	100.00%	12.806%
22	6.054	1463	1466	1468	rBV	592	323	0.02%	0.003%
23	6.247	1512	1526	1547	rVV	461555	874746	53.67%	6.873%
24	6.359	1558	1561	1562	rBV2	801	433	0.03%	0.003%
25	6.539	1604	1617	1633	rVB6	22621	47408	2.91%	0.373%
26	6.690	1649	1664	1686	rBV	386589	750166	46.03%	5.894%
27	6.957	1745	1747	1753	rVV2	484	399	0.02%	0.003%
28	6.993	1753	1758	1763	rVV5	437	525	0.03%	0.004%
29	7.038	1767	1772	1774	rBV3	554	506	0.03%	0.004%
30	7.070	1778	1782	1789	rVB4	562	566	0.03%	0.004%
31	7.189	1810	1819	1830	rBV7	1488	2805	0.17%	0.022%
32	7.423	1887	1892	1895	rBV2	319	305	0.02%	0.002%
33	7.478	1906	1909	1914	rBV2	322	326	0.02%	0.003%
34	7.565	1923	1936	1957	rBV	184127	323629	19.86%	2.543%
35	7.796	2005	2008	2016	rVB4	499	538	0.03%	0.004%
36	7.896	2025	2039	2054	rBV	662791	1154744	70.85%	9.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050848.D
 Acq On : 20 Sep 2022 21:56
 Operator : JC/MD
 Sample : N4651-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	8.179	2111	2127	2149	rBV	127777	223996	13.74%	1.760%
38	8.292	2160	2162	2165	rBV2	653	438	0.03%	0.003%
39	8.401	2190	2196	2201	rBV4	1987	2662	0.16%	0.021%
40	8.472	2214	2218	2221	rBV2	611	506	0.03%	0.004%
41	8.549	2238	2242	2244	rBV3	977	777	0.05%	0.006%
42	8.632	2253	2268	2306	rBV2	546234	1042155	63.95%	8.189%
43	8.909	2352	2354	2356	rBV2	549	324	0.02%	0.003%
44	9.192	2436	2442	2443	rBV2	369	341	0.02%	0.003%
45	9.417	2498	2512	2538	rBV	624952	1051325	64.51%	8.261%
46	9.571	2554	2560	2573	rVB2	5414	7987	0.49%	0.063%
47	9.623	2573	2576	2582	rVB2	512	446	0.03%	0.004%
48	9.693	2588	2598	2611	rVB3	6032	9855	0.60%	0.077%
49	9.854	2642	2648	2653	rVB3	713	898	0.06%	0.007%
50	10.018	2696	2699	2703	rVV2	357	341	0.02%	0.003%
51	10.044	2703	2707	2710	rVB2	468	405	0.02%	0.003%
52	10.099	2715	2724	2738	rVB2	10822	17286	1.06%	0.136%
53	10.243	2764	2769	2772	rBV	353	328	0.02%	0.003%
54	10.381	2807	2812	2815	rBV2	372	369	0.02%	0.003%
55	10.488	2838	2845	2850	rBV4	1820	2048	0.13%	0.016%
56	10.568	2866	2870	2872	rBV	394	322	0.02%	0.003%
57	10.664	2893	2900	2909	rBV4	1421	2483	0.15%	0.020%
58	10.754	2914	2928	2951	rBV	549517	881297	54.08%	6.925%
59	10.906	2964	2975	2980	rVV4	2058	2863	0.18%	0.022%
60	10.996	2996	3003	3020	rVB	7324	12836	0.79%	0.101%
61	11.092	3025	3033	3039	rBV5	2095	3246	0.20%	0.026%
62	11.227	3067	3075	3078	rVV2	384	546	0.03%	0.004%
63	11.246	3078	3081	3083	rVV	465	329	0.02%	0.003%
64	11.266	3083	3087	3088	rVV3	461	367	0.02%	0.003%
65	11.291	3088	3095	3106	rVB5	5895	9477	0.58%	0.074%
66	11.381	3117	3123	3129	rBV2	475	596	0.04%	0.005%
67	11.414	3131	3133	3138	rVV2	381	316	0.02%	0.002%
68	11.468	3138	3150	3163	rVB2	13664	22302	1.37%	0.175%
69	11.555	3170	3177	3180	rBV2	367	391	0.02%	0.003%
70	11.574	3180	3183	3187	rBV4	567	472	0.03%	0.004%
71	11.687	3215	3218	3220	rBV2	815	488	0.03%	0.004%
72	11.809	3243	3256	3272	rBV	491796	797789	48.95%	6.269%
73	11.893	3275	3282	3293	rVB2	9064	13899	0.85%	0.109%
74	11.967	3302	3305	3315	rVB5	2119	2728	0.17%	0.021%
75	12.060	3331	3334	3337	rBV3	559	402	0.02%	0.003%
76	12.089	3337	3343	3353	rVB6	3294	5265	0.32%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050848.D
 Acq On : 20 Sep 2022 21:56
 Operator : JC/MD
 Sample : N4651-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.192	3362	3375	3396	rBV	563211	911206	55.91%	7.160%
78	12.317	3408	3414	3416	rBV4	893	1036	0.06%	0.008%
79	12.385	3432	3435	3443	rBV4	717	523	0.03%	0.004%
80	12.478	3456	3464	3473	rBV4	5846	8199	0.50%	0.064%
81	12.587	3495	3498	3501	rBV3	639	468	0.03%	0.004%
82	12.877	3584	3588	3590	rBV	494	481	0.03%	0.004%
83	12.918	3599	3601	3606	rVB2	479	356	0.02%	0.003%
84	13.102	3654	3658	3661	rBV2	373	341	0.02%	0.003%
85	13.343	3729	3733	3735	rBV2	439	359	0.02%	0.003%
86	13.442	3761	3764	3769	rVB3	451	369	0.02%	0.003%
87	13.549	3794	3797	3805	rVB3	454	449	0.03%	0.004%
88	13.979	3927	3931	3933	rBV3	539	484	0.03%	0.004%
89	14.092	3955	3966	3971	rBV8	2255	3832	0.24%	0.030%
90	14.179	3990	3993	3996	rBV4	634	499	0.03%	0.004%
91	14.336	4039	4042	4048	rVB4	660	593	0.04%	0.005%
92	14.385	4052	4057	4060	rBV2	512	625	0.04%	0.005%
93	14.503	4092	4094	4099	rBV4	481	458	0.03%	0.004%
94	14.757	4170	4173	4176	rBV	678	499	0.03%	0.004%
95	14.902	4216	4218	4223	rVB3	635	354	0.02%	0.003%
96	15.047	4260	4263	4264	rBV2	597	318	0.02%	0.002%
97	15.163	4296	4299	4302	rBV3	740	566	0.03%	0.004%
98	15.211	4312	4314	4317	rBV3	652	440	0.03%	0.003%
99	15.484	4396	4399	4404	rBV4	747	813	0.05%	0.006%
100	15.667	4452	4456	4457	rBV2	798	579	0.04%	0.005%




Sum of corrected areas: 12726705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050848.D
Acq On : 20 Sep 2022 21:56
Operator : JC/MD
Sample : N4651-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

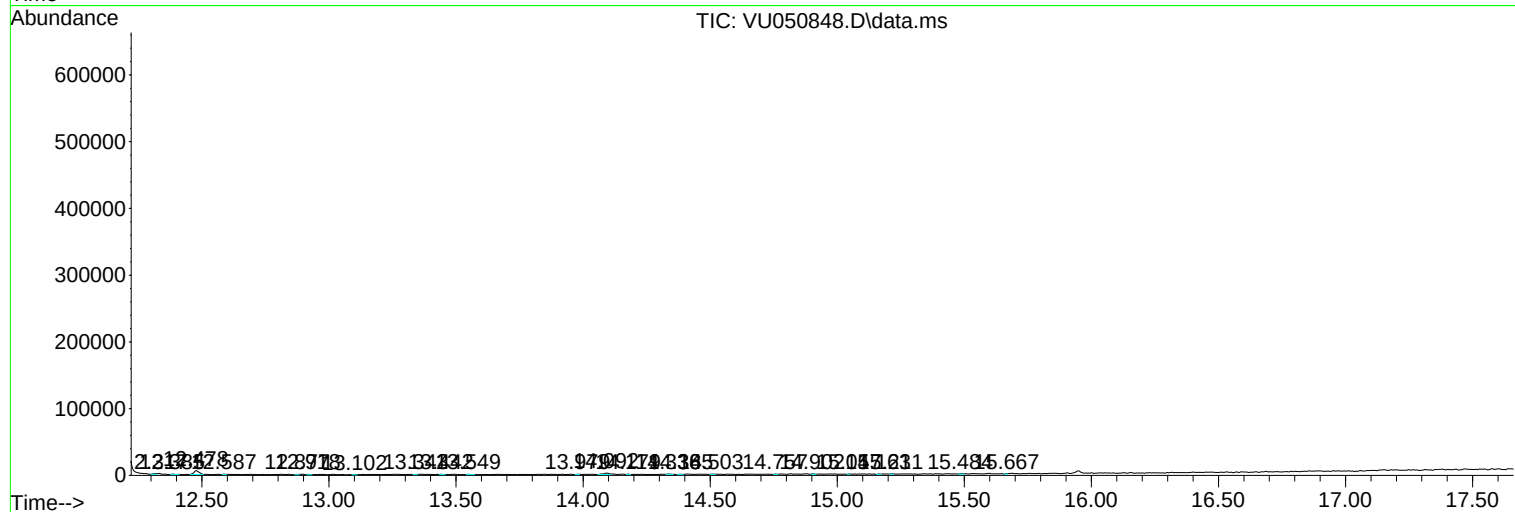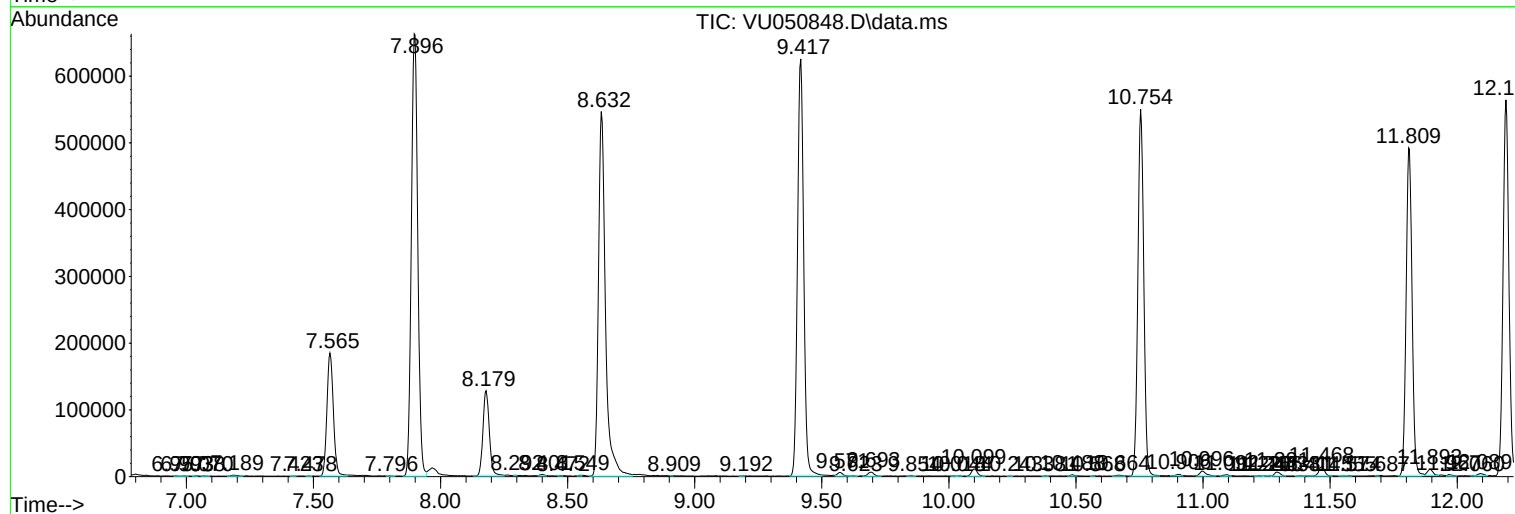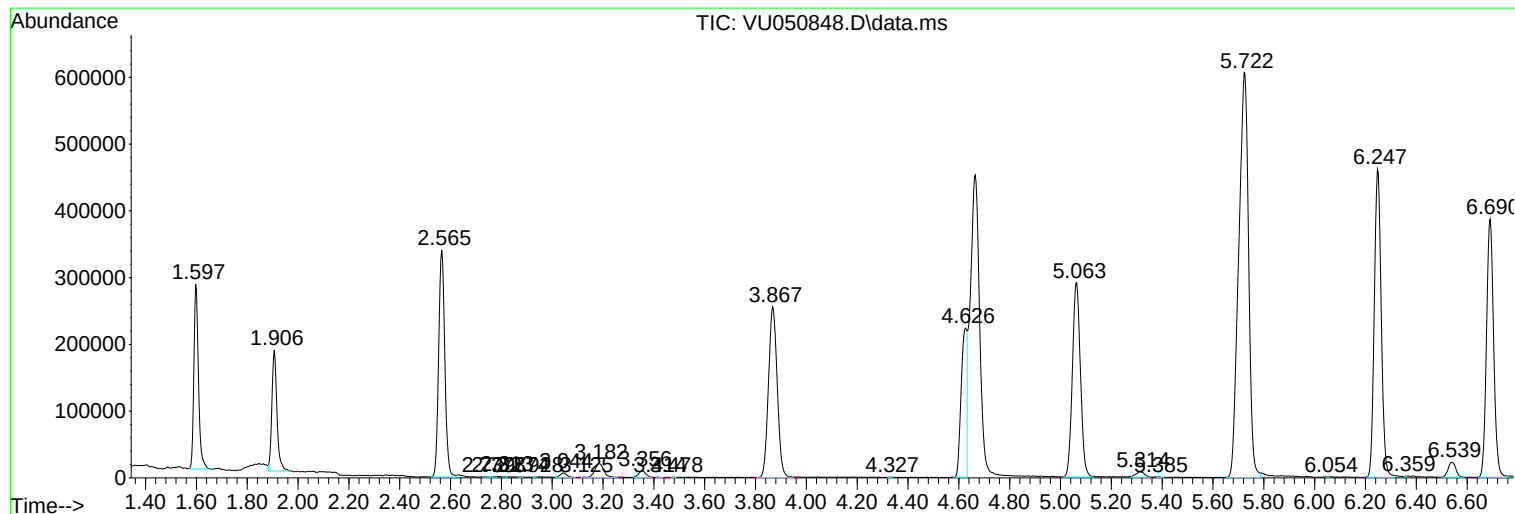

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050848.D
Acq On : 20 Sep 2022 21:56
Operator : JC/MD
Sample : N4651-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050848.D
Acq On : 20 Sep 2022 21:56
Operator : JC/MD
Sample : N4651-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------