

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050849.D
 Acq On : 20 Sep 2022 22:19
 Operator : JC/MD
 Sample : VIBLK133
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK133

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	267037	311033	15.89%	2.192%
2	1.909	169	177	201	rVB	227592	305707	15.62%	2.155%
3	2.565	368	381	400	rBV	406100	665503	34.01%	4.690%
4	2.790	447	451	454	rBV2	749	750	0.04%	0.005%
5	3.002	512	517	519	rBV3	416	373	0.02%	0.003%
6	3.041	519	529	541	rVB3	8281	16138	0.82%	0.114%
7	3.121	550	554	558	rBV2	356	290	0.01%	0.002%
8	3.183	558	573	588	rBV	14253	32001	1.64%	0.226%
9	3.298	605	609	613	rBV2	566	476	0.02%	0.003%
10	3.375	630	633	637	rBV2	277	274	0.01%	0.002%
11	3.710	735	737	740	rVB2	550	301	0.02%	0.002%
12	3.742	740	747	748	rBV	324	325	0.02%	0.002%
13	3.855	778	782	784	rBV2	379	274	0.01%	0.002%
14	4.015	828	832	835	rVV2	391	297	0.02%	0.002%
15	4.096	851	857	860	rBV	348	279	0.01%	0.002%
16	4.183	880	884	890	rVB	284	318	0.02%	0.002%
17	4.237	895	901	906	rBV2	424	499	0.03%	0.004%
18	4.404	950	953	957	rVB2	337	267	0.01%	0.002%
19	4.626	1005	1022	1052	rBV	216725	572838	29.27%	4.037%
20	4.922	1111	1114	1116	rBV2	559	367	0.02%	0.003%
21	5.064	1140	1158	1190	rBV	350596	775934	39.65%	5.469%
22	5.334	1238	1242	1245	rVB3	580	443	0.02%	0.003%
23	5.649	1333	1340	1341	rBV	427	445	0.02%	0.003%
24	5.723	1341	1363	1393	rBV2	726326	1956877	100.00%	13.792%
25	5.973	1437	1441	1446	rVB3	792	748	0.04%	0.005%
26	5.999	1446	1449	1452	rVB4	660	296	0.02%	0.002%
27	6.051	1463	1465	1471	rVB2	536	341	0.02%	0.002%
28	6.170	1497	1502	1507	rVB3	481	463	0.02%	0.003%
29	6.247	1511	1526	1552	rBV	556586	1055956	53.96%	7.442%
30	6.526	1604	1613	1625	rVB4	6589	12515	0.64%	0.088%
31	6.690	1649	1664	1684	rBV	465811	904719	46.23%	6.376%
32	7.031	1765	1770	1772	rBV2	450	377	0.02%	0.003%
33	7.141	1801	1804	1808	rVB2	520	400	0.02%	0.003%
34	7.182	1808	1817	1818	rBV4	1300	1139	0.06%	0.008%
35	7.449	1898	1900	1905	rVB2	432	285	0.01%	0.002%
36	7.501	1911	1916	1921	rBV2	460	541	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050849.D
 Acq On : 20 Sep 2022 22:19
 Operator : JC/MD
 Sample : VIBLK133
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK133

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.565	1924	1936	1954	rBV	222645	392020	20.03%	2.763%
38	7.687	1971	1974	1975	rBV	581	305	0.02%	0.002%
39	7.784	2001	2004	2006	rBV2	618	528	0.03%	0.004%
40	7.899	2025	2040	2055	rBV	804218	1398432	71.46%	9.856%
41	8.118	2104	2108	2111	rVB3	393	275	0.01%	0.002%
42	8.179	2115	2127	2151	rBV	157183	272139	13.91%	1.918%
43	8.366	2183	2185	2191	rVB4	498	425	0.02%	0.003%
44	8.462	2212	2215	2216	rBV2	709	380	0.02%	0.003%
45	8.552	2239	2243	2248	rVB7	844	858	0.04%	0.006%
46	8.632	2256	2268	2300	rBV2	607405	1143828	58.45%	8.061%
47	8.874	2340	2343	2347	rBV4	507	519	0.03%	0.004%
48	8.915	2352	2356	2367	rVB3	3254	4537	0.23%	0.032%
49	9.160	2426	2432	2437	rBV5	583	733	0.04%	0.005%
50	9.205	2441	2446	2449	rVV2	268	293	0.01%	0.002%
51	9.243	2453	2458	2462	rVV2	264	263	0.01%	0.002%
52	9.417	2498	2512	2550	rBV	770378	1287865	65.81%	9.077%
53	9.571	2555	2560	2563	rBV2	975	1002	0.05%	0.007%
54	9.649	2582	2584	2587	rVV	599	395	0.02%	0.003%
55	9.671	2587	2591	2593	rVV2	571	500	0.03%	0.004%
56	9.694	2593	2598	2607	rVB5	1033	1625	0.08%	0.011%
57	9.841	2638	2644	2648	rBV	526	472	0.02%	0.003%
58	9.874	2648	2654	2657	rBV	428	460	0.02%	0.003%
59	10.163	2738	2744	2747	rBV2	371	430	0.02%	0.003%
60	10.340	2795	2799	2802	rVV	471	314	0.02%	0.002%
61	10.459	2831	2836	2839	rBV3	366	313	0.02%	0.002%
62	10.533	2855	2859	2863	rBV2	340	331	0.02%	0.002%
63	10.668	2893	2901	2909	rVB5	2143	3118	0.16%	0.022%
64	10.755	2914	2928	2951	rVV	637428	1035962	52.94%	7.301%
65	10.957	2987	2991	2997	rVV2	517	547	0.03%	0.004%
66	11.015	3007	3009	3014	rVV2	556	330	0.02%	0.002%
67	11.092	3026	3033	3035	rVV5	750	848	0.04%	0.006%
68	11.128	3039	3044	3048	rVB4	719	686	0.04%	0.005%
69	11.221	3070	3073	3076	rVB2	385	280	0.01%	0.002%
70	11.320	3101	3104	3109	rBV2	369	360	0.02%	0.003%
71	11.459	3136	3147	3152	rBV6	1730	3183	0.16%	0.022%
72	11.671	3210	3213	3215	rBV2	431	300	0.02%	0.002%
73	11.690	3217	3219	3224	rVB3	737	592	0.03%	0.004%
74	11.809	3243	3256	3283	rBV	567222	929353	47.49%	6.550%
75	11.964	3302	3304	3305	rBV	588	265	0.01%	0.002%
76	11.999	3313	3315	3318	rBV	450	292	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050849.D
 Acq On : 20 Sep 2022 22:19
 Operator : JC/MD
 Sample : VIBLK133
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK133

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.070	3335	3337	3340	rBV2	435	307	0.02%	0.002%
78	12.124	3351	3354	3359	rBV2	449	376	0.02%	0.003%
79	12.192	3359	3375	3396	rBV	656390	1068612	54.61%	7.531%
80	12.327	3415	3417	3421	rVB2	915	597	0.03%	0.004%
81	12.462	3456	3459	3460	rBV2	700	341	0.02%	0.002%
82	12.584	3494	3497	3500	rBV	580	407	0.02%	0.003%
83	12.806	3562	3566	3569	rBV3	589	453	0.02%	0.003%
84	12.877	3586	3588	3591	rVV3	567	298	0.02%	0.002%
85	12.909	3591	3598	3601	rVV2	612	832	0.04%	0.006%
86	12.925	3601	3603	3606	rVV2	823	441	0.02%	0.003%
87	12.986	3618	3622	3626	rBV3	431	333	0.02%	0.002%
88	13.041	3636	3639	3644	rVB3	502	420	0.02%	0.003%
89	13.076	3644	3650	3652	rBV2	636	553	0.03%	0.004%
90	13.144	3668	3671	3674	rVV2	749	544	0.03%	0.004%
91	13.169	3677	3679	3682	rVV3	692	450	0.02%	0.003%
92	13.234	3692	3699	3703	rBV3	696	988	0.05%	0.007%
93	13.266	3707	3709	3715	rBV4	273	291	0.01%	0.002%
94	13.327	3725	3728	3731	rBV3	508	452	0.02%	0.003%
95	13.369	3738	3741	3743	rBV3	462	320	0.02%	0.002%
96	13.462	3762	3770	3773	rBV3	717	1105	0.06%	0.008%
97	13.726	3849	3852	3856	rVV3	544	415	0.02%	0.003%
98	14.336	4039	4042	4047	rBV4	848	774	0.04%	0.005%
99	14.983	4240	4243	4245	rBV2	609	377	0.02%	0.003%
100	15.944	4539	4542	4550	rVB8	3642	4102	0.21%	0.029%




Sum of corrected areas: 14188935

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050849.D
Acq On : 20 Sep 2022 22:19
Operator : JC/MD
Sample : VIBLK133
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

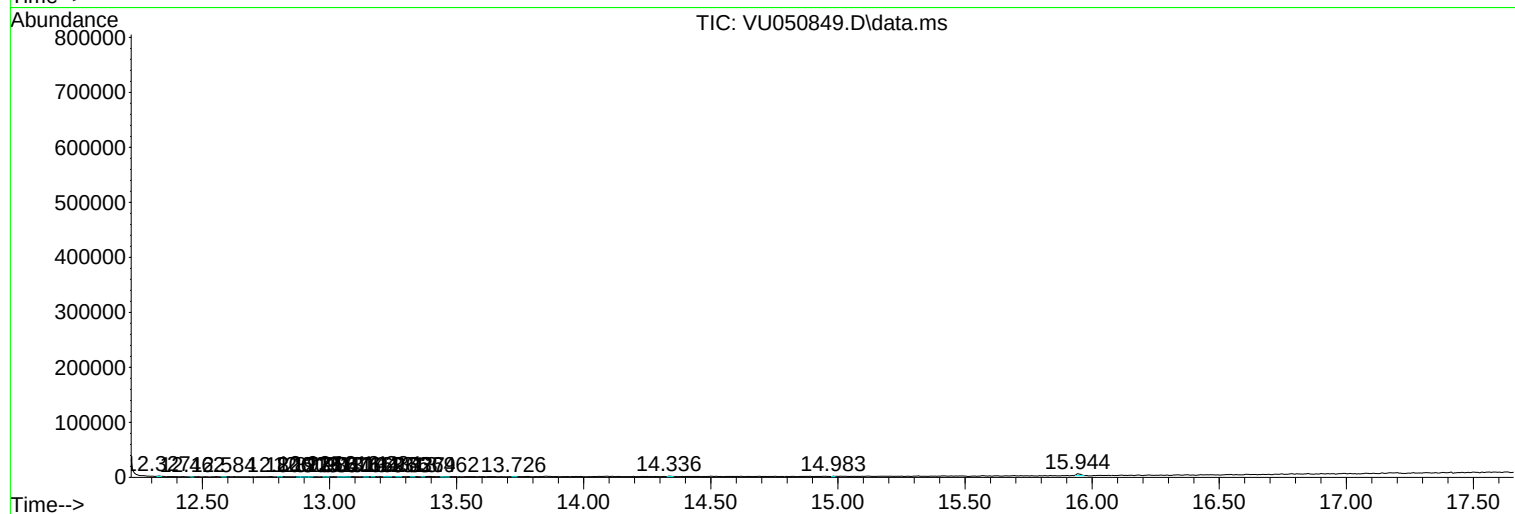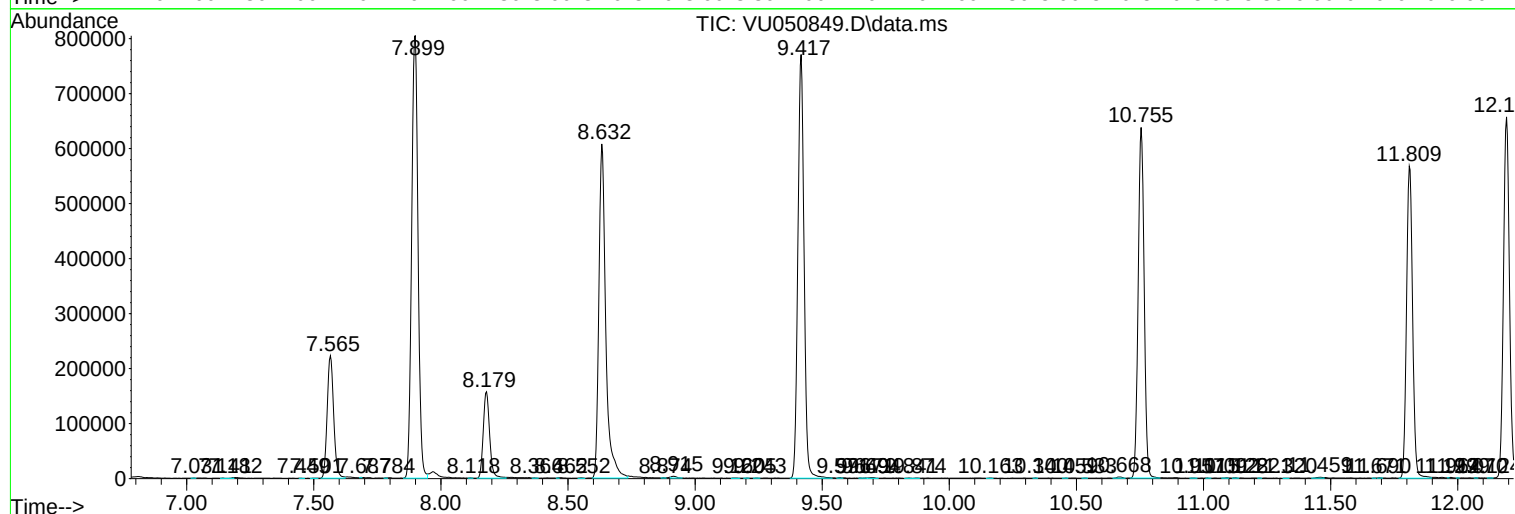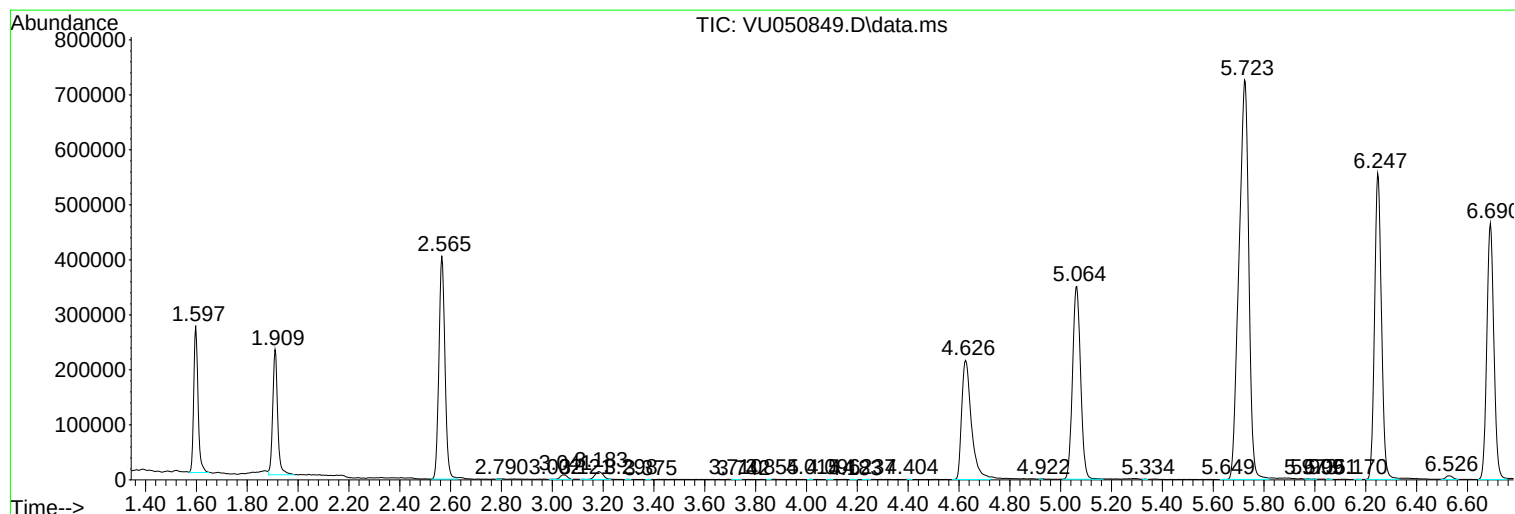

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050849.D
Acq On : 20 Sep 2022 22:19
Operator : JC/MD
Sample : VIBLK133
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050849.D
Acq On : 20 Sep 2022 22:19
Operator : JC/MD
Sample : VIBLK133
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
