

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050850.D
 Acq On : 20 Sep 2022 22:43
 Operator : JC/MD
 Sample : N4651-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	261839	307301	4.40%	1.134%
2	1.906	168	176	196	rVB	200410	271385	3.89%	1.002%
3	2.077	225	229	237	rVB2	14798	18342	0.26%	0.068%
4	2.138	241	248	253	rBV	15351	22391	0.32%	0.083%
5	2.575	368	384	411	rBV4	1298483	2399337	34.36%	8.857%
6	2.768	436	444	463	rVB3	6361	14971	0.21%	0.055%
7	2.925	490	493	496	rBV3	940	535	0.01%	0.002%
8	3.048	521	531	540	rVB6	2836	5501	0.08%	0.020%
9	3.096	540	546	549	rBV2	401	418	0.01%	0.002%
10	3.176	563	571	577	rBV2	1768	2543	0.04%	0.009%
11	3.257	593	596	604	rBV3	500	622	0.01%	0.002%
12	3.353	612	626	648	rBV2	37167	74688	1.07%	0.276%
13	3.671	719	725	732	rVB3	389	502	0.01%	0.002%
14	3.748	740	749	753	rBV3	605	859	0.01%	0.003%
15	3.867	766	786	816	rBV	931298	2203439	31.56%	8.134%
16	4.073	844	850	852	rBV3	630	591	0.01%	0.002%
17	4.318	922	926	930	rBV3	328	381	0.01%	0.001%
18	4.446	962	966	970	rBV2	364	391	0.01%	0.001%
19	4.556	995	1000	1002	rBV3	608	405	0.01%	0.001%
20	4.620	1006	1020	1024	rBV	219461	407092	5.83%	1.503%
21	5.060	1141	1157	1183	rBV	342118	778512	11.15%	2.874%
22	5.189	1194	1197	1199	rBV3	575	312	0.00%	0.001%
23	5.314	1216	1236	1259	rBV	3121470	6982466	100.00%	25.777%
24	5.723	1342	1363	1394	rBV2	703219	1881479	26.95%	6.946%
25	6.150	1491	1496	1499	rBV2	367	362	0.01%	0.001%
26	6.247	1513	1526	1552	rBV	508958	965432	13.83%	3.564%
27	6.453	1588	1590	1596	rVB3	433	335	0.00%	0.001%
28	6.539	1603	1617	1637	rBV	572653	1087139	15.57%	4.013%
29	6.690	1649	1664	1684	rBV	439914	854620	12.24%	3.155%
30	6.973	1748	1752	1755	rBV3	694	634	0.01%	0.002%
31	7.038	1766	1772	1778	rBV3	563	704	0.01%	0.003%
32	7.170	1804	1813	1815	rBV2	1246	1173	0.02%	0.004%
33	7.247	1832	1837	1840	rVB2	379	372	0.01%	0.001%
34	7.276	1840	1846	1850	rBV2	407	464	0.01%	0.002%
35	7.449	1897	1900	1906	rVB2	392	423	0.01%	0.002%
36	7.475	1906	1908	1912	rBV	435	321	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050850.D
 Acq On : 20 Sep 2022 22:43
 Operator : JC/MD
 Sample : N4651-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.565	1923	1936	1951	rBV	209700	371367	5.32%	1.371%
38	7.690	1970	1975	1978	rBV6	1049	1174	0.02%	0.004%
39	7.797	2003	2008	2013	rVB2	497	519	0.01%	0.002%
40	7.819	2013	2015	2023	rVB3	563	576	0.01%	0.002%
41	7.896	2023	2039	2054	rBV	782913	1338075	19.16%	4.940%
42	8.179	2115	2127	2145	rBV	152885	259969	3.72%	0.960%
43	8.401	2185	2196	2209	rVB2	29480	49721	0.71%	0.184%
44	8.469	2214	2217	2226	rVB4	1247	1472	0.02%	0.005%
45	8.552	2230	2243	2256	rBV	890496	1486790	21.29%	5.489%
46	8.633	2257	2268	2299	rVB2	590156	1115756	15.98%	4.119%
47	8.922	2354	2358	2359	rBV3	504	341	0.00%	0.001%
48	9.314	2475	2480	2482	rBV2	341	329	0.00%	0.001%
49	9.417	2499	2512	2533	rBV	710006	1176130	16.84%	4.342%
50	9.571	2554	2560	2564	rBV6	853	1220	0.02%	0.005%
51	9.690	2591	2597	2605	rVB6	1158	1646	0.02%	0.006%
52	9.726	2605	2608	2617	rBV5	917	1328	0.02%	0.005%
53	9.938	2670	2674	2677	rBV3	593	441	0.01%	0.002%
54	9.996	2690	2692	2698	rVB3	483	463	0.01%	0.002%
55	10.031	2698	2703	2708	rBV3	447	579	0.01%	0.002%
56	10.099	2721	2724	2728	rVB3	508	502	0.01%	0.002%
57	10.202	2749	2756	2761	rBV3	557	629	0.01%	0.002%
58	10.671	2892	2902	2910	rVB5	1696	3064	0.04%	0.011%
59	10.755	2915	2928	2957	rBV	627360	1005922	14.41%	3.713%
60	10.874	2961	2965	2967	rBV3	887	712	0.01%	0.003%
61	11.057	3019	3022	3029	rBV3	315	318	0.00%	0.001%
62	11.089	3029	3032	3035	rBV2	416	326	0.00%	0.001%
63	11.214	3067	3071	3076	rBV3	466	522	0.01%	0.002%
64	11.356	3110	3115	3119	rBV3	321	379	0.01%	0.001%
65	11.443	3136	3142	3143	rVV	831	518	0.01%	0.002%
66	11.462	3145	3148	3158	rVV6	1802	2663	0.04%	0.010%
67	11.565	3175	3180	3183	rBV2	336	367	0.01%	0.001%
68	11.642	3198	3204	3209	rBV3	452	616	0.01%	0.002%
69	11.700	3215	3222	3226	rBV5	990	1149	0.02%	0.004%
70	11.739	3231	3234	3235	rBV2	590	328	0.00%	0.001%
71	11.809	3244	3256	3279	rBV	556511	895418	12.82%	3.306%
72	11.954	3298	3301	3302	rBV2	628	344	0.00%	0.001%
73	12.073	3327	3338	3348	rBV6	2429	4447	0.06%	0.016%
74	12.192	3361	3375	3392	rBV	650490	1059577	15.17%	3.912%
75	12.317	3408	3414	3415	rBV5	803	717	0.01%	0.003%
76	12.378	3429	3433	3436	rBV2	840	747	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050850.D
 Acq On : 20 Sep 2022 22:43
 Operator : JC/MD
 Sample : N4651-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.446	3449	3454	3457	rBV	741	747	0.01%	0.003%
78	12.600	3500	3502	3507	rVV	435	313	0.00%	0.001%
79	12.639	3510	3514	3516	rVV3	527	411	0.01%	0.002%
80	12.713	3534	3537	3542	rBV2	491	422	0.01%	0.002%
81	12.758	3548	3551	3557	rVV2	360	383	0.01%	0.001%
82	12.896	3591	3594	3596	rBV3	785	422	0.01%	0.002%
83	13.224	3692	3696	3699	rBV2	1031	938	0.01%	0.003%
84	13.272	3706	3711	3713	rBV4	700	566	0.01%	0.002%
85	13.288	3713	3716	3719	rVB2	565	367	0.01%	0.001%
86	13.340	3729	3732	3739	rBV4	459	599	0.01%	0.002%
87	13.369	3739	3741	3744	rBV2	520	430	0.01%	0.002%
88	13.436	3757	3762	3765	rBV2	635	572	0.01%	0.002%
89	13.909	3905	3909	3912	rBV2	640	556	0.01%	0.002%
90	13.992	3932	3935	3938	rBV2	976	693	0.01%	0.003%
91	14.137	3977	3980	3984	rVB2	744	475	0.01%	0.002%
92	14.173	3988	3991	3993	rBV	624	363	0.01%	0.001%
93	14.333	4037	4041	4045	rVB3	1036	757	0.01%	0.003%
94	14.353	4045	4047	4050	rBV2	717	406	0.01%	0.001%
95	14.520	4096	4099	4102	rBV2	737	495	0.01%	0.002%
96	14.684	4148	4150	4155	rVB2	569	312	0.00%	0.001%
97	14.938	4226	4229	4231	rVB2	679	316	0.00%	0.001%
98	15.147	4291	4294	4296	rVB2	787	427	0.01%	0.002%
99	15.475	4393	4396	4397	rBV3	705	466	0.01%	0.002%
100	15.947	4539	4543	4550	rVB8	2908	3267	0.05%	0.012%




Sum of corrected areas: 27088306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050850.D
Acq On : 20 Sep 2022 22:43
Operator : JC/MD
Sample : N4651-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

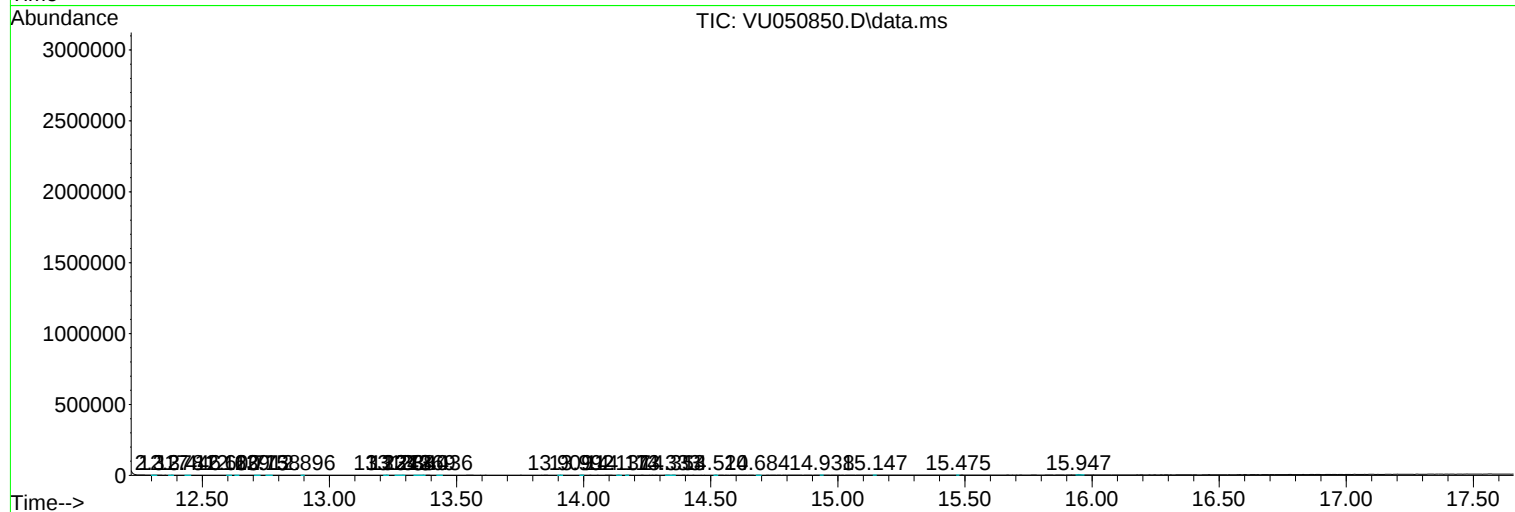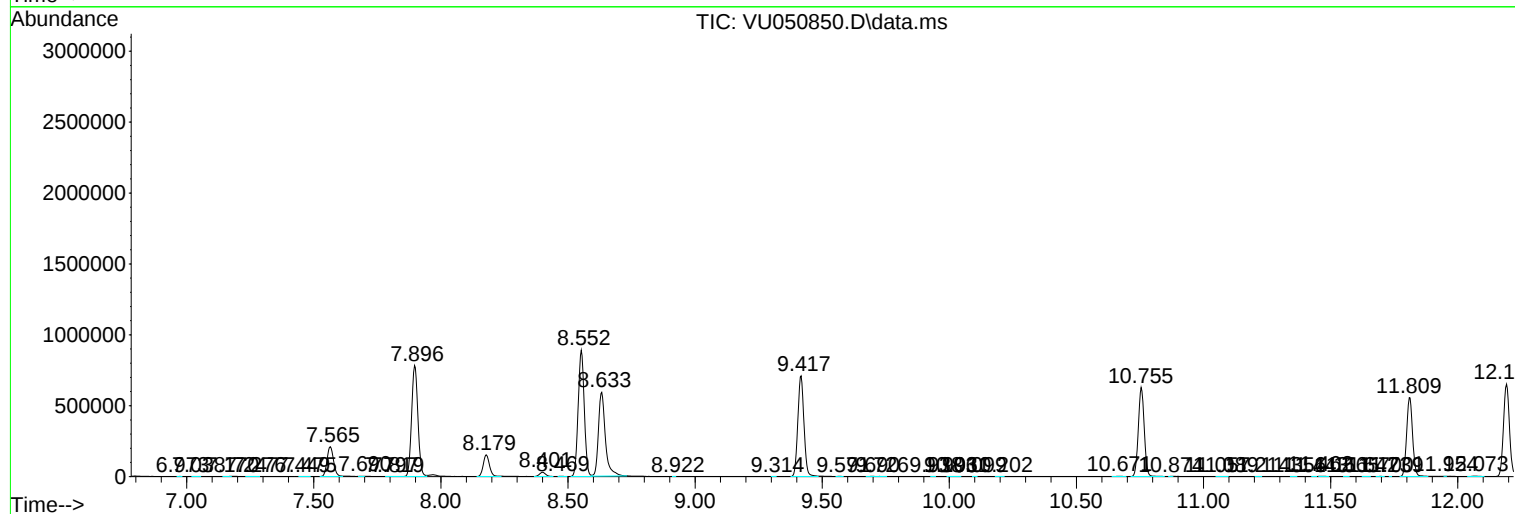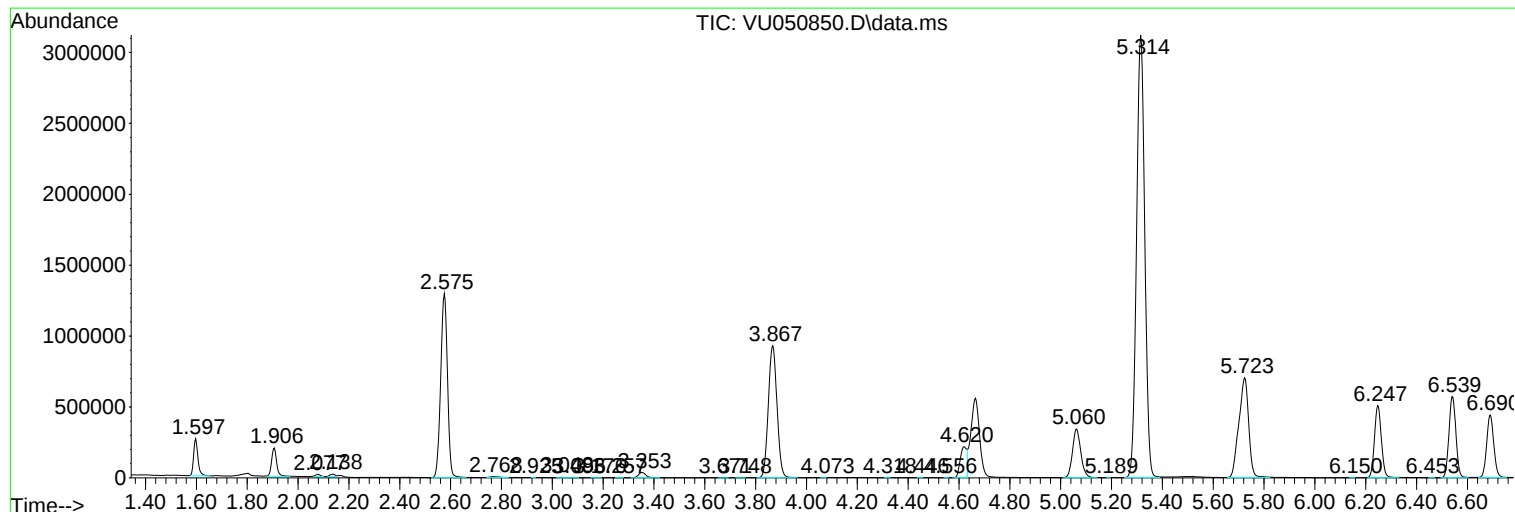

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050850.D
Acq On : 20 Sep 2022 22:43
Operator : JC/MD
Sample : N4651-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050850.D
Acq On : 20 Sep 2022 22:43
Operator : JC/MD
Sample : N4651-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc