

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050852.D
 Acq On : 20 Sep 2022 23:54
 Operator : JC/MD
 Sample : VU0920WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	288123	341049	17.01%	2.387%
2	1.909	169	177	200	rVB	238022	319437	15.93%	2.236%
3	2.565	368	381	400	rBV	436155	711247	35.47%	4.979%
4	2.851	467	470	475	rVV2	534	459	0.02%	0.003%
5	2.900	482	485	489	rBV2	301	278	0.01%	0.002%
6	2.951	498	501	503	rBV2	459	303	0.02%	0.002%
7	3.041	520	529	541	rVB3	6228	11492	0.57%	0.080%
8	3.176	561	571	573	rBV2	4663	5352	0.27%	0.037%
9	3.263	594	598	599	rBV2	481	278	0.01%	0.002%
10	3.318	609	615	617	rBV2	401	400	0.02%	0.003%
11	3.343	617	623	625	rBV2	753	655	0.03%	0.005%
12	3.568	690	693	701	rVB2	448	428	0.02%	0.003%
13	3.607	701	705	707	rBV2	421	364	0.02%	0.003%
14	3.758	748	752	757	rBV3	318	288	0.01%	0.002%
15	3.854	776	782	784	rBV2	247	283	0.01%	0.002%
16	3.877	786	789	795	rVB4	723	808	0.04%	0.006%
17	3.925	800	804	806	rBV	332	282	0.01%	0.002%
18	4.096	851	857	862	rBV2	426	508	0.03%	0.004%
19	4.356	932	938	943	rBV2	414	512	0.03%	0.004%
20	4.504	981	984	991	rVB3	364	343	0.02%	0.002%
21	4.623	1008	1021	1051	rBV	214145	555013	27.68%	3.885%
22	5.063	1139	1158	1183	rBV	358610	793383	39.56%	5.554%
23	5.211	1202	1204	1207	rVV2	447	337	0.02%	0.002%
24	5.285	1221	1227	1230	rBV3	1033	1227	0.06%	0.009%
25	5.369	1250	1253	1256	rBV	867	628	0.03%	0.004%
26	5.488	1284	1290	1293	rBV2	439	342	0.02%	0.002%
27	5.533	1299	1304	1308	rBV2	362	340	0.02%	0.002%
28	5.613	1321	1329	1334	rVB2	420	434	0.02%	0.003%
29	5.723	1341	1363	1385	rBV2	749350	2005381	100.00%	14.038%
30	6.108	1480	1483	1487	rBV2	384	377	0.02%	0.003%
31	6.247	1512	1526	1545	rBV	540114	1019624	50.84%	7.138%
32	6.420	1577	1580	1583	rVB2	812	508	0.03%	0.004%
33	6.462	1589	1593	1598	rVB	9546	5822	0.29%	0.041%
34	6.533	1604	1615	1624	rVB7	7516	13952	0.70%	0.098%
35	6.690	1649	1664	1683	rBV	475414	922015	45.98%	6.454%
36	7.054	1775	1777	1783	rVB3	595	424	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050852.D
 Acq On : 20 Sep 2022 23:54
 Operator : JC/MD
 Sample : VU0920WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.099	1788	1791	1795	rVB2	306	269	0.01%	0.002%
38	7.189	1812	1819	1826	rBV6	1501	2331	0.12%	0.016%
39	7.414	1884	1889	1894	rBV2	427	388	0.02%	0.003%
40	7.565	1921	1936	1956	rBV	217908	391362	19.52%	2.740%
41	7.838	2017	2021	2025	rVB2	354	345	0.02%	0.002%
42	7.896	2025	2039	2055	rBV	837299	1436500	71.63%	10.056%
43	8.179	2115	2127	2142	rBV	157381	266556	13.29%	1.866%
44	8.401	2194	2196	2200	rVB2	529	323	0.02%	0.002%
45	8.549	2238	2242	2244	rBV6	1567	1454	0.07%	0.010%
46	8.632	2253	2268	2303	rBV2	606480	1161724	57.93%	8.132%
47	8.890	2346	2348	2351	rVB4	521	265	0.01%	0.002%
48	8.912	2351	2355	2358	rBV4	929	889	0.04%	0.006%
49	8.973	2371	2374	2378	rBV	355	294	0.01%	0.002%
50	9.160	2428	2432	2436	rBV3	438	444	0.02%	0.003%
51	9.417	2498	2512	2546	rBV	754035	1250135	62.34%	8.751%
52	9.575	2557	2561	2565	rVB2	848	731	0.04%	0.005%
53	9.697	2591	2599	2610	rVB4	1636	2859	0.14%	0.020%
54	9.758	2613	2618	2621	rBV2	370	332	0.02%	0.002%
55	9.896	2658	2661	2664	rBV2	404	293	0.01%	0.002%
56	10.050	2705	2709	2711	rBV2	428	325	0.02%	0.002%
57	10.089	2717	2721	2724	rBV	857	798	0.04%	0.006%
58	10.111	2724	2728	2738	rVB5	1487	2246	0.11%	0.016%
59	10.481	2837	2843	2849	rVB3	718	872	0.04%	0.006%
60	10.574	2869	2872	2878	rBV	300	283	0.01%	0.002%
61	10.645	2891	2894	2895	rBV2	572	270	0.01%	0.002%
62	10.668	2896	2901	2902	rBV2	1313	1103	0.06%	0.008%
63	10.755	2915	2928	2945	rBV	649762	1050083	52.36%	7.351%
64	10.973	2993	2996	3001	rVB3	406	405	0.02%	0.003%
65	11.089	3022	3032	3034	rBV3	847	1219	0.06%	0.009%
66	11.256	3081	3084	3090	rBV2	388	363	0.02%	0.003%
67	11.359	3110	3116	3118	rBV3	551	518	0.03%	0.004%
68	11.449	3140	3144	3145	rBV3	707	524	0.03%	0.004%
69	11.465	3145	3149	3160	rVB6	2227	3623	0.18%	0.025%
70	11.513	3160	3164	3167	rBV2	342	320	0.02%	0.002%
71	11.562	3175	3179	3180	rBV	532	355	0.02%	0.002%
72	11.613	3190	3195	3199	rVB2	620	630	0.03%	0.004%
73	11.697	3218	3221	3227	rVB3	612	541	0.03%	0.004%
74	11.745	3227	3236	3244	rBV7	1966	3453	0.17%	0.024%
75	11.812	3244	3257	3276	rBV	549317	880609	43.91%	6.164%
76	12.008	3316	3318	3322	rVB3	466	317	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050852.D
 Acq On : 20 Sep 2022 23:54
 Operator : JC/MD
 Sample : VU0920WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.115	3348	3351	3353	rBV2	640	366	0.02%	0.003%
78	12.192	3360	3375	3400	rBV	651068	1067063	53.21%	7.470%
79	12.372	3428	3431	3435	rBV4	372	304	0.02%	0.002%
80	12.494	3466	3469	3472	rBV3	391	284	0.01%	0.002%
81	12.825	3569	3572	3579	rVB2	761	674	0.03%	0.005%
82	12.864	3580	3584	3587	rBV3	443	359	0.02%	0.003%
83	12.996	3621	3625	3631	rVB4	766	893	0.04%	0.006%
84	13.224	3689	3696	3704	rBV8	2745	3706	0.18%	0.026%
85	13.356	3734	3737	3742	rVB4	486	447	0.02%	0.003%
86	13.497	3779	3781	3785	rVB3	537	268	0.01%	0.002%
87	13.561	3799	3801	3806	rVB3	464	424	0.02%	0.003%
88	13.770	3862	3866	3873	rBV3	726	827	0.04%	0.006%
89	13.844	3882	3889	3897	rBV7	3420	5138	0.26%	0.036%
90	14.092	3956	3966	3974	rBV2	5083	7887	0.39%	0.055%
91	14.198	3993	3999	4002	rBV3	720	795	0.04%	0.006%
92	14.301	4028	4031	4032	rBV2	610	370	0.02%	0.003%
93	14.336	4035	4042	4051	rVB6	4102	6354	0.32%	0.044%
94	14.397	4059	4061	4065	rBV2	484	362	0.02%	0.003%
95	14.571	4112	4115	4119	rBV2	458	334	0.02%	0.002%
96	14.709	4156	4158	4162	rBV3	667	480	0.02%	0.003%
97	14.835	4195	4197	4199	rBV	495	289	0.01%	0.002%
98	15.298	4337	4341	4345	rBV5	652	691	0.03%	0.005%
99	15.844	4504	4511	4514	rBV5	1714	2058	0.10%	0.014%
100	15.947	4538	4543	4547	rBV6	3279	3885	0.19%	0.027%




Sum of corrected areas: 14285182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050852.D
Acq On : 20 Sep 2022 23:54
Operator : JC/MD
Sample : VU0920WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

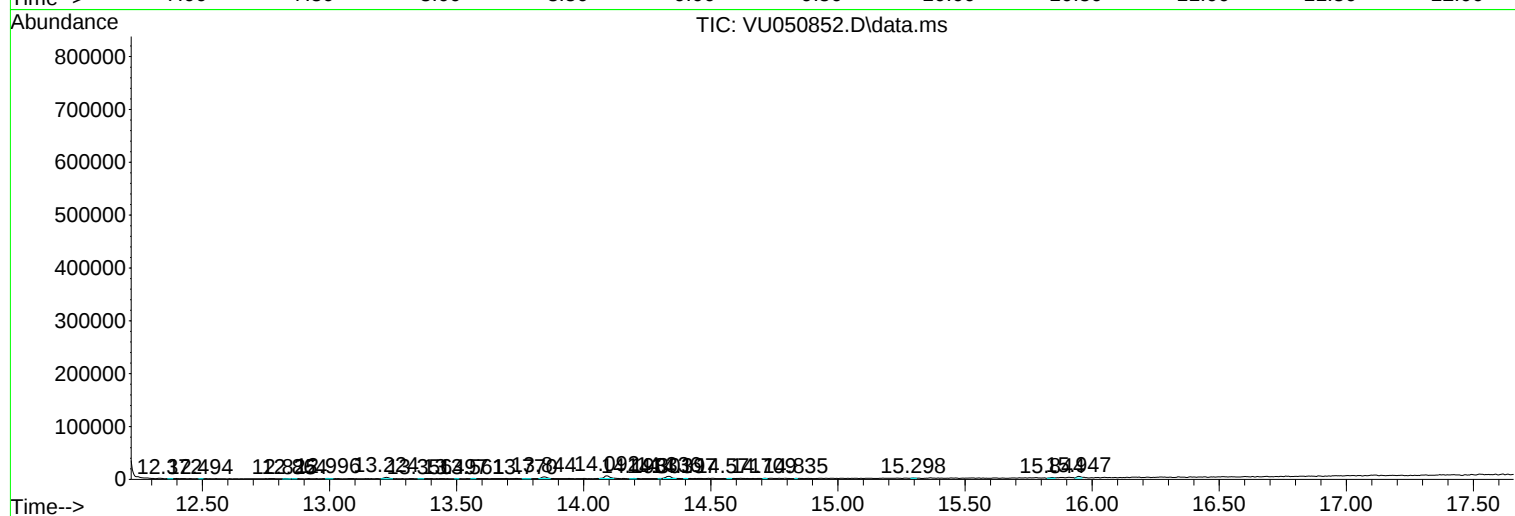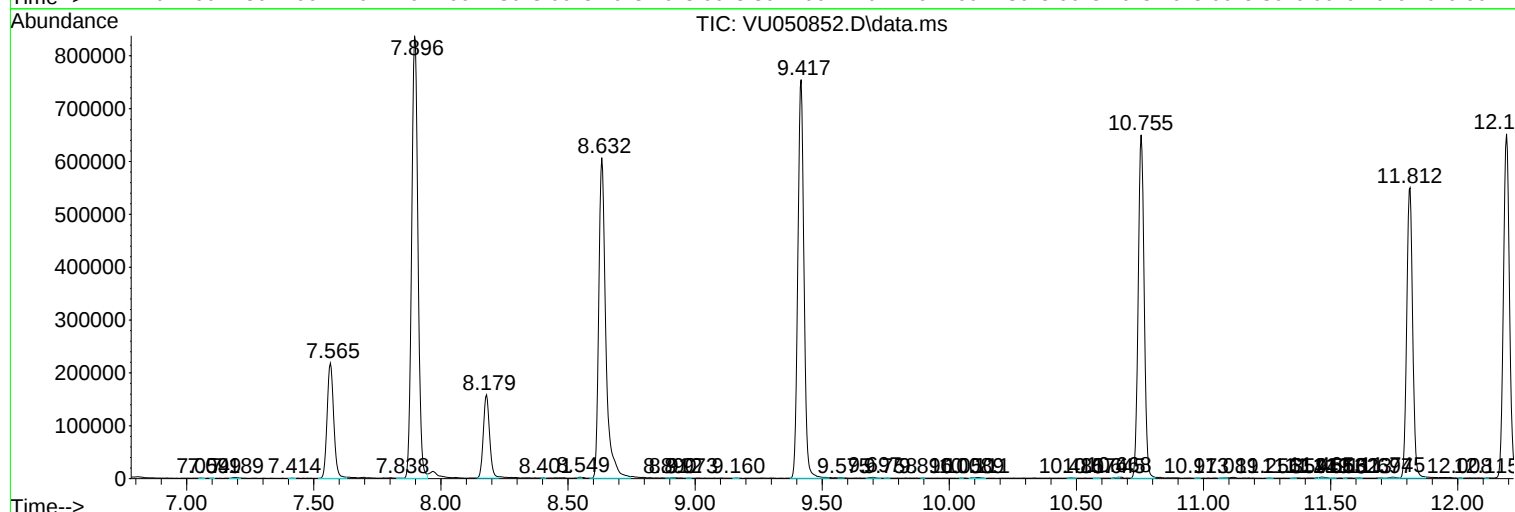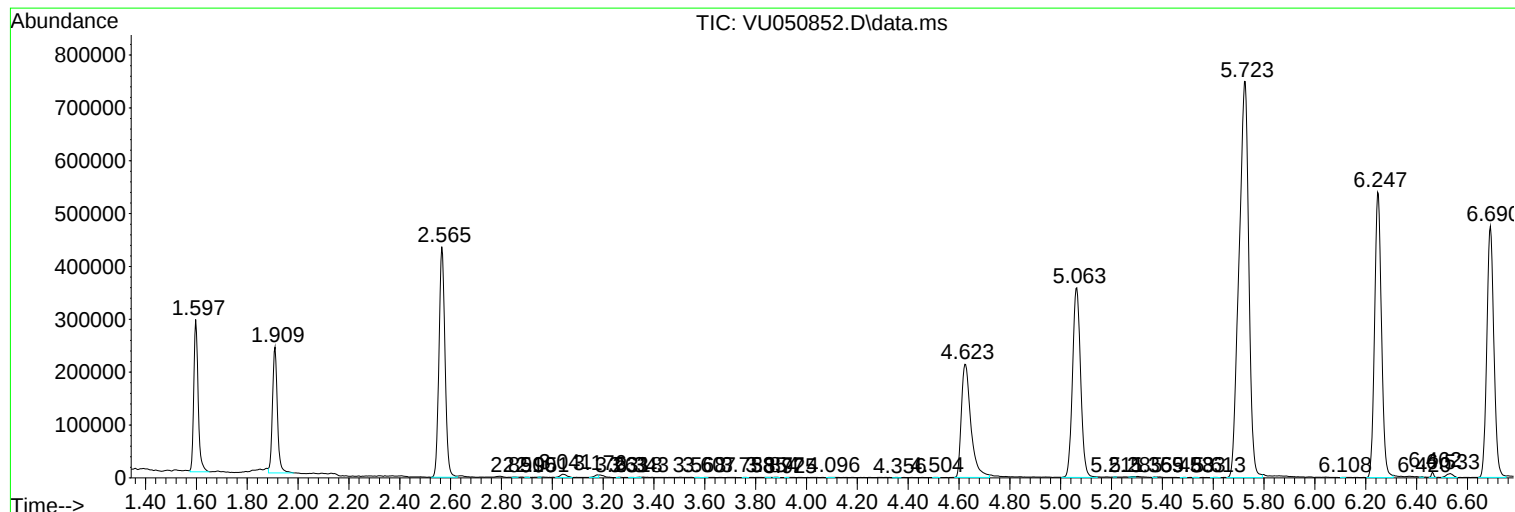

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050852.D
Acq On : 20 Sep 2022 23:54
Operator : JC/MD
Sample : VU0920WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050852.D
Acq On : 20 Sep 2022 23:54
Operator : JC/MD
Sample : VU0920WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc