

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050853.D
 Acq On : 21 Sep 2022 00:17
 Operator : JC/MD
 Sample : N4650-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	249025	289268	15.55%	1.972%
2	1.906	169	176	197	rVB	198156	270252	14.53%	1.842%
3	2.565	368	381	396	rBV2	398149	679572	36.53%	4.633%
4	2.787	436	450	464	rBV3	9055	27849	1.50%	0.190%
5	3.048	522	531	538	rVB5	1831	3072	0.17%	0.021%
6	3.176	563	571	574	rBV3	1933	2347	0.13%	0.016%
7	3.356	616	627	636	rVV6	4357	8513	0.46%	0.058%
8	3.867	771	786	808	rVB2	70083	163833	8.81%	1.117%
9	4.099	855	858	863	rBV2	424	357	0.02%	0.002%
10	4.250	899	905	908	rBV3	284	344	0.02%	0.002%
11	4.620	1008	1020	1055	rBV	201156	563982	30.31%	3.845%
12	5.064	1140	1158	1182	rVV	335857	742860	39.93%	5.064%
13	5.314	1217	1236	1256	rBV	425324	959326	51.56%	6.540%
14	5.533	1302	1304	1308	rVB2	838	593	0.03%	0.004%
15	5.555	1308	1311	1313	rBV2	485	352	0.02%	0.002%
16	5.726	1340	1364	1397	rBV2	682695	1860500	100.00%	12.683%
17	5.973	1439	1441	1448	rVB5	828	775	0.04%	0.005%
18	6.035	1457	1460	1462	rBV2	506	407	0.02%	0.003%
19	6.051	1462	1465	1467	rVB3	617	359	0.02%	0.002%
20	6.118	1481	1486	1488	rBV2	763	603	0.03%	0.004%
21	6.247	1512	1526	1554	rBV	522762	1010564	54.32%	6.889%
22	6.539	1604	1617	1632	rVB4	22346	46036	2.47%	0.314%
23	6.607	1636	1638	1643	rVB3	602	308	0.02%	0.002%
24	6.636	1643	1647	1649	rBV2	437	373	0.02%	0.003%
25	6.690	1649	1664	1683	rBV	445617	857240	46.08%	5.844%
26	6.912	1730	1733	1737	rBV3	400	323	0.02%	0.002%
27	6.938	1737	1741	1744	rBV2	875	747	0.04%	0.005%
28	6.983	1750	1755	1759	rBV4	491	636	0.03%	0.004%
29	7.060	1775	1779	1784	rVB2	603	616	0.03%	0.004%
30	7.086	1784	1787	1789	rBV	466	312	0.02%	0.002%
31	7.179	1810	1816	1818	rBV3	1332	1042	0.06%	0.007%
32	7.192	1818	1820	1826	rVB4	1029	910	0.05%	0.006%
33	7.269	1842	1844	1853	rVB3	468	628	0.03%	0.004%
34	7.356	1863	1871	1874	rBV2	462	576	0.03%	0.004%
35	7.565	1923	1936	1957	rBV	210609	371493	19.97%	2.532%
36	7.787	2002	2005	2012	rBV3	727	881	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050853.D
 Acq On : 21 Sep 2022 00:17
 Operator : JC/MD
 Sample : N4650-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.896	2023	2039	2055	rBV	762721	1302851	70.03%	8.881%
38	8.179	2115	2127	2142	rBV	147084	249894	13.43%	1.704%
39	8.401	2188	2196	2203	rVB6	1460	2117	0.11%	0.014%
40	8.469	2209	2217	2227	rBV6	1144	2296	0.12%	0.016%
41	8.552	2232	2243	2256	rVB2	43308	72863	3.92%	0.497%
42	8.633	2256	2268	2296	rBV2	568040	1081492	58.13%	7.372%
43	8.870	2338	2342	2344	rBV2	681	489	0.03%	0.003%
44	8.977	2373	2375	2379	rVB	581	345	0.02%	0.002%
45	9.015	2382	2387	2388	rBV2	428	371	0.02%	0.003%
46	9.189	2438	2441	2444	rBV2	394	286	0.02%	0.002%
47	9.288	2468	2472	2474	rBV	383	284	0.02%	0.002%
48	9.343	2487	2489	2494	rVB	492	330	0.02%	0.002%
49	9.417	2498	2512	2536	rBV	732057	1219953	65.57%	8.316%
50	9.594	2565	2567	2573	rVB3	754	593	0.03%	0.004%
51	9.700	2588	2600	2606	rBV7	1200	1983	0.11%	0.014%
52	9.858	2646	2649	2653	rVB4	603	489	0.03%	0.003%
53	9.883	2653	2657	2662	rBV3	307	294	0.02%	0.002%
54	10.105	2718	2726	2727	rBV3	768	720	0.04%	0.005%
55	10.205	2753	2757	2759	rBV	392	331	0.02%	0.002%
56	10.333	2791	2797	2803	rBV3	368	465	0.02%	0.003%
57	10.565	2864	2869	2874	rVB3	589	585	0.03%	0.004%
58	10.591	2874	2877	2881	rBV3	397	439	0.02%	0.003%
59	10.665	2891	2900	2901	rBV5	1070	1292	0.07%	0.009%
60	10.755	2914	2928	2952	rBV	613118	988990	53.16%	6.742%
61	10.848	2952	2957	2962	rVV4	706	908	0.05%	0.006%
62	10.951	2986	2989	2994	rVB2	406	281	0.02%	0.002%
63	10.980	2994	2998	3001	rBV2	405	341	0.02%	0.002%
64	11.089	3027	3032	3035	rVV6	1085	1102	0.06%	0.008%
65	11.118	3037	3041	3046	rVB3	1260	1373	0.07%	0.009%
66	11.173	3052	3058	3064	rBV3	517	731	0.04%	0.005%
67	11.231	3071	3076	3079	rBV	406	342	0.02%	0.002%
68	11.304	3096	3099	3105	rVB	380	321	0.02%	0.002%
69	11.353	3109	3114	3118	rVB2	622	488	0.03%	0.003%
70	11.404	3126	3130	3132	rBV2	432	278	0.01%	0.002%
71	11.414	3132	3133	3138	rVB2	665	301	0.02%	0.002%
72	11.439	3138	3141	3143	rBV	413	310	0.02%	0.002%
73	11.459	3143	3147	3149	rBV2	1334	1013	0.05%	0.007%
74	11.742	3231	3235	3236	rBV2	1230	564	0.03%	0.004%
75	11.809	3244	3256	3277	rBV	542821	868240	46.67%	5.919%
76	12.076	3333	3339	3343	rBV6	842	991	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050853.D
 Acq On : 21 Sep 2022 00:17
 Operator : JC/MD
 Sample : N4650-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3394	rBV	607113	978871	52.61%	6.673%
78	12.459	3454	3458	3461	rVB2	344	285	0.02%	0.002%
79	12.478	3461	3464	3468	rBV3	567	463	0.02%	0.003%
80	12.552	3483	3487	3491	rBV2	507	426	0.02%	0.003%
81	12.706	3529	3535	3538	rBV2	486	567	0.03%	0.004%
82	12.761	3549	3552	3555	rBV2	572	484	0.03%	0.003%
83	12.816	3566	3569	3573	rBV2	324	342	0.02%	0.002%
84	12.906	3595	3597	3602	rVB3	536	422	0.02%	0.003%
85	12.931	3602	3605	3608	rBV	489	401	0.02%	0.003%
86	13.044	3631	3640	3642	rBV4	487	605	0.03%	0.004%
87	13.131	3664	3667	3671	rVB3	407	311	0.02%	0.002%
88	13.153	3671	3674	3677	rBV3	476	356	0.02%	0.002%
89	13.189	3681	3685	3690	rBV3	320	310	0.02%	0.002%
90	13.218	3690	3694	3697	rBV4	1018	914	0.05%	0.006%
91	13.353	3731	3736	3740	rBV4	658	596	0.03%	0.004%
92	13.722	3848	3851	3853	rBV2	437	290	0.02%	0.002%
93	13.800	3867	3875	3879	rBV2	831	1260	0.07%	0.009%
94	13.845	3885	3889	3898	rVB4	1824	2491	0.13%	0.017%
95	14.102	3960	3969	3976	rVB6	1926	2759	0.15%	0.019%
96	14.198	3996	3999	4002	rVB	596	379	0.02%	0.003%
97	14.430	4068	4071	4077	rBV3	389	446	0.02%	0.003%
98	14.838	4195	4198	4199	rBV	614	332	0.02%	0.002%
99	14.973	4237	4240	4241	rBV2	679	372	0.02%	0.003%
100	15.471	4393	4395	4399	rBV3	654	460	0.02%	0.003%




Sum of corrected areas: 14669327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050853.D
Acq On : 21 Sep 2022 00:17
Operator : JC/MD
Sample : N4650-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

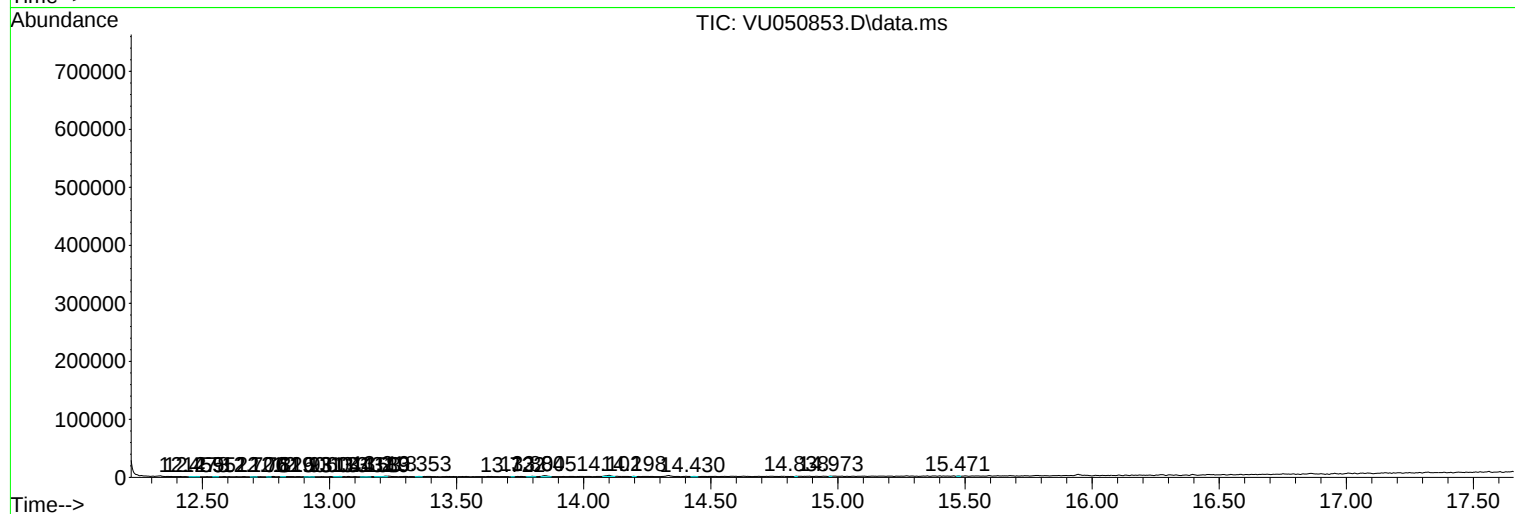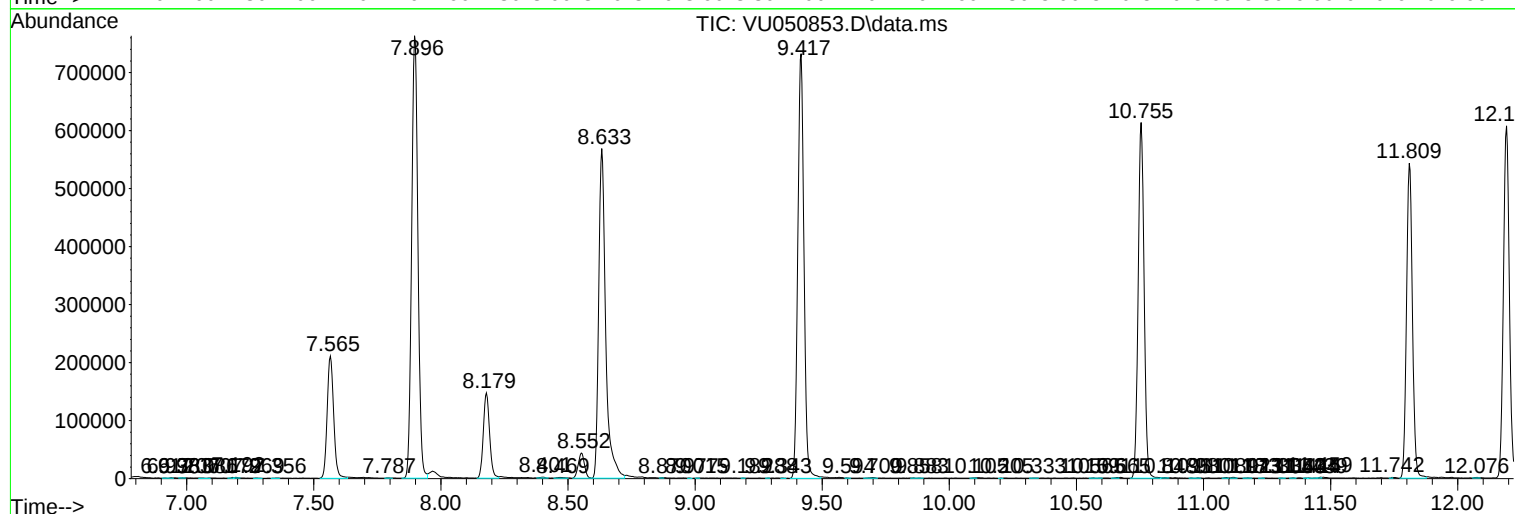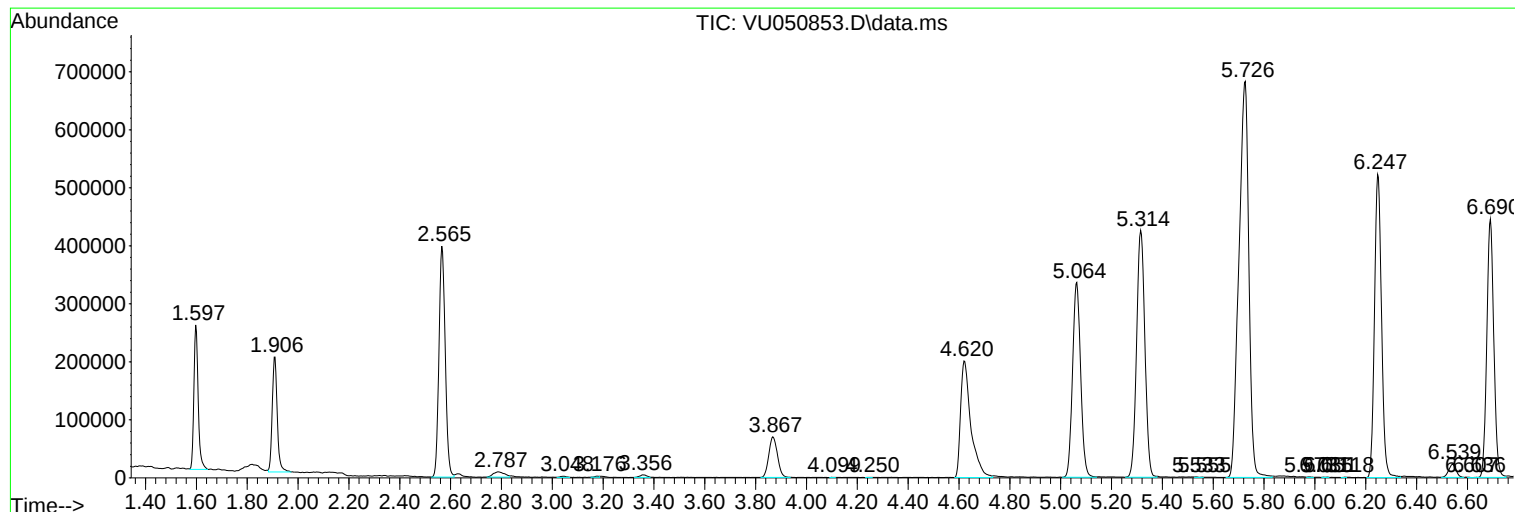

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050853.D
Acq On : 21 Sep 2022 00:17
Operator : JC/MD
Sample : N4650-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050853.D
Acq On : 21 Sep 2022 00:17
Operator : JC/MD
Sample : N4650-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc