

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050854.D
 Acq On : 21 Sep 2022 00:41
 Operator : JC/MD
 Sample : N4650-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	96	rVB2	324452	399177	20.21%	2.385%
2	1.909	169	177	200	rVB2	203650	354584	17.95%	2.118%
3	2.565	368	381	396	rBV2	401086	666375	33.74%	3.981%
4	2.771	433	445	446	rBV	15702	21982	1.11%	0.131%
5	2.951	496	501	504	rBV3	844	865	0.04%	0.005%
6	2.999	512	516	517	rBV3	390	296	0.01%	0.002%
7	3.038	523	528	538	rVB7	1774	2784	0.14%	0.017%
8	3.099	544	547	550	rBV2	396	299	0.02%	0.002%
9	3.189	562	575	588	rBV3	3111	7823	0.40%	0.047%
10	3.356	614	627	639	rBV6	7590	15398	0.78%	0.092%
11	3.478	657	665	667	rBV3	314	316	0.02%	0.002%
12	3.616	704	708	715	rVB2	731	839	0.04%	0.005%
13	3.652	715	719	725	rBV	675	516	0.03%	0.003%
14	3.867	761	786	815	rBV	288337	689680	34.92%	4.120%
15	4.343	931	934	936	rBV2	437	323	0.02%	0.002%
16	4.359	936	939	943	rVB2	300	301	0.02%	0.002%
17	4.411	949	955	959	rBV2	335	437	0.02%	0.003%
18	4.620	1005	1020	1026	rBV	211978	445750	22.57%	2.663%
19	5.060	1135	1157	1184	rBV	337452	744555	37.70%	4.448%
20	5.314	1218	1236	1258	rBV	880594	1974891	100.00%	11.798%
21	5.722	1341	1363	1398	rBV2	693184	1888507	95.63%	11.282%
22	5.973	1438	1441	1442	rBV2	540	291	0.01%	0.002%
23	6.134	1487	1491	1496	rVB4	655	675	0.03%	0.004%
24	6.185	1505	1507	1510	rBV2	440	352	0.02%	0.002%
25	6.247	1512	1526	1546	rBV	509925	972160	49.23%	5.808%
26	6.443	1583	1587	1590	rVB4	752	598	0.03%	0.004%
27	6.542	1604	1618	1633	rBV2	59613	117506	5.95%	0.702%
28	6.690	1647	1664	1683	rBV	441619	860193	43.56%	5.139%
29	6.983	1752	1755	1761	rBV4	712	703	0.04%	0.004%
30	7.124	1796	1799	1803	rBV2	429	296	0.01%	0.002%
31	7.150	1803	1807	1810	rVB2	423	332	0.02%	0.002%
32	7.189	1810	1819	1828	rBV5	1846	3260	0.17%	0.019%
33	7.304	1852	1855	1861	rBV2	456	502	0.03%	0.003%
34	7.385	1877	1880	1886	rBV2	619	433	0.02%	0.003%
35	7.504	1913	1917	1922	rBV2	362	408	0.02%	0.002%
36	7.565	1924	1936	1953	rBV	210894	369277	18.70%	2.206%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050854.D
 Acq On : 21 Sep 2022 00:41
 Operator : JC/MD
 Sample : N4650-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.896	2023	2039	2055	rBV	778088	1325151	67.10%	7.916%
38	8.179	2113	2127	2143	rBV	150130	254961	12.91%	1.523%
39	8.398	2192	2195	2198	rBV2	633	408	0.02%	0.002%
40	8.552	2231	2243	2256	rBV2	196897	332981	16.86%	1.989%
41	8.632	2256	2268	2303	rVV2	584017	1107142	56.06%	6.614%
42	8.867	2333	2341	2345	rBV5	1358	1928	0.10%	0.012%
43	8.915	2353	2356	2359	rBV5	1126	768	0.04%	0.005%
44	9.005	2381	2384	2389	rVB2	420	306	0.02%	0.002%
45	9.031	2389	2392	2397	rVB2	464	413	0.02%	0.002%
46	9.417	2499	2512	2541	rBV	709038	1184254	59.97%	7.075%
47	9.558	2553	2556	2557	rBV2	783	395	0.02%	0.002%
48	9.648	2579	2584	2589	rVB5	443	501	0.03%	0.003%
49	9.687	2589	2596	2599	rBV6	1867	2067	0.10%	0.012%
50	9.838	2639	2643	2646	rBV2	423	290	0.01%	0.002%
51	9.886	2655	2658	2662	rBV3	356	308	0.02%	0.002%
52	9.973	2680	2685	2687	rBV2	415	416	0.02%	0.002%
53	10.031	2699	2703	2707	rBV5	515	557	0.03%	0.003%
54	10.105	2719	2726	2731	rBV5	1059	1595	0.08%	0.010%
55	10.272	2772	2778	2786	rVB5	1726	2219	0.11%	0.013%
56	10.369	2806	2808	2810	rBV	560	290	0.01%	0.002%
57	10.430	2823	2827	2831	rBV2	565	541	0.03%	0.003%
58	10.475	2836	2841	2842	rBV2	1198	765	0.04%	0.005%
59	10.561	2865	2868	2873	rBV3	422	389	0.02%	0.002%
60	10.642	2891	2893	2894	rBV2	589	292	0.01%	0.002%
61	10.754	2915	2928	2951	rBV	621778	1002301	50.75%	5.988%
62	10.902	2961	2974	2983	rVB7	2895	5920	0.30%	0.035%
63	11.082	3024	3030	3031	rBV3	1986	1444	0.07%	0.009%
64	11.295	3086	3096	3106	rVB3	7529	12003	0.61%	0.072%
65	11.375	3116	3121	3124	rBV2	860	644	0.03%	0.004%
66	11.414	3129	3133	3140	rBV4	819	1172	0.06%	0.007%
67	11.468	3140	3150	3164	rVB4	6382	10679	0.54%	0.064%
68	11.600	3188	3191	3193	rBV3	655	419	0.02%	0.003%
69	11.642	3197	3204	3210	rVV2	3114	3344	0.17%	0.020%
70	11.696	3216	3221	3224	rBV3	663	678	0.03%	0.004%
71	11.745	3233	3236	3242	rVB5	2078	1745	0.09%	0.010%
72	11.809	3242	3256	3278	rBV	536679	858638	43.48%	5.129%
73	11.886	3278	3280	3282	rBV2	1161	747	0.04%	0.004%
74	11.970	3304	3306	3310	rVB5	952	589	0.03%	0.004%
75	12.063	3327	3335	3336	rBV4	3630	3499	0.18%	0.021%
76	12.092	3339	3344	3352	rVB3	6566	9477	0.48%	0.057%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050854.D
 Acq On : 21 Sep 2022 00:41
 Operator : JC/MD
 Sample : N4650-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3406	rVB	640075	1035391	52.43%	6.185%
78	12.304	3406	3410	3412	rBV4	606	513	0.03%	0.003%
79	12.336	3418	3420	3425	rVB4	1020	557	0.03%	0.003%
80	12.372	3428	3431	3436	rVB6	1281	1018	0.05%	0.006%
81	12.465	3455	3460	3462	rBV4	1243	1194	0.06%	0.007%
82	12.526	3476	3479	3480	rBV2	490	344	0.02%	0.002%
83	12.571	3488	3493	3495	rBV4	1038	1016	0.05%	0.006%
84	12.690	3521	3530	3533	rBV6	3814	5379	0.27%	0.032%
85	12.976	3616	3619	3626	rVB2	765	724	0.04%	0.004%
86	13.076	3644	3650	3655	rBV4	469	754	0.04%	0.005%
87	13.221	3693	3695	3701	rVB3	1136	745	0.04%	0.004%
88	13.365	3737	3740	3742	rBV2	522	347	0.02%	0.002%
89	13.455	3761	3768	3773	rVV5	1955	2301	0.12%	0.014%
90	13.571	3802	3804	3808	rBV	547	447	0.02%	0.003%
91	13.619	3814	3819	3824	rBV6	1273	1495	0.08%	0.009%
92	13.719	3848	3850	3854	rVB2	591	341	0.02%	0.002%
93	13.738	3854	3856	3860	rBV	420	296	0.01%	0.002%
94	13.838	3882	3887	3889	rBV4	1244	1176	0.06%	0.007%
95	14.053	3950	3954	3955	rBV	483	360	0.02%	0.002%
96	14.092	3959	3966	3978	rVV4	4870	7798	0.39%	0.047%
97	14.516	4096	4098	4100	rBV2	585	300	0.02%	0.002%
98	14.770	4175	4177	4180	rBV2	515	328	0.02%	0.002%
99	15.028	4255	4257	4259	rBV2	681	413	0.02%	0.002%
100	16.072	4578	4582	4586	rBV4	1332	1443	0.07%	0.009%




Sum of corrected areas: 16739600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050854.D
Acq On : 21 Sep 2022 00:41
Operator : JC/MD
Sample : N4650-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

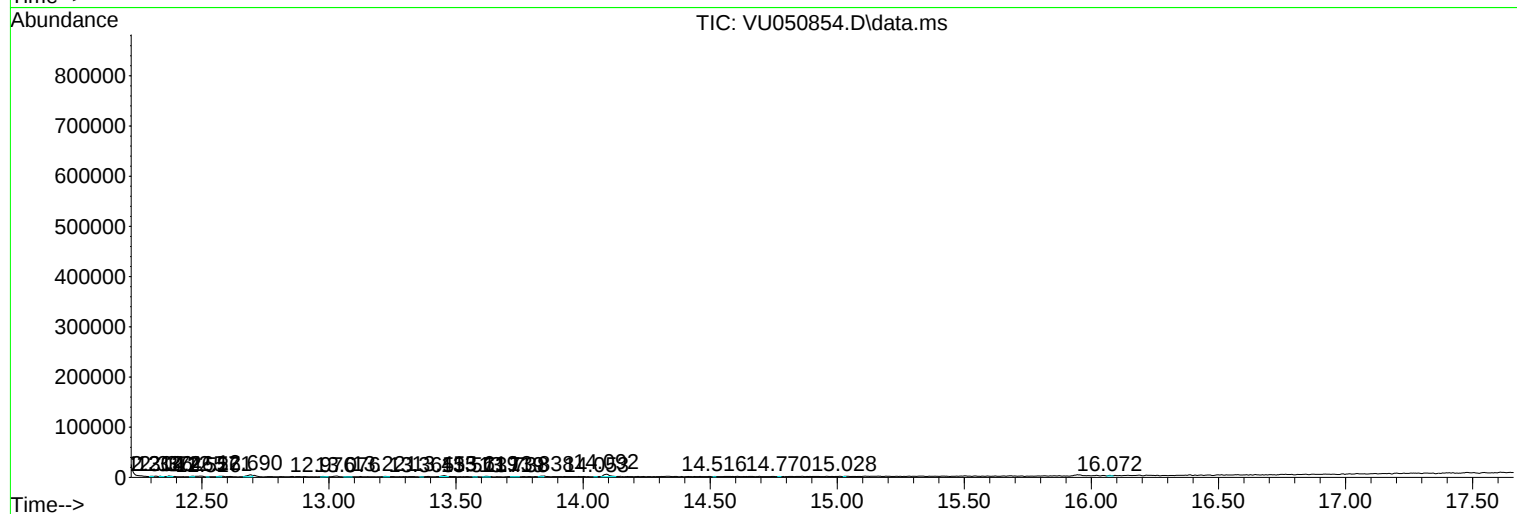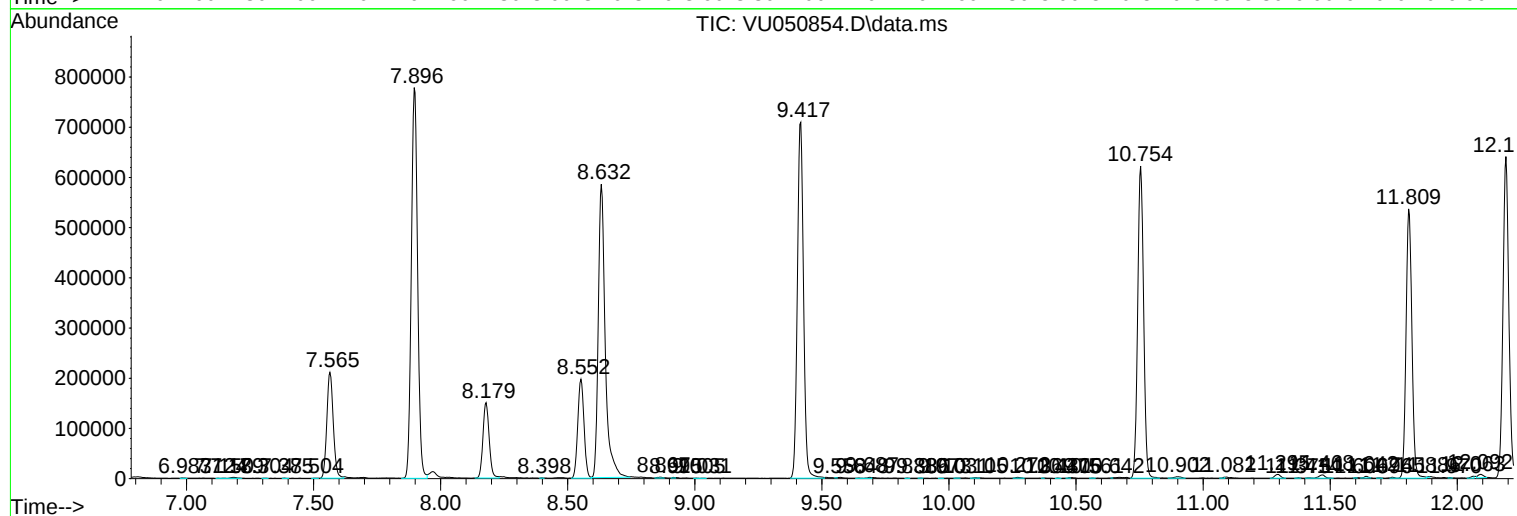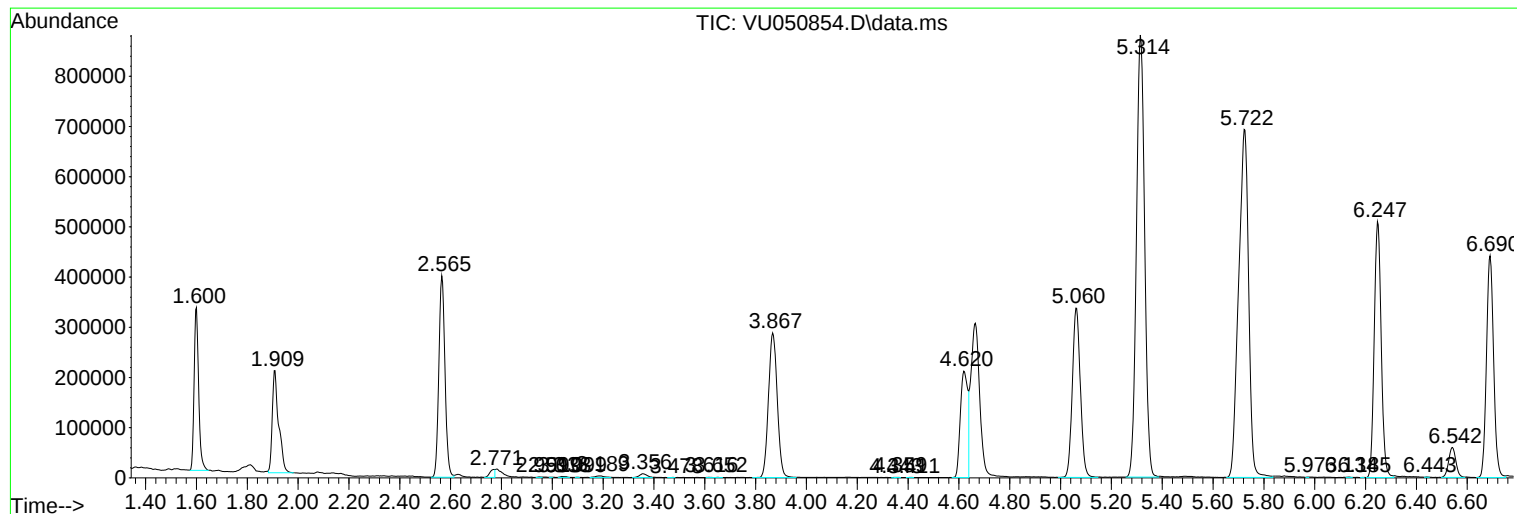

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050854.D
Acq On : 21 Sep 2022 00:41
Operator : JC/MD
Sample : N4650-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050854.D
Acq On : 21 Sep 2022 00:41
Operator : JC/MD
Sample : N4650-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------