

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050856.D
 Acq On : 21 Sep 2022 01:28
 Operator : JC/MD
 Sample : N4650-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	260642	296962	15.56%	1.910%
2	1.906	168	176	194	rVB	201675	266139	13.95%	1.712%
3	2.565	368	381	396	rBV2	410926	689667	36.14%	4.435%
4	2.761	431	442	459	rVV2	11892	27444	1.44%	0.176%
5	2.996	513	515	521	rBV2	342	308	0.02%	0.002%
6	3.044	523	530	537	rVB6	2131	3394	0.18%	0.022%
7	3.179	560	572	575	rBV4	3655	5552	0.29%	0.036%
8	3.263	593	598	599	rBV	415	326	0.02%	0.002%
9	3.353	617	626	637	rBV6	3318	6106	0.32%	0.039%
10	3.440	648	653	656	rBV2	374	304	0.02%	0.002%
11	3.459	656	659	666	rVB2	343	326	0.02%	0.002%
12	3.626	707	711	715	rBV3	330	305	0.02%	0.002%
13	3.867	769	786	812	rVB	59222	139232	7.30%	0.895%
14	4.456	966	969	976	rVB2	464	407	0.02%	0.003%
15	4.501	980	983	990	rVB3	377	331	0.02%	0.002%
16	4.616	1006	1019	1054	rBV	221141	587885	30.81%	3.781%
17	5.060	1140	1157	1183	rBV	345491	760659	39.86%	4.892%
18	5.314	1218	1236	1257	rBV	594287	1339336	70.19%	8.613%
19	5.504	1293	1295	1301	rBV4	589	613	0.03%	0.004%
20	5.584	1317	1320	1324	rBV4	501	419	0.02%	0.003%
21	5.620	1328	1331	1333	rBV3	535	326	0.02%	0.002%
22	5.722	1341	1363	1387	rBV2	713652	1908200	100.00%	12.272%
23	5.967	1437	1439	1440	rBV	715	343	0.02%	0.002%
24	6.070	1469	1471	1475	rBV2	378	365	0.02%	0.002%
25	6.102	1480	1481	1485	rVV2	678	441	0.02%	0.003%
26	6.150	1492	1496	1499	rBV2	402	314	0.02%	0.002%
27	6.247	1511	1526	1546	rBV	528272	987235	51.74%	6.349%
28	6.391	1568	1571	1574	rVB3	884	538	0.03%	0.003%
29	6.478	1594	1598	1601	rBV	419	363	0.02%	0.002%
30	6.539	1604	1617	1632	rVB6	30011	59888	3.14%	0.385%
31	6.690	1649	1664	1688	rBV	451286	886994	46.48%	5.704%
32	7.044	1769	1774	1776	rBV2	354	371	0.02%	0.002%
33	7.150	1802	1807	1809	rBV2	510	404	0.02%	0.003%
34	7.185	1813	1818	1826	rVB5	1019	1477	0.08%	0.009%
35	7.330	1859	1863	1867	rVV2	374	308	0.02%	0.002%
36	7.407	1879	1887	1890	rBV2	454	533	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050856.D
 Acq On : 21 Sep 2022 01:28
 Operator : JC/MD
 Sample : N4650-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.565	1922	1936	1955	rBV	216883	380430	19.94%	2.447%
38	7.896	2022	2039	2056	rBV	792989	1364644	71.51%	8.776%
39	8.095	2097	2101	2104	rVB2	505	388	0.02%	0.002%
40	8.176	2113	2126	2141	rBV	156114	274419	14.38%	1.765%
41	8.295	2161	2163	2170	rVB4	671	525	0.03%	0.003%
42	8.346	2175	2179	2181	rBV4	512	419	0.02%	0.003%
43	8.401	2189	2196	2202	rBV5	1590	1943	0.10%	0.012%
44	8.465	2210	2216	2228	rVB7	1462	2572	0.13%	0.017%
45	8.552	2231	2243	2255	rBV	99292	167124	8.76%	1.075%
46	8.632	2255	2268	2304	rBV2	608390	1160133	60.80%	7.461%
47	8.931	2356	2361	2365	rBV4	511	390	0.02%	0.003%
48	9.031	2388	2392	2397	rVB4	664	627	0.03%	0.004%
49	9.256	2459	2462	2466	rBV2	455	327	0.02%	0.002%
50	9.417	2495	2512	2538	rBV	717696	1196057	62.68%	7.692%
51	9.603	2567	2570	2576	rBV3	519	490	0.03%	0.003%
52	9.635	2576	2580	2584	rVB	507	319	0.02%	0.002%
53	9.661	2584	2588	2590	rBV	633	416	0.02%	0.003%
54	9.690	2593	2597	2598	rBV	567	327	0.02%	0.002%
55	9.899	2658	2662	2664	rBV2	361	357	0.02%	0.002%
56	10.095	2718	2723	2725	rBV	697	661	0.03%	0.004%
57	10.108	2725	2727	2734	rVB5	675	628	0.03%	0.004%
58	10.497	2842	2848	2850	rBV3	360	371	0.02%	0.002%
59	10.552	2862	2865	2871	rVB3	432	428	0.02%	0.003%
60	10.623	2883	2887	2891	rBV2	292	316	0.02%	0.002%
61	10.668	2893	2901	2906	rVB4	1541	1932	0.10%	0.012%
62	10.693	2906	2909	2913	rVB	471	315	0.02%	0.002%
63	10.754	2914	2928	2946	rBV	655734	1041035	54.56%	6.695%
64	10.893	2966	2971	2977	rBV6	1236	1464	0.08%	0.009%
65	10.996	3001	3003	3009	rBV4	307	325	0.02%	0.002%
66	11.082	3026	3030	3035	rBV4	809	946	0.05%	0.006%
67	11.205	3066	3068	3073	rVB2	558	442	0.02%	0.003%
68	11.282	3089	3092	3094	rBV	781	530	0.03%	0.003%
69	11.410	3129	3132	3140	rBV6	898	1152	0.06%	0.007%
70	11.471	3140	3151	3162	rVV6	4808	8279	0.43%	0.053%
71	11.632	3196	3201	3204	rVB2	369	369	0.02%	0.002%
72	11.664	3205	3211	3214	rVB3	342	351	0.02%	0.002%
73	11.693	3214	3220	3226	rBV4	1077	1088	0.06%	0.007%
74	11.745	3232	3236	3240	rVB3	506	451	0.02%	0.003%
75	11.809	3243	3256	3277	rBV	554085	878342	46.03%	5.649%
76	11.976	3306	3308	3312	rVB4	1251	756	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050856.D
 Acq On : 21 Sep 2022 01:28
 Operator : JC/MD
 Sample : N4650-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.024	3320	3323	3327	rBV2	496	415	0.02%	0.003%
78	12.066	3327	3336	3343	rBV7	2763	4735	0.25%	0.030%
79	12.192	3362	3375	3401	rBV	653064	1057712	55.43%	6.802%
80	12.330	3414	3418	3425	rBV5	818	890	0.05%	0.006%
81	12.459	3456	3458	3463	rVB3	518	421	0.02%	0.003%
82	12.523	3474	3478	3481	rBV3	385	324	0.02%	0.002%
83	12.571	3489	3493	3497	rVB4	801	531	0.03%	0.003%
84	12.719	3537	3539	3542	rBV2	423	306	0.02%	0.002%
85	12.947	3608	3610	3615	rVB2	550	388	0.02%	0.002%
86	12.979	3615	3620	3622	rBV4	665	632	0.03%	0.004%
87	13.034	3633	3637	3642	rVB3	924	853	0.04%	0.005%
88	13.188	3682	3685	3690	rVB4	614	618	0.03%	0.004%
89	13.214	3690	3693	3694	rBV4	806	370	0.02%	0.002%
90	13.291	3713	3717	3720	rBV2	611	420	0.02%	0.003%
91	13.394	3744	3749	3752	rBV2	759	760	0.04%	0.005%
92	13.458	3764	3769	3773	rVB6	1063	1072	0.06%	0.007%
93	13.844	3887	3889	3893	rVB3	781	501	0.03%	0.003%
94	14.095	3957	3967	3978	rBV2	4280	7537	0.39%	0.048%
95	14.568	4110	4114	4120	rBV4	850	921	0.05%	0.006%
96	14.706	4154	4157	4160	rVB4	741	472	0.02%	0.003%
97	15.233	4315	4321	4326	rBV4	1217	1939	0.10%	0.012%
98	15.349	4355	4357	4366	rVB5	820	732	0.04%	0.005%
99	15.838	4507	4509	4512	rVB2	1155	500	0.03%	0.003%
100	15.857	4512	4515	4516	rBV	946	573	0.03%	0.004%




Sum of corrected areas: 15549525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050856.D
Acq On : 21 Sep 2022 01:28
Operator : JC/MD
Sample : N4650-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

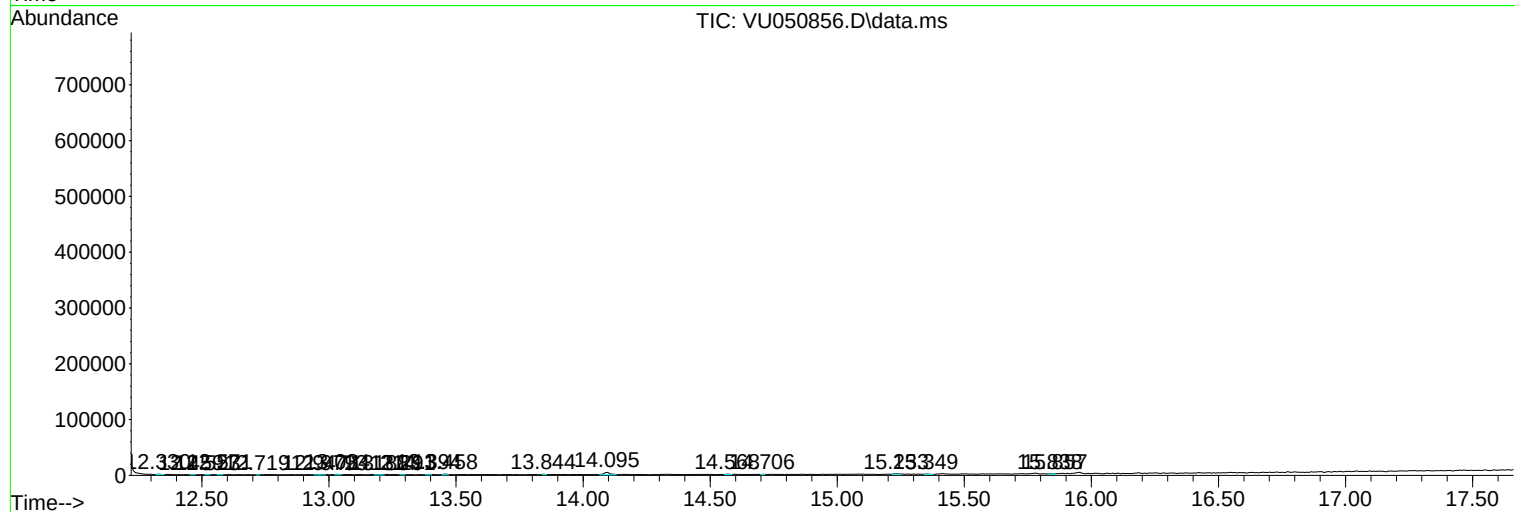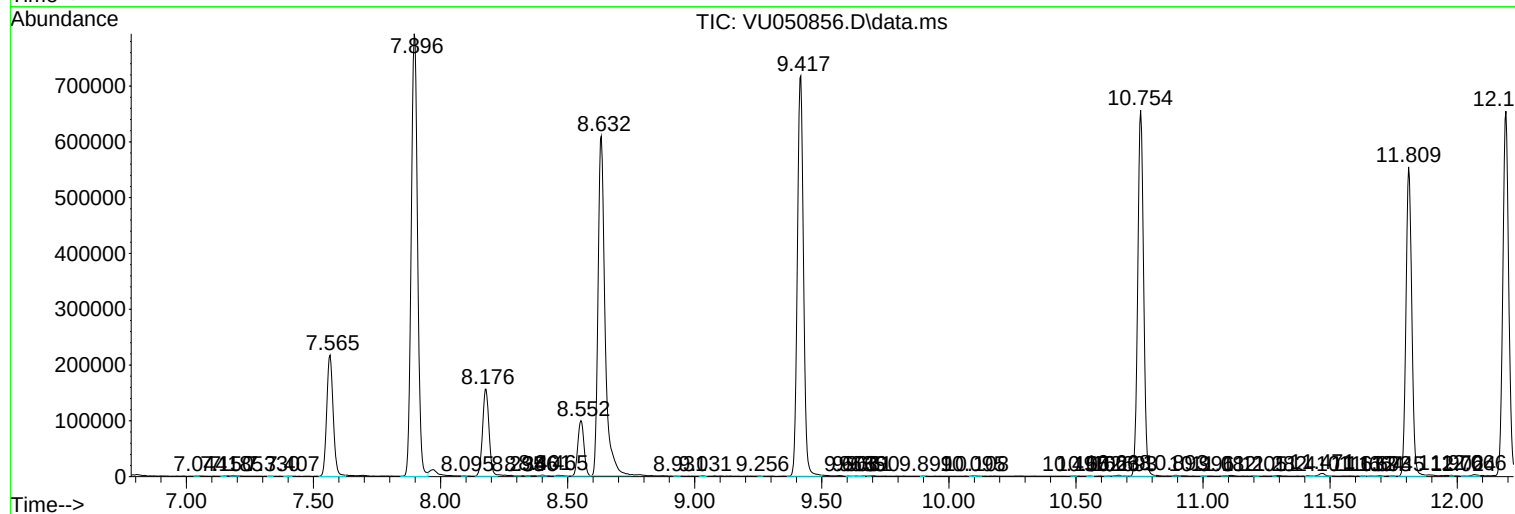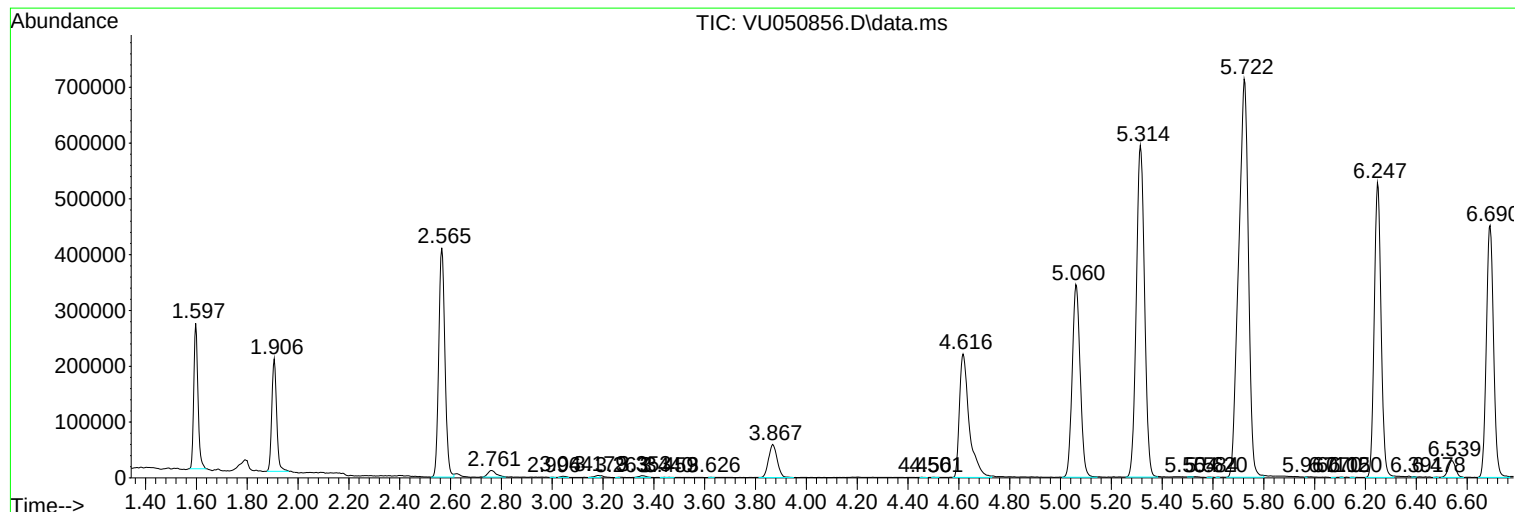

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050856.D
Acq On : 21 Sep 2022 01:28
Operator : JC/MD
Sample : N4650-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050856.D
Acq On : 21 Sep 2022 01:28
Operator : JC/MD
Sample : N4650-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------