

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050857.D
 Acq On : 21 Sep 2022 01:51
 Operator : JC/MD
 Sample : N4650-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	221643	259963	12.83%	1.619%
2	1.909	169	177	189	rVB	179223	236082	11.66%	1.470%
3	2.565	369	381	398	rBV2	358273	632085	31.21%	3.937%
4	2.794	444	452	453	rBV5	1745	1981	0.10%	0.012%
5	2.938	495	497	502	rBV	584	572	0.03%	0.004%
6	3.048	523	531	537	rVB6	1628	2652	0.13%	0.017%
7	3.173	561	570	571	rBV2	1500	1623	0.08%	0.010%
8	3.250	588	594	596	rBV2	563	493	0.02%	0.003%
9	3.289	603	606	617	rBV3	397	517	0.03%	0.003%
10	3.347	617	624	630	rBV6	1195	1683	0.08%	0.010%
11	3.392	635	638	641	rVB	437	284	0.01%	0.002%
12	3.462	654	660	663	rBV2	314	406	0.02%	0.003%
13	3.642	711	716	726	rBV3	996	1599	0.08%	0.010%
14	3.787	758	761	765	rVB3	502	337	0.02%	0.002%
15	3.871	771	787	804	rVV	43704	103376	5.10%	0.644%
16	3.935	804	807	812	rVB2	510	420	0.02%	0.003%
17	3.990	819	824	829	rVB2	443	512	0.03%	0.003%
18	4.247	899	904	906	rVV3	328	287	0.01%	0.002%
19	4.363	936	940	945	rVB2	279	303	0.01%	0.002%
20	4.623	1005	1021	1062	rBV	201776	602261	29.73%	3.751%
21	4.938	1115	1119	1121	rVB2	572	362	0.02%	0.002%
22	5.060	1139	1157	1183	rBV	298335	654972	32.34%	4.079%
23	5.150	1183	1185	1190	rVB4	600	357	0.02%	0.002%
24	5.211	1201	1204	1207	rBV3	586	523	0.03%	0.003%
25	5.314	1218	1236	1262	rBV	901193	2025460	100.00%	12.615%
26	5.636	1334	1336	1341	rVB4	521	470	0.02%	0.003%
27	5.723	1341	1363	1392	rBV2	610504	1641095	81.02%	10.221%
28	5.977	1438	1442	1445	rBV4	761	486	0.02%	0.003%
29	6.025	1453	1457	1460	rBV2	415	395	0.02%	0.002%
30	6.170	1497	1502	1508	rBV2	406	365	0.02%	0.002%
31	6.247	1512	1526	1547	rBV	469585	877054	43.30%	5.462%
32	6.433	1582	1584	1588	rVB3	432	273	0.01%	0.002%
33	6.462	1591	1593	1597	rVB3	620	374	0.02%	0.002%
34	6.491	1597	1602	1604	rBV2	474	435	0.02%	0.003%
35	6.543	1604	1618	1644	rBV	222597	428463	21.15%	2.668%
36	6.633	1644	1646	1648	rBV2	624	346	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050857.D
 Acq On : 21 Sep 2022 01:51
 Operator : JC/MD
 Sample : N4650-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1689	rVV	388047	755797	37.31%	4.707%
38	7.060	1775	1779	1784	rVB3	380	394	0.02%	0.002%
39	7.189	1811	1819	1827	rBV4	1507	2693	0.13%	0.017%
40	7.565	1920	1936	1952	rBV	180252	323225	15.96%	2.013%
41	7.694	1969	1976	1983	rBV7	1169	1826	0.09%	0.011%
42	7.790	2003	2006	2014	rVB3	499	624	0.03%	0.004%
43	7.896	2023	2039	2055	rBV	677665	1162529	57.40%	7.240%
44	8.179	2115	2127	2150	rBV	128023	222977	11.01%	1.389%
45	8.401	2189	2196	2204	rVB7	2551	4184	0.21%	0.026%
46	8.446	2204	2210	2212	rBV3	713	726	0.04%	0.005%
47	8.552	2227	2243	2256	rBV	801010	1354713	66.88%	8.437%
48	8.633	2257	2268	2305	rVB2	554536	1074571	53.05%	6.692%
49	8.870	2339	2342	2346	rVB3	559	409	0.02%	0.003%
50	8.960	2362	2370	2375	rBV5	734	1011	0.05%	0.006%
51	9.031	2389	2392	2395	rBV3	576	443	0.02%	0.003%
52	9.060	2400	2401	2405	rVB2	531	279	0.01%	0.002%
53	9.153	2424	2430	2433	rBV3	413	437	0.02%	0.003%
54	9.214	2445	2449	2452	rBV2	366	368	0.02%	0.002%
55	9.298	2472	2475	2479	rVB	545	332	0.02%	0.002%
56	9.324	2479	2483	2485	rBV	361	289	0.01%	0.002%
57	9.417	2499	2512	2536	rBV	647635	1064161	52.54%	6.628%
58	9.652	2582	2585	2589	rBV3	537	468	0.02%	0.003%
59	9.694	2593	2598	2606	rVB4	855	961	0.05%	0.006%
60	9.825	2635	2639	2645	rVB3	544	610	0.03%	0.004%
61	9.854	2645	2648	2651	rBV2	344	281	0.01%	0.002%
62	9.903	2660	2663	2667	rVB	496	364	0.02%	0.002%
63	9.928	2667	2671	2674	rBV	364	309	0.02%	0.002%
64	10.163	2742	2744	2750	rVB2	330	302	0.01%	0.002%
65	10.481	2840	2843	2846	rVB3	695	441	0.02%	0.003%
66	10.513	2846	2853	2855	rBV2	547	547	0.03%	0.003%
67	10.536	2855	2860	2864	rVB2	281	330	0.02%	0.002%
68	10.668	2891	2901	2908	rVB4	1295	2249	0.11%	0.014%
69	10.755	2912	2928	2950	rBV	565188	902561	44.56%	5.621%
70	10.893	2964	2971	2980	rVB7	1460	2581	0.13%	0.016%
71	10.996	2997	3003	3006	rBV4	409	521	0.03%	0.003%
72	11.092	3030	3033	3036	rBV2	654	407	0.02%	0.003%
73	11.118	3036	3041	3044	rBV3	788	621	0.03%	0.004%
74	11.179	3057	3060	3065	rBV2	324	288	0.01%	0.002%
75	11.292	3091	3095	3099	rVB2	377	360	0.02%	0.002%
76	11.311	3099	3101	3104	rBV3	419	278	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050857.D
 Acq On : 21 Sep 2022 01:51
 Operator : JC/MD
 Sample : N4650-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.436	3134	3140	3141	rBV	400	373	0.02%	0.002%
78	11.468	3144	3150	3160	rVV4	1859	2931	0.14%	0.018%
79	11.693	3215	3220	3223	rBV3	787	760	0.04%	0.005%
80	11.745	3234	3236	3241	rVB3	530	385	0.02%	0.002%
81	11.809	3244	3256	3280	rBV	489727	779338	38.48%	4.854%
82	12.070	3332	3337	3344	rVB6	1053	1430	0.07%	0.009%
83	12.192	3362	3375	3394	rBV	549715	898074	44.34%	5.593%
84	12.507	3470	3473	3478	rVB	983	777	0.04%	0.005%
85	12.542	3479	3484	3487	rBV3	491	498	0.02%	0.003%
86	12.700	3527	3533	3534	rBV	397	347	0.02%	0.002%
87	12.729	3539	3542	3545	rVB2	676	433	0.02%	0.003%
88	12.925	3599	3603	3607	rBV4	541	325	0.02%	0.002%
89	13.028	3632	3635	3638	rBV	336	288	0.01%	0.002%
90	13.073	3645	3649	3651	rBV2	423	328	0.02%	0.002%
91	13.160	3673	3676	3680	rVB3	465	350	0.02%	0.002%
92	13.539	3789	3794	3796	rBV3	492	476	0.02%	0.003%
93	13.594	3804	3811	3814	rBV3	532	734	0.04%	0.005%
94	13.870	3894	3897	3902	rVB3	589	384	0.02%	0.002%
95	13.893	3902	3904	3908	rBV2	523	370	0.02%	0.002%
96	13.957	3920	3924	3926	rBV2	597	444	0.02%	0.003%
97	14.089	3959	3965	3966	rBV3	987	971	0.05%	0.006%
98	14.684	4147	4150	4151	rBV	522	301	0.01%	0.002%
99	14.819	4190	4192	4197	rVB3	620	383	0.02%	0.002%
100	15.706	4465	4468	4471	rBV2	906	568	0.03%	0.004%




Sum of corrected areas: 16056601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050857.D
Acq On : 21 Sep 2022 01:51
Operator : JC/MD
Sample : N4650-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

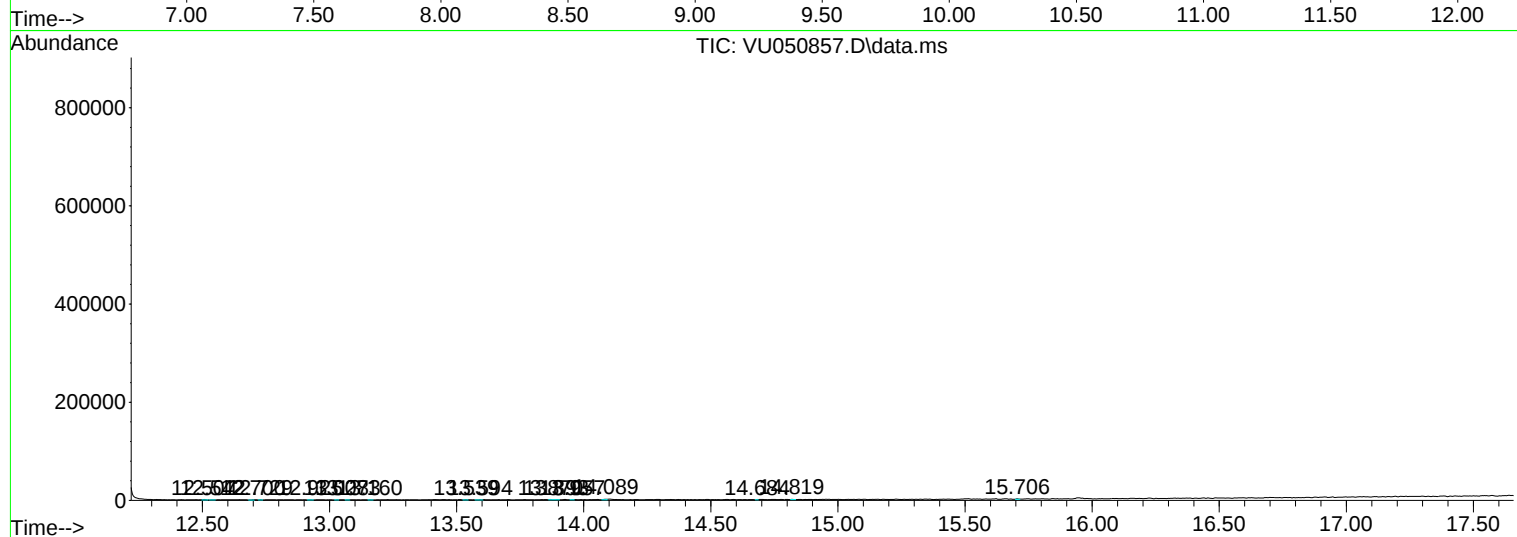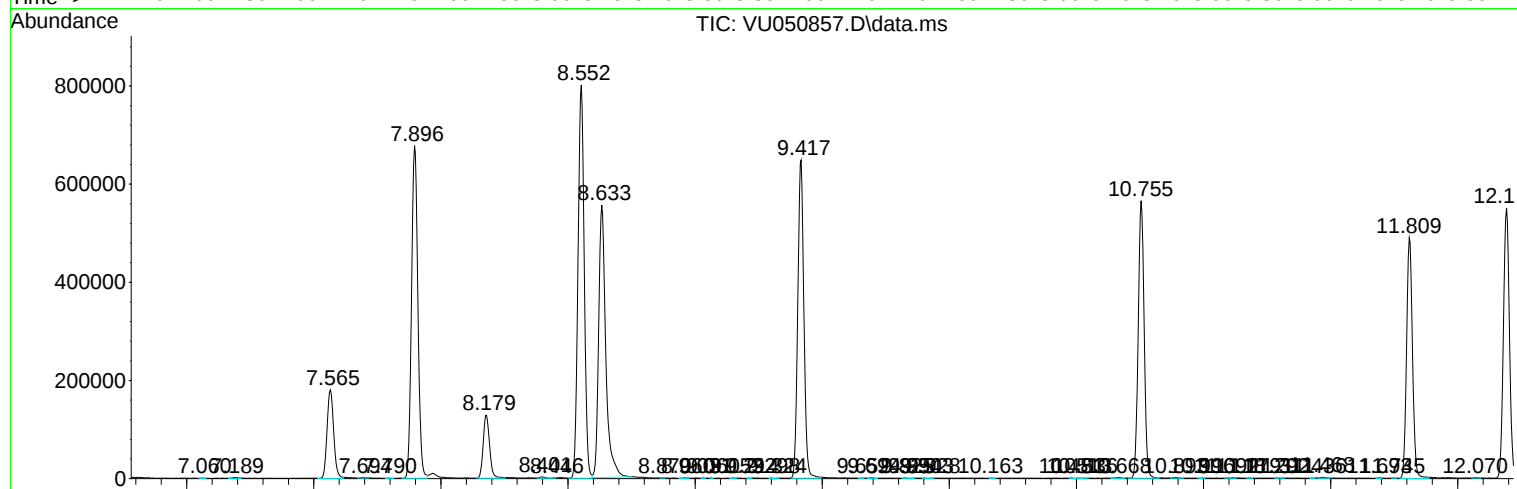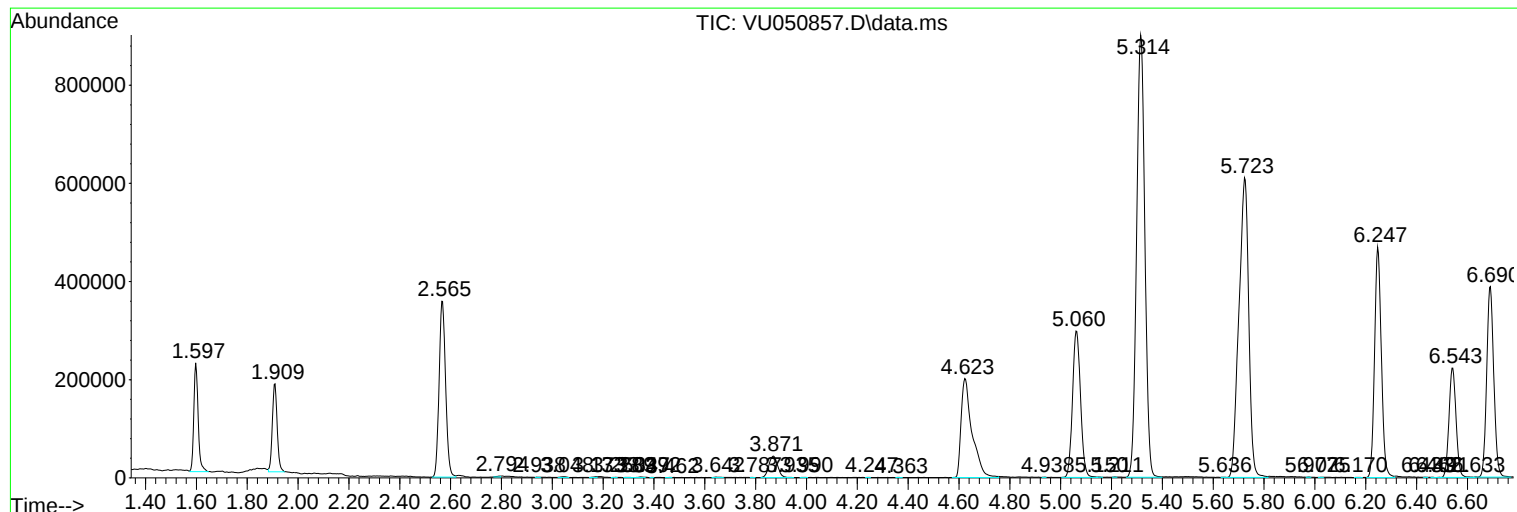

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050857.D
Acq On : 21 Sep 2022 01:51
Operator : JC/MD
Sample : N4650-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050857.D
Acq On : 21 Sep 2022 01:51
Operator : JC/MD
Sample : N4650-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------