

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050858.D
 Acq On : 21 Sep 2022 02:15
 Operator : JC/MD
 Sample : N4650-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	99	rVB	229069	270114	15.79%	2.162%
2	1.906	169	176	193	rVB	181869	241855	14.14%	1.936%
3	2.565	368	381	395	rBV	353228	580251	33.92%	4.644%
4	2.951	498	501	503	rBV3	750	538	0.03%	0.004%
5	3.015	518	521	522	rBV	413	159	0.01%	0.001%
6	3.179	563	572	588	rBV4	3025	7204	0.42%	0.058%
7	3.257	592	596	599	rVB2	384	268	0.02%	0.002%
8	3.289	599	606	613	rBV3	606	749	0.04%	0.006%
9	3.327	615	618	621	rBV3	256	188	0.01%	0.002%
10	3.411	640	644	645	rBV	242	168	0.01%	0.001%
11	3.453	654	657	661	rVB3	396	238	0.01%	0.002%
12	3.472	661	663	665	rBV	198	100	0.01%	0.001%
13	3.578	693	696	698	rBV2	279	168	0.01%	0.001%
14	3.652	713	719	723	rBV	898	835	0.05%	0.007%
15	3.739	743	746	750	rBV2	417	356	0.02%	0.003%
16	3.871	775	787	799	rBV2	3552	8716	0.51%	0.070%
17	3.941	806	809	813	rBV2	234	216	0.01%	0.002%
18	4.102	856	859	861	rBV	199	107	0.01%	0.001%
19	4.121	861	865	872	rVV2	494	534	0.03%	0.004%
20	4.192	882	887	888	rBV2	217	150	0.01%	0.001%
21	4.234	898	900	906	rVB	212	156	0.01%	0.001%
22	4.273	906	912	915	rBV	267	303	0.02%	0.002%
23	4.321	923	927	929	rBV	198	145	0.01%	0.001%
24	4.350	933	936	940	rVV2	231	154	0.01%	0.001%
25	4.446	961	966	971	rBV2	289	355	0.02%	0.003%
26	4.501	978	983	984	rBV	298	176	0.01%	0.001%
27	4.533	990	993	997	rVB	278	169	0.01%	0.001%
28	4.559	997	1001	1002	rBV	178	159	0.01%	0.001%
29	4.620	1007	1020	1053	rBV	206831	535762	31.32%	4.288%
30	5.060	1142	1157	1179	rVB	310829	672757	39.33%	5.384%
31	5.311	1220	1235	1249	rBV5	5776	14858	0.87%	0.119%
32	5.411	1264	1266	1271	rVB2	834	598	0.03%	0.005%
33	5.443	1271	1276	1279	rBV	446	299	0.02%	0.002%
34	5.485	1287	1289	1293	rBV2	149	94	0.01%	0.001%
35	5.546	1306	1308	1310	rBV	268	158	0.01%	0.001%
36	5.559	1310	1312	1314	rVB2	221	75	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050858.D
 Acq On : 21 Sep 2022 02:15
 Operator : JC/MD
 Sample : N4650-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.575	1314	1317	1321	rBV	173	116	0.01%	0.001%
38	5.594	1321	1323	1326	rVB	167	74	0.00%	0.001%
39	5.617	1327	1330	1336	rBV2	244	265	0.02%	0.002%
40	5.723	1340	1363	1395	rBV2	629556	1710631	100.00%	13.690%
41	5.973	1438	1441	1443	rBV2	668	357	0.02%	0.003%
42	6.070	1469	1471	1474	rBV2	281	104	0.01%	0.001%
43	6.108	1481	1483	1486	rBV	315	272	0.02%	0.002%
44	6.247	1510	1526	1548	rBV	467766	883521	51.65%	7.071%
45	6.533	1603	1615	1623	rBV9	5658	11189	0.65%	0.090%
46	6.690	1648	1664	1687	rBV	407386	794433	46.44%	6.358%
47	6.938	1738	1741	1746	rVB	546	379	0.02%	0.003%
48	6.970	1746	1751	1753	rBV2	1703	1550	0.09%	0.012%
49	7.054	1774	1777	1782	rVB2	572	465	0.03%	0.004%
50	7.092	1786	1789	1793	rVB3	359	207	0.01%	0.002%
51	7.125	1796	1799	1801	rVV	411	213	0.01%	0.002%
52	7.150	1805	1807	1810	rVV	230	149	0.01%	0.001%
53	7.189	1810	1819	1828	rVV8	1701	3095	0.18%	0.025%
54	7.227	1828	1831	1835	rVB3	390	267	0.02%	0.002%
55	7.256	1835	1840	1842	rBV2	201	138	0.01%	0.001%
56	7.301	1851	1854	1855	rBV2	195	109	0.01%	0.001%
57	7.372	1873	1876	1879	rBV	241	162	0.01%	0.001%
58	7.433	1888	1895	1898	rVB3	544	625	0.04%	0.005%
59	7.565	1923	1936	1959	rBV	191153	335477	19.61%	2.685%
60	7.764	1996	1998	1999	rBV	306	114	0.01%	0.001%
61	7.793	1999	2007	2021	rVB6	2801	4805	0.28%	0.038%
62	7.896	2024	2039	2056	rBV	708051	1213276	70.93%	9.710%
63	8.105	2101	2104	2108	rBV3	634	503	0.03%	0.004%
64	8.176	2111	2126	2141	rBV	138535	251470	14.70%	2.013%
65	8.436	2205	2207	2208	rBV	343	133	0.01%	0.001%
66	8.552	2236	2243	2253	rVB5	3951	5706	0.33%	0.046%
67	8.633	2253	2268	2300	rBV2	560680	1078261	63.03%	8.629%
68	9.047	2396	2397	2399	rBV	318	102	0.01%	0.001%
69	9.092	2405	2411	2412	rBV	684	449	0.03%	0.004%
70	9.150	2426	2429	2430	rBV2	244	134	0.01%	0.001%
71	9.176	2434	2437	2440	rBV2	306	232	0.01%	0.002%
72	9.192	2440	2442	2444	rVB3	285	103	0.01%	0.001%
73	9.211	2444	2448	2451	rVB3	329	237	0.01%	0.002%
74	9.227	2451	2453	2455	rBV	265	148	0.01%	0.001%
75	9.269	2461	2466	2473	rBV4	1006	1163	0.07%	0.009%
76	9.327	2482	2484	2486	rBV	422	183	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050858.D
 Acq On : 21 Sep 2022 02:15
 Operator : JC/MD
 Sample : N4650-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	9.359	2491	2494	2497	rVB2	437	259	0.02%	0.002%
78	9.414	2497	2511	2540	rBV	653723	1091444	63.80%	8.735%
79	9.697	2594	2599	2607	rVB3	859	1194	0.07%	0.010%
80	9.742	2608	2613	2616	rVB2	433	364	0.02%	0.003%
81	9.758	2616	2618	2619	rBV	206	102	0.01%	0.001%
82	9.925	2666	2670	2675	rBV3	557	686	0.04%	0.005%
83	10.176	2745	2748	2751	rVB	429	247	0.01%	0.002%
84	10.195	2751	2754	2757	rBV2	481	320	0.02%	0.003%
85	10.285	2780	2782	2785	rBV2	332	172	0.01%	0.001%
86	10.671	2894	2902	2914	rBV5	2480	3792	0.22%	0.030%
87	10.755	2914	2928	2946	rBV	576193	937429	54.80%	7.502%
88	10.861	2959	2961	2962	rBV2	525	197	0.01%	0.002%
89	10.970	2988	2995	2997	rBV3	509	485	0.03%	0.004%
90	11.086	3026	3031	3032	rBV	376	269	0.02%	0.002%
91	11.391	3123	3126	3128	rBV2	484	323	0.02%	0.003%
92	11.639	3197	3203	3206	rBV7	946	960	0.06%	0.008%
93	11.732	3229	3232	3233	rBV2	424	238	0.01%	0.002%
94	11.742	3233	3235	3240	rVB3	672	509	0.03%	0.004%
95	11.809	3244	3256	3274	rBV	527106	831917	48.63%	6.658%
96	12.192	3363	3375	3397	rVB	606088	981078	57.35%	7.852%
97	12.324	3412	3416	3419	rBV5	1639	1628	0.10%	0.013%
98	12.652	3516	3518	3521	rBV	414	277	0.02%	0.002%
99	13.259	3703	3707	3710	rBV3	922	1028	0.06%	0.008%
100	13.504	3781	3783	3787	rBV2	655	384	0.02%	0.003%




Sum of corrected areas: 12495251

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050858.D
Acq On : 21 Sep 2022 02:15
Operator : JC/MD
Sample : N4650-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

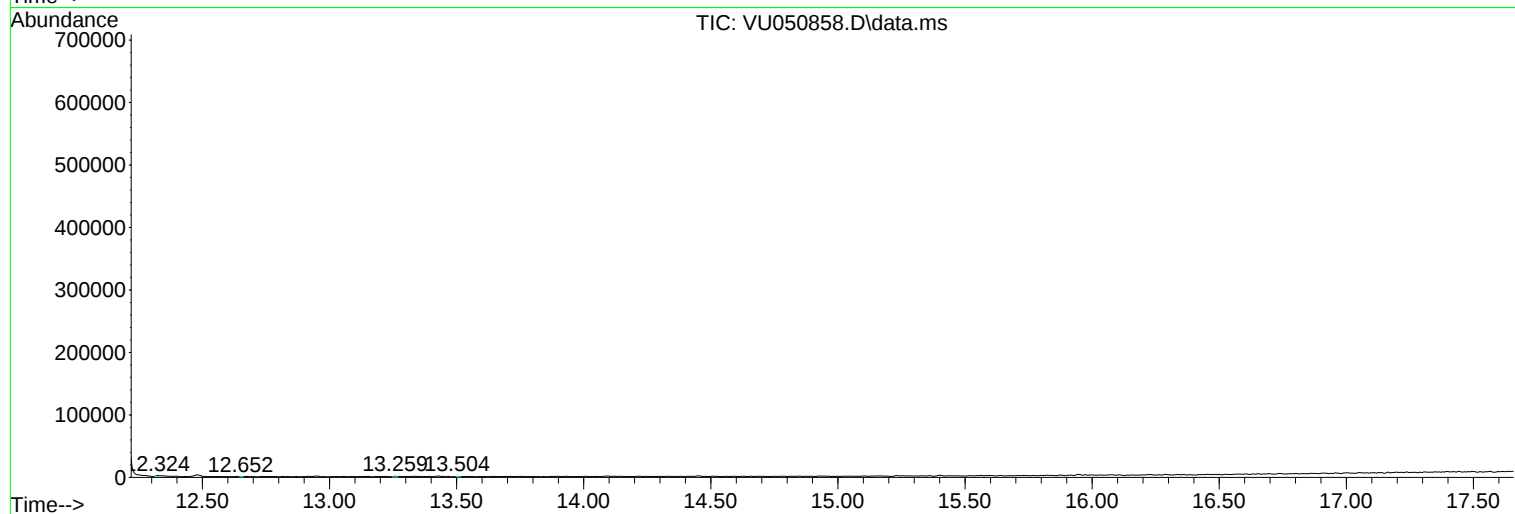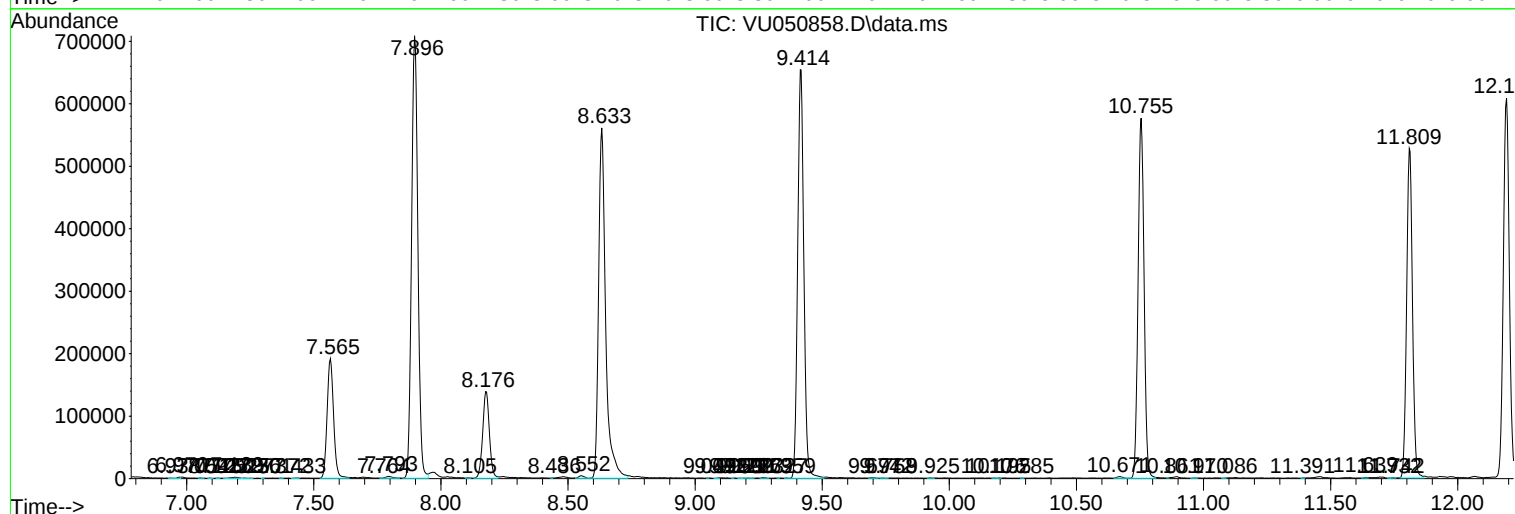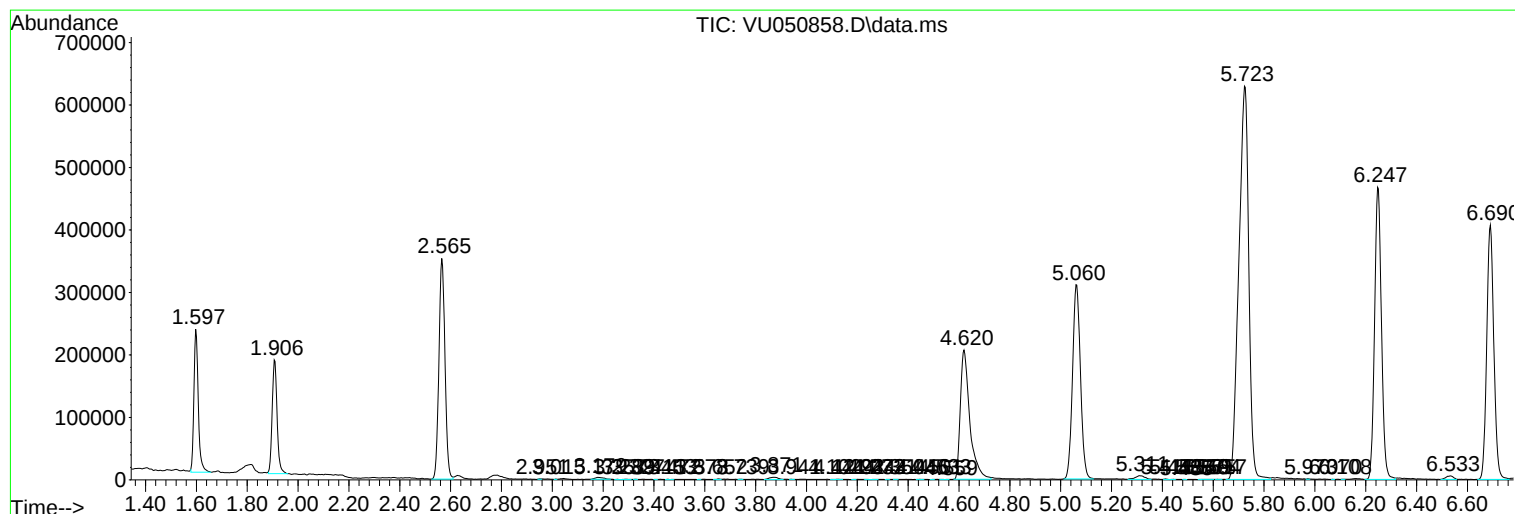

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050858.D
Acq On : 21 Sep 2022 02:15
Operator : JC/MD
Sample : N4650-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050858.D
Acq On : 21 Sep 2022 02:15
Operator : JC/MD
Sample : N4650-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------