

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050859.D
 Acq On : 21 Sep 2022 02:38
 Operator : JC/MD
 Sample : N4650-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	231864	270520	15.09%	1.842%
2	1.909	169	177	194	rVB	200624	266879	14.89%	1.817%
3	2.491	356	358	362	rVB2	714	457	0.03%	0.003%
4	2.565	369	381	398	rBV2	378492	657390	36.67%	4.475%
5	2.809	440	457	464	rBV3	6263	19626	1.09%	0.134%
6	3.041	523	529	538	rVB5	1544	2322	0.13%	0.016%
7	3.083	540	542	548	rVB2	263	256	0.01%	0.002%
8	3.121	548	554	555	rBV2	342	296	0.02%	0.002%
9	3.176	565	571	572	rBV3	918	880	0.05%	0.006%
10	3.353	615	626	639	rVV2	17445	34544	1.93%	0.235%
11	3.504	669	673	675	rBV	714	468	0.03%	0.003%
12	3.649	711	718	720	rBV2	369	380	0.02%	0.003%
13	3.867	770	786	816	rVV2	170037	401761	22.41%	2.735%
14	4.054	842	844	849	rVB3	412	292	0.02%	0.002%
15	4.192	879	887	889	rBV2	453	431	0.02%	0.003%
16	4.247	899	904	908	rBV3	367	355	0.02%	0.002%
17	4.340	929	933	936	rVB2	337	320	0.02%	0.002%
18	4.440	960	964	969	rBV3	319	354	0.02%	0.002%
19	4.623	1006	1021	1027	rBV	209885	444549	24.80%	3.026%
20	4.960	1124	1126	1131	rVB4	705	511	0.03%	0.003%
21	5.063	1141	1158	1181	rBV	320053	708657	39.53%	4.824%
22	5.205	1198	1202	1205	rBV	677	625	0.03%	0.004%
23	5.314	1219	1236	1257	rBV	515429	1169975	65.27%	7.965%
24	5.491	1287	1291	1295	rBV3	782	799	0.04%	0.005%
25	5.722	1341	1363	1395	rBV2	661579	1792497	100.00%	12.202%
26	5.993	1444	1447	1450	rVB3	368	268	0.01%	0.002%
27	6.112	1480	1484	1485	rBV	479	336	0.02%	0.002%
28	6.186	1501	1507	1510	rBV2	350	356	0.02%	0.002%
29	6.247	1511	1526	1556	rBV	490910	938651	52.37%	6.390%
30	6.539	1604	1617	1631	rVB6	14551	29843	1.66%	0.203%
31	6.607	1636	1638	1641	rVB2	472	308	0.02%	0.002%
32	6.690	1648	1664	1685	rBV	423151	819674	45.73%	5.580%
33	7.189	1813	1819	1825	rBV5	1714	2137	0.12%	0.015%
34	7.565	1923	1936	1953	rBV	194747	347011	19.36%	2.362%
35	7.677	1968	1971	1974	rBV2	665	534	0.03%	0.004%
36	7.796	2004	2008	2014	rVB3	562	539	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050859.D
 Acq On : 21 Sep 2022 02:38
 Operator : JC/MD
 Sample : N4650-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.838	2018	2021	2026	rBV2	391	323	0.02%	0.002%
38	7.896	2026	2039	2056	rBV	731892	1262030	70.41%	8.591%
39	8.034	2080	2082	2085	rBV2	545	295	0.02%	0.002%
40	8.063	2089	2091	2096	rVB3	447	290	0.02%	0.002%
41	8.111	2104	2106	2112	rVB3	548	392	0.02%	0.003%
42	8.179	2112	2127	2144	rBV	143450	266566	14.87%	1.815%
43	8.398	2187	2195	2202	rVB6	2374	3639	0.20%	0.025%
44	8.462	2210	2215	2216	rBV2	1131	817	0.05%	0.006%
45	8.472	2216	2218	2230	rVB4	2200	2818	0.16%	0.019%
46	8.552	2230	2243	2256	rBV	71727	118593	6.62%	0.807%
47	8.632	2256	2268	2306	rBV2	574961	1113625	62.13%	7.581%
48	8.957	2366	2369	2372	rVB2	414	272	0.02%	0.002%
49	8.986	2376	2378	2384	rVB3	343	289	0.02%	0.002%
50	9.179	2433	2438	2441	rVB3	280	283	0.02%	0.002%
51	9.308	2475	2478	2481	rVV2	433	314	0.02%	0.002%
52	9.365	2491	2496	2497	rVV2	345	283	0.02%	0.002%
53	9.417	2497	2512	2546	rVV	698351	1146650	63.97%	7.806%
54	9.536	2546	2549	2555	rVV3	1046	1248	0.07%	0.008%
55	9.568	2557	2559	2565	rVV4	666	562	0.03%	0.004%
56	9.616	2570	2574	2577	rVB3	426	274	0.02%	0.002%
57	9.697	2593	2599	2607	rBV4	948	1511	0.08%	0.010%
58	9.806	2630	2633	2637	rBV2	413	353	0.02%	0.002%
59	10.234	2761	2766	2770	rBV3	379	451	0.03%	0.003%
60	10.394	2812	2816	2822	rBV2	695	628	0.04%	0.004%
61	10.539	2854	2861	2864	rBV2	467	435	0.02%	0.003%
62	10.668	2896	2901	2908	rVV5	1524	1738	0.10%	0.012%
63	10.754	2912	2928	2948	rBV	608872	967288	53.96%	6.585%
64	10.877	2963	2966	2967	rBV2	623	309	0.02%	0.002%
65	10.896	2967	2972	2975	rVV2	1332	1226	0.07%	0.008%
66	10.970	2992	2995	2999	rBV3	494	335	0.02%	0.002%
67	11.050	3017	3020	3025	rVB3	652	439	0.02%	0.003%
68	11.092	3029	3033	3036	rBV2	485	429	0.02%	0.003%
69	11.160	3050	3054	3056	rVB2	449	286	0.02%	0.002%
70	11.504	3160	3161	3166	rVB2	595	318	0.02%	0.002%
71	11.565	3174	3180	3182	rBV2	389	364	0.02%	0.002%
72	11.687	3216	3218	3226	rBV5	663	617	0.03%	0.004%
73	11.809	3244	3256	3273	rBV	550593	862116	48.10%	5.869%
74	12.070	3329	3337	3348	rBV4	2459	4222	0.24%	0.029%
75	12.192	3361	3375	3393	rBV	622668	1000943	55.84%	6.814%
76	12.324	3413	3416	3420	rBV5	684	672	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050859.D
 Acq On : 21 Sep 2022 02:38
 Operator : JC/MD
 Sample : N4650-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ36

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.401	3437	3440	3445	rVB5	580	566	0.03%	0.004%
78	12.430	3445	3449	3451	rBV2	491	381	0.02%	0.003%
79	12.478	3460	3464	3470	rVB3	536	480	0.03%	0.003%
80	12.536	3479	3482	3485	rBV2	427	304	0.02%	0.002%
81	12.565	3486	3491	3495	rVB3	781	810	0.05%	0.006%
82	12.597	3495	3501	3508	rBV4	758	1173	0.07%	0.008%
83	12.635	3508	3513	3515	rBV2	321	375	0.02%	0.003%
84	12.729	3537	3542	3544	rBV2	409	284	0.02%	0.002%
85	12.742	3544	3546	3549	rVB2	595	325	0.02%	0.002%
86	12.758	3549	3551	3553	rBV	538	351	0.02%	0.002%
87	13.179	3678	3682	3684	rBV2	450	316	0.02%	0.002%
88	13.230	3695	3698	3701	rVB3	553	404	0.02%	0.003%
89	13.262	3705	3708	3711	rVB3	540	287	0.02%	0.002%
90	13.523	3785	3789	3793	rVB3	421	427	0.02%	0.003%
91	13.545	3793	3796	3801	rVB2	428	358	0.02%	0.002%
92	13.706	3843	3846	3849	rBV	322	312	0.02%	0.002%
93	13.828	3880	3884	3887	rBV2	398	357	0.02%	0.002%
94	13.941	3914	3919	3920	rBV	443	425	0.02%	0.003%
95	14.044	3949	3951	3956	rVB2	611	337	0.02%	0.002%
96	14.642	4135	4137	4140	rBV	621	377	0.02%	0.003%
97	15.008	4249	4251	4256	rBV3	480	272	0.02%	0.002%
98	15.153	4294	4296	4300	rVB3	773	524	0.03%	0.004%
99	15.253	4322	4327	4331	rBV5	605	751	0.04%	0.005%
100	15.873	4518	4520	4523	rBV3	1006	552	0.03%	0.004%




Sum of corrected areas: 14689792

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050859.D
Acq On : 21 Sep 2022 02:38
Operator : JC/MD
Sample : N4650-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

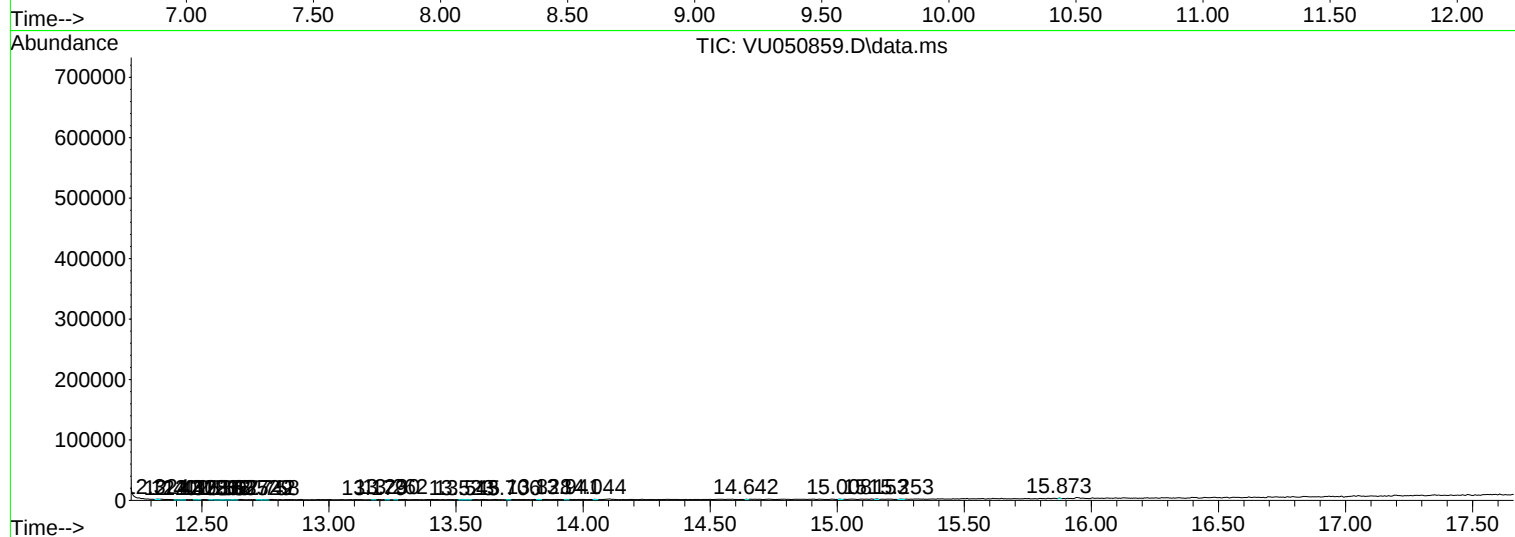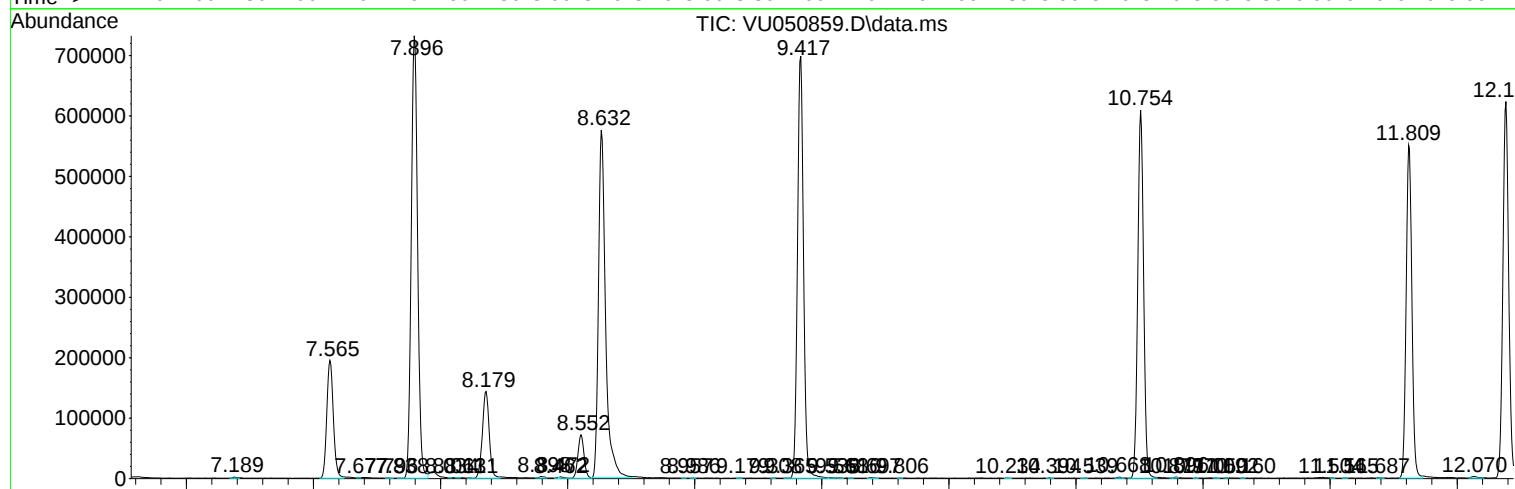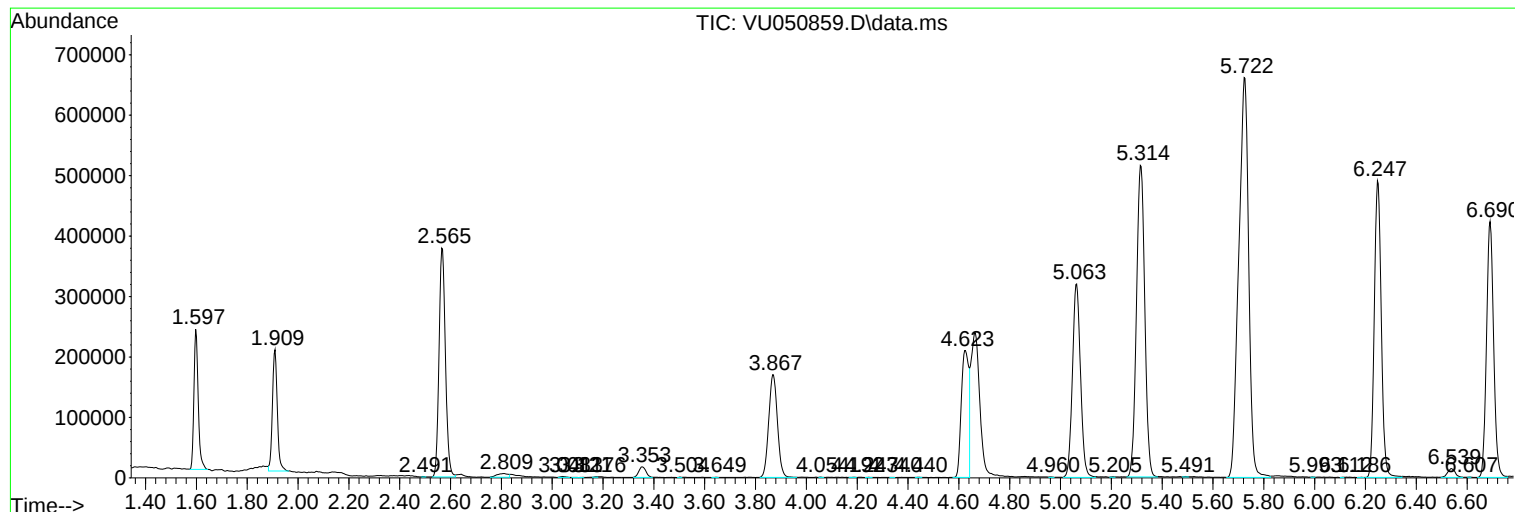

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050859.D
Acq On : 21 Sep 2022 02:38
Operator : JC/MD
Sample : N4650-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050859.D
Acq On : 21 Sep 2022 02:38
Operator : JC/MD
Sample : N4650-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------