

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050860.D
 Acq On : 21 Sep 2022 03:01
 Operator : JC/MD
 Sample : N4650-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	97	rVB	254552	298029	15.48%	2.111%
2	1.909	170	177	193	rVB	208916	271730	14.11%	1.924%
3	2.565	368	381	396	rBV	389903	653194	33.93%	4.626%
4	2.797	438	453	461	rBV5	5195	13823	0.72%	0.098%
5	3.131	555	557	559	rBV3	343	147	0.01%	0.001%
6	3.150	559	563	567	rVV2	295	239	0.01%	0.002%
7	3.356	615	627	642	rVB2	21629	42569	2.21%	0.301%
8	3.430	648	650	654	rBV2	213	165	0.01%	0.001%
9	3.507	671	674	679	rBV2	300	230	0.01%	0.002%
10	3.539	682	684	685	rBV	120	52	0.00%	0.000%
11	3.562	689	691	693	rBV	245	110	0.01%	0.001%
12	3.707	734	736	737	rBV	185	81	0.00%	0.001%
13	3.755	746	751	756	rBV3	982	992	0.05%	0.007%
14	3.870	772	787	805	rBV	36551	84959	4.41%	0.602%
15	3.954	810	813	814	rBV	212	84	0.00%	0.001%
16	3.977	817	820	822	rBV	197	106	0.01%	0.001%
17	4.018	832	833	838	rVB	239	117	0.01%	0.001%
18	4.044	838	841	842	rBV	163	108	0.01%	0.001%
19	4.096	854	857	859	rBV2	247	143	0.01%	0.001%
20	4.176	879	882	884	rVB2	138	60	0.00%	0.000%
21	4.192	884	887	890	rVB	338	204	0.01%	0.001%
22	4.205	890	891	892	rVB	191	37	0.00%	0.000%
23	4.215	892	894	897	rBV	346	221	0.01%	0.002%
24	4.301	918	921	922	rBV2	196	116	0.01%	0.001%
25	4.337	929	932	935	rBV	162	90	0.00%	0.001%
26	4.452	965	968	971	rVB2	270	150	0.01%	0.001%
27	4.507	982	985	993	rVB	251	252	0.01%	0.002%
28	4.546	993	997	1002	rBV2	453	381	0.02%	0.003%
29	4.623	1008	1021	1027	rBV	219376	465024	24.15%	3.293%
30	5.060	1141	1157	1178	rBV	346629	768335	39.91%	5.441%
31	5.314	1222	1236	1251	rVB	88934	198700	10.32%	1.407%
32	5.430	1268	1272	1274	rBV	296	172	0.01%	0.001%
33	5.462	1278	1282	1284	rBV2	212	112	0.01%	0.001%
34	5.491	1286	1291	1293	rBV	198	188	0.01%	0.001%
35	5.514	1296	1298	1300	rVB	191	83	0.00%	0.001%
36	5.530	1300	1303	1310	rBV2	439	442	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050860.D
 Acq On : 21 Sep 2022 03:01
 Operator : JC/MD
 Sample : N4650-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.568	1314	1315	1318	rVB	242	108	0.01%	0.001%
38	5.587	1318	1321	1325	rBV	266	186	0.01%	0.001%
39	5.613	1325	1329	1331	rBV	310	206	0.01%	0.001%
40	5.723	1341	1363	1401	rBV2	707686	1925224	100.00%	13.634%
41	6.012	1449	1453	1458	rVB3	639	581	0.03%	0.004%
42	6.038	1459	1461	1465	rBV2	395	283	0.01%	0.002%
43	6.198	1510	1511	1512	rBV	116	25	0.00%	0.000%
44	6.250	1512	1527	1546	rBV	511730	977760	50.79%	6.924%
45	6.539	1602	1617	1637	rBV4	73416	146579	7.61%	1.038%
46	6.690	1649	1664	1683	rBV	454961	878426	45.63%	6.221%
47	6.893	1725	1727	1729	rBV3	383	177	0.01%	0.001%
48	6.948	1742	1744	1748	rVB2	199	148	0.01%	0.001%
49	6.980	1748	1754	1755	rBV2	415	377	0.02%	0.003%
50	7.073	1781	1783	1786	rVB3	293	145	0.01%	0.001%
51	7.092	1786	1789	1790	rBV	333	184	0.01%	0.001%
52	7.147	1798	1806	1809	rBV4	537	633	0.03%	0.004%
53	7.192	1811	1820	1823	rBV6	1998	2827	0.15%	0.020%
54	7.269	1842	1844	1845	rBV	148	36	0.00%	0.000%
55	7.279	1845	1847	1848	rBV	129	55	0.00%	0.000%
56	7.330	1860	1863	1865	rBV2	242	121	0.01%	0.001%
57	7.366	1871	1874	1878	rBV2	354	328	0.02%	0.002%
58	7.388	1878	1881	1886	rVB2	430	326	0.02%	0.002%
59	7.420	1888	1891	1896	rBV2	267	199	0.01%	0.001%
60	7.443	1896	1898	1900	rBV	122	55	0.00%	0.000%
61	7.478	1907	1909	1914	rVB2	278	186	0.01%	0.001%
62	7.504	1916	1917	1918	rBB2	54	37	0.00%	0.000%
63	7.565	1922	1936	1954	rBV	203623	367295	19.08%	2.601%
64	7.841	2019	2022	2023	rBV	187	96	0.00%	0.001%
65	7.896	2025	2039	2056	rBV	779307	1335019	69.34%	9.455%
66	8.179	2113	2127	2145	rBV	155696	284072	14.76%	2.012%
67	8.456	2210	2213	2214	rBV2	367	196	0.01%	0.001%
68	8.552	2232	2243	2256	rBV	87572	146300	7.60%	1.036%
69	8.632	2256	2268	2299	rBV2	605877	1170575	60.80%	8.290%
70	8.954	2367	2368	2372	rVB	384	182	0.01%	0.001%
71	8.973	2372	2374	2379	rVB3	532	315	0.02%	0.002%
72	9.089	2407	2410	2412	rBV2	335	185	0.01%	0.001%
73	9.102	2412	2414	2417	rVV	328	258	0.01%	0.002%
74	9.134	2421	2424	2427	rBV2	297	228	0.01%	0.002%
75	9.227	2451	2453	2456	rBV2	323	208	0.01%	0.001%
76	9.295	2471	2474	2476	rBV2	317	188	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050860.D
 Acq On : 21 Sep 2022 03:01
 Operator : JC/MD
 Sample : N4650-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	9.308	2476	2478	2481	rBV	287	211	0.01%	0.001%
78	9.417	2498	2512	2539	rBV	709582	1177267	61.15%	8.337%
79	9.693	2592	2598	2600	rBV3	658	775	0.04%	0.005%
80	9.722	2605	2607	2611	rVB	512	298	0.02%	0.002%
81	9.764	2617	2620	2622	rVB2	370	154	0.01%	0.001%
82	9.787	2625	2627	2629	rVV	398	224	0.01%	0.002%
83	9.800	2629	2631	2636	rVB3	559	356	0.02%	0.003%
84	9.845	2641	2645	2649	rBV2	559	449	0.02%	0.003%
85	9.867	2649	2652	2655	rBV3	314	261	0.01%	0.002%
86	10.446	2829	2832	2833	rBB2	67	55	0.00%	0.000%
87	10.491	2839	2846	2849	rBV3	458	572	0.03%	0.004%
88	10.590	2874	2877	2881	rBV	333	319	0.02%	0.002%
89	10.661	2896	2899	2900	rBV	837	474	0.02%	0.003%
90	10.754	2915	2928	2952	rBV	642992	1031301	53.57%	7.304%
91	10.890	2967	2970	2971	rBV2	793	491	0.03%	0.003%
92	10.999	3002	3004	3006	rBV	198	86	0.00%	0.001%
93	11.025	3006	3012	3015	rBV2	374	479	0.02%	0.003%
94	11.369	3116	3119	3120	rBV2	404	249	0.01%	0.002%
95	11.410	3129	3132	3134	rBV2	723	397	0.02%	0.003%
96	11.449	3140	3144	3145	rBV2	935	624	0.03%	0.004%
97	11.642	3202	3204	3206	rBV2	248	74	0.00%	0.001%
98	11.745	3233	3236	3239	rBV	674	485	0.03%	0.003%
99	11.809	3242	3256	3273	rBV	529366	843993	43.84%	5.977%
100	12.192	3362	3375	3393	rBV	626201	1018963	52.93%	7.216%




Sum of corrected areas: 14120331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050860.D
Acq On : 21 Sep 2022 03:01
Operator : JC/MD
Sample : N4650-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

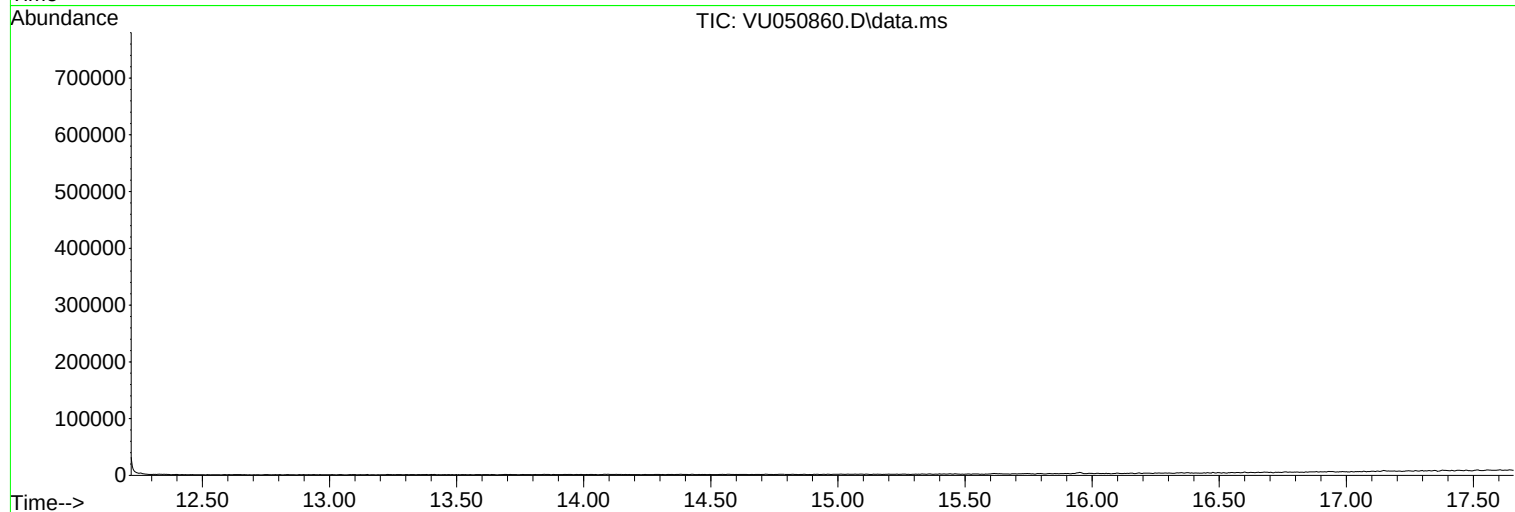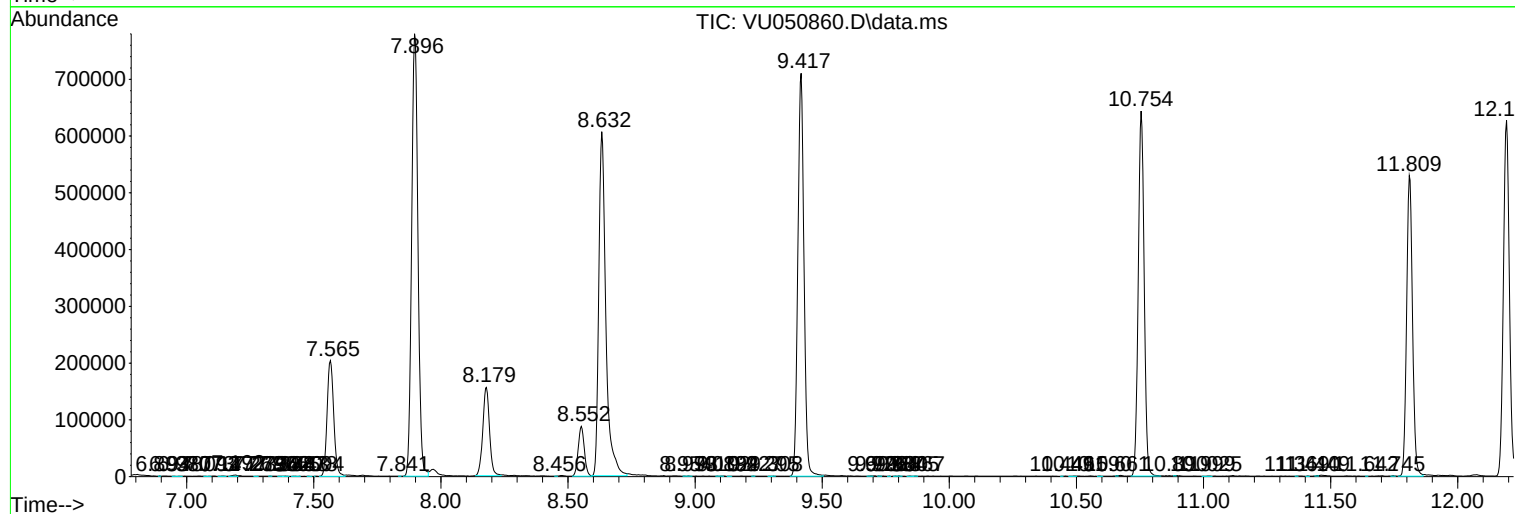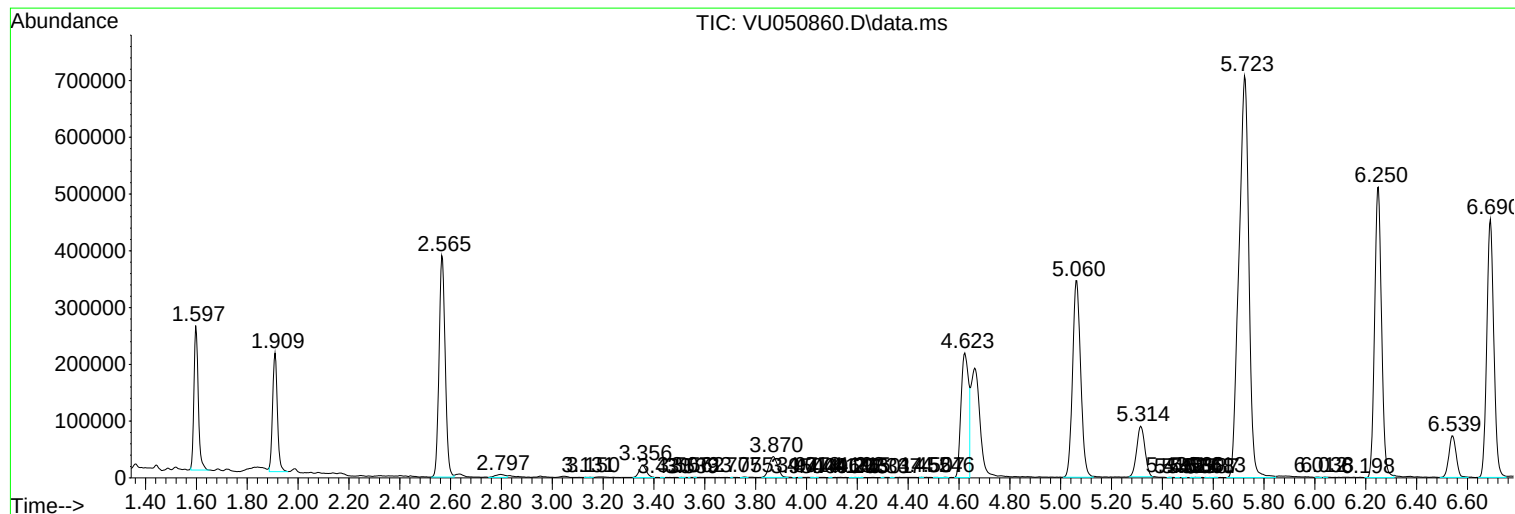

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050860.D
Acq On : 21 Sep 2022 03:01
Operator : JC/MD
Sample : N4650-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050860.D
Acq On : 21 Sep 2022 03:01
Operator : JC/MD
Sample : N4650-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------