

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050863.D
 Acq On : 21 Sep 2022 04:12
 Operator : JC/MD
 Sample : N4650-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	104	rVB	246452	291482	11.60%	1.743%
2	1.912	170	178	197	rBV	207224	269055	10.71%	1.609%
3	2.565	369	381	418	rBV	373974	640110	25.48%	3.828%
4	2.726	427	431	436	rVB3	316	320	0.01%	0.002%
5	2.771	441	445	447	rBV3	345	322	0.01%	0.002%
6	2.787	447	450	451	rBV	563	390	0.02%	0.002%
7	2.845	463	468	471	rBV3	456	493	0.02%	0.003%
8	2.903	484	486	490	rVB4	563	373	0.01%	0.002%
9	2.925	490	493	496	rBV3	439	317	0.01%	0.002%
10	2.977	506	509	512	rVB3	510	379	0.02%	0.002%
11	3.044	519	530	545	rVV2	8594	15613	0.62%	0.093%
12	3.186	559	574	590	rBV	23251	53542	2.13%	0.320%
13	3.356	616	627	640	rBV3	6859	12610	0.50%	0.075%
14	3.552	683	688	691	rBV3	296	295	0.01%	0.002%
15	3.870	770	787	808	rBV2	57893	136770	5.44%	0.818%
16	4.031	830	837	840	rBV2	805	747	0.03%	0.004%
17	4.186	881	885	892	rVB3	262	334	0.01%	0.002%
18	4.272	908	912	916	rVB2	348	331	0.01%	0.002%
19	4.665	1010	1034	1075	rBV2	911284	2512333	100.00%	15.022%
20	5.063	1140	1158	1180	rBV	340730	751808	29.92%	4.495%
21	5.314	1220	1236	1255	rVB	370806	831811	33.11%	4.974%
22	5.558	1310	1312	1315	rVB	685	352	0.01%	0.002%
23	5.597	1319	1324	1326	rBV2	632	509	0.02%	0.003%
24	5.623	1330	1332	1341	rVB3	532	577	0.02%	0.003%
25	5.726	1341	1364	1398	rBV2	698050	1897564	75.53%	11.346%
26	5.973	1438	1441	1442	rBV3	518	294	0.01%	0.002%
27	6.044	1461	1463	1472	rVB4	480	412	0.02%	0.002%
28	6.153	1495	1497	1504	rVB3	586	471	0.02%	0.003%
29	6.247	1509	1526	1554	rBV	524406	1004468	39.98%	6.006%
30	6.446	1583	1588	1590	rBV4	323	339	0.01%	0.002%
31	6.533	1603	1615	1626	rBV4	9892	19883	0.79%	0.119%
32	6.603	1635	1637	1645	rVB4	378	363	0.01%	0.002%
33	6.690	1645	1664	1689	rBV	445305	877887	34.94%	5.249%
34	6.854	1712	1715	1717	rBV	559	361	0.01%	0.002%
35	6.893	1723	1727	1732	rVB4	678	659	0.03%	0.004%
36	6.919	1732	1735	1738	rBV2	651	374	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050863.D
 Acq On : 21 Sep 2022 04:12
 Operator : JC/MD
 Sample : N4650-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.986	1752	1756	1759	rBV3	587	369	0.01%	0.002%
38	7.182	1806	1817	1818	rBV4	1292	1309	0.05%	0.008%
39	7.218	1826	1828	1833	rVB4	907	633	0.03%	0.004%
40	7.304	1849	1855	1857	rBV3	476	427	0.02%	0.003%
41	7.385	1877	1880	1888	rVB	436	452	0.02%	0.003%
42	7.430	1891	1894	1901	rVB2	585	466	0.02%	0.003%
43	7.565	1922	1936	1960	rBV	207865	370760	14.76%	2.217%
44	7.684	1970	1973	1975	rBV3	837	624	0.02%	0.004%
45	7.793	2000	2007	2008	rBV4	804	889	0.04%	0.005%
46	7.896	2025	2039	2054	rBV	763093	1304044	51.91%	7.798%
47	8.105	2100	2104	2107	rBV4	380	348	0.01%	0.002%
48	8.179	2115	2127	2143	rBV2	147649	256958	10.23%	1.536%
49	8.401	2190	2196	2206	rVB10	2052	3059	0.12%	0.018%
50	8.465	2211	2216	2219	rBV2	655	512	0.02%	0.003%
51	8.552	2234	2243	2253	rVB4	8610	14416	0.57%	0.086%
52	8.632	2255	2268	2302	rBV2	603237	1188537	47.31%	7.107%
53	8.870	2337	2342	2347	rBV4	1059	1378	0.05%	0.008%
54	8.938	2359	2363	2366	rBV2	447	327	0.01%	0.002%
55	9.095	2410	2412	2416	rBV2	427	344	0.01%	0.002%
56	9.308	2474	2478	2482	rBV3	362	293	0.01%	0.002%
57	9.417	2498	2512	2540	rBV	699816	1182725	47.08%	7.072%
58	9.571	2550	2560	2570	rVB6	2861	5557	0.22%	0.033%
59	9.693	2589	2598	2608	rVV2	8093	12601	0.50%	0.075%
60	9.922	2662	2669	2672	rBV3	875	832	0.03%	0.005%
61	10.102	2714	2725	2734	rVV3	6738	11303	0.45%	0.068%
62	10.211	2757	2759	2764	rVV2	323	311	0.01%	0.002%
63	10.343	2794	2800	2802	rBV3	622	588	0.02%	0.004%
64	10.549	2861	2864	2869	rVB3	432	317	0.01%	0.002%
65	10.626	2884	2888	2892	rVB3	555	390	0.02%	0.002%
66	10.668	2892	2901	2911	rBV4	1986	3300	0.13%	0.020%
67	10.754	2913	2928	2951	rBV	639731	1034091	41.16%	6.183%
68	10.902	2970	2974	2983	rVB7	1601	2593	0.10%	0.016%
69	10.999	2995	3004	3008	rBV2	5785	8780	0.35%	0.052%
70	11.086	3023	3031	3038	rBV3	5291	8614	0.34%	0.052%
71	11.291	3085	3095	3105	rBV3	6173	9337	0.37%	0.056%
72	11.410	3128	3132	3137	rVV4	756	715	0.03%	0.004%
73	11.468	3140	3150	3164	rVV2	14257	23446	0.93%	0.140%
74	11.610	3191	3194	3195	rBV2	424	296	0.01%	0.002%
75	11.642	3198	3204	3207	rBV2	698	719	0.03%	0.004%
76	11.706	3216	3224	3229	rBV4	973	1170	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050863.D
 Acq On : 21 Sep 2022 04:12
 Operator : JC/MD
 Sample : N4650-14 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.742	3229	3235	3238	rBV3	743	843	0.03%	0.005%
78	11.809	3243	3256	3275	rBV	554071	877014	34.91%	5.244%
79	11.893	3276	3282	3294	rVB2	10664	16332	0.65%	0.098%
80	11.960	3300	3303	3304	rBV2	664	420	0.02%	0.003%
81	12.063	3328	3335	3337	rVV4	2167	2398	0.10%	0.014%
82	12.095	3340	3345	3352	rVB7	3355	4378	0.17%	0.026%
83	12.192	3362	3375	3393	rBV	629457	1020208	40.61%	6.100%
84	12.372	3427	3431	3433	rBV3	1038	855	0.03%	0.005%
85	12.481	3456	3465	3475	rBV6	8558	14813	0.59%	0.089%
86	12.565	3488	3491	3492	rBV2	659	415	0.02%	0.002%
87	12.616	3503	3507	3511	rVB2	369	291	0.01%	0.002%
88	12.677	3524	3526	3530	rVB2	794	492	0.02%	0.003%
89	12.709	3530	3536	3537	rBV4	720	660	0.03%	0.004%
90	12.873	3583	3587	3588	rBV2	707	428	0.02%	0.003%
91	12.944	3606	3609	3612	rBV	652	418	0.02%	0.002%
92	12.973	3614	3618	3623	rVB3	1021	1036	0.04%	0.006%
93	13.031	3631	3636	3645	rVB5	1445	1899	0.08%	0.011%
94	13.391	3744	3748	3752	rBV3	648	660	0.03%	0.004%
95	13.516	3784	3787	3792	rBV2	407	397	0.02%	0.002%
96	13.622	3818	3820	3823	rVV	617	443	0.02%	0.003%
97	13.639	3823	3825	3829	rVB	578	312	0.01%	0.002%
98	13.825	3880	3883	3886	rBV2	612	456	0.02%	0.003%
99	13.896	3902	3905	3907	rBV	484	328	0.01%	0.002%
100	14.774	4174	4178	4181	rBV2	644	584	0.02%	0.003%




Sum of corrected areas: 16723858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050863.D
Acq On : 21 Sep 2022 04:12
Operator : JC/MD
Sample : N4650-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

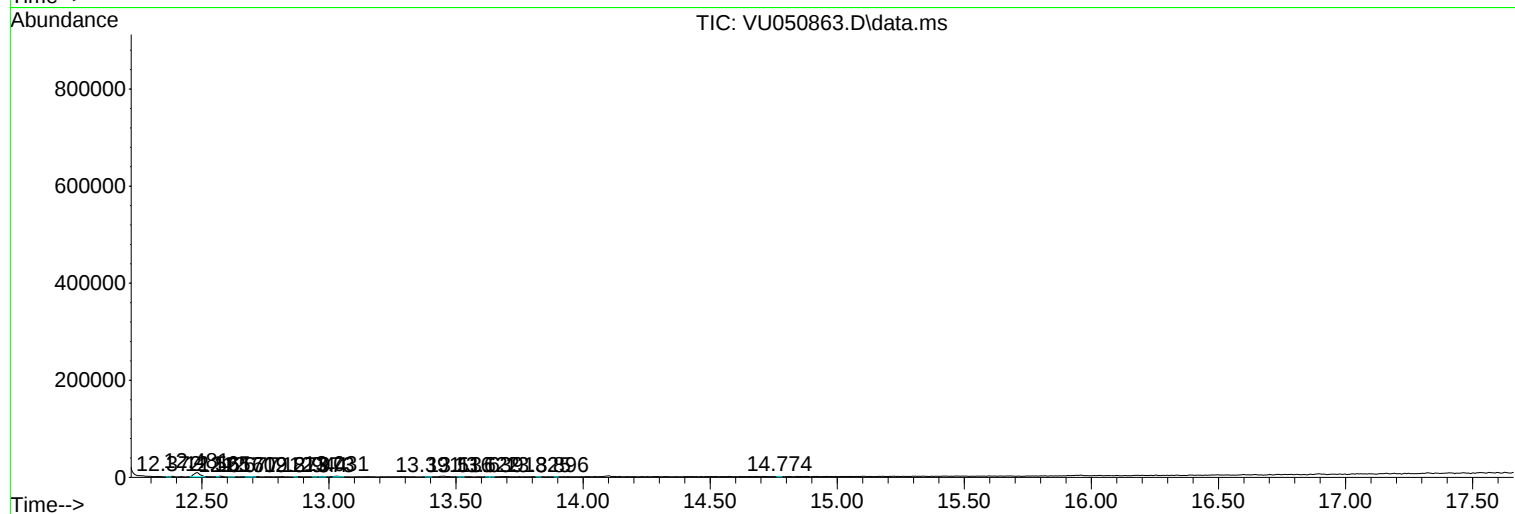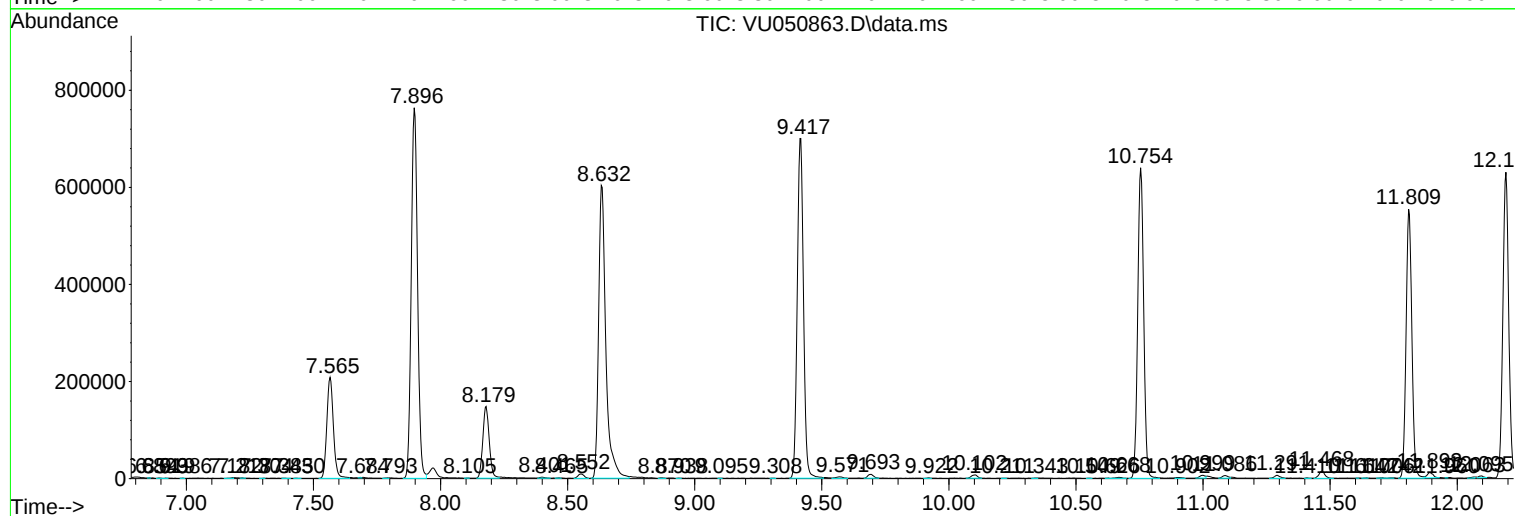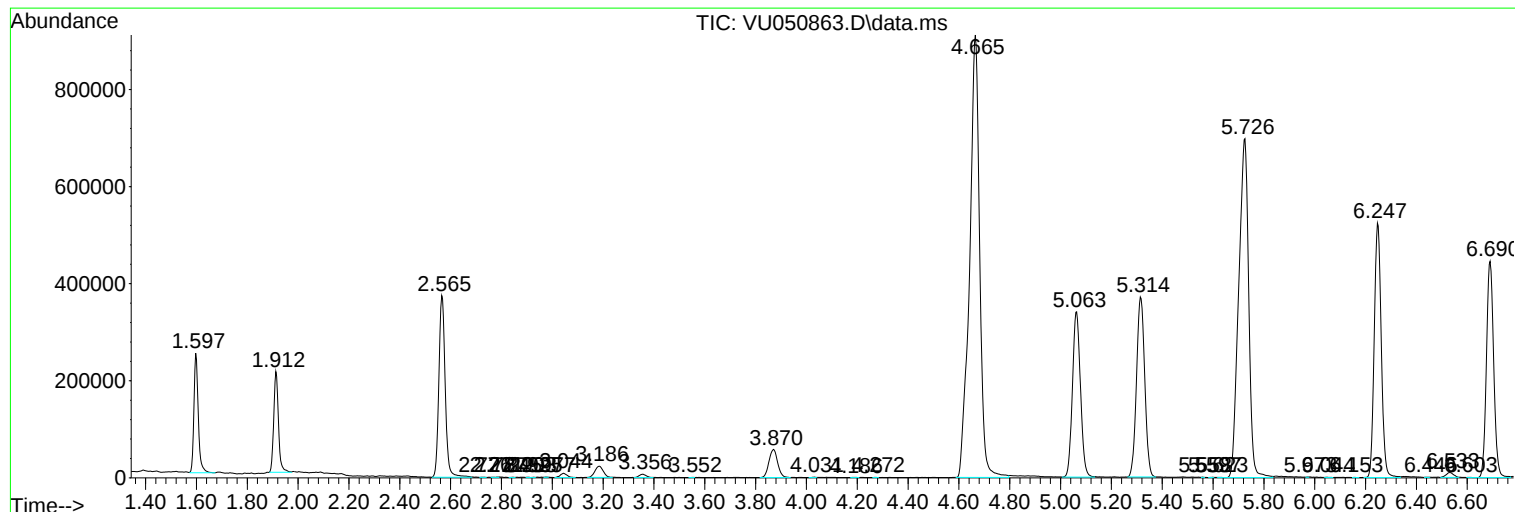

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050863.D
Acq On : 21 Sep 2022 04:12
Operator : JC/MD
Sample : N4650-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050863.D
Acq On : 21 Sep 2022 04:12
Operator : JC/MD
Sample : N4650-14 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc