

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050867.D
 Acq On : 21 Sep 2022 05:46
 Operator : JC/MD
 Sample : N4650-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	247400	291633	4.02%	1.065%
2	1.909	169	177	196	rVB	198054	262144	3.61%	0.957%
3	2.079	226	230	239	rVB	14360	17272	0.24%	0.063%
4	2.137	243	248	254	rBV2	14958	18210	0.25%	0.067%
5	2.578	369	385	416	rBV4	1318563	2432288	33.49%	8.883%
6	2.771	439	445	446	rBV3	3821	3767	0.05%	0.014%
7	3.044	522	530	538	rVB2	2432	3509	0.05%	0.013%
8	3.118	548	553	554	rBV3	650	480	0.01%	0.002%
9	3.141	558	560	564	rVV3	477	344	0.00%	0.001%
10	3.189	569	575	581	rVV4	1170	2208	0.03%	0.008%
11	3.353	614	626	646	rVV2	37826	74222	1.02%	0.271%
12	3.469	659	662	668	rVB2	419	441	0.01%	0.002%
13	3.507	668	674	676	rBV2	417	412	0.01%	0.002%
14	3.867	764	786	815	rBV	936996	2215202	30.50%	8.090%
15	4.086	852	854	858	rBV3	482	368	0.01%	0.001%
16	4.147	871	873	882	rVB4	437	517	0.01%	0.002%
17	4.304	920	922	927	rVB3	447	381	0.01%	0.001%
18	4.459	963	970	973	rBV3	465	582	0.01%	0.002%
19	4.623	1007	1021	1024	rBV2	212930	385436	5.31%	1.408%
20	4.874	1094	1099	1105	rBV7	1006	1653	0.02%	0.006%
21	5.063	1141	1158	1183	rBV	344490	782693	10.78%	2.859%
22	5.314	1213	1236	1262	rBV	3250926	7262345	100.00%	26.523%
23	5.722	1342	1363	1396	rBV2	683192	1865709	25.69%	6.814%
24	5.964	1435	1438	1441	rBV2	935	669	0.01%	0.002%
25	6.247	1508	1526	1548	rBV	521783	989578	13.63%	3.614%
26	6.542	1603	1618	1640	rBV	590774	1113479	15.33%	4.067%
27	6.690	1649	1664	1688	rVB	443071	857366	11.81%	3.131%
28	6.793	1693	1696	1697	rBV2	1297	853	0.01%	0.003%
29	7.115	1793	1796	1802	rVB2	345	343	0.00%	0.001%
30	7.150	1802	1807	1810	rBV2	486	458	0.01%	0.002%
31	7.176	1810	1815	1816	rBV4	1340	1052	0.01%	0.004%
32	7.330	1859	1863	1867	rBV3	534	535	0.01%	0.002%
33	7.436	1891	1896	1901	rVB3	442	528	0.01%	0.002%
34	7.565	1923	1936	1951	rBV	212211	366436	5.05%	1.338%
35	7.790	2000	2006	2014	rVB3	517	732	0.01%	0.003%
36	7.835	2014	2020	2022	rBV3	353	355	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050867.D
 Acq On : 21 Sep 2022 05:46
 Operator : JC/MD
 Sample : N4650-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.896	2023	2039	2056	rBV	777859	1330238	18.32%	4.858%
38	8.179	2115	2127	2142	rBV	148117	249634	3.44%	0.912%
39	8.401	2185	2196	2207	rVB2	27970	48081	0.66%	0.176%
40	8.465	2207	2216	2219	rBV8	1254	1674	0.02%	0.006%
41	8.552	2229	2243	2256	rBV	934126	1564108	21.54%	5.712%
42	8.632	2257	2268	2298	rVB2	574065	1106271	15.23%	4.040%
43	9.185	2434	2440	2443	rBV3	442	573	0.01%	0.002%
44	9.201	2443	2445	2453	rVB2	538	546	0.01%	0.002%
45	9.320	2477	2482	2486	rBV3	503	443	0.01%	0.002%
46	9.362	2490	2495	2498	rBV3	437	355	0.00%	0.001%
47	9.417	2498	2512	2535	rBV	721682	1188589	16.37%	4.341%
48	9.581	2561	2563	2567	rVB2	757	350	0.00%	0.001%
49	9.700	2597	2600	2605	rVV2	903	732	0.01%	0.003%
50	9.735	2606	2611	2615	rVB2	1263	1121	0.02%	0.004%
51	9.790	2624	2628	2633	rBV3	417	416	0.01%	0.002%
52	9.864	2648	2651	2656	rBV2	490	443	0.01%	0.002%
53	9.896	2658	2661	2668	rVB3	576	568	0.01%	0.002%
54	9.944	2673	2676	2682	rVB3	328	363	0.00%	0.001%
55	10.279	2771	2780	2782	rBV3	393	420	0.01%	0.002%
56	10.307	2782	2789	2792	rBV2	518	598	0.01%	0.002%
57	10.359	2802	2805	2811	rVB3	440	508	0.01%	0.002%
58	10.648	2891	2895	2897	rBV2	426	343	0.00%	0.001%
59	10.671	2897	2902	2912	rVB5	1712	1876	0.03%	0.007%
60	10.754	2915	2928	2948	rBV	634205	1002419	13.80%	3.661%
61	10.867	2960	2963	2967	rBV3	645	544	0.01%	0.002%
62	10.889	2967	2970	2976	rVB4	1078	1056	0.01%	0.004%
63	11.095	3032	3034	3037	rVV3	525	338	0.00%	0.001%
64	11.121	3038	3042	3046	rVB3	1098	904	0.01%	0.003%
65	11.230	3073	3076	3080	rBV3	382	406	0.01%	0.001%
66	11.372	3114	3120	3125	rBV4	565	656	0.01%	0.002%
67	11.462	3140	3148	3156	rBV6	1303	2661	0.04%	0.010%
68	11.571	3180	3182	3190	rVB4	574	632	0.01%	0.002%
69	11.735	3229	3233	3236	rBV2	374	418	0.01%	0.002%
70	11.809	3243	3256	3281	rBV	544873	875569	12.06%	3.198%
71	11.944	3296	3298	3302	rBV4	452	415	0.01%	0.002%
72	11.973	3305	3307	3322	rVB7	1298	2035	0.03%	0.007%
73	12.066	3332	3336	3344	rBV6	1398	2094	0.03%	0.008%
74	12.192	3361	3375	3395	rBV	625396	1025083	14.12%	3.744%
75	12.307	3408	3411	3414	rBV4	698	471	0.01%	0.002%
76	12.420	3442	3446	3451	rBV3	475	489	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050867.D
 Acq On : 21 Sep 2022 05:46
 Operator : JC/MD
 Sample : N4650-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	12.523	3475	3478	3482	rBV2	435	421	0.01%	0.002%
78	12.574	3492	3494	3499	rVB	605	439	0.01%	0.002%
79	12.979	3615	3620	3621	rBV2	553	484	0.01%	0.002%
80	13.008	3624	3629	3631	rVV3	437	432	0.01%	0.002%
81	13.127	3662	3666	3669	rBV3	438	382	0.01%	0.001%
82	13.156	3669	3675	3678	rVV2	607	571	0.01%	0.002%
83	13.320	3723	3726	3730	rBV3	479	371	0.01%	0.001%
84	13.475	3769	3774	3775	rBV	553	474	0.01%	0.002%
85	13.532	3789	3792	3798	rVB2	643	504	0.01%	0.002%
86	13.735	3852	3855	3857	rBV	463	342	0.00%	0.001%
87	13.896	3902	3905	3910	rBV2	334	374	0.01%	0.001%
88	13.957	3922	3924	3929	rVB2	555	389	0.01%	0.001%
89	14.079	3957	3962	3963	rBV3	434	387	0.01%	0.001%
90	14.114	3970	3973	3975	rBV	555	357	0.00%	0.001%
91	14.269	4018	4021	4024	rBV2	724	518	0.01%	0.002%
92	14.536	4101	4104	4108	rBV2	570	451	0.01%	0.002%
93	14.732	4162	4165	4169	rBV4	642	536	0.01%	0.002%
94	14.757	4169	4173	4176	rBV2	814	781	0.01%	0.003%
95	14.835	4193	4197	4201	rBV3	1263	1222	0.02%	0.004%
96	15.172	4300	4302	4304	rBV2	583	372	0.01%	0.001%
97	15.269	4330	4332	4335	rBV3	597	395	0.01%	0.001%
98	15.336	4351	4353	4356	rBV2	674	427	0.01%	0.002%
99	15.410	4373	4376	4379	rBV2	879	597	0.01%	0.002%
100	15.558	4419	4422	4427	rBV6	1098	1351	0.02%	0.005%




Sum of corrected areas: 27381217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050867.D
Acq On : 21 Sep 2022 05:46
Operator : JC/MD
Sample : N4650-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

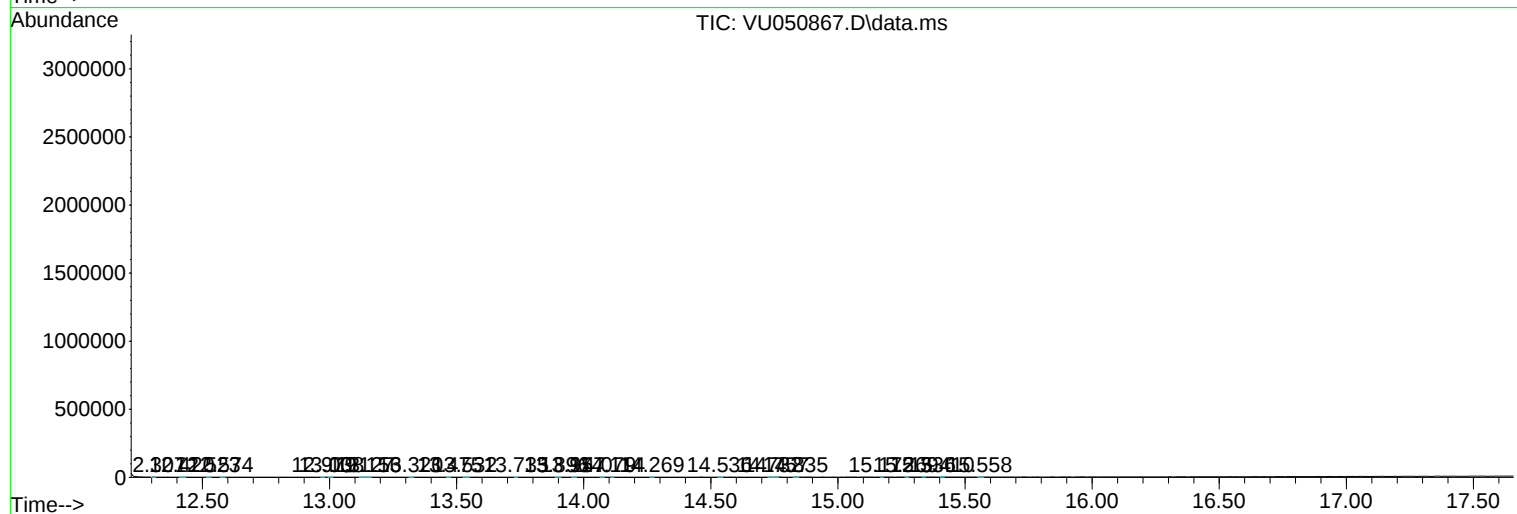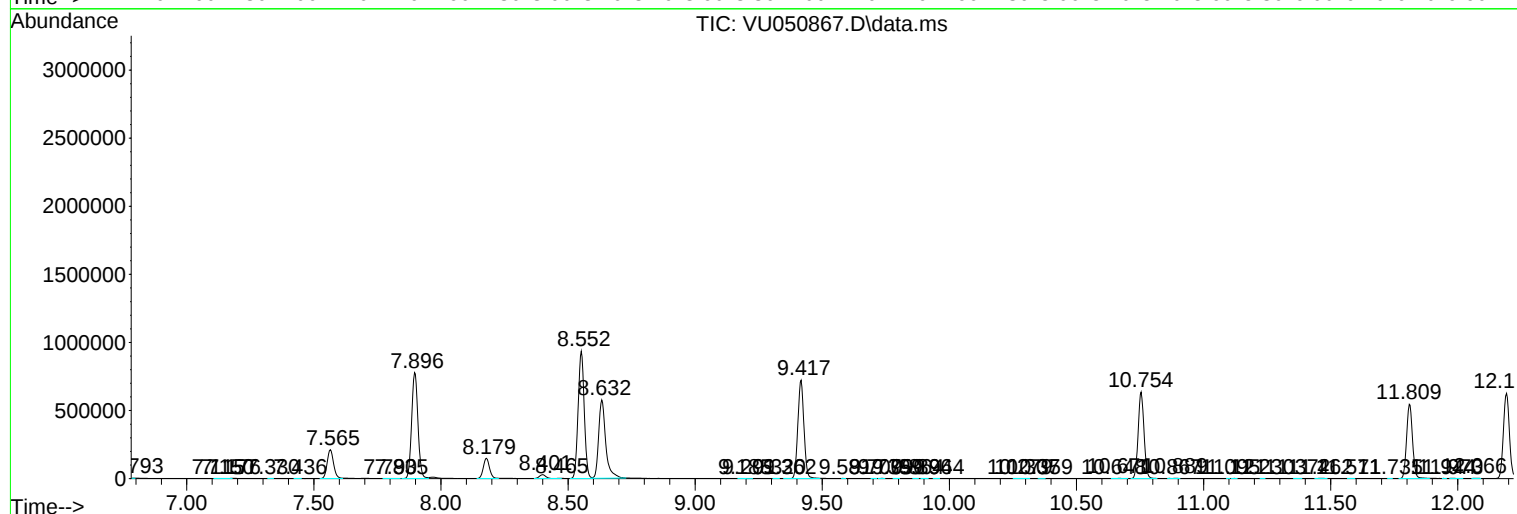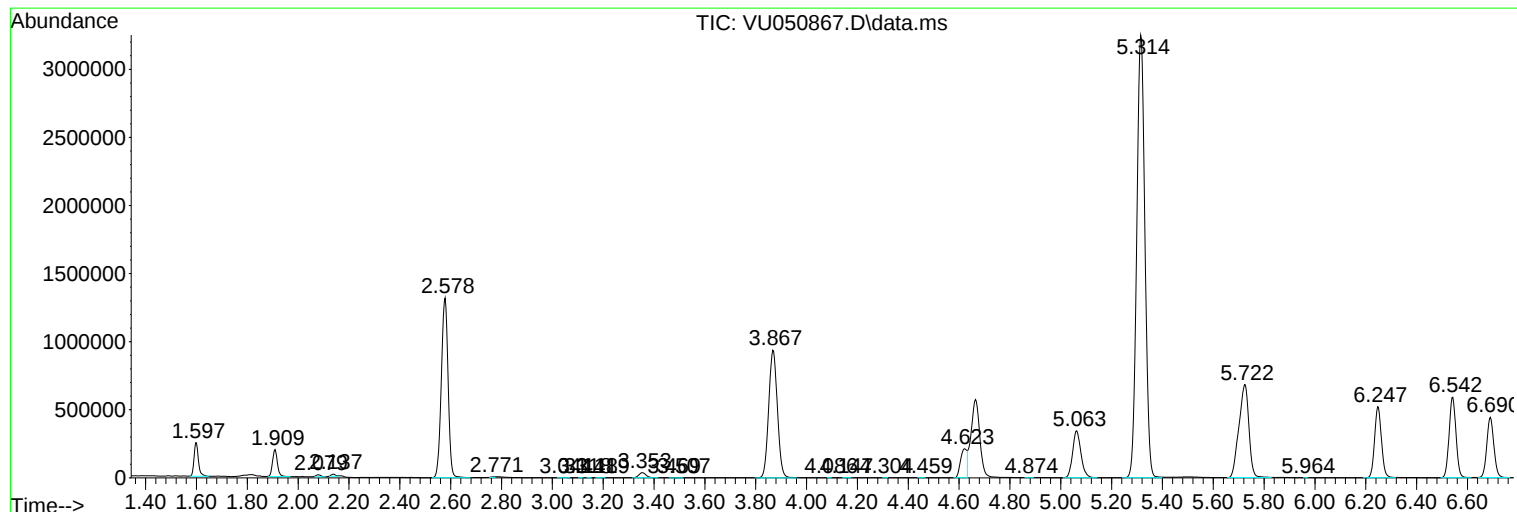

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050867.D
Acq On : 21 Sep 2022 05:46
Operator : JC/MD
Sample : N4650-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050867.D
Acq On : 21 Sep 2022 05:46
Operator : JC/MD
Sample : N4650-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc