

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050868.D
 Acq On : 21 Sep 2022 06:09
 Operator : JC/MD
 Sample : N4650-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	251812	300828	5.06%	1.037%
2	1.909	169	177	196	rVB	222376	291031	4.89%	1.003%
3	2.080	225	230	237	rVB2	9611	12273	0.21%	0.042%
4	2.138	242	248	254	rBV	15528	19640	0.33%	0.068%
5	2.578	368	385	421	rBV4	1374735	2535691	42.61%	8.741%
6	2.700	421	423	427	rVV4	574	347	0.01%	0.001%
7	3.044	523	530	540	rVB8	2252	3950	0.07%	0.014%
8	3.099	542	547	549	rBV4	267	294	0.00%	0.001%
9	3.167	564	568	571	rBV5	572	570	0.01%	0.002%
10	3.257	593	596	599	rBV3	379	332	0.01%	0.001%
11	3.285	599	605	609	rVV2	437	540	0.01%	0.002%
12	3.356	613	627	646	rVB2	22514	45479	0.76%	0.157%
13	3.472	656	663	668	rVB3	426	536	0.01%	0.002%
14	3.520	674	678	684	rVB2	390	378	0.01%	0.001%
15	3.552	684	688	690	rBV	352	315	0.01%	0.001%
16	3.716	736	739	748	rVB3	458	530	0.01%	0.002%
17	3.867	763	786	813	rBV	647851	1531246	25.73%	5.279%
18	4.060	840	846	847	rBV2	452	433	0.01%	0.001%
19	4.215	891	894	900	rBV3	448	451	0.01%	0.002%
20	4.311	919	924	927	rBV3	354	341	0.01%	0.001%
21	4.330	927	930	933	rVV3	452	339	0.01%	0.001%
22	4.385	944	947	950	rVB3	424	338	0.01%	0.001%
23	4.665	1008	1034	1070	rBV2	888058	2515800	42.28%	8.673%
24	5.064	1141	1158	1181	rBV2	354691	842017	14.15%	2.903%
25	5.314	1217	1236	1258	rBV	2654574	5950990	100.00%	20.515%
26	5.723	1342	1363	1382	rBV2	710425	1916536	32.21%	6.607%
27	5.986	1441	1445	1448	rVB4	554	363	0.01%	0.001%
28	6.022	1453	1456	1458	rBV	442	286	0.00%	0.001%
29	6.247	1510	1526	1549	rBV	531711	1015216	17.06%	3.500%
30	6.453	1587	1590	1595	rVB3	545	458	0.01%	0.002%
31	6.539	1602	1617	1640	rBV	1210958	2261178	38.00%	7.795%
32	6.690	1650	1664	1686	rVB	456549	885597	14.88%	3.053%
33	6.996	1752	1759	1762	rBV4	1167	1409	0.02%	0.005%
34	7.186	1811	1818	1820	rBV3	1511	1791	0.03%	0.006%
35	7.565	1923	1936	1957	rBV	217446	381574	6.41%	1.315%
36	7.662	1964	1966	1970	rVB3	955	583	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050868.D
 Acq On : 21 Sep 2022 06:09
 Operator : JC/MD
 Sample : N4650-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.735	1988	1989	1997	rVB4	763	750	0.01%	0.003%
38	7.774	1997	2001	2005	rBV	652	499	0.01%	0.002%
39	7.803	2005	2010	2013	rVV5	651	572	0.01%	0.002%
40	7.838	2018	2021	2025	rBV2	483	396	0.01%	0.001%
41	7.896	2025	2039	2055	rBV	800627	1367058	22.97%	4.713%
42	8.179	2111	2127	2143	rBV2	152480	259363	4.36%	0.894%
43	8.398	2184	2195	2207	rBV2	32811	55849	0.94%	0.193%
44	8.465	2214	2216	2223	rVB4	728	870	0.01%	0.003%
45	8.552	2229	2243	2257	rBV	832729	1383529	23.25%	4.769%
46	8.633	2257	2268	2299	rVB2	610756	1177901	19.79%	4.061%
47	8.887	2345	2347	2353	rVB4	634	504	0.01%	0.002%
48	8.915	2353	2356	2360	rVB2	405	300	0.01%	0.001%
49	9.025	2388	2390	2400	rVB3	483	489	0.01%	0.002%
50	9.105	2412	2415	2422	rVB3	644	494	0.01%	0.002%
51	9.137	2422	2425	2427	rBV	428	283	0.00%	0.001%
52	9.269	2460	2466	2468	rBV	492	562	0.01%	0.002%
53	9.417	2498	2512	2530	rBV	735028	1218541	20.48%	4.201%
54	9.616	2572	2574	2579	rVB2	661	492	0.01%	0.002%
55	9.642	2579	2582	2585	rBV2	425	295	0.00%	0.001%
56	9.694	2592	2598	2605	rVV4	1091	1287	0.02%	0.004%
57	9.838	2637	2643	2644	rBV2	341	285	0.00%	0.001%
58	9.861	2644	2650	2654	rVV2	229	293	0.00%	0.001%
59	10.038	2700	2705	2707	rBV2	444	344	0.01%	0.001%
60	10.099	2721	2724	2727	rVV2	490	320	0.01%	0.001%
61	10.173	2742	2747	2750	rBV2	312	329	0.01%	0.001%
62	10.234	2757	2766	2770	rVB3	290	489	0.01%	0.002%
63	10.292	2777	2784	2787	rBV2	614	719	0.01%	0.002%
64	10.366	2800	2807	2810	rBV2	516	617	0.01%	0.002%
65	10.468	2835	2839	2843	rBV3	601	494	0.01%	0.002%
66	10.517	2849	2854	2859	rBV3	422	474	0.01%	0.002%
67	10.626	2884	2888	2892	rBV3	429	370	0.01%	0.001%
68	10.668	2894	2901	2905	rBV4	1629	1932	0.03%	0.007%
69	10.755	2915	2928	2951	rVV	645527	1039623	17.47%	3.584%
70	10.896	2964	2972	2977	rBV4	1324	1448	0.02%	0.005%
71	10.931	2980	2983	2990	rBV3	345	425	0.01%	0.001%
72	11.028	3011	3013	3018	rVB2	543	360	0.01%	0.001%
73	11.086	3027	3031	3032	rBV2	456	310	0.01%	0.001%
74	11.112	3035	3039	3047	rVV6	1156	1412	0.02%	0.005%
75	11.378	3117	3122	3123	rBV2	574	347	0.01%	0.001%
76	11.465	3141	3149	3153	rVV4	958	1448	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050868.D
 Acq On : 21 Sep 2022 06:09
 Operator : JC/MD
 Sample : N4650-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.546	3169	3174	3176	rBV4	470	414	0.01%	0.001%
78	11.620	3194	3197	3201	rVB3	444	306	0.01%	0.001%
79	11.748	3232	3237	3241	rBV	331	362	0.01%	0.001%
80	11.809	3241	3256	3280	rBV	568348	893899	15.02%	3.082%
81	11.976	3304	3308	3310	rVB3	692	444	0.01%	0.002%
82	12.070	3328	3337	3345	rBV5	2663	4087	0.07%	0.014%
83	12.102	3345	3347	3358	rVB6	996	1313	0.02%	0.005%
84	12.192	3358	3375	3395	rBV	653177	1058159	17.78%	3.648%
85	12.523	3475	3478	3481	rBV2	516	328	0.01%	0.001%
86	12.546	3481	3485	3488	rVV	730	489	0.01%	0.002%
87	12.610	3501	3505	3509	rBV3	541	422	0.01%	0.001%
88	12.668	3518	3523	3528	rBV	706	972	0.02%	0.003%
89	12.742	3544	3546	3550	rVB2	543	312	0.01%	0.001%
90	12.767	3552	3554	3560	rVB2	752	560	0.01%	0.002%
91	12.967	3613	3616	3620	rVB3	586	338	0.01%	0.001%
92	13.259	3704	3707	3710	rBV3	459	322	0.01%	0.001%
93	13.414	3752	3755	3757	rBV2	450	361	0.01%	0.001%
94	13.674	3832	3836	3839	rBV	545	464	0.01%	0.002%
95	13.767	3861	3865	3867	rBV2	715	523	0.01%	0.002%
96	14.330	4038	4040	4044	rBV2	408	337	0.01%	0.001%
97	14.832	4193	4196	4202	rBV4	508	489	0.01%	0.002%
98	14.935	4226	4228	4232	rVB2	651	350	0.01%	0.001%
99	14.957	4232	4235	4239	rBV3	954	746	0.01%	0.003%
100	15.349	4354	4357	4360	rBV2	689	391	0.01%	0.001%




Sum of corrected areas: 29008141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050868.D
Acq On : 21 Sep 2022 06:09
Operator : JC/MD
Sample : N4650-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

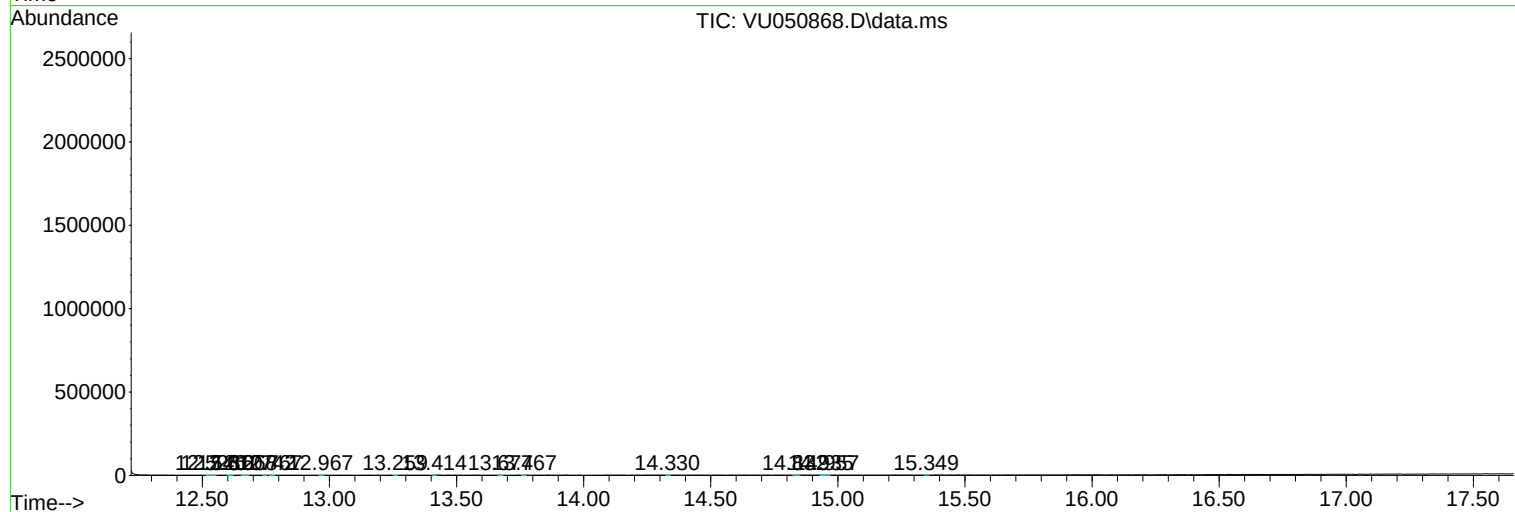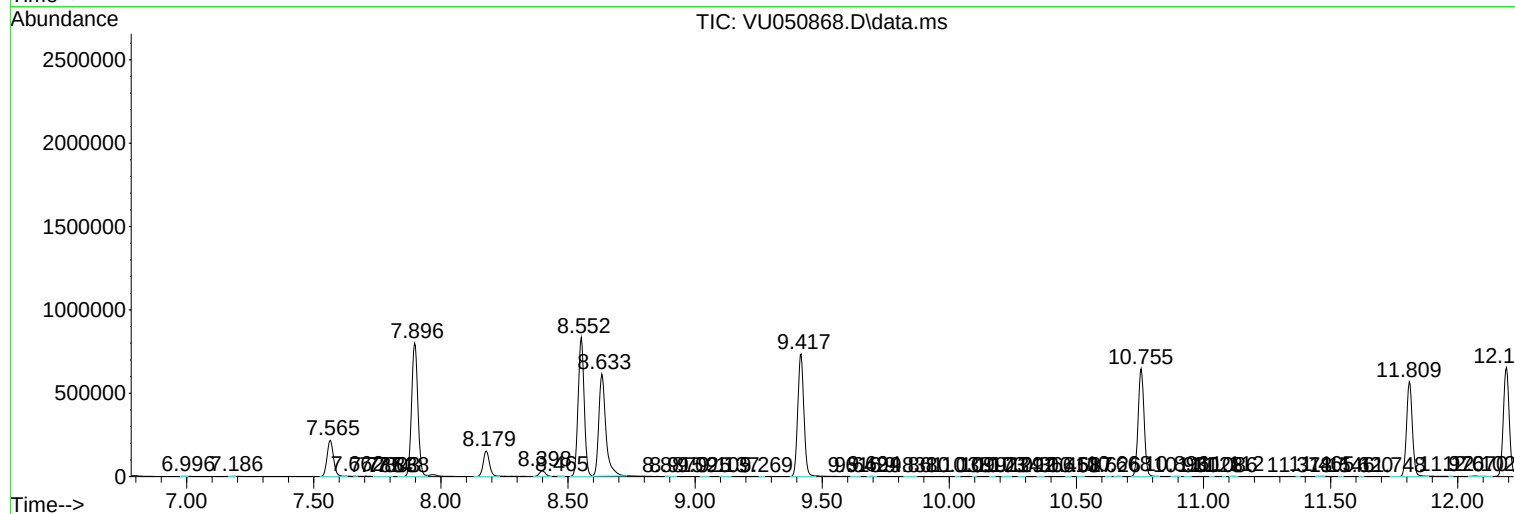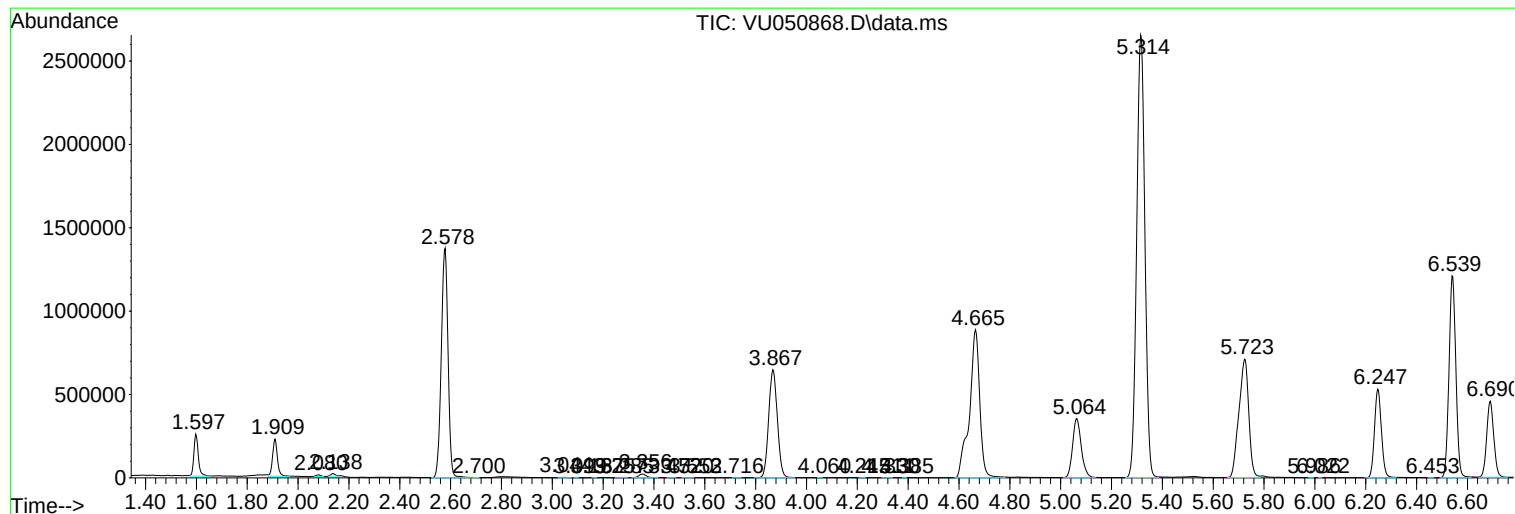

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050868.D
Acq On : 21 Sep 2022 06:09
Operator : JC/MD
Sample : N4650-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
Data File : VU050868.D
Acq On : 21 Sep 2022 06:09
Operator : JC/MD
Sample : N4650-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc