
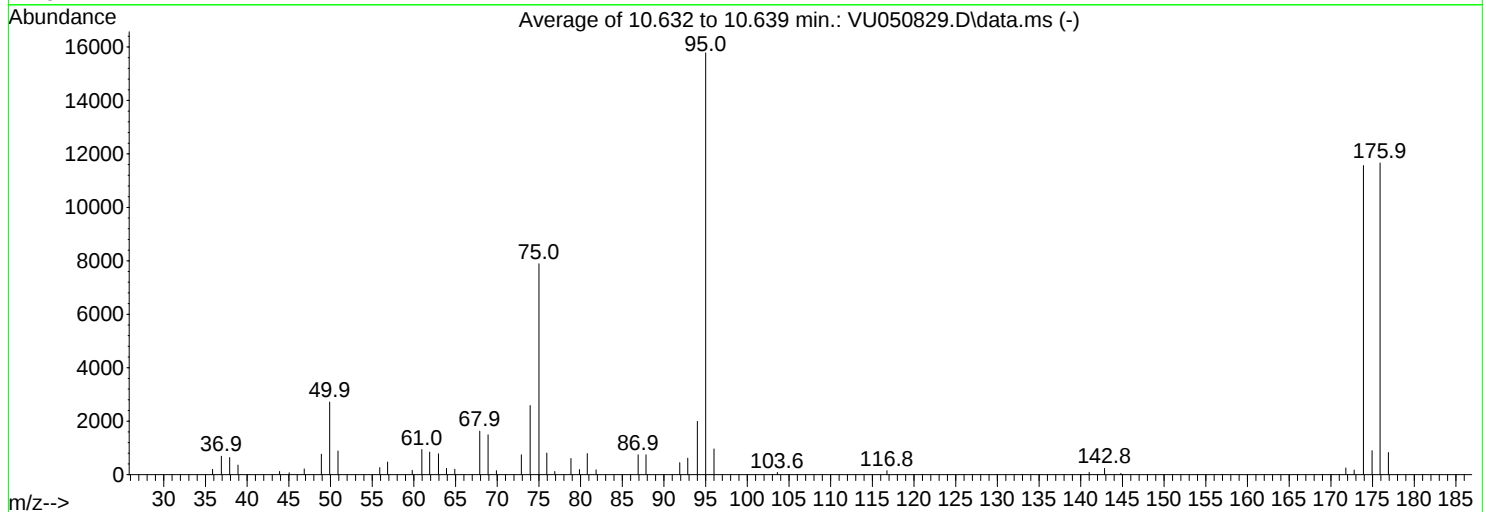


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092022\
 Data File : VU050829.D
 Acq On : 20 Sep 2022 11:49
 Operator : JC/MD
 Sample : BFB127
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB127

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 24 00:22:43 2022

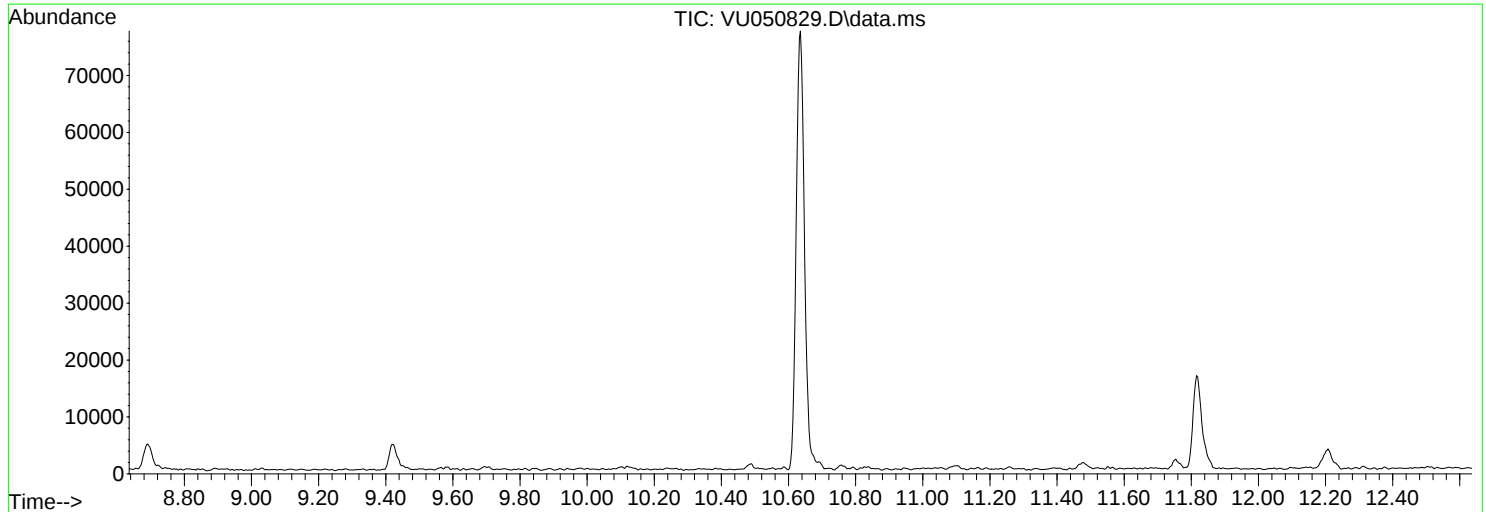

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	2715	PASS
75	95	30	80	50.0	7892	PASS
95	95	100	100	100.0	15781	PASS
96	95	5	9	6.1	966	PASS
173	174	0.00	2	1.5	174	PASS
174	95	50	120	73.3	11564	PASS
175	174	5	9	7.8	900	PASS
176	174	95	101	100.9	11664	PASS
177	176	5	9	7.1	826	PASS

m/z	Abundance
39.80	277.0
43.90	475.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.90	209.0
36.90	624.0
37.90	775.0
38.90	404.0
39.80	298.0
44.00	680.0
45.00	115.0
46.80	213.0
48.90	718.0
49.90	2804.0
50.90	1007.0
55.90	243.0
56.90	449.0
59.80	118.0
60.90	984.0
61.90	879.0
63.00	810.0
63.90	226.0
64.90	243.0
67.90	1523.0
68.90	1501.0
69.90	165.0
72.90	746.0
74.00	2724.0
75.00	7790.0
76.00	866.0
76.80	139.0
78.90	609.0
79.90	204.0
80.80	820.0
81.90	166.0
86.90	802.0
87.80	785.0
91.90	446.0
92.90	537.0
94.00	1908.0
95.00	15998.0
96.00	981.0
103.60	114.0
116.70	148.0
141.00	126.0
142.80	242.0
171.80	265.0
172.80	207.0
173.90	11584.0
174.90	862.0
175.90	11794.0
176.90	791.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.90	202.0
36.90	701.0
37.90	660.0
38.90	376.0
39.80	233.0
43.90	583.0
45.10	108.0
46.80	236.0
48.90	804.0
49.90	2719.0
50.90	909.0
55.90	265.0
56.90	482.0
59.80	172.0
61.00	991.0
61.90	858.0
62.90	795.0
63.90	261.0
64.90	203.0
67.90	1683.0
68.90	1540.0
69.90	146.0
72.90	793.0
74.00	2676.0
75.00	8174.0
76.00	820.0
76.90	106.0
78.90	620.0
79.90	173.0
80.80	799.0
81.90	188.0
86.90	769.0
87.80	769.0
91.90	456.0
92.90	627.0
94.00	2053.0
95.00	16244.0
96.00	972.0
103.60	133.0
116.70	157.0
141.00	135.0
142.80	241.0
171.80	261.0
172.80	178.0
173.90	11826.0
175.00	960.0
175.90	11909.0
176.90	821.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.80	184.0
36.90	745.0
37.90	481.0
38.90	304.0
39.80	226.0
43.80	527.0
46.90	201.0
48.90	784.0
49.90	2623.0
50.90	750.0
55.90	280.0
56.80	498.0
59.80	193.0
61.00	855.0
61.90	804.0
63.00	730.0
63.90	222.0
64.90	170.0
67.90	1673.0
68.90	1437.0
69.90	131.0
72.90	696.0
73.90	2362.0
75.00	7712.0
75.90	731.0
77.00	111.0
78.80	581.0
79.80	204.0
80.80	751.0
81.80	180.0
86.90	662.0
87.90	676.0
91.90	451.0
92.80	681.0
94.00	2016.0
95.00	15101.0
96.00	946.0
116.80	144.0
142.90	218.0
144.80	139.0
171.80	224.0
172.80	136.0
173.90	11281.0
175.00	878.0
175.90	11288.0
176.90	867.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127