




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092024\  
Data File : VU060947.D  
Acq On : 20 Sep 2024 16:49  
Operator : MD/SY  
Sample : P3987-05DL 20X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BH8P5DL

Manual IntegrationsAPPROVED

Quant Time: Sep 22 22:16:47 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091624WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Sep 21 01:39:49 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024  
Supervised By :Semsettin Yesilyurt 09/24/2024

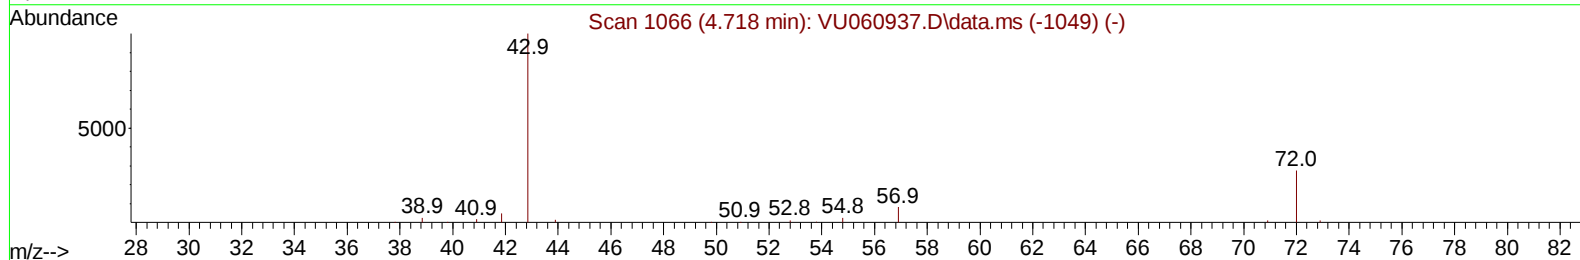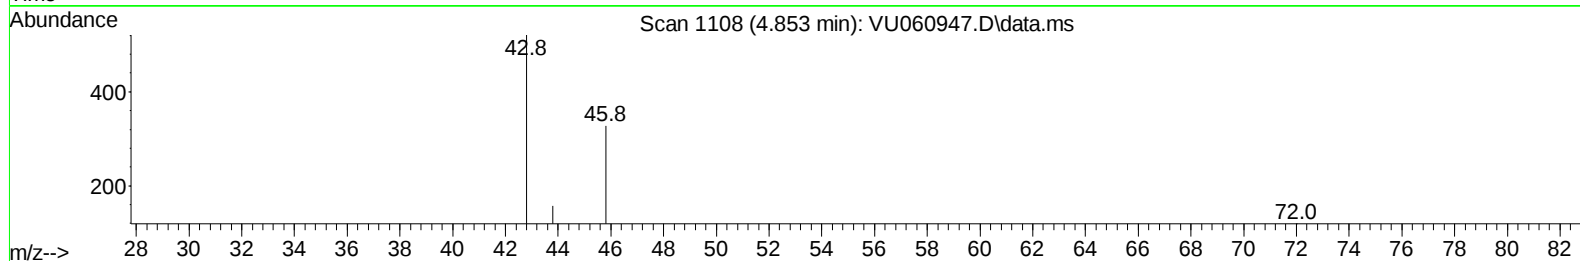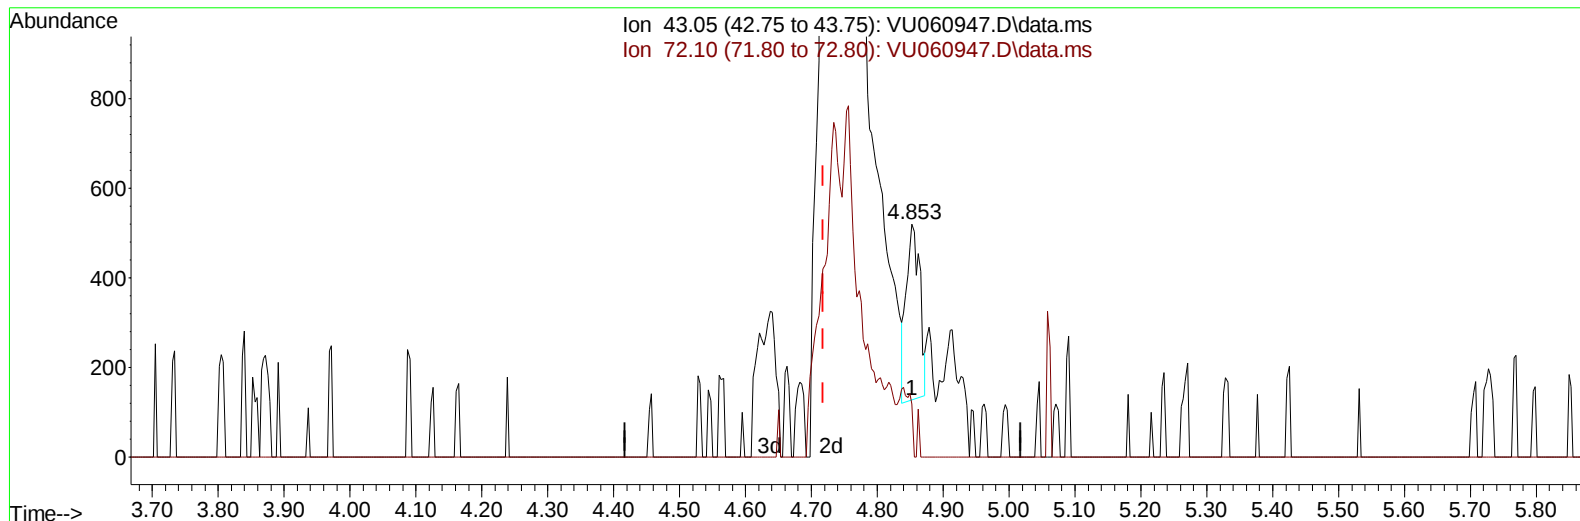

TIC: VU060947.D\data.ms

(21) 2-Butanone (T)

4.853min (+ 0.135) 0.28 ug/L

response 560

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 72.10 | 29.50  | 33.39  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092024\  
Data File : VU060947.D  
Acq On : 20 Sep 2024 16:49  
Operator : MD/SY  
Sample : P3987-05DL 20X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BH8P5DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 01:42:41 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091624WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Sep 21 01:39:49 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024  
Supervised By :Semsettin Yesilyurt 09/24/2024

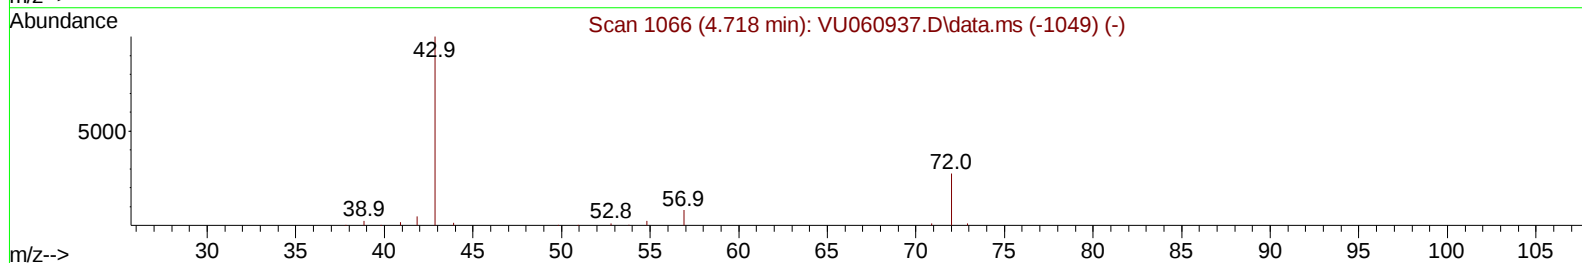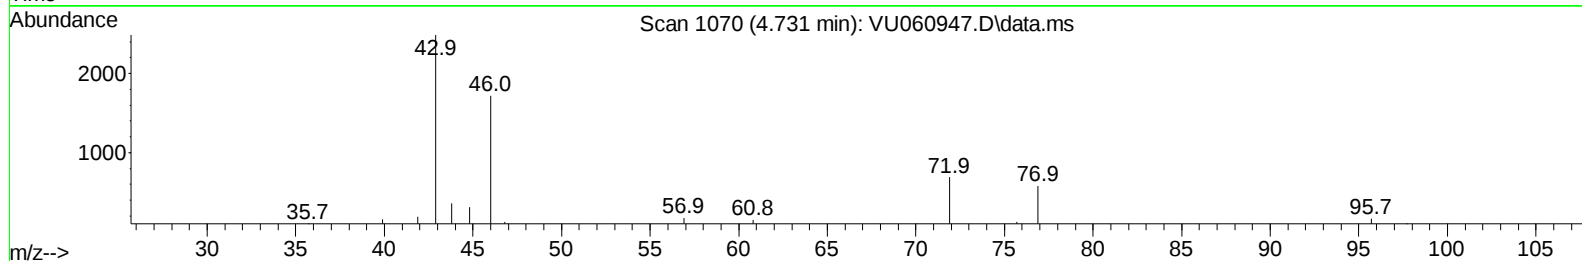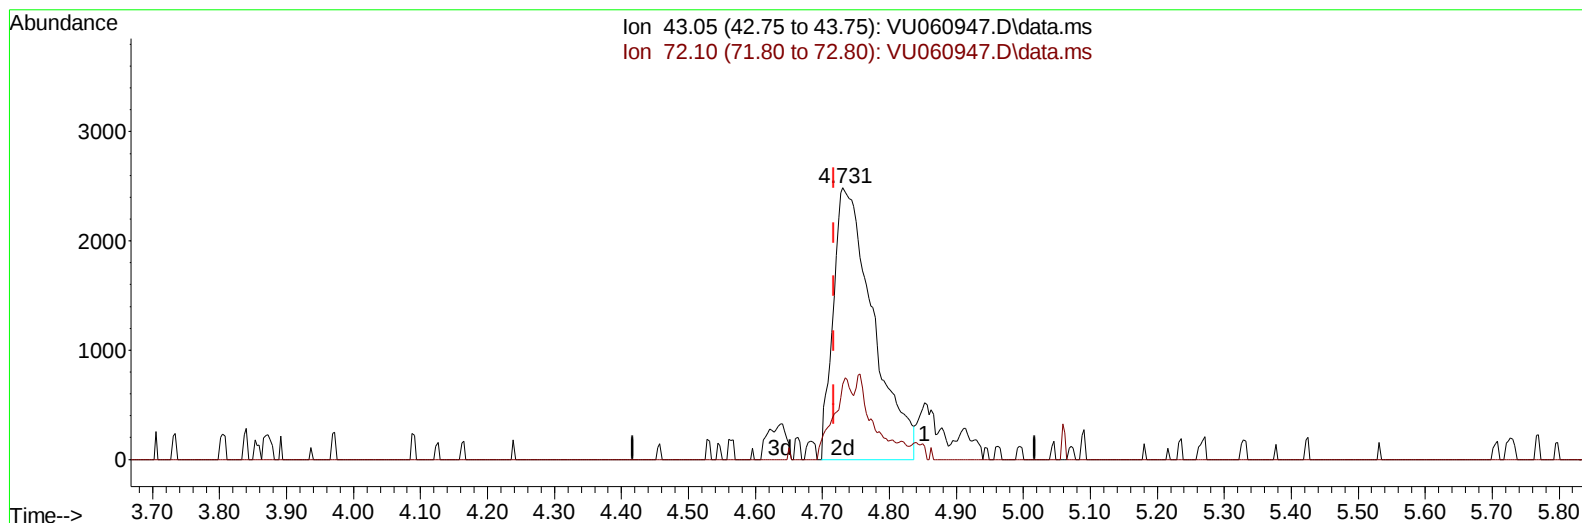

TIC: VU060947.D\data.ms

(21) 2-Butanone (T)

4.731min (+ 0.013) 5.14 ug/L m

response 10207

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 72.10 | 29.50  | 0.00#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092024\  
 Data File : VU060947.D  
 Acq On : 20 Sep 2024 16:49  
 Operator : MD/SY  
 Sample : P3987-05DL 20X  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BH8P5DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 01:42:41 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091624WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Sep 21 01:39:49 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024  
 Supervised By :Semsettin Yesilyurt 09/24/2024

| Compound                      | R.T.     | Q     | Ion | Response | Conc   | Units   | Dev(Min) |
|-------------------------------|----------|-------|-----|----------|--------|---------|----------|
| -----                         |          |       |     |          |        |         |          |
| Internal Standards            |          |       |     |          |        |         |          |
| 1) 1,4-Difluorobenzene        | 6.242    | 114   |     | 126626   | 5.000  | ug/L    | 0.00     |
| 28) Chlorobenzene-d5          | 9.412    | 117   |     | 134984   | 5.000  | ug/L    | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.807   | 152   |     | 55625    | 5.000  | ug/L    | 0.00     |
| System Monitoring Compounds   |          |       |     |          |        |         |          |
| 4) Vinyl Chloride-d3          | 1.596    | 65    |     | 48693    | 4.275  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 40 | - 130 |     | Recovery | =      | 85.600% |          |
| 7) Chloroethane-d5            | 1.907    | 69    |     | 37017    | 4.565  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 130 |     | Recovery | =      | 91.200% |          |
| 11) 1,1-Dichloroethene-d2     | 2.551    | 65    |     | 17865    | 4.426  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 125 |     | Recovery | =      | 88.600% |          |
| 20) 2-Butanone-d5             | 4.637    | 46    |     | 84158    | 46.029 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 40 | - 130 |     | Recovery | =      | 92.060% |          |
| 24) Chloroform-d              | 5.052    | 84    |     | 74891    | 4.301  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 |     | Recovery | =      | 86.000% |          |
| 26) 1,2-Dichloroethane-d4     | 5.695    | 65    |     | 38490    | 4.625  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 |     | Recovery | =      | 92.400% |          |
| 32) Benzene-d6                | 5.718    | 84    |     | 148723   | 4.111  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 |     | Recovery | =      | 82.200% |          |
| 36) 1,2-Dichloropropane-d6    | 6.682    | 67    |     | 48959    | 4.374  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 140 |     | Recovery | =      | 87.400% |          |
| 41) Toluene-d8                | 7.891    | 98    |     | 124735   | 3.782  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 |     | Recovery | =      | 75.600% |          |
| 43) trans-1,3-Dichloroprop... | 8.177    | 79    |     | 15811    | 3.924  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 55 | - 130 |     | Recovery | =      | 78.400% |          |
| 46) 2-Hexanone-d5             | 8.637    | 63    |     | 66808    | 42.032 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 45 | - 130 |     | Recovery | =      | 84.060% |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.753   | 84    |     | 38350    | 4.373  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 120 |     | Recovery | =      | 87.400% |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.187   | 152   |     | 41477    | 4.438  | ug/L    | 0.00     |
| Spiked Amount 5.000           | Range 80 | - 120 |     | Recovery | =      | 88.800% |          |
| Target Compounds              |          |       |     |          |        |         |          |
| 12) 1,1-Dichloroethene        | 2.567    | 96    |     | 9505     | 1.193  | ug/L    | # 27     |
| 13) Acetone                   | 2.647    | 43    |     | 26224    | 21.499 | ug/L    | 96       |
| 15) Methyl Acetate            | 2.952    | 43    |     | 43355    | 14.578 | ug/L    | 92       |
| 19) 1,1-Dichloroethane        | 3.856    | 63    |     | 33035    | 1.994  | ug/L    | 98       |
| 21) 2-Butanone                | 4.731    | 43    |     | 10207m   | 5.140  | ug/L    |          |
| 22) cis-1,2-Dichloroethene    | 4.660    | 96    |     | 17121    | 1.874  | ug/L    | 96       |
| 34) Trichloroethene           | 6.534    | 95    |     | 28178    | 2.896  | ug/L    | 99       |
| -----                         |          |       |     |          |        |         |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU092024\  
Data File : VU060947.D  
Acq On : 20 Sep 2024 16:49  
Operator : MD/SY  
Sample : P3987-05DL 20X  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BH8P5DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 01:42:41 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR091624WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Sep 21 01:39:49 2024  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/24/2024  
Supervised By :Semsettin Yesilyurt 09/24/2024

