


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092024\
Data File : VU060936.D
Acq On : 20 Sep 2024 11:27
Operator : MD/SY
Sample : BFB002
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB002

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 21 01:39:49 2024

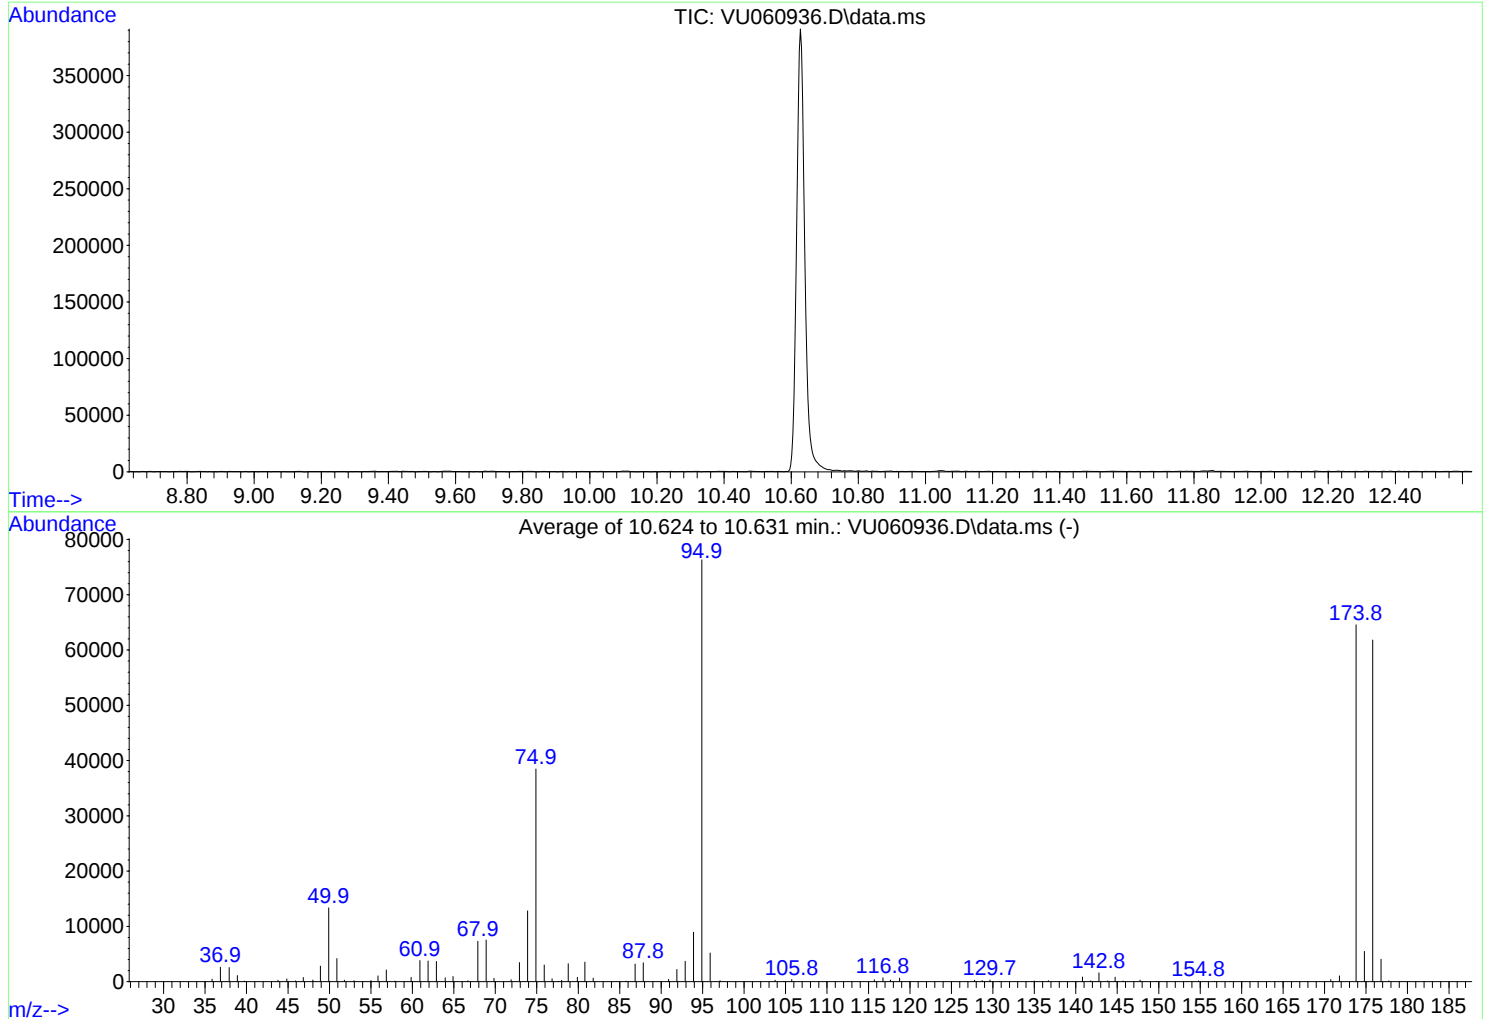

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	13340	PASS
75	95	30	80	50.4	38467	PASS
95	95	100	100	100.0	76312	PASS
96	95	5	9	6.8	5189	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.6	64547	PASS
175	174	5	9	8.5	5471	PASS
176	174	95	101	95.8	61805	PASS
177	176	5	9	6.6	4062	PASS

m/z	Abundance
39.90	125.0
43.80	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.90	464.0
36.90	2729.0
37.90	2651.0
38.90	1083.0
39.70	200.0
43.90	461.0
44.80	498.0
45.90	200.0
46.90	752.0
48.00	255.0
48.90	2572.0
49.90	13446.0
50.90	4046.0
51.80	269.0
52.90	176.0
55.00	180.0
55.80	1033.0
56.90	2170.0
59.90	801.0
60.90	3803.0
61.90	3772.0
62.90	3570.0
63.90	774.0
64.90	897.0
66.70	163.0
67.90	6769.0
68.90	7518.0
69.80	612.0
71.90	321.0
72.90	3295.0
73.90	12624.0
74.90	38064.0
75.90	3029.0
76.90	532.0
78.00	351.0
78.80	3232.0
79.90	684.0
80.80	3443.0
81.80	654.0
85.80	125.0
86.80	2943.0
87.90	3420.0
90.90	350.0
91.90	2090.0
92.90	3664.0
93.90	8485.0
94.90	74752.0
95.90	5255.0
97.10	185.0
103.80	279.0
105.70	386.0
115.70	328.0
116.80	772.0
117.60	305.0
118.70	573.0
127.80	299.0
128.70	256.0
129.60	242.0
134.70	134.0
136.70	146.0
140.80	759.0
141.90	153.0
142.80	1669.0
143.80	157.0
144.70	766.0
145.70	113.0
147.70	338.0
154.70	174.0
156.70	114.0
170.90	300.0
171.80	991.0
173.80	62432.0
174.80	5249.0
175.80	60736.0
176.80	4026.0
177.70	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	490.0
36.90	2600.0
37.90	2640.0
38.90	1124.0
39.70	226.0
43.80	493.0
44.90	489.0
45.90	174.0
46.80	745.0
48.00	299.0
48.90	2962.0
49.90	13740.0
50.90	4332.0
51.80	294.0
52.90	175.0
55.00	204.0
55.90	1035.0
56.90	2191.0
57.90	165.0
59.80	799.0
60.90	3908.0
61.90	3914.0
62.90	3824.0
64.00	729.0
64.90	943.0
66.70	185.0
67.90	7546.0
68.90	7765.0
69.80	647.0
71.90	355.0
72.90	3588.0
73.90	13110.0
74.90	39648.0
75.90	3152.0
76.80	532.0
77.60	188.0
78.00	353.0
78.80	3316.0
79.90	823.0
80.80	3634.0
81.80	658.0
85.70	124.0
86.80	3366.0
87.80	3540.0
90.90	431.0
91.90	2232.0
92.90	3842.0
93.90	9130.0
94.90	79000.0
95.90	5319.0
97.10	179.0
103.80	268.0
105.80	372.0
115.70	369.0
116.80	708.0
117.70	293.0
118.80	648.0
127.80	263.0
128.70	202.0
129.70	292.0
135.00	160.0
136.70	204.0
140.80	855.0
141.80	130.0
142.80	1689.0
143.80	144.0
144.80	825.0
145.70	119.0
147.80	280.0
154.80	120.0
158.70	107.0
170.70	385.0
171.80	1086.0
173.80	66456.0
174.80	5714.0
175.80	63880.0
176.80	4145.0
177.80	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002

m/z	Abundance
35.80	463.0
36.80	2518.0
37.90	2377.0
38.90	1105.0
39.70	212.0
43.80	514.0
44.90	481.0
45.90	116.0
46.80	748.0
48.00	297.0
48.90	2931.0
49.90	12834.0
50.90	4102.0
51.80	248.0
53.00	162.0
55.00	198.0
55.90	1057.0
56.80	1986.0
57.90	201.0
59.80	722.0
60.90	3758.0
61.90	3568.0
62.90	3513.0
63.90	630.0
64.90	919.0
66.70	175.0
67.90	7588.0
68.90	7317.0
69.90	566.0
71.90	409.0
72.90	3502.0
73.90	12666.0
74.90	37688.0
75.90	2876.0
76.80	519.0
78.80	3199.0
79.90	888.0
80.80	3542.0
81.80	638.0
86.90	3278.0
87.80	3306.0
90.90	417.0
91.90	2286.0
92.90	3542.0
93.90	9237.0
94.90	75184.0
95.90	4994.0
97.10	127.0
103.70	248.0
104.80	102.0
105.80	334.0
115.70	390.0
116.70	572.0
117.70	263.0
118.80	676.0
127.80	258.0
128.80	139.0
129.70	296.0
130.80	119.0
135.00	189.0
136.70	223.0
140.80	873.0
141.70	128.0
142.80	1439.0
143.90	118.0
144.80	833.0
145.70	107.0
147.80	211.0
149.70	105.0
154.90	103.0
156.80	109.0
158.70	108.0
170.60	409.0
171.80	1041.0
173.80	64752.0
174.80	5449.0
175.80	60800.0
176.80	4015.0
177.80	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB002