

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050873.D
 Acq On : 21 Sep 2022 10:58
 Operator : JC/MD
 Sample : VU0921WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	271359	327889	15.93%	2.213%
2	1.906	169	176	198	rVB	224690	299728	14.56%	2.023%
3	2.565	368	381	398	rBV	432287	703373	34.16%	4.748%
4	2.899	482	485	486	rBV	528	224	0.01%	0.002%
5	3.044	521	530	543	rVB3	3557	6777	0.33%	0.046%
6	3.096	543	546	550	rBV2	509	325	0.02%	0.002%
7	3.182	560	573	594	rBV2	16843	40293	1.96%	0.272%
8	3.285	603	605	607	rBV	294	158	0.01%	0.001%
9	3.346	621	624	625	rBV2	789	500	0.02%	0.003%
10	3.382	633	635	641	rVB2	430	332	0.02%	0.002%
11	3.433	646	651	654	rBV2	304	260	0.01%	0.002%
12	3.469	659	662	664	rBV	142	112	0.01%	0.001%
13	3.565	689	692	694	rBV	185	126	0.01%	0.001%
14	3.610	703	706	712	rVB2	246	138	0.01%	0.001%
15	3.639	712	715	717	rVB2	341	162	0.01%	0.001%
16	3.652	717	719	721	rBV	190	124	0.01%	0.001%
17	3.697	730	733	737	rBV3	211	150	0.01%	0.001%
18	3.716	737	739	742	rBV2	220	155	0.01%	0.001%
19	3.768	752	755	762	rBV	235	274	0.01%	0.002%
20	3.864	783	785	790	rVB	376	277	0.01%	0.002%
21	3.912	796	800	806	rVB2	248	277	0.01%	0.002%
22	3.967	814	817	822	rVB2	323	269	0.01%	0.002%
23	4.076	847	851	858	rBV3	819	1090	0.05%	0.007%
24	4.208	889	892	896	rBV2	431	315	0.02%	0.002%
25	4.308	919	923	926	rBV	205	187	0.01%	0.001%
26	4.353	932	937	938	rBV2	324	261	0.01%	0.002%
27	4.440	962	964	966	rBV	222	120	0.01%	0.001%
28	4.620	1007	1020	1049	rBV	240665	601098	29.20%	4.058%
29	5.060	1141	1157	1179	rBV	370827	813507	39.51%	5.492%
30	5.427	1269	1271	1275	rVB2	387	155	0.01%	0.001%
31	5.456	1278	1280	1282	rBV	269	114	0.01%	0.001%
32	5.501	1288	1294	1298	rBV2	377	397	0.02%	0.003%
33	5.645	1336	1339	1340	rBV2	214	108	0.01%	0.001%
34	5.722	1340	1363	1392	rBV2	753481	2058835	100.00%	13.898%
35	6.066	1468	1470	1473	rBV	272	131	0.01%	0.001%
36	6.086	1474	1476	1479	rVB2	543	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050873.D
 Acq On : 21 Sep 2022 10:58
 Operator : JC/MD
 Sample : VU0921WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	6.166	1496	1501	1503	rBV2	452	381	0.02%	0.003%
38	6.247	1513	1526	1549	rBV	553592	1044084	50.71%	7.048%
39	6.529	1604	1614	1628	rVB5	11548	21682	1.05%	0.146%
40	6.623	1641	1643	1647	rBV2	318	189	0.01%	0.001%
41	6.690	1649	1664	1685	rBV	487195	947102	46.00%	6.394%
42	6.886	1723	1725	1728	rBV2	504	243	0.01%	0.002%
43	6.941	1740	1742	1743	rBV	349	161	0.01%	0.001%
44	6.983	1750	1755	1758	rBV3	462	497	0.02%	0.003%
45	7.028	1765	1769	1771	rBV2	470	360	0.02%	0.002%
46	7.041	1771	1773	1776	rVV	347	176	0.01%	0.001%
47	7.192	1807	1820	1828	rBV6	2123	4086	0.20%	0.028%
48	7.298	1850	1853	1855	rBV2	244	162	0.01%	0.001%
49	7.333	1862	1864	1867	rBV2	277	179	0.01%	0.001%
50	7.394	1880	1883	1888	rBV	431	274	0.01%	0.002%
51	7.420	1888	1891	1894	rBV3	246	172	0.01%	0.001%
52	7.481	1907	1910	1913	rBV2	304	253	0.01%	0.002%
53	7.501	1914	1916	1919	rVB	271	122	0.01%	0.001%
54	7.565	1922	1936	1952	rBV	239958	426923	20.74%	2.882%
55	7.767	1997	1999	2000	rBV2	394	133	0.01%	0.001%
56	7.896	2025	2039	2055	rBV	856742	1472031	71.50%	9.937%
57	8.179	2115	2127	2143	rBV	171943	289880	14.08%	1.957%
58	8.472	2213	2218	2222	rBV3	623	659	0.03%	0.004%
59	8.526	2234	2235	2238	rBV2	326	217	0.01%	0.001%
60	8.632	2256	2268	2303	rBV2	634445	1214558	58.99%	8.199%
61	8.960	2367	2370	2373	rBV3	418	337	0.02%	0.002%
62	8.989	2373	2379	2383	rVV3	458	649	0.03%	0.004%
63	9.025	2388	2390	2392	rVB3	261	107	0.01%	0.001%
64	9.037	2392	2394	2397	rVB2	315	196	0.01%	0.001%
65	9.060	2398	2401	2404	rBV2	249	175	0.01%	0.001%
66	9.076	2404	2406	2411	rBV4	496	296	0.01%	0.002%
67	9.234	2453	2455	2457	rBV4	388	177	0.01%	0.001%
68	9.336	2485	2487	2495	rVB3	274	257	0.01%	0.002%
69	9.417	2497	2512	2541	rBV	769943	1280716	62.21%	8.646%
70	9.632	2577	2579	2580	rBV2	396	182	0.01%	0.001%
71	9.661	2586	2588	2589	rBV2	325	155	0.01%	0.001%
72	9.806	2628	2633	2636	rVB3	536	507	0.02%	0.003%
73	9.828	2636	2640	2642	rBV3	352	278	0.01%	0.002%
74	9.902	2661	2663	2665	rVB	239	97	0.00%	0.001%
75	9.951	2676	2678	2681	rBV	184	105	0.01%	0.001%
76	10.105	2721	2726	2731	rBV6	1134	1500	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050873.D
 Acq On : 21 Sep 2022 10:58
 Operator : JC/MD
 Sample : VU0921WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK184

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

77	10.439	2827	2830	2836	rBV	363	322	0.02%	0.002%
78	10.468	2836	2839	2840	rBV	257	146	0.01%	0.001%
79	10.561	2866	2868	2872	rVB2	307	156	0.01%	0.001%
80	10.584	2872	2875	2880	rVB2	453	382	0.02%	0.003%
81	10.613	2880	2884	2887	rBV2	416	404	0.02%	0.003%
82	10.668	2897	2901	2911	rVB5	2590	3050	0.15%	0.021%
83	10.754	2915	2928	2948	rBV	670804	1079908	52.45%	7.290%
84	10.963	2991	2993	2995	rBV2	176	109	0.01%	0.001%
85	11.015	3006	3009	3012	rVB2	309	171	0.01%	0.001%
86	11.057	3016	3022	3024	rBV	424	447	0.02%	0.003%
87	11.214	3068	3071	3075	rBV2	415	291	0.01%	0.002%
88	11.262	3084	3086	3093	rBV2	390	416	0.02%	0.003%
89	11.417	3131	3134	3138	rBV2	672	492	0.02%	0.003%
90	11.571	3179	3182	3188	rBV2	532	623	0.03%	0.004%
91	11.696	3213	3221	3226	rBV3	1065	1354	0.07%	0.009%
92	11.745	3231	3236	3244	rVB3	1974	2594	0.13%	0.018%
93	11.809	3244	3256	3280	rBV	617398	978209	47.51%	6.604%
94	12.073	3336	3338	3340	rBV	387	245	0.01%	0.002%
95	12.192	3362	3375	3395	rBV	719138	1162968	56.49%	7.851%
96	12.603	3499	3503	3506	rBV2	541	477	0.02%	0.003%
97	12.854	3577	3581	3582	rBV	481	318	0.02%	0.002%
98	12.999	3622	3626	3633	rBV6	919	1449	0.07%	0.010%
99	13.227	3689	3697	3703	rBV6	2723	3943	0.19%	0.027%
100	13.841	3884	3888	3899	rVB6	4270	6168	0.30%	0.042%




Sum of corrected areas: 14813380

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050873.D
Acq On : 21 Sep 2022 10:58
Operator : JC/MD
Sample : VU0921WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

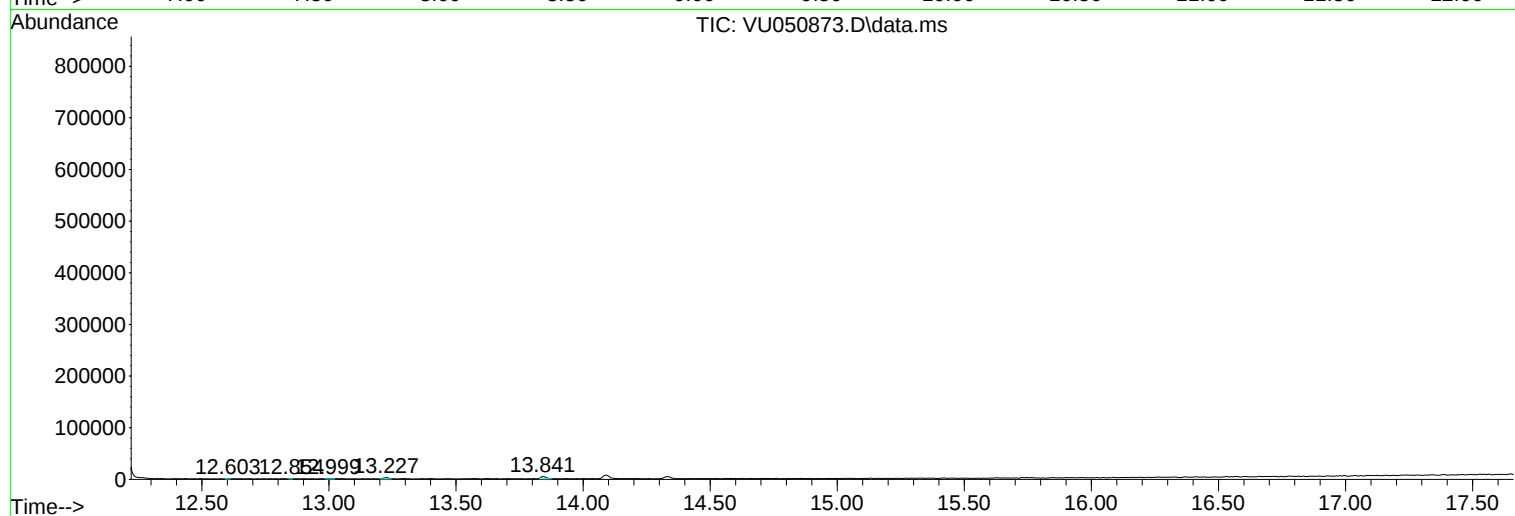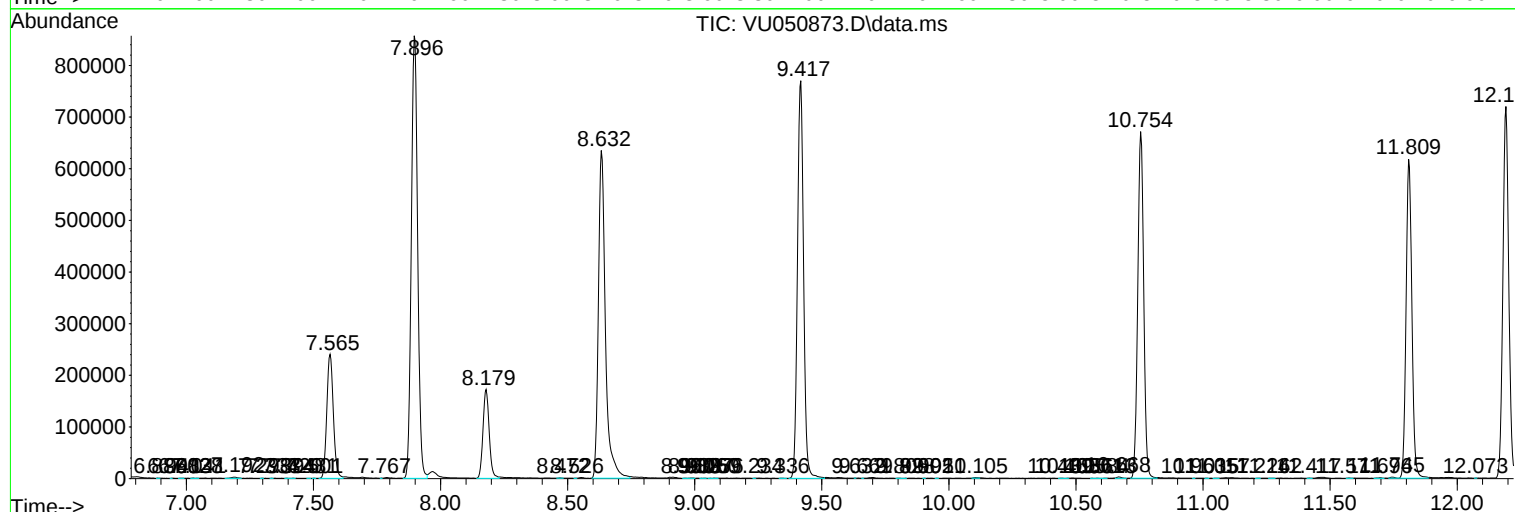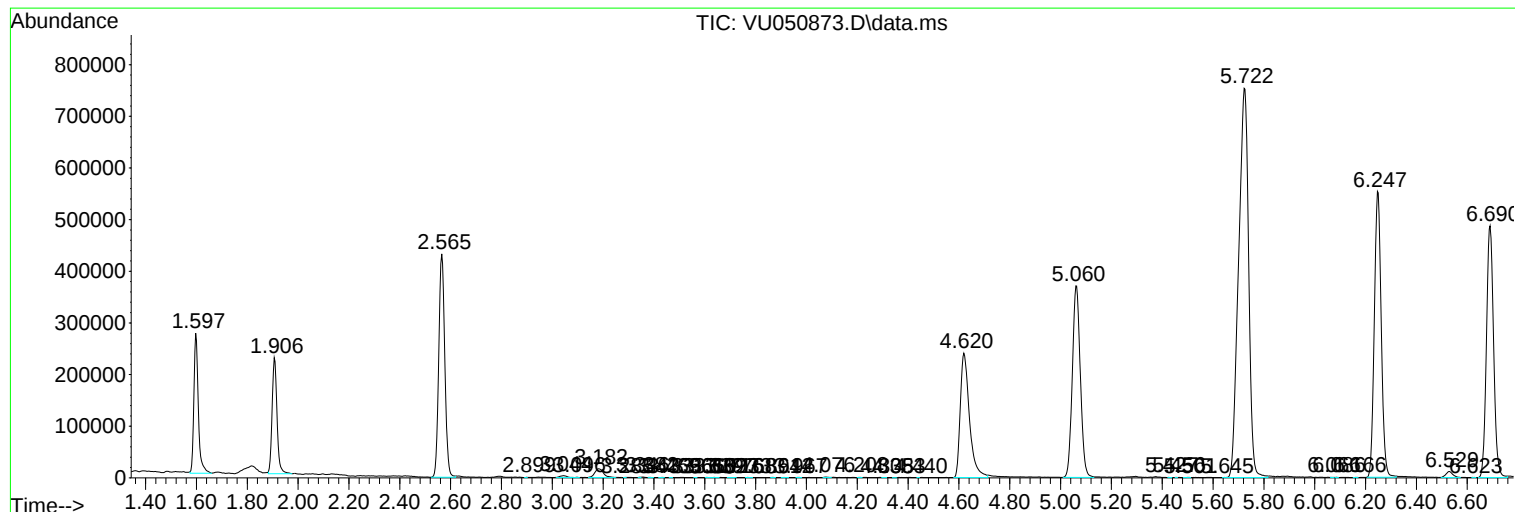

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050873.D
Acq On : 21 Sep 2022 10:58
Operator : JC/MD
Sample : VU0921WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050873.D
Acq On : 21 Sep 2022 10:58
Operator : JC/MD
Sample : VU0921WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK184

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------